


LB126613

7470A

INSTRUMENT ID: CV2

Linear

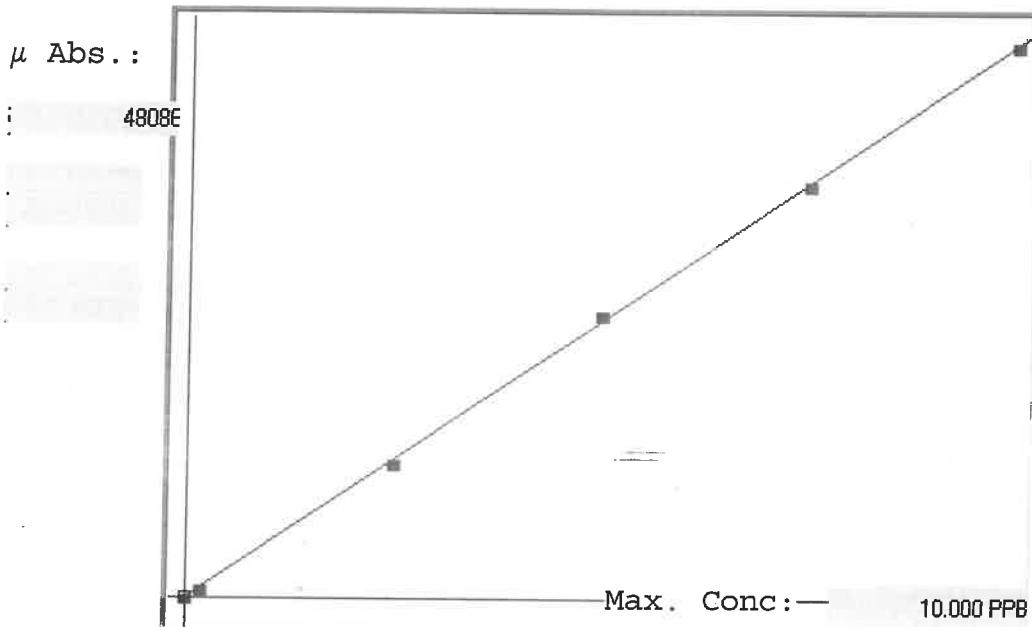

A= 0.0000e+000

B= 2.0747e-004

C= -5.7559e-003

Rho= 0.9998465

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0 D
0.0	0.000	0.024	0.024	145	0.000	145	0				
0.2	0.200	0.163	-0.037	813	0.0 %	813					-19
2.5	2.500	2.441	-0.059	11795	0.0 %	11795					2
5.0	5.000	5.133	0.133	24770	0.0 %	24770					3
7.5	7.500	7.468	-0.032	36022	0.0 %	36022					0
10.0	10.000	9.971	-0.029	48086	0.0 %	48086					0

LB126613 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Jul 2023 10:58:32

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	145	-	0.0000	7470A	PPB	27 Jul 2023 11:03:25	S	Std
0.2 - 1	50.2	813	-	0.2000	7470A	PPB	27 Jul 2023 11:05:41	S	Std
2.5 - 1	52.5	11795	-	2.5000	7470A	PPB	27 Jul 2023 11:07:58	S	Std
5.0 - 1	55	24770	-	5.0000	7470A	PPB	27 Jul 2023 11:10:15	S	Std
7.5 - 1	57.5	36022	-	7.5000	7470A	PPB	27 Jul 2023 11:12:31	S	Std
10.0 - 1	510	48086	-	10.0000	7470A	PPB	27 Jul 2023 11:14:47	S	Std
ICV87 - 1	ICV87	18589	3.8509	-	7470A	PPB	27 Jul 2023 11:17:36	U	SMPL
ICB87 - 1	ICB87	190	0.0337	-	7470A	PPB	27 Jul 2023 11:19:51	U	SMPL
CCV10 - 1	CCV10	22744	4.7129	-	7470A	PPB	27 Jul 2023 11:22:05	U	SMPL
CCB10 - 1	CCB10	162	0.0279	-	7470A	PPB	27 Jul 2023 11:24:20	U	SMPL
CRA - 1	CRA	927	0.1866	-	7470A	PPB	27 Jul 2023 11:29:07	U	SMPL
HighStd - 1	HighStd	47010	9.7473	-	7470A	PPB	27 Jul 2023 11:31:21	U	SMPL
ChkStd - 1	ChkStd	33081	6.8575	-	7470A	PPB	27 Jul 2023 11:33:37	U	SMPL
PB154473BL - 1	PBW	-39	-0.0138	-	7470A	PPB	27 Jul 2023 11:35:52	U	SMPL
PB154473BS - 1	LCSW	16987	3.5185	-	7470A	PPB	27 Jul 2023 11:38:08	U	SMPL
O3746-01 - 1	A455	1025	0.2069	-	7470A	PPB	27 Jul 2023 11:45:18	U	SMPL
O3746-01DUP - 1	A455DUP	998	0.2013	-	7470A	PPB	27 Jul 2023 11:47:34	U	SMPL
O3746-01MS - 1	A455MS	16751	3.4695	-	7470A	PPB	27 Jul 2023 11:49:51	U	SMPL
O3746-01MSD - 1	A455MSD	16817	3.4832	-	7470A	PPB	27 Jul 2023 11:55:24	U	SMPL
O3767-01 - 1	MMC-COMP	194	0.0345	-	7470A	PPB	27 Jul 2023 11:57:38	U	SMPL
CCV11 - 1	CCV11	23392	4.8473	-	7470A	PPB	27 Jul 2023 11:59:54	U	SMPL
CCB11 - 1	CCB11	196	0.0349	-	7470A	PPB	27 Jul 2023 12:02:10	U	SMPL
O3771-01 - 1	PATERSON-GSMP-COMP	951	0.1915	-	7470A	PPB	27 Jul 2023 12:04:25	U	SMPL
O3746-01LX5 - 1		147	0.0247	-	7470A	PPB	27 Jul 2023 12:06:40	U	SMPL
O3746-01A - 1		17741	3.6749	-	7470A	PPB	27 Jul 2023 12:08:55	U	SMPL
CCV12 - 1	CCV12	23852	4.9428	-	7470A	PPB	27 Jul 2023 12:11:11	U	SMPL
CCB12 - 1	CCB12	214	0.0386	-	7470A	PPB	27 Jul 2023 12:13:26	U	SMPL