


LB 126652

7471B

INSTRUMENT ID: CV1

Linear

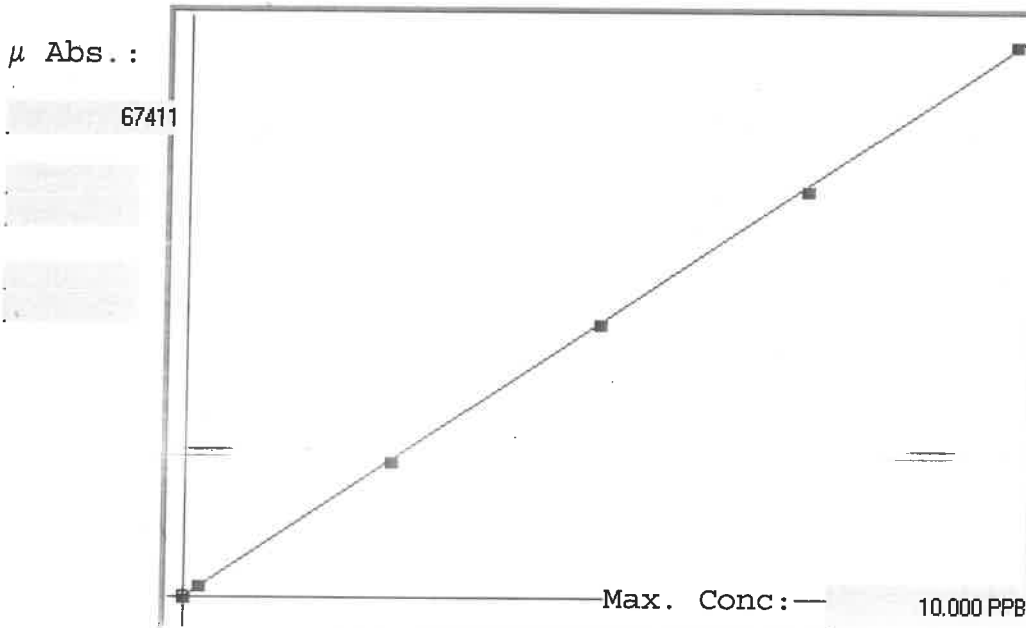

A= 0.0000e+000

B= 1.4921e-004

C= 3.5379e-003

Rho= 0.9999404

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.016	0.016	84	0.000	84					
0.2	0.200	0.214	0.014	1409	0.0 %	1409					
2.5	2.500	2.497	-0.003	16713	0.0 %	16713					
5.0	5.000	4.983	-0.017	33371	0.0 %	33371					
7.5	7.500	7.428	-0.072	49760	0.0 %	49760					
10.0	10.000	10.062	0.062	67411	0.0 %	67411					

17001

LB126652 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 28 Jul 2023 15:28:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	84	-	0.0000	7471B	PPB	28 Jul 2023 15:31:03	S	Std
0.2 - 1	50.2	1409	-	0.2000	7471B	PPB	28 Jul 2023 15:33:19	S	Std
2.5 - 1	52.5	16713	-	2.5000	7471B	PPB	28 Jul 2023 15:35:36	S	Std
5.0 - 1	55	33371	-	5.0000	7471B	PPB	28 Jul 2023 15:37:53	S	Std
7.5 - 1	57.5	49760	-	7.5000	7471B	PPB	28 Jul 2023 15:40:09	S	Std
10.0 - 1	510	67411	-	10.0000	7471B	PPB	28 Jul 2023 15:42:24	S	Std
ICV91 - 1	ICV91	26951	4.0249	-	7471B	PPB	28 Jul 2023 15:45:10	U	SMPL
ICB91 - 1	ICB91	-7	0.0025	-	7471B	PPB	28 Jul 2023 15:47:24	U	SMPL
CCV25 - 1	CCV25	33017	4.9300	-	7471B	PPB	28 Jul 2023 15:49:40	U	SMPL
CCB25 - 1	CCB25	-11	0.0019	-	7471B	PPB	28 Jul 2023 15:51:54	U	SMPL
CRA - 1	CRA	1393	0.2114	-	7471B	PPB	28 Jul 2023 15:54:09	U	SMPL
HighStd - 1	HighStd	66711	9.9574	-	7471B	PPB	28 Jul 2023 15:56:24	U	SMPL
ChkStd - 1	ChkStd	45564	6.8021	-	7471B	PPB	28 Jul 2023 15:58:39	U	SMPL
PB154520BL - 1	PBS	-46	-0.0033	-	7471B	PPB	28 Jul 2023 16:00:55	U	SMPL
PB154520BS - 1	LCSS	22960	3.4294	-	7471B	PPB	28 Jul 2023 16:03:12	U	SMPL
O3795-01 - 1	TOPSOIL-OU3-DENALI-TEMP	2204	0.3324	-	7471B	PPB	28 Jul 2023 16:05:28	U	SMPL
O3797-01 - 1	HANOVER-ST-1	22533	3.3657	-	7471B	PPB	28 Jul 2023 16:07:44	U	SMPL
O3797-04 - 1	HANOVER-ST-2	4841	0.7259	-	7471B	PPB	28 Jul 2023 16:10:01	U	SMPL
O3810-01 - 1	B-P3A	2736	0.4118	-	7471B	PPB	28 Jul 2023 16:12:18	U	SMPL
O3810-02 - 1	B-P3B	1184	0.1802	-	7471B	PPB	28 Jul 2023 16:14:34	U	SMPL
CCV26 - 1	CCV26	33286	4.9701	-	7471B	PPB	28 Jul 2023 16:16:48	U	SMPL
CCB26 - 1	CCB26	35	0.0088	-	7471B	PPB	28 Jul 2023 16:19:04	U	SMPL
O3810-03 - 1	B-P16A	6515	0.9756	-	7471B	PPB	28 Jul 2023 16:21:19	U	SMPL
O3810-04 - 1	B-P16B	13283	1.9855	-	7471B	PPB	28 Jul 2023 16:23:34	U	SMPL
O3810-05 - 1	B-P7A	2820	0.4243	-	7471B	PPB	28 Jul 2023 16:25:50	U	SMPL
O3810-06 - 1	B-P7B	2123	0.3203	-	7471B	PPB	28 Jul 2023 16:28:05	U	SMPL
O3810-07 - 1	B-P15B	763	0.1174	-	7471B	PPB	28 Jul 2023 16:30:21	U	SMPL
O3810-08 - 1	B-P1A	1214	0.1847	-	7471B	PPB	28 Jul 2023 16:32:37	U	SMPL
O3810-09 - 1	B-P1B	213	0.0353	-	7471B	PPB	28 Jul 2023 16:34:53	U	SMPL
O3810-11 - 1	B-P08A	2792	0.4201	-	7471B	PPB	28 Jul 2023 16:37:10	U	SMPL
O3810-12 - 1	B-P08B	772	0.1187	-	7471B	PPB	28 Jul 2023 16:39:27	U	SMPL
O3810-12DUP - 1	B-P08BDUP	826	0.1268	-	7471B	PPB	28 Jul 2023 16:41:42	U	SMPL
CCV27 - 1	CCV27	33110	4.9439	-	7471B	PPB	28 Jul 2023 16:43:57	U	SMPL
CCB27 - 1	CCB27	47	0.0106	-	7471B	PPB	28 Jul 2023 16:46:13	U	SMPL
O3810-12MS - 1	B-P08BMS	24004	3.5852	-	7471B	PPB	28 Jul 2023 16:48:28	U	SMPL
O3810-12MSD - 1	B-P08BMSD	25648	3.8305	-	7471B	PPB	28 Jul 2023 16:50:44	U	SMPL
O3812-01 - 1	WC-1	15638	2.3369	-	7471B	PPB	28 Jul 2023 16:53:00	U	SMPL
O3813-01 - 1	PLAUDERVILLE-1	5020	0.7526	-	7471B	PPB	28 Jul 2023 16:55:15	U	SMPL
O3813-04 - 1	PLAUDERVILLE-2	787	0.1210	-	7471B	PPB	28 Jul 2023 16:57:31	U	SMPL
O3813-07 - 1	PLAUDERVILLE-3	1423	0.2159	-	7471B	PPB	28 Jul 2023 16:59:47	U	SMPL
O3810-12LX5 - 1		126	0.0223	-	7471B	PPB	28 Jul 2023 17:02:03	U	SMPL
O3810-12A - 1		24694	3.6881	-	7471B	PPB	28 Jul 2023 17:04:20	U	SMPL
CCV28 - 1	CCV28	33384	4.9847	-	7471B	PPB	28 Jul 2023 17:08:44	U	SMPL
CCB28 - 1	CCB28	-9	0.0022	-	7471B	PPB	28 Jul 2023 17:10:59	U	SMPL