

LB126794


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

4429E

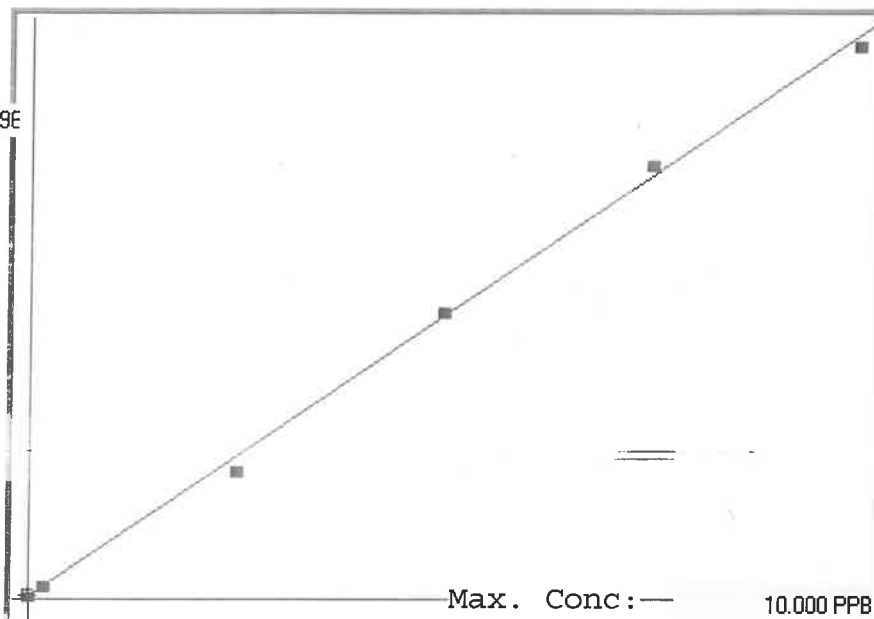

A= 0.0000e+000

B= 2.2260e-004

C= -3.7813e-002

Rho= 0.9991186

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.041	0.041	354	0.000	354	0				
0.2	0.200	0.233	0.033	1217	0.0 %	1217					17
2.5	2.500	2.277	-0.223	10398	0.0 %	10398					-9
5.0	5.000	5.107	0.107	23112	0.0 %	23112					2
7.5	7.500	7.720	0.220	34851	0.0 %	34851					3
10.0	10.000	9.822	-0.178	44296	0.0 %	44296					2

LB126794 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 09 Aug 2023 10:00:54

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	354	-	0.0000	7470A	PPB	09 Aug 2023 10:05:04	S	Std
0.2 - 1	50.2	1217	-	0.2000	7470A	PPB	09 Aug 2023 10:07:21	S	Std
2.5 - 1	52.5	10398	-	2.5000	7470A	PPB	09 Aug 2023 10:09:38	S	Std
5.0 - 1	55	23112	-	5.0000	7470A	PPB	09 Aug 2023 10:11:55	S	Std
7.5 - 1	57.5	34851	-	7.5000	7470A	PPB	09 Aug 2023 10:14:11	S	Std
10.0 - 1	510	44296	-	10.0000	7470A	PPB	09 Aug 2023 10:16:26	S	Std
ICV09 - 1	ICV09	16844	3.7116	-	7470A	PPB	09 Aug 2023 10:19:16	U	SMPL
ICB09 - 1	ICB09	244	0.0165	-	7470A	PPB	09 Aug 2023 10:21:30	U	SMPL
CCV87 - 1	CCV87	21116	4.6626	-	7470A	PPB	09 Aug 2023 10:23:45	U	SMPL
CCB87 - 1	CCB87	272	0.0227	-	7470A	PPB	09 Aug 2023 10:26:00	U	SMPL
CRA - 1	CRA	1061	0.1984	-	7470A	PPB	09 Aug 2023 10:28:15	U	SMPL
HighStd - 1	HighStd	43423	9.6280	-	7470A	PPB	09 Aug 2023 10:30:30	U	SMPL
ChkStd - 1	ChkStd	30740	6.8048	-	7470A	PPB	09 Aug 2023 10:32:45	U	SMPL
PB154710BL - 1	PBW	-4	-0.0387	-	7470A	PPB	09 Aug 2023 10:35:01	U	SMPL
PB154710BS - 1	LCSW	17455	3.8476	-	7470A	PPB	09 Aug 2023 10:39:48	U	SMPL
O3896-03 - 1	50119	24322	5.3762	-	7470A	PPB	09 Aug 2023 10:42:03	U	SMPL
O3903-12 - 1	MW-01W	2003	0.4080	-	7470A	PPB	09 Aug 2023 10:44:19	U	SMPL
O3903-12DUP - 1	MW-01WDUP	1692	0.3388	-	7470A	PPB	09 Aug 2023 10:46:38	U	SMPL
O3903-12MS - 1	MW-01WMS	19066	4.2062	-	7470A	PPB	09 Aug 2023 10:48:55	U	SMPL
O3903-12MSD - 1	MW-01WMSD	18705	4.1259	-	7470A	PPB	09 Aug 2023 10:51:10	U	SMPL
CCV88 - 1	CCV88	22959	5.0728	-	7470A	PPB	09 Aug 2023 10:53:25	U	SMPL
CCB88 - 1	CCB88	311	0.0314	-	7470A	PPB	09 Aug 2023 10:55:40	U	SMPL
O3903-13 - 1	MW-03W	13660	3.0029	-	7470A	PPB	09 Aug 2023 10:57:56	U	SMPL
O3903-14 - 1	MW-04W	3439	0.7277	-	7470A	PPB	09 Aug 2023 11:00:11	U	SMPL
O3903-15 - 1	MW-05W	2094	0.4283	-	7470A	PPB	09 Aug 2023 11:02:26	U	SMPL
O3903-16 - 1	MW-06W	1322	0.2565	-	7470A	PPB	09 Aug 2023 11:04:42	U	SMPL
O3903-17 - 1	MW-07W	805	0.1414	-	7470A	PPB	09 Aug 2023 11:07:01	U	SMPL
O3903-18 - 1	MW-08W	1845	0.3729	-	7470A	PPB	09 Aug 2023 11:09:19	U	SMPL
O3903-19 - 1	MW-09W	2519	0.5229	-	7470A	PPB	09 Aug 2023 11:11:35	U	SMPL
O3903-20 - 1	MW-10W	995	0.1837	-	7470A	PPB	09 Aug 2023 11:13:52	U	SMPL
O3912-01 - 1	COMPOSITE-1	3827	0.8141	-	7470A	PPB	09 Aug 2023 11:16:09	U	SMPL
O3917-05 - 1	FB03	45	-0.0278	-	7470A	PPB	09 Aug 2023 11:18:25	U	SMPL
CCV89 - 1	CCV89	23778	5.2551	-	7470A	PPB	09 Aug 2023 11:20:41	U	SMPL
CCB89 - 1	CCB89	258	0.0196	-	7470A	PPB	09 Aug 2023 11:22:56	U	SMPL
O3917-06 - 1	FB03	321	0.0336	-	7470A	PPB	09 Aug 2023 11:25:11	U	SMPL
O3924-02 - 1	08922	368	0.0441	-	7470A	PPB	09 Aug 2023 11:27:26	U	SMPL
O3903-12LX5 - 1		383	0.0474	-	7470A	PPB	09 Aug 2023 11:29:42	U	SMPL
O3903-12A - 1		19429	4.2870	-	7470A	PPB	09 Aug 2023 11:31:57	U	SMPL
CCV90 - 1	CCV90	23733	5.2451	-	7470A	PPB	09 Aug 2023 11:34:13	U	SMPL
CCB90 - 1	CCB90	313	0.0319	-	7470A	PPB	09 Aug 2023 11:36:32	U	SMPL