

LB126877

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/15/2023 15:16

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.035	0.0	0.111	
ICB1	-0.001	0.0	0.006	
CCV1	1.016	0.0	0.109	
CCB1	0.002	0.0	0.007	
PB154852BS	1.042	0.0	0.111	
O3572-09	0.027	0.0	0.009	
PB154853BL	0.001	0.0	0.007	
PB154853BS	1.043	0.0	0.111	
O3572-03	0.027	0.0	0.009	
PB154852BL	0.001	0.0	0.007	
CCV2	1.018	0.0	0.109	
CCB2	-0.003	0.0	0.006	

N	12
Mean	0.434
SD	0.5271
CV%	121.46

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/15/2023 14:02


Test Phenolics-

Accepted 8/15/2023 14:02

Factor 9.936
Bias 0.006

Coeff. of det. 0.999893

Errors

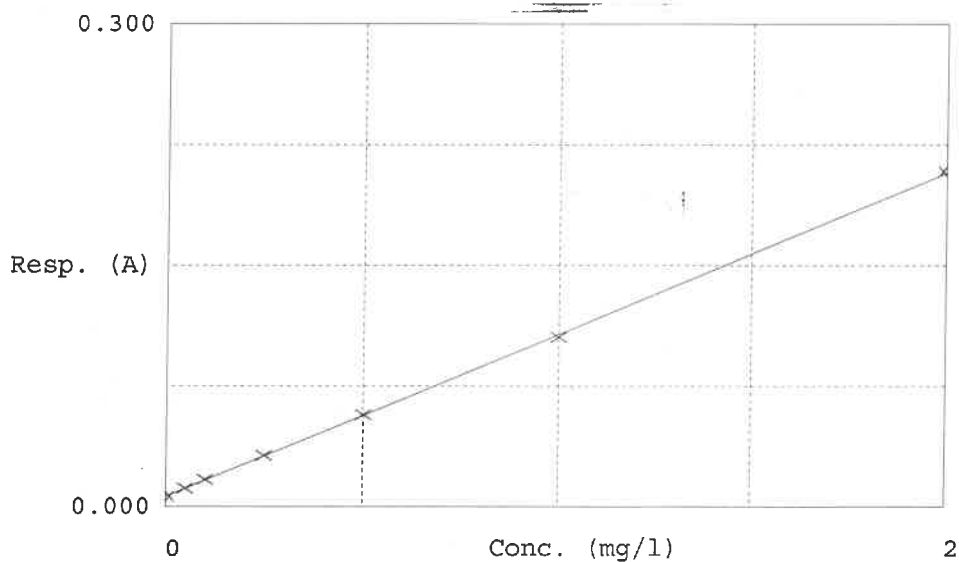

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.00PPM	0.006	-0.0004	0.0000	-
2	Phenol-2	0.011	0.0499	0.0500	-0.2
3	Phenol-2	0.017	0.1035	0.1000	3.5
4	Phenol-2	0.032	0.2530	0.2500	1.2
5	Phenol-2	0.057	0.5035	0.5000	0.7
6	Phenol-2	0.105	0.9839	1.0000	-1.6
7	Phenol-2	0.208	2.0066	2.0000	0.3

RM

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 15 13:36:41 2023

Tue Aug 15 15:09:26 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.00PPM	A	Phenolics-	P	-0.0004	mg/l	8/15/2023 13:58:44
0.05PPM	A	Phenolics-	P	0.0499	mg/l	8/15/2023 13:58:45
0.1PPM	A	Phenolics-	P	0.1035	mg/l	8/15/2023 13:58:46
0.25PPM	A	Phenolics-	P	0.253	mg/l	8/15/2023 13:58:47
0.50PPM	A	Phenolics-	P	0.5035	mg/l	8/15/2023 13:58:48
1.0PPM	A	Phenolics-	P	0.9839	mg/l	8/15/2023 13:58:49
2.0PPM	A	Phenolics-	P	2.0066	mg/l	8/15/2023 13:58:50
ICV1	S	Phenolics-	P	1.0352	mg/l	8/15/2023 14:36:34
ICB1	S	Phenolics-	P	-0.0015	mg/l	8/15/2023 14:36:36
CCV1	S	Phenolics-	P	1.0164	mg/l	8/15/2023 14:36:37
CCB1	S	Phenolics-	P	0.0022	mg/l	8/15/2023 14:36:40
PB154852BS	S	Phenolics-	P	1.0423	mg/l	8/15/2023 14:36:43
O3572-09	S	Phenolics-	P	0.0269	mg/l	8/15/2023 14:46:35
PB154853BL	S	Phenolics-	P	0.0007	mg/l	8/15/2023 14:46:38
PB154853BS	S	Phenolics-	P	1.0432	mg/l	8/15/2023 14:46:40
O3572-03	S	Phenolics-	P	0.0266	mg/l	8/15/2023 14:46:42
PB154852BL	S	Phenolics-	P	0.0014	mg/l	8/15/2023 15:09:21
CCV2	S	Phenolics-	P	1.0177	mg/l	8/15/2023 15:09:23
CCB2	S	Phenolics-	P	-0.0034	mg/l	8/15/2023 15:09:24