


LB126923

7470A

INSTRUMENT ID: CV1

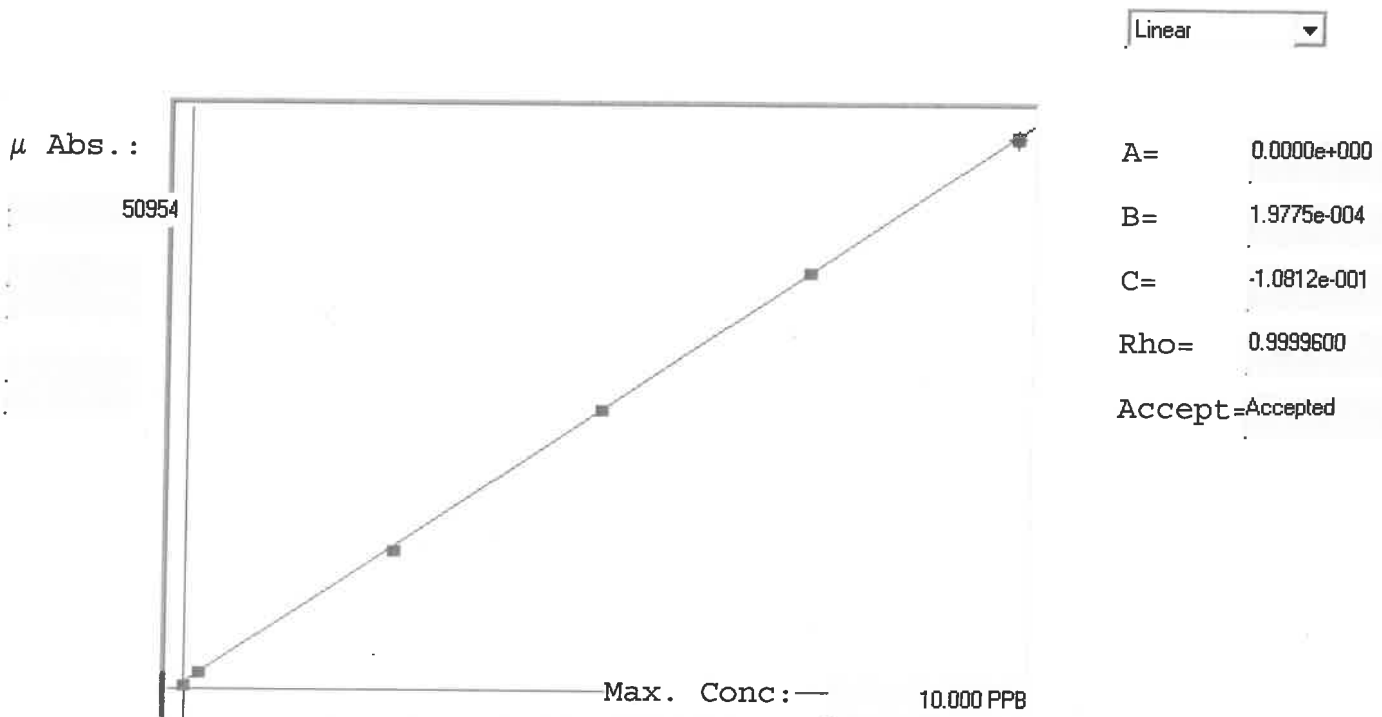

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0 D
0.0	0.000	-0.017	-0.017	460	0.000	460	0				13
0.2	0.200	0.226	0.026	1688	0.0 %	1688					
2.5	2.500	2.454	-0.046	12957	0.0 %	12957					-2
5.0	5.000	5.039	0.039	26028	0.0 %	26028					1
7.5	7.500	7.531	0.031	38629	0.0 %	38629					0
10.0	10.000	9.968	-0.032	50954	0.0 %	50954					0

LB126923 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Aug 2023 13:36:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	460	-	0.0000	7470A	PPB	18 Aug 2023 13:54:29	S	Std
0.2 - 1	50.2	1688	-	0.2000	7470A	PPB	18 Aug 2023 13:56:48	S	Std
2.5 - 1	52.5	12957	-	2.5000	7470A	PPB	18 Aug 2023 13:59:05	S	Std
5.0 - 1	55	26028	-	5.0000	7470A	PPB	18 Aug 2023 14:03:56	S	Std
7.5 - 1	57.5	38629	-	7.5000	7470A	PPB	18 Aug 2023 14:08:46	S	Std
10.0 - 1	516	50954	-	10.0000	7470A	PPB	18 Aug 2023 14:13:43	S	Std
ICV24 - 1	ICV24	19105	3.6698	-	7470A	PPB	18 Aug 2023 14:16:31	U	SMPL
ICB24 - 1	ICB24	326	-0.0437	-	7470A	PPB	18 Aug 2023 14:18:47	U	SMPL
CCV51 - 1	CCV51	26147	5.0624	-	7470A	PPB	18 Aug 2023 14:21:03	U	SMPL
CCB51 - 1	CCB51	352	-0.0385	-	7470A	PPB	18 Aug 2023 14:23:18	U	SMPL
CRA - 1	CRA	1604	0.2091	-	7470A	PPB	18 Aug 2023 14:28:34	U	SMPL
HighStd - 1	HighStd	50648	9.9074	-	7470A	PPB	18 Aug 2023 14:30:49	U	SMPL
ChkStd - 1	ChkStd	35484	6.9087	-	7470A	PPB	18 Aug 2023 14:33:04	U	SMPL
PB154885BL - 1	PBW	493	-0.0106	-	7470A	PPB	18 Aug 2023 14:35:20	U	SMPL
PB154885BS - 1	LCSW	17860	3.4236	-	7470A	PPB	18 Aug 2023 14:40:14	U	SMPL
O4020-03 - 1	E-2	585	0.0076	-	7470A	PPB	18 Aug 2023 14:42:29	U	SMPL
O4022-02 - 1	TP-16	997	0.0890	-	7470A	PPB	18 Aug 2023 14:44:46	U	SMPL
O4022-05 - 1	TP-15	691	0.0285	-	7470A	PPB	18 Aug 2023 14:47:03	U	SMPL
O4022-08 - 1	TP-24	822	0.0544	-	7470A	PPB	18 Aug 2023 14:49:19	U	SMPL
O4030-01 - 1	COMP-1	888	0.0675	-	7470A	PPB	18 Aug 2023 14:51:34	U	SMPL
CCV52 - 1	CCV52	25990	5.0313	-	7470A	PPB	18 Aug 2023 14:53:49	U	SMPL
CCB52 - 1	CCB52	399	-0.0292	-	7470A	PPB	18 Aug 2023 14:56:05	U	SMPL
O4042-02 - 1	TP-376	745	0.0392	-	7470A	PPB	18 Aug 2023 14:58:19	U	SMPL
O4043-02 - 1	E-4	803	0.0507	-	7470A	PPB	18 Aug 2023 15:00:36	U	SMPL
O4043-02DUP - 1	E-4DUP	593	0.0091	-	7470A	PPB	18 Aug 2023 15:02:50	U	SMPL
O4043-02MS - 1	E-4MS	19477	3.7434	-	7470A	PPB	18 Aug 2023 15:05:06	U	SMPL
O4043-02MSD - 1	E-4MSD	19008	3.6507	-	7470A	PPB	18 Aug 2023 15:07:22	U	SMPL
PB154886BL - 1	PBW	481	-0.0130	-	7470A	PPB	18 Aug 2023 15:09:38	U	SMPL
PB154886BS - 1	LCSW	18169	3.4847	-	7470A	PPB	18 Aug 2023 15:11:54	U	SMPL
O4030-02 - 1	8410	631	0.0167	-	7470A	PPB	18 Aug 2023 15:14:11	U	SMPL
O4030-02DUP - 1	8410DUP	629	0.0163	-	7470A	PPB	18 Aug 2023 15:16:28	U	SMPL
O4030-02MS - 1	8410MS	20410	3.9279	-	7470A	PPB	18 Aug 2023 15:24:07	U	SMPL
CCV53 - 1	CCV53	24620	4.7604	-	7470A	PPB	18 Aug 2023 15:26:22	U	SMPL
CCB53 - 1	CCB53	374	-0.0342	-	7470A	PPB	18 Aug 2023 15:28:38	U	SMPL
O4030-02MSD - 1	8410MSD	19775	3.8023	-	7470A	PPB	18 Aug 2023 15:30:52	U	SMPL
O4030-03 - 1	8395	414	-0.0263	-	7470A	PPB	18 Aug 2023 15:33:09	U	SMPL
PB154869TB - 1		402	-0.0286	-	7470A	PPB	18 Aug 2023 15:35:24	U	SMPL
PB154875TB - 1		649	0.0202	-	7470A	PPB	18 Aug 2023 15:37:40	U	SMPL
O4043-02LX5 - 1		683	0.0269	-	7470A	PPB	18 Aug 2023 15:39:56	U	SMPL
O4043-02A - 1		21930	4.2285	-	7470A	PPB	18 Aug 2023 15:42:12	U	SMPL
O4030-02LX5 - 1		442	-0.0207	-	7470A	PPB	18 Aug 2023 15:44:28	U	SMPL
O4030-02A - 1		23779	4.5941	-	7470A	PPB	18 Aug 2023 15:46:45	U	SMPL
CCV54 - 1	CCV54	24071	4.6519	-	7470A	PPB	18 Aug 2023 15:54:47	U	SMPL
CCB54 - 1	CCB54	473	-0.0146	-	7470A	PPB	18 Aug 2023 15:57:03	U	SMPL