

Clear table

Instrument ID: IC-2					Analyst : IZ		Method: 300.0 / 9056A				
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-16_	8/16/23 10:22		IZ/MA
STD2	0.5170	0.7140	0.7080	2.3850	0.6010	1.2930	3.6900	2023-08-16_	8/16/23 10:53		IZ/MA
STD3	0.8610	1.2350	1.2320	4.1330	1.0330	2.0420	6.2110	2023-08-16_	8/16/23 11:23		IZ/MA
STD4	1.0210	1.4590	1.4860	4.9650	1.2440	2.4360	7.4390	2023-08-16_	8/16/23 11:54		IZ/MA
STD5	1.8330	2.8770	2.8550	9.4730	2.3620	4.6420	14.0710	2023-08-16_	8/16/23 12:25		IZ/MA
STD6	3.9840	5.8970	5.8810	19.5220	4.8740	9.8130	29.2620	2023-08-16_	8/16/23 12:55		IZ/MA
STD7	5.0540	7.6180	7.6330	25.5100	6.3830	12.7470	38.3140	2023-08-16_	8/16/23 13:26		IZ/MA
ICV	1.9790	3.0870	3.0980	10.2630	2.5820	5.1620	15.2830	2023-08-16_	8/16/23 13:57		IZ/MA
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-16_	8/16/23 14:28		IZ/MA
CCV	2.0630	3.0590	2.7890	10.0910	2.5060	5.0110	14.9730	2023-08-21_	8/21/23 9:54		IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-21_	8/21/23 10:25		IZ/MA
LB126960BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-21_	8/21/23 10:55		IZ/MA
LB126960BSW	2.0450	3.0500	2.9750	10.1370	2.5260	5.1190	15.0540	2023-08-21_	8/21/23 11:26		IZ/MA
O4032-01X10	0.0000	147.7330	0.0000	1.1480	0.0000	0.9500	1.9900	2023-08-21_	8/21/23 11:57		IZ/MA
O4032-01DLX300	0.0000	3.5360	0.0000	0.0000	0.0000	0.0000	1.1530	2023-08-21_	8/21/23 12:27		IZ/MA
O4074-01	1.3300	68.3740	0.0000	0.0000	0.0000	0.0000	56.3030	2023-08-21_	8/21/23 12:58		IZ/MA
O4074-01MS	4.0100	69.7240	3.1010	10.4500	2.6120	12.1880	72.7160	2023-08-21_	8/21/23 13:29		IZ/MA
O4074-01MSD	3.6990	69.7220	3.0020	10.1320	2.5600	12.0190	71.8110	2023-08-21_	8/21/23 13:59		IZ/MA
CCV	2.1970	3.1070	3.1160	10.3110	2.6280	6.9790	15.2590	2023-08-21_	8/21/23 14:30		IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-21_	8/21/23 15:01		IZ/MA

Clear table


Instrument ID: IC-2		Analyst: IZ		Method: 300.0 / 9056A		file name		date time		Initial wt/ Final Vol		Analyst
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4					
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-08-16	8/16/23 10:22			IZ/MA
STD2	0.5170	0.7140	0.7080	2.3850	0.6010	1.2930	3.6900	2023-08-16	8/16/23 10:53			IZ/MA
STD3	0.8610	1.2350	1.2320	4.1330	1.0330	2.0420	6.2110	2023-08-16	8/16/23 11:23			IZ/MA
STD4	1.0210	1.4590	1.4860	4.9650	1.2440	2.4360	7.4390	2023-08-16	8/16/23 11:54			IZ/MA
STD5	1.8330	2.8770	2.8550	9.4730	2.3620	4.6420	14.0710	2023-08-16	8/16/23 12:25			IZ/MA
STD6	3.9840	5.8970	5.8810	19.5220	4.8740	9.8130	29.2620	2023-08-16	8/16/23 12:55			IZ/MA
STD7	5.0540	7.6180	7.6330	25.5100	6.3830	12.7470	38.3140	2023-08-16	8/16/23 13:26			IZ/MA

ident	True Value F-	True Value CL-		True Value NO2		True Value BR-		True Value NO3		True Value HPO4		True Value SO4	
		Relative Error	CL-	Relative Error	NO2	Relative Error	BR-	Relative Error	NO3	Relative Error	HPO4	Relative Error	SO4
STD1	0.0000		0.0000		0.0000		0.0000		0.0000		0.0000		0.0000
STD2	0.4000		0.6000		0.6000		2.0000		0.5000		1.0000		3.0000
STD3	0.8000		1.2000		1.2000		4.0000		1.0000		2.0000		6.0000
STD4	1.0000		1.5000		1.5000		5.0000		1.2500		2.5000		7.5000
STD5	2.0000		3.0000		3.0000		10.0000		2.5000		5.0000		15.0000
STD6	4.0000		6.0000		6.0000		20.0000		5.0000		10.0000		30.0000
STD7	5.0000		7.5000		7.5000		25.0000		6.2500		12.5000		37.0000

ident	Relative Error F-	Relative Error CL-		Relative Error NO2		Relative Error BR-		Relative Error NO3		Relative Error HPO4		Relative Error SO4	
		Relative Error	CL-	Relative Error	NO2	Relative Error	BR-	Relative Error	NO3	Relative Error	HPO4	Relative Error	SO4
STD1													
STD2	29.2500		19.0000		18.0000		19.2500		20.2000		29.3000		23.0000
STD3	7.6250		2.9167		2.6667		3.3250		3.3000		2.1000		3.5167
STD4	2.1000		-2.7333		-0.9333		-0.7000		-0.4800		-2.5600		-0.8133
STD5	-8.3500		-4.1000		-4.8333		-5.2700		-5.5200		-7.1600		-6.1933
STD6	-0.4000		-1.7167		-1.9833		-2.3900		-2.5200		-1.8700		-2.4600
STD7	1.0800		1.5733		1.7733		2.0400		2.1280		1.9760		3.5514

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.0928952 \cdot A + 4.37011$
 RSD: 4.408 %
 Correlation coefficient: 0.998941

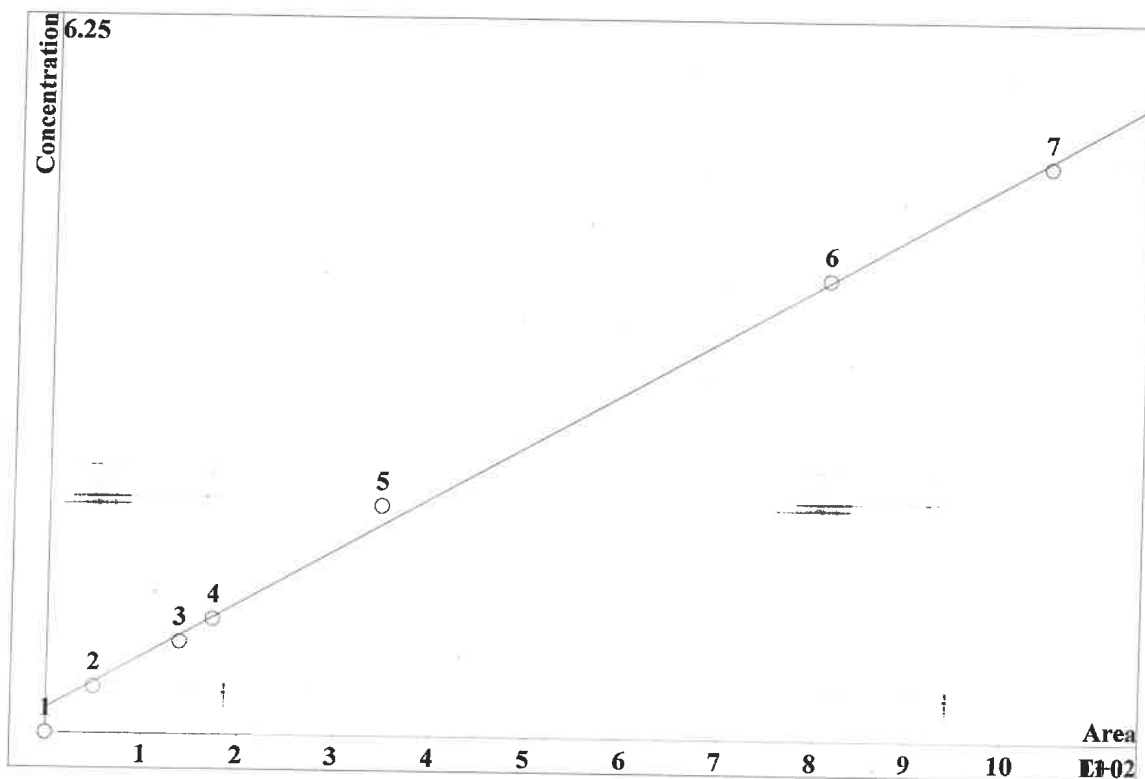


K3 = 0 K2 = 0 K1 = 0.0928952 K0 = 4.37011
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	0.7326	49.05	0.4	20	6.387	
3	1.771	138.4	0.8	20	6.387	
4	2.174	172.8	1	20	6.387	
5	4.648	347.5	2	20	6.387	
6	11.31	810.7	4	20	6.387	
7	14.93	1041	5	20	6.387	

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.128621 \cdot A + 3.39946$
 RSD: 3.576 %
 Correlation coefficient: 0.999303

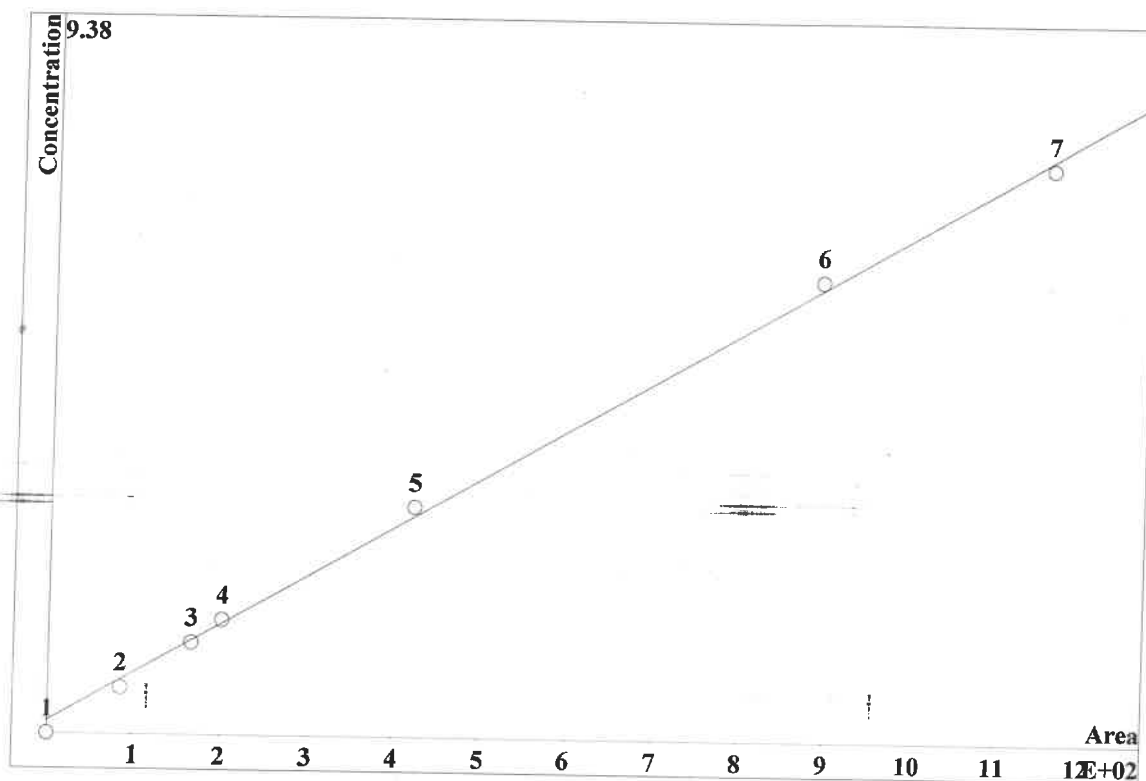


K3 = 0 K2 = 0 K1 = 0.128621 K0 = 3.39946
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.955	84.61	0.6	20	8.96		
3	11.74	165.7	1.2	20	8.96		
4	14.85	200.5	1.5	20	8.96		
5	30.42	420.9	3	20	8.96		
6	65.28	890.5	6	20	8.96		
7	87.19	1158	7.5	20	8.96		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.058091 \cdot A + 3.6939$
 RSD: 3.919 %
 Correlation coefficient: 0.999163

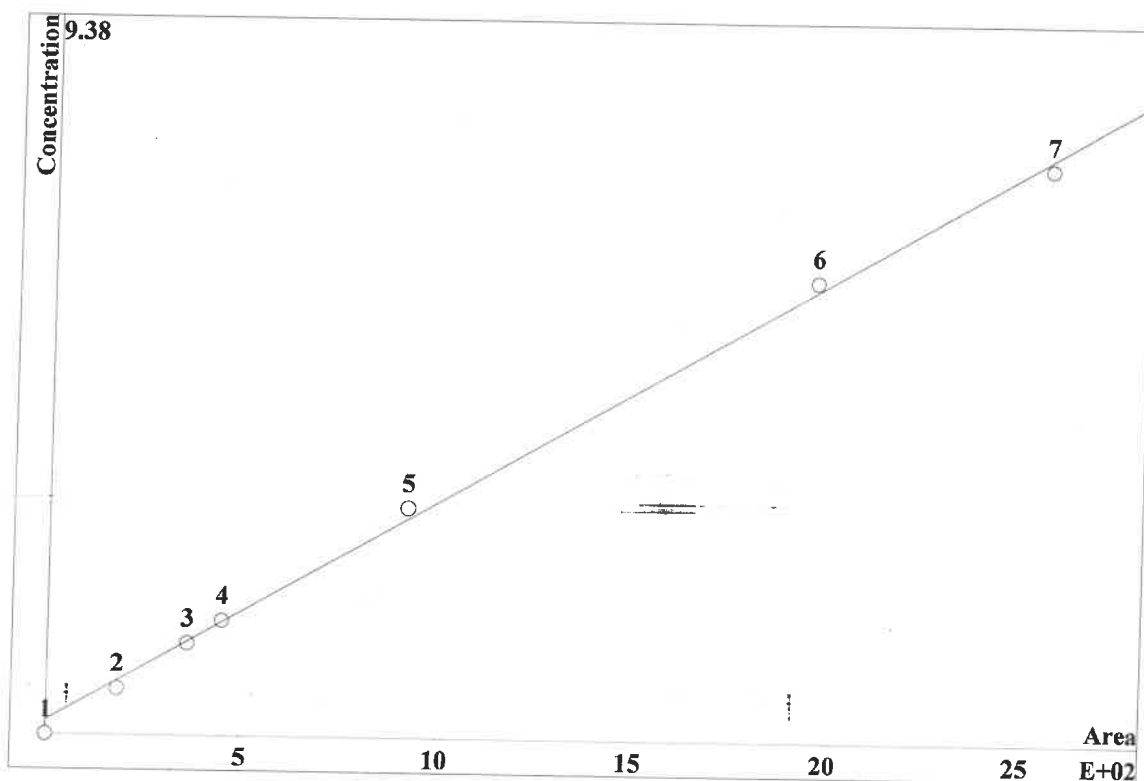


K3 = 0 K2 = 0 K1 = 0.058091 K0 = 3.6939
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.28	182	0.6	20	10.79		
3	20.32	360.6	1.2	20	10.79		
4	25.63	448	1.5	20	10.79		
5	50.59	919.3	3	20	10.79		
6	105.7	1961	6	20	10.79		
7	137	2564	7.5	20	10.79		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.286569 \cdot A + 13.7702$
 RSD: 4.416 %
 Correlation coefficient: 0.998937

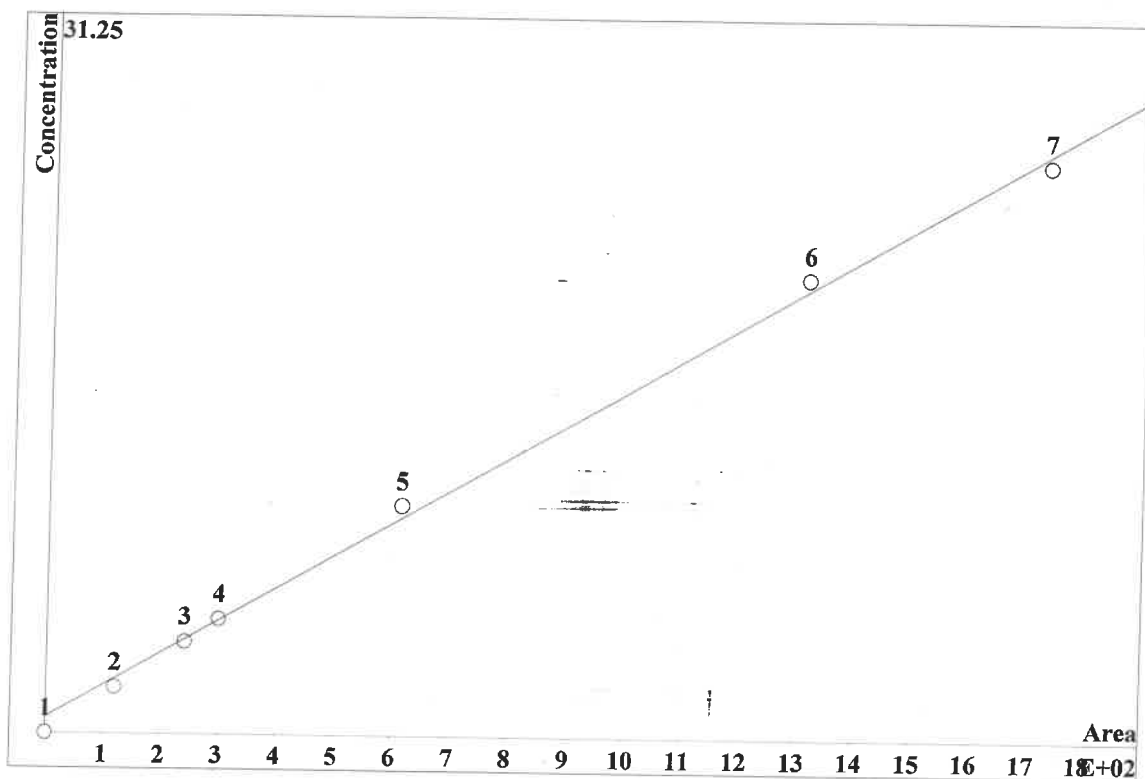


K3 = 0 K2 = 0 K1 = 0.286569 K0 = 13.7702
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0		0	0	0		0
2	6.113	119.3		2	20		13.99
3	12.32	240.4		4	20		13.99
4	15.71	298.5		5	20		13.99
5	32.71	613.1		10	20		13.99
6	71.72	1314		20	20		13.99
7	96.98	1732		25	20		13.99

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.0501685 \cdot A + 3.33819$
 RSD: 4.620 %
 Correlation coefficient: 0.998836

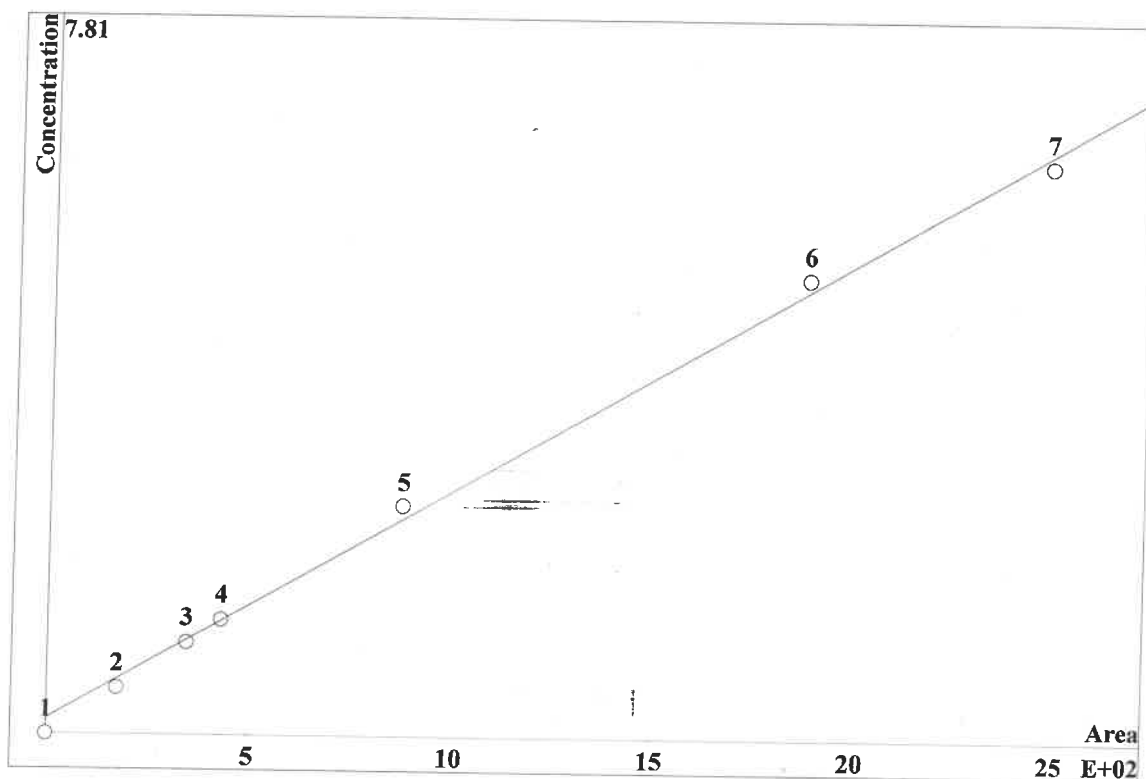


K3 = 0 K2 = 0 K1 = 0.0501685 K0 = 3.33819
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.242	174.3	0.5	20	17.17		
3	14.43	345.2	1	20	17.17		
4	18.31	429.4	1.25	20	17.17		
5	37.66	874.9	2.5	20	17.17		
6	81.62	1877	5	20	17.17		
7	109.9	2478	6.25	20	17.17		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.0589348 \cdot A + 15.5986$
 RSD: 5.243 %
 Correlation coefficient: 0.998501

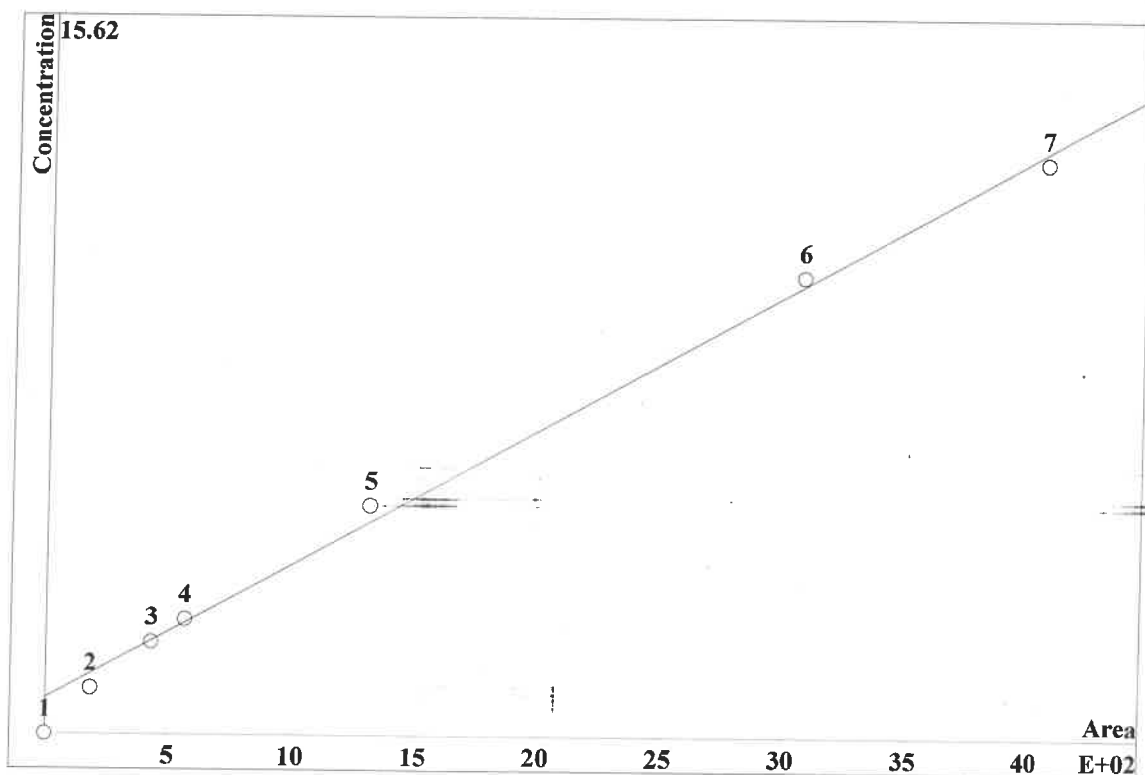


K3 = 0 K2 = 0 K1 = 0.0589348 K0 = 15.5986
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	4.422	183.4	1	20	22.61	
3	10.13	428.3	2	20	22.61	
4	13.32	562.1	2.5	20	22.61	
5	31.64	1310	5	20	22.61	
6	78.15	3065	10	20	22.61	
7	106.3	4061	12.5	20	22.61	

DES

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-081623.mtw
 Equation: $Q = 0.164503 \cdot A + 19.1769$
 RSD: 4.899 %
 Correlation coefficient: 0.998691

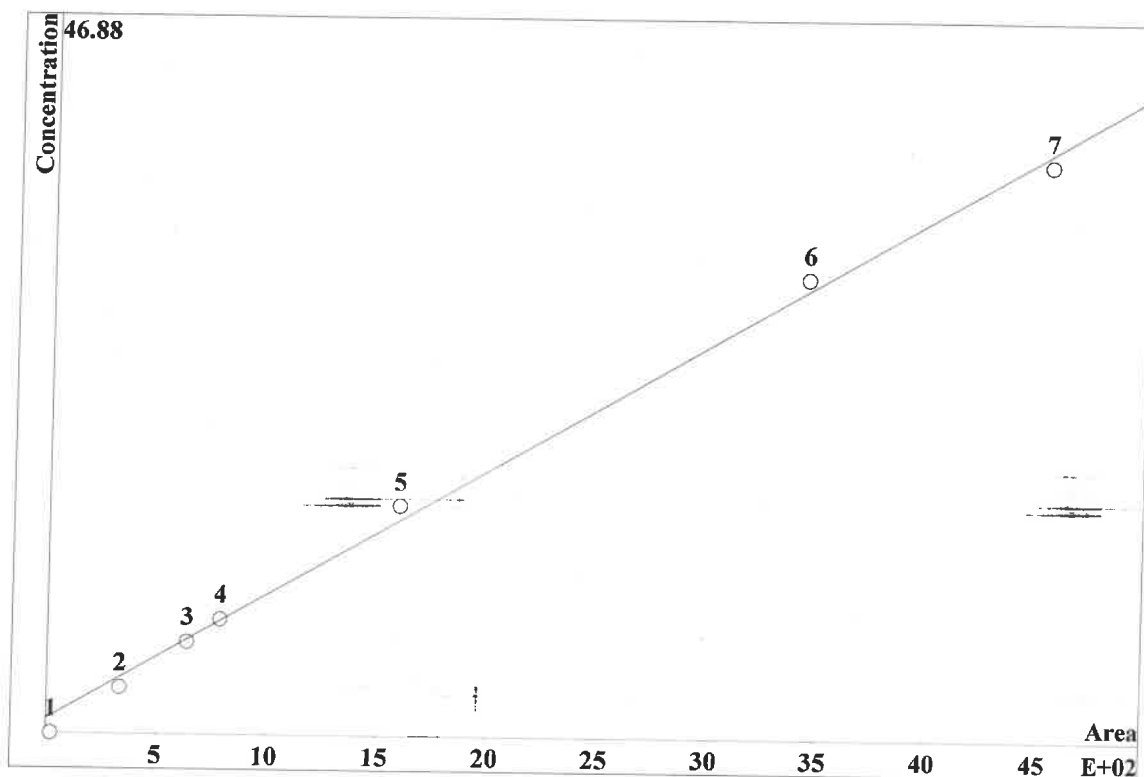

K3 = 0 K2 = 0 K1 = 0.164503 K0 = 19.1769
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0.5497		23.22	0	20		24.69
2	10.86		333.6	3	20		24.69
3	21.23		638.5	6	20		24.69
4	26.68		787.8	7.5	20		24.69
5	54.98		1594	15	20		24.69
6	121		3441	30	20		24.69
7	161.9		4542	37.5	20		24.69

Report date: 8/16/2023 2:03:34 PM
Printed by: wet


Ident: STD1
Analysis from: 8/16/2023 10:22:38 AM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35148

Last save: 8/16/2023 1:23:

SAMPLE:
:
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

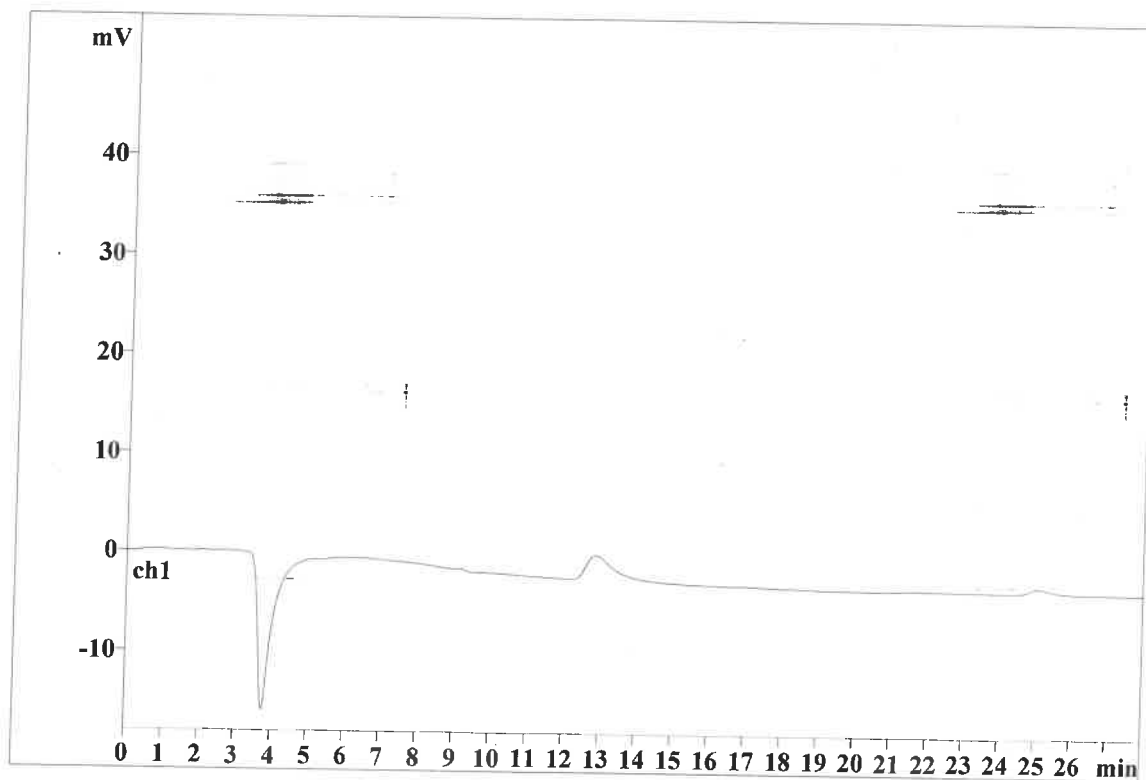

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:10:03 PM
Printed by: wet


Ident: STD2
Analysis from: 8/16/2023 10:53:16 AM
File: _2023-08-16_

Last save: 8/16/2023 2:09:59 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35149

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

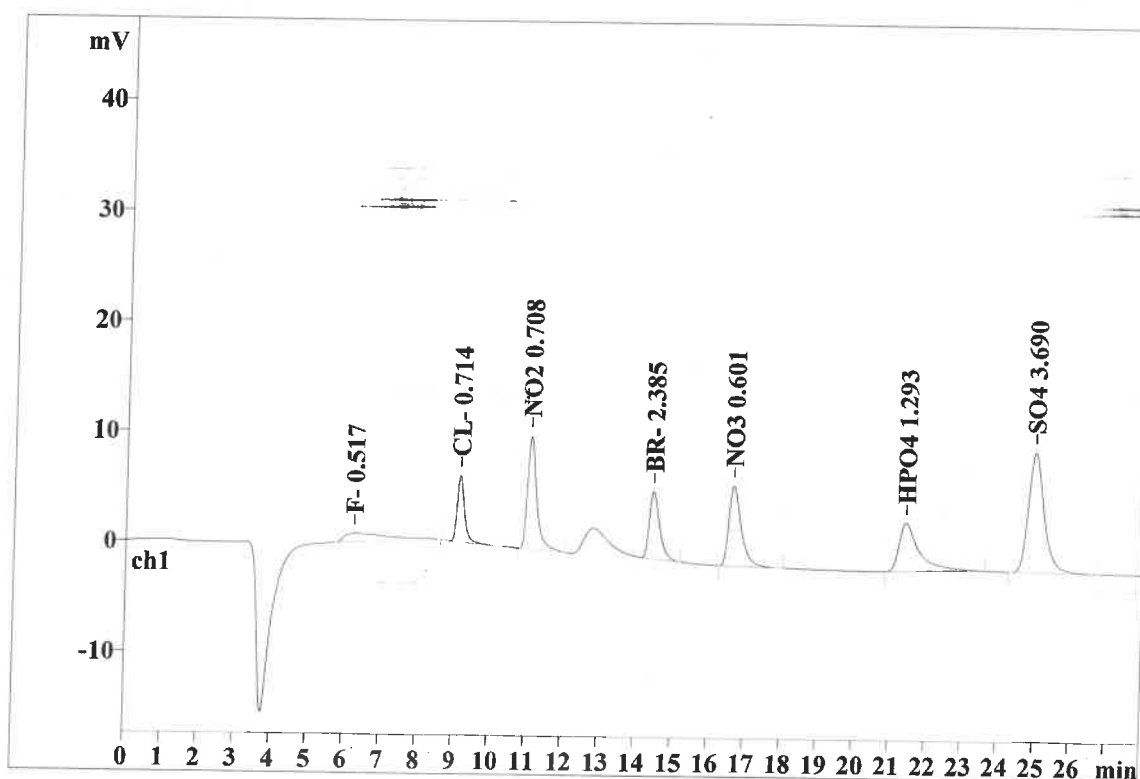

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.22	1.263	0.77	1.68	64.363	5.71
2	9.15	0.202	5.97	13.09	84.592	7.51
3	11.10	0.249	10.27	22.51	180.241	15.99
4	14.45	0.291	6.10	13.38	118.418	10.51
5	16.64	0.352	7.24	15.87	173.141	15.36
6	21.41	0.510	4.40	9.65	174.109	15.45
7	24.97	0.451	10.86	23.80	332.074	29.47
7	28.00	0.474	45.62	99.98	1126.939	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:03:50 PM
Printed by: wet


Ident: STD3
Analysis from: 8/16/2023 11:23:54 AM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35150

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

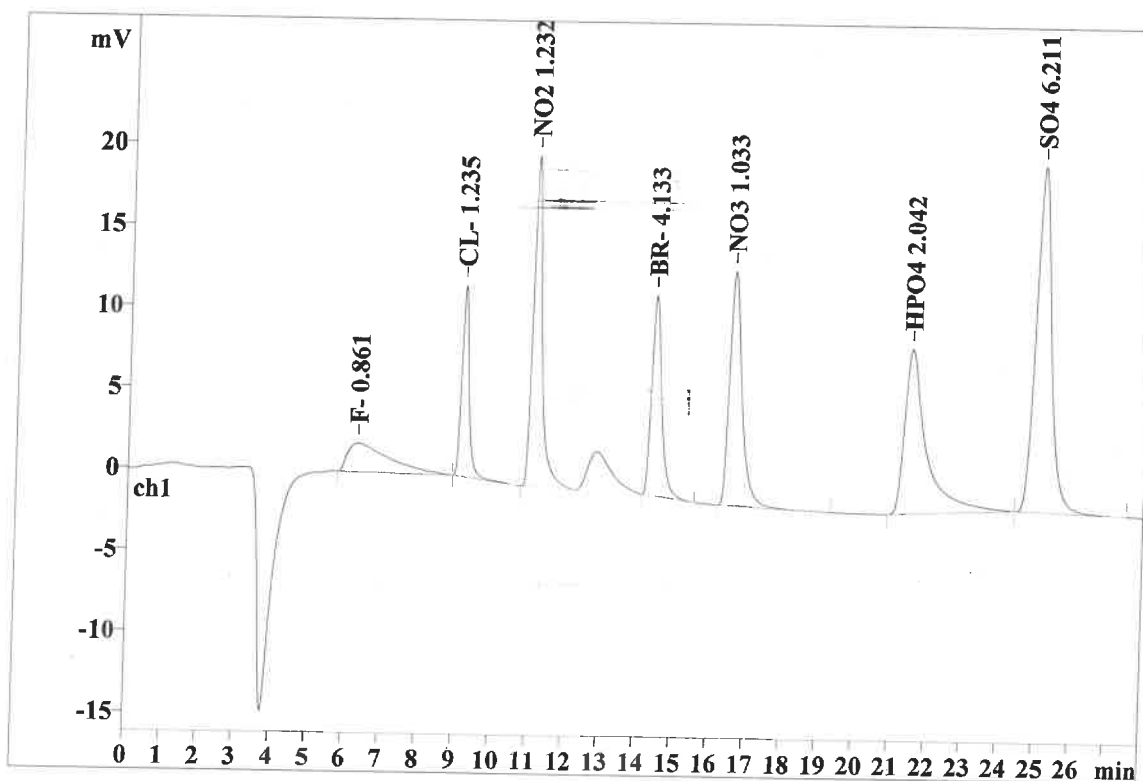

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.30	1.200	1.77	1.92	138.395	5.97
2	9.16	0.203	11.74	12.77	165.670	7.15
3	11.09	0.249	20.32	22.11	360.599	15.56
4	14.42	0.289	12.32	13.40	240.371	10.37
5	16.57	0.349	14.42	15.69	345.201	14.90
6	21.50	0.527	10.13	11.01	428.346	18.49
7	25.06	0.445	21.23	23.09	638.538	27.56
7	28.00	0.466	91.93	99.99	2317.119	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:03:57 PM
Printed by: wet


Ident: STD4
Analysis from: 8/16/2023 11:54:33 AM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35151

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

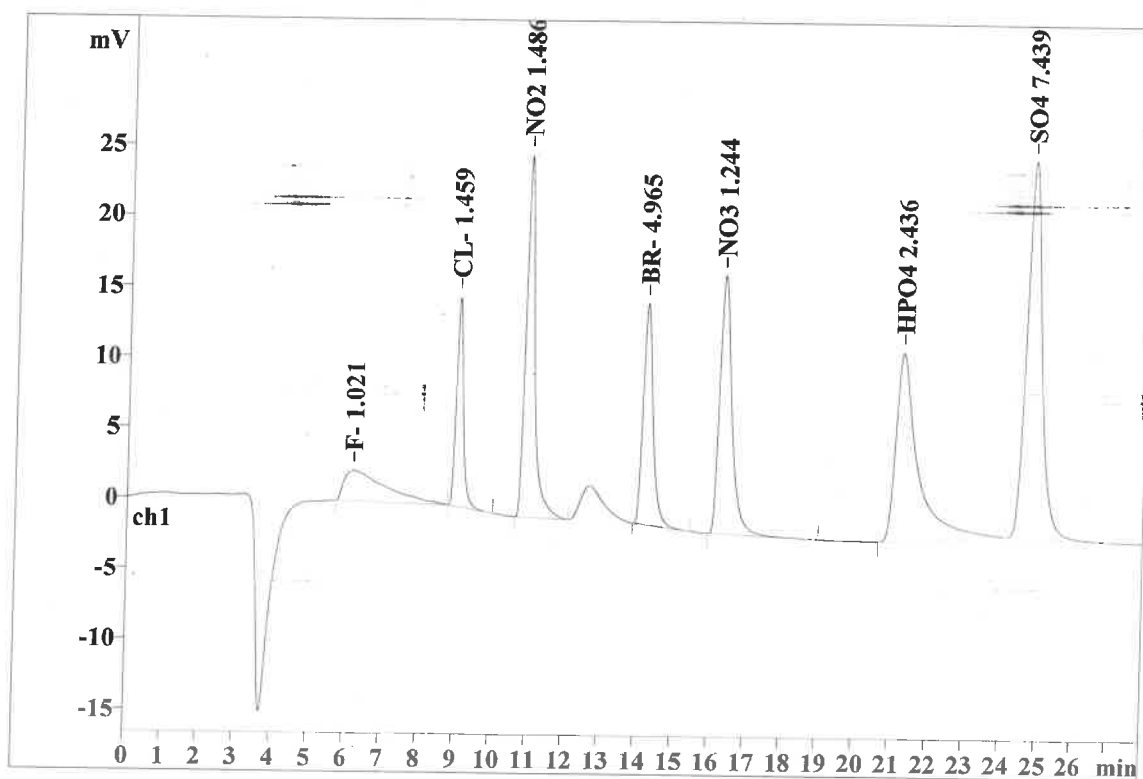

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.20	1.212	2.17	1.86	172.837	5.96
2	9.05	0.198	14.85	12.73	200.472	6.92
3	10.94	0.246	25.63	21.97	447.962	15.45
4	14.21	0.281	15.71	13.46	298.465	10.30
5	16.31	0.342	18.31	15.69	429.367	14.81
6	21.28	0.525	13.32	11.42	562.078	19.39
7	24.80	0.437	26.68	22.87	787.818	27.18
7	28.00	0.463	116.66	100.00	2898.999	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:04:06 PM
Printed by: wet


Ident: STD5
Analysis from: 8/16/2023 12:25:10 PM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35152

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

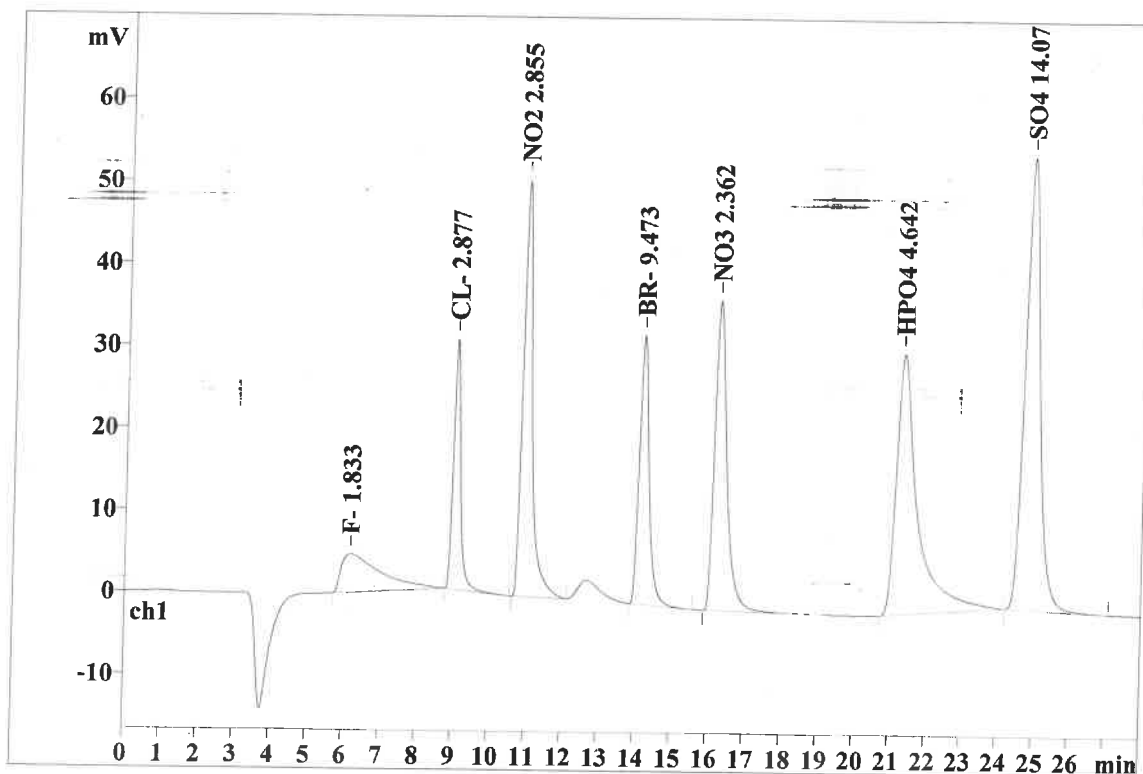

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.17	1.102	4.65	1.91	347.494	5.72
2	9.05	0.198	30.42	12.54	420.877	6.92
3	10.92	0.254	50.59	20.85	919.300	15.12
4	14.17	0.276	32.72	13.48	613.054	10.08
5	16.23	0.338	37.66	15.52	874.945	14.39
6	21.31	0.518	31.64	13.04	1310.484	21.55
7	24.84	0.430	54.98	22.66	1594.100	26.22
7	28.00	0.445	242.65	100.00	6080.254	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:04:13 PM
Printed by: wet


Ident: STD6
Analysis from: 8/16/2023 12:55:48 PM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35153

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

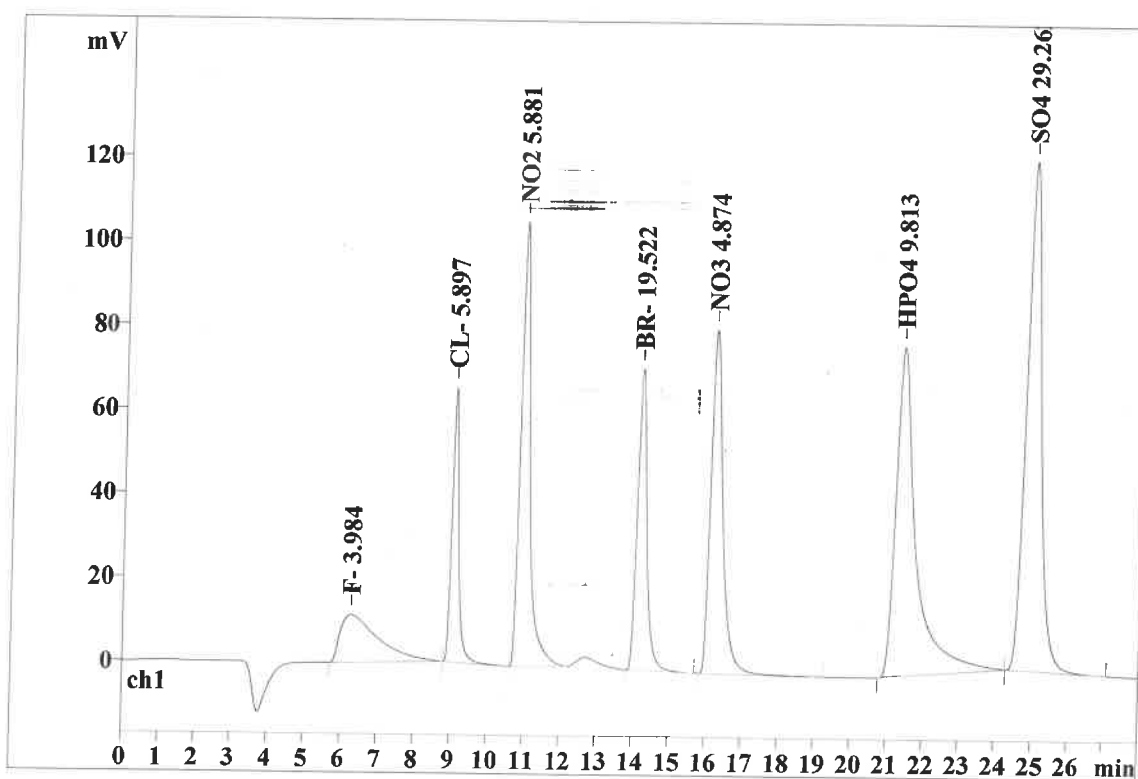

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.27	1.080	11.30	2.11	810.735	6.07
2	9.06	0.196	65.28	12.21	890.487	6.67
3	10.91	0.259	105.66	19.76	1961.217	14.68
4	14.17	0.269	71.72	13.41	1314.401	9.84
5	16.18	0.333	81.62	15.26	1876.691	14.05
6	21.35	0.494	78.15	14.62	3065.492	22.95
7	24.91	0.423	121.00	22.63	3441.098	25.76
7	28.00	0.436	534.74	100.00	13360.120	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 2:04:21 PM
Printed by: wet


Ident: STD7
Analysis from: 8/16/2023 1:26:26 PM
File: _2023-08-16_

Last save: 8/16/2023 1:57:43 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35154

Last save: 8/16/2023 1:23:

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

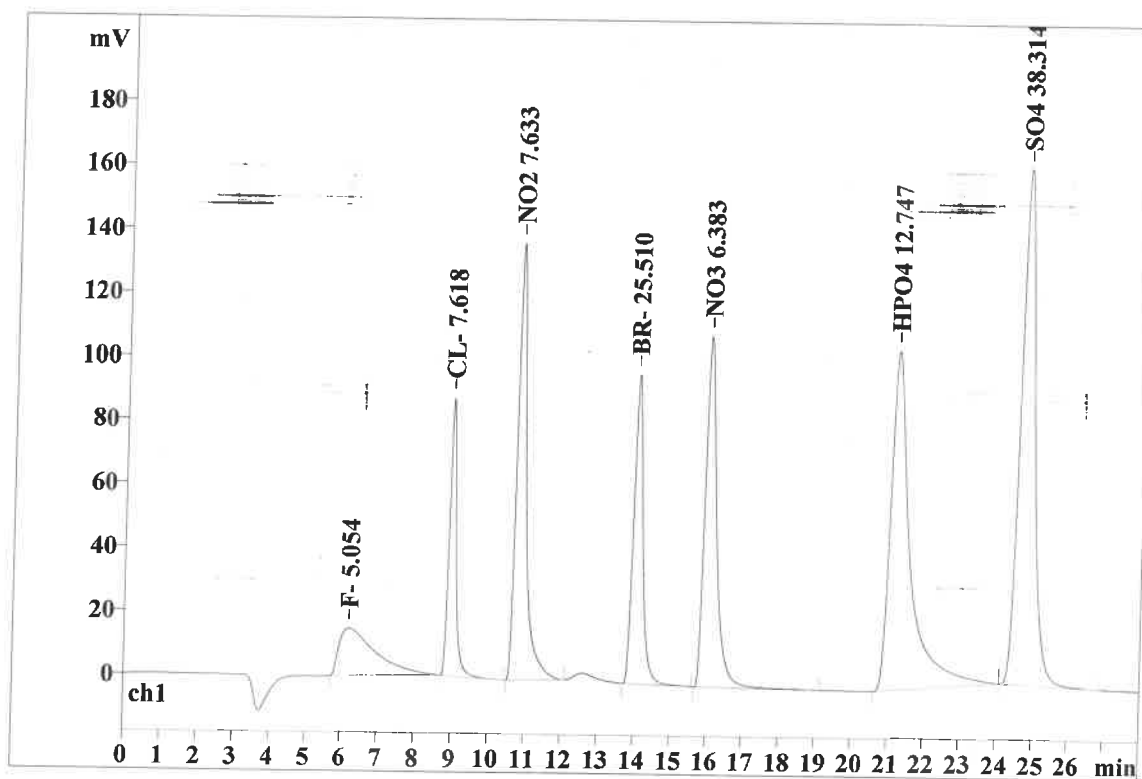

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.19	1.037	14.93	2.09	1041.140	5.92
2	8.97	0.191	87.19	12.21	1158.114	6.59
3	10.79	0.261	137.02	19.18	2564.315	14.59
4	14.02	0.261	96.98	13.58	1732.292	9.86
5	15.99	0.326	109.94	15.39	2478.120	14.10
6	21.18	0.482	106.32	14.88	4061.000	23.10
7	24.71	0.418	161.89	22.66	4541.624	25.84
7	28.00	0.425	714.26	100.00	17576.604	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 3:37:11 PM
Printed by: wet


Ident: ICV
Analysis from: 8/16/2023 1:57:04 PM
File: _2023-08-16_

Last save: 8/16/2023 2:25:04 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35155

Last save: 8/16/2023 1:54:

SAMPLE:
: IZ/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

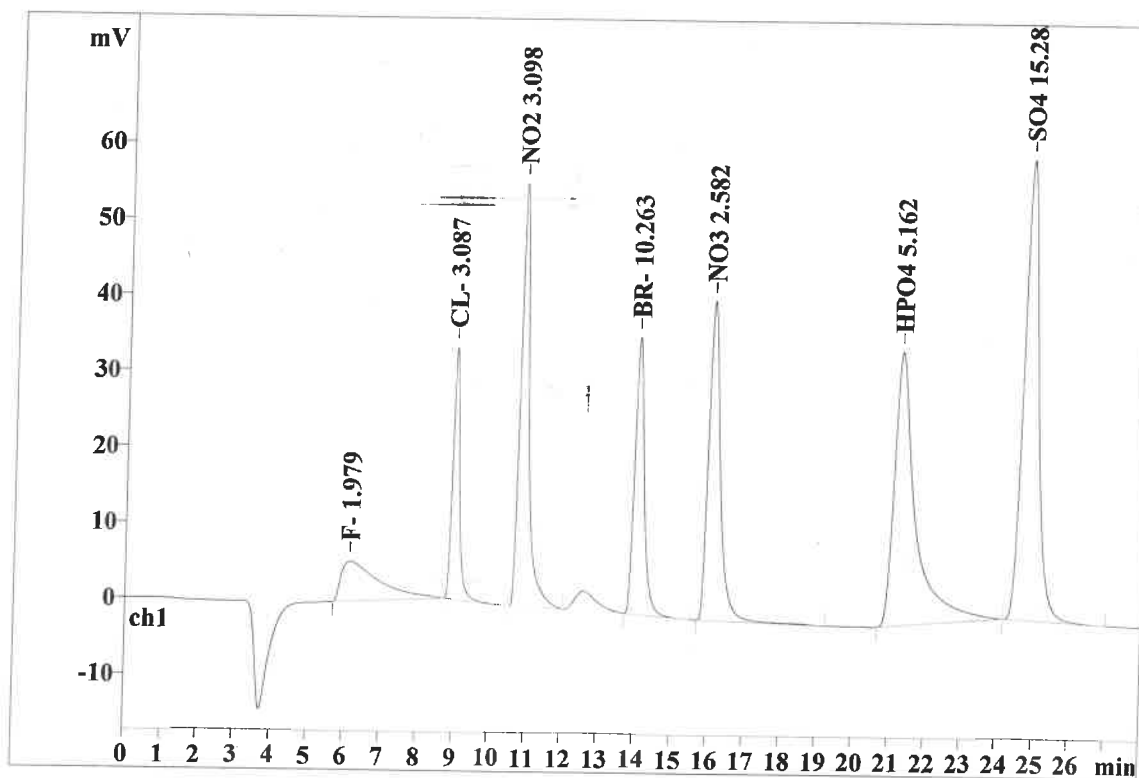

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.15	1.060	5.23	1.94	379.086	5.66
2	8.99	0.196	33.29	12.35	453.564	6.77
3	10.83	0.251	55.78	20.69	1002.940	14.98
4	14.04	0.270	36.55	13.56	668.204	9.98
5	16.05	0.330	42.09	15.61	962.703	14.38
6	21.26	0.515	36.04	13.37	1486.975	22.21
7	24.78	0.427	60.61	22.48	1741.500	26.01
7	28.00	0.435	269.60	100.00	6694.973	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/16/2023 3:37:19 PM
Printed by: wet


Ident: ICB
Analysis from: 8/16/2023 2:28:05 PM
File: _2023-08-16_

Last save: 8/16/2023 2:56:05 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35156

Last save: 8/16/2023 1:54:

SAMPLE:
: IZ/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

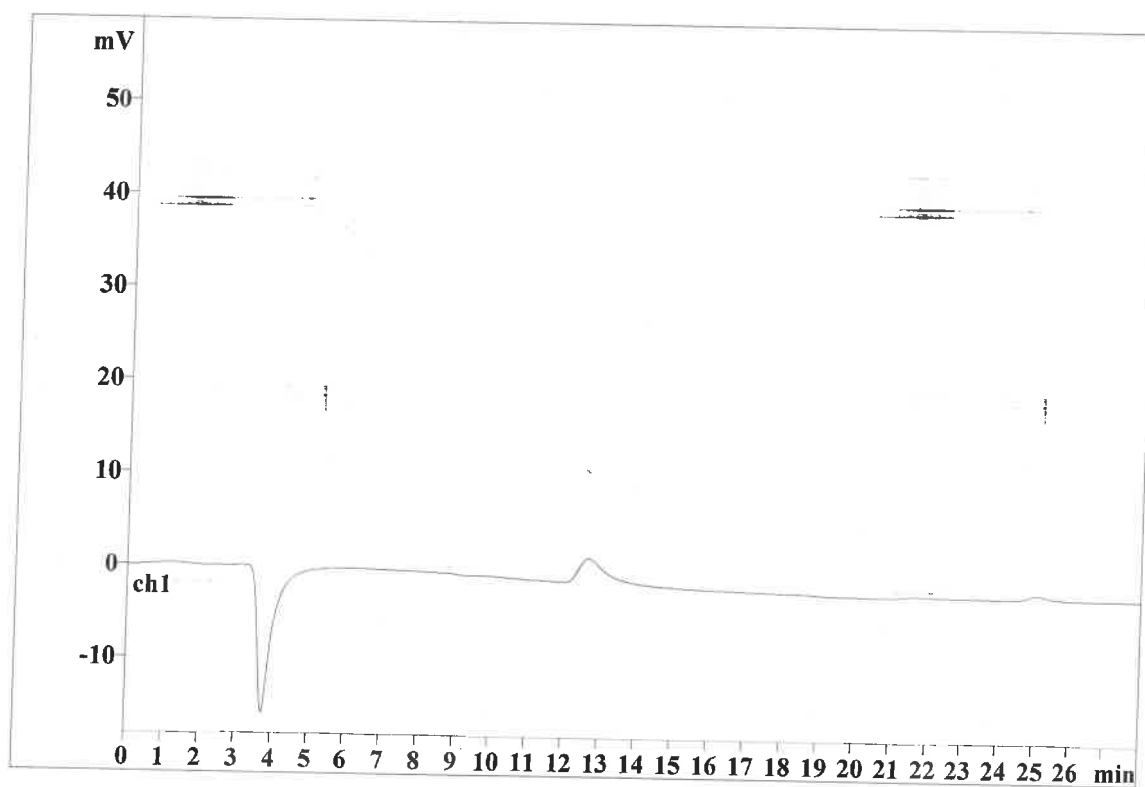

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:37:34 PM
Printed by: wet


Ident: CCV
Analysis from: 8/21/2023 2:30:27 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35215

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

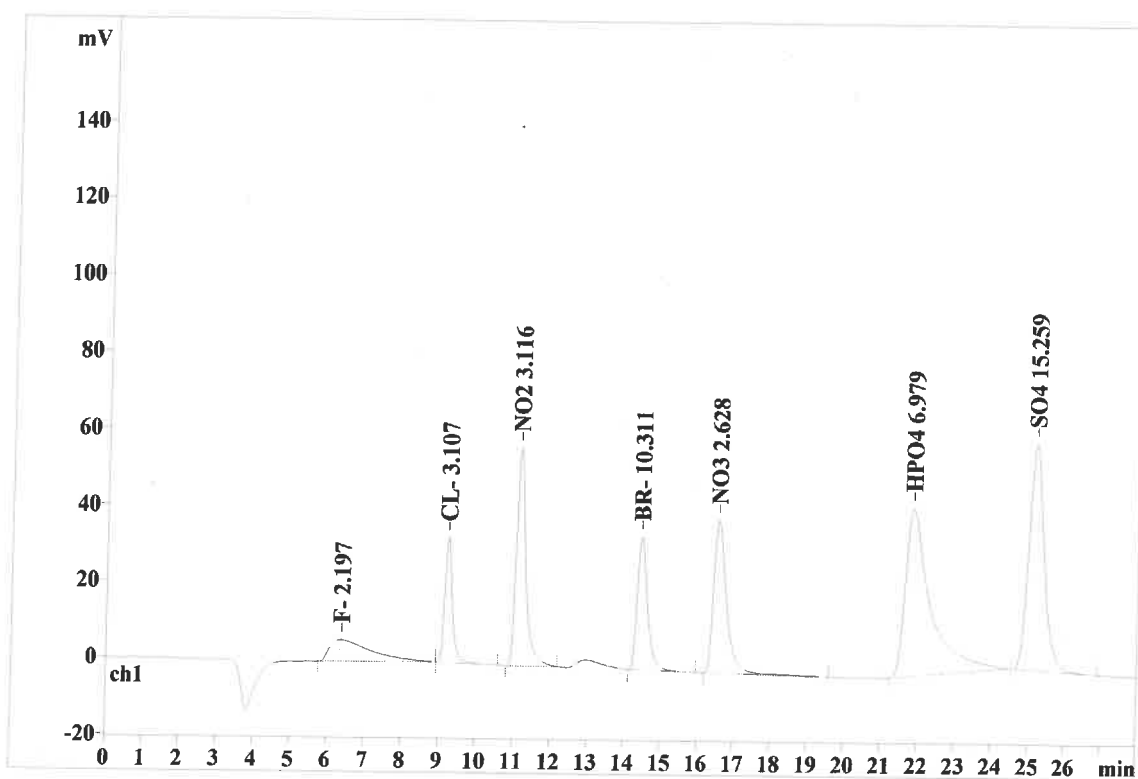

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.38	1.163	5.55	2.04	425.957	5.7
2	9.22	0.204	32.46	11.96	456.651	6.1
3	11.14	0.254	56.65	20.88	1009.263	13.6
4	14.43	0.288	34.47	12.70	671.539	9.0
5	16.53	0.353	39.78	14.66	981.071	13.2
6	21.83	0.609	43.64	16.08	2103.612	28.4
7	25.14	0.442	58.79	21.67	1738.531	23.5
7	28.00	0.473	271.34	100.00	7386.623	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:37:48 PM
Printed by: wet


Ident: CCB
Analysis from: 8/21/2023 3:01:05 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35216

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

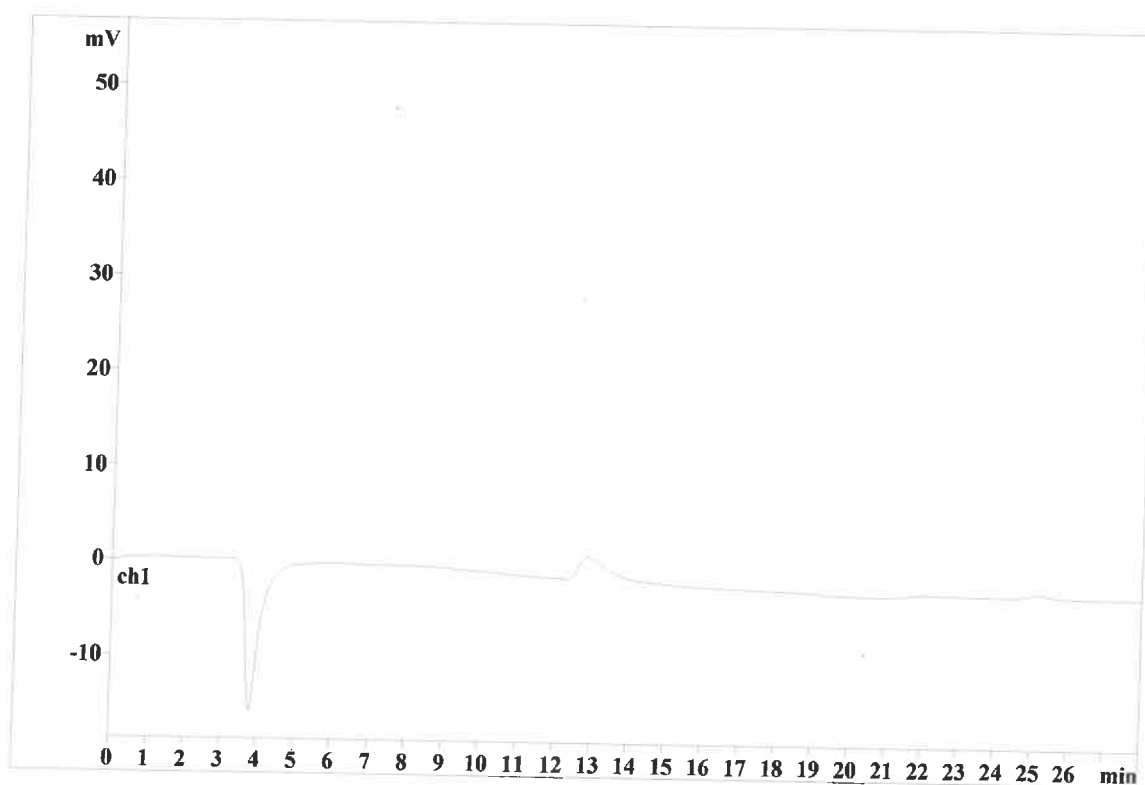

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:34:14 PM
Printed by: wet


Ident: LB126960BLW
Analysis from: 8/21/2023 10:55:58 AM
File: _2023-08-21_

Last save: 8/22/2023 1:32:34 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35208

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

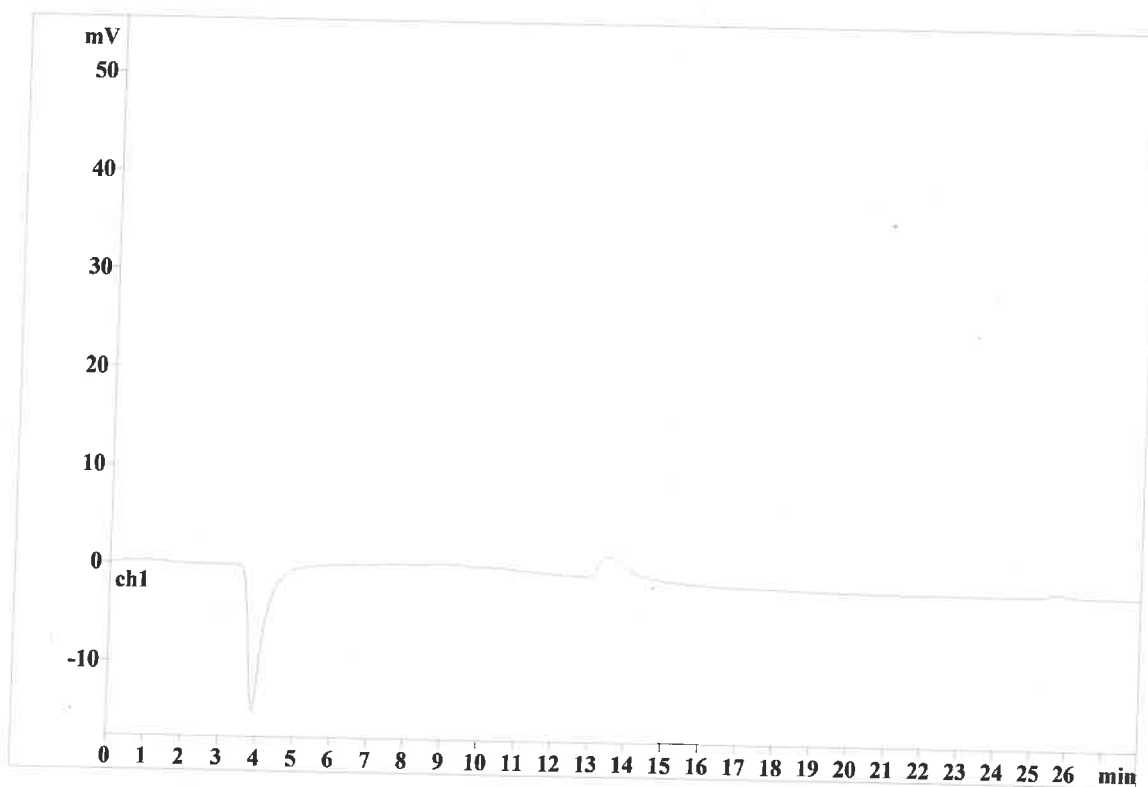

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:34:51 PM
Printed by: wet


Ident: LB126960BSW
Analysis from: 8/21/2023 11:26:36 AM
File: _2023-08-21_

Last save: 8/22/2023 1:34:48 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35209

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

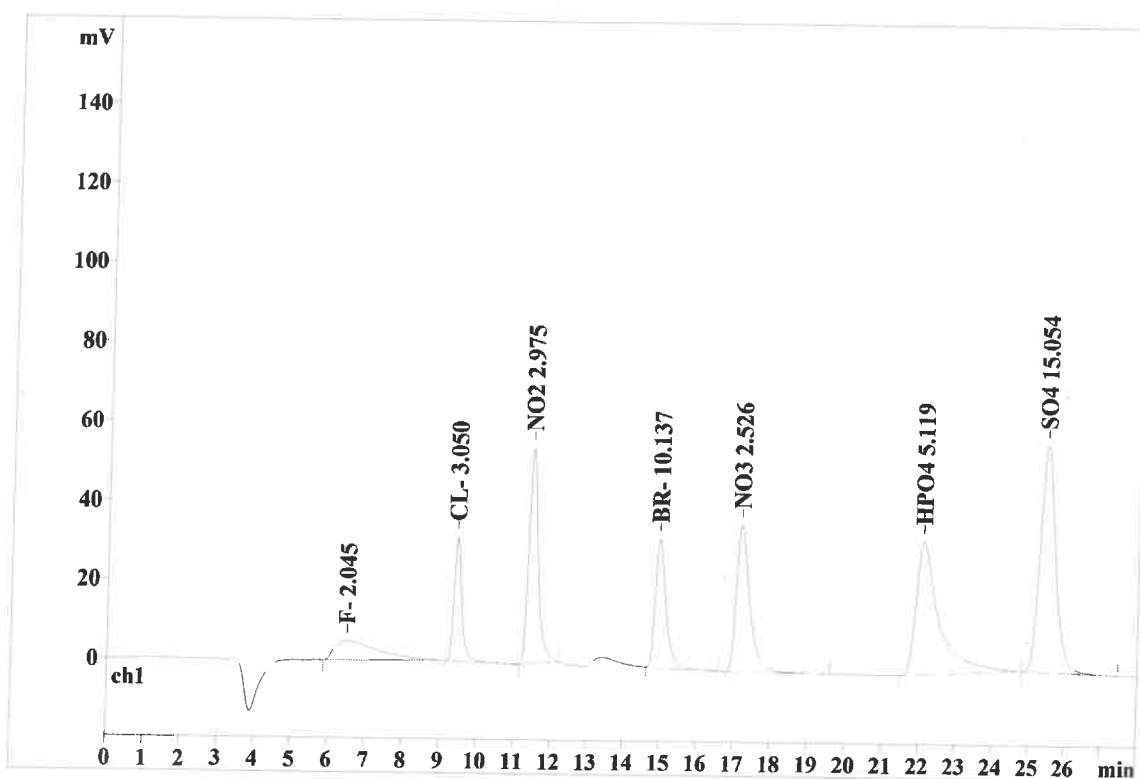

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.49	1.241	4.83	1.93	393.337	5.9
2	9.44	0.209	31.05	12.43	447.856	6.8
3	11.45	0.260	54.19	21.71	960.596	14.5
4	14.94	0.300	32.39	12.97	659.446	10.0
5	17.15	0.372	36.84	14.76	940.579	14.2
6	22.09	0.560	33.41	13.38	1472.400	22.3
7	25.44	0.448	56.97	22.82	1713.721	26.0
7	28.00	0.484	249.68	100.00	6587.935	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:36:06 PM
 Printed by: wet


Ident: 04032-01X10
 Analysis from: 8/21/2023 11:57:14 AM
 File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
 Run operator: wet
 Analysis number: 35210

Last save: 8/17/2023 8:4

SAMPLE:
 : IZ/MA
 Vial number: 20
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

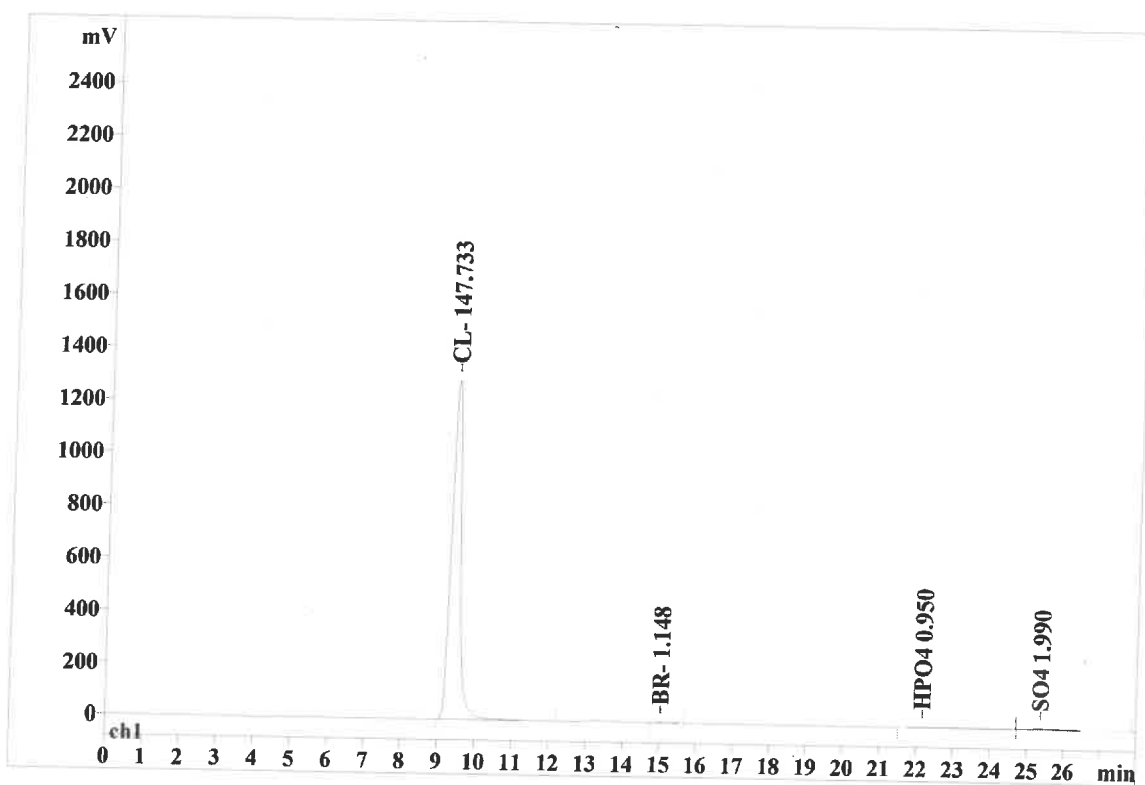

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	0.00	0.000	0.00	0.00	0.000	0.0
2	9.39	0.260	1289.04	99.52	22945.302	99.0
3	0.00	0.000	0.00	0.00	0.000	0.0
4	15.02	0.284	1.72	0.13	32.069	0.1
5	0.00	0.000	0.00	0.00	0.000	0.0
6	22.16	0.954	0.84	0.06	57.724	0.2
7	25.36	0.487	3.66	0.28	125.352	0.5
7	28.00	0.284	1295.27	100.00	23160.446	100.0

This report has been created by IC Net
 METROHM LTD

Report date: 8/22/2023 1:36:29 PM
Printed by: wet


Ident: O4032-01DLX300
Analysis from: 8/21/2023 12:27:52 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35211

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

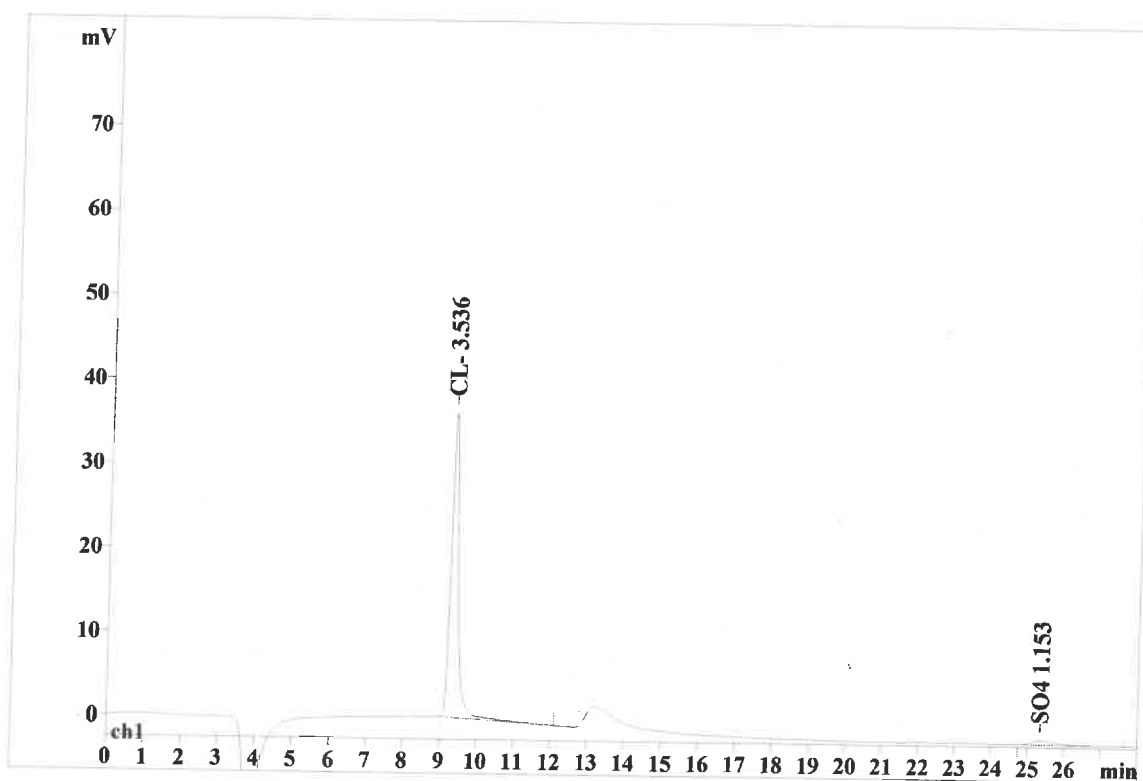

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	0.00	0.000	0.00	0.00	0.000	0.0
2	9.30	0.204	36.12	98.58	523.420	95.6
3	0.00	0.000	0.00	0.00	0.000	0.0
4	0.00	0.000	0.00	0.00	0.000	0.0
5	0.00	0.000	0.00	0.00	0.000	0.0
6	0.00	0.000	0.00	0.00	0.000	0.0
7	25.35	0.646	0.52	1.41	23.592	4.3
7	28.00	0.121	36.64	99.99	547.011	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:36:52 PM
Printed by: wet


Ident: O4074-01
Analysis from: 8/21/2023 12:58:29 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35212

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

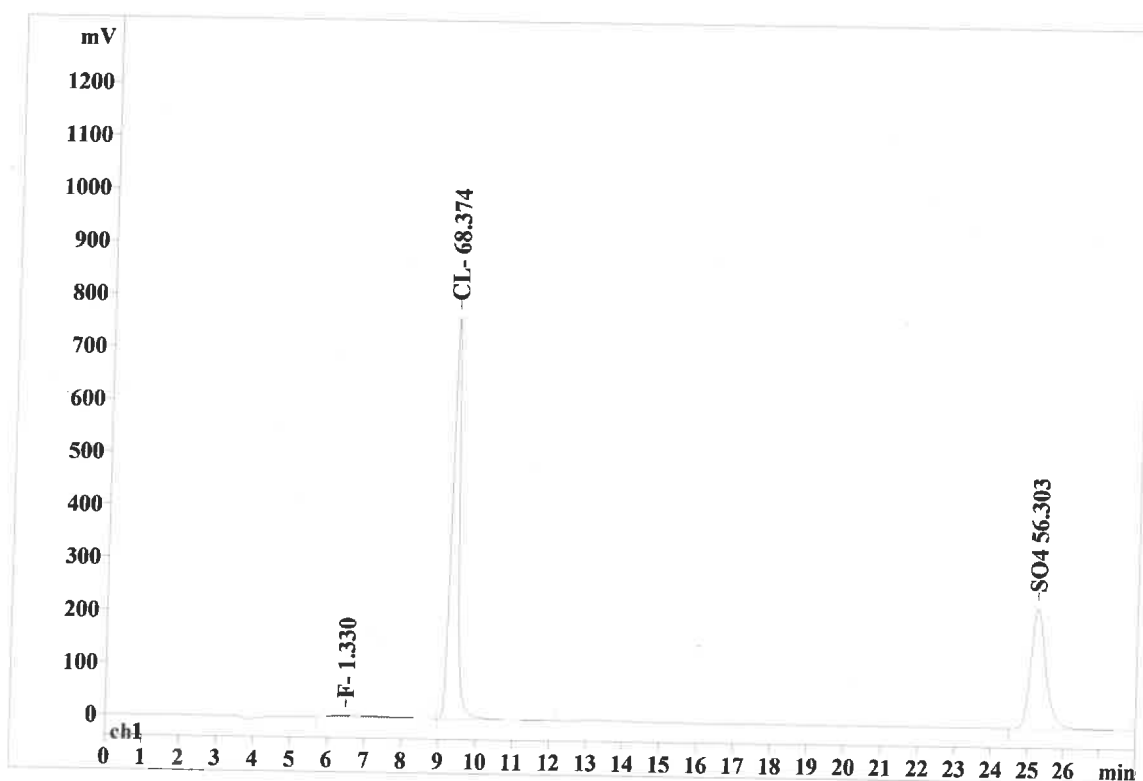

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.49	1.327	2.80	0.28	239.376	1.3
2	9.32	0.201	762.81	76.79	10605.402	60.3
3	0.00	0.000	0.00	0.00	0.000	0.0
4	0.00	0.000	0.00	0.00	0.000	0.0
5	0.00	0.000	0.00	0.00	0.000	0.0
6	0.00	0.000	0.00	0.00	0.000	0.0
7	25.23	0.437	227.76	22.93	6728.703	38.2
7	28.00	0.281	993.37	100.00	17573.481	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:37:03 PM
Printed by: wet


Ident: O4074-01MS
Analysis from: 8/21/2023 1:29:07 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35213

Last save: 8/17/2023 8:4

SAMPLE:
:
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

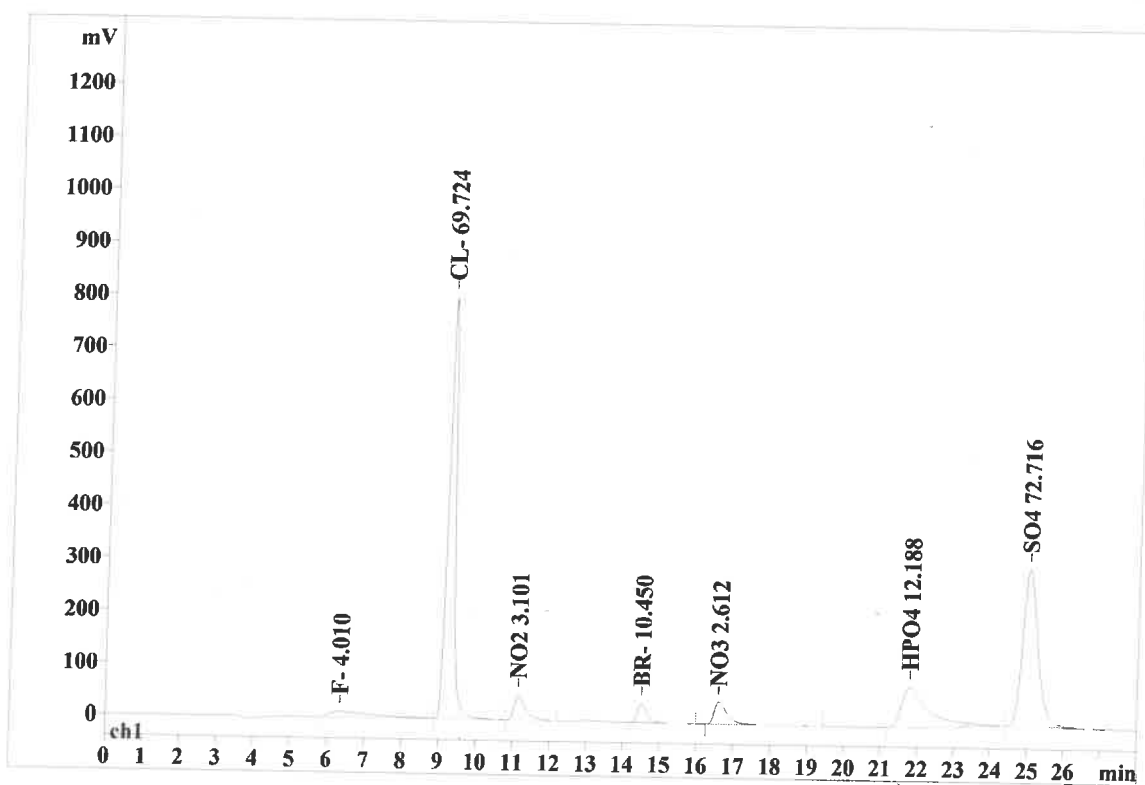

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.34	1.144	10.74	0.82	816.385	3.0
2	9.22	0.197	799.38	61.20	10815.358	40.2
3	11.14	0.294	46.36	3.55	1004.069	3.7
4	14.50	0.280	35.93	2.75	681.284	2.5
5	16.60	0.350	40.67	3.11	974.884	3.6
6	21.78	0.669	74.29	5.69	3871.339	14.4
7	25.01	0.436	298.86	22.88	8724.066	32.4
7	28.00	0.481	1306.24	100.00	26887.384	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:37:17 PM
Printed by: wet


Ident: O4074-01MSD
Analysis from: 8/21/2023 1:59:44 PM
File: _2023-08-21_

Last save: 8/22/2023 1:32:36 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35214

Last save: 8/17/2023 8:4

SAMPLE:
:
Vial number: 24
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

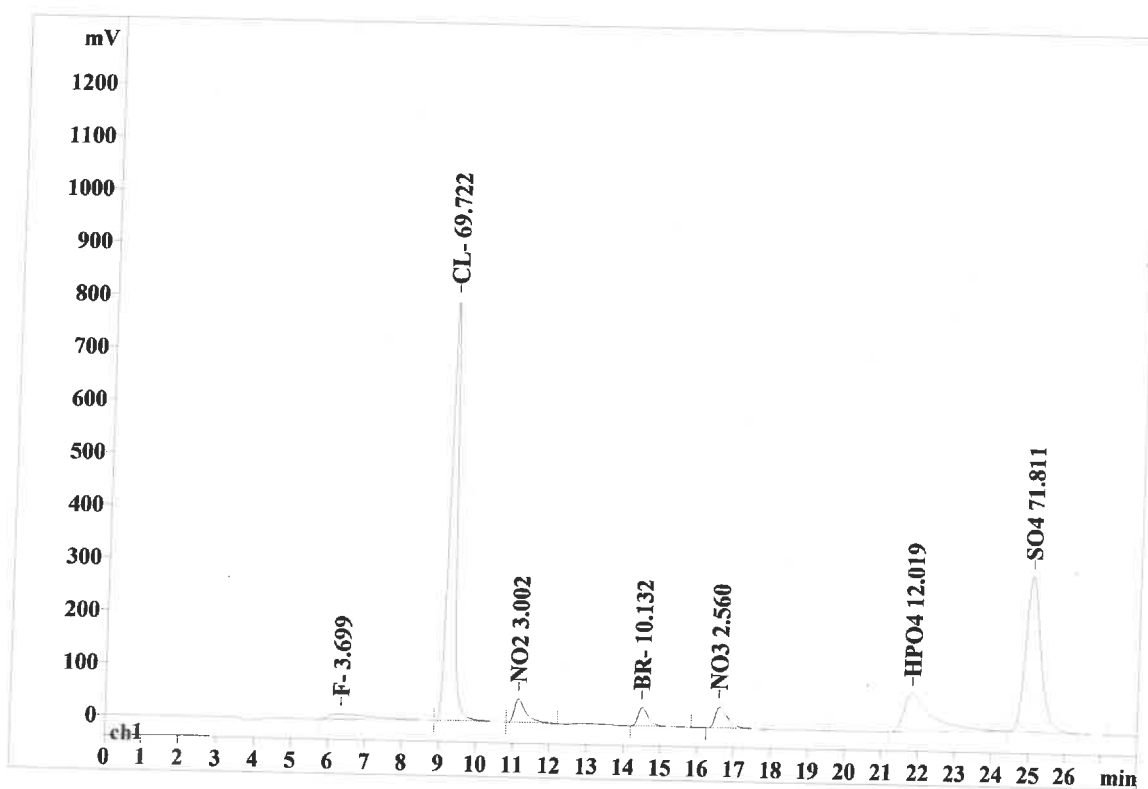

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.33	1.186	9.66	0.75	749.323	2.6
2	9.22	0.198	796.61	61.70	10815.068	40.7
3	11.14	0.298	44.27	3.43	969.851	3.6
4	14.48	0.281	34.68	2.69	659.045	2.4
5	16.57	0.349	39.40	3.05	954.192	3.5
6	21.81	0.679	72.19	5.59	3813.986	14.3
7	25.04	0.438	294.26	22.79	8614.078	32.4
7	28.00	0.490	1291.08	100.00	26575.541	100.C

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:32:54 PM
Printed by: wet


Ident: CCV
Analysis from: 8/21/2023 9:54:43 AM
File: _2023-08-21_

Last save: 8/22/2023 1:32:34 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35206

Last save: 8/17/2023 8:4

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

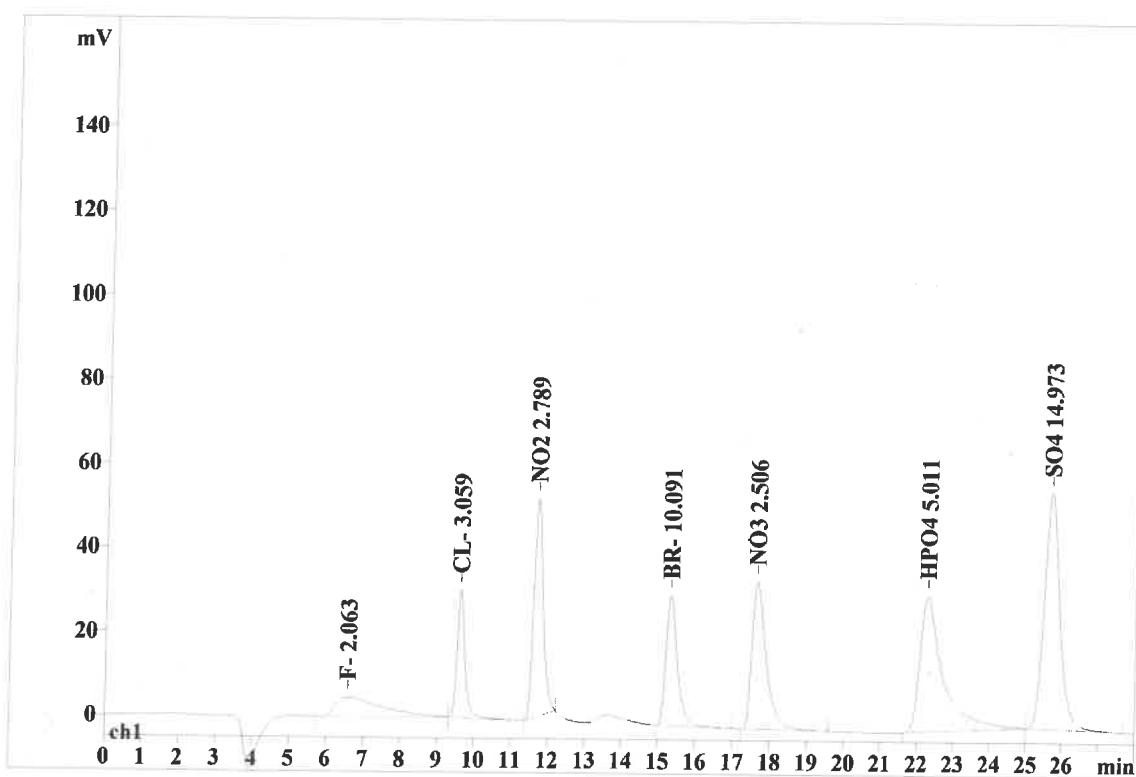

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.58	1.342	4.55	1.89	397.141	6.1
2	9.60	0.214	30.29	12.60	449.184	6.9
3	11.68	0.263	51.71	21.51	896.611	13.8
4	15.30	0.314	30.76	12.80	656.188	10.1
5	17.62	0.389	34.91	14.52	932.664	14.4
6	22.27	0.567	32.17	13.38	1435.857	22.1
7	25.65	0.453	56.01	23.30	1703.821	26.3
7	28.00	0.506	240.39	100.00	6471.467	100.0

This report has been created by IC Net
METROHM LTD

Report date: 8/22/2023 1:33:43 PM
Printed by: wet


Ident: CCB
Analysis from: 8/21/2023 10:25:21 AM
File: _2023-08-21_

Last save: 8/22/2023 1:32:34 PM

Method: AnionsIC2-081623.mtw
Run operator: wet
Analysis number: 35207

Last save: 8/17/2023 8:4

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

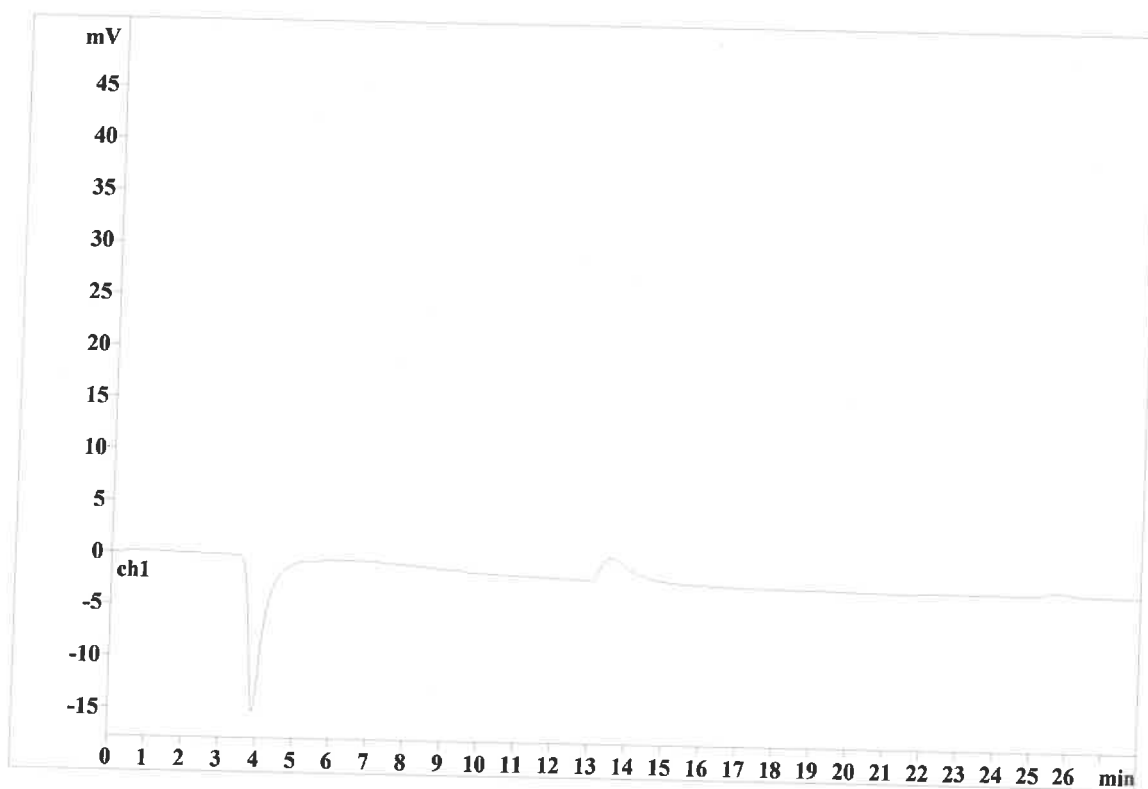

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD