


LB126968

7471B

INSTRUMENT ID: CV1

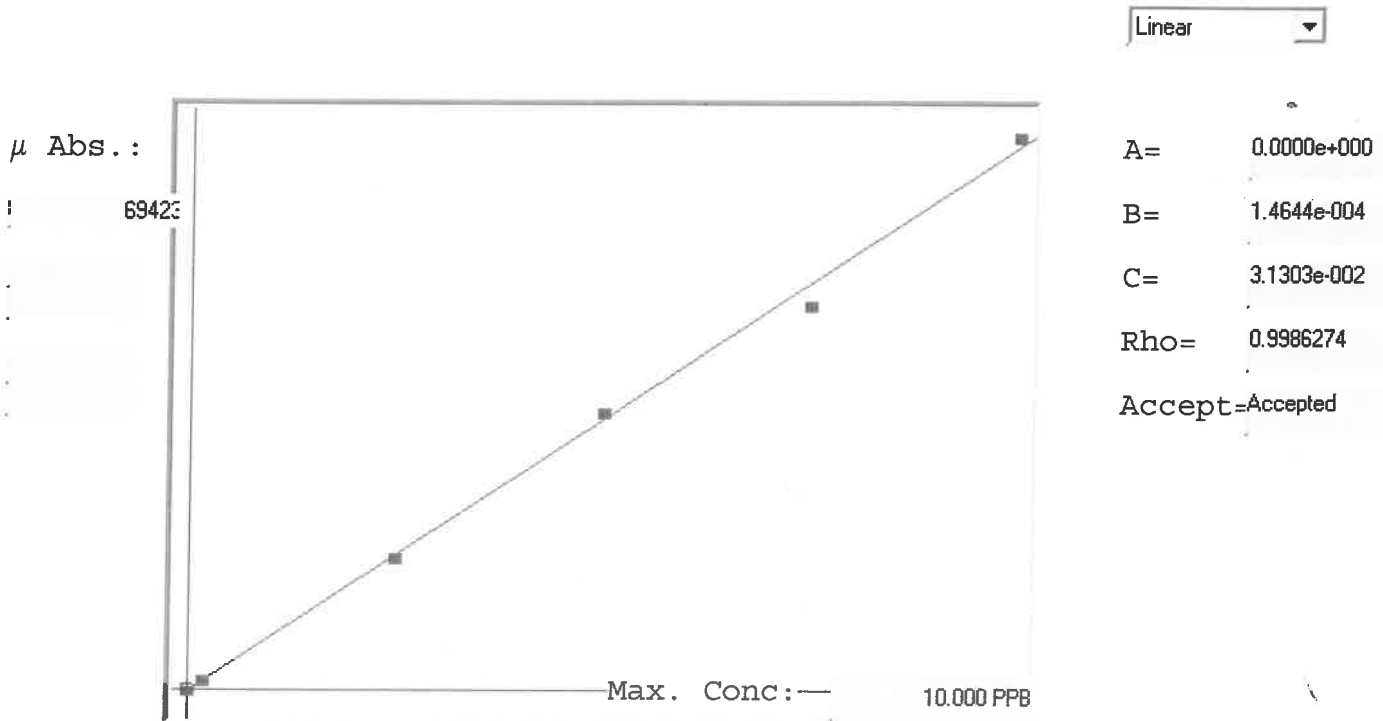

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/1
0.0	0.000	0.052	0.052	140	0.000	140					5
0.2	0.200	0.210	0.010	1223	0.0 %	1223					1
2.5	2.500	2.469	-0.031	16645	0.0 %	16645					3
5.0	5.000	5.164	0.164	35049	0.0 %	35049					5
7.5	7.500	7.107	-0.393	48318	0.0 %	48318					2
10.0	10.000	10.198	0.198	69423	0.0 %	69423					

LB126968 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Aug 2023 08:36:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	140	-	0.0000	7471B	PPB	23 Aug 2023 08:54:05	S	Std
0.2 - 1	50.2	1223	-	0.2000	7471B	PPB	23 Aug 2023 08:56:23	S	Std
2.5 - 1	52.5	16645	-	2.5000	7471B	PPB	23 Aug 2023 08:58:39	S	Std
5.0 - 1	35	35049	-	5.0000	7471B	PPB	23 Aug 2023 09:04:55	S	Std
7.5 - 1	37.5	48318	-	7.5000	7471B	PPB	23 Aug 2023 09:07:11	S	Std
10.0 - 1	510	69423	-	10.0000	7471B	PPB	23 Aug 2023 09:12:06	S	Std
ICV28 - 1	ICV28	28382	4.1876	-	7471B	PPB	23 Aug 2023 09:15:08	U	SMPL
ICB28 - 1	ICB28	123	0.0493	-	7471B	PPB	23 Aug 2023 09:17:23	U	SMPL
CCV76 - 1	CCV76	33812	4.9828	-	7471B	PPB	23 Aug 2023 09:19:37	U	SMPL
CCB76 - 1	CCB76	115	0.0481	-	7471B	PPB	23 Aug 2023 09:21:52	U	SMPL
CRA - 1	CRA	1192	0.2059	-	7471B	PPB	23 Aug 2023 09:24:08	U	SMPL
HighStd - 1	HighStd	69544	10.2155	-	7471B	PPB	23 Aug 2023 09:26:23	U	SMPL
PB155013BL - 1	PBS	63	0.0405	-	7471B	PPB	23 Aug 2023 09:30:56	U	SMPL
O4110-01 - 1	SS-TP-01(0-0.2)	3511	0.5455	-	7471B	PPB	23 Aug 2023 09:35:27	U	SMPL
O4110-02 - 1	TP-03(2-4)	1519	0.2537	-	7471B	PPB	23 Aug 2023 09:37:44	U	SMPL
O4110-03 - 1	TP-04(1-2)	4734	0.7246	-	7471B	PPB	23 Aug 2023 09:40:01	U	SMPL
O4110-03DUP - 1	TP-04(1-2)DUP	5127	0.7821	-	7471B	PPB	23 Aug 2023 09:42:17	U	SMPL
O4110-04 - 1	O4110-03MS	28238	4.1666	-	7471B	PPB	23 Aug 2023 09:44:32	U	SMPL
ChkStd - 1	ChkStd	48365	7.1140	-	7471B	PPB	23 Aug 2023 09:47:11	U	SMPL
PB155013BS - 1	LCSS	28332	4.1803	-	7471B	PPB	23 Aug 2023 09:52:21	U	SMPL
CCV77 - 1	CCV77	33680	4.9635	-	7471B	PPB	23 Aug 2023 09:56:27	U	SMPL
CCB77 - 1	CCB77	80	0.0430	-	7471B	PPB	23 Aug 2023 09:58:41	U	SMPL
O4110-05 - 1	O4110-03MSD	28266	4.1707	-	7471B	PPB	23 Aug 2023 10:00:58	U	SMPL
O4110-06 - 1	SS-TP-05(0-0.2)	7675	1.1553	-	7471B	PPB	23 Aug 2023 10:03:13	U	SMPL
O4110-07 - 1	TP-07(1-3)	9888	1.4793	-	7471B	PPB	23 Aug 2023 10:05:29	U	SMPL
O4110-08 - 1	DUP-01(X-X)	6029	0.9142	-	7471B	PPB	23 Aug 2023 10:07:44	U	SMPL
O4110-09 - 1	SS-TP-09(0-0.2)	21428	3.1693	-	7471B	PPB	23 Aug 2023 10:10:00	U	SMPL
O4110-10 - 1	TP-11(1-2)	51772	7.6130	-	7471B	PPB	23 Aug 2023 10:12:16	U	SMPL
O4110-11 - 1	TP-12(5-7)	1676	0.2767	-	7471B	PPB	23 Aug 2023 10:14:33	U	SMPL
O4110-12 - 1	TP-15(2-3)	15220	2.2602	-	7471B	PPB	23 Aug 2023 10:16:51	U	SMPL
O4110-13 - 1	SS-TP-19(0-1)	14476	2.1512	-	7471B	PPB	23 Aug 2023 10:19:08	U	SMPL
O4110-14 - 1	TP-21(3-4)	16456	2.4412	-	7471B	PPB	23 Aug 2023 10:21:23	U	SMPL
CCV78 - 1	CCV78	33847	4.9880	-	7471B	PPB	23 Aug 2023 10:23:39	U	SMPL
CCB78 - 1	CCB78	110	0.0474	-	7471B	PPB	23 Aug 2023 10:25:55	U	SMPL
O4110-15 - 1	TP-22(3-4)	73610	10.8110	-	7471B	PPB	23 Aug 2023 10:28:10	U	SMPL
O4110-16 - 1	SS-TP-23(0-1)	8590	1.2892	-	7471B	PPB	23 Aug 2023 10:30:26	U	SMPL
O4110-17 - 1	TP-24(4-5)	28845	4.2555	-	7471B	PPB	23 Aug 2023 10:32:43	U	SMPL
O4110-18 - 1	TP-26(1-2)	10107	1.5114	-	7471B	PPB	23 Aug 2023 10:34:58	U	SMPL
O4110-19 - 1	SS-TP-27(0-1)	10055	1.5038	-	7471B	PPB	23 Aug 2023 10:37:14	U	SMPL
O4110-20 - 1	TP-28(1.5-2.5)	74230	10.9018	-	7471B	PPB	23 Aug 2023 10:39:30	U	SMPL
O4110-23 - 1	TP-10(6-7)	719	0.1366	-	7471B	PPB	23 Aug 2023 10:41:46	U	SMPL
O4110-24 - 1	TP-20(2-3)	83738	12.2942	-	7471B	PPB	23 Aug 2023 10:44:04	U	SMPL
PB155014BL - 1	PBS	-24	0.0278	-	7471B	PPB	23 Aug 2023 10:46:21	U	SMPL
PB155014BS - 1	LCSS	23112	3.4159	-	7471B	PPB	23 Aug 2023 10:48:37	U	SMPL
CCV79 - 1	CCV79	33957	5.0041	-	7471B	PPB	23 Aug 2023 10:50:53	U	SMPL
CCB79 - 1	CCB79	108	0.0471	-	7471B	PPB	23 Aug 2023 10:53:09	U	SMPL
O4093-01 - 1	NEVINS-SB04-Z45-46	521	0.1076	-	7471B	PPB	23 Aug 2023 10:55:24	U	SMPL
O4093-02 - 1	NEVINS-SB04-Z52-53	457	0.0982	-	7471B	PPB	23 Aug 2023 10:57:40	U	SMPL
O4093-03 - 1	NEVINS-SB04-Z83-84	533	0.1094	-	7471B	PPB	23 Aug 2023 10:59:55	U	SMPL
O4093-04 - 1	NEVINS-SB04-Z94-95	503	0.1050	-	7471B	PPB	23 Aug 2023 11:02:10	U	SMPL
O4103-01 - 1	OR-2-082123	2072	0.3347	-	7471B	PPB	23 Aug 2023 11:04:26	U	SMPL
O4109-01 - 1	TP-01(6-7)	851	0.1559	-	7471B	PPB	23 Aug 2023 11:06:42	U	SMPL
O4109-01DUP - 1	TP-01(6-7)DUP	963	0.1723	-	7471B	PPB	23 Aug 2023 11:11:40	U	SMPL
O4109-02 - 1	O4109-01MS	24745	3.6550	-	7471B	PPB	23 Aug 2023 11:13:57	U	SMPL
O4109-03 - 1	O4109-01MSD	25477	3.7622	-	7471B	PPB	23 Aug 2023 11:16:14	U	SMPL
O4109-08 - 1	DUP-1	1189	0.2054	-	7471B	PPB	23 Aug 2023 11:18:29	U	SMPL
CCV80 - 1	CCV80	35654	5.2526	-	7471B	PPB	23 Aug 2023 11:20:45	U	SMPL
CCB80 - 1	CCB80	95	0.0452	-	7471B	PPB	23 Aug 2023 11:23:01	U	SMPL
O4116-01 - 1	TP-1	3489	0.5422	-	7471B	PPB	23 Aug 2023 11:25:16	U	SMPL
O4116-03 - 1	TP-2	4232	0.6510	-	7471B	PPB	23 Aug 2023 11:27:32	U	SMPL
O4116-05 - 1	TP-3	2733	0.4315	-	7471B	PPB	23 Aug 2023 11:29:47	U	SMPL
O4116-07 - 1	TP-4	4871	0.7446	-	7471B	PPB	23 Aug 2023 11:32:02	U	SMPL
O4116-09 - 1	TP-5	2800	0.4413	-	7471B	PPB	23 Aug 2023 11:34:19	U	SMPL
O4119-01 - 1	RT2674	1758	0.2887	-	7471B	PPB	23 Aug 2023 11:36:35	U	SMPL
O4119-03 - 1	RB21153	7151	1.0785	-	7471B	PPB	23 Aug 2023 11:38:51	U	SMPL
O4112-01 - 1	RBR-22282	3079	0.4822	-	7471B	PPB	23 Aug 2023 11:41:08	U	SMPL
CCV81 - 1	CCV81	35468	5.2253	-	7471B	PPB	23 Aug 2023 11:43:25	U	SMPL
CCB81 - 1	CCB81	110	0.0474	-	7471B	PPB	23 Aug 2023 11:45:41	U	SMPL
O4110-03LX5 - 1		944	0.1695	-	7471B	PPB	23 Aug 2023 11:47:56	U	SMPL
O4110-03A - 1		29035	4.2833	-	7471B	PPB	23 Aug 2023 11:50:13	U	SMPL
O4109-01LX5 - 1		163	0.0552	-	7471B	PPB	23 Aug 2023 11:52:29	U	SMPL
O4109-01A - 1		28855	4.2569	-	7471B	PPB	23 Aug 2023 11:54:44	U	SMPL
O4110-15DLX2 - 1		36298	5.3469	-	7471B	PPB	23 Aug 2023 11:57:00	U	SMPL
O4110-20DLX2 - 1		39429	5.8054	-	7471B	PPB	23 Aug 2023 11:59:16	U	SMPL
O4110-24DLX2 - 1		42458	6.2490	-	7471B	PPB	23 Aug 2023 12:01:32	U	SMPL
CCV82 - 1	CCV82	33646	4.9585	-	7471B	PPB	23 Aug 2023 12:03:48	U	SMPL
CCB82 - 1	CCB82	120	0.0489	-	7471B	PPB	23 Aug 2023 12:06:05	U	SMPL