


LB127009

7471B

INSTRUMENT ID: CVL

Linear

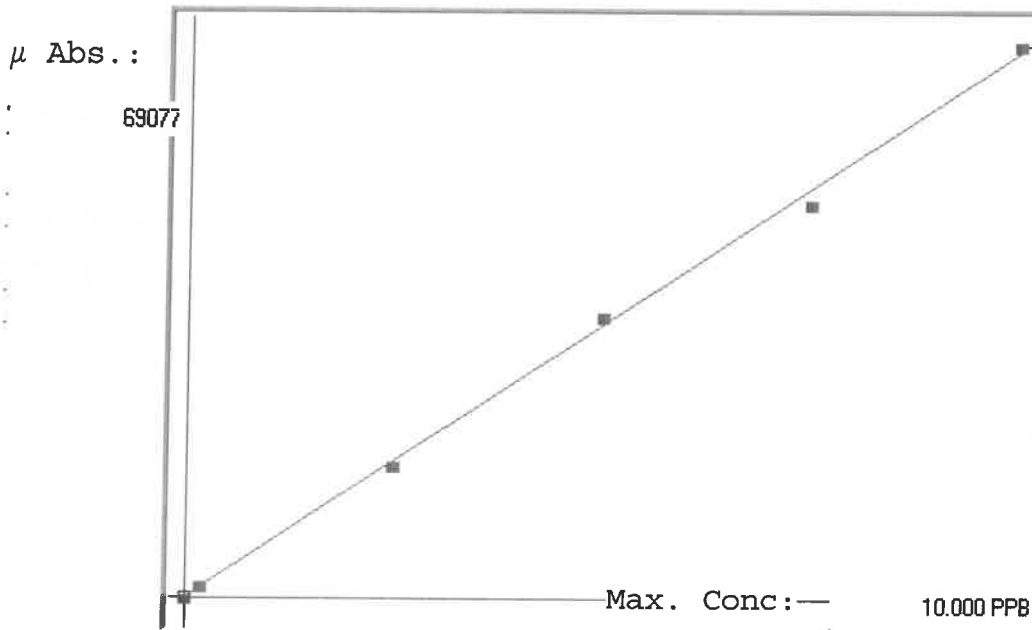

A= 0.0000e+000

B= 1.4661e-004

C= -5.5401e-003

Rho= 0.9992481

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.026	0.026	214	0.000	214					-
0.2	0.200	0.220	0.020	1540	0.0 %	1540					10
2.5	2.500	2.432	-0.068	16624	0.0 %	16624					-3
5.0	5.000	5.171	0.171	35308	0.0 %	35308					3
7.5	7.500	7.230	-0.270	49351	0.0 %	49351					-4
10.0	10.000	10.122	0.122	69077	0.0 %	69077					1

LB127009 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 25 Aug 2023 14:02:28

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	214	-	0.0000	7471B	PPB	25 Aug 2023 14:06:10	S	Std
0.2 - 1	50.2	1540	-	0.2000	7471B	PPB	25 Aug 2023 14:08:27	S	Std
2.5 - 1	52.5	16624	-	2.5000	7471B	PPB	25 Aug 2023 14:10:44	S	Std
5.0 - 1	45	35308	-	5.0000	7471B	PPB	25 Aug 2023 14:13:01	S	Std
7.5 - 1	53.5	49351	-	7.5000	7471B	PPB	25 Aug 2023 14:17:51	S	Std
10.0 - 1	510	69077	-	10.0000	7471B	PPB	25 Aug 2023 14:22:47	S	Std
ICV33 - 1	ICV33	28432	4.1628	-	7471B	PPB	25 Aug 2023 14:26:17	U	SMPL
ICB33 - 1	ICB33	108	0.0103	-	7471B	PPB	25 Aug 2023 14:28:32	U	SMPL
CCV94 - 1	CCV94	35217	5.1575	-	7471B	PPB	25 Aug 2023 14:32:44	U	SMPL
CCB94 - 1	CCB94	159	0.0178	-	7471B	PPB	25 Aug 2023 14:34:59	U	SMPL
CRA - 1	CRA	1500	0.2144	-	7471B	PPB	25 Aug 2023 14:37:14	U	SMPL
HighStd - 1	HighStd	70323	10.3044	-	7471B	PPB	25 Aug 2023 14:39:29	U	SMPL
ChkStd - 1	ChkStd	46514	6.8138	-	7471B	PPB	25 Aug 2023 14:41:44	U	SMPL
PB155061BL - 1	PBS	-24	-0.0091	-	7471B	PPB	25 Aug 2023 14:44:01	U	SMPL
O4133-01 - 1	OK-2-082323	3360	0.4871	-	7471B	PPB	25 Aug 2023 14:48:34	U	SMPL
O4133-01DUP - 1	OK-2-082323DUP	3165	0.4585	-	7471B	PPB	25 Aug 2023 14:50:50	U	SMPL
O4133-01MS - 1	OK-2-082323MS	27595	4.0401	-	7471B	PPB	25 Aug 2023 14:53:07	U	SMPL
O4133-01MSD - 1	OK-2-082323MSD	27210	3.9837	-	7471B	PPB	25 Aug 2023 14:55:24	U	SMPL
O4135-02 - 1	328	4068	0.5909	-	7471B	PPB	25 Aug 2023 14:57:39	U	SMPL
CCV95 - 1	CCV95	34695	5.0810	-	7471B	PPB	25 Aug 2023 14:59:54	U	SMPL
CCB95 - 1	CCB95	158	0.0176	-	7471B	PPB	25 Aug 2023 15:02:09	U	SMPL
O4145-01 - 1	WC-1	8388	1.2242	-	7471B	PPB	25 Aug 2023 15:04:24	U	SMPL
O4146-01 - 1	72-12013	2043	0.2940	-	7471B	PPB	25 Aug 2023 15:06:39	U	SMPL
O4147-01 - 1	SB-05(46-47)	462	0.0622	-	7471B	PPB	25 Aug 2023 15:08:54	U	SMPL
O4147-02 - 1	SB-03(27-29)	612	0.0842	-	7471B	PPB	25 Aug 2023 15:11:10	U	SMPL
O4147-03 - 1	SB-03(48-50)	320	0.0414	-	7471B	PPB	25 Aug 2023 15:13:26	U	SMPL
O4147-04 - 1	SB-04(21.5-23)	15765	2.3057	-	7471B	PPB	25 Aug 2023 15:15:42	U	SMPL
O4160-01 - 1	CHRT-24449	7166	1.0451	-	7471B	PPB	25 Aug 2023 15:17:58	U	SMPL
O4160-03 - 1	CHRT-26706	18785	2.7485	-	7471B	PPB	25 Aug 2023 15:20:15	U	SMPL
O4161-01 - 1	CHRT-25659	984	0.1387	-	7471B	PPB	25 Aug 2023 15:22:32	U	SMPL
O4165-01 - 1	VNJ-208	2899	0.4195	-	7471B	PPB	25 Aug 2023 15:24:47	U	SMPL
CCV96 - 1	CCV96	35474	5.1952	-	7471B	PPB	25 Aug 2023 15:27:03	U	SMPL
CCV96 - 1	CC96	177	0.0204	-	7471B	PPB	25 Aug 2023 15:29:19	U	SMPL
O4165-03 - 1	VNJ-210	6324	0.9216	-	7471B	PPB	25 Aug 2023 15:31:36	U	SMPL
O4169-01 - 1	PL-01-082423	4339	0.6306	-	7471B	PPB	25 Aug 2023 15:33:51	U	SMPL
O4133-01LX5 - 1		513	0.0697	-	7471B	PPB	25 Aug 2023 15:36:06	U	SMPL
O4133-01A - 1		28896	4.2308	-	7471B	PPB	25 Aug 2023 15:38:22	U	SMPL
PB155061BS - 1	LCSS	25047	3.6665	-	7471B	PPB	25 Aug 2023 15:55:31	U	SMPL
CCV97 - 1	CCV97	31618	4.6299	-	7471B	PPB	25 Aug 2023 15:58:03	U	SMPL
CCB97 - 1	CCB97	-373	-0.0602	-	7471B	PPB	25 Aug 2023 16:00:19	U	SMPL