


LB127098

7470A

INSTRUMENT ID: CV1

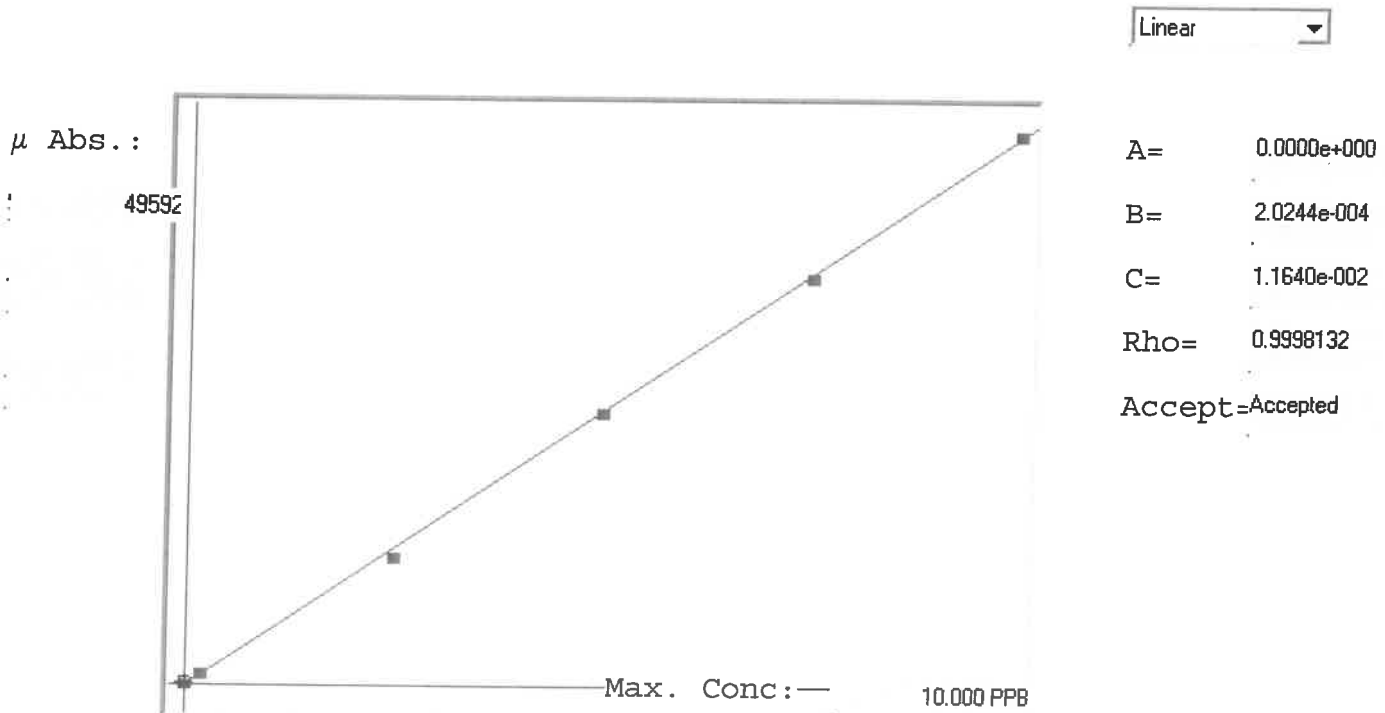

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.077	0.077	324	0.000	324	0				9/01)
0.2	0.200	0.238	0.038	1116	0.0 %	1116					19
2.5	2.500	2.360	-0.140	11598	0.0 %	11598					-6
5.0	5.000	5.003	0.003	24655	0.0 %	24655					00
7.5	7.500	7.472	-0.028	36851	0.0 %	36851					00
10.0	10.000	10.051	0.051	49592	0.0 %	49592					1

LB127098 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Aug 2023 15:44:26

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	324	-	0.0000	7470A	PPB	31 Aug 2023 15:50:46	S	Std
0.2 - 1	50.2	1116	-	0.2000	7470A	PPB	31 Aug 2023 15:53:03	S	Std
2.5 - 1	52.5	11598	-	2.5000	7470A	PPB	31 Aug 2023 15:55:20	S	Std
5.0 - 1	55	24655	-	5.0000	7470A	PPB	31 Aug 2023 15:57:37	S	Std
7.5 - 1	57.5	36851	-	7.5000	7470A	PPB	31 Aug 2023 15:59:52	S	Std
10.0 - 1	510	49592	-	10.0000	7470A	PPB	31 Aug 2023 16:02:08	S	Std
ICV43 - 1	ICV43	20859	4.2343	-	7470A	PPB	31 Aug 2023 16:05:09	U	SMPL
ICB43 - 1	ICB43	228	0.0578	-	7470A	PPB	31 Aug 2023 16:07:23	U	SMPL
CCV35 - 1	CCV35	25184	5.1099	-	7470A	PPB	31 Aug 2023 16:09:38	U	SMPL
CCB35 - 1	CCB35	224	0.0570	-	7470A	PPB	31 Aug 2023 16:11:53	U	SMPL
CRA - 1	CRA	1104	0.2351	-	7470A	PPB	31 Aug 2023 16:14:08	U	SMPL
HighStd - 1	HighStd	49737	10.0804	-	7470A	PPB	31 Aug 2023 16:16:22	U	SMPL
ChkStd - 1	ChkStd	36393	7.3791	-	7470A	PPB	31 Aug 2023 16:18:38	U	SMPL
PB155251BL - 1	PBW	129	0.0378	-	7470A	PPB	31 Aug 2023 16:20:53	U	SMPL
PB155251BS - 1	LCSW	20630	4.1880	-	7470A	PPB	31 Aug 2023 16:23:09	U	SMPL
O4232-01 - 1	SBG-1	133	0.0386	-	7470A	PPB	31 Aug 2023 16:25:25	U	SMPL
O4232-02 - 1	SBG-2	421	0.0969	-	7470A	PPB	31 Aug 2023 16:27:41	U	SMPL
O4232-03 - 1	SBG-3	324	0.0772	-	7470A	PPB	31 Aug 2023 16:29:58	U	SMPL
O4232-04 - 1	SBG-4	409	0.0944	-	7470A	PPB	31 Aug 2023 16:32:15	U	SMPL
O4232-05 - 1	SBG-5	237	0.0596	-	7470A	PPB	31 Aug 2023 16:34:30	U	SMPL
CCV36 - 1	CCV36	26596	5.3957	-	7470A	PPB	31 Aug 2023 16:36:45	U	SMPL
CCB36 - 1	CCB36	243	0.0608	-	7470A	PPB	31 Aug 2023 16:39:01	U	SMPL
O4232-06 - 1	SBG-6	170	0.0461	-	7470A	PPB	31 Aug 2023 16:41:16	U	SMPL
O4232-07 - 1	SBG-7	340	0.0805	-	7470A	PPB	31 Aug 2023 16:43:30	U	SMPL
O4232-08 - 1	SBG-8	626	0.1384	-	7470A	PPB	31 Aug 2023 16:45:46	U	SMPL
O4232-09 - 1	SB-11	190	0.0501	-	7470A	PPB	31 Aug 2023 16:48:01	U	SMPL
O4232-10 - 1	SB-12	352	0.0829	-	7470A	PPB	31 Aug 2023 16:50:17	U	SMPL
O4232-10DUP - 1	SB-12DUP	251	0.0625	-	7470A	PPB	31 Aug 2023 16:52:33	U	SMPL
O4232-10MS - 1	SB-12MS	22611	4.5890	-	7470A	PPB	31 Aug 2023 16:54:49	U	SMPL
O4232-10MSD - 1	SB-12MSD	20490	4.1596	-	7470A	PPB	31 Aug 2023 16:57:06	U	SMPL
PB155259BL - 1	PBW	172	0.0465	-	7470A	PPB	31 Aug 2023 16:59:23	U	SMPL
PB155259BS - 1	LCSW	21192	4.3018	-	7470A	PPB	31 Aug 2023 17:01:39	U	SMPL
CCV37 - 1	CCV37	24742	5.0204	-	7470A	PPB	31 Aug 2023 17:06:53	U	SMPL
CCB37 - 1	CCB37	242	0.0606	-	7470A	PPB	31 Aug 2023 17:09:08	U	SMPL
O4201-01 - 1	31989	531	0.1191	-	7470A	PPB	31 Aug 2023 17:11:23	U	SMPL
O4211-01 - 1	TRE-1767	517	0.1163	-	7470A	PPB	31 Aug 2023 17:13:38	U	SMPL
O4222-01 - 1	1039	1506	0.3165	-	7470A	PPB	31 Aug 2023 17:15:54	U	SMPL
O4222-02 - 1	1040	8201	1.6719	-	7470A	PPB	31 Aug 2023 17:18:09	U	SMPL
O4222-02DUP - 1	1040DUP	8903	1.8140	-	7470A	PPB	31 Aug 2023 17:20:25	U	SMPL
O4222-02MS - 1	1040MS	20876	4.2378	-	7470A	PPB	31 Aug 2023 17:22:41	U	SMPL
O4222-02MSD - 1	1040MSD	21811	4.4271	-	7470A	PPB	31 Aug 2023 17:24:59	U	SMPL
CCV38 - 1	CCV38	24736	5.0192	-	7470A	PPB	31 Aug 2023 17:27:18	U	SMPL
CCB38 - 1	CCB38	301	0.0726	-	7470A	PPB	31 Aug 2023 17:29:36	U	SMPL
PB155231TYB - 1		110	0.0339	-	7470A	PPB	31 Aug 2023 17:31:52	U	SMPL
O4232-10LX5 - 1		3	0.0122	-	7470A	PPB	31 Aug 2023 17:34:07	U	SMPL
O4232-10A - 1		21254	4.3143	-	7470A	PPB	31 Aug 2023 17:36:23	U	SMPL
O4222-02LX5 - 1		1946	0.4056	-	7470A	PPB	31 Aug 2023 17:38:38	U	SMPL
O4222-02A - 1		29722	6.0286	-	7470A	PPB	31 Aug 2023 17:40:53	U	SMPL
CCV39 - 1	CCV39	23980	4.8662	-	7470A	PPB	31 Aug 2023 17:43:09	U	SMPL
CCB39 - 1	CCB39	258	0.0639	-	7470A	PPB	31 Aug 2023 17:45:24	U	SMPL