


LB127210

SFAM01.1

INSTRUMENT ID: CV1

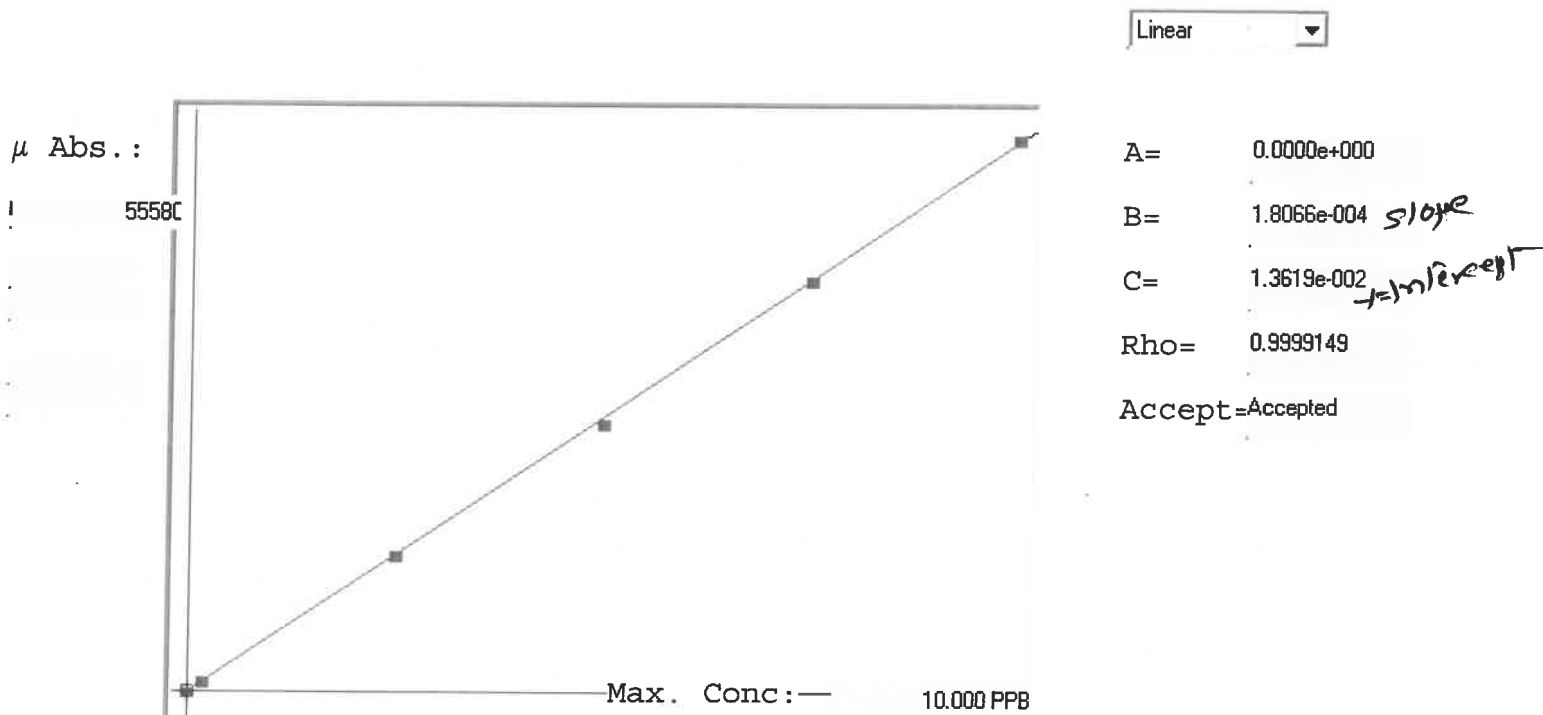

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	<i>1/01</i>
0.00	0.000	0.041	0.041	149	0.000	149					
0.05	0.050					501	0				
0.20	0.200	0.221	0.021	1147	0.0 %	1147					
2.50	2.500	2.485	-0.015	13680	0.0 %	13680					
5.00	5.000	4.908	-0.092	27090	0.0 %	27090					
7.50	7.500	7.491	-0.009	41387	0.0 %	41387					
10.0	10.000	10.055	0.055	55580	0.0 %	55580					

LB127210

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	149	-		0 SFAM01.1	PPB	9/8/2023 16:57	Std
	0.2 S01	1147	-		0.2 SFAM01.1	PPB	9/8/2023 16:59	Std
	2.5 S02	13680	-		2.5 SFAM01.1	PPB	9/8/2023 17:03	Std
	5 S03	27090	-		5 SFAM01.1	PPB	9/8/2023 17:05	Std
	7.5 S04	41387	-		7.5 SFAM01.1	PPB	9/8/2023 17:08	Std
	10 S05	55580	-		10 SFAM01.1	PPB	9/8/2023 17:10	Std
ICV055	ICV055	21266	3.8556 -		SFAM01.1	PPB	9/8/2023 17:13	SMPL
ICB055	ICB055	90	0.0299 -		SFAM01.1	PPB	9/8/2023 17:15	SMPL
CCV073	CCV073	27009	4.8932 -		SFAM01.1	PPB	9/8/2023 17:17	SMPL
CCB073	CCB073	82	0.0284 -		SFAM01.1	PPB	9/8/2023 17:20	SMPL
PB155432BL	PBW432	285	0.0651 -		SFAM01.1	PPB	9/8/2023 17:22	SMPL
PB155432TB	LEB432	353	0.0774 -		SFAM01.1	PPB	9/8/2023 17:24	SMPL
O4193-01	MH1S8	1501	0.2848 -		SFAM01.1	PPB	9/8/2023 17:26	SMPL
O4193-02	MH1S9	650	0.1311 -		SFAM01.1	PPB	9/8/2023 17:29	SMPL
O4193-03	MH1T0	404	0.0866 -		SFAM01.1	PPB	9/8/2023 17:31	SMPL
O4193-04	MH1T0D	242	0.0573 -		SFAM01.1	PPB	9/8/2023 17:33	SMPL
O4193-05	MH1T0S	5681	1.04 -		SFAM01.1	PPB	9/8/2023 17:35	SMPL
CCV074	CCV074	27039	4.8986 -		SFAM01.1	PPB	9/8/2023 17:38	SMPL
CCB074	CCB074	111	0.0337 -		SFAM01.1	PPB	9/8/2023 17:40	SMPL