

LB 127244


245.1

INSTRUMENT ID: CV1

Linear

 μ Abs.:

52970

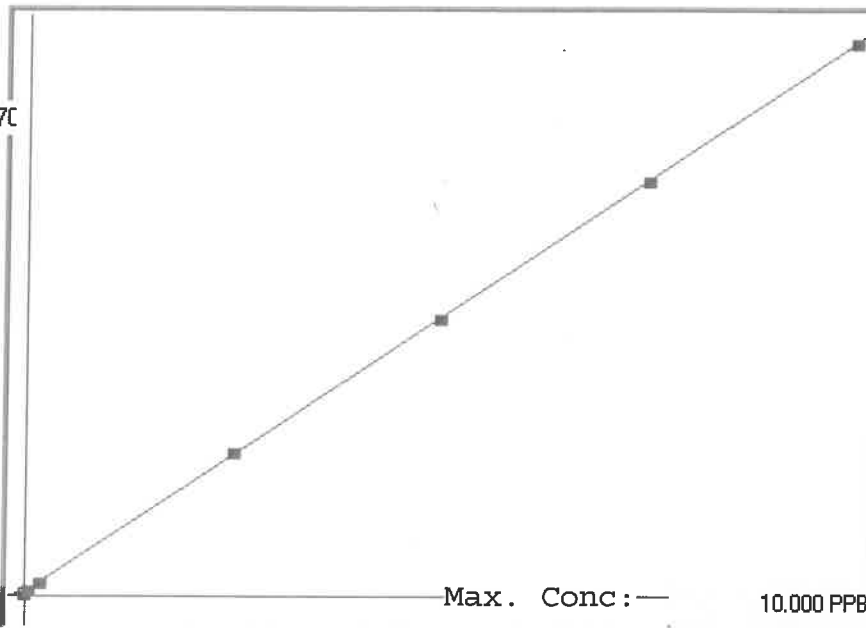

A= 0.0000e+000

B= 1.8992e-004

C= -6.7645e-002

Rho= 0.9999859

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.009	-0.009	310	0.000	310					-
0.05	0.050	0.047	-0.003	602	0.0 %	602	0				-6
0.2	0.200	0.187	-0.013	1341	0.0 %	1341					-7
2.5	2.500	2.544	0.044	13750	0.0 %	13750					2
5.0	5.000	4.980	-0.020	26578	0.0 %	26578					0
7.5	7.500	7.509	0.009	39895	0.0 %	39895					0
10.0	10.000	9.992	-0.008	52970	0.0 %	52970					0

LB127244 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 12 Sep 2023 13:20:39

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	310	-	0.0000	245.1	PPB	12 Sep 2023 13:25:12	S	Std
0.05 - 1	SD 0.5	602	-	0.0500	245.1	PPB	12 Sep 2023 13:27:29	S	Std
0.2 - 1	SD 2	1341	-	0.2000	245.1	PPB	12 Sep 2023 13:29:46	S	Std
2.5 - 1	SD 2.5	13750	-	2.5000	245.1	PPB	12 Sep 2023 13:32:03	S	Std
5.0 - 1	SD 5	26578	-	5.0000	245.1	PPB	12 Sep 2023 13:34:19	S	Std
7.5 - 1	SD 7.5	39895	-	7.5000	245.1	PPB	12 Sep 2023 13:36:34	S	Std
10.0 - 1	SD 10	52970	-	10.0000	245.1	PPB	12 Sep 2023 13:51:50	S	Std
ICV58 - 1	ICV58	20535	3.8323	-245.1		PPB	12 Sep 2023 13:57:19	U	SMPL
ICB58 - 1	ICB58	508	0.0288	-245.1		PPB	12 Sep 2023 13:59:34	U	SMPL
CCV82 - 1	CCV82	24707	4.6246	-245.1		PPB	12 Sep 2023 14:01:49	U	SMPL
CCB82 - 1	CCB82	487	0.0248	-245.1		PPB	12 Sep 2023 14:04:04	U	SMPL
CRA - 1	CRA	571	0.0408	-245.1		PPB	12 Sep 2023 14:06:18	U	SMPL
HighStd - 1	HighStd	49335	9.3019	-245.1		PPB	12 Sep 2023 14:08:33	U	SMPL
ChkStd - 1	ChkStd	36397	6.8448	-245.1		PPB	12 Sep 2023 14:10:48	U	SMPL
PB155497BL - 1	PBW	128	-0.0433	-245.1		PPB	12 Sep 2023 14:13:04	U	SMPL
PB155497BS - 1	LCSW	21442	4.0046	-245.1		PPB	12 Sep 2023 14:15:19	U	SMPL
O4299-09 - 1	MW-01	3005	0.5031	-245.1		PPB	12 Sep 2023 14:17:35	U	SMPL
O4299-09DUP - 1	MW-01DUP	2800	0.4641	-245.1		PPB	12 Sep 2023 14:19:51	U	SMPL
O4299-09MS - 1	MW-01MS	22936	4.2883	-245.1		PPB	12 Sep 2023 14:22:08	U	SMPL
O4299-09MSD - 1	MW-01MSD	20875	3.8969	-245.1		PPB	12 Sep 2023 14:24:25	U	SMPL
O4299-10 - 1	TWP-01	6374	1.1429	-245.1		PPB	12 Sep 2023 14:26:41	U	SMPL
CCV83 - 1	CCV83	25434	4.7627	-245.1		PPB	12 Sep 2023 14:28:56	U	SMPL
CCB83 - 1	CCB83	486	0.0247	-245.1		PPB	12 Sep 2023 14:31:12	U	SMPL
O4343-01 - 1	SAMPLE-1-14TH-ST	3155	0.5315	-245.1		PPB	12 Sep 2023 14:33:26	U	SMPL
O4343-02 - 1	SAMPLE-2-23RD-ST	424	0.0129	-245.1		PPB	12 Sep 2023 14:35:41	U	SMPL
O4299-09LX5 - 1		882	0.0999	-245.1		PPB	12 Sep 2023 14:41:49	U	SMPL
O4299-09A - 1		22151	4.1392	-245.1		PPB	12 Sep 2023 14:44:04	U	SMPL
CCV84 - 1	CCV84	25360	4.7487	-245.1		PPB	12 Sep 2023 14:46:19	U	SMPL
CCB84 - 1	CCB84	254	-0.0194	-245.1		PPB	12 Sep 2023 14:48:36	U	SMPL