


L8127249

7470A

INSTRUMENT ID: CV1

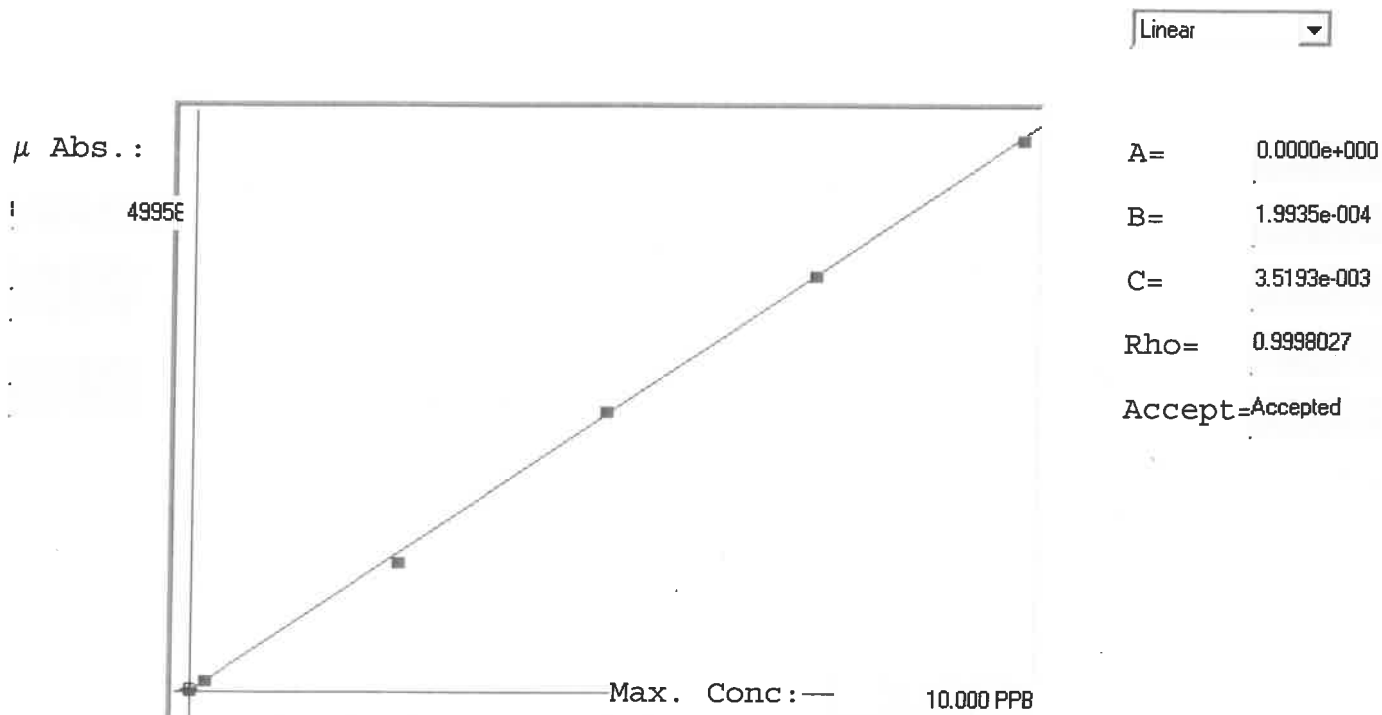

| Std ID | Conc.  | Calc. | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | 0/01D |
|--------|--------|-------|--------|-------|------------|-------|-------|-------|-------|-------|-------|
| 0.0    | 0.000  | 0.045 | 0.045  | 207   | 0.000      | 207   | 0     |       |       |       | 6     |
| 0.2    | 0.200  | 0.212 | 0.012  | 1046  | 0.0 %      | 1046  |       |       |       |       | 6     |
| 2.5    | 2.500  | 2.359 | -0.141 | 11816 | 0.0 %      | 11816 |       |       |       |       | 2     |
| 5.0    | 5.000  | 5.088 | 0.088  | 25505 | 0.0 %      | 25505 |       |       |       |       | 0     |
| 7.5    | 7.500  | 7.533 | 0.033  | 37770 | 0.0 %      | 37770 |       |       |       |       | 0     |
| 10.0   | 10.000 | 9.963 | -0.037 | 49958 | 0.0 %      | 49958 |       |       |       |       | 0     |

## LB127249 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Sep 2023 15:18:05

| Sample ID       | Extended ID                        | µ Abs | Conc    | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|------------------------------------|-------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | So                                 | 207   | -       | 0.000    | 7470A  | PPB   | 12 Sep 2023 15:22:11 | S    | Std  |
| 0.2 - 1         | 51.2                               | 1046  | -       | 0.200    | 7470A  | PPB   | 12 Sep 2023 15:24:28 | S    | Std  |
| 2.5 - 1         | 52.5                               | 11816 | -       | 2.500    | 7470A  | PPB   | 12 Sep 2023 15:26:45 | S    | Std  |
| 5.0 - 1         | 55                                 | 25505 | -       | 5.000    | 7470A  | PPB   | 12 Sep 2023 15:29:01 | S    | Std  |
| 7.5 - 1         | 57.5                               | 37770 | -       | 7.500    | 7470A  | PPB   | 12 Sep 2023 15:31:17 | S    | Std  |
| 10.0 - 1        | 57.5                               | 49958 | -       | 10.000   | 7470A  | PPB   | 12 Sep 2023 15:33:33 | S    | Std  |
| ICV59 - 1       | ICV59                              | 20112 | 4.0129  | -        | 7470A  | PPB   | 12 Sep 2023 15:38:57 | U    | SMPL |
| ICB59 - 1       | ICB59                              | 125   | 0.0284  | -        | 7470A  | PPB   | 12 Sep 2023 15:41:11 | U    | SMPL |
| CCV85 - 1       | CCV85                              | 25363 | 5.0597  | -        | 7470A  | PPB   | 12 Sep 2023 15:43:26 | U    | SMPL |
| CCB85 - 1       | CCB85                              | 150   | 0.0334  | -        | 7470A  | PPB   | 12 Sep 2023 15:45:40 | U    | SMPL |
| CRA - 1         | CRA                                | 1096  | 0.2220  | -        | 7470A  | PPB   | 12 Sep 2023 15:47:55 | U    | SMPL |
| HighStd - 1     | HighStd                            | 49507 | 9.8730  | -        | 7470A  | PPB   | 12 Sep 2023 15:50:10 | U    | SMPL |
| ChkStd - 1      | ChkStd                             | 34651 | 6.9114  | -        | 7470A  | PPB   | 12 Sep 2023 15:52:25 | U    | SMPL |
| PB155458BL - 1  | PBW                                | 34    | 0.0103  | -        | 7470A  | PPB   | 12 Sep 2023 15:54:41 | U    | SMPL |
| PB155458BS - 1  | LCSW                               | 18725 | 3.7364  | -        | 7470A  | PPB   | 12 Sep 2023 15:56:56 | U    | SMPL |
| O4322-03 - 1    | COMP-1                             | 1141  | 0.2310  | -        | 7470A  | PPB   | 12 Sep 2023 15:59:12 | U    | SMPL |
| O4338-03 - 1    | TP4                                | -154  | -0.0272 | -        | 7470A  | PPB   | 12 Sep 2023 16:01:28 | U    | SMPL |
| O4338-06 - 1    | TP3                                | 92    | 0.0219  | -        | 7470A  | PPB   | 12 Sep 2023 16:03:46 | U    | SMPL |
| O4338-09 - 1    | TP2                                | 167   | 0.0368  | -        | 7470A  | PPB   | 12 Sep 2023 16:06:02 | U    | SMPL |
| O4338-09DUP - 1 | TP2DUP                             | 164   | 0.0362  | -        | 7470A  | PPB   | 12 Sep 2023 16:08:17 | U    | SMPL |
| CCV86 - 1       | CCV86                              | 24678 | 4.9232  | -        | 7470A  | PPB   | 12 Sep 2023 16:10:33 | U    | SMPL |
| CCB86 - 1       | CCB86                              | 149   | 0.0332  | -        | 7470A  | PPB   | 12 Sep 2023 16:12:48 | U    | SMPL |
| O4338-09MS - 1  | TP2MS                              | 16572 | 3.3072  | -        | 7470A  | PPB   | 12 Sep 2023 16:15:03 | U    | SMPL |
| O4338-09MSD - 1 | TP2MSD                             | 17577 | 3.5076  | -        | 7470A  | PPB   | 12 Sep 2023 16:17:22 | U    | SMPL |
| PB155500BL - 1  | PBW                                | 127   | 0.0288  | -        | 7470A  | PPB   | 12 Sep 2023 16:19:37 | U    | SMPL |
| PB155500BS - 1  | LCSW                               | 18678 | 3.7271  | -        | 7470A  | PPB   | 12 Sep 2023 16:27:43 | U    | SMPL |
| O4341-01 - 1    | AUD-1046-TOTE                      | 20127 | 4.0159  | -        | 7470A  | PPB   | 12 Sep 2023 16:29:59 | U    | SMPL |
| O4341-02 - 1    | AUD-1047                           | 321   | 0.0675  | -        | 7470A  | PPB   | 12 Sep 2023 16:32:15 | U    | SMPL |
| O4341-02DUP - 1 | AUD-1047DUP                        | 362   | 0.0757  | -        | 7470A  | PPB   | 12 Sep 2023 16:37:10 | U    | SMPL |
| O4341-02MS - 1  | AUD-1047MS                         | 11062 | 2.2068  | -        | 7470A  | PPB   | 12 Sep 2023 16:39:27 | U    | SMPL |
| O4341-02MSD - 1 | AUD-1047MSD                        | 9991  | 1.9953  | -        | 7470A  | PPB   | 12 Sep 2023 16:41:44 | U    | SMPL |
| O4351-11 - 1    | FB                                 | 27    | 0.0089  | -        | 7470A  | PPB   | 12 Sep 2023 16:44:00 | U    | SMPL |
| CCV87 - 1       | CCV87                              | 24610 | 4.9096  | -        | 7470A  | PPB   | 12 Sep 2023 16:46:15 | U    | SMPL |
| CCB87 - 1       | CCB87                              | 174   | 0.0382  | -        | 7470A  | PPB   | 12 Sep 2023 16:48:30 | U    | SMPL |
| O4356-01 - 1    | DISCHARGE-BAY-STREET-SPRING-STREET | 238   | 0.0510  | -        | 7470A  | PPB   | 12 Sep 2023 16:50:46 | U    | SMPL |
| PB155416TB - 1  | PB155416TB                         | 170   | 0.0374  | -        | 7470A  | PPB   | 12 Sep 2023 16:53:01 | U    | SMPL |
| O4338-09LX5 - 1 |                                    | 20    | 0.0075  | -        | 7470A  | PPB   | 12 Sep 2023 16:55:17 | U    | SMPL |
| O4338-09A - 1   |                                    | 19368 | 3.8646  | -        | 7470A  | PPB   | 12 Sep 2023 16:57:32 | U    | SMPL |
| O4341-02LX5 - 1 |                                    | 135   | 0.0304  | -        | 7470A  | PPB   | 12 Sep 2023 16:59:48 | U    | SMPL |
| O4341-02A - 1   |                                    | 18493 | 3.6902  | -        | 7470A  | PPB   | 12 Sep 2023 17:02:04 | U    | SMPL |
| CCV88 - 1       | CCV88                              | 25044 | 4.9962  | -        | 7470A  | PPB   | 12 Sep 2023 17:08:54 | U    | SMPL |
| CCB88 - 1       | CCB88                              | 156   | 0.0346  | -        | 7470A  | PPB   | 12 Sep 2023 17:11:11 | U    | SMPL |