


LB127289

SFAM01.1

INSTRUMENT ID: CV1

Linear

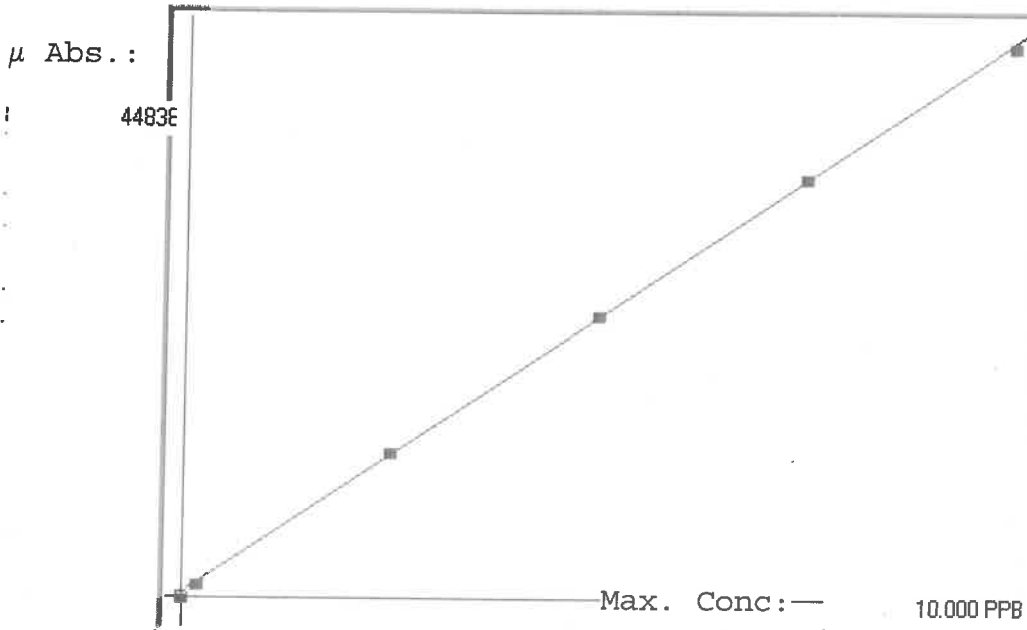

A= 0.0000e+000

B= 2.2330e-004 slope

C= -8.1919e-002 $y = mx + c$

Rho= 0.9999061

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/611
0.00	0.000	-0.058	-0.058	107	0.000	107					5
0.05	0.050					501	0				-8
0.20	0.200	0.185	-0.015	1195	0.0 %	1195					2
2.50	2.500	2.553	0.053	11798	0.0 %	11798					1
5.00	5.000	5.049	0.049	22980	0.0 %	22980					1
7.50	7.500	7.541	0.041	34138	0.0 %	34138					1
10.0	10.000	9.930	-0.070	44838	0.0 %	44838					-1

LB127289

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	107	-		0 SFAM01.1	PPB	9/14/2023 11:58	Std
	0.2 S01	1195	-		0.2 SFAM01.1	PPB	9/14/2023 12:00	Std
	2.5 S02	11798	-		2.5 SFAM01.1	PPB	9/14/2023 12:03	Std
	5 S03	22980	-		5 SFAM01.1	PPB	9/14/2023 12:05	Std
	7.5 S04	34138	-		7.5 SFAM01.1	PPB	9/14/2023 12:07	Std
	10 S05	44838	-		10 SFAM01.1	PPB	9/14/2023 12:23	Std
ICV062	ICV062	17102	3.7369 -		SFAM01.1	PPB	9/14/2023 12:28	SMPL
ICB062	ICB062	14	-0.0788 -		SFAM01.1	PPB	9/14/2023 12:31	SMPL
CCV001	CCV001	21225	4.6575 -		SFAM01.1	PPB	9/14/2023 12:36	SMPL
CCB001	CCB001	24	-0.0766 -		SFAM01.1	PPB	9/14/2023 12:38	SMPL
PB155561BL	PBW561	70	-0.0663 -		SFAM01.1	PPB	9/14/2023 12:40	SMPL
O4176-04	MEZYP0	62	-0.0681 -		SFAM01.1	PPB	9/14/2023 12:43	SMPL
O4176-14	MEZYP1	61	-0.0683 -		SFAM01.1	PPB	9/14/2023 12:45	SMPL
PB155564BL	PBW564	64	-0.0676 -		SFAM01.1	PPB	9/14/2023 12:47	SMPL
O4331-01	MEZYP2	52	-0.0703 -		SFAM01.1	PPB	9/14/2023 12:49	SMPL
O4331-07	MEZYP3	96	-0.0605 -		SFAM01.1	PPB	9/14/2023 12:52	SMPL
O4331-20	MEZYP4	96	-0.0605 -		SFAM01.1	PPB	9/14/2023 12:54	SMPL
CCV002	CCV002	23104	5.0771 -		SFAM01.1	PPB	9/14/2023 12:56	SMPL
CCB002	CCB002	21	-0.0772 -		SFAM01.1	PPB	9/14/2023 12:58	SMPL