


7471B

LB127294

INSTRUMENT ID: CV1

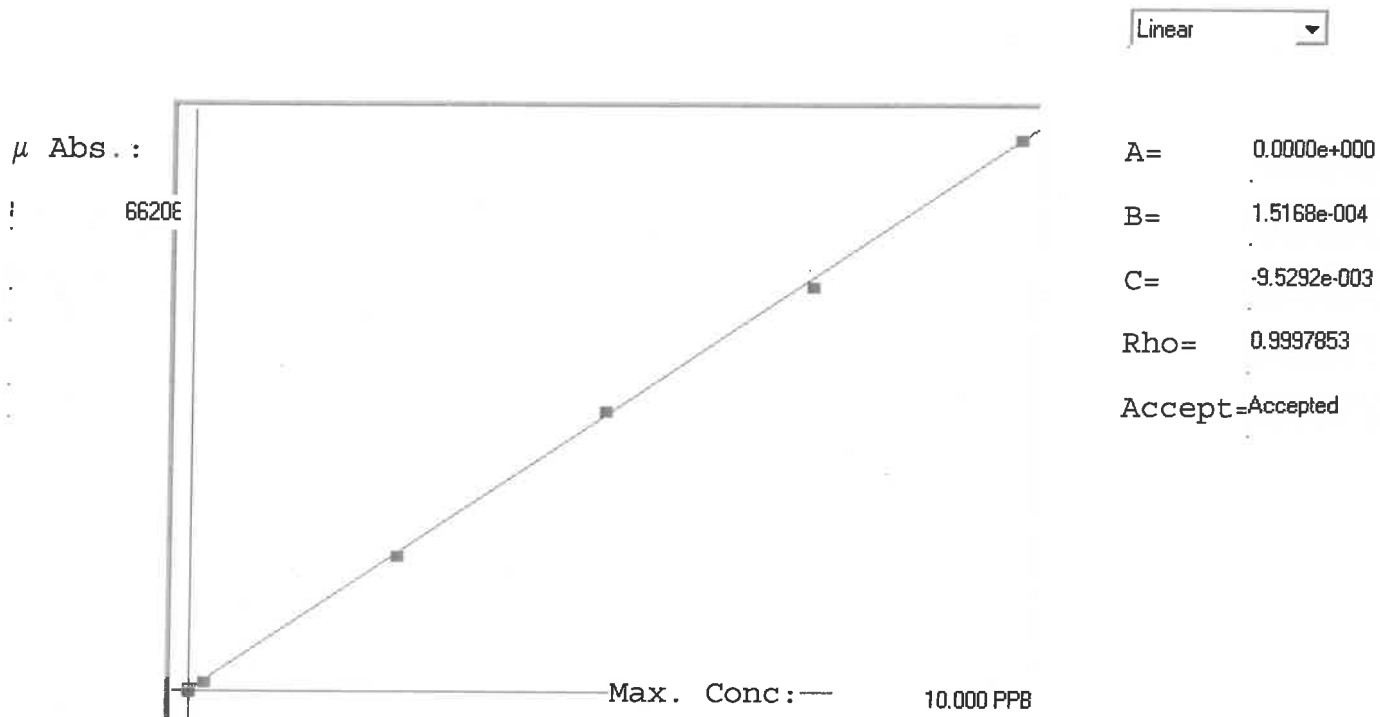

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/1)
0.0	0.000	0.002	0.002	77	0.000	77					
0.2	0.200	0.195	-0.005	1348	0.0 %	1348					
2.5	2.500	2.462	-0.038	16295	0.0 %	16295					
5.0	5.000	5.131	0.131	33891	0.0 %	33891					
7.5	7.500	7.376	-0.124	48692	0.0 %	48692					
10.0	10.000	10.033	0.033	66208	0.0 %	66208					

0/1)

1
3
2
3
2
0

LB127294 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 14 Sep 2023 14:32:52

Sample ID	Extended ID	μ Abs	Conc	Std Conc/Method	Units	Date	Type	Type
0.0 - 1	50	77	-	0.00007471B	PPB	14 Sep 2023 14:37:21	S	Std
0.2 - 1	50-2	1348	-	0.20007471B	PPB	14 Sep 2023 14:39:37	S	Std
2.5 - 1	52-T	16295	-	2.50007471B	PPB	14 Sep 2023 14:41:54	S	Std
5.0 - 1	55	33891	-	5.00007471B	PPB	14 Sep 2023 14:44:10	S	Std
7.5 - 1	57.5	48692	-	7.50007471B	PPB	14 Sep 2023 14:46:28	S	Std
10.0 - 1	518	66208	-	10.00007471B	PPB	14 Sep 2023 14:48:42	S	Std
ICV63 - 1	ICV63	25160	3.8069	-7471B	PPB	14 Sep 2023 14:51:38	U	SMPL
ICB63 - 1	ICB63	1	-0.0094	-7471B	PPB	14 Sep 2023 14:53:53	U	SMPL
CCV03 - 1	CCV03	33183	5.0238	-7471B	PPB	14 Sep 2023 14:56:08	U	SMPL
CCB03 - 1	CCB03	15	-0.0073	-7471B	PPB	14 Sep 2023 14:58:23	U	SMPL
CRA - 1	CRA	1327	0.1918	-7471B	PPB	14 Sep 2023 15:00:38	U	SMPL
HighStd - 1	HighStd	65257	9.8890	-7471B	PPB	14 Sep 2023 15:02:53	U	SMPL
ChkStd - 1	ChkStd	45982	6.9652	-7471B	PPB	14 Sep 2023 15:05:08	U	SMPL
PB155574BL - 1	PBS	-36	-0.0150	-7471B	PPB	14 Sep 2023 15:07:25	U	SMPL
PB155574BS - 1	LCSS	22760	3.4428	-7471B	PPB	14 Sep 2023 15:09:42	U	SMPL
O3572-01 - 1	LOD-MDL-SOIL-01-QT3-2023	393	0.0501	-7471B	PPB	14 Sep 2023 15:14:33	U	SMPL
O3572-01RE - 1	LOD-MDL-SOIL-01-QT3-2023RE	916	0.1294	-7471B	PPB	14 Sep 2023 15:16:49	U	SMPL
O3572-03 - 1	MDL-SOIL-03-QT3-2023	377	0.0477	-7471B	PPB	14 Sep 2023 15:19:05	U	SMPL
O4409-01 - 1	WC-1(0-2)COMP	2086	0.3069	-7471B	PPB	14 Sep 2023 15:21:22	U	SMPL
O4409-04 - 1	WC-2(0-2)COMP	2136	0.3145	-7471B	PPB	14 Sep 2023 15:23:37	U	SMPL
CCV04 - 1	CCV04	32782	4.9630	-7471B	PPB	14 Sep 2023 15:25:52	U	SMPL
CCB04 - 1	CCB04	25	-0.0057	-7471B	PPB	14 Sep 2023 15:28:08	U	SMPL
O4409-07 - 1	WC-3(0-2)COMP	1525	0.2218	-7471B	PPB	14 Sep 2023 15:30:23	U	SMPL
O4409-10 - 1	WC-4(0-6)COMP	10264	1.5474	-7471B	PPB	14 Sep 2023 15:32:38	U	SMPL
O4409-13 - 1	WC-5(0-6)COMP	8751	1.3179	-7471B	PPB	14 Sep 2023 15:34:53	U	SMPL
O4409-16 - 1	WC-6(0-6)COMP	3760	0.5593	-7471B	PPB	14 Sep 2023 15:37:08	U	SMPL
O4423-01 - 1	HD-01-09132023	2585	0.3826	-7471B	PPB	14 Sep 2023 15:39:24	U	SMPL
O4424-01 - 1	SU-03-09132023	1673	0.2442	-7471B	PPB	14 Sep 2023 15:41:40	U	SMPL
O4432-01 - 1	PILE-1	718	0.0994	-7471B	PPB	14 Sep 2023 15:43:56	U	SMPL
O4433-01 - 1	PILE-2	313	0.0379	-7471B	PPB	14 Sep 2023 15:46:13	U	SMPL
O4434-01 - 1	DIRTY-PILE-3	453	0.0592	-7471B	PPB	14 Sep 2023 15:48:30	U	SMPL
O4434-01DUP - 1	DIRTY-PILE-3DUP	415	0.0534	-7471B	PPB	14 Sep 2023 15:50:45	U	SMPL
CCV05 - 1	CCV05	32812	4.9675	-7471B	PPB	14 Sep 2023 15:53:01	U	SMPL
CCB05 - 1	CCB05	37	-0.0039	-7471B	PPB	14 Sep 2023 15:55:16	U	SMPL
O4434-01MS - 1	DIRTY-PILE-3MS	24593	3.7209	-7471B	PPB	14 Sep 2023 15:57:32	U	SMPL
O4434-01MSD - 1	DIRTY-PILE-3MSD	25117	3.8003	-7471B	PPB	14 Sep 2023 15:59:47	U	SMPL
O4434-01LX5 - 1		52	-0.0016	-7471B	PPB	14 Sep 2023 16:02:02	U	SMPL
O4434-01A - 1		24376	3.6879	-7471B	PPB	14 Sep 2023 16:04:17	U	SMPL
CCV06 - 1	CCV06	32882	4.9782	-7471B	PPB	14 Sep 2023 16:06:33	U	SMPL
CCB06 - 1	CCB06	21	-0.0063	-7471B	PPB	14 Sep 2023 16:08:49	U	SMPL