


LB127311

7470A

INSTRUMENT ID: EV1

Linear

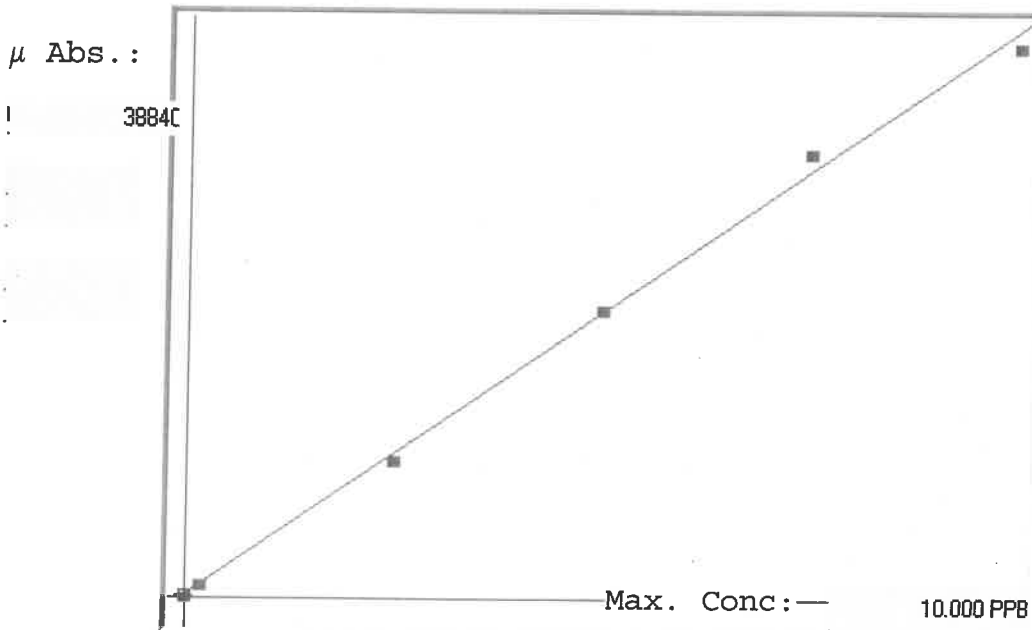

A= 0.0000e+000

B= 2.5159e-004

C= -5.4319e-002

Rho= 0.9986967

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	01,10
0.0	0.000	-0.009	-0.009	182	0.000	182	0				-3
0.2	0.200	0.195	-0.005	992	0.0 %	992					-4
2.5	2.500	2.381	-0.119	9678	0.0 %	9678					2
5.0	5.000	5.081	0.081	20411	0.0 %	20411					4
7.5	7.500	7.835	0.335	31357	0.0 %	31357					-3
10.0	10.000	9.717	-0.283	38840	0.0 %	38840					

LB127311 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Sep 2023 13:29:50

Sample ID	Extended ID	μ Abs	Conc	Stnd Conc	Method	Units	Date	Type	Type
0.0 - 1		182	-	0.0000	7470A	PPB	15 Sep 2023 13:43:36	S	Std
0.2 - 1		992	-	0.2000	7470A	PPB	15 Sep 2023 13:45:53	S	Std
2.5 - 1		9678	-	2.5000	7470A	PPB	15 Sep 2023 13:48:10	S	Std
5.0 - 1		20411	-	5.0000	7470A	PPB	15 Sep 2023 13:50:28	S	Std
7.5 - 1		31357	-	7.5000	7470A	PPB	15 Sep 2023 13:55:31	S	Std
10.0 - 1		38840	-	10.0000	7470A	PPB	15 Sep 2023 14:00:20	S	Std
ICV65 - 1	ICV65	17362	4.3137	-	7470A	PPB	15 Sep 2023 14:03:21	U	SMPL
ICB65 - 1	ICB65	156	-0.0151	-	7470A	PPB	15 Sep 2023 14:05:35	U	SMPL
CCV09 - 1	CCV09	19966	4.9688	-	7470A	PPB	15 Sep 2023 14:07:50	U	SMPL
CCB09 - 1	CCB09	157	-0.0148	-	7470A	PPB	15 Sep 2023 14:10:05	U	SMPL
CRA - 1	CRA	986	0.1937	-	7470A	PPB	15 Sep 2023 14:12:19	U	SMPL
HighStd - 1	HighStd	38835	9.7160	-	7470A	PPB	15 Sep 2023 14:14:34	U	SMPL
ChkStd - 1	ChkStd	28593	7.1393	-	7470A	PPB	15 Sep 2023 14:16:49	U	SMPL
PB155595BL - 1	PBW	123	-0.0234	-	7470A	PPB	15 Sep 2023 14:19:06	U	SMPL
PB155595BS - 1	LCSW	15321	3.8002	-	7470A	PPB	15 Sep 2023 14:21:23	U	SMPL
O3572-07 - 1	LOD-MDL-WATER-01-QT3-2023	458	0.0609	-	7470A	PPB	15 Sep 2023 14:26:21	U	SMPL
O3572-07RE - 1	LOD-MDL-WATER-01-QT3-2023RE	707	0.1236	-	7470A	PPB	15 Sep 2023 14:28:36	U	SMPL
O3572-09 - 1	MDL-WATER-03-QT3-2023	442	0.0569	-	7470A	PPB	15 Sep 2023 14:33:30	U	SMPL
O4348-07 - 1	PT-HG-WP	103324	25.9406	-	7470A	PPB	15 Sep 2023 14:35:46	U	SMPL
CCV10 - 1	CCV10	19770	4.9195	-	7470A	PPB	15 Sep 2023 14:40:19	U	SMPL
CCB10 - 1	CCB10	39	-0.0445	-	7470A	PPB	15 Sep 2023 14:42:38	U	SMPL
O4416-01 - 1	A591	169	-0.0118	-	7470A	PPB	15 Sep 2023 14:44:53	U	SMPL
O4416-01DUP - 1	A591DUP	172	-0.0110	-	7470A	PPB	15 Sep 2023 14:47:08	U	SMPL
O4416-01MS - 1	A591MS	13701	3.3927	-	7470A	PPB	15 Sep 2023 14:49:24	U	SMPL
O4416-01MSD - 1	A591MSD	13866	3.4342	-	7470A	PPB	15 Sep 2023 14:51:39	U	SMPL
O4416-02 - 1	A591	87	-0.0324	-	7470A	PPB	15 Sep 2023 14:53:56	U	SMPL
O4436-21 - 1	FB-9-13	98	-0.0297	-	7470A	PPB	15 Sep 2023 14:56:14	U	SMPL
O4416-01LX5 - 1		18	-0.0498	-	7470A	PPB	15 Sep 2023 14:58:30	U	SMPL
O4416-01A - 1		15545	3.8566	-	7470A	PPB	15 Sep 2023 15:00:46	U	SMPL
CCV11 - 1	CCV11	19999	4.9771	-	7470A	PPB	15 Sep 2023 15:07:37	U	SMPL
CCB11 - 1	CCB11	55	-0.0405	-	7470A	PPB	15 Sep 2023 15:09:55	U	SMPL
O4348-07DLX5 - 1	PT-HG-WP	20727	5.1603	-	7470A	PPB	15 Sep 2023 15:16:41	U	SMPL
CCV12 - 1	CCV12	19543	4.8624	-	7470A	PPB	15 Sep 2023 15:18:56	U	SMPL
CCB12 - 1	CCB12	101	-0.0289	-	7470A	PPB	15 Sep 2023 15:21:12	U	SMPL