

Clear table


Clear table

Clear table

Instrument ID: IC-2									
Analyst : IZ				Method: 300.0 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 11:34
STD2	0.4370	0.6640	0.6720	2.2480	0.5650	0.9910	3.5010	2023-09-13_	9/13/23 12:04
STD3	0.8560	1.1860	1.1800	3.9540	0.9900	1.9910	5.9710	2023-09-13_	9/13/23 12:35
STD4	0.9990	1.5150	1.5110	5.0350	1.2610	2.6440	7.5340	2023-09-13_	9/13/23 13:17
STD5	1.8950	2.9390	2.9450	9.7600	2.4350	4.8490	14.4550	2023-09-13_	9/13/23 13:48
STD6	3.9370	5.9070	5.8970	19.6950	4.9130	9.9780	29.4710	2023-09-13_	9/13/23 14:19
STD7	5.0750	7.5900	7.5960	25.3080	6.3360	12.5480	38.0680	2023-09-13_	9/13/23 14:49
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4	Initial wt/ Final Vol	Analyst
STD1									
STD2	9.2500	10.6667	12.0000	12.4000	13.0000	-0.9000	16.7000		
STD3	7.0000	-1.1667	-1.6667	-1.1500	-1.0000	-0.4500	-0.4833		
STD4	-0.1000	1.0000	0.7333	0.7000	0.8800	5.7600	0.4533		
STD5	-5.2500	-2.0333	-1.8333	-2.4000	-2.6000	-3.0200	-3.6333		
STD6	-1.5750	-1.5500	-1.7167	-1.5250	-1.7400	-0.2200	-1.7633		
STD7	1.5000	1.2000	1.2800	1.2320	1.3760	0.3840	2.8865		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0789497 \cdot A + 4.35704$
 RSD: 3.602 %
 Correlation coefficient: 0.999293

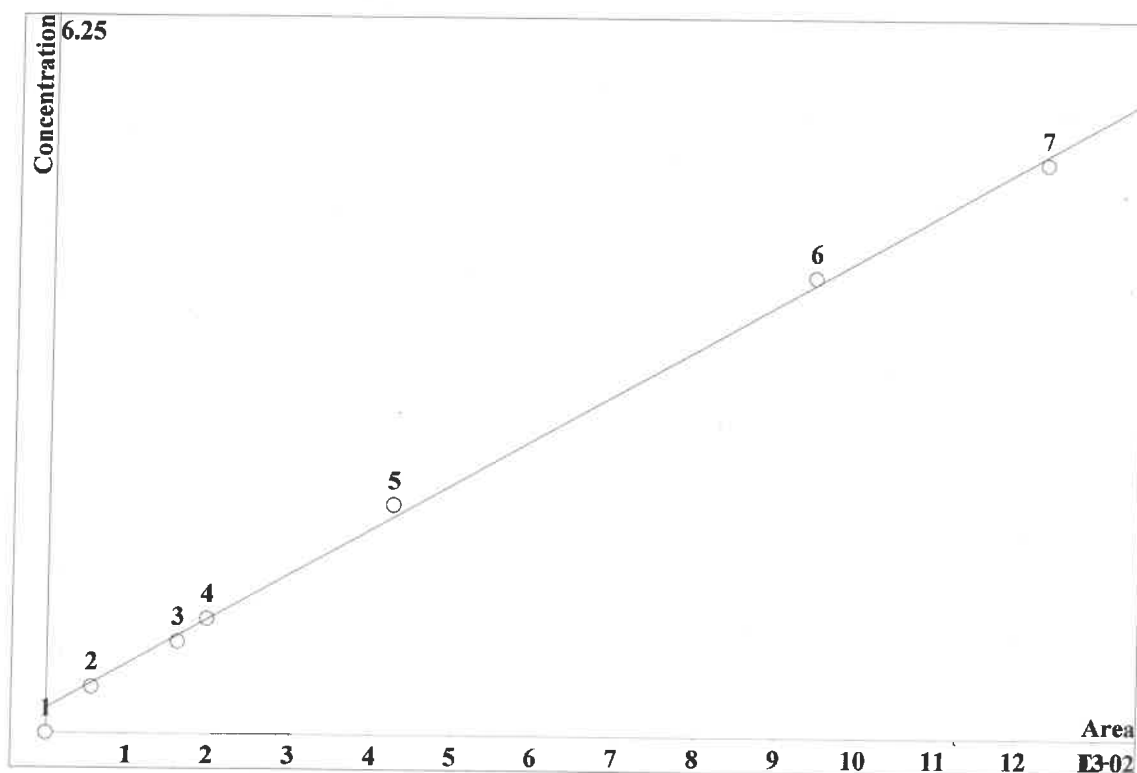


K3 = 0 K2 = 0 K1 = 0.0789497 K0 = 4.35704
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.173	55.53	0.4	20	6.387		
3	1.981	161.8	0.8	20	6.387		
4	2.625	197.8	1	20	6.387		
5	7.098	424.9	2	20	6.387		
6	12.25	942.3	4	20	6.387		
7	16.27	1230	5	20	6.387		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.12855 \cdot A + 3.3899$
 RSD: 2.393 %
 Correlation coefficient: 0.999688

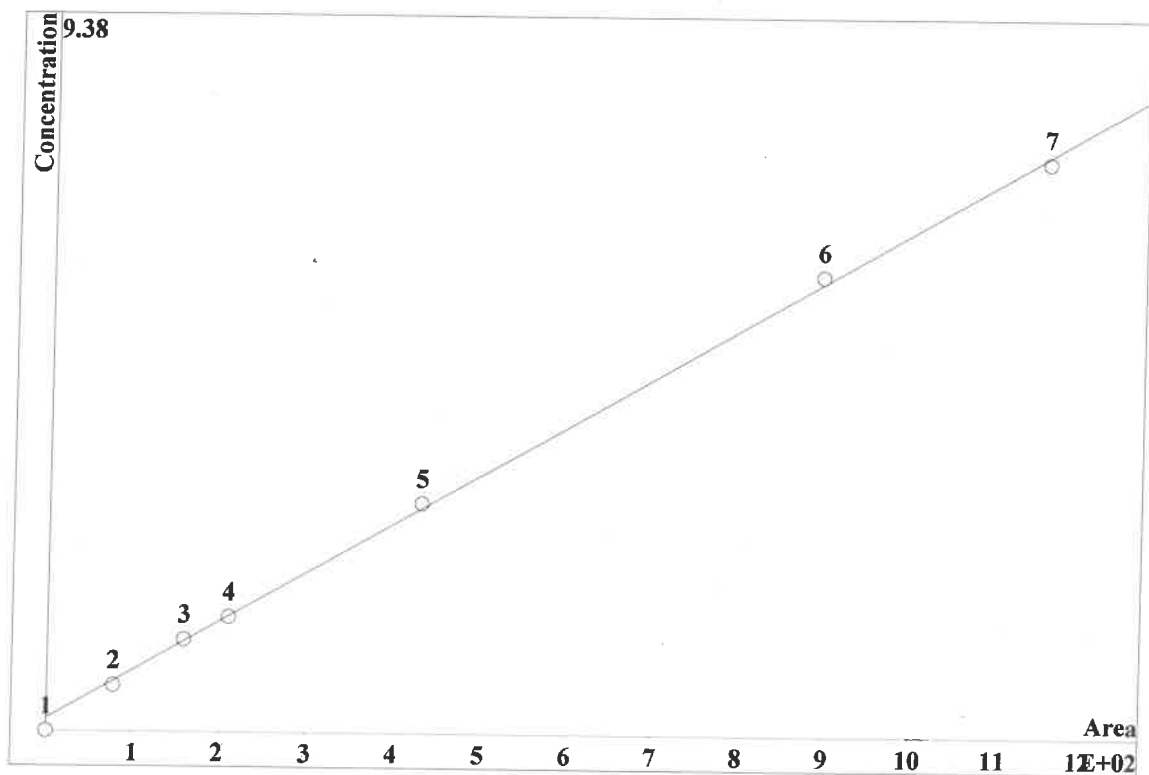


K3 = 0 K2 = 0 K1 = 0.12855 K0 = 3.3899
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.077	76.88	0.6	20	9.512		
3	10.24	158.1	1.2	20	9.512		
4	13.7	209.4	1.5	20	9.512		
5	28.03	430.8	3	20	9.512		
6	58.53	892.6	6	20	9.512		
7	76.44	1154	7.5	20	9.512		
* &							

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0563308 \cdot A + 3.32518$
 RSD: 2.560 %
 Correlation coefficient: 0.999643

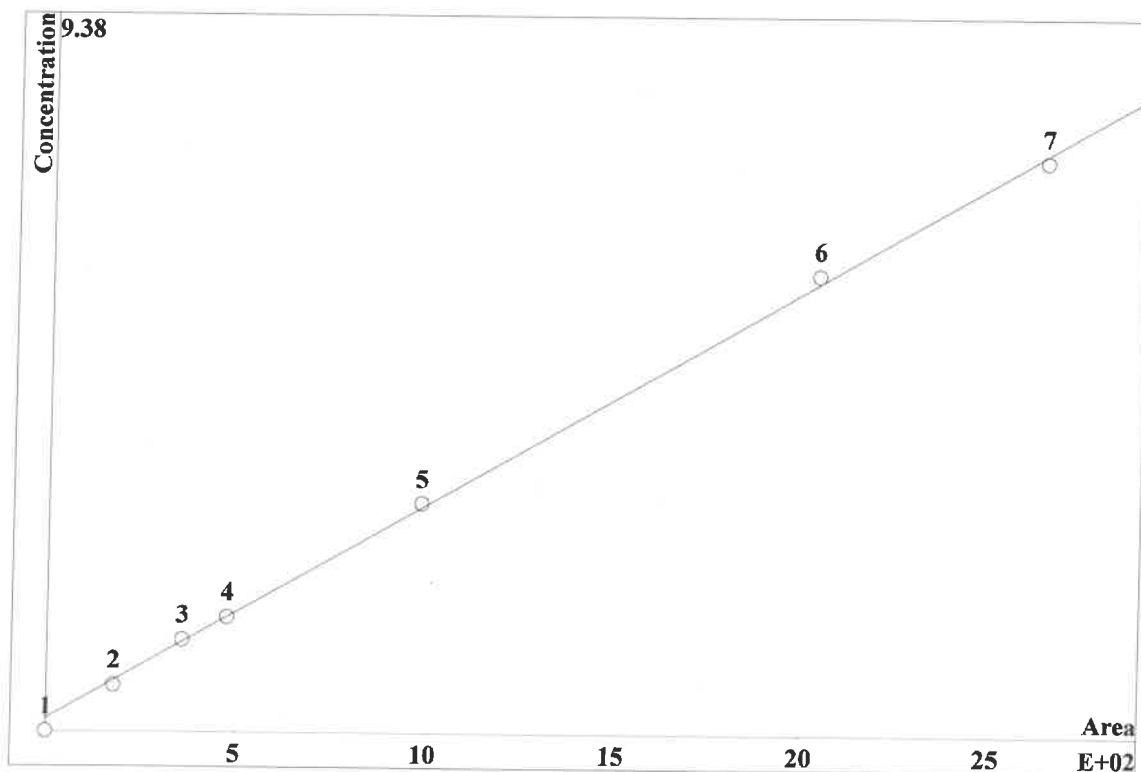


K3 = 0 K2 = 0 K1 = 0.0563308 K0 = 3.32518
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.366	179.4	0.6	20	11.51		
3	18.73	359.8	1.2	20	11.51		
4	25.07	477.3	1.5	20	11.51		
5	50.57	986.7	3	20	11.51		
6	103.2	2035	6	20	11.51		
7	132.4	2638	7.5	20	11.51		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.284269 \cdot A + 12.2101$
 RSD: 2.532 %
 Correlation coefficient: 0.999650

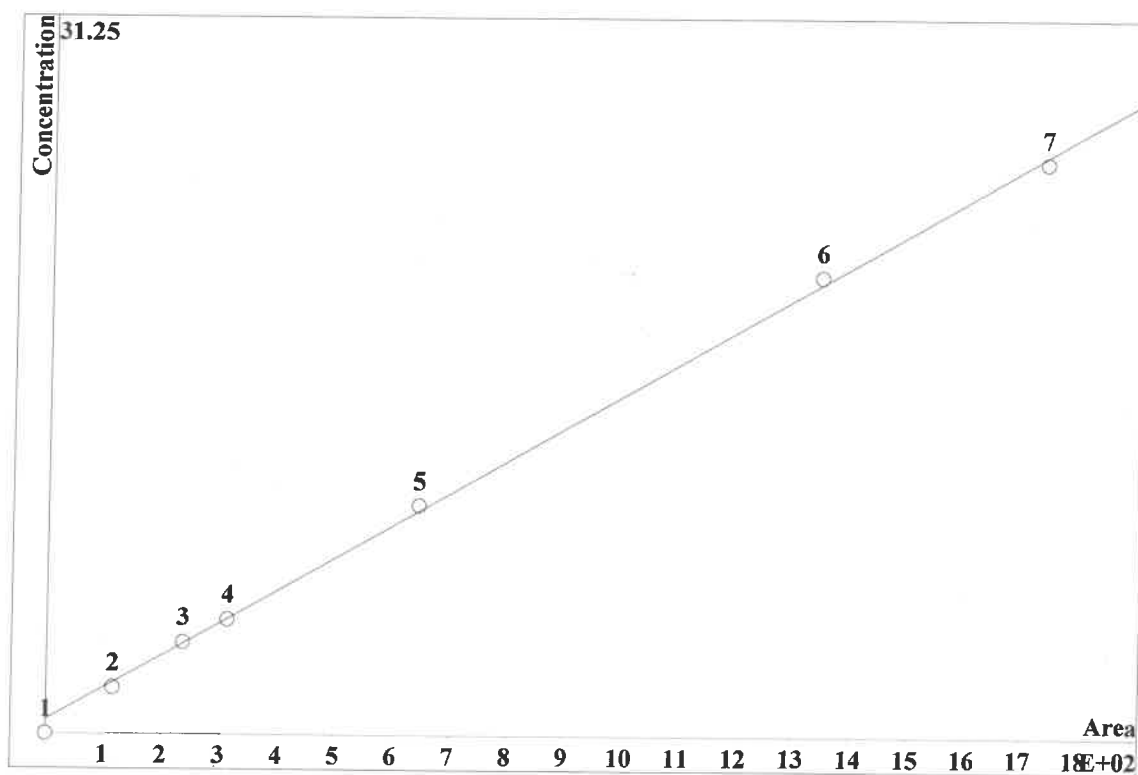


K3 = 0 K2 = 0 K1 = 0.284269 K0 = 12.2101
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.363	115.2	2	20			15
3	10.95	235.3	4	20			15
4	14.67	311.3	5	20			15
5	30.45	643.7	10	20			15
6	64.2	1343	20	20			15
7	83.93	1738	25	20			15

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0496365 \cdot A + 2.72507$
 RSD: 2.794 %
 Correlation coefficient: 0.999574

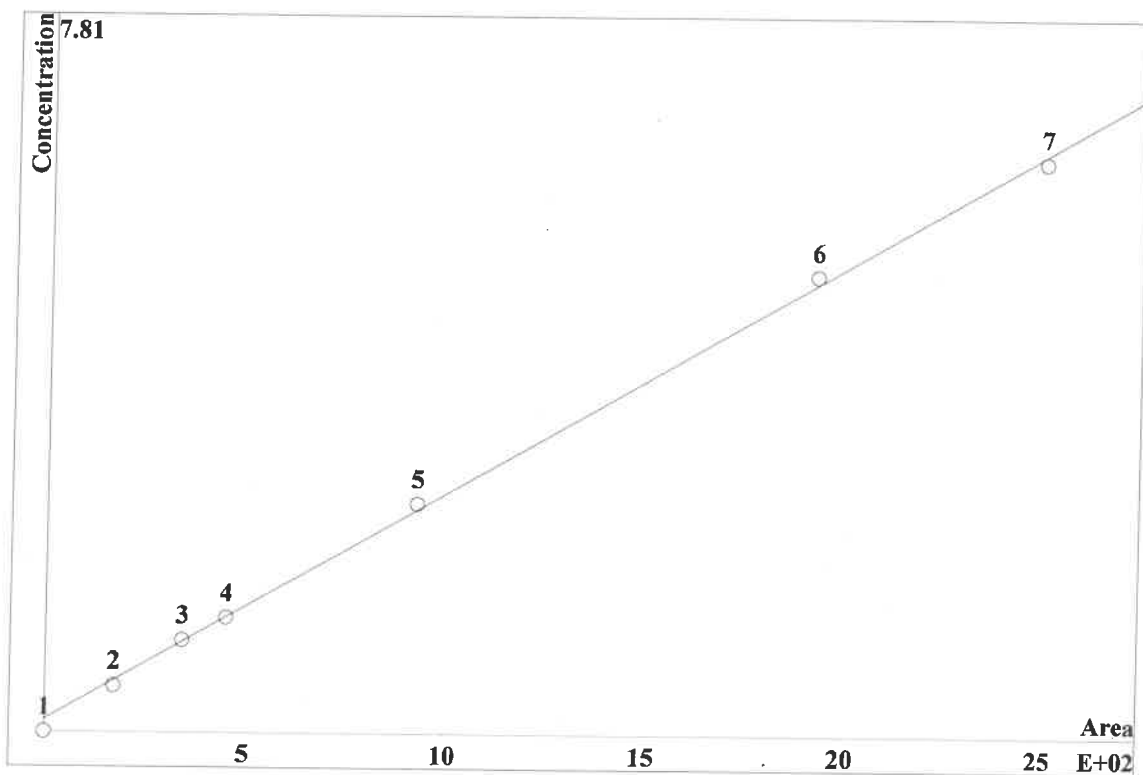


K3 = 0 K2 = 0 K1 = 0.0496365 K0 = 2.72507
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.457	172.6	0.5	20	17.17		
3	12.91	344.1	1	20	17.17		
4	17.23	453.2	1.25	20	17.17		
5	35.37	926.4	2.5	20	17.17		
6	74.05	1925	5	20	17.17		
7	96.74	2498	6.25	20	17.17		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0538776 \cdot A + 5.92726$
 RSD: 1.958 %
 Correlation coefficient: 0.999791

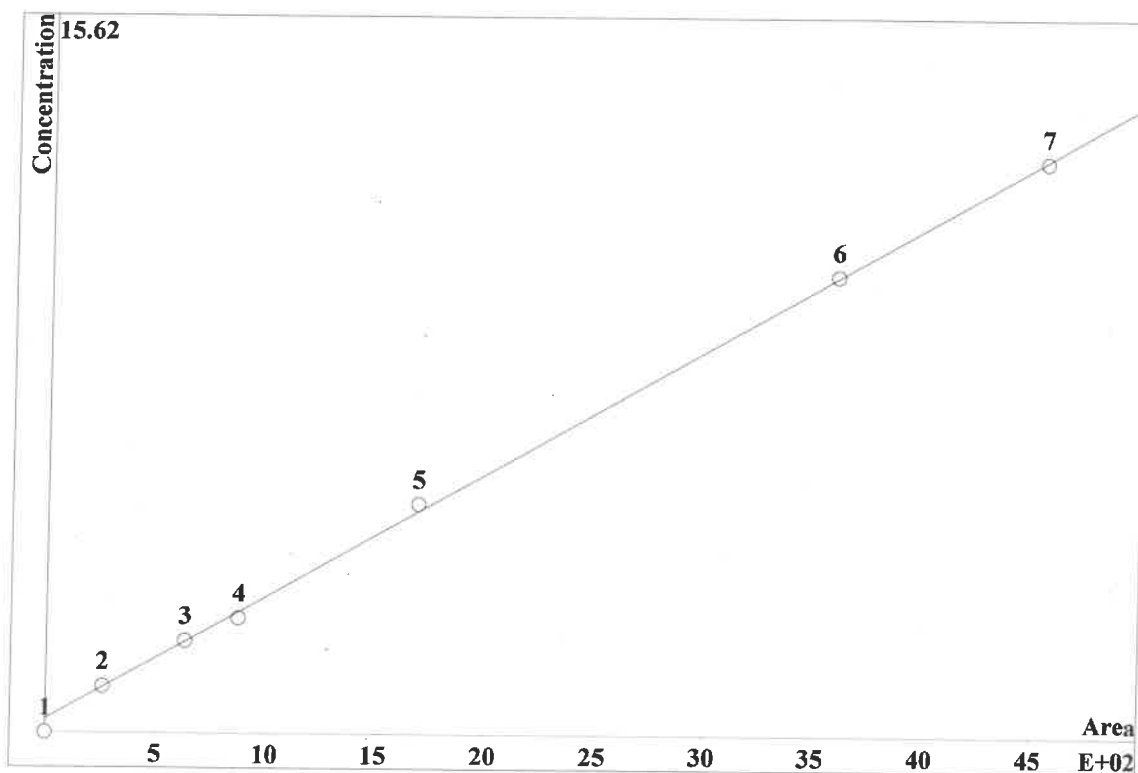


K3 = 0 K2 = 0 K1 = 0.0538776 K0 = 5.92726
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.064	257.8	1	20	22.61		
3	10.79	629	2	20	22.61		
4	15.58	871.3	2.5	20	22.61		
5	31.27	1690	5	20	22.61		
6	74.25	3594	10	20	22.61		
7	97.74	4548	12.5	20	22.61		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.162289 \cdot A + 17.402$
 RSD: 3.254 %
 Correlation coefficient: 0.999423

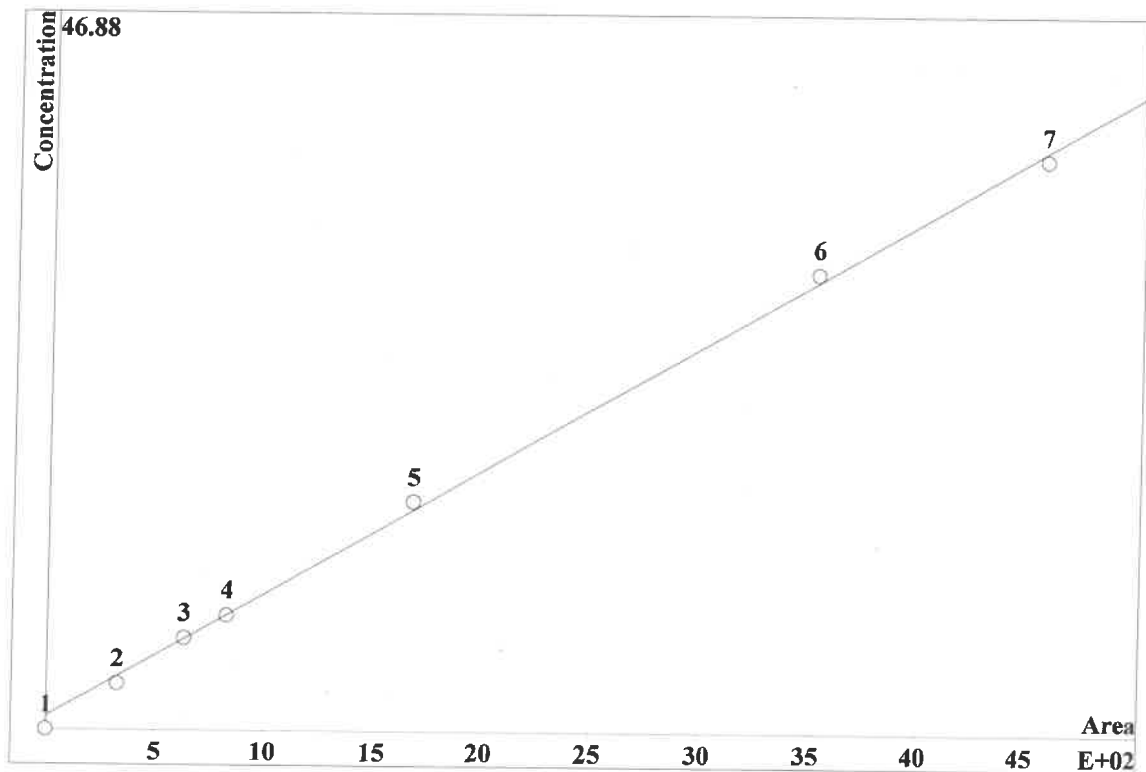

K3 = 0 K2 = 0 K1 = 0.162289 K0 = 17.402
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.494	324.2	3	20	26.01		
3	18.79	628.6	6	20	26.01		
4	25.03	821.3	7.5	20	26.01		
5	51.9	1674	15	20	26.01		
6	110.6	3525	30	20	26.01		
7	145.3	4584	37.5	20	26.01		

Report date: 9/14/2023 10:30:13 AM
Printed by: wet


Ident: STD1
Analysis from: 9/13/2023 11:34:20 AM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35408

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

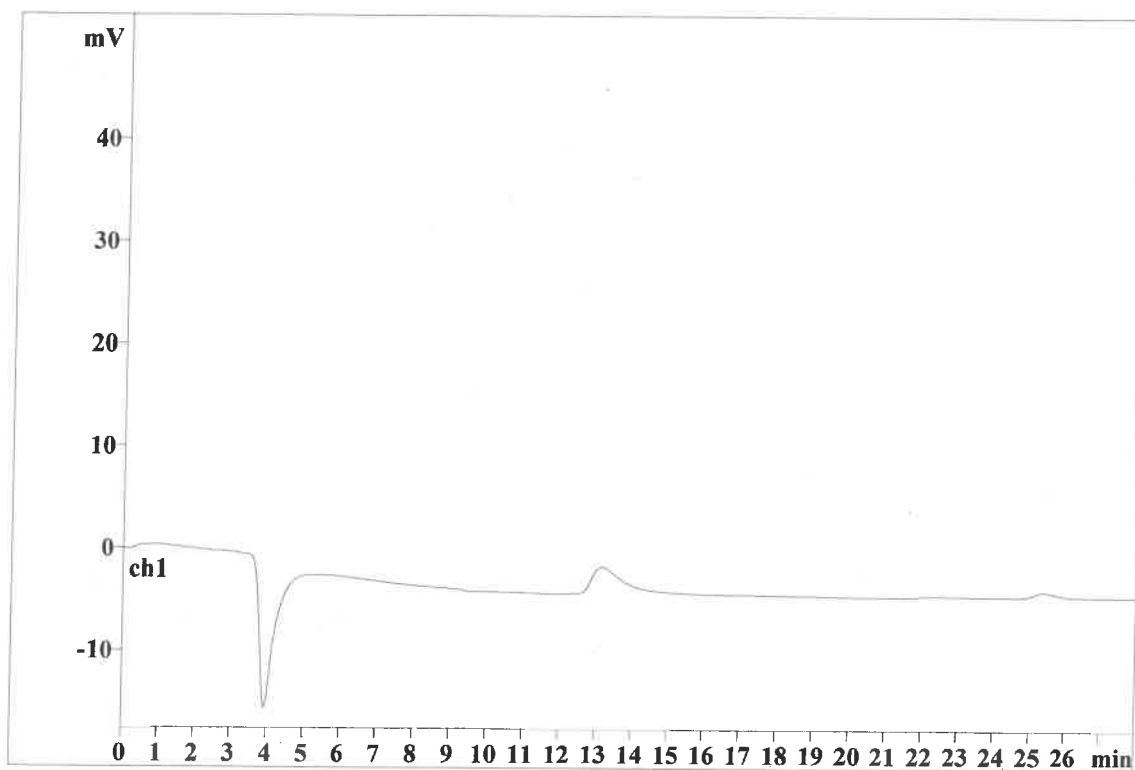

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:19 AM
Printed by: wet


Ident: STD2
Analysis from: 9/13/2023 12:04:58 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35409

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

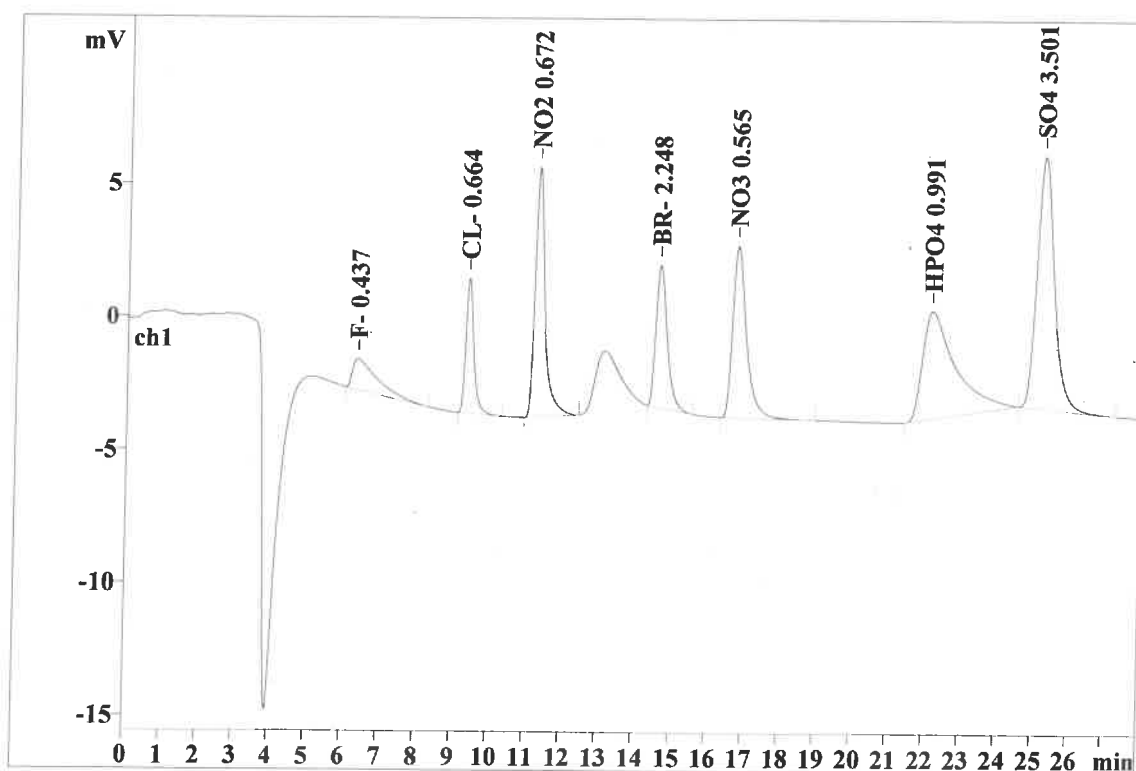

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.35	0.702	1.17	2.86	55.531	4.70
2	9.37	0.223	5.08	12.38	76.877	6.51
3	11.27	0.270	9.37	22.85	179.424	15.18
4	14.62	0.323	5.36	13.08	115.202	9.75
5	16.75	0.390	6.46	15.75	172.628	14.61
6	22.15	0.874	4.06	9.91	257.801	21.82
7	25.23	0.511	9.49	23.16	324.202	27.44
7	28.00	0.470	40.98	99.98	1181.665	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:25 AM
Printed by: wet


Ident: STD3
Analysis from: 9/13/2023 12:35:36 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35410

Last save: 9/13/2023 2:47:

SAMPLE:
:
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

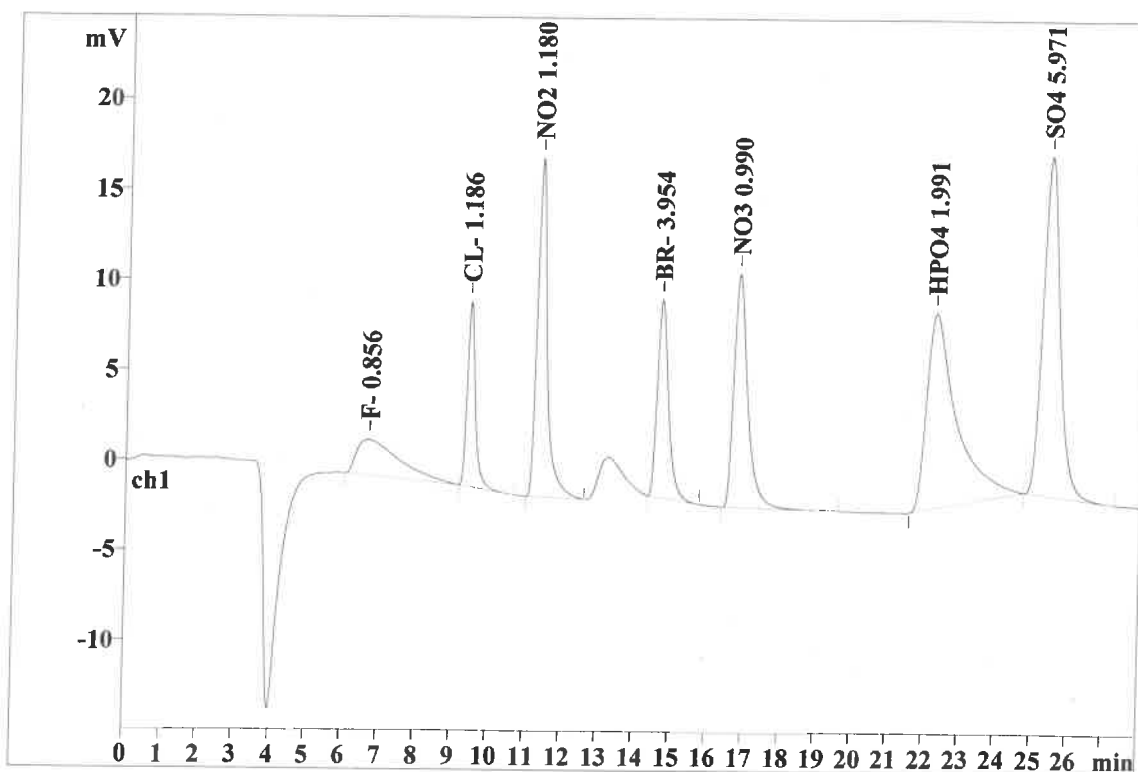

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.67	1.250	1.98	2.35	161.783	6.43
2	9.43	0.224	10.23	12.13	158.085	6.28
3	11.33	0.269	18.73	22.20	359.823	14.30
4	14.68	0.321	10.94	12.97	235.268	9.35
5	16.80	0.388	12.91	15.30	344.076	13.67
6	22.27	0.782	10.79	12.78	629.000	24.99
7	25.41	0.503	18.79	22.26	628.591	24.98
7	28.00	0.534	84.38	99.99	2516.626	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:31 AM
Printed by: wet


Ident: STD4
Analysis from: 9/13/2023 1:17:58 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35411

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

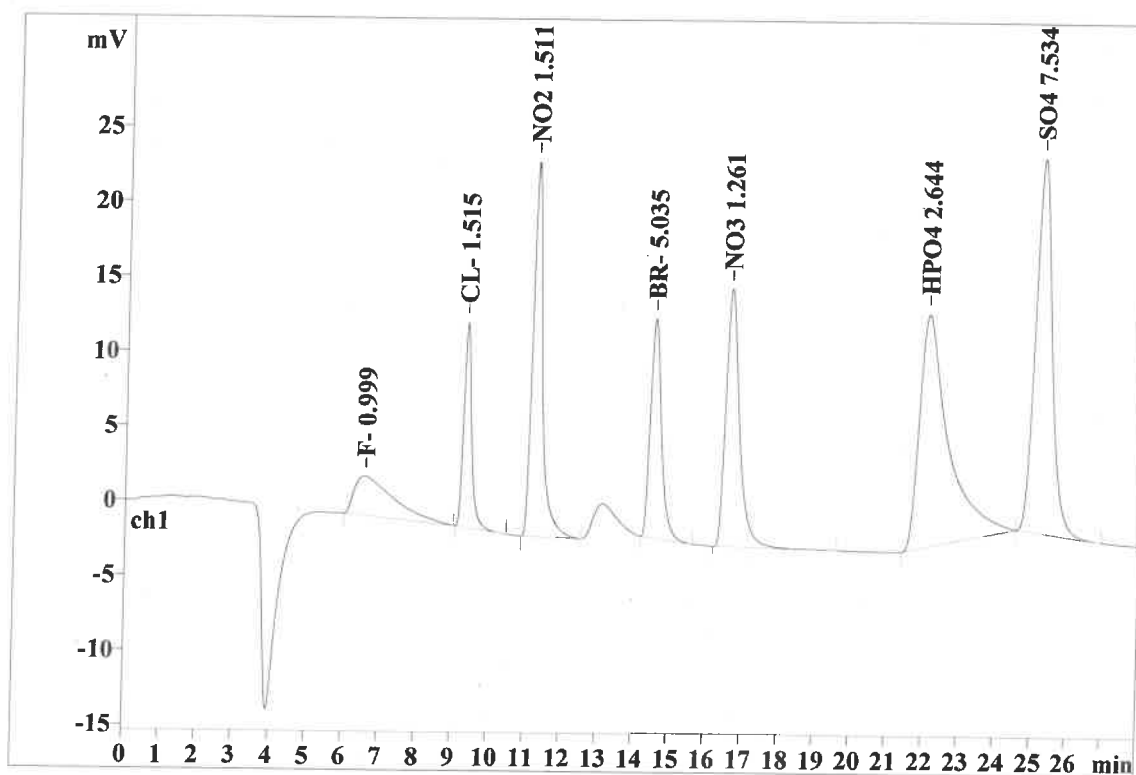

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.56	1.152	2.62	2.30	197.781	5.92
2	9.33	0.222	13.70	12.03	209.390	6.27
3	11.21	0.267	25.07	22.01	477.275	14.28
4	14.52	0.317	14.67	12.88	311.264	9.32
5	16.61	0.384	17.23	15.13	453.175	13.56
6	22.06	0.744	15.57	13.67	871.333	26.08
7	25.19	0.494	25.03	21.97	821.280	24.58
7	28.00	0.512	113.90	99.99	3341.497	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:37 AM
Printed by: wet


Ident: STD5
Analysis from: 9/13/2023 1:48:36 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35412

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

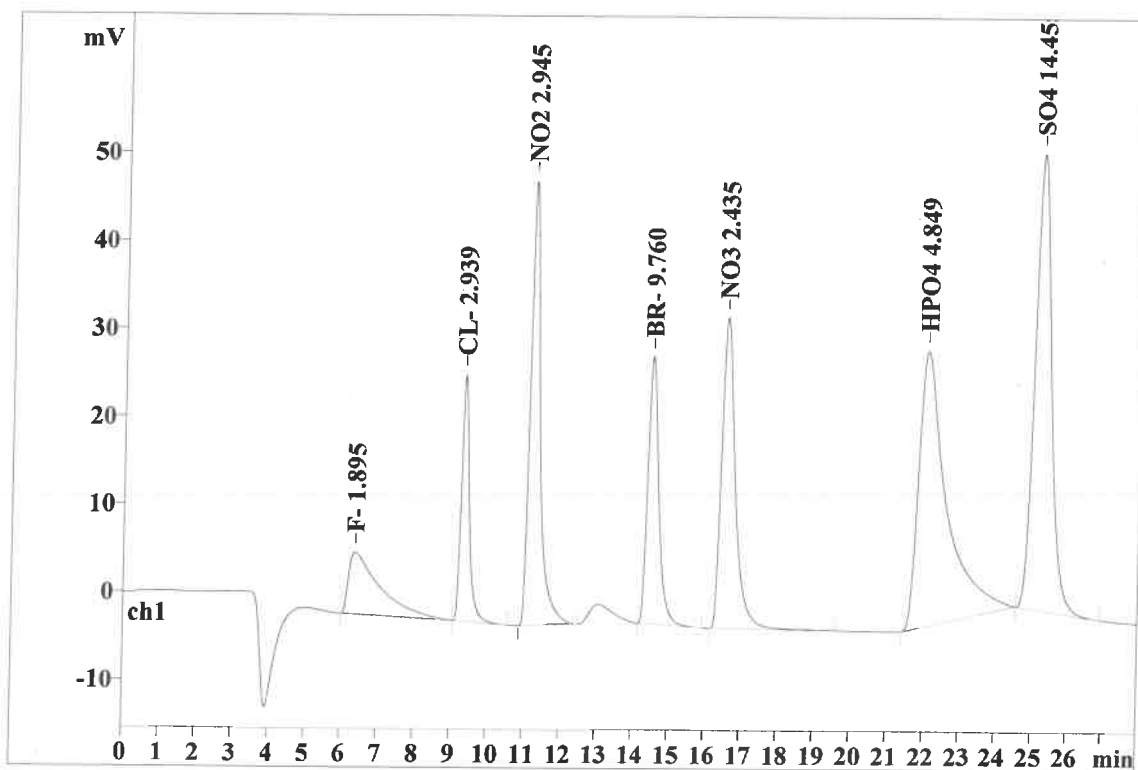

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	0.836	7.10	3.02	424.913	6.27
2	9.35	0.221	28.03	11.94	430.836	6.36
3	11.21	0.273	50.57	21.55	986.701	14.56
4	14.51	0.314	30.45	12.98	643.703	9.50
5	16.56	0.381	35.37	15.07	926.368	13.67
6	22.07	0.712	31.27	13.32	1689.979	24.94
7	25.22	0.486	51.90	22.11	1674.138	24.70
7	28.00	0.460	234.68	100.00	6776.639	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:42 AM
Printed by: wet


Ident: STD6
Analysis from: 9/13/2023 2:19:14 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35413

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

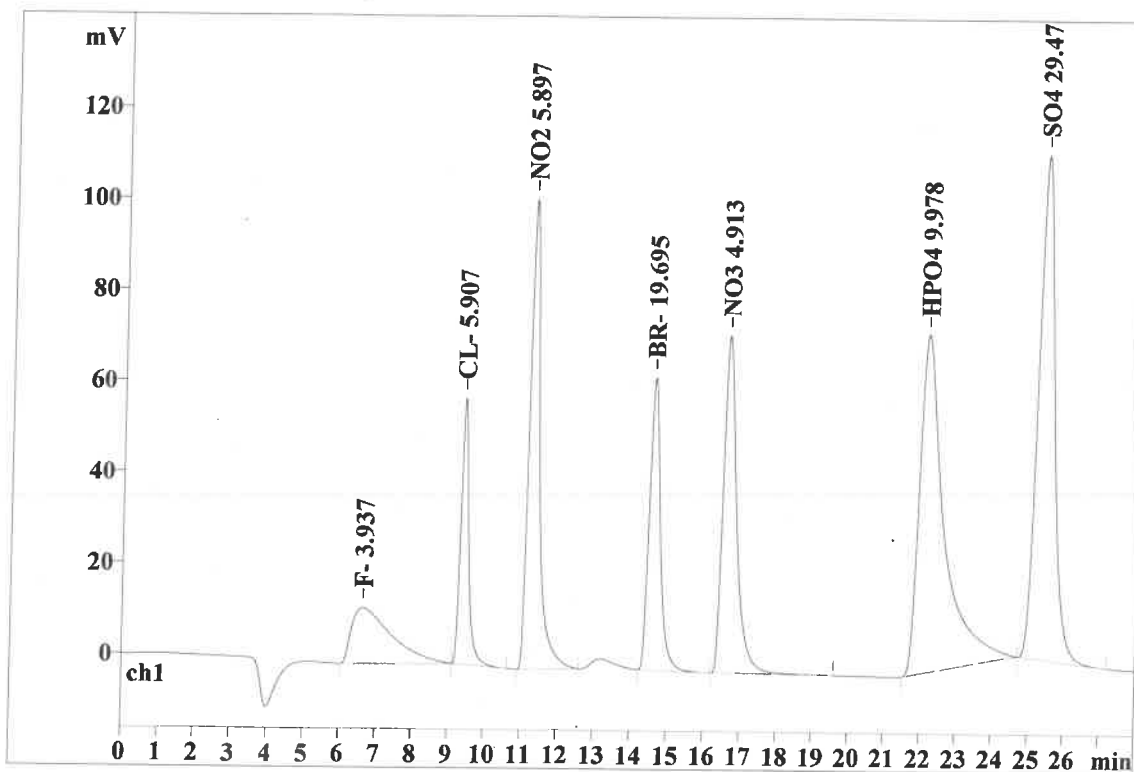

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.63	1.180	12.25	2.46	942.277	6.61
2	9.40	0.219	58.53	11.78	892.649	6.26
3	11.25	0.276	103.16	20.75	2034.568	14.27
4	14.57	0.309	64.20	12.92	1342.719	9.42
5	16.60	0.378	74.04	14.90	1924.573	13.50
6	22.13	0.632	74.25	14.94	3593.867	25.21
7	25.36	0.480	110.60	22.25	3524.692	24.73
7	28.00	0.496	497.04	100.00	14255.344	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:49 AM
Printed by: wet


Ident: STD7
Analysis from: 9/13/2023 2:49:59 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35414

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

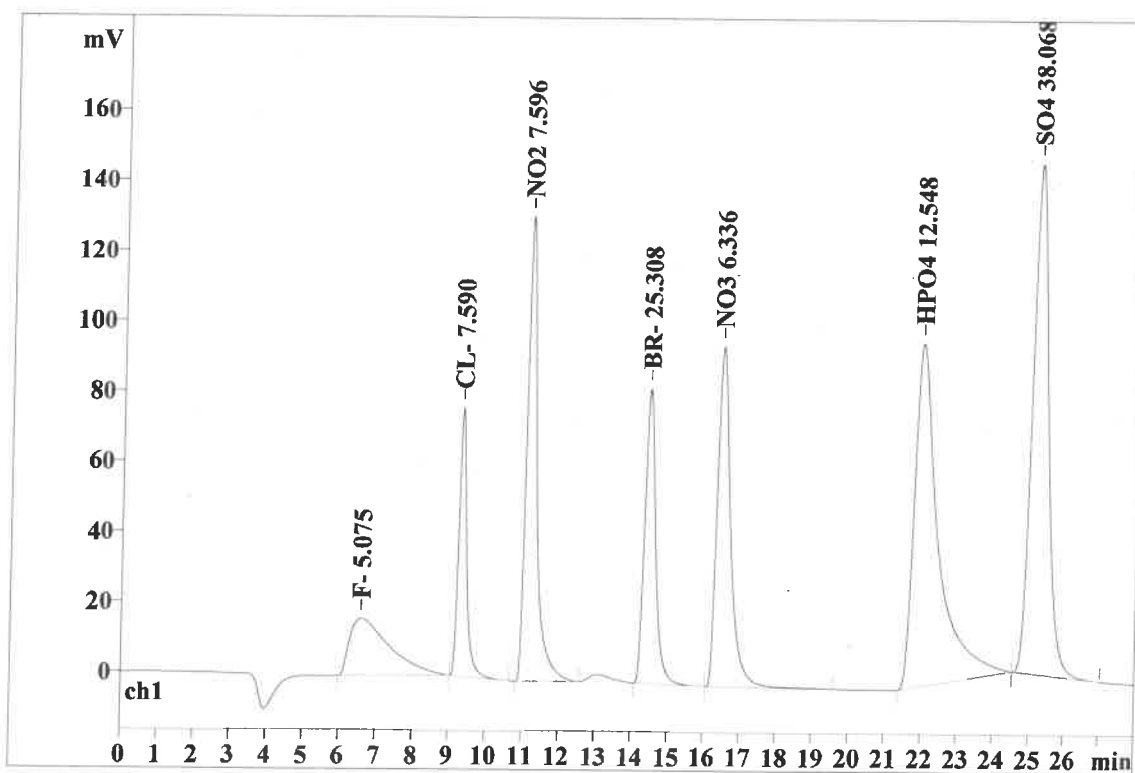

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.60	1.161	16.27	2.51	1230.492	6.69
2	9.32	0.216	76.44	11.78	1154.451	6.28
3	11.16	0.279	132.37	20.40	2637.937	14.34
4	14.46	0.306	83.93	12.94	1737.625	9.45
5	16.45	0.374	96.73	14.91	2498.109	13.58
6	21.96	0.608	97.74	15.07	4547.922	24.73
7	25.19	0.475	145.28	22.39	4584.192	24.93
7	28.00	0.488	648.75	100.00	18390.726	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:54 AM
Printed by: wet


Ident: ICV
Analysis from: 9/13/2023 3:20:37 PM
File: 2023-09-13_

Last save: 9/13/2023 3:48:37 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35415

Last save: 9/13/2023 3:17:

SAMPLE:
: IZ/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

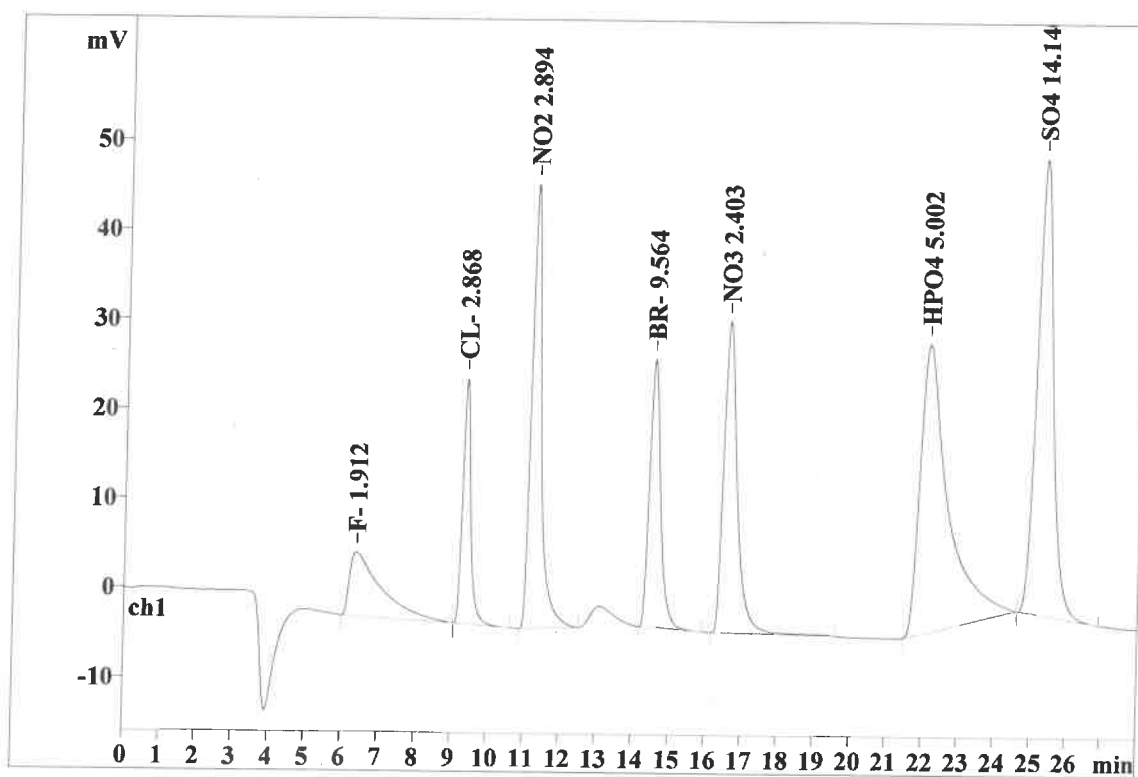

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	0.832	7.15	3.08	426.246	6.33
2	9.35	0.222	27.36	11.79	419.563	6.23
3	11.21	0.274	49.60	21.38	967.809	14.37
4	14.52	0.313	29.96	12.92	629.939	9.35
5	16.57	0.381	34.76	14.99	912.668	13.55
6	22.10	0.713	32.21	13.89	1745.208	25.91
7	25.25	0.484	50.92	21.95	1634.390	24.26
7	28.00	0.460	231.96	100.00	6735.825	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:31:34 AM
Printed by: wet


Ident: ICB
Analysis from: 9/13/2023 3:52:42 PM
File: _2023-09-13_

Last save: 9/14/2023 10:31:13 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35416

Last save: 9/13/2023 3:17:

SAMPLE:
: IZ/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

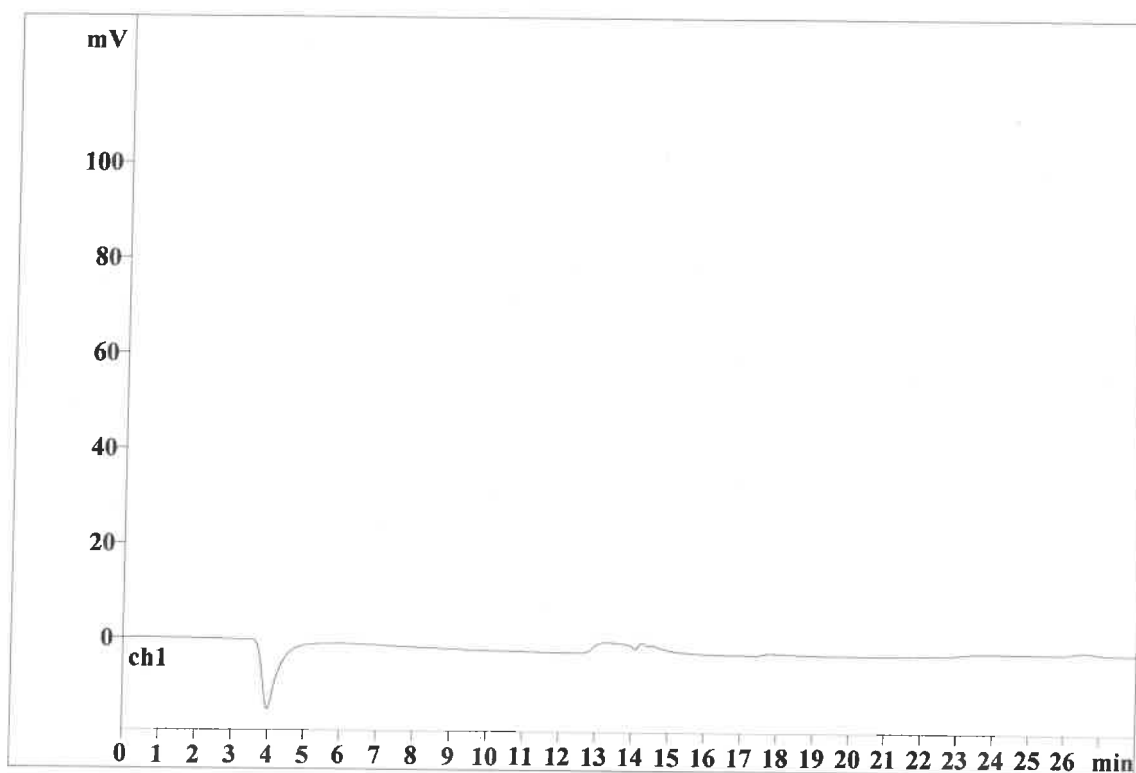

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 2:52:04 PM
Printed by: wet


Ident: CCV
Analysis from: 9/15/2023 6:50:02 PM
File: _2023-09-15_

Last save: 9/18/2023 12:10:29 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35500

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

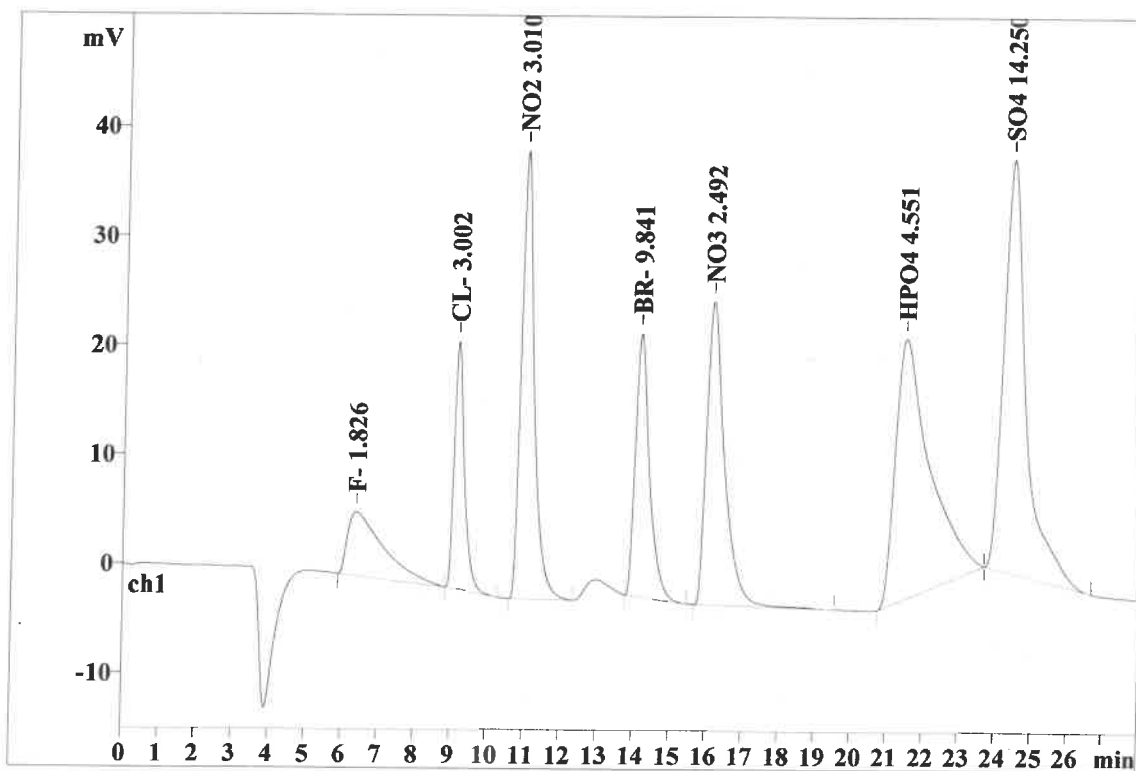

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	1.033	5.85	3.20	404.456	6.06
2	9.14	0.283	22.66	12.39	440.392	6.60
3	10.96	0.356	40.99	22.41	1009.188	15.11
4	14.14	0.395	24.05	13.15	649.423	9.73
5	16.12	0.494	27.71	15.15	948.376	14.20
6	21.44	0.926	23.86	13.05	1577.623	23.63
7	24.37	0.596	37.78	20.65	1647.908	24.68
7	28.00	0.584	182.91	100.00	6677.365	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 2:52:12 PM
Printed by: wet


Ident: CCB
Analysis from: 9/15/2023 7:51:18 PM
File: _2023-09-15_

Last save: 9/15/2023 8:19:17 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35502

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

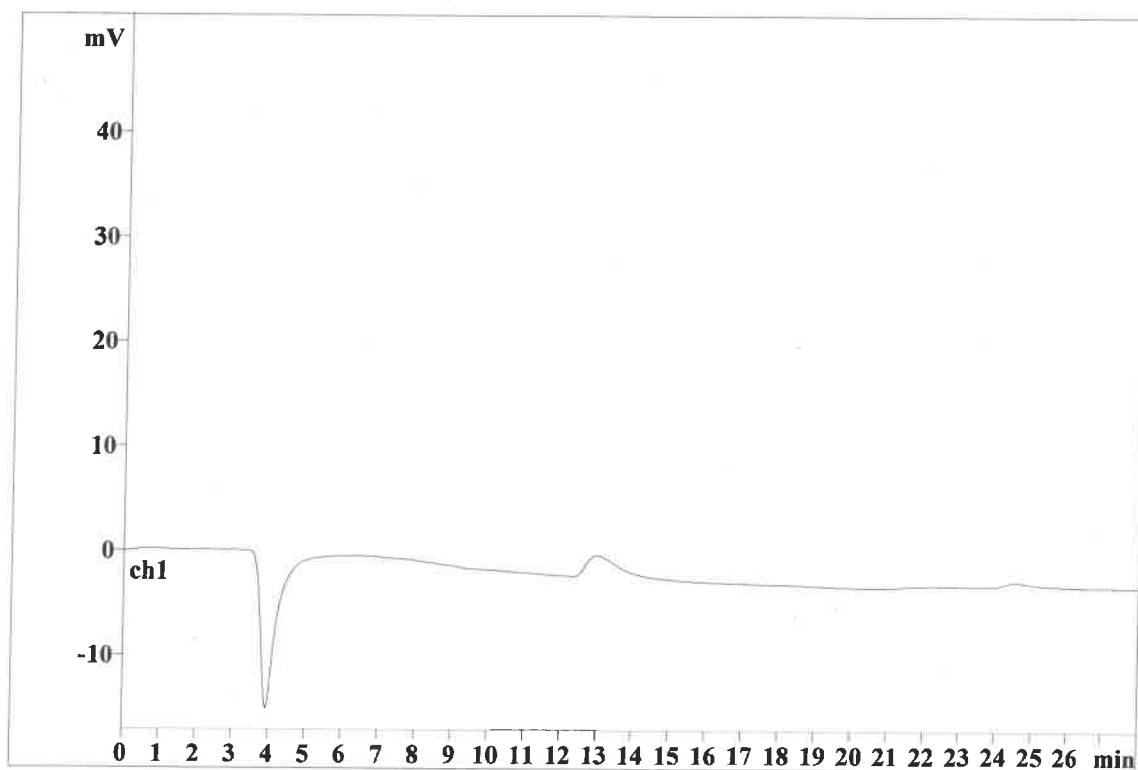

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 2:52:21 PM
Printed by: wet


Ident: LB127341BLW
Analysis from: 9/15/2023 8:21:53 PM
File: _2023-09-15_

Last save: 9/18/2023 1:58:16 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35503

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

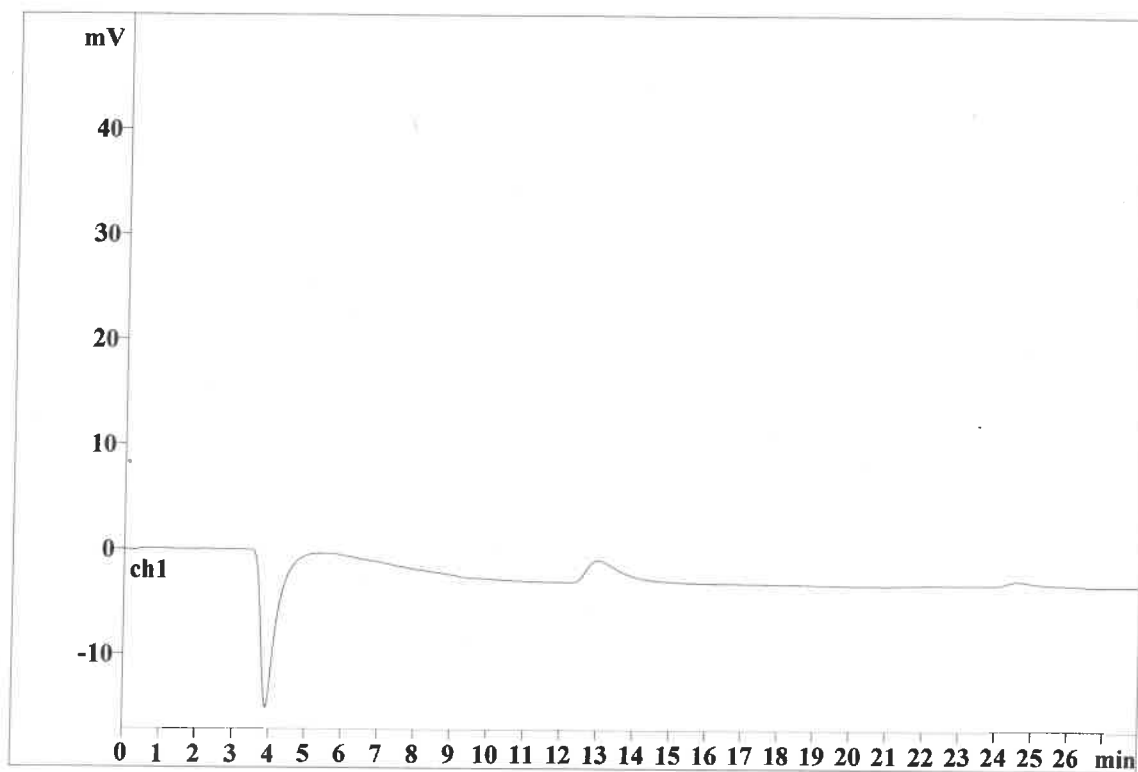

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 2:52:28 PM
Printed by: wet


Ident: LB127341BSW
Analysis from: 9/15/2023 8:52:28 PM
File: _2023-09-15_

Last save: 9/18/2023 1:58:16 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35504

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

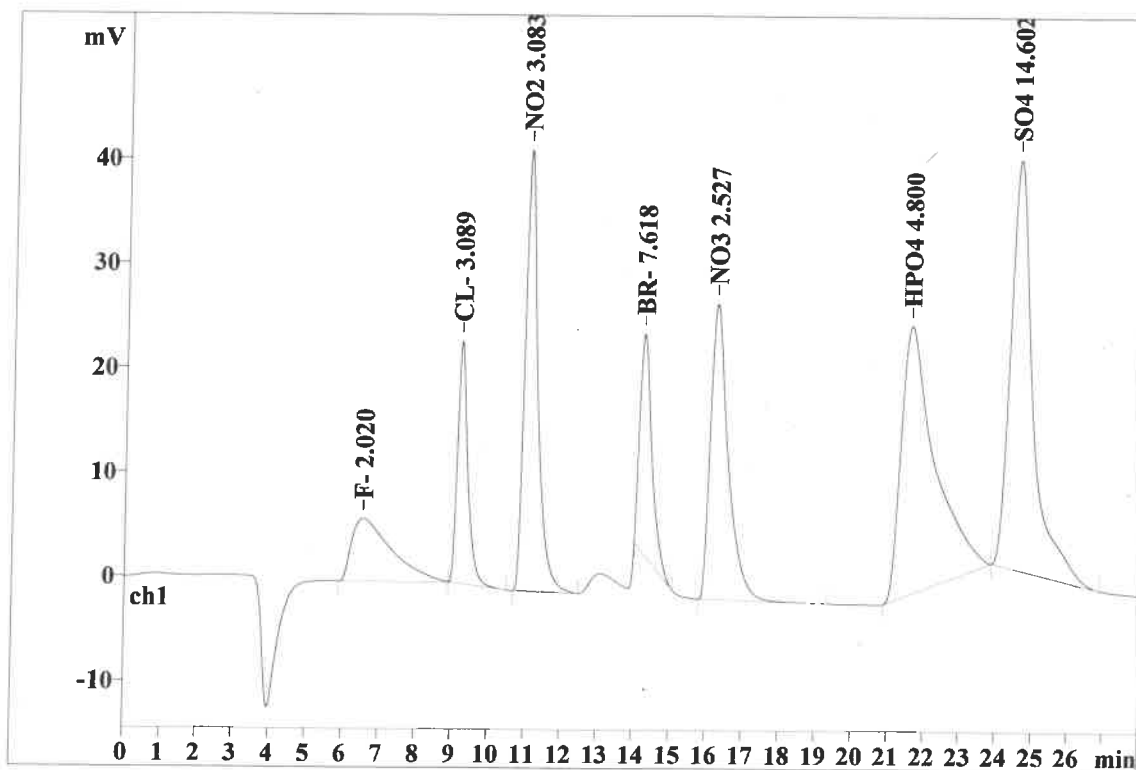

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.54	1.156	6.01	3.24	453.930	6.72
2	9.20	0.282	23.19	12.49	453.839	6.71
3	11.03	0.350	42.21	22.74	1035.133	15.31
4	14.23	0.357	20.96	11.29	493.016	7.29
5	16.21	0.491	28.32	15.26	962.613	14.24
6	21.55	0.891	25.72	13.86	1670.071	24.71
7	24.52	0.588	39.19	21.12	1691.335	25.02
7	28.00	0.588	185.61	100.00	6759.937	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:19:33 PM
Printed by: wet


Ident: 04466-01
Analysis from: 9/15/2023 9:23:08 PM
File: _2023-09-15_

Last save: 9/18/2023 12:22:36 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35505

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

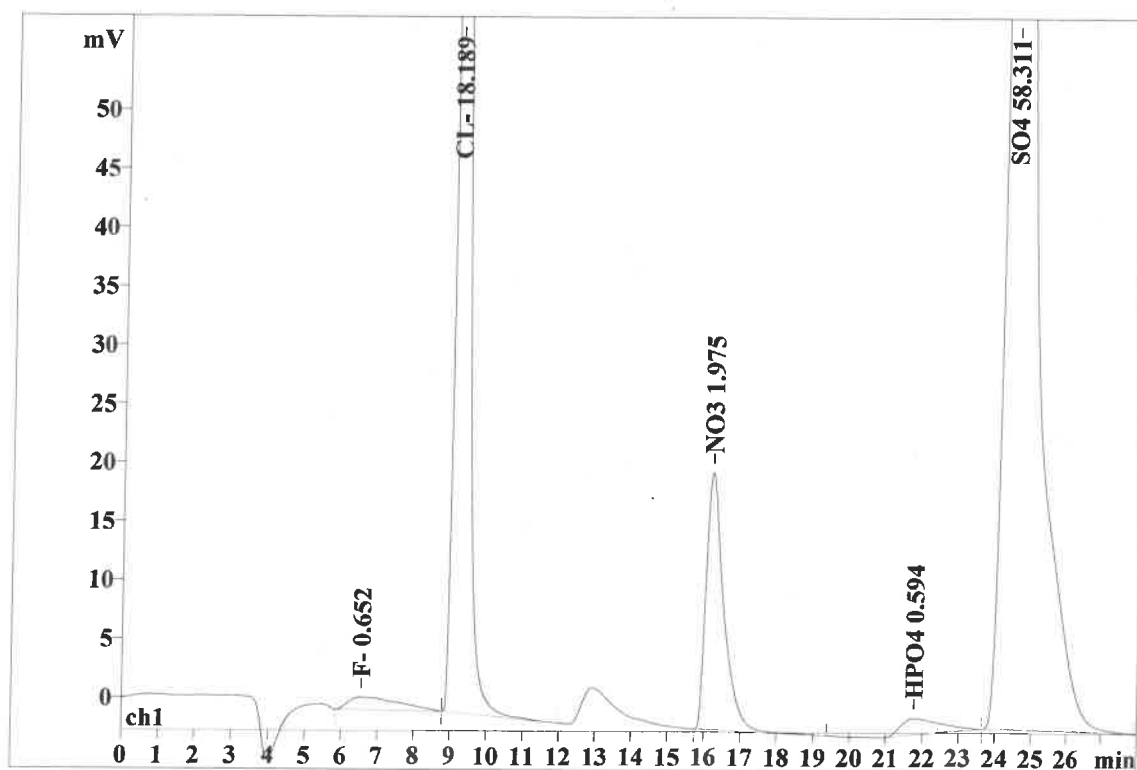

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.54	1.653	1.08	0.33	105.258	0.97
2	9.14	0.285	140.65	43.11	2804.874	25.88
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.18	0.491	21.88	6.71	739.932	6.83
6	21.75	1.233	1.40	0.43	107.127	0.99
7	24.45	0.588	161.25	49.42	7080.663	65.33
7	28.00	0.607	326.26	100.00	10837.853	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:19:42 PM
Printed by: wet


Ident: O4466-02
Analysis from: 9/15/2023 9:53:43 PM
File: _2023-09-15_

Last save: 9/18/2023 12:22:53 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35506

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

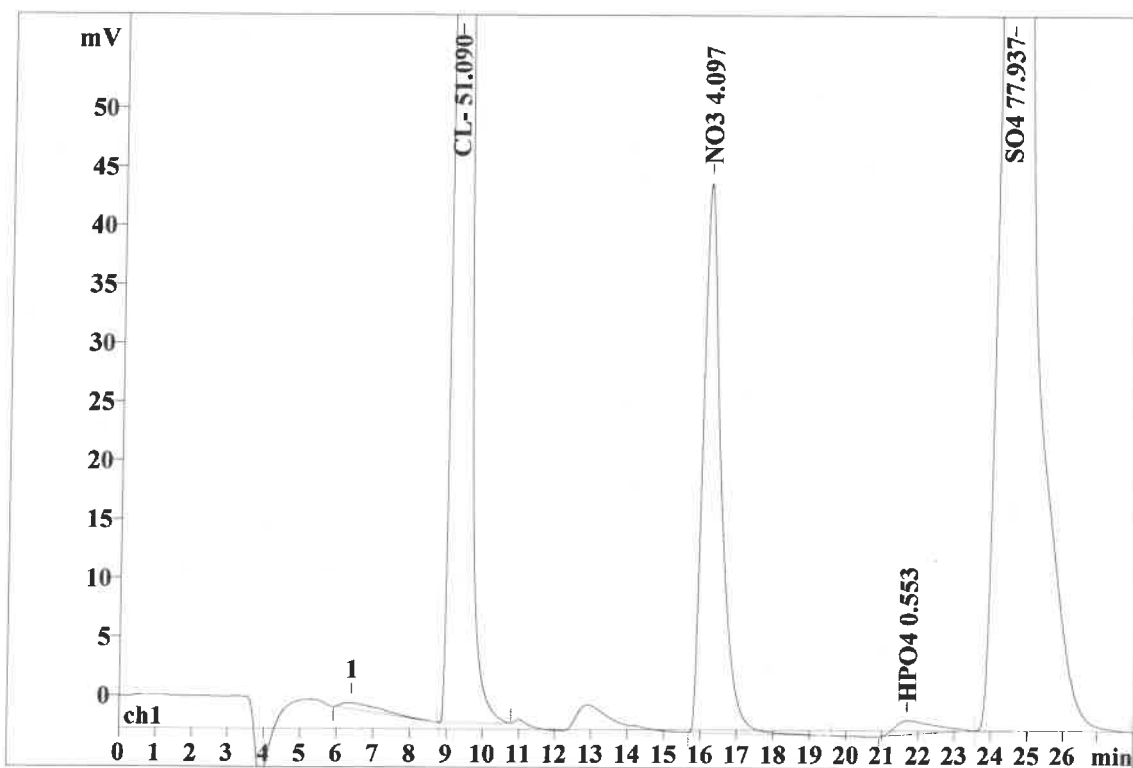

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.18	0.262	431.45	62.11	7927.238	41.38
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.13	0.494	46.76	6.73	1595.659	8.33
6	21.70	1.238	1.21	0.17	91.996	0.48
7	24.40	0.595	214.64	30.90	9500.635	49.59
7	28.00	0.370	694.05	99.92	19115.528	99.77

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:19:50 PM
Printed by: wet


Ident: O4466-03
Analysis from: 9/15/2023 10:24:19 PM
File: _2023-09-15_

Last save: 9/18/2023 12:24:25 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35507

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

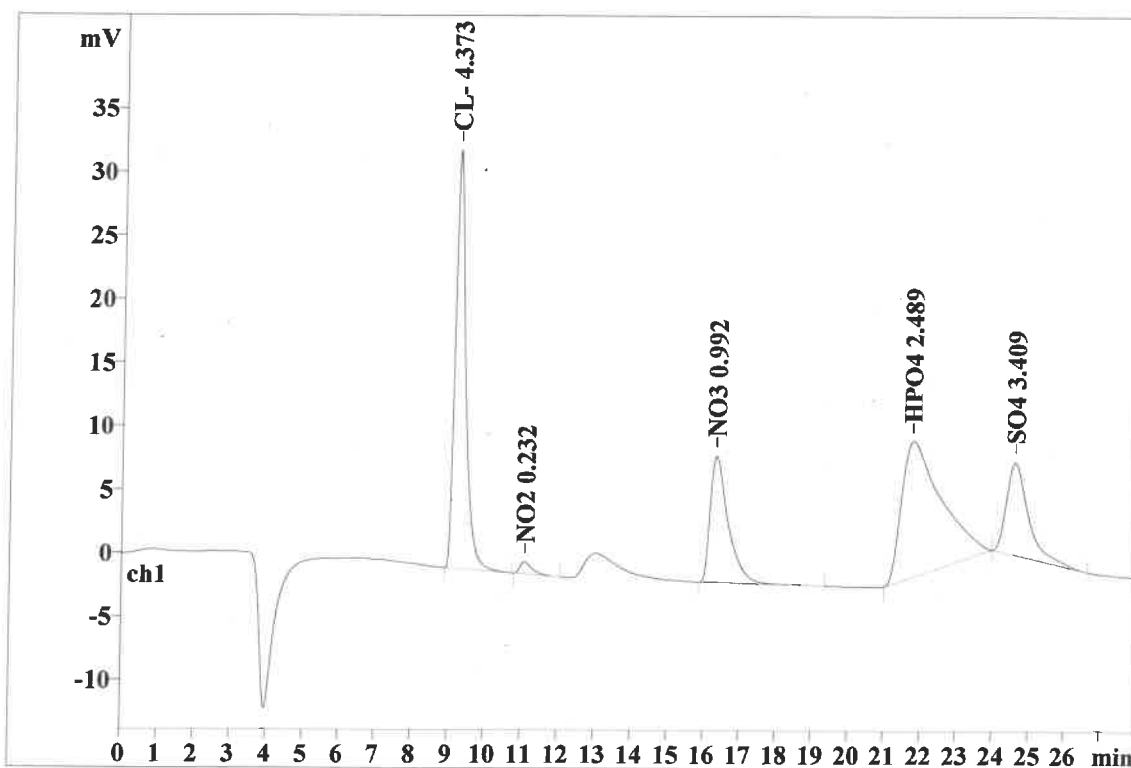

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.22	0.284	32.93	53.30	653.852	30.52
3	11.09	0.344	0.94	1.52	21.958	1.02
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.32	0.498	9.94	16.09	343.708	16.04
6	21.74	1.151	10.70	17.32	811.558	37.88
7	24.58	0.610	7.27	11.76	311.202	14.53
7	28.00	0.412	61.77	99.99	2142.278	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:20:24 PM
Printed by: wet


Ident: O4466-03MS
Analysis from: 9/15/2023 10:54:54 PM
File: _2023-09-15_

Last save: 9/18/2023 3:20:22 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35508

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

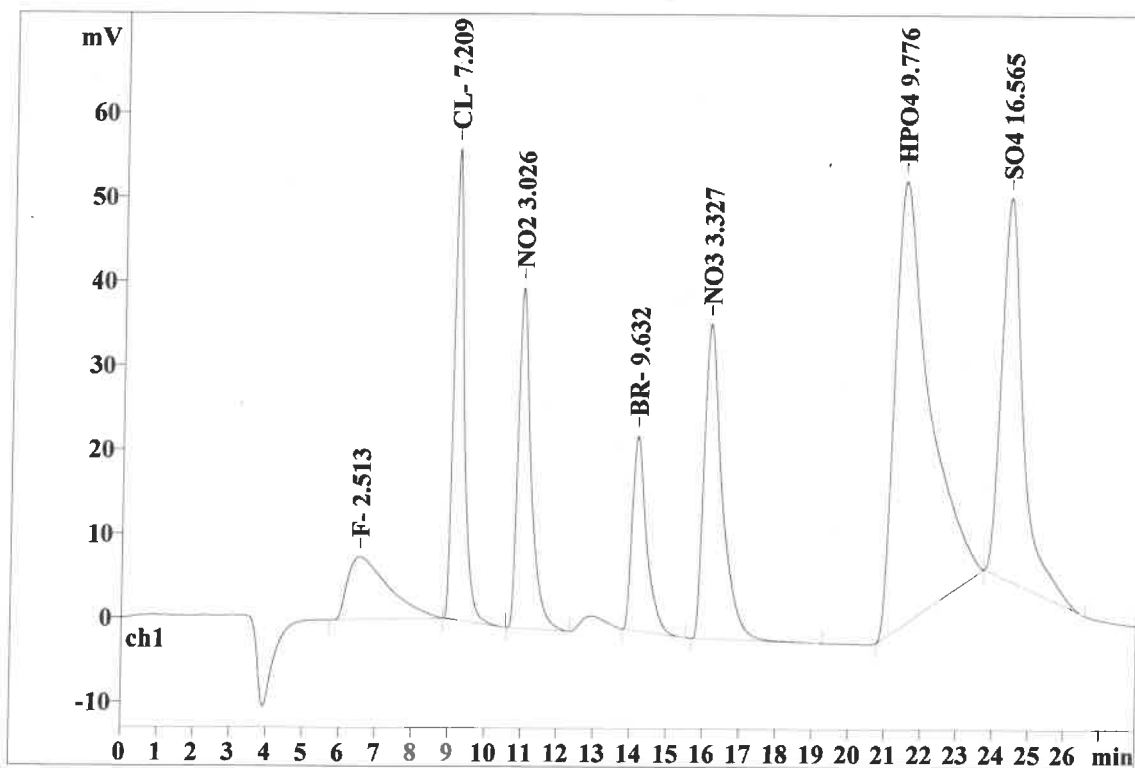

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.53	1.194	7.46	2.84	579.476	5.76
2	9.14	0.279	56.02	21.31	1095.363	10.89
3	10.96	0.358	40.49	15.41	1014.779	10.09
4	14.15	0.398	23.17	8.82	634.686	6.31
5	16.12	0.494	37.42	14.24	1285.081	12.77
6	21.44	0.928	52.87	20.12	3519.141	34.97
7	24.37	0.595	45.39	17.27	1933.352	19.21
7	28.00	0.606	262.81	100.00	10061.879	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:20:50 PM
Printed by: wet


Ident: O4466-03MSD
Analysis from: 9/15/2023 11:25:30 PM
File: _2023-09-15_

Last save: 9/18/2023 3:20:48 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35509

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

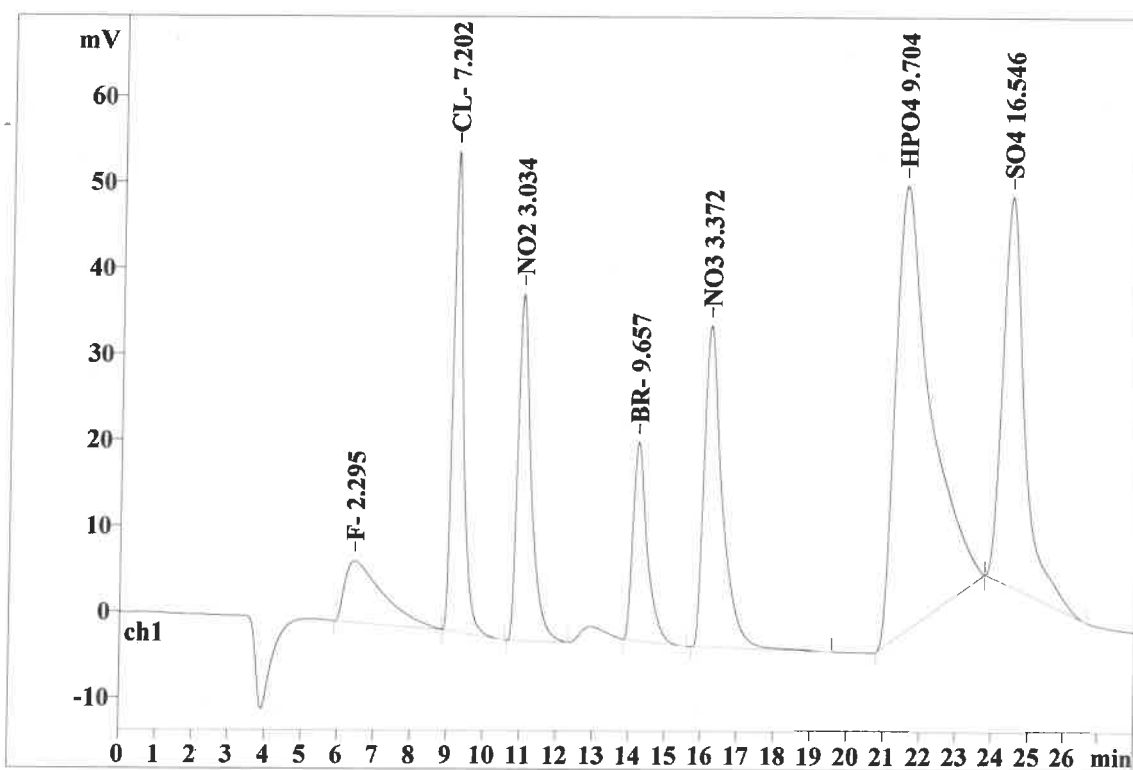

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.43	1.114	7.18	2.75	523.829	5.24
2	9.17	0.279	55.89	21.40	1094.220	10.94
3	11.00	0.362	40.29	15.42	1017.470	10.18
4	14.20	0.399	23.13	8.85	636.435	6.37
5	16.18	0.495	37.41	14.32	1303.451	13.04
6	21.50	0.936	52.10	19.94	3492.276	34.93
7	24.43	0.597	45.23	17.31	1930.955	19.31
7	28.00	0.598	261.23	100.00	9998.637	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:21:14 PM
Printed by: wet


Ident: CCV
Analysis from: 9/16/2023 12:57:27 AM
File: _2023-09-16_

Last save: 9/18/2023 9:21:05 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35512

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

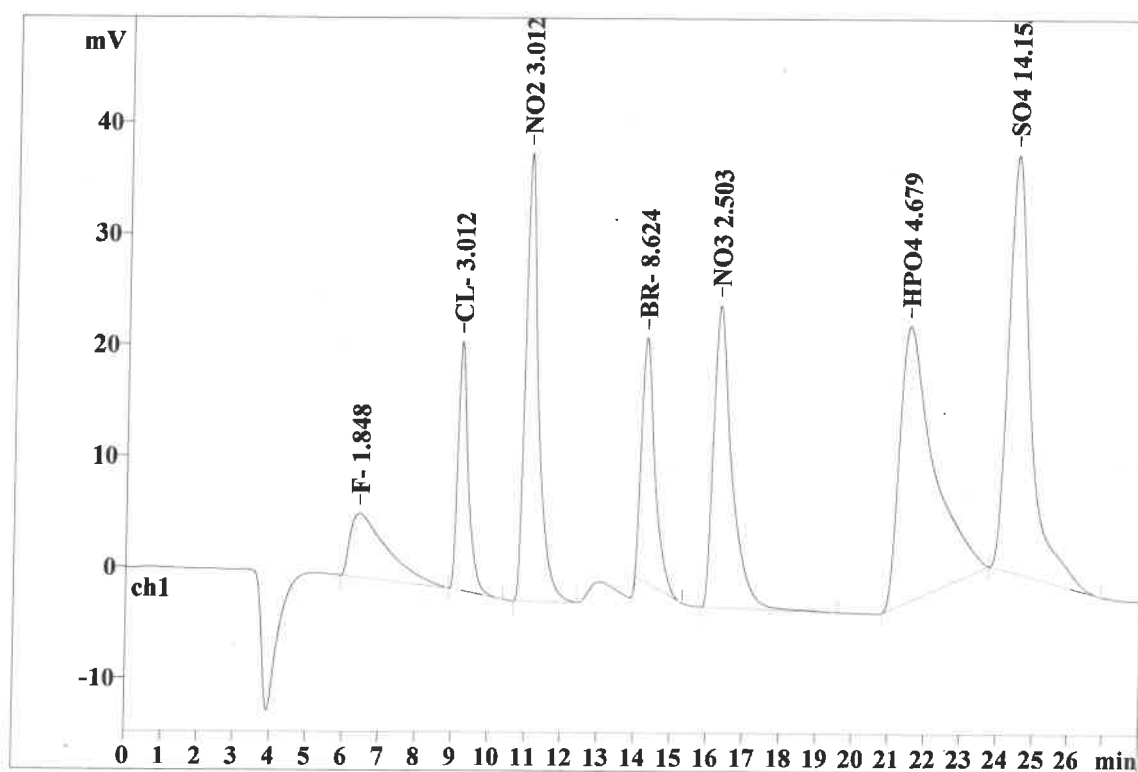

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.42	1.077	5.76	3.20	409.942	6.17
2	9.20	0.282	22.39	12.45	441.949	6.66
3	11.04	0.354	40.28	22.39	1009.847	15.21
4	14.26	0.380	21.93	12.19	563.787	8.49
5	16.27	0.495	27.13	15.08	952.951	14.35
6	21.50	0.901	24.83	13.80	1625.078	24.48
7	24.45	0.601	37.56	20.88	1635.945	24.64
7	28.00	0.584	179.87	100.00	6639.498	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:21:23 PM
Printed by: wet


Ident: CCB
Analysis from: 9/16/2023 1:58:43 AM
File: _2023-09-16_

Last save: 9/16/2023 2:26:43 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35514

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

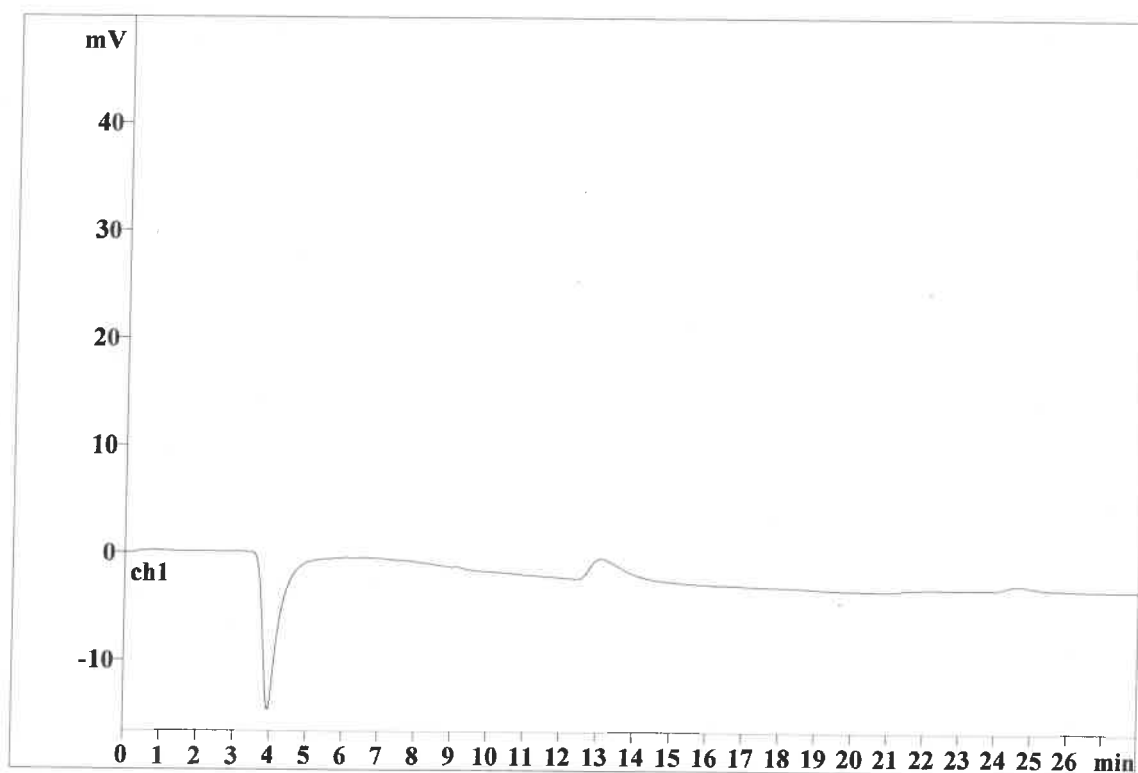

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:45:55 PM
Printed by: wet


Ident: CCV
Analysis from: 9/18/2023 10:07:16 AM
File: _2023-09-18_

Last save: 9/18/2023 10:35:16 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35517

Last save: 9/18/2023 9:36:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

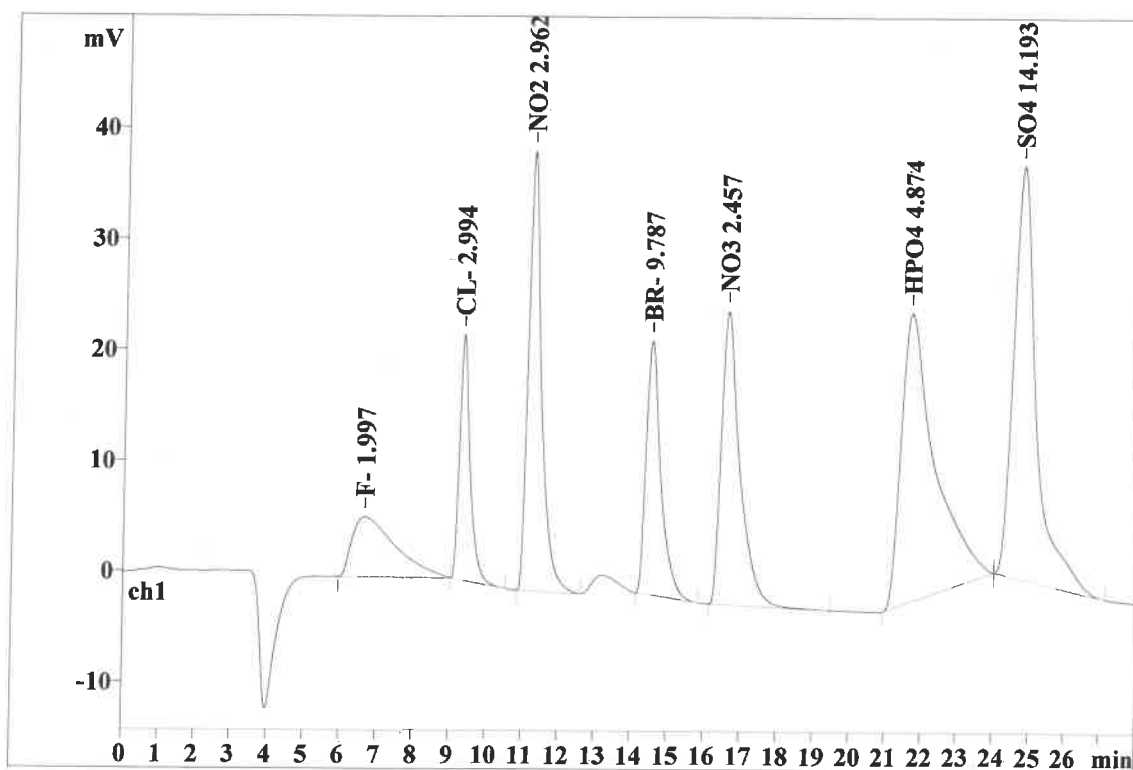

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.64	1.281	5.42	3.01	447.982	6.59
2	9.32	0.283	22.15	12.32	439.138	6.46
3	11.20	0.353	39.65	22.04	991.955	14.59
4	14.50	0.407	22.92	12.74	645.621	9.50
5	16.57	0.506	26.46	14.71	934.492	13.75
6	21.63	0.877	26.09	14.50	1697.498	24.97
7	24.70	0.601	37.19	20.67	1640.817	24.14
7	28.00	0.615	179.88	100.00	6797.504	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:46:03 PM
Printed by: wet


Ident: CCB
Analysis from: 9/18/2023 10:41:49 AM
File: _2023-09-18_

Last save: 9/18/2023 11:09:49 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35518

Last save: 9/18/2023 9:36:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

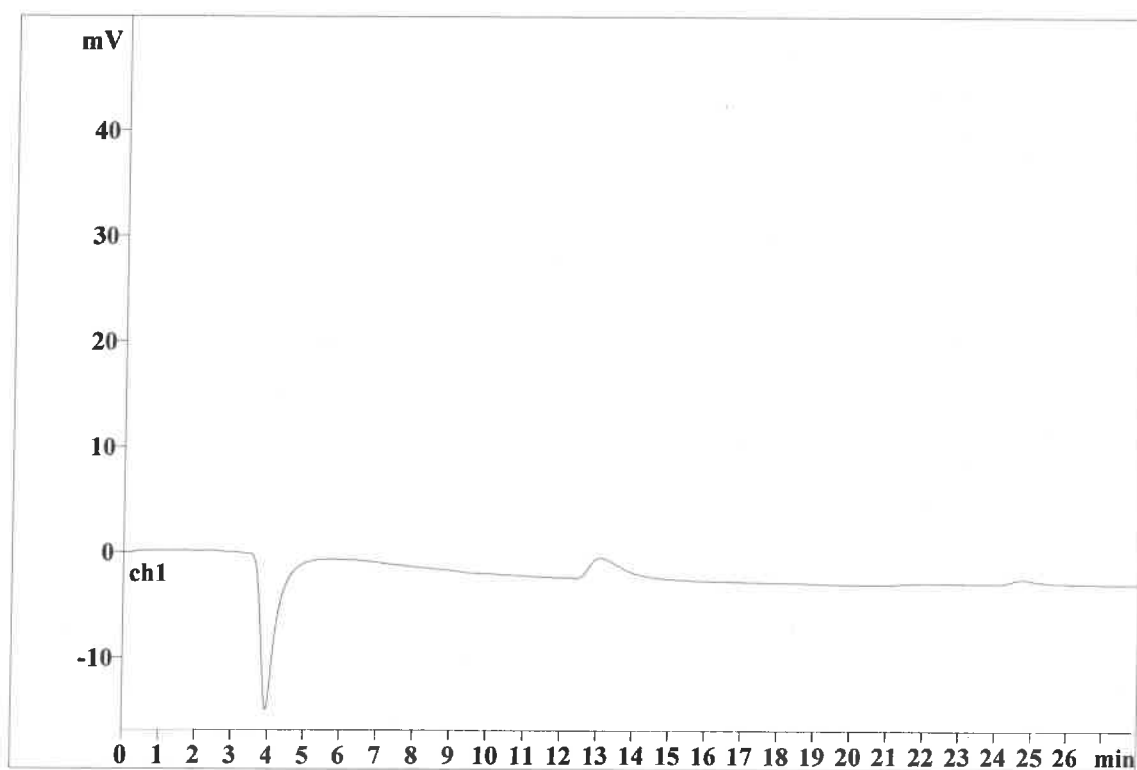

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:46:37 PM
Printed by: wet


Ident: LB127341BLW2
Analysis from: 9/18/2023 11:12:29 AM
File: _2023-09-18_

Last save: 9/18/2023 3:46:36 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35519

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

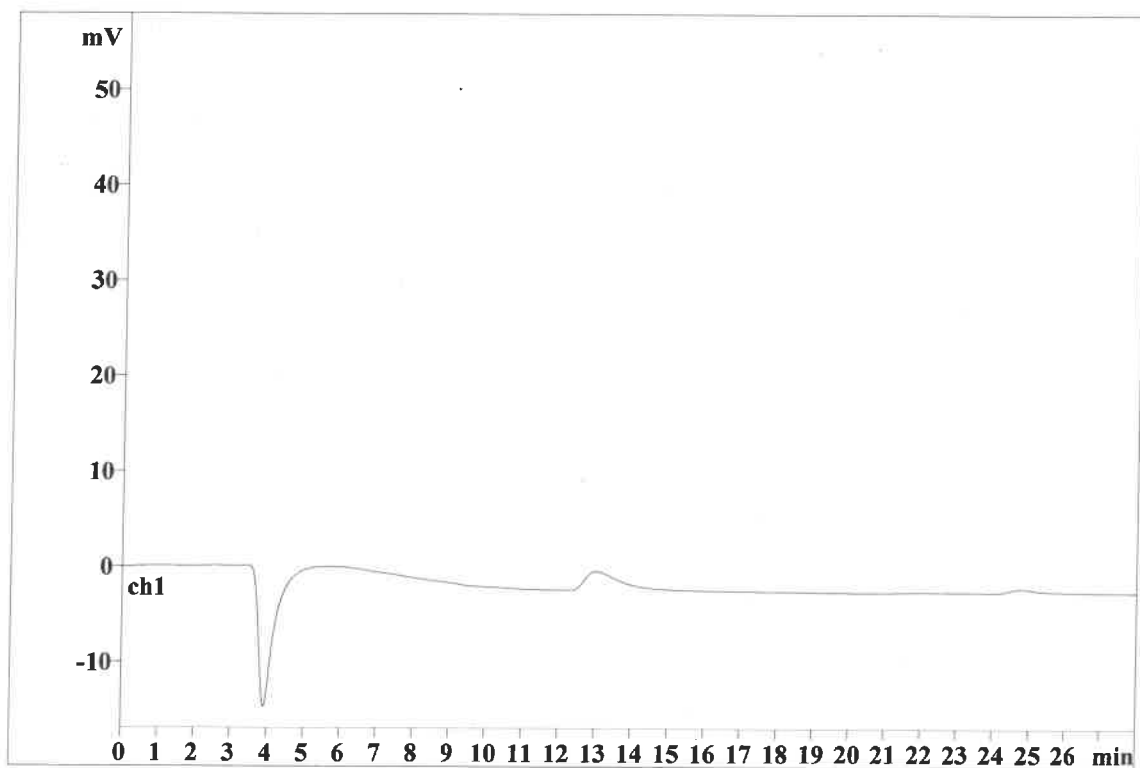

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:46:45 PM
Printed by: wet


Ident: LB127341BSW2
Analysis from: 9/18/2023 11:43:04 AM
File: _2023-09-18_

Last save: 9/18/2023 1:58:16 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35520

Last save: 9/14/2023 9:40:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

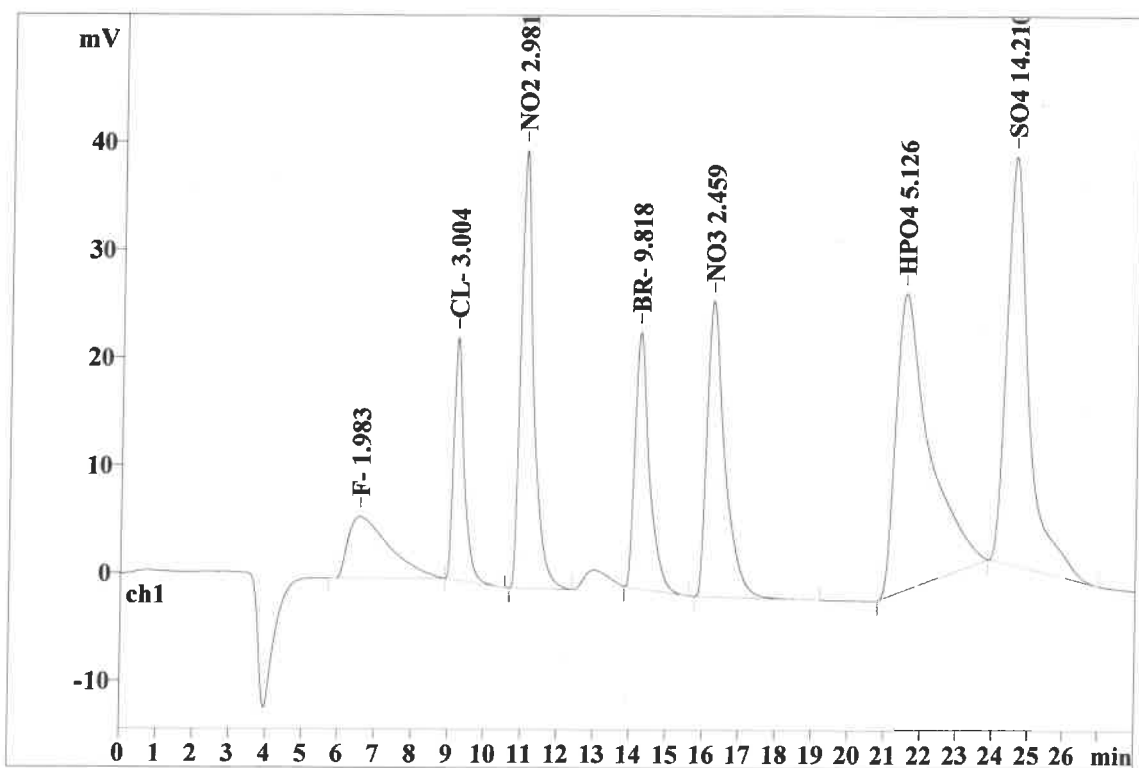

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.55	1.203	5.72	3.08	444.584	6.44
2	9.19	0.279	22.51	12.13	440.625	6.38
3	11.02	0.346	40.65	21.90	998.633	14.47
4	14.21	0.393	23.75	12.79	647.808	9.39
5	16.21	0.486	27.46	14.79	935.263	13.55
6	21.50	0.873	27.63	14.88	1791.288	25.96
7	24.55	0.591	37.90	20.42	1642.979	23.81
7	28.00	0.596	185.62	100.00	6901.181	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:46:54 PM
Printed by: wet


Ident: O4466-02DLX5
Analysis from: 9/18/2023 12:34:29 PM
File: _2023-09-18_

Last save: 9/18/2023 2:51:50 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35521

Last save: 9/18/2023 12:16

SAMPLE:
: IZ/MA
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

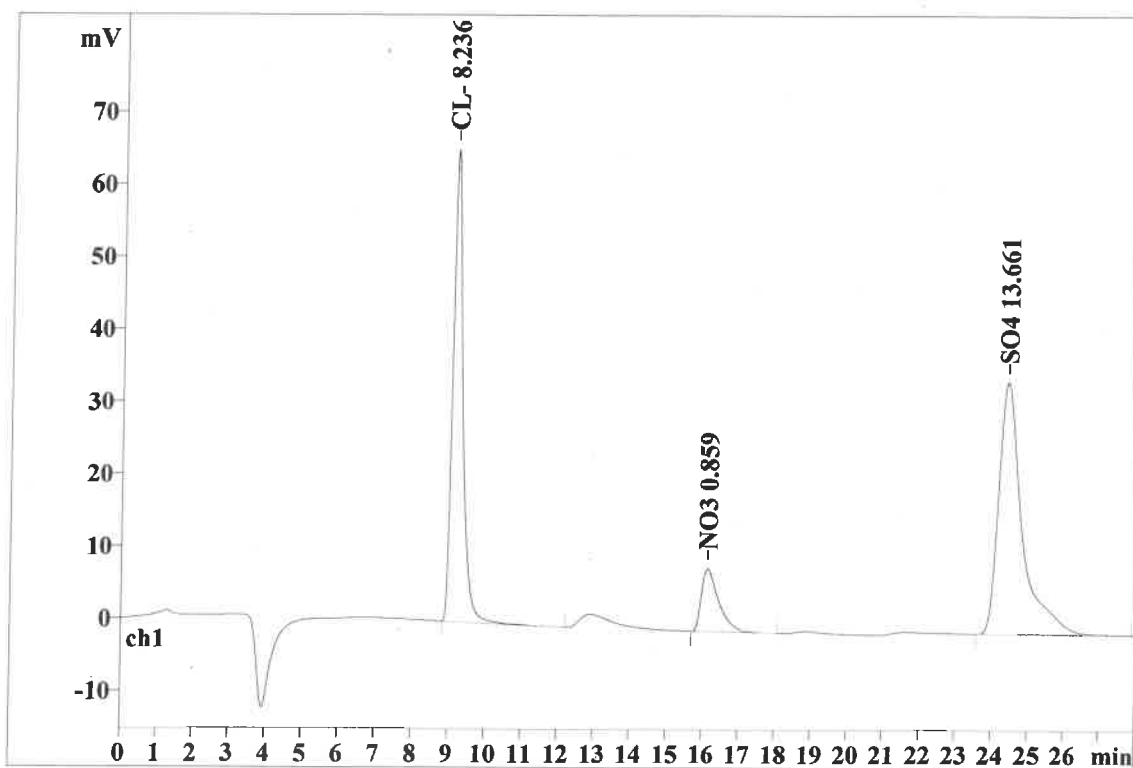

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.14	0.274	65.24	59.99	1255.296	40.23
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.13	0.490	8.68	7.98	290.077	9.30
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.40	0.604	34.84	32.03	1575.310	50.48
7	28.00	0.195	108.76	100.00	3120.683	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:47:01 PM
Printed by: wet


Ident: O4466-01DLX5
Analysis from: 9/18/2023 1:05:05 PM
File: _2023-09-18_

Last save: 9/18/2023 2:51:50 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35522

Last save: 9/18/2023 12:16

SAMPLE:
: IZ/MA
Vial number: 31
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

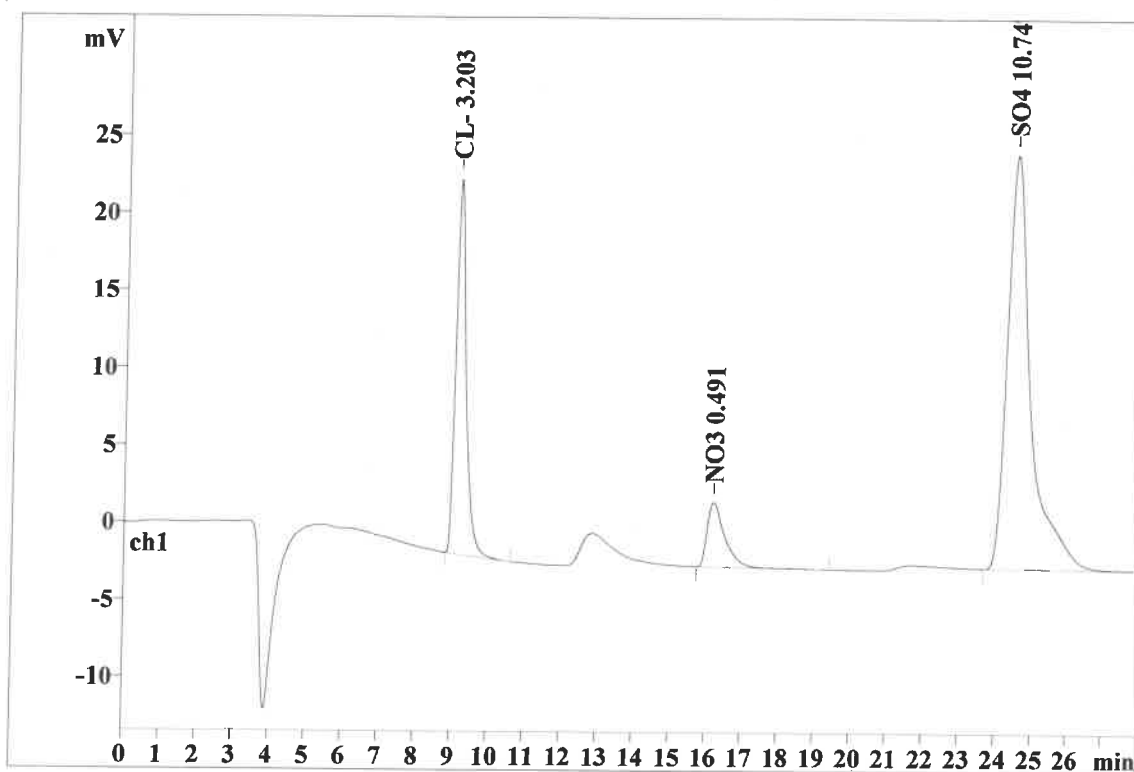

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.14	0.281	24.24	43.94	471.714	25.79
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.19	0.487	4.17	7.55	141.669	7.74
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.46	0.605	26.76	48.51	1215.928	66.47
7	28.00	0.196	55.16	100.00	1829.311	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:47:09 PM
Printed by: wet


Ident: CCV
Analysis from: 9/18/2023 1:35:48 PM
File: _2023-09-18_

Last save: 9/18/2023 2:03:48 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35523

Last save: 9/18/2023 12:16

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

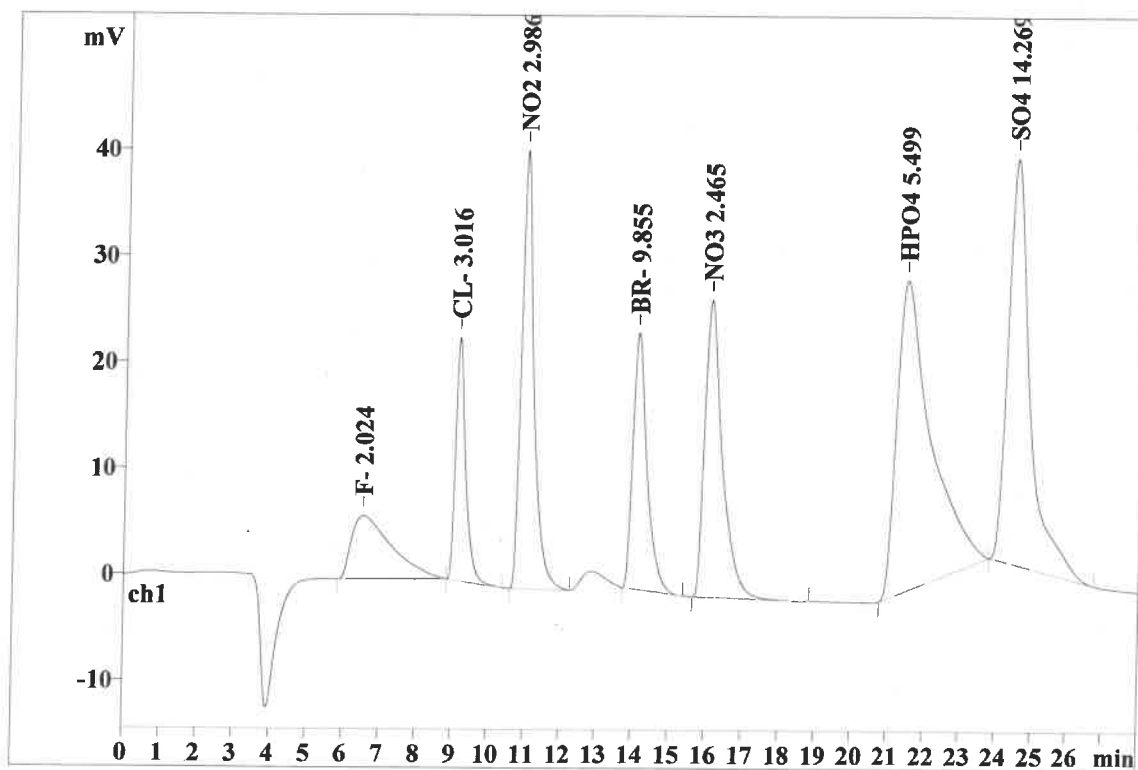

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.53	1.178	5.96	3.14	454.886	6.44
2	9.15	0.279	22.89	12.06	442.525	6.26
3	10.95	0.347	41.29	21.75	1000.668	14.16
4	14.10	0.391	24.16	12.72	650.401	9.20
5	16.08	0.483	28.02	14.76	937.692	13.27
6	21.46	0.899	29.34	15.45	1929.726	27.31
7	24.48	0.592	38.19	20.12	1650.197	23.35
7	28.00	0.596	189.86	100.00	7066.096	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/18/2023 3:47:18 PM
Printed by: wet


Ident: CCB
Analysis from: 9/18/2023 3:07:55 PM
File: _2023-09-18_

Last save: 9/18/2023 3:35:55 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35526

Last save: 9/18/2023 12:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

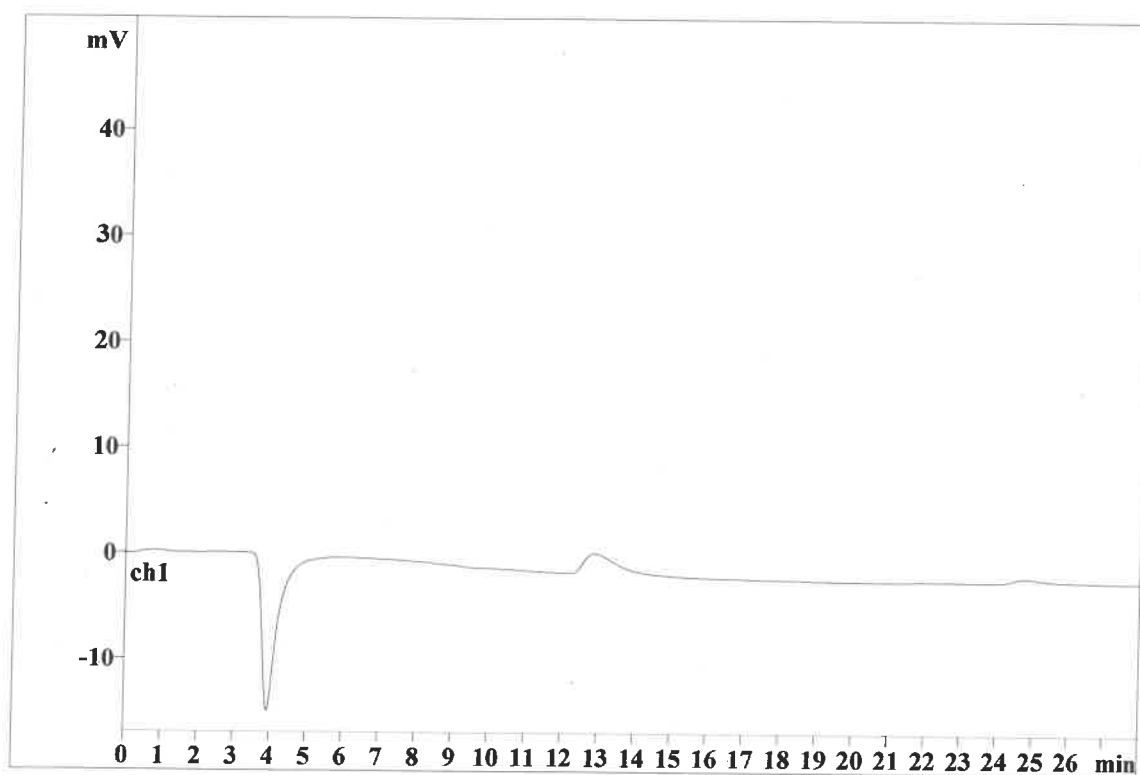

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD