


LB127359

7471B

INSTRUMENT ID: CV1

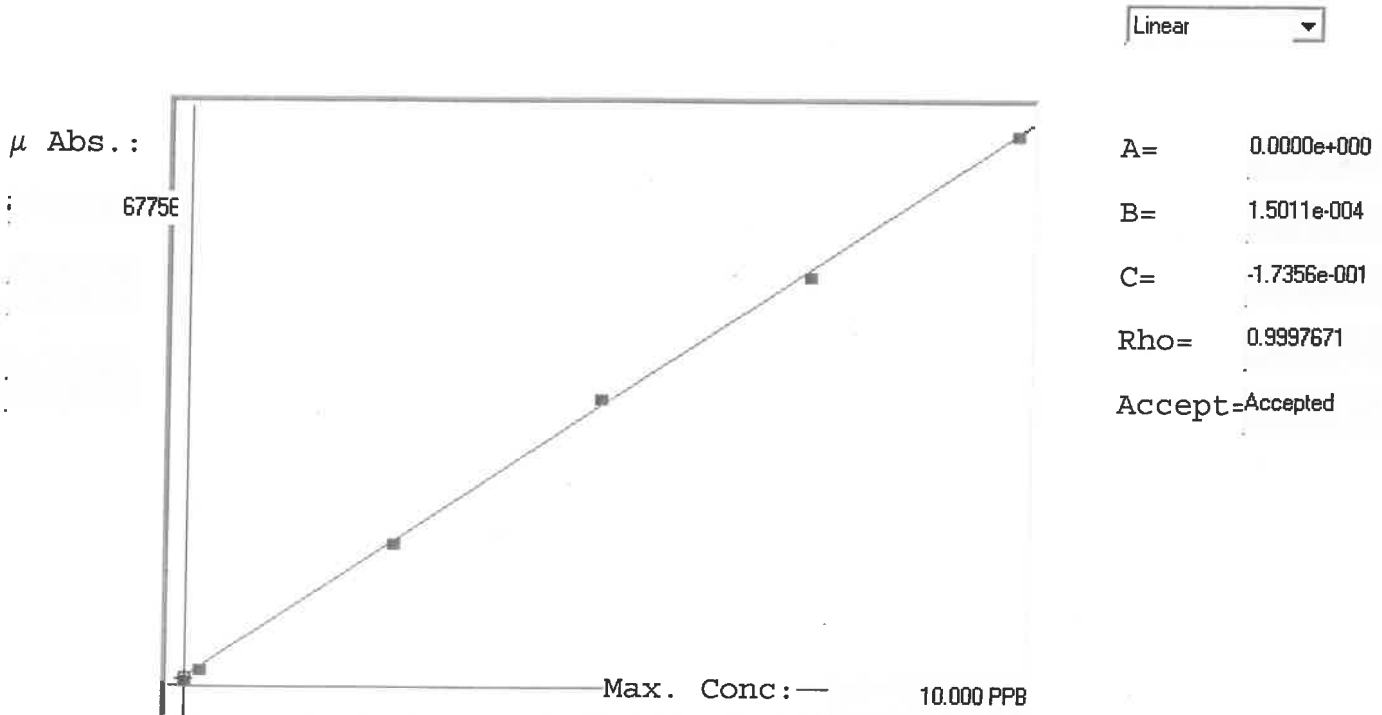

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.014	-0.014	1062	0.000	1062					
0.2	0.200	0.167	-0.033	2270	0.0 %	2270					
2.5	2.500	2.495	-0.005	17780	0.0 %	17780					
5.0	5.000	5.160	0.160	35531	0.0 %	35531					
7.5	7.500	7.394	-0.106	50416	0.0 %	50416					
10.0	10.000	9.997	-0.003	67756	0.0 %	67756					

0.0
1.5
0
3
0

LB127359 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 19 Sep 2023 13:06:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1062	-	0.0000	7471B	PPB	19 Sep 2023 13:09:38	S	Std
0.2 - 1	50.2	2270	-	0.2000	7471B	PPB	19 Sep 2023 13:11:55	S	Std
2.5 - 1	52.5	17780	-	2.5000	7471B	PPB	19 Sep 2023 13:14:12	S	Std
5.0 - 1	55	35531	-	5.0000	7471B	PPB	19 Sep 2023 13:16:28	S	Std
7.5 - 1	57.5	50416	-	7.5000	7471B	PPB	19 Sep 2023 13:18:45	S	Std
10.0 - 1	114	67756	-	10.0000	7471B	PPB	19 Sep 2023 13:24:26	S	Std
ICV70 - 1	ICV70	26716	3.8368	-	7471B	PPB	19 Sep 2023 13:27:12	U	SMPL
ICB70 - 1	ICB70	784	-0.0559	-	7471B	PPB	19 Sep 2023 13:29:27	U	SMPL
CCV19 - 1	CCV19	34990	5.0788	-	7471B	PPB	19 Sep 2023 13:31:42	U	SMPL
CCB19 - 1	CCB19	778	-0.0568	-	7471B	PPB	19 Sep 2023 13:33:57	U	SMPL
CRA - 1	CRA	2236	0.1621	-	7471B	PPB	19 Sep 2023 13:36:13	U	SMPL
HighStd - 1	HighStd	68560	10.1179	-	7471B	PPB	19 Sep 2023 13:38:28	U	SMPL
ChkStd - 1	ChkStd	47799	7.0015	-	7471B	PPB	19 Sep 2023 13:40:43	U	SMPL
PB155657BL - 1	PBS	1023	-0.0200	-	7471B	PPB	19 Sep 2023 13:45:33	U	SMPL
PB155657BS - 1	LCSS	24870	3.5597	-	7471B	PPB	19 Sep 2023 13:47:48	U	SMPL
O4451-01 - 1	WC-1	3831	0.4015	-	7471B	PPB	19 Sep 2023 13:50:04	U	SMPL
O4451-01DUP - 1	WC-1DUP	4077	0.4384	-	7471B	PPB	19 Sep 2023 13:52:20	U	SMPL
O4451-01MS - 1	WC-1MS	29684	4.2823	-	7471B	PPB	19 Sep 2023 13:54:37	U	SMPL
O4451-01MSD - 1	WC-1MSD	31859	4.6088	-	7471B	PPB	19 Sep 2023 13:56:54	U	SMPL
O4453-02 - 1	CPT102-13	4801	0.5471	-	7471B	PPB	19 Sep 2023 13:59:10	U	SMPL
CCV20 - 1	CCV20	35383	5.1378	-	7471B	PPB	19 Sep 2023 14:01:26	U	SMPL
CCB20 - 1	CCB20	780	-0.0565	-	7471B	PPB	19 Sep 2023 14:03:41	U	SMPL
O4453-04 - 1	CPT102-12	1516	0.0540	-	7471B	PPB	19 Sep 2023 14:05:56	U	SMPL
O4453-06 - 1	B102-07	1601	0.0668	-	7471B	PPB	19 Sep 2023 14:08:11	U	SMPL
O4453-08 - 1	CPT102-14	2071	0.1373	-	7471B	PPB	19 Sep 2023 14:10:27	U	SMPL
O4453-10 - 1	B102-02	2934	0.2669	-	7471B	PPB	19 Sep 2023 14:12:42	U	SMPL
O4460-01 - 1	DEL-2-RIGHT-SIDE	3230	0.3113	-	7471B	PPB	19 Sep 2023 14:14:58	U	SMPL
O4460-04 - 1	DEL-1-LEFT-SIDE	3630	0.3713	-	7471B	PPB	19 Sep 2023 14:17:14	U	SMPL
O4479-05 - 1	1029	1257	0.0151	-	7471B	PPB	19 Sep 2023 14:19:31	U	SMPL
O4479-06 - 1	1028	4509	0.5033	-	7471B	PPB	19 Sep 2023 14:21:48	U	SMPL
O4491-02 - 1	B102-05	844	-0.0469	-	7471B	PPB	19 Sep 2023 14:24:05	U	SMPL
O4491-04 - 1	B102-04	3071	0.2874	-	7471B	PPB	19 Sep 2023 14:26:20	U	SMPL
CCV21 - 1	CCV21	35530	5.1598	-	7471B	PPB	19 Sep 2023 14:28:35	U	SMPL
CCB21 - 1	CCB21	809	-0.0521	-	7471B	PPB	19 Sep 2023 14:30:51	U	SMPL
O4491-06 - 1	CPT102-07	3628	0.3710	-	7471B	PPB	19 Sep 2023 14:33:07	U	SMPL
O4491-08 - 1	B102-03	13468	1.8481	-	7471B	PPB	19 Sep 2023 14:35:22	U	SMPL
O4493-01 - 1	WC-1	6903	0.8626	-	7471B	PPB	19 Sep 2023 14:37:37	U	SMPL
O4451-01A - 1		30548	4.4120	-	7471B	PPB	19 Sep 2023 14:42:08	U	SMPL
O4451-01LX5 - 1		1249	0.0139	-	7471B	PPB	19 Sep 2023 14:54:21	U	SMPL
CCV22 - 1	CCV22	33406	4.8410	-	7471B	PPB	19 Sep 2023 14:56:55	U	SMPL
CCB22 - 1	CCB22	938	-0.0328	-	7471B	PPB	19 Sep 2023 14:59:11	U	SMPL