

Clear table

Instrument ID: IC-2											
Analyst : IZ											
Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 11:34		IZ/MA
STD2	0.4370	0.6640	0.6720	2.2480	0.5650	0.9910	3.5010	2023-09-13_	9/13/23 12:04		IZ/MA
STD3	0.8560	1.1860	1.1800	3.9540	0.9900	1.9910	5.9710	2023-09-13_	9/13/23 12:35		IZ/MA
STD4	0.9990	1.5150	1.5110	5.0350	1.2610	2.6440	7.5340	2023-09-13_	9/13/23 13:17		IZ/MA
STD5	1.8950	2.9390	2.9450	9.7600	2.4350	4.8490	14.4550	2023-09-13_	9/13/23 13:48		IZ/MA
STD6	3.9370	5.9070	5.8970	19.6950	4.9130	9.9780	29.4710	2023-09-13_	9/13/23 14:19		IZ/MA
STD7	5.0750	7.5900	7.5960	25.3080	6.3360	12.5480	38.0680	2023-09-13_	9/13/23 14:49		IZ/MA
ICV	1.9120	2.8680	2.8940	9.5640	2.4030	5.0020	14.1400	2023-09-13_	9/13/23 15:20		IZ/MA
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 15:52		IZ/MA
CCV	2.0160	3.2050	3.1670	10.4150	2.6170	4.6670	14.9140	2023-09-13_	9/13/23 11:35		IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-19_	9/19/23 12:06		IZ/MA
LB127409BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-19_	9/19/23 12:37		IZ/MA
LB127409BSW	2.0610	3.1750	3.1110	10.3130	2.5840	4.7880	14.7240	2023-09-19_	9/19/23 13:07		IZ/MA
O4500-01	0.0000	0.0000	0.0000	0.0000	0.2340	0.0000	0.0000	2023-09-19_	9/19/23 13:52		IZ/MA
O4500-01MS	1.8900	2.8730	2.8720	9.3230	2.4610	4.5110	13.4940	2023-09-19_	9/19/23 14:23		IZ/MA
O4500-01MSD	1.9570	2.9640	2.9750	9.6250	2.5390	4.6550	13.9070	2023-09-19_	9/19/23 14:54		IZ/MA
O4474-04	0.8990	350.6060	0.0000	0.0000	0.0000	0.0000	5.3410	2023-09-19_	9/19/23 15:24		IZ/MA
CCV	2.0420	3.1170	3.1080	10.1550	2.5580	4.9740	14.5310	2023-09-19_	9/19/23 16:28		IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-19_	9/19/23 16:58		IZ/MA

Report date: 9/21/2023 1:54:05 PM
Printed by: wet


Ident: CCV
Analysis from: 9/19/2023 11:35:18 AM
File: _2023-09-19_

Last save: 9/19/2023 12:03:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35540

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

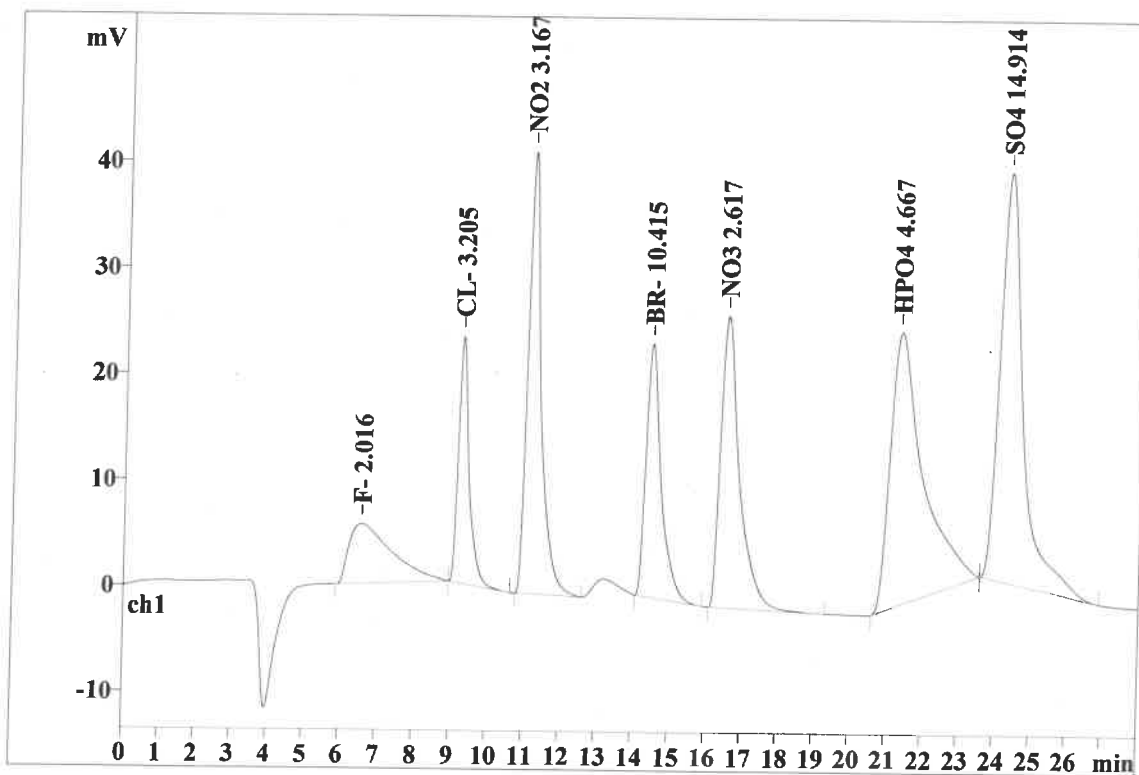

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.56	1.247	5.64	3.03	452.891	6.44
2	9.25	0.284	23.26	12.48	471.948	6.71
3	11.13	0.353	41.70	22.37	1064.768	15.15
4	14.44	0.412	23.90	12.82	689.755	9.81
5	16.51	0.511	27.48	14.74	998.851	14.21
6	21.32	0.849	25.80	13.84	1620.508	23.06
7	24.29	0.622	38.62	20.72	1729.719	24.61
7	28.00	0.611	186.39	99.99	7028.439	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:54:13 PM
Printed by: wet


Ident: CCB
Analysis from: 9/19/2023 12:06:25 PM
File: _2023-09-19_

Last save: 9/19/2023 12:34:25 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35541

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

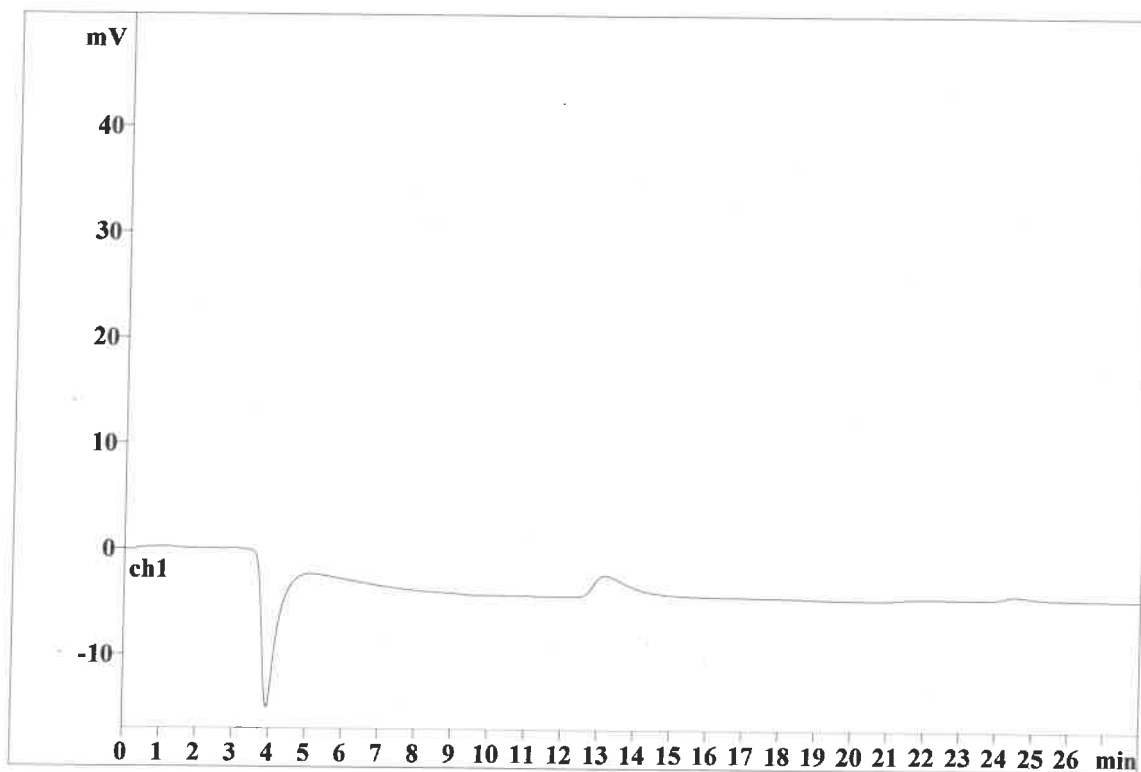

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:54:28 PM
Printed by: wet


Ident: LB127409BLW
Analysis from: 9/19/2023 12:37:01 PM
File: _2023-09-19_

Last save: 9/21/2023 1:54:25 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35542

Last save: 9/18/2023 4:37:

SAMPLE:
:
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

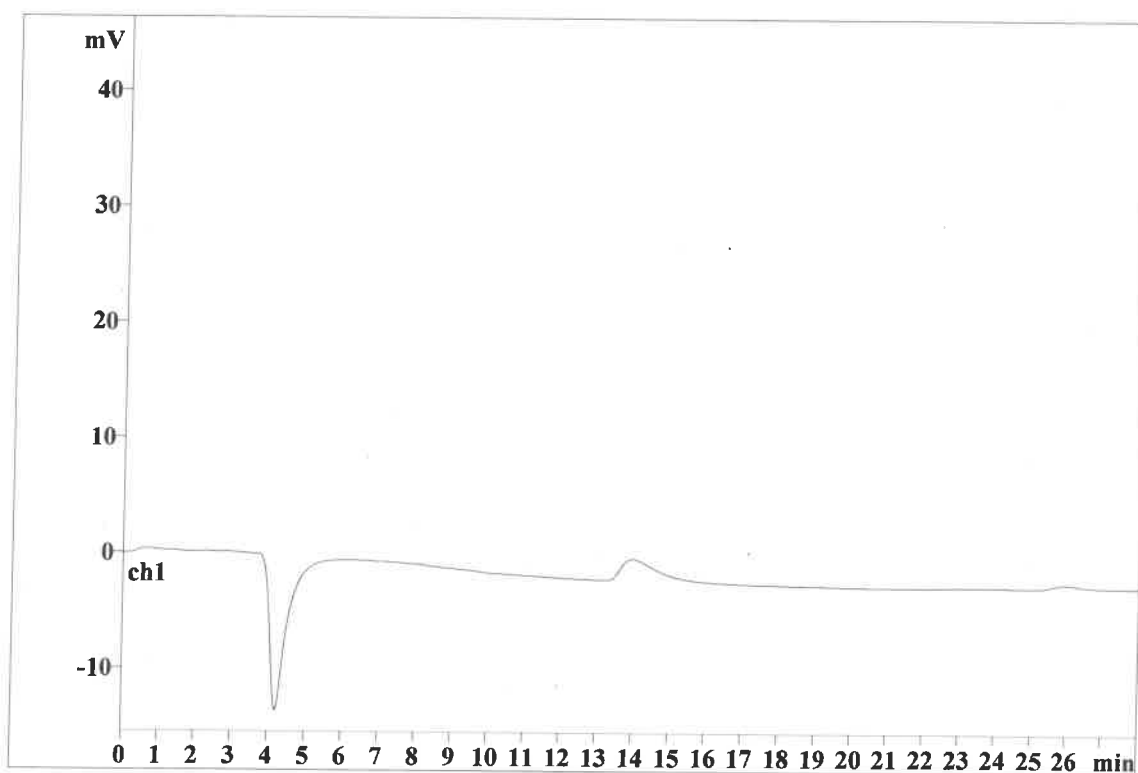

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:54:36 PM
Printed by: wet


Ident: LB127409BSW
Analysis from: 9/19/2023 1:07:36 PM
File: _2023-09-19_

Last save: 9/21/2023 1:53:50 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35543

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

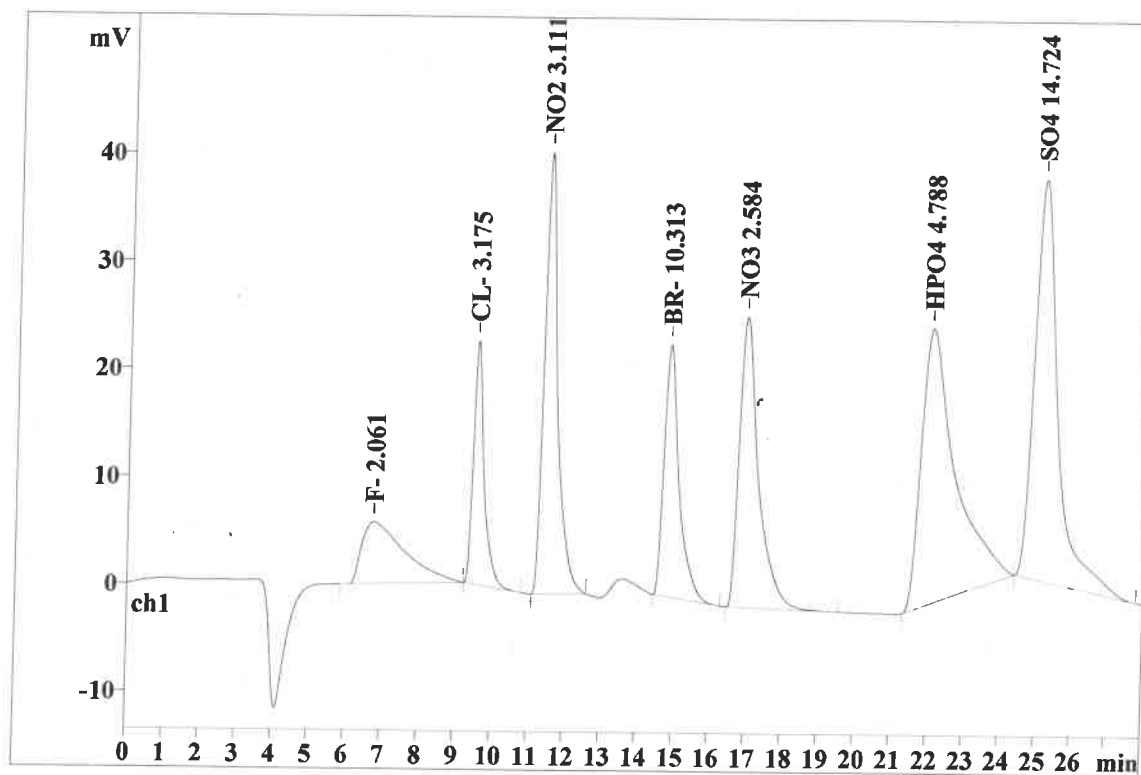

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.76	1.248	5.72	3.13	464.276	6.62
2	9.54	0.289	22.68	12.42	467.308	6.66
3	11.46	0.357	40.99	22.45	1044.923	14.89
4	14.83	0.416	23.39	12.81	682.631	9.73
5	16.94	0.514	26.97	14.77	985.735	14.05
6	22.05	0.878	25.60	14.02	1665.694	23.74
7	25.11	0.637	37.21	20.38	1706.397	24.32
7	28.00	0.620	182.56	100.00	7016.964	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:55:14 PM
Printed by: wet


Ident: 04500-01
Analysis from: 9/19/2023 1:52:51 PM
File: _2023-09-19_

Last save: 9/21/2023 1:55:11 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35544

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

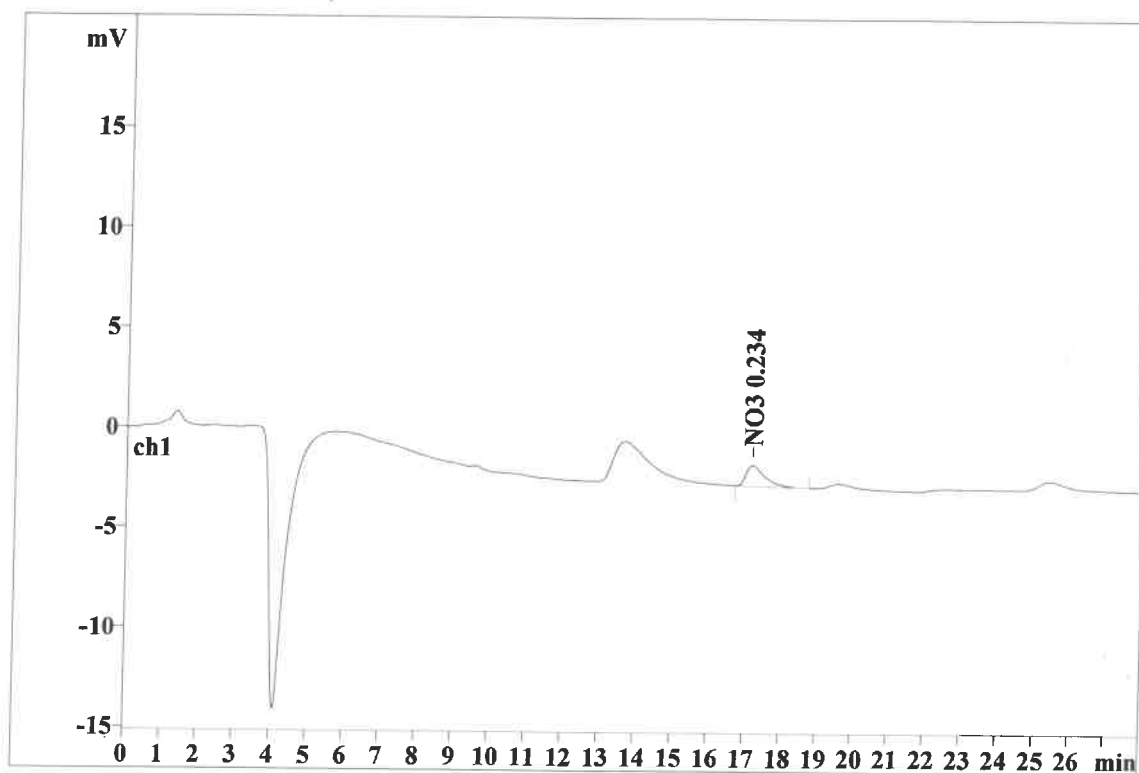

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.18	0.527	1.04	99.87	38.007	100.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.075	1.04	99.87	38.007	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:55:20 PM
Printed by: wet


Ident: O4500-01MS
Analysis from: 9/19/2023 2:23:26 PM
File: _2023-09-19_

Last save: 9/19/2023 2:51:26 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35545

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

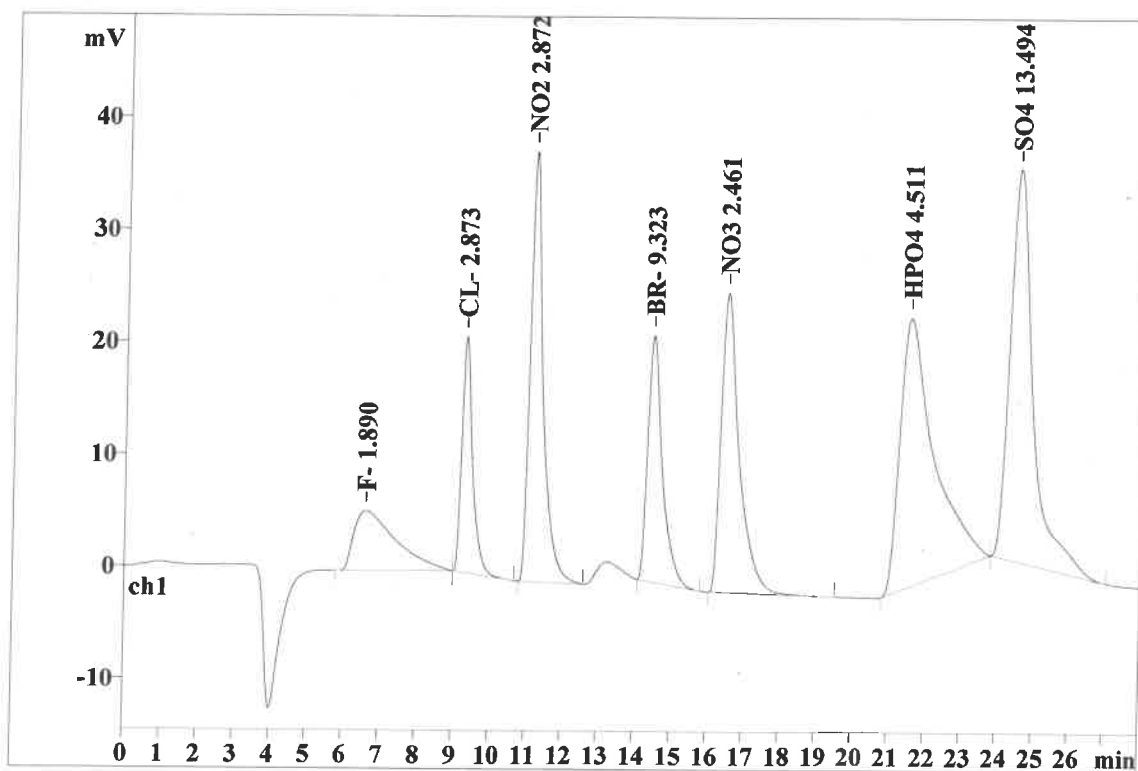

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.60	1.212	5.30	3.08	420.693	6.50
2	9.30	0.283	21.05	12.23	420.294	6.50
3	11.16	0.350	38.30	22.24	960.099	14.85
4	14.46	0.401	21.96	12.75	612.981	9.48
5	16.49	0.497	26.67	15.49	935.869	14.47
6	21.54	0.884	23.98	13.93	1562.575	24.16
7	24.53	0.614	34.94	20.29	1554.725	24.04
7	28.00	0.606	172.20	100.00	6467.236	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:55:27 PM
Printed by: wet


Ident: O4500-01MSD
Analysis from: 9/19/2023 2:54:01 PM
File: _2023-09-19_

Last save: 9/19/2023 3:22:01 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35546

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

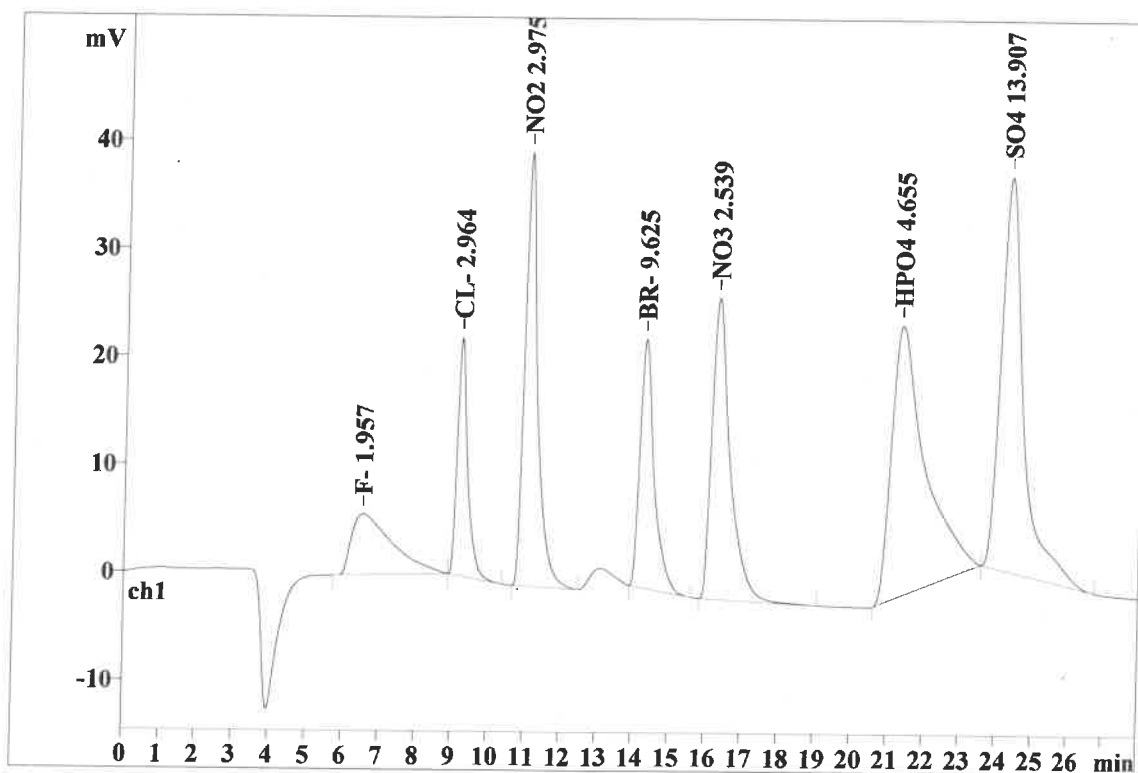

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.52	1.193	5.63	3.12	437.877	6.54
2	9.18	0.280	22.03	12.21	434.431	6.49
3	11.02	0.346	40.14	22.26	996.419	14.89
4	14.27	0.396	23.04	12.77	634.165	9.48
5	16.27	0.490	27.91	15.47	967.331	14.45
6	21.31	0.872	25.13	13.93	1616.362	24.15
7	24.27	0.608	36.48	20.23	1605.553	23.99
7	28.00	0.598	180.36	100.00	6692.138	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:55:39 PM
Printed by: wet


Ident: 04474-04
Analysis from: 9/19/2023 3:24:41 PM
File: _2023-09-19_

Last save: 9/19/2023 3:52:42 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35547

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

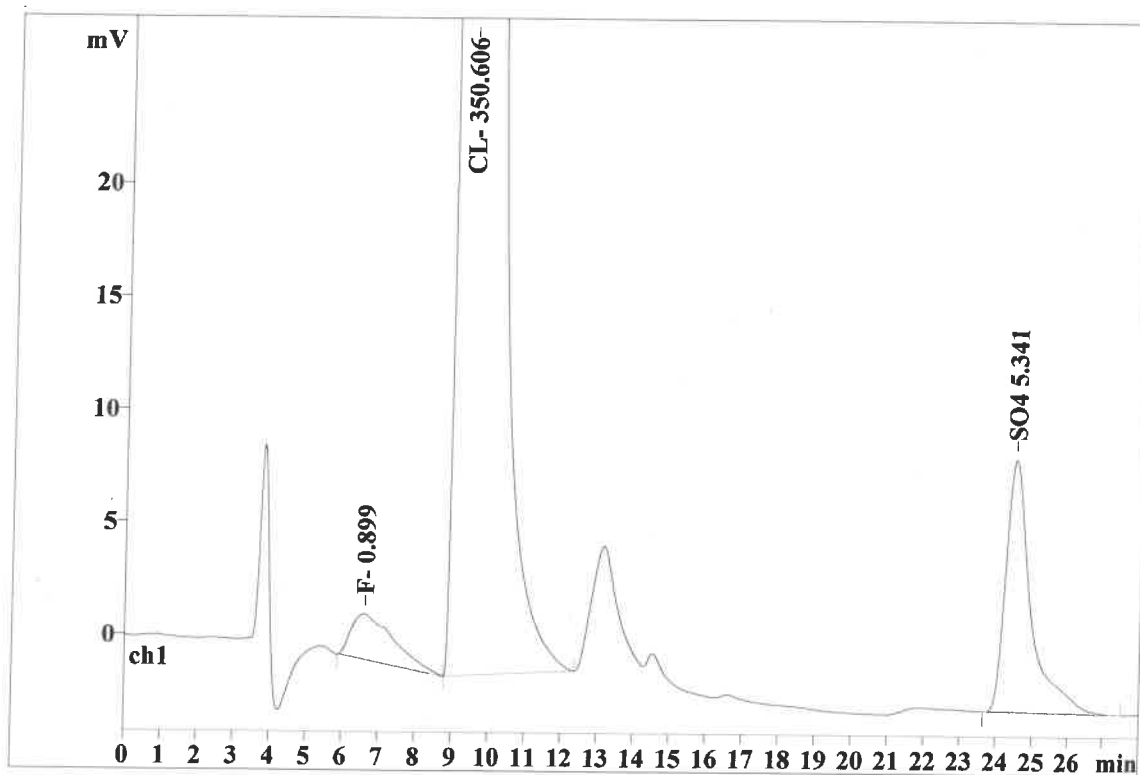

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.61	1.325	2.03	0.13	168.408	0.30
2	9.43	0.549	1560.78	99.16	54559.060	98.70
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	24.48	0.650	11.19	0.71	549.429	0.99
7	28.00	0.361	1574.00	100.00	55276.896	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:55:54 PM
Printed by: wet


Ident: CCV
Analysis from: 9/19/2023 4:28:06 PM
File: _2023-09-19_

Last save: 9/19/2023 4:56:06 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35549

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

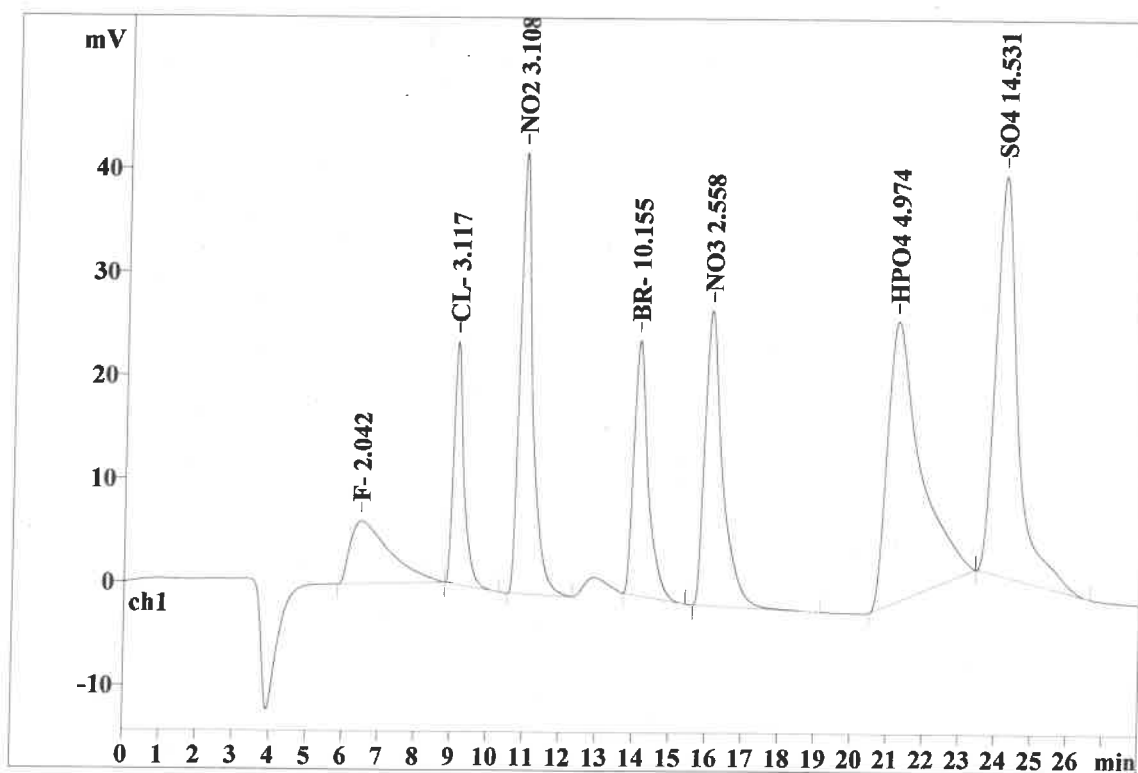

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.46	1.164	6.05	3.16	459.511	6.54
2	9.10	0.276	23.47	12.27	458.200	6.52
3	10.91	0.341	42.65	22.30	1043.927	14.86
4	14.08	0.390	24.67	12.90	671.475	9.56
5	16.04	0.480	28.55	14.93	975.211	13.88
6	21.19	0.866	27.19	14.22	1734.909	24.69
7	24.12	0.603	38.64	20.21	1682.544	23.95
7	28.00	0.589	191.21	100.00	7025.777	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/21/2023 1:56:13 PM
Printed by: wet


Ident: CCB
Analysis from: 9/19/2023 4:58:46 PM
File: _2023-09-19_

Last save: 9/21/2023 1:56:11 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35550

Last save: 9/18/2023 4:37:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

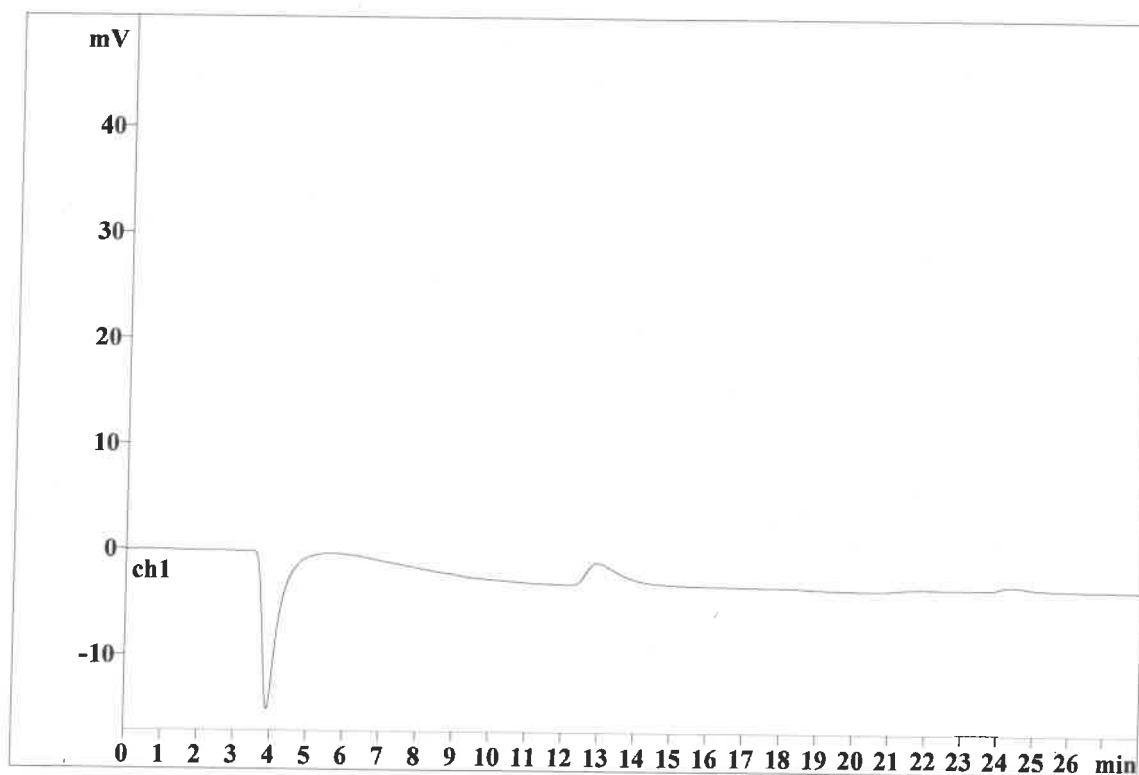

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD