


LB127441

SFAM01.1

INSTRUMENT ID: CV1

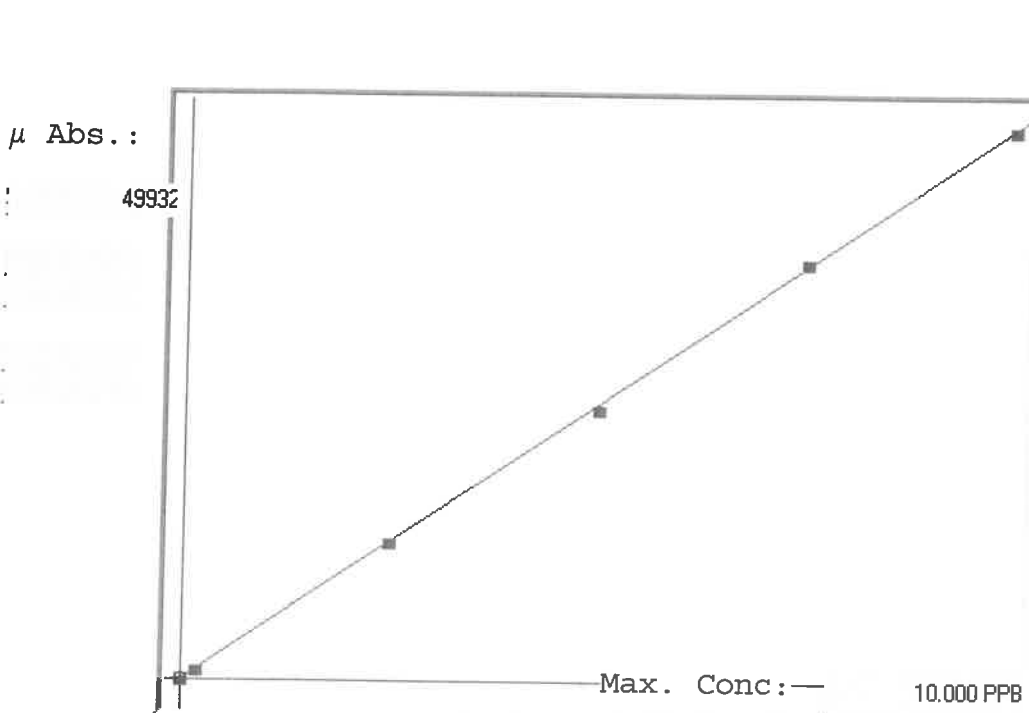

Linear

A= 0.0000e+000

B= 1.9975e-004 slope

C= -3.5440e-003 y-intercept

Rho= 0.9999208

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.012	0.012	80	0.000	80					0.0
0.05	0.050					372	0				1
0.20	0.200	0.201	0.001	1024	0.0 %	1024					0
2.50	2.500	2.503	0.003	12547	0.0 %	12547					0
5.00	5.000	4.930	-0.070	24698	0.0 %	24698					1
7.50	7.500	7.584	0.084	37983	0.0 %	37983					1
10.0	10.000	9.970	-0.030	49932	0.0 %	49932					0

LB127441

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	80	-		0 SFAM01.1	PPB	9/22/2023 15:30	Std
	0.2 S01	1024	-		0.2 SFAM01.1	PPB	9/22/2023 15:32	Std
	2.5 S02	12547	-		2.5 SFAM01.1	PPB	9/22/2023 15:37	Std
	5 S03	24698	-		5 SFAM01.1	PPB	9/22/2023 15:39	Std
	7.5 S04	37983	-		7.5 SFAM01.1	PPB	9/22/2023 15:42	Std
	10 S05	49932	-		10 SFAM01.1	PPB	9/22/2023 15:44	Std
ICV077	ICV077	21479	4.2869 -		SFAM01.1	PPB	9/22/2023 15:47	SMPL
ICB077	ICB077	6	-0.0023 -		SFAM01.1	PPB	9/22/2023 15:49	SMPL
CCV046	CCV046	24950	4.9802 -		SFAM01.1	PPB	9/22/2023 15:51	SMPL
CCB046	CCB046	11	-0.0013 -		SFAM01.1	PPB	9/22/2023 15:54	SMPL
PB155767BL	PBW767	43	0.005 -		SFAM01.1	PPB	9/22/2023 15:56	SMPL
O4418-07	MEZYP5	119	0.0202 -		SFAM01.1	PPB	9/22/2023 15:58	SMPL
PB155768BL	PBW768	53	0.007 -		SFAM01.1	PPB	9/22/2023 16:00	SMPL
O4443-15	MJKW39	101	0.0166 -		SFAM01.1	PPB	9/22/2023 16:03	SMPL
PB155769BL	PBW769	54	0.0072 -		SFAM01.1	PPB	9/22/2023 16:05	SMPL
O4355-07	X1246	45528	9.0907 -		SFAM01.1	PPB	9/22/2023 16:09	SMPL
CCV047	CCV047	25342	5.0585 -		SFAM01.1	PPB	9/22/2023 16:16	SMPL
CCB047	CCB047	-15	-0.0065 -		SFAM01.1	PPB	9/22/2023 16:19	SMPL