


LB127563

7470A

INSTRUMENT ID: CY1

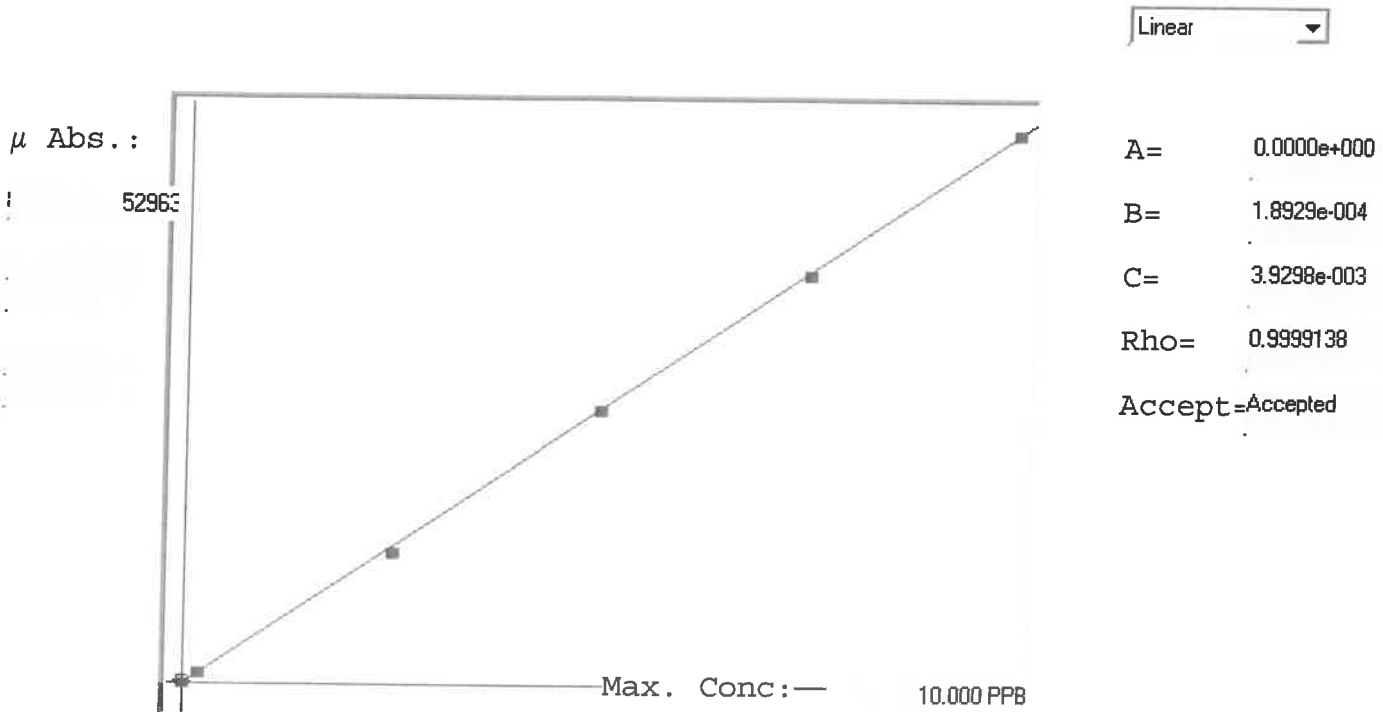

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.059	0.059	291	0.000	291					
0.2	0.200	0.216	0.016	1119	0.0 %	1119					
2.5	2.500	2.404	-0.096	12677	0.0 %	12677					
5.0	5.000	5.005	0.005	26419	0.0 %	26419					
7.5	7.500	7.487	-0.013	39533	0.0 %	39533					
10.0	10.000	10.029	0.029	52963	0.0 %	52963					

0.000
1.8
-4
0
0
0
0

LB127563 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Oct 2023 11:18:09

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50	291	-	0.0000	7470A	PPB	02 Oct 2023 11:20:42	S	Std
0.2 - 1	50.2	1119	-	0.2000	7470A	PPB	02 Oct 2023 11:22:59	S	Std
2.5 - 1	52.5	12677	-	2.5000	7470A	PPB	02 Oct 2023 11:25:16	S	Std
5.0 - 1	55	26419	-	5.0000	7470A	PPB	02 Oct 2023 11:27:33	S	Std
7.5 - 1	59.5	39533	-	7.5000	7470A	PPB	02 Oct 2023 11:29:49	S	Std
10.0 - 1	516	52963	-	10.0000	7470A	PPB	02 Oct 2023 11:32:04	S	Std
ICV89 - 1	ICV89	19570	3.7084	-	7470A	PPB	02 Oct 2023 11:35:03	U	SMPL
ICB89 - 1	ICB89	122	0.0270	-	7470A	PPB	02 Oct 2023 11:37:17	U	SMPL
CCV94 - 1	CCV94	26191	4.9617	-	7470A	PPB	02 Oct 2023 11:39:33	U	SMPL
CCB94 - 1	CCB94	126	0.0278	-	7470A	PPB	02 Oct 2023 11:41:48	U	SMPL
CRA - 1	CRA	1096	0.2114	-	7470A	PPB	02 Oct 2023 11:44:02	U	SMPL
HighStd - 1	HighStd	52904	10.0183	-	7470A	PPB	02 Oct 2023 11:46:17	U	SMPL
ChkStd - 1	ChkStd	35801	6.7808	-	7470A	PPB	02 Oct 2023 11:48:33	U	SMPL
PB156024BL - 1	PBW	89	0.0208	-	7470A	PPB	02 Oct 2023 11:50:50	U	SMPL
PB156024BS - 1	LCSW	19054	3.6107	-	7470A	PPB	02 Oct 2023 11:53:05	U	SMPL
O4622-03 - 1	FB-1	79	0.0189	-	7470A	PPB	02 Oct 2023 11:55:21	U	SMPL
O4661-02 - 1	TT-054-IDWGW-20230927	102	0.0232	-	7470A	PPB	02 Oct 2023 11:57:38	U	SMPL
O4661-03 - 1	TT-055-IDWGW-20230927	337	0.0677	-	7470A	PPB	02 Oct 2023 11:59:54	U	SMPL
O4661-04 - 1	TT-056-IDWGW-20230927	123	0.0272	-	7470A	PPB	02 Oct 2023 12:02:11	U	SMPL
O4661-05 - 1	TT-057-IDWGW-20230927	108	0.0244	-	7470A	PPB	02 Oct 2023 12:04:26	U	SMPL
CCV95 - 1	CCV95	25902	4.9070	-	7470A	PPB	02 Oct 2023 12:06:42	U	SMPL
CCB95 - 1	CCB95	109	0.0246	-	7470A	PPB	02 Oct 2023 12:08:57	U	SMPL
O4667-01 - 1	FRAC-TANK-A2970	679	0.1325	-	7470A	PPB	02 Oct 2023 12:11:12	U	SMPL
O4667-01DUP - 1	FRAC-TANK-A2970DUP	668	0.1304	-	7470A	PPB	02 Oct 2023 12:13:27	U	SMPL
O4667-01MS - 1	FRAC-TANK-A2970MS	18395	3.4860	-	7470A	PPB	02 Oct 2023 12:15:43	U	SMPL
O4667-01MSD - 1	FRAC-TANK-A2970MSD	17167	3.2535	-	7470A	PPB	02 Oct 2023 12:17:58	U	SMPL
O4667-01LX5 - 1		88	0.0206	-	7470A	PPB	02 Oct 2023 12:20:15	U	SMPL
O4667-01A - 1		19469	3.6893	-	7470A	PPB	02 Oct 2023 12:30:57	U	SMPL
CCV96 - 1	CCV96	25912	4.9089	-	7470A	PPB	02 Oct 2023 12:33:13	U	SMPL
CCB96 - 1	CCB96	121	0.0268	-	7470A	PPB	02 Oct 2023 12:35:30	U	SMPL