

16127587

Result archive

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

10/3/2023 10:12

Sample id	Test id	Result	Status	Date	Errors
ICV1	Total CN	92.925	man acc	10/2/2023	
ICB1	Total CN	-0.686	man acc	10/2/2023	
CCV1	Total CN	245.820	man acc	10/2/2023	
CCB1	Total CN	-0.588	man acc	10/2/2023	
PB156066BL	Total CN	-0.837	man acc	10/2/2023	
O4703-02	Total CN	-0.984	man acc	10/2/2023	
O4703-04	Total CN	-1.073	man acc	10/2/2023	
O4703-06	Total CN	-1.085	man acc	10/2/2023	
O4703-02DUP	Total CN	-0.950	man acc	10/2/2023	
CCV2	Total CN	245.191	man acc	10/2/2023	
CCB2	Total CN	-0.737	man acc	10/2/2023	

Aquakem v. 7.2AQ1

Results from time period:

Mon Oct 02 17:17:37 2023

Mon Oct 02 17:28:36 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.6506	µg/l	10/2/2023 15:16:30	
5.0PPBCN	A	Total CN	P	4.132	µg/l	10/2/2023 15:16:31	
10PPBCN	A	Total CN	P	9.1669	µg/l	10/2/2023 15:16:32	
50PPBCN	A	Total CN	P	49.2198	µg/l	10/2/2023 15:16:33	
100PPBCN	A	Total CN	P	98.8809	µg/l	10/2/2023 15:16:34	
250PPBCN	A	Total CN	P	257.8477	µg/l	10/2/2023 15:16:35	
500PPBCN	A	Total CN	P	496.4033	µg/l	10/2/2023 15:16:36	
ICV1	S	Total CN	P	92.9254	µg/l	10/2/2023 17:17:37	
ICB1	S	Total CN	P	-0.6857	µg/l	10/2/2023 17:17:39	
CCV1	S	Total CN	P	245.8203	µg/l	10/2/2023 17:17:41	
CCB1	S	Total CN	P	-0.5876	µg/l	10/2/2023 17:17:43	
PB156066BL	S	Total CN	P	-0.8372	µg/l	10/2/2023 17:17:45	
O4703-02	S	Total CN	P	-0.9835	µg/l	10/2/2023 17:17:47	
O4703-04	S	Total CN	P	-1.0728	µg/l	10/2/2023 17:25:16	
O4703-06	S	Total CN	P	-1.0848	µg/l	10/2/2023 17:25:18	
O4703-02DUP	S	Total CN	P	-0.9497	µg/l	10/2/2023 17:25:19	
CCV2	S	Total CN	P	245.1907	µg/l	10/2/2023 17:25:22	
CCB2	S	Total CN	P	-0.7375	µg/l	10/2/2023 17:28:36	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

10/2/2023 15:18


Test Total CN

Accepted 10/2/2023 15:18

Factor 1355
Bias 0.001

Coeff. of det. 0.999619

Errors

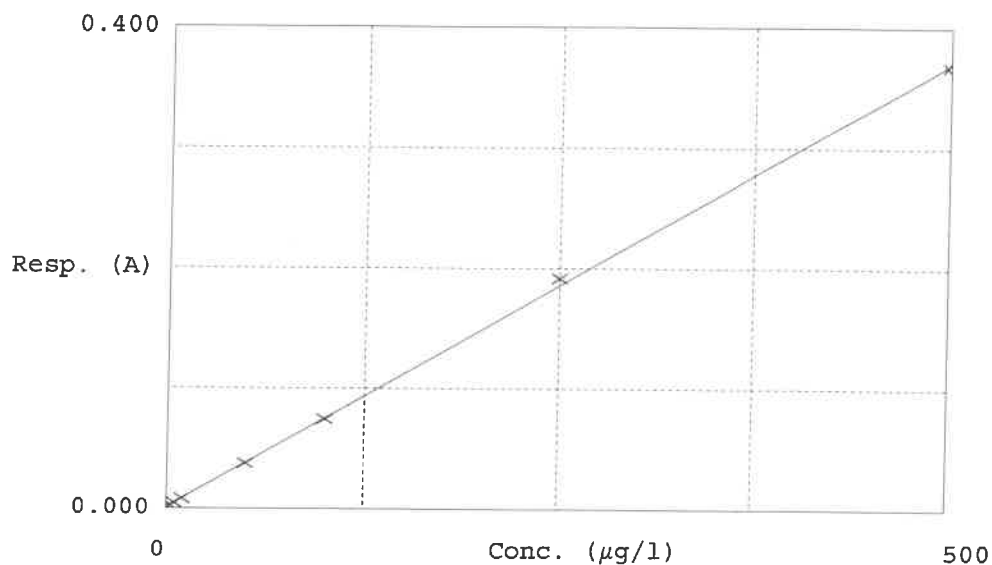

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.0PPBCN	0.001	-0.6506	0.0000	-
2	5.0PPBCN	0.004	4.1320	5.0000	-17.4
3	10PPBCN	0.008	9.1669	10.0000	-8.3
4	50PPBCN	0.038	49.2198	50.0000	-1.6
5	100PPBCN	0.074	98.8809	100.0000	-1.1
6	250PPBCN	0.192	257.8477	250.0000	3.1
7	500PPBCN	0.368	496.4033	500.0000	-0.7

12

10/2/23