


LB127610

SFAM01.1

INSTRUMENT ID: CV1

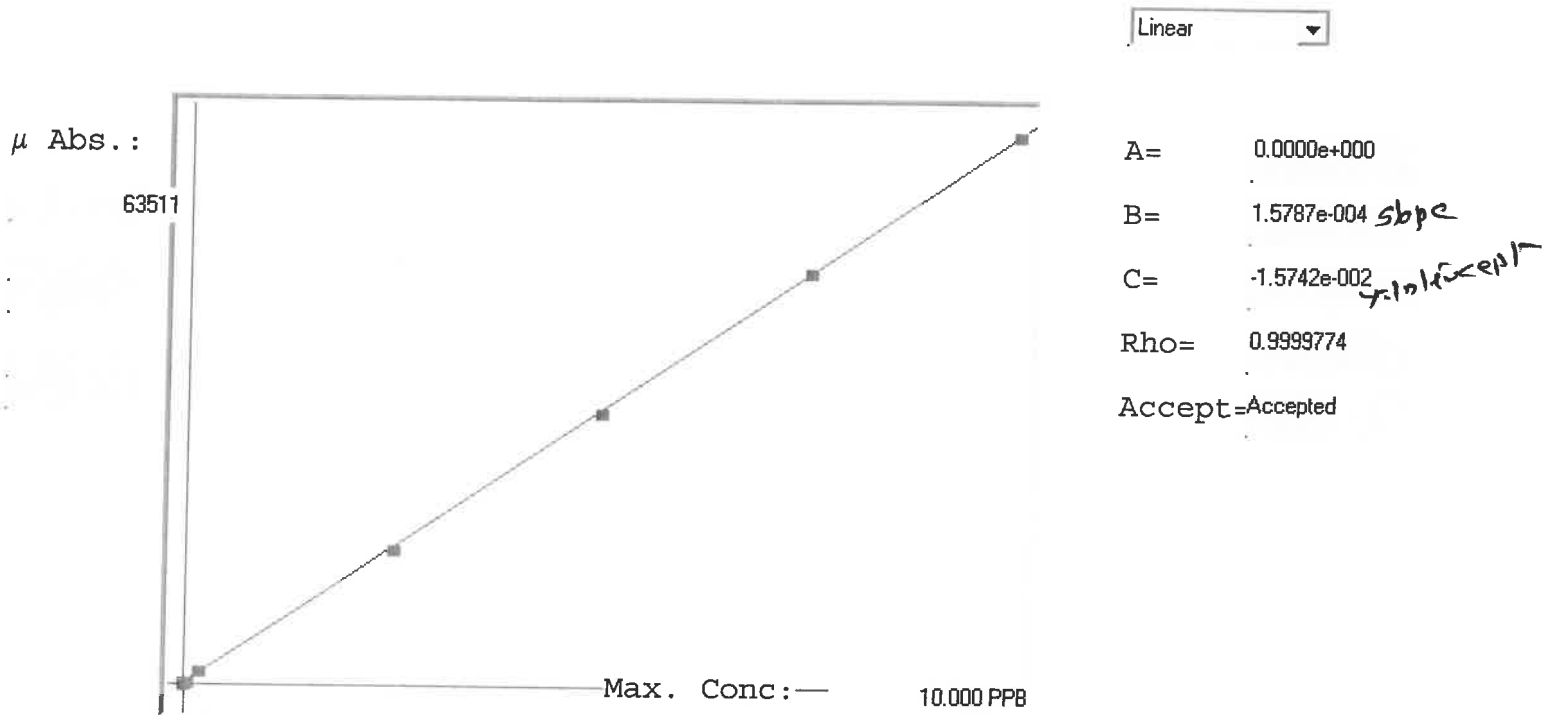

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%H
0.00	0.000	0.014	0.014	189	0.000	189					
0.05	0.050	0.042	-0.008	364	0.0 %	364	0				-16
0.20	0.200	0.234	0.034	1585	0.0 %	1585					17
2.50	2.500	2.464	-0.036	15709	0.0 %	15709					11
5.00	5.000	4.966	-0.034	31554	0.0 %	31554					11
7.50	7.500	7.519	0.019	47724	0.0 %	47724					0
10.0	10.000	10.011	0.011	63511	0.0 %	63511					0

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	189	-		0 SFAM01.1	PPB	10/4/2023 13:41	Std
	0.05 S01	364	-		0.05 SFAM01.1	PPB	10/4/2023 13:48	Std
	0.2 S02	1585	-		0.2 SFAM01.1	PPB	10/4/2023 13:50	Std
	2.5 S03	15709	-		2.5 SFAM01.1	PPB	10/4/2023 13:55	Std
	5 S04	31554	-		5 SFAM01.1	PPB	10/4/2023 13:57	Std
	7.5 S05	47724	-		7.5 SFAM01.1	PPB	10/4/2023 14:00	Std
	10 S06	63511	-		10 SFAM01.1	PPB	10/4/2023 14:11	Std
ICV095	ICV095	25265	3.9729 -		SFAM01.1	PPB	10/4/2023 14:14	SMPL
ICB095	ICB095	127	0.0043 -		SFAM01.1	PPB	10/4/2023 14:16	SMPL
CCV019	CCV019	31709	4.9903 -		SFAM01.1	PPB	10/4/2023 14:19	SMPL
CCB019	CCB019	127	0.0043 -		SFAM01.1	PPB	10/4/2023 14:21	SMPL
PB156112BL	PBS112	30	-0.011 -		SFAM01.1	PPB	10/4/2023 14:23	SMPL
O4518-01	MJUB81	453	0.0558 -		SFAM01.1	PPB	10/4/2023 14:25	SMPL
O4518-02	MJUB82	400	0.0474 -		SFAM01.1	PPB	10/4/2023 14:28	SMPL
O4518-03	MJUB82D	252	0.024 -		SFAM01.1	PPB	10/4/2023 14:30	SMPL
O4518-04	MJUB82S	15470	2.4266 -		SFAM01.1	PPB	10/4/2023 14:32	SMPL
O4518-05	MJUB83	711	0.0965 -		SFAM01.1	PPB	10/4/2023 14:34	SMPL
O4518-06	MJUB84	650	0.0869 -		SFAM01.1	PPB	10/4/2023 14:37	SMPL
O4518-07	MJUB85	1636	0.2425 -		SFAM01.1	PPB	10/4/2023 14:39	SMPL
O4518-08	MJUB86	771	0.106 -		SFAM01.1	PPB	10/4/2023 14:41	SMPL
O4518-09	MJUB87	806	0.1115 -		SFAM01.1	PPB	10/4/2023 14:44	SMPL
O4518-10	MJUB88	1296	0.1889 -		SFAM01.1	PPB	10/4/2023 14:46	SMPL
O4518-11	MJUB89	587	0.0769 -		SFAM01.1	PPB	10/4/2023 14:48	SMPL
O4518-12	MJUB90	258	0.025 -		SFAM01.1	PPB	10/4/2023 14:50	SMPL
O4518-13	MJUB91	839	0.1167 -		SFAM01.1	PPB	10/4/2023 14:53	SMPL
O4518-14	MJUB92	2256	0.3404 -		SFAM01.1	PPB	10/4/2023 14:55	SMPL
O4518-15	MJUB93	7618	1.1869 -		SFAM01.1	PPB	10/4/2023 14:57	SMPL
O4518-16	MJUB94	7731	1.2048 -		SFAM01.1	PPB	10/4/2023 14:59	SMPL
O4518-17	MJUB95	3691	0.567 -		SFAM01.1	PPB	10/4/2023 15:02	SMPL
O4518-18	MJUB96	2289	0.3456 -		SFAM01.1	PPB	10/4/2023 15:04	SMPL
O4518-19	MJUB97	2732	0.4156 -		SFAM01.1	PPB	10/4/2023 15:06	SMPL
CCV020	CCV020	31397	4.941 -		SFAM01.1	PPB	10/4/2023 15:08	SMPL
CCB020	CCB020	143	0.0068 -		SFAM01.1	PPB	10/4/2023 15:11	SMPL
O4518-20	MJUB98	4244	0.6543 -		SFAM01.1	PPB	10/4/2023 15:13	SMPL
O4518-21	MJUB99	297	0.0311 -		SFAM01.1	PPB	10/4/2023 15:15	SMPL
PB156113BL	PBS113	28	-0.0113 -		SFAM01.1	PPB	10/4/2023 15:17	SMPL
O4519-01	MJUBA0	300	0.0316 -		SFAM01.1	PPB	10/4/2023 15:20	SMPL
O4519-02	MJUBA1	2078	0.3123 -		SFAM01.1	PPB	10/4/2023 15:22	SMPL
O4519-03	MJUBA2	4925	0.7618 -		SFAM01.1	PPB	10/4/2023 15:24	SMPL
O4519-04	MJUBA3	11822	1.8506 -		SFAM01.1	PPB	10/4/2023 15:26	SMPL
O4519-05	MJUBA4	5861	0.9096 -		SFAM01.1	PPB	10/4/2023 15:29	SMPL
O4519-06	MJUBA5	3847	0.5916 -		SFAM01.1	PPB	10/4/2023 15:31	SMPL
O4519-07	MJUBA6	5544	0.8595 -		SFAM01.1	PPB	10/4/2023 15:33	SMPL
O4519-08	MJUBA7	387	0.0454 -		SFAM01.1	PPB	10/4/2023 15:36	SMPL
O4519-09	MJUBA8	287	0.0296 -		SFAM01.1	PPB	10/4/2023 15:38	SMPL
O4519-10	MJUBA9	296	0.031 -		SFAM01.1	PPB	10/4/2023 15:40	SMPL

O4519-11	MJUBB0	371	0.0428 -	SFAM01.1	PPB	10/4/2023 15:42 SMPL
O4519-12	MJUBC2	599	0.0788 -	SFAM01.1	PPB	10/4/2023 15:45 SMPL
O4519-13	MJUBC3	252	0.024 -	SFAM01.1	PPB	10/4/2023 15:47 SMPL
O4519-14	MJUBC4	225	0.0198 -	SFAM01.1	PPB	10/4/2023 15:49 SMPL
O4519-15	MJUBD1	2296	0.3467 -	SFAM01.1	PPB	10/4/2023 15:51 SMPL
O4519-16	MJUBD2	798	0.1102 -	SFAM01.1	PPB	10/4/2023 15:54 SMPL
O4519-17	MJUBD2D	831	0.1155 -	SFAM01.1	PPB	10/4/2023 15:56 SMPL
CCV021	CCV021	31031	4.8832 -	SFAM01.1	PPB	10/4/2023 15:58 SMPL
CCB021	CCB021	159	0.0094 -	SFAM01.1	PPB	10/4/2023 16:00 SMPL
O4519-18	MJUBD2S	17011	2.6698 -	SFAM01.1	PPB	10/4/2023 16:03 SMPL
O4519-19	MJUBD3	907	0.1274 -	SFAM01.1	PPB	10/4/2023 16:05 SMPL
O4519-20	MJUBD4	6836	1.0635 -	SFAM01.1	PPB	10/4/2023 16:07 SMPL
O4519-21	MJUBD5	5049	0.7814 -	SFAM01.1	PPB	10/4/2023 16:10 SMPL
O4519-22	MJUBD6	2266	0.342 -	SFAM01.1	PPB	10/4/2023 16:12 SMPL
PB156114BL	PBS114	124	0.0038 -	SFAM01.1	PPB	10/4/2023 16:14 SMPL
O4520-01	MJUBD7	2308	0.3486 -	SFAM01.1	PPB	10/4/2023 16:16 SMPL
O4520-02	MJUBD8	759	0.1041 -	SFAM01.1	PPB	10/4/2023 16:19 SMPL
O4520-03	MJUBD9	1084	0.1554 -	SFAM01.1	PPB	10/4/2023 16:21 SMPL
O4520-04	MJUBE0	796	0.1099 -	SFAM01.1	PPB	10/4/2023 16:23 SMPL
O4520-05	MJUBE1	2877	0.4385 -	SFAM01.1	PPB	10/4/2023 16:25 SMPL
O4520-06	MJUBF4	3847	0.5916 -	SFAM01.1	PPB	10/4/2023 16:28 SMPL
O4520-07	MJUBF5	2130	0.3205 -	SFAM01.1	PPB	10/4/2023 16:30 SMPL
O4520-08	MJUBF6	2294	0.3464 -	SFAM01.1	PPB	10/4/2023 16:32 SMPL
O4520-09	MJUBF7	1007	0.1432 -	SFAM01.1	PPB	10/4/2023 16:34 SMPL
O4520-10	MJUBF8	2163	0.3257 -	SFAM01.1	PPB	10/4/2023 16:37 SMPL
O4520-11	MJUBF9	11092	1.7354 -	SFAM01.1	PPB	10/4/2023 16:39 SMPL
O4520-12	MJUBG0	6191	0.9617 -	SFAM01.1	PPB	10/4/2023 16:41 SMPL
O4520-13	MJUBG1	3845	0.5913 -	SFAM01.1	PPB	10/4/2023 16:44 SMPL
O4520-14	MJUBG2	3562	0.5466 -	SFAM01.1	PPB	10/4/2023 16:46 SMPL
CCV022	CCV022	30907	4.8637 -	SFAM01.1	PPB	10/4/2023 16:48 SMPL
CCB022	CCB022	156	0.0089 -	SFAM01.1	PPB	10/4/2023 16:50 SMPL
O4520-15	MJUBG2D	3738	0.5744 -	SFAM01.1	PPB	10/4/2023 16:53 SMPL
O4520-16	MJUBG2S	18998	2.9835 -	SFAM01.1	PPB	10/4/2023 16:55 SMPL
O4520-17	MJUBG3	2795	0.4255 -	SFAM01.1	PPB	10/4/2023 16:57 SMPL
O4520-18	MJUBG4	3354	0.5138 -	SFAM01.1	PPB	10/4/2023 16:59 SMPL
O4520-19	MJUBG5	4265	0.6576 -	SFAM01.1	PPB	10/4/2023 17:02 SMPL
CCV023	CCV023	31173	4.9057 -	SFAM01.1	PPB	10/4/2023 17:04 SMPL
CCB023	CCB023	145	0.0071 -	SFAM01.1	PPB	10/4/2023 17:06 SMPL