

Clear table


Instrument ID: IC-2				Analyst :		IZ		Method:		300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-09-13	9/13/23 11:34		Iz/MA
STD2	0.4370	0.6640	0.6720	2.2480	0.5650	0.9910	3.5010	0.0000_2023-09-13	9/13/23 12:04		Iz/MA
STD3	0.8560	1.1860	1.1800	3.9540	0.9900	1.9910	5.9710	0.0000_2023-09-13	9/13/23 12:35		Iz/MA
STD4	0.9990	1.5150	1.5110	5.0350	1.2610	2.6440	7.5340	0.0000_2023-09-13	9/13/23 13:17		Iz/MA
STD5	1.8950	2.9390	2.9450	9.7600	2.4350	4.8490	14.4550	0.0000_2023-09-13	9/13/23 13:48		Iz/MA
STD6	3.9370	5.9070	5.8970	19.6950	4.9130	9.9780	29.4710	0.0000_2023-09-13	9/13/23 14:19		Iz/MA
STD7	5.0750	7.5900	7.5960	25.3080	6.3360	12.5480	38.0680	0.0000_2023-09-13	9/13/23 14:49		Iz/MA
ICV	1.9120	2.8680	2.8940	9.5640	2.4030	5.0020	14.1400	0.0000_2023-09-13	9/13/23 15:20		Iz/MA
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-09-13	9/13/23 15:52		Iz/MA
CCV	1.9370	2.9990	3.0040	9.7420	2.4430	4.9550	14.4420	0.0000_2023-10-05	10/5/23 23:54		Iz/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 0:26		Iz/MA
LB127682BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 0:58		Iz/MA
LB127682BSW	2.0210	3.1550	3.1470	10.1960	2.5590	5.1360	15.1020	0.0000_2023-10-06	10/6/23 1:29		Iz/MA
O4723-01	0.9550	163.2150	0.0000	0.0000	2.3420	0.4470	54.9460	0.0000_2023-10-06	10/6/23 2:01		Iz/MA
O4723-01MS	3.1970	158.5170	2.9940	10.3520	4.8670	8.2010	69.9190	0.0000_2023-10-06	10/6/23 2:33		Iz/MA
O4723-01MSD	3.1490	160.1690	2.8880	9.9570	4.7640	7.5740	68.8890	0.0000_2023-10-06	10/6/23 3:04		Iz/MA
O4723-02	0.4710	482.8050	0.0000	0.0000	0.0000	2.3970	44.8430	0.0000_2023-10-06	10/6/23 3:36		Iz/MA
O4723-03	1.3150	727.1420	0.0000	0.0000	0.0000	2.9390	56.5890	0.0000_2023-10-06	10/6/23 4:07		Iz/MA
O4723-04	0.0000	76.3370	0.0000	0.0000	4.4140	0.5390	23.2560	0.0000_2023-10-06	10/6/23 4:39		Iz/MA
O4724-01	0.7200	173.8920	0.0000	0.0000	0.0000	0.0000	27.5840	0.0000_2023-10-06	10/6/23 5:11		Iz/MA
O4724-02	0.0000	671.2470	0.0000	0.0000	5.7830	0.0000	450.5580	0.0000_2023-10-06	10/6/23 5:42		Iz/MA
CCV	1.8190	2.9780	2.9340	9.6490	2.4200	4.7240	14.2060	0.0000_2023-10-06	10/6/23 6:46		Iz/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 7:18		Iz/MA
O4724-03	0.5130	956.7700	0.0000	0.0000	7.3660	0.6060	23.4610	0.0000_2023-10-06	10/6/23 7:49		Iz/MA
O4724-04	0.6780	39.2590	0.0000	0.0000	0.9670	5.3120	15.0720	0.0000_2023-10-06	10/6/23 8:21		Iz/MA
CCV	1.9320	3.1890	3.1230	10.2730	2.5700	0.6320	23.6730	0.0000_2023-10-06	10/6/23 8:53		Iz/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 9:24		Iz/MA
LB127682BLW2	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 9:56		Iz/MA
LB127682BSW2	1.8390	3.1010	3.0330	9.9270	2.4900	4.8080	14.6110	0.0000_2023-10-06	10/6/23 10:28		Iz/MA
O4723-01DLX2	0.6700	78.1890	0.0000	0.0000	0.0000	0.0000	26.0860	0.0000_2023-10-06	10/6/23 11:00		Iz/MA
O4723-02DLX2	0.0000	301.0600	0.0000	0.0000	0.0000	1.1450	21.0680	0.0000_2023-10-06	10/6/23 11:31		Iz/MA
O4723-03DLX2	0.6500	483.4100	0.0000	0.0000	0.0000	1.4750	26.6150	0.0000_2023-10-06	10/6/23 12:03		Iz/MA
O4724-02DLX20	0.0000	62.9170	0.0000	0.0000	0.3830	0.0000	16.3250	0.0000_2023-10-06	10/6/23 12:34		Iz/MA
O4724-03DLX2	0.0000	635.8970	0.0000	0.0000	3.5170	0.4450	105.8240	0.0000_2023-10-06	10/6/23 13:06		Iz/MA
O4724-03DL2X10	0.0000	225.8040	0.0000	0.0000	0.7760	0.0000	18.8770	0.0000_2023-10-06	10/6/23 13:38		Iz/MA
CCV	1.9380	3.0580	3.0200	9.7740	2.4630	4.7410	14.4450	0.0000_2023-10-06	10/6/23 14:09		Iz/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2023-10-06	10/6/23 14:41		Iz/MA

Clear table

Instrument ID: IC-2									
Analyst : IZ				Method: 300.0 / 9056A					
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 11:34
STD2	0.4370	0.6640	0.6720	2.2480	0.5650	0.9910	3.5010	2023-09-13_	9/13/23 12:04
STD3	0.8560	1.1860	1.1800	3.9540	0.9900	1.9910	5.9710	2023-09-13_	9/13/23 12:35
STD4	0.9990	1.5150	1.5110	5.0350	1.2610	2.6440	7.5340	2023-09-13_	9/13/23 13:17
STD5	1.8950	2.9390	2.9450	9.7600	2.4350	4.8490	14.4550	2023-09-13_	9/13/23 13:48
STD6	3.9370	5.9070	5.8970	19.6950	4.9130	9.9780	29.4710	2023-09-13_	9/13/23 14:19
STD7	5.0750	7.5900	7.5960	25.3080	6.3360	12.5480	38.0680	2023-09-13_	9/13/23 14:49
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4	Initial wt/ Final Vol	Analyst
STD1									
STD2	9.2500	10.6667	12.0000	12.4000	13.0000	-0.9000	16.7000		
STD3	7.0000	-1.1667	-1.6667	-1.1500	-1.0000	-0.4500	-0.4833		
STD4	-0.1000	1.0000	0.7333	0.7000	0.8800	5.7600	0.4533		
STD5	-5.2500	-2.0333	-1.8333	-2.4000	-2.6000	-3.0200	-3.6333		
STD6	-1.5750	-1.5500	-1.7167	-1.5250	-1.7400	-0.2200	-1.7633		
STD7	1.5000	1.2000	1.2800	1.2320	1.3760	0.3840	2.8865		

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0789497 \cdot A + 4.35704$
 RSD: 3.602 %
 Correlation coefficient: 0.999293

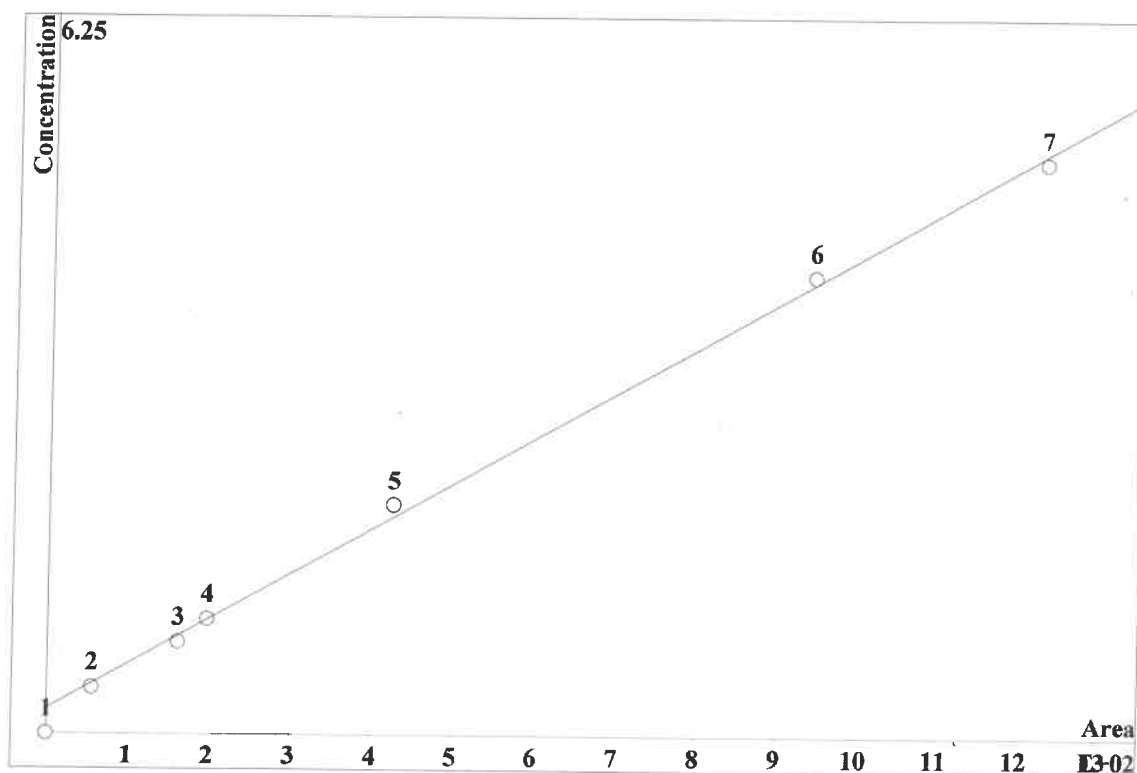


K3 = 0 K2 = 0 K1 = 0.0789497 K0 = 4.35704
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.173	55.53	0.4	20	6.387		
3	1.981	161.8	0.8	20	6.387		
4	2.625	197.8	1	20	6.387		
5	7.098	424.9	2	20	6.387		
6	12.25	942.3	4	20	6.387		
7	16.27	1230	5	20	6.387		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.12855 \cdot A + 3.3899$
 RSD: 2.393 %
 Correlation coefficient: 0.999688

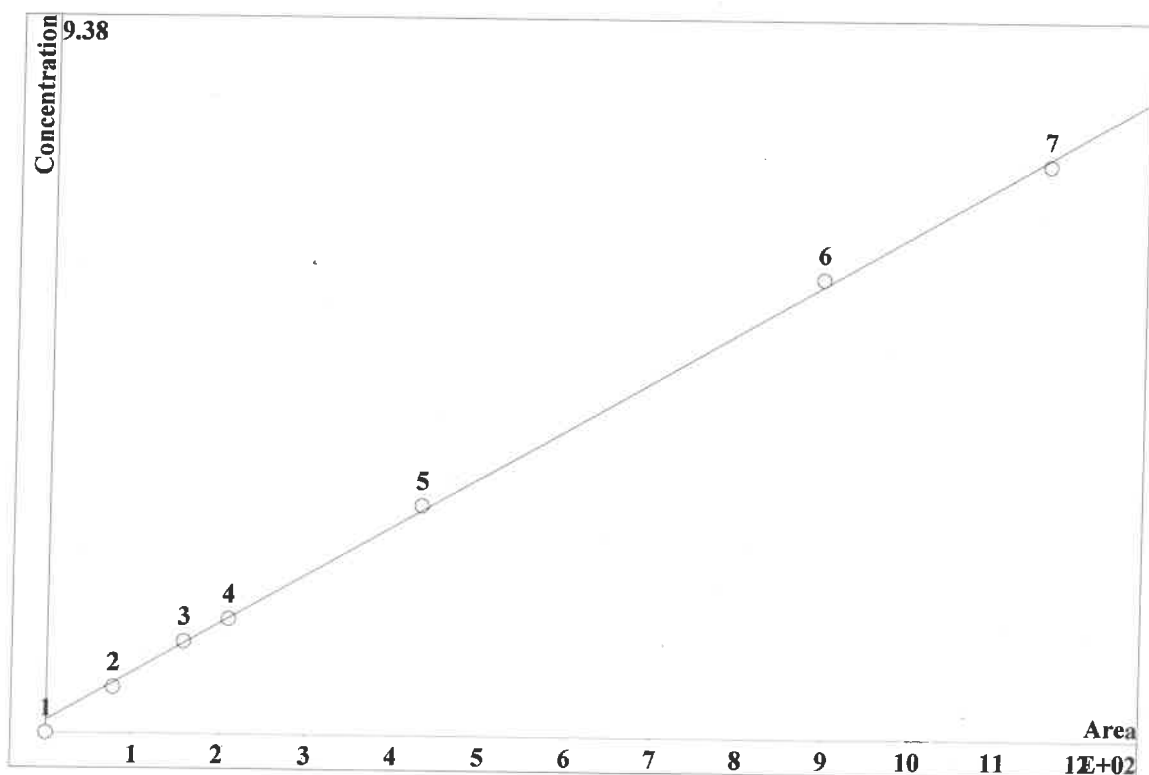


K3 = 0 K2 = 0 K1 = 0.12855 K0 = 3.3899
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.077	76.88	0.6	20	9.512		
3	10.24	158.1	1.2	20	9.512		
4	13.7	209.4	1.5	20	9.512		
5	28.03	430.8	3	20	9.512		
6	58.53	892.6	6	20	9.512		
7	76.44	1154	7.5	20	9.512		
* &							

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0563308 \cdot A + 3.32518$
 RSD: 2.560 %
 Correlation coefficient: 0.999643

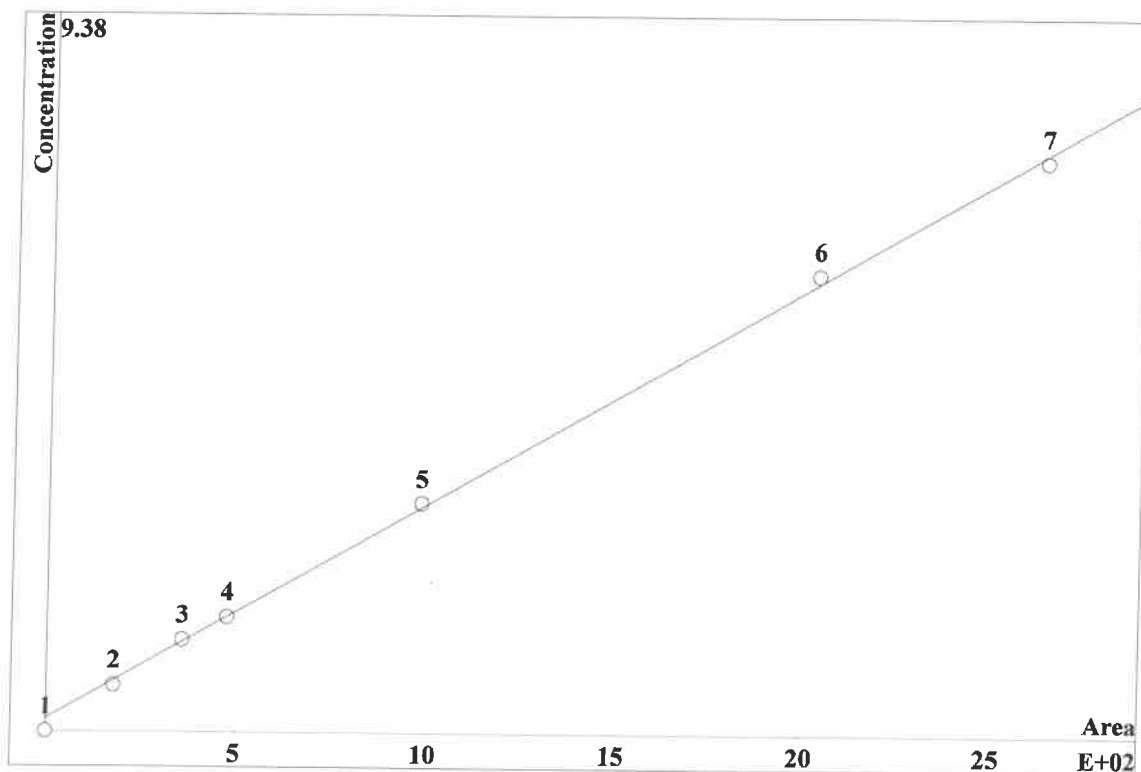


K3 = 0 K2 = 0 K1 = 0.0563308 K0 = 3.32518
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.366	179.4	0.6	20	11.51		
3	18.73	359.8	1.2	20	11.51		
4	25.07	477.3	1.5	20	11.51		
5	50.57	986.7	3	20	11.51		
6	103.2	2035	6	20	11.51		
7	132.4	2638	7.5	20	11.51		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.284269 \cdot A + 12.2101$
 RSD: 2.532 %
 Correlation coefficient: 0.999650

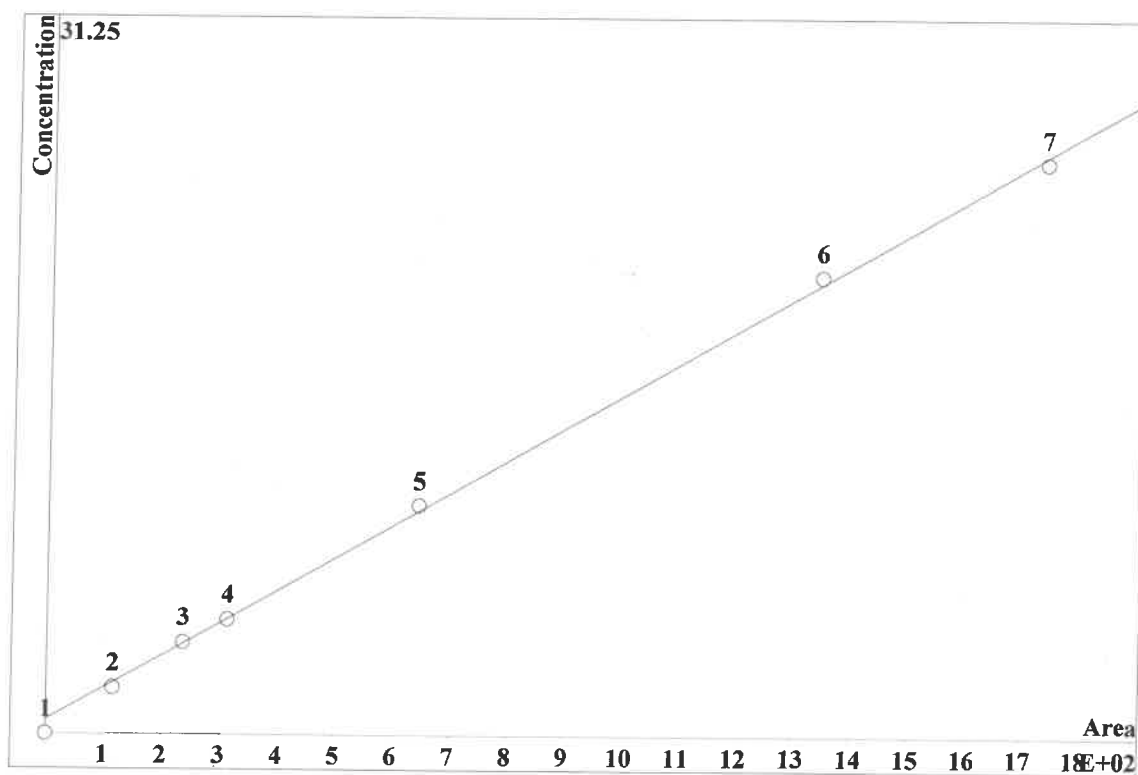


K3 = 0 K2 = 0 K1 = 0.284269 K0 = 12.2101
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.363	115.2	2	20			15
3	10.95	235.3	4	20			15
4	14.67	311.3	5	20			15
5	30.45	643.7	10	20			15
6	64.2	1343	20	20			15
7	83.93	1738	25	20			15

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0496365 \cdot A + 2.72507$
 RSD: 2.794 %
 Correlation coefficient: 0.999574

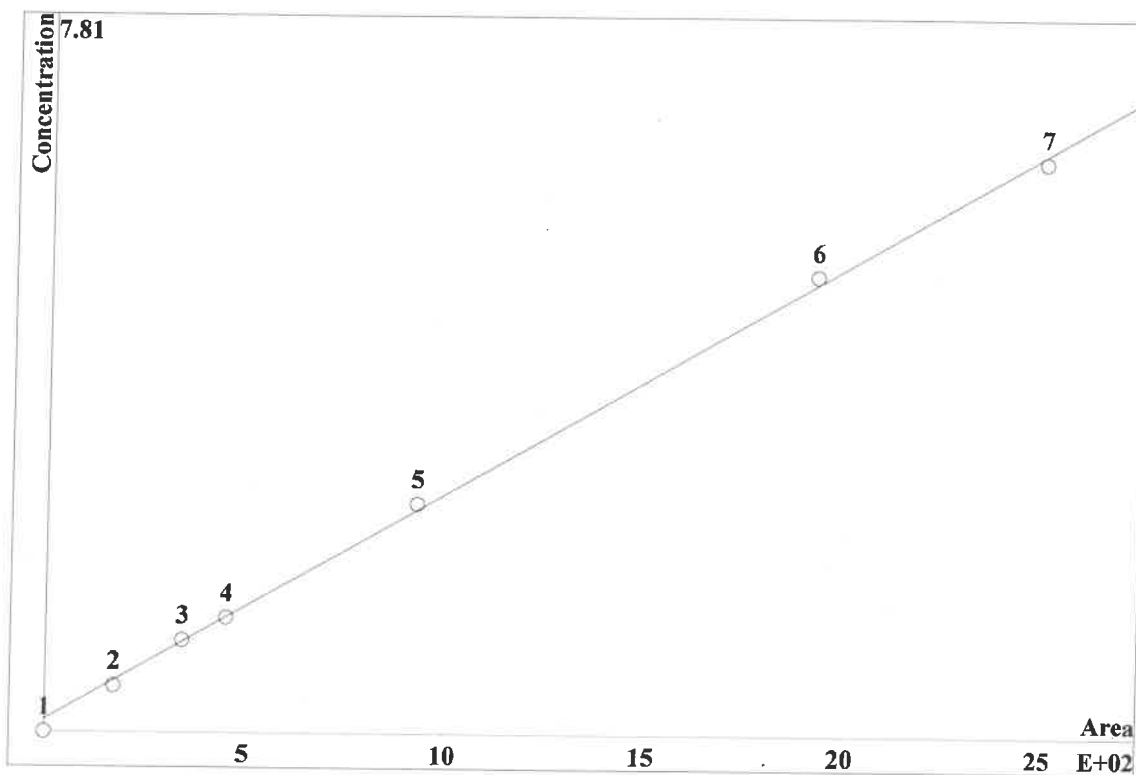


K3 = 0 K2 = 0 K1 = 0.0496365 K0 = 2.72507
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.457	172.6	0.5	20	17.17		
3	12.91	344.1	1	20	17.17		
4	17.23	453.2	1.25	20	17.17		
5	35.37	926.4	2.5	20	17.17		
6	74.05	1925	5	20	17.17		
7	96.74	2498	6.25	20	17.17		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.0538776 \cdot A + 5.92726$
 RSD: 1.958 %
 Correlation coefficient: 0.999791

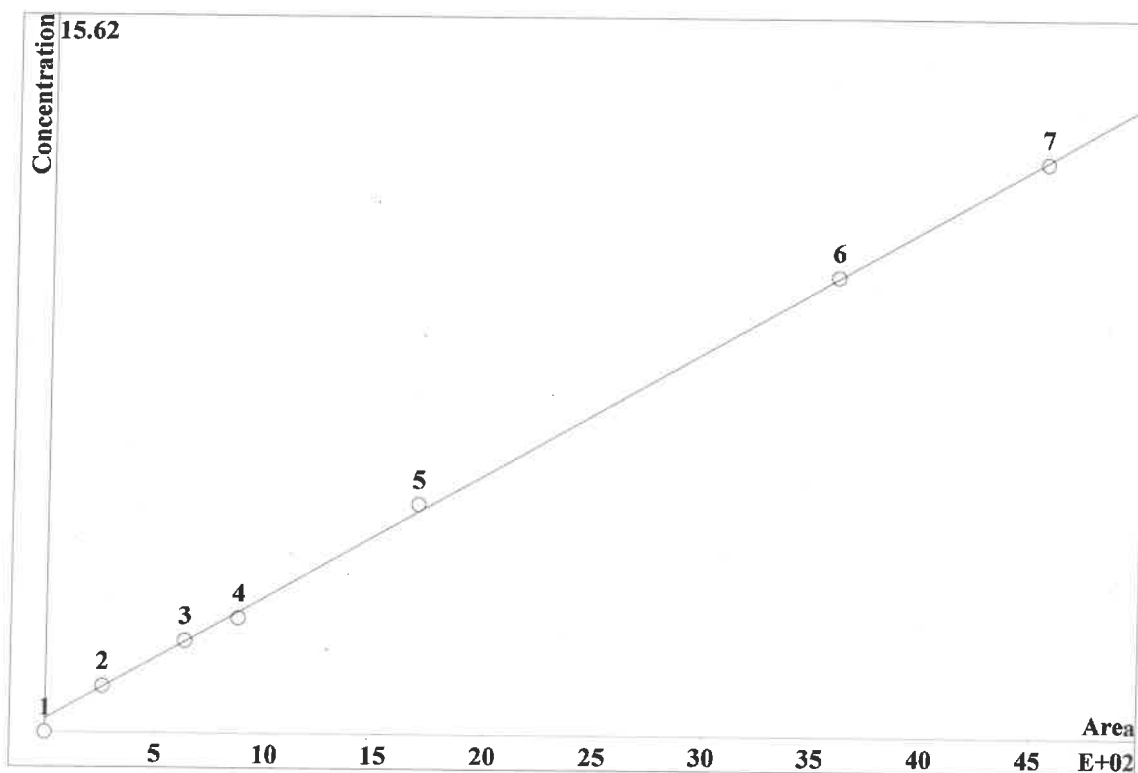


K3 = 0 K2 = 0 K1 = 0.0538776 K0 = 5.92726
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.064	257.8	1	20	22.61		
3	10.79	629	2	20	22.61		
4	15.58	871.3	2.5	20	22.61		
5	31.27	1690	5	20	22.61		
6	74.25	3594	10	20	22.61		
7	97.74	4548	12.5	20	22.61		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-091323.mtw
 Equation: $Q = 0.162289 \cdot A + 17.402$
 RSD: 3.254 %
 Correlation coefficient: 0.999423

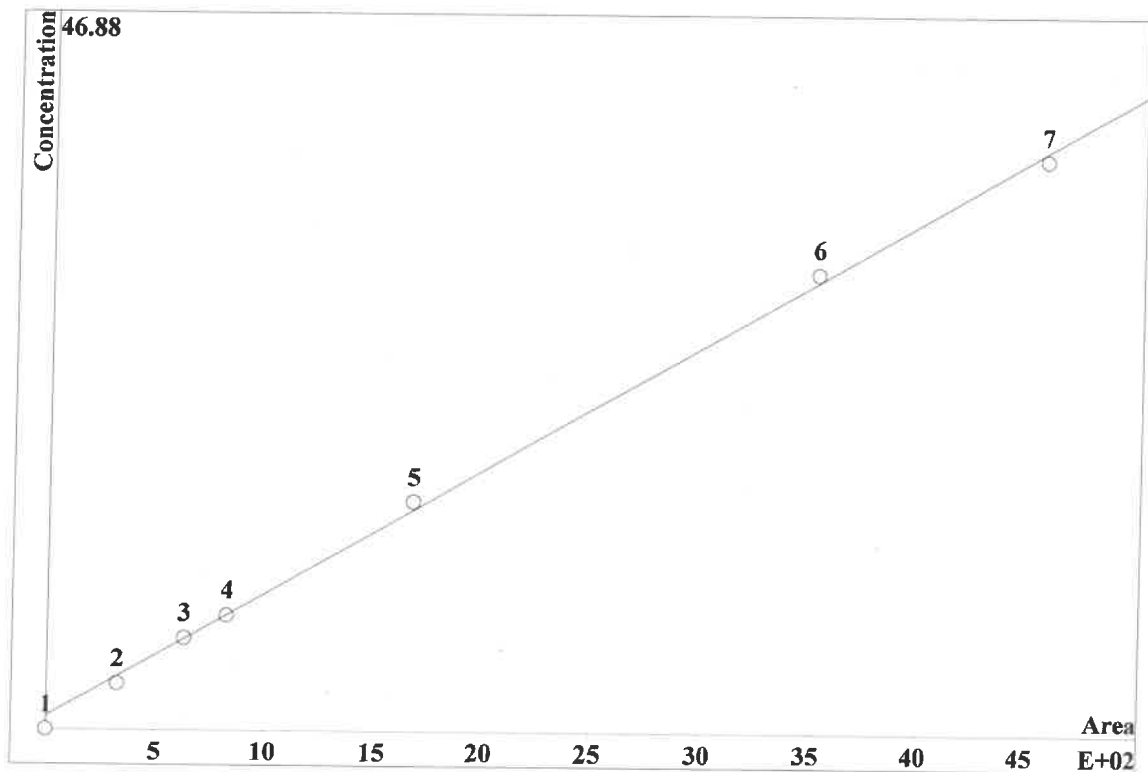

K3 = 0 K2 = 0 K1 = 0.162289 K0 = 17.402
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	9.494	324.2	3	20	26.01		
3	18.79	628.6	6	20	26.01		
4	25.03	821.3	7.5	20	26.01		
5	51.9	1674	15	20	26.01		
6	110.6	3525	30	20	26.01		
7	145.3	4584	37.5	20	26.01		

Report date: 9/14/2023 10:30:13 AM
Printed by: wet


Ident: STD1
Analysis from: 9/13/2023 11:34:20 AM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35408

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

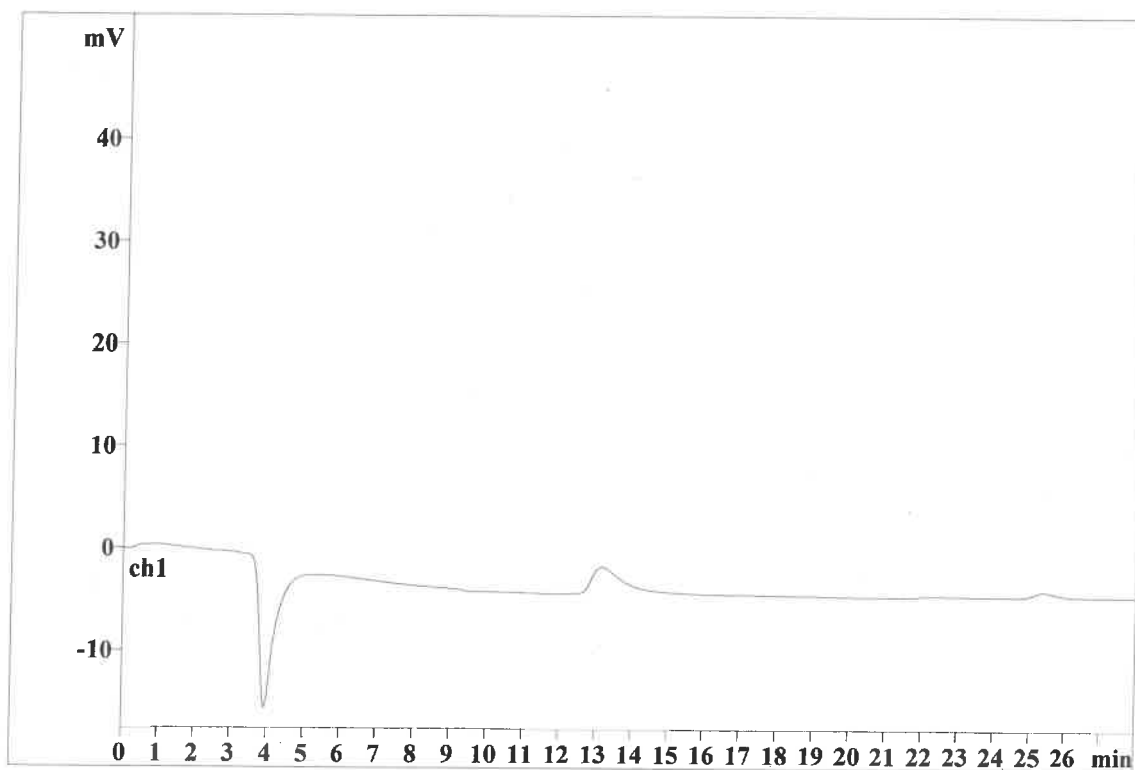

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:19 AM
Printed by: wet


Ident: STD2
Analysis from: 9/13/2023 12:04:58 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35409

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

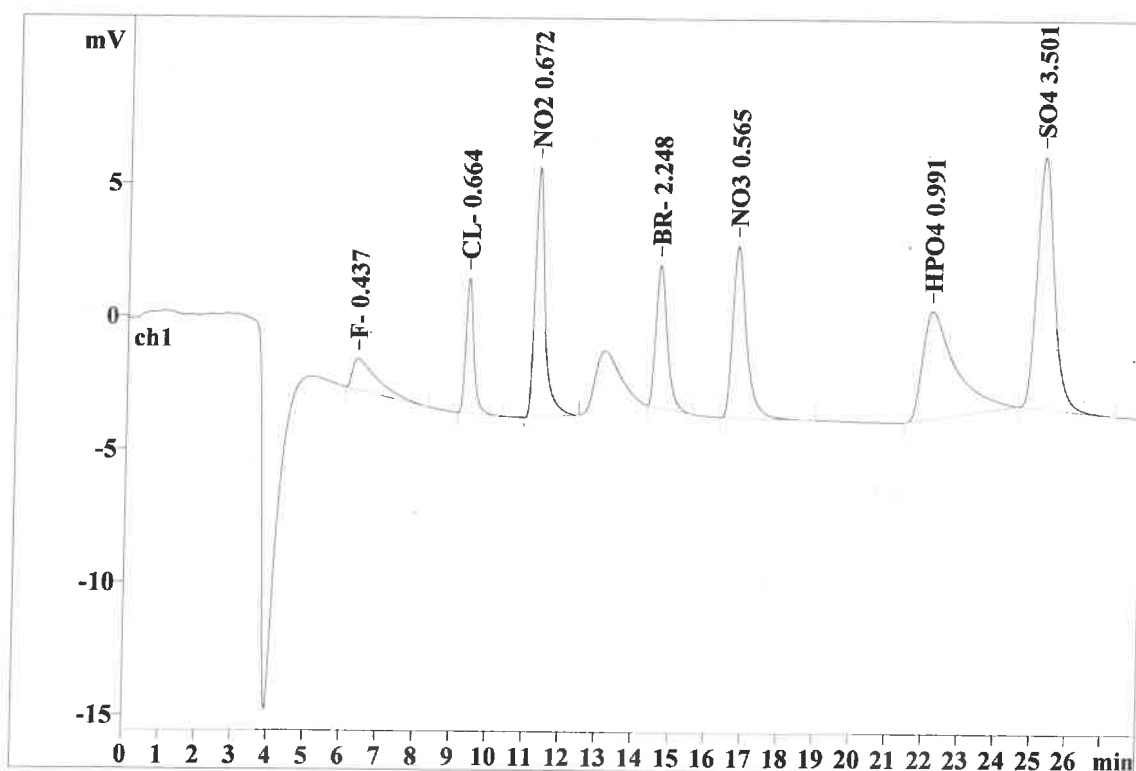

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.35	0.702	1.17	2.86	55.531	4.70
2	9.37	0.223	5.08	12.38	76.877	6.51
3	11.27	0.270	9.37	22.85	179.424	15.18
4	14.62	0.323	5.36	13.08	115.202	9.75
5	16.75	0.390	6.46	15.75	172.628	14.61
6	22.15	0.874	4.06	9.91	257.801	21.82
7	25.23	0.511	9.49	23.16	324.202	27.44
7	28.00	0.470	40.98	99.98	1181.665	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:25 AM
Printed by: wet


Ident: STD3
Analysis from: 9/13/2023 12:35:36 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35410

Last save: 9/13/2023 2:47:

SAMPLE:
:
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

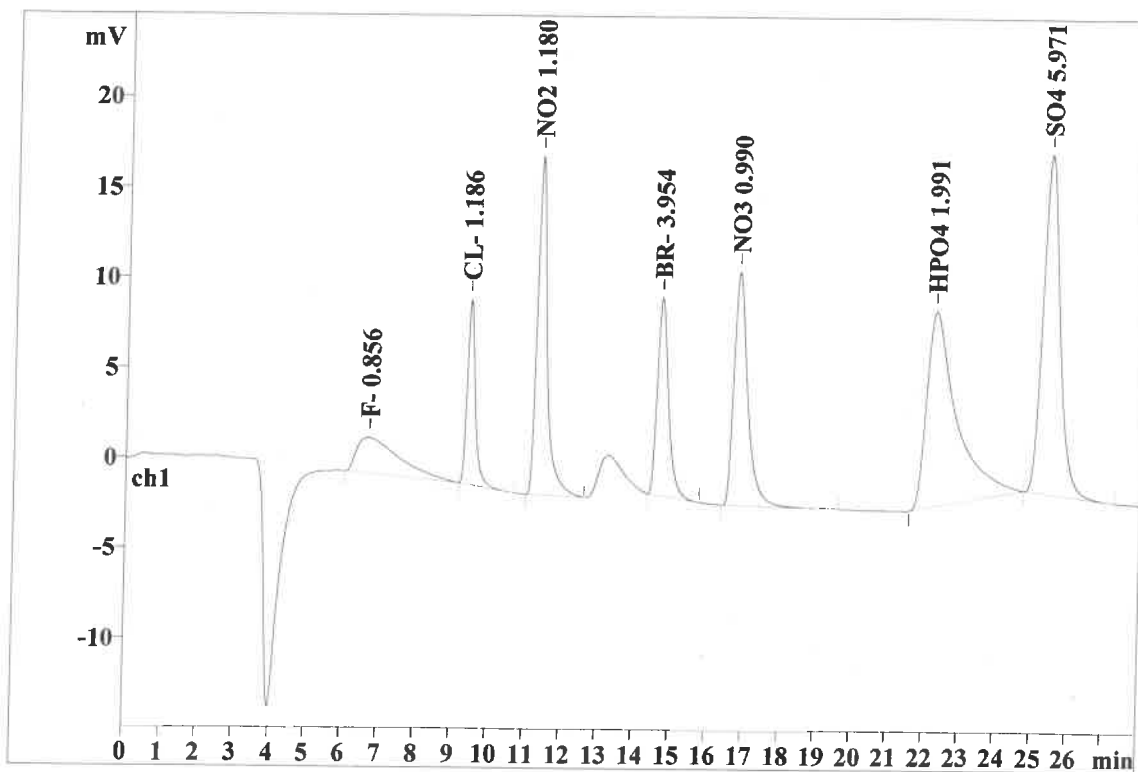

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.67	1.250	1.98	2.35	161.783	6.43
2	9.43	0.224	10.23	12.13	158.085	6.28
3	11.33	0.269	18.73	22.20	359.823	14.30
4	14.68	0.321	10.94	12.97	235.268	9.35
5	16.80	0.388	12.91	15.30	344.076	13.67
6	22.27	0.782	10.79	12.78	629.000	24.99
7	25.41	0.503	18.79	22.26	628.591	24.98
7	28.00	0.534	84.38	99.99	2516.626	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:31 AM
Printed by: wet


Ident: STD4
Analysis from: 9/13/2023 1:17:58 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35411

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

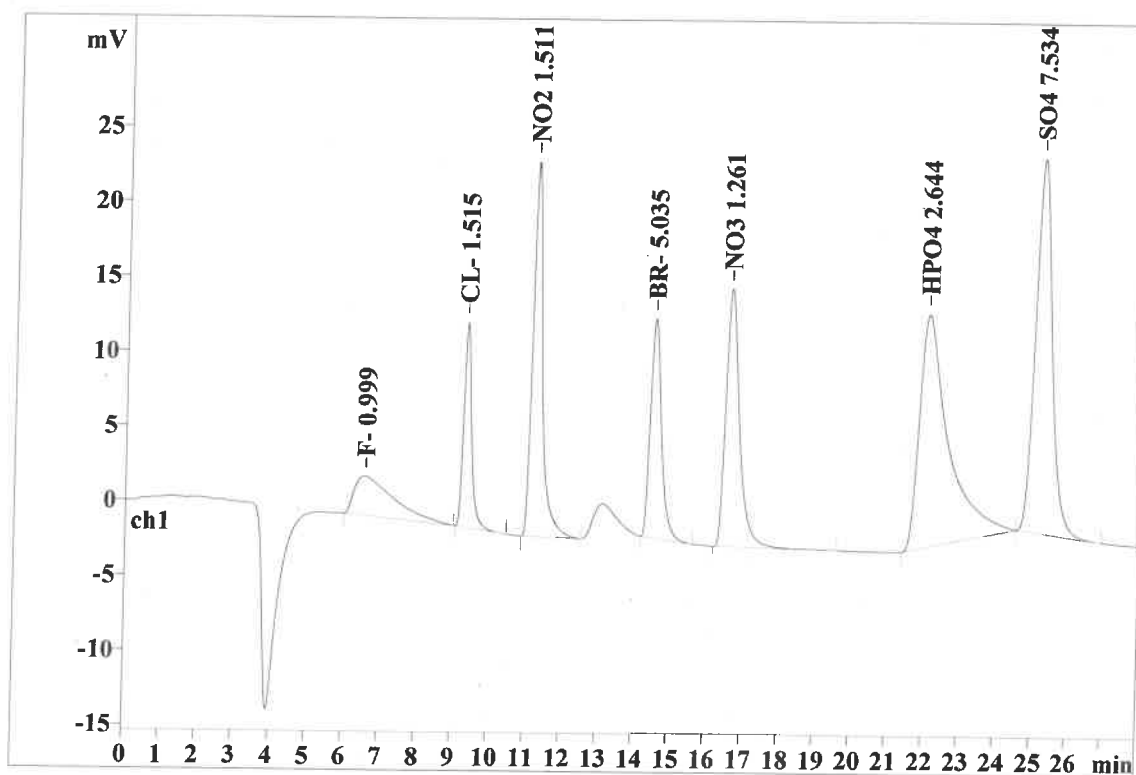

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.56	1.152	2.62	2.30	197.781	5.92
2	9.33	0.222	13.70	12.03	209.390	6.27
3	11.21	0.267	25.07	22.01	477.275	14.28
4	14.52	0.317	14.67	12.88	311.264	9.32
5	16.61	0.384	17.23	15.13	453.175	13.56
6	22.06	0.744	15.57	13.67	871.333	26.08
7	25.19	0.494	25.03	21.97	821.280	24.58
7	28.00	0.512	113.90	99.99	3341.497	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:37 AM
Printed by: wet


Ident: STD5
Analysis from: 9/13/2023 1:48:36 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35412

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

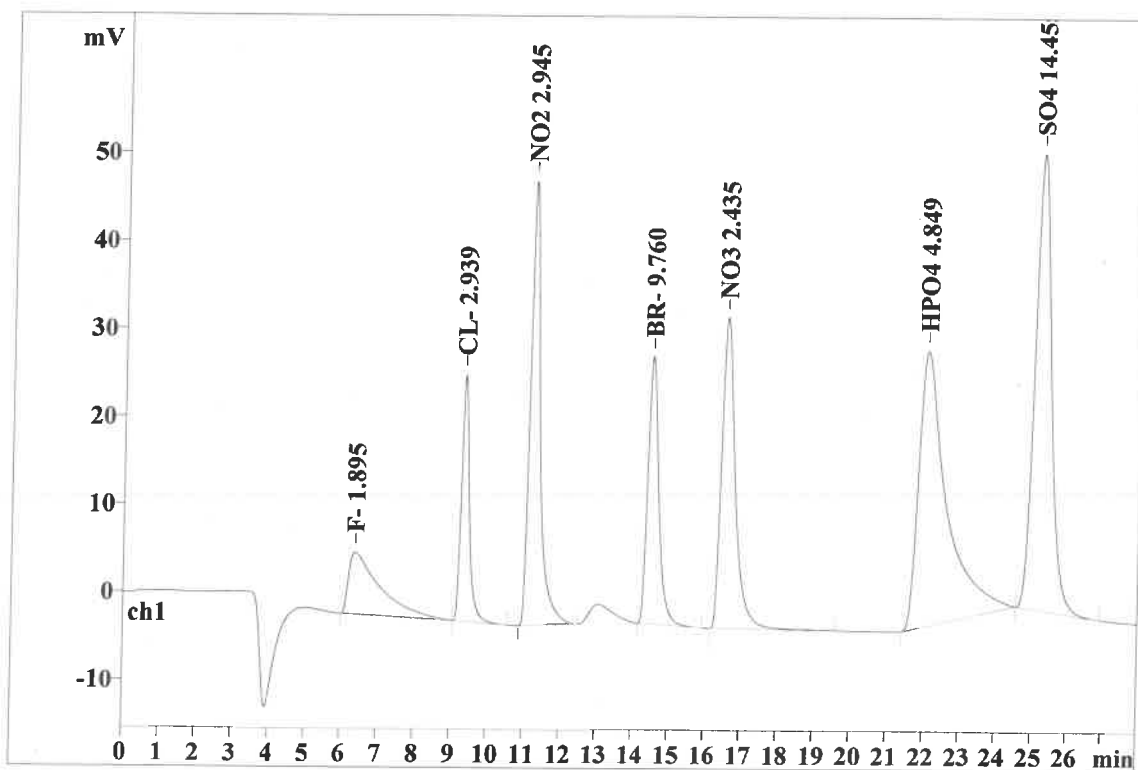

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	0.836	7.10	3.02	424.913	6.27
2	9.35	0.221	28.03	11.94	430.836	6.36
3	11.21	0.273	50.57	21.55	986.701	14.56
4	14.51	0.314	30.45	12.98	643.703	9.50
5	16.56	0.381	35.37	15.07	926.368	13.67
6	22.07	0.712	31.27	13.32	1689.979	24.94
7	25.22	0.486	51.90	22.11	1674.138	24.70
7	28.00	0.460	234.68	100.00	6776.639	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:42 AM
Printed by: wet


Ident: STD6
Analysis from: 9/13/2023 2:19:14 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35413

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

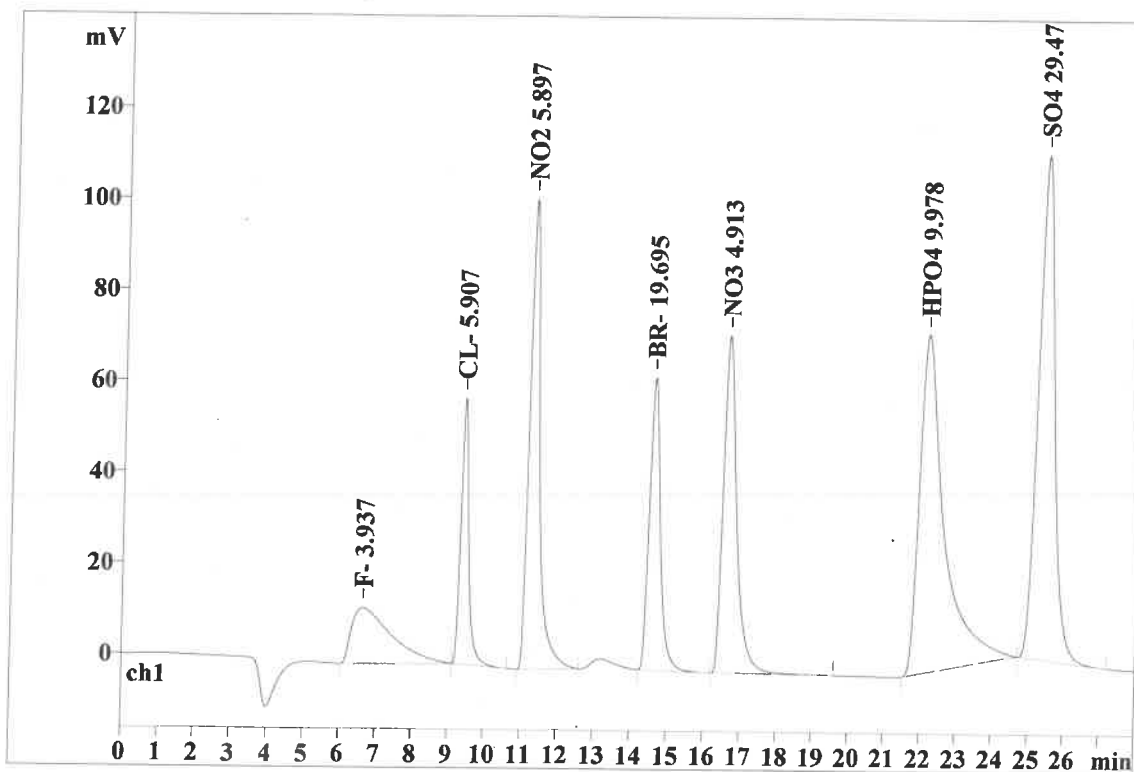

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.63	1.180	12.25	2.46	942.277	6.61
2	9.40	0.219	58.53	11.78	892.649	6.26
3	11.25	0.276	103.16	20.75	2034.568	14.27
4	14.57	0.309	64.20	12.92	1342.719	9.42
5	16.60	0.378	74.04	14.90	1924.573	13.50
6	22.13	0.632	74.25	14.94	3593.867	25.21
7	25.36	0.480	110.60	22.25	3524.692	24.73
7	28.00	0.496	497.04	100.00	14255.344	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:49 AM
Printed by: wet


Ident: STD7
Analysis from: 9/13/2023 2:49:59 PM
File: _2023-09-13_

Last save: 9/13/2023 3:28:05 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35414

Last save: 9/13/2023 2:47:

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

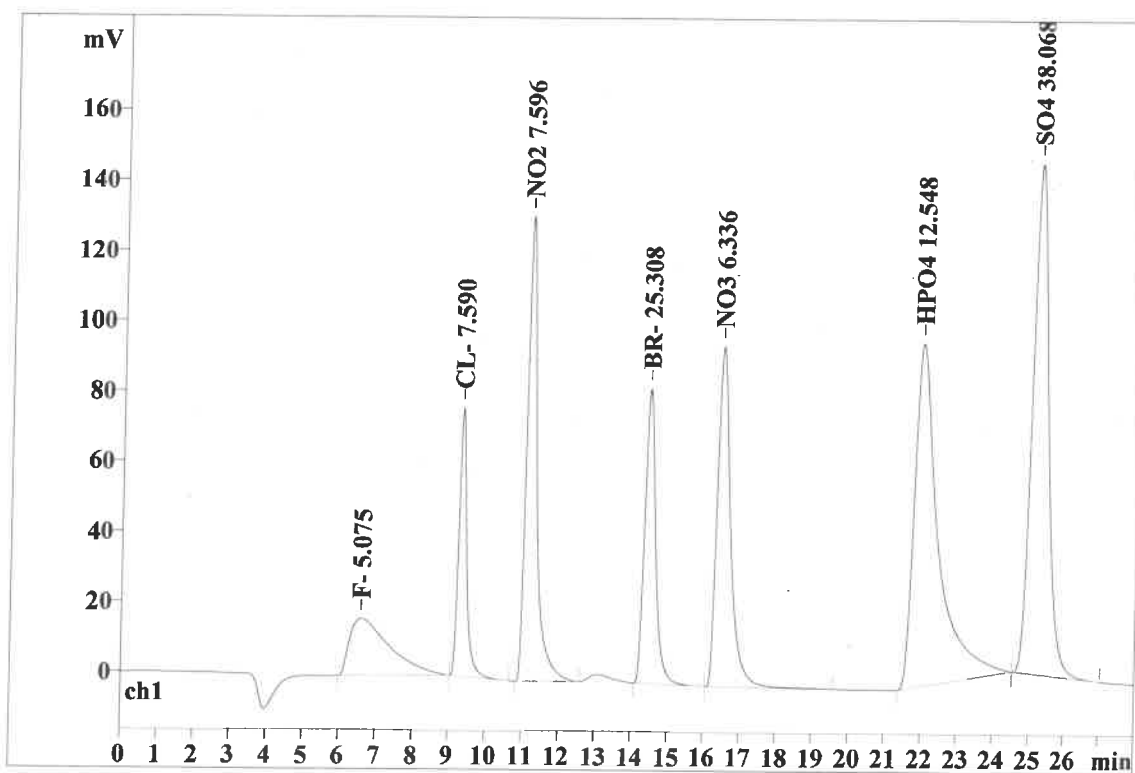

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.60	1.161	16.27	2.51	1230.492	6.69
2	9.32	0.216	76.44	11.78	1154.451	6.28
3	11.16	0.279	132.37	20.40	2637.937	14.34
4	14.46	0.306	83.93	12.94	1737.625	9.45
5	16.45	0.374	96.73	14.91	2498.109	13.58
6	21.96	0.608	97.74	15.07	4547.922	24.73
7	25.19	0.475	145.28	22.39	4584.192	24.93
7	28.00	0.488	648.75	100.00	18390.726	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:30:54 AM
Printed by: wet


Ident: ICV
Analysis from: 9/13/2023 3:20:37 PM
File: 2023-09-13_

Last save: 9/13/2023 3:48:37 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35415

Last save: 9/13/2023 3:17:

SAMPLE:
: IZ/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

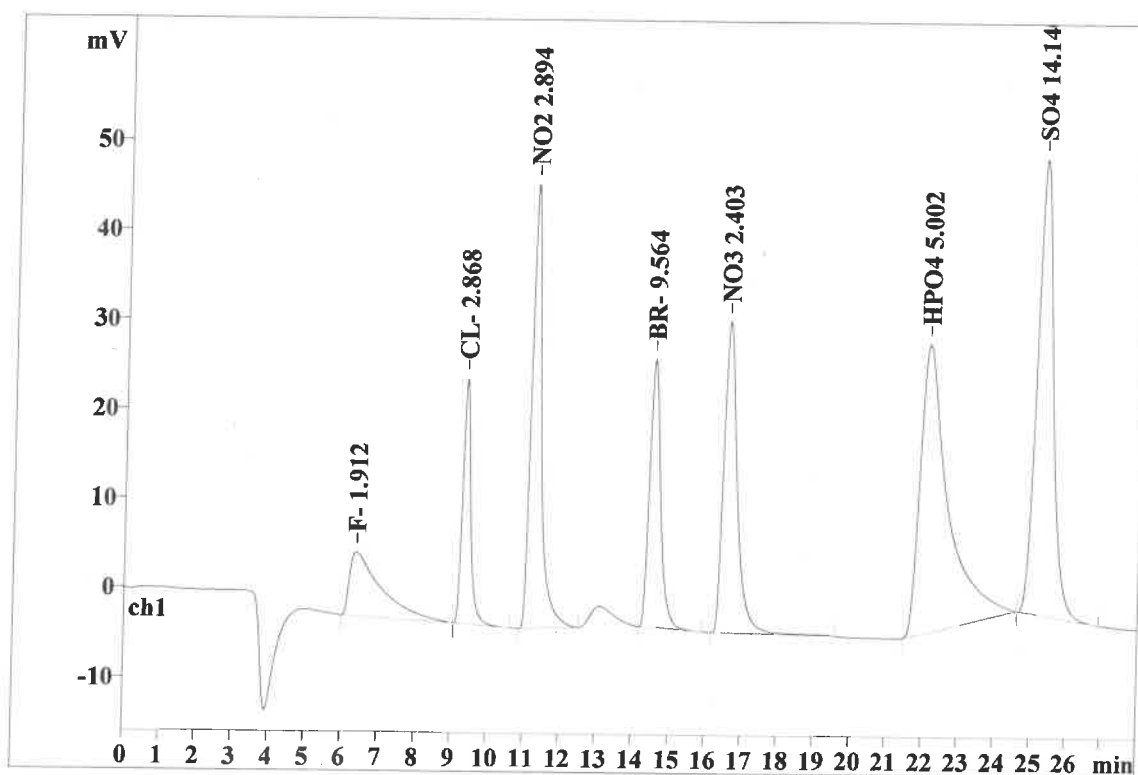

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	0.832	7.15	3.08	426.246	6.33
2	9.35	0.222	27.36	11.79	419.563	6.23
3	11.21	0.274	49.60	21.38	967.809	14.37
4	14.52	0.313	29.96	12.92	629.939	9.35
5	16.57	0.381	34.76	14.99	912.668	13.55
6	22.10	0.713	32.21	13.89	1745.208	25.91
7	25.25	0.484	50.92	21.95	1634.390	24.26
7	28.00	0.460	231.96	100.00	6735.825	100.00

This report has been created by IC Net
METROHM LTD

Report date: 9/14/2023 10:31:34 AM
Printed by: wet


Ident: ICB
Analysis from: 9/13/2023 3:52:42 PM
File: _2023-09-13_

Last save: 9/14/2023 10:31:13 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35416

Last save: 9/13/2023 3:17:

SAMPLE:
: IZ/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

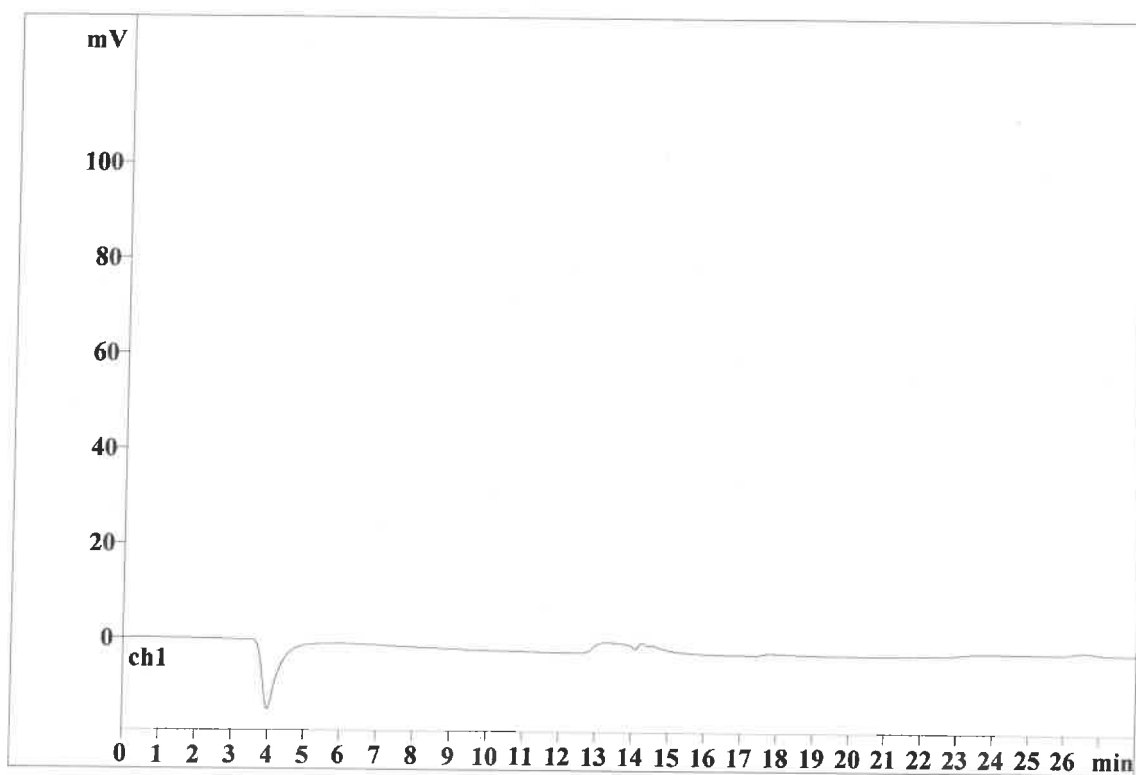

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:07:39 PM
Printed by: wet


Ident: CCV
Analysis from: 10/5/2023 11:54:37 PM
File: 2023-10-05

Last save: 10/6/2023 12:23:37 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35892

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 37
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

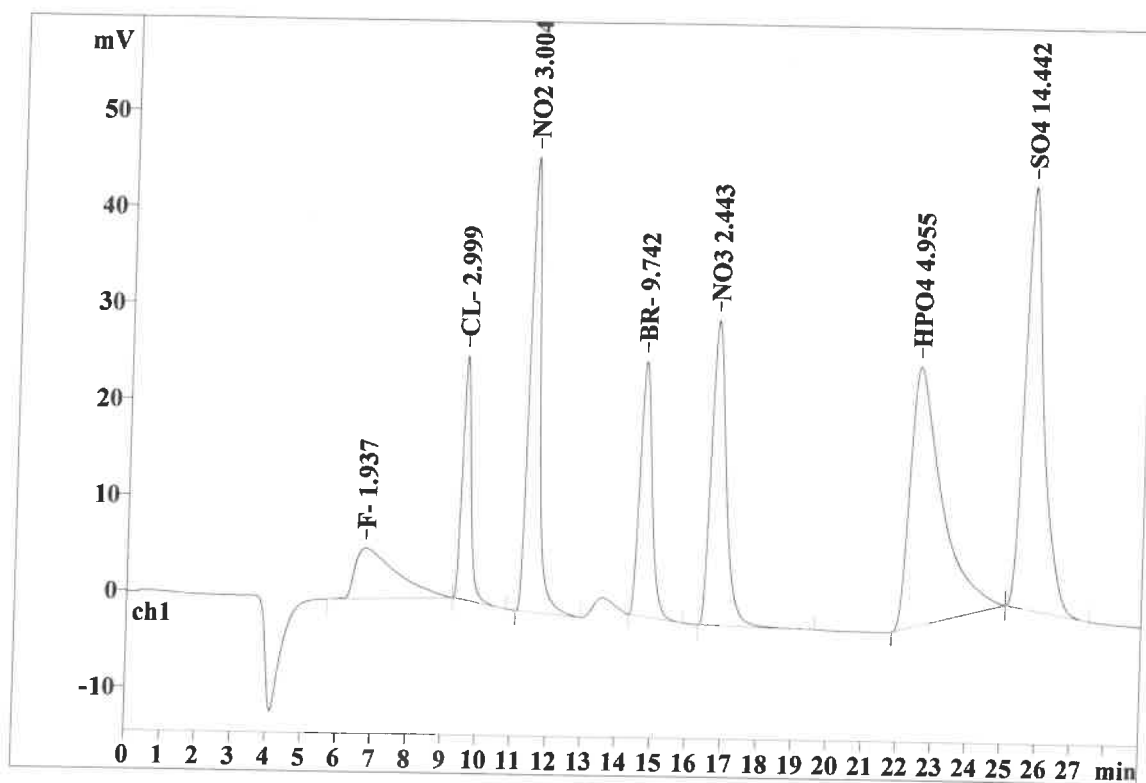

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.76	1.254	5.28	2.55	432.688	6.32
2	9.56	0.259	25.41	12.28	439.971	6.42
3	11.44	0.315	47.28	22.85	1006.920	14.70
4	14.68	0.372	26.48	12.80	642.419	9.38
5	16.72	0.444	31.64	15.29	928.740	13.56
6	22.49	0.913	26.96	13.03	1727.666	25.22
7	25.68	0.548	43.87	21.20	1671.618	24.40
7	29.00	0.586	206.92	100.00	6850.023	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:07:47 PM
Printed by: wet


Ident: CCB
Analysis from: 10/6/2023 12:26:24 AM
File: _2023-10-06_

Last save: 10/6/2023 12:55:24 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35893

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

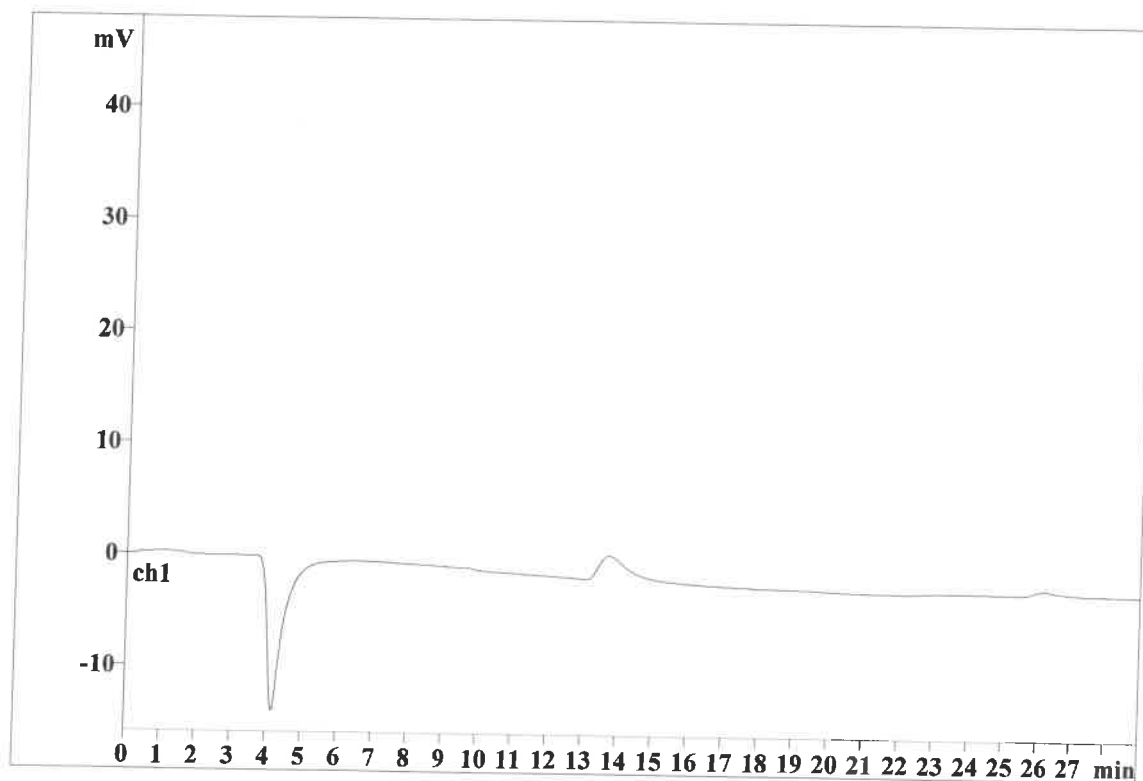

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:07:54 PM
Printed by: wet


Ident: LB127682BLW
Analysis from: 10/6/2023 12:58:02 AM
File: _2023-10-06_

Last save: 10/10/2023 3:07:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35894

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

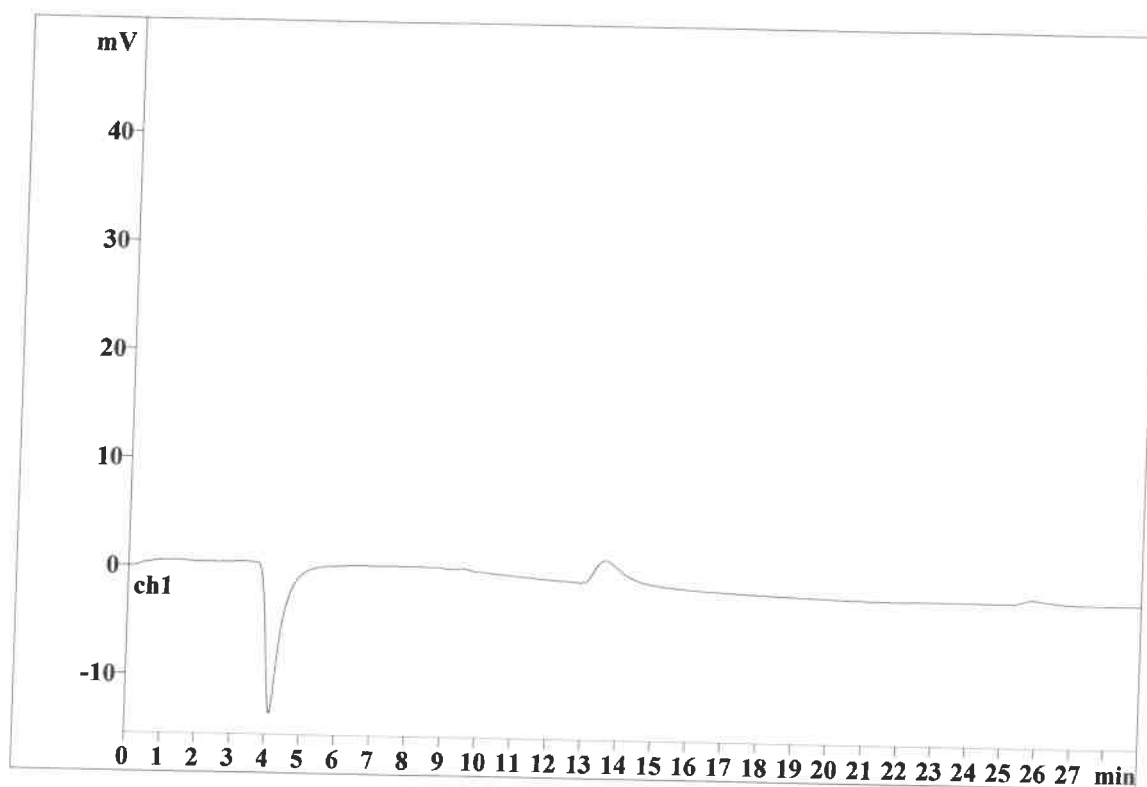

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:08:02 PM
Printed by: wet


Ident: LB127682BSW
Analysis from: 10/6/2023 1:29:40 AM
File: _2023-10-06_

Last save: 10/10/2023 3:07:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35895

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

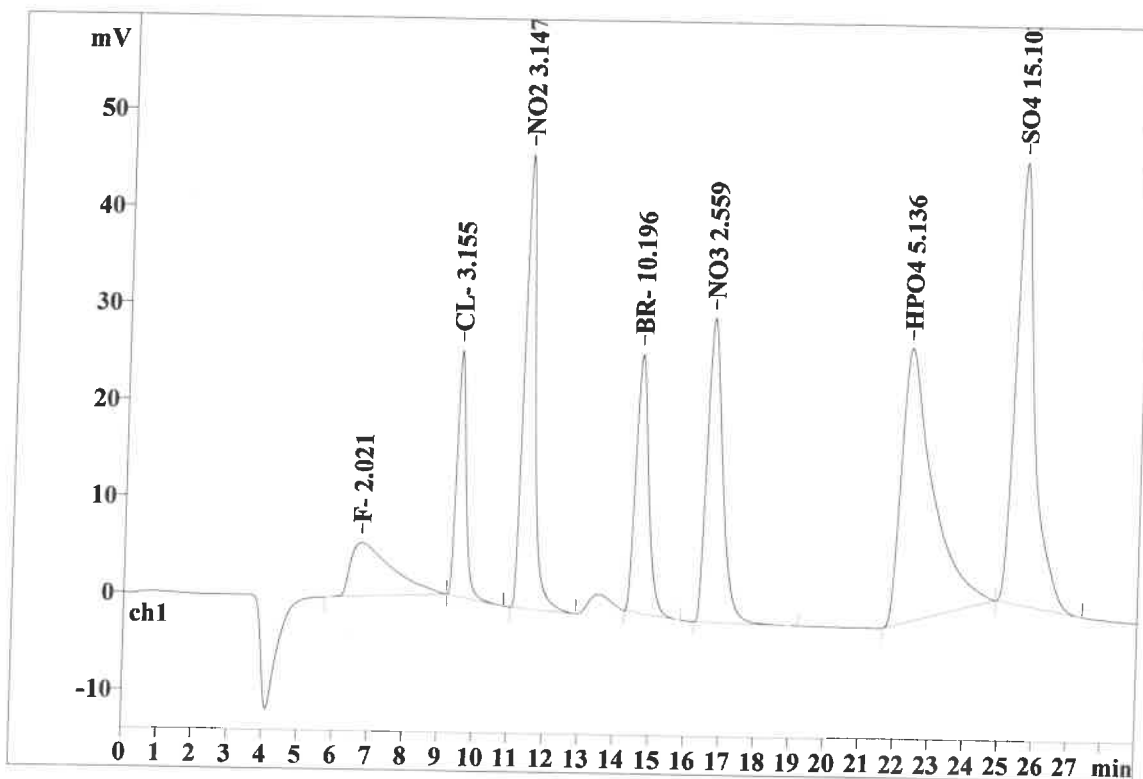

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.73	1.253	5.55	2.64	454.126	6.33
2	9.50	0.274	25.40	12.10	464.189	6.47
3	11.37	0.335	46.91	22.34	1057.760	14.74
4	14.62	0.386	26.71	12.72	674.367	9.40
5	16.63	0.472	31.45	14.97	975.399	13.60
6	22.32	0.893	28.32	13.48	1795.038	25.02
7	25.50	0.533	45.66	21.74	1752.933	24.44
7	29.00	0.592	209.99	100.00	7173.811	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:54:29 PM
Printed by: wet


Ident: 04723-01
Analysis from: 10/6/2023 2:01:23 AM
File: _2023-10-06_

Last save: 10/6/2023 2:30:23 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35896

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

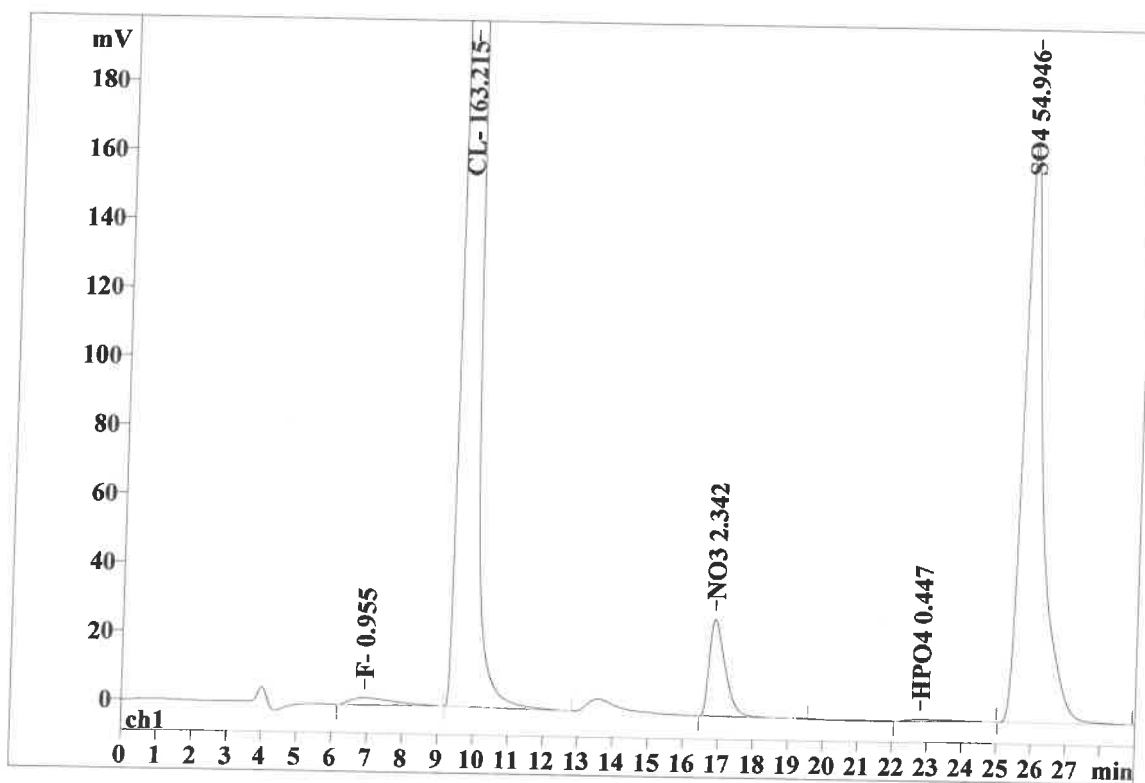

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.91	1.368	2.11	0.14	182.528	0.55
2	9.63	0.293	1276.87	86.50	25384.017	76.52
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.87	0.485	28.12	1.90	888.176	2.68
6	22.80	1.378	0.62	0.04	52.690	0.16
7	25.76	0.544	168.50	11.41	6665.729	20.09
7	29.00	0.581	1476.22	100.00	33173.140	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:54:40 PM
Printed by: wet


Ident: O4723-01MS
Analysis from: 10/6/2023 2:33:01 AM
File: _2023-10-06_

Last save: 10/6/2023 3:02:01 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35897

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

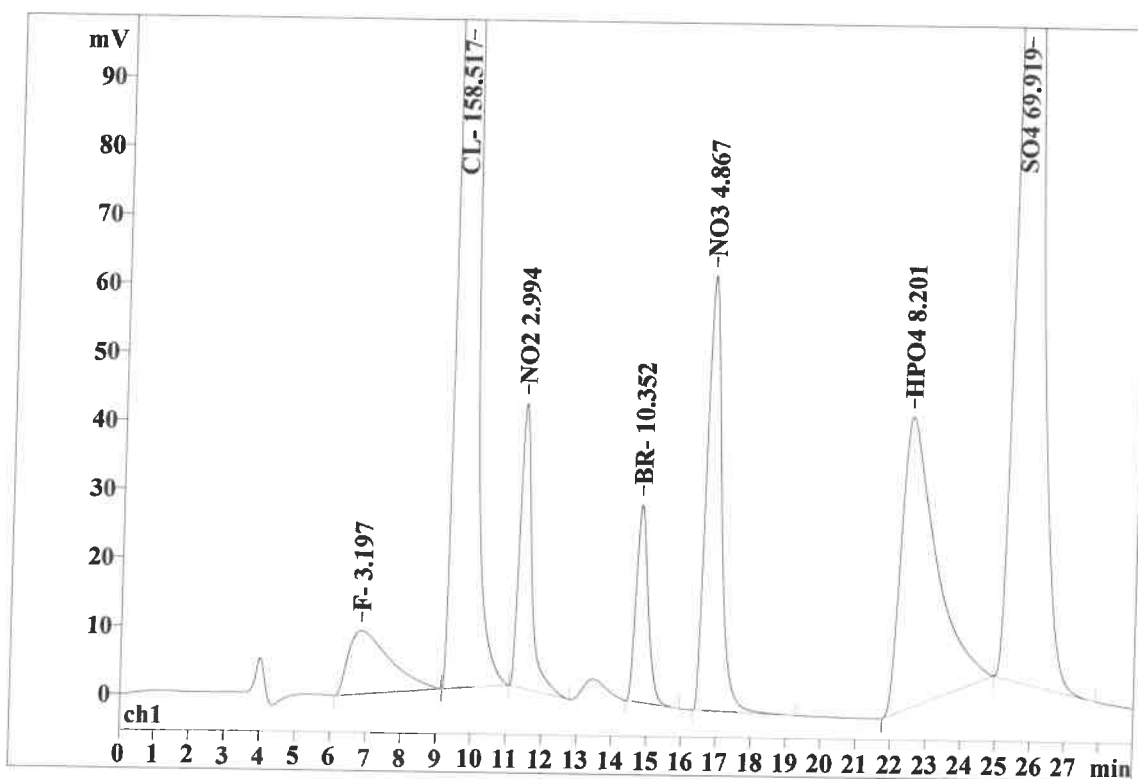

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.84	1.273	9.24	0.55	753.694	1.86
2	9.58	0.287	1279.32	75.98	24652.600	60.95
3	11.40	0.348	41.48	2.46	1003.468	2.48
4	14.75	0.365	28.82	1.71	685.353	1.69
5	16.72	0.460	63.32	3.76	1906.289	4.71
6	22.45	1.008	42.54	2.53	2933.898	7.25
7	25.58	0.552	218.97	13.01	8511.948	21.04
7	29.00	0.613	1683.71	100.00	40447.249	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:54:48 PM
Printed by: wet


Ident: O4723-01MSD
Analysis from: 10/6/2023 3:04:39 AM
File: _2023-10-06_

Last save: 10/6/2023 3:33:39 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35898

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

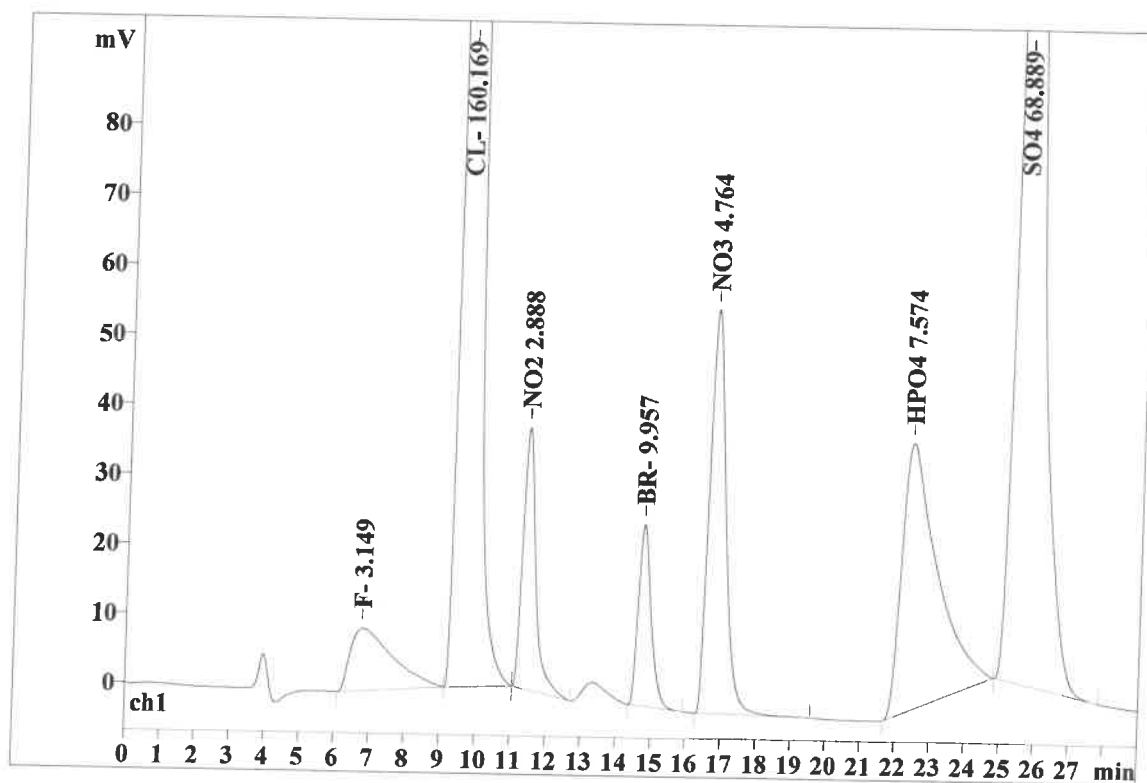

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.77	1.300	8.94	0.55	741.396	1.84
2	9.56	0.293	1256.09	76.80	24909.749	61.93
3	11.38	0.378	37.44	2.29	965.690	2.40
4	14.72	0.385	26.02	1.59	657.531	1.63
5	16.68	0.494	57.80	3.53	1864.791	4.64
6	22.38	1.039	38.37	2.35	2700.793	6.71
7	25.49	0.552	210.96	12.90	8384.983	20.85
7	29.00	0.634	1635.63	100.00	40224.933	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:55:06 PM
Printed by: wet


Ident: 04723-02
Analysis from: 10/6/2023 3:36:17 AM
File: _2023-10-06_

Last save: 10/6/2023 4:05:17 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35899

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

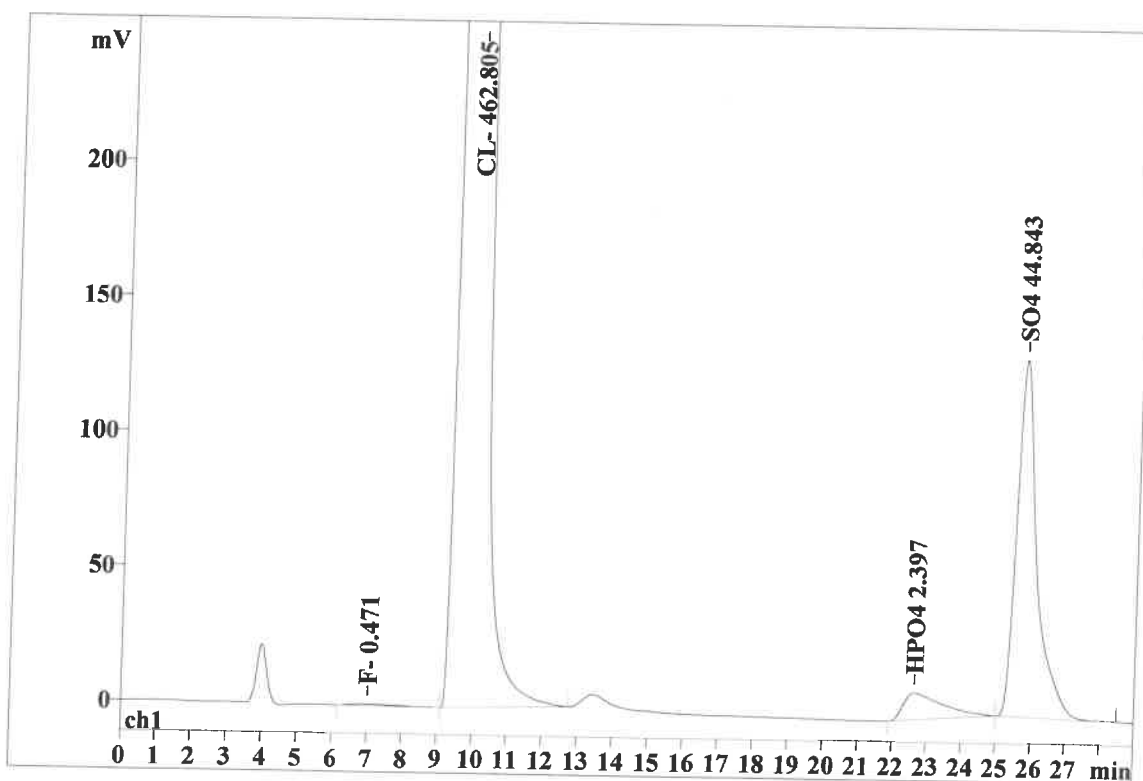

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	7.00	1.502	0.64	0.04	59.333	0.08
2	9.95	0.732	1625.87	91.93	72027.289	92.01
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	22.65	1.223	9.86	0.56	777.253	0.99
7	25.69	0.563	132.09	7.47	5420.116	6.92
7	29.00	0.574	1768.47	100.00	78283.991	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:55:17 PM
Printed by: wet


Ident: O4723-03
Analysis from: 10/6/2023 4:07:55 AM
File: _2023-10-06_

Last save: 10/6/2023 10:33:12 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35900

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 31
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

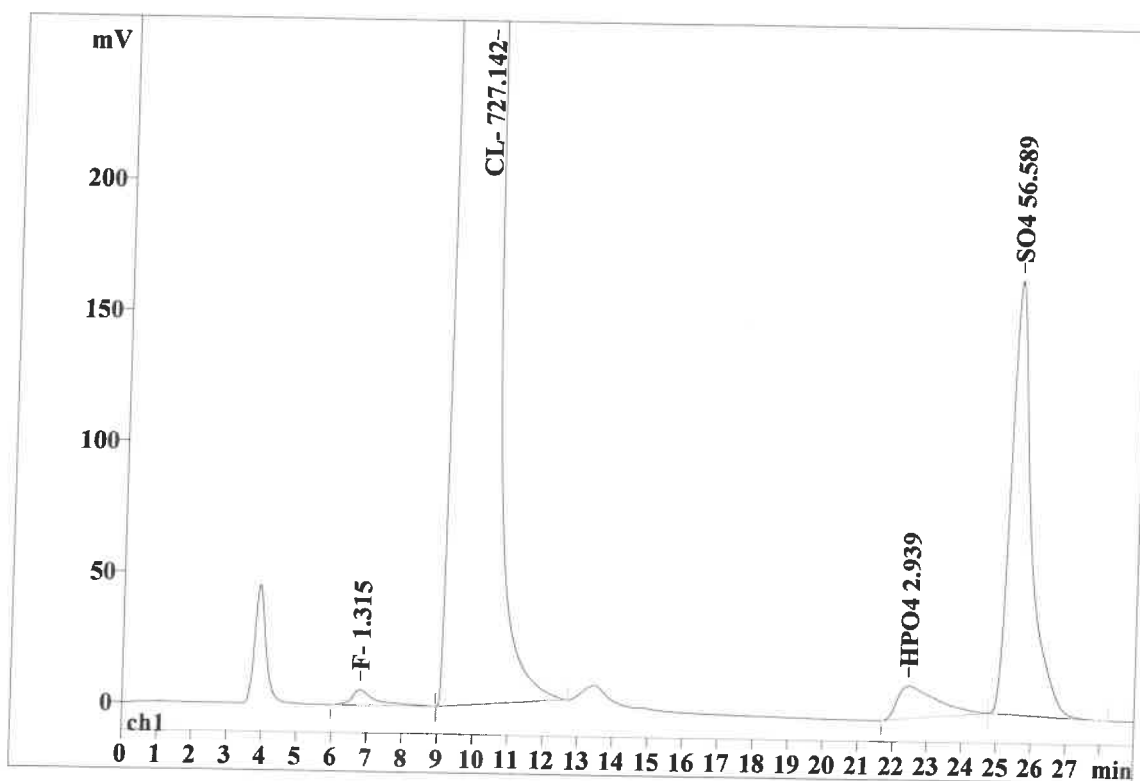

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.78	0.539	5.95	0.32	274.339	0.23
2	10.15	1.131	1676.02	90.11	113182.082	93.30
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	22.44	1.227	12.42	0.67	978.798	0.81
7	25.46	0.573	165.52	8.90	6868.390	5.66
7	29.00	0.496	1859.91	100.00	121303.609	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:55:27 PM
Printed by: wet


Ident: 04723-04
Analysis from: 10/6/2023 4:39:33 AM
File: _2023-10-06_

Last save: 10/6/2023 5:08:33 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35901

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 32
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

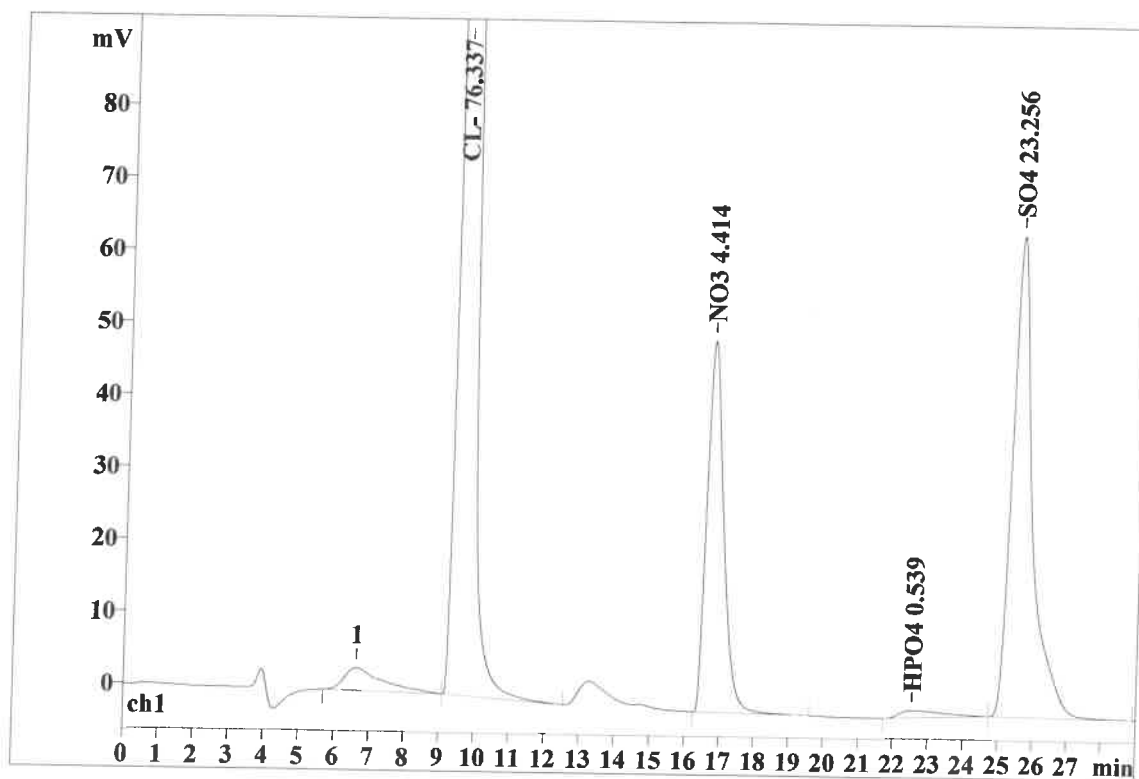

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.50	0.283	614.10	83.44	11857.896	71.15
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.67	0.514	51.28	6.97	1723.387	10.34
6	22.54	1.383	1.01	0.14	86.916	0.52
7	25.47	0.563	66.42	9.02	2758.295	16.55
7	29.00	0.392	732.82	99.57	16426.494	98.56

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:55:38 PM
Printed by: wet


Ident: 04724-01
Analysis from: 10/6/2023 5:11:10 AM
File: _2023-10-06_

Last save: 10/6/2023 5:40:10 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35902

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 33
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

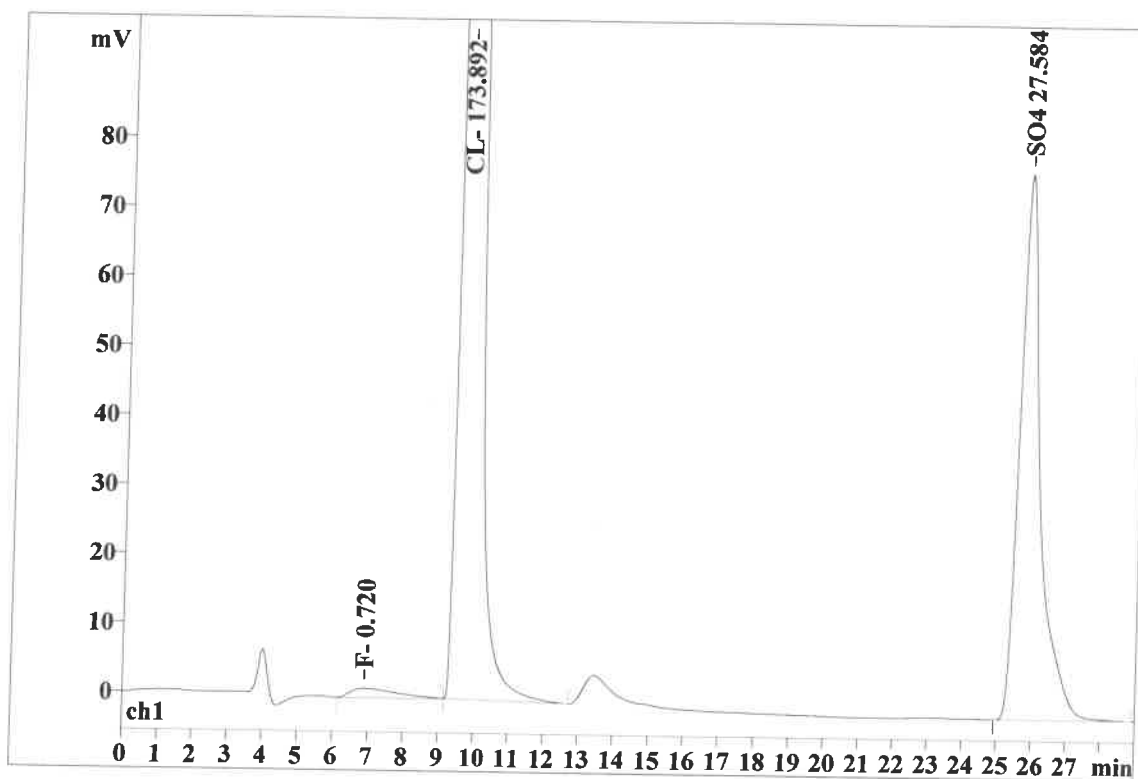

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.89	1.435	1.36	0.10	122.685	0.40
2	9.63	0.315	1266.41	94.06	27046.301	88.79
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.70	0.566	78.56	5.83	3292.000	10.81
7	29.00	0.331	1346.33	100.00	30460.986	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:55:50 PM
Printed by: wet


Ident: O4724-02
Analysis from: 10/6/2023 5:42:48 AM
File: _2023-10-06_

Last save: 10/6/2023 6:11:48 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35903

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 34
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

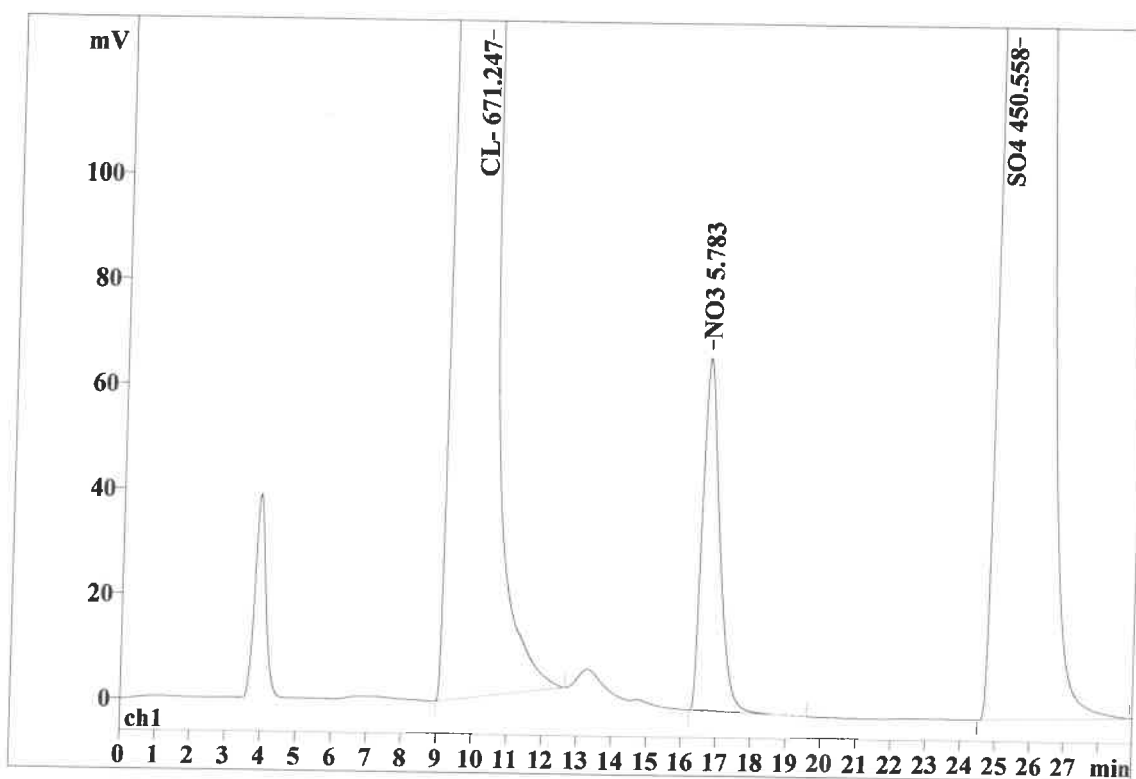

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	10.09	1.058	1670.43	57.42	104479.867	64.41
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.64	0.521	67.07	2.31	2275.371	1.40
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.19	0.672	1171.66	40.27	55445.354	34.18
7	29.00	0.322	2909.16	100.00	162200.592	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:00 PM
Printed by: wet


Ident: CCV
Analysis from: 10/6/2023 6:46:21 AM
File: _2023-10-06_

Last save: 10/6/2023 7:15:21 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35905

Last save: 10/3/2023 9:33:

SAMPLE:
:
Vial number: 37
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

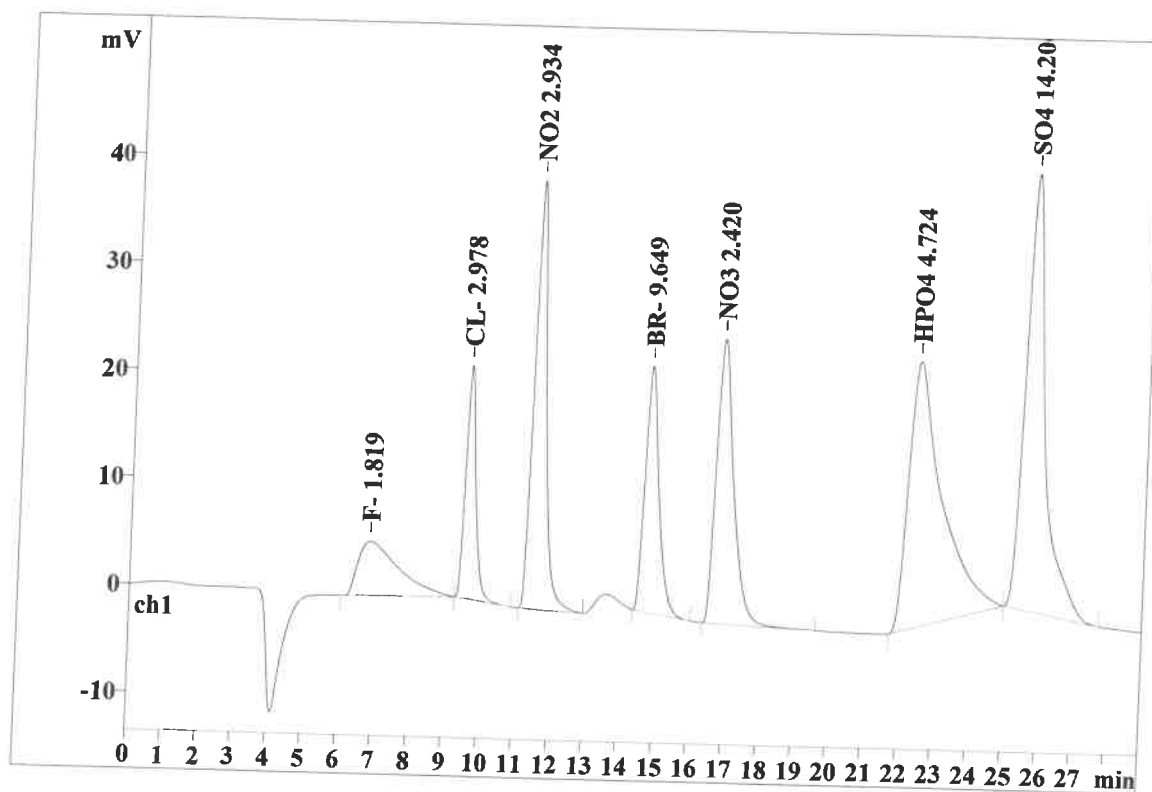

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.84	1.224	5.05	2.78	402.675	6.05
2	9.56	0.299	21.72	11.98	436.627	6.55
3	11.45	0.363	39.85	21.98	982.207	14.75
4	14.73	0.418	22.88	12.62	635.899	9.55
5	16.78	0.522	26.46	14.60	919.400	13.80
6	22.40	0.914	24.75	13.65	1641.688	24.65
7	25.61	0.546	40.61	22.40	1642.497	24.66
7	29.00	0.612	181.31	100.00	6660.992	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:07 PM
Printed by: wet


Ident: CCB
Analysis from: 10/6/2023 7:18:08 AM
File: _2023-10-06_

Last save: 10/6/2023 7:47:08 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35906

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

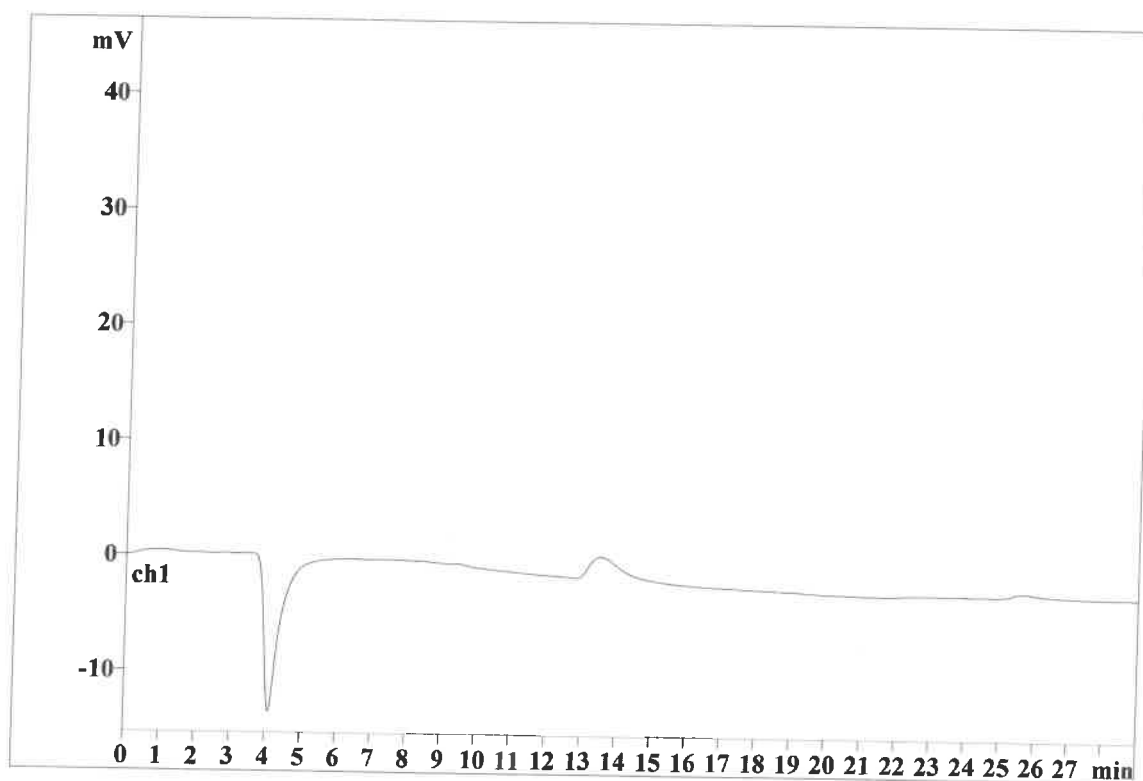

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:15 PM
Printed by: wet


Ident: O4724-03
Analysis from: 10/6/2023 7:49:53 AM
File: _2023-10-06_

Last save: 10/6/2023 8:18:54 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35907

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 35
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

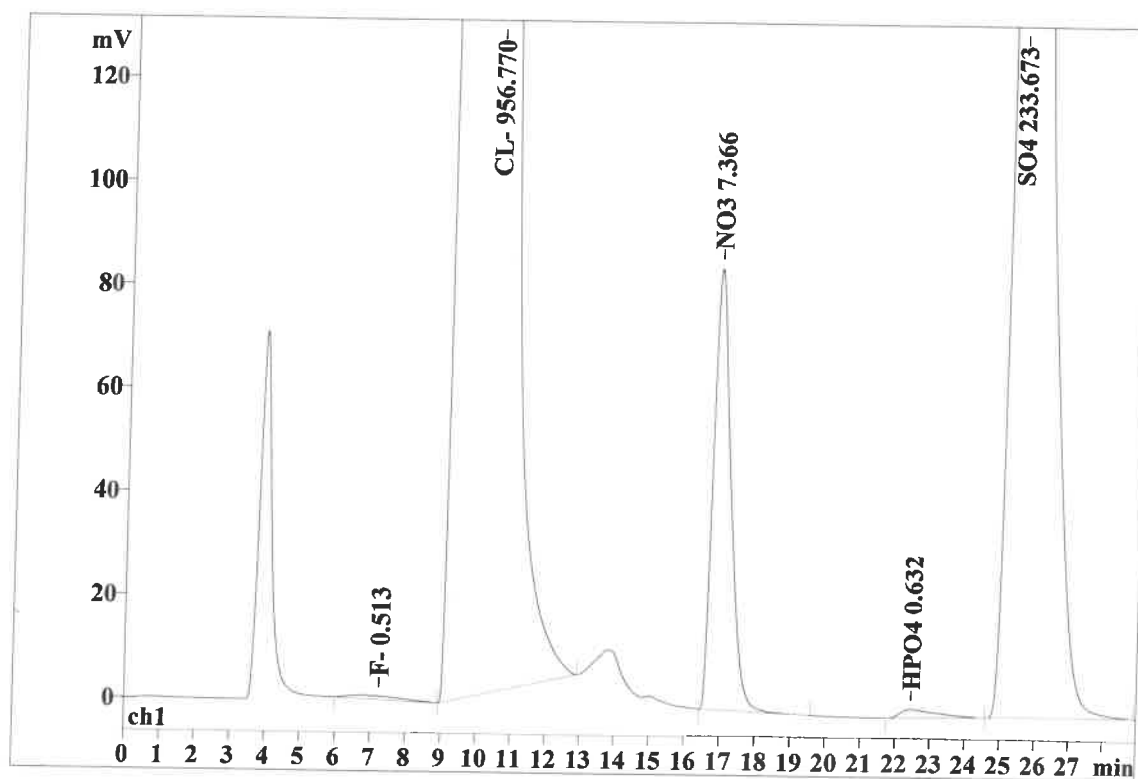

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	7.24	1.722	0.68	0.03	69.931	0.04
2	10.42	1.483	1696.10	70.03	148932.980	82.40
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.83	0.528	85.13	3.51	2913.781	1.61
6	22.45	1.142	1.66	0.07	121.391	0.07
7	25.41	0.618	638.49	26.36	28703.111	15.88
7	29.00	0.785	2422.06	100.00	180741.194	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:22 PM
Printed by: wet


Ident: 04724-04
Analysis from: 10/6/2023 8:21:32 AM
File: _2023-10-06_

Last save: 10/6/2023 8:50:32 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35908

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 36
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

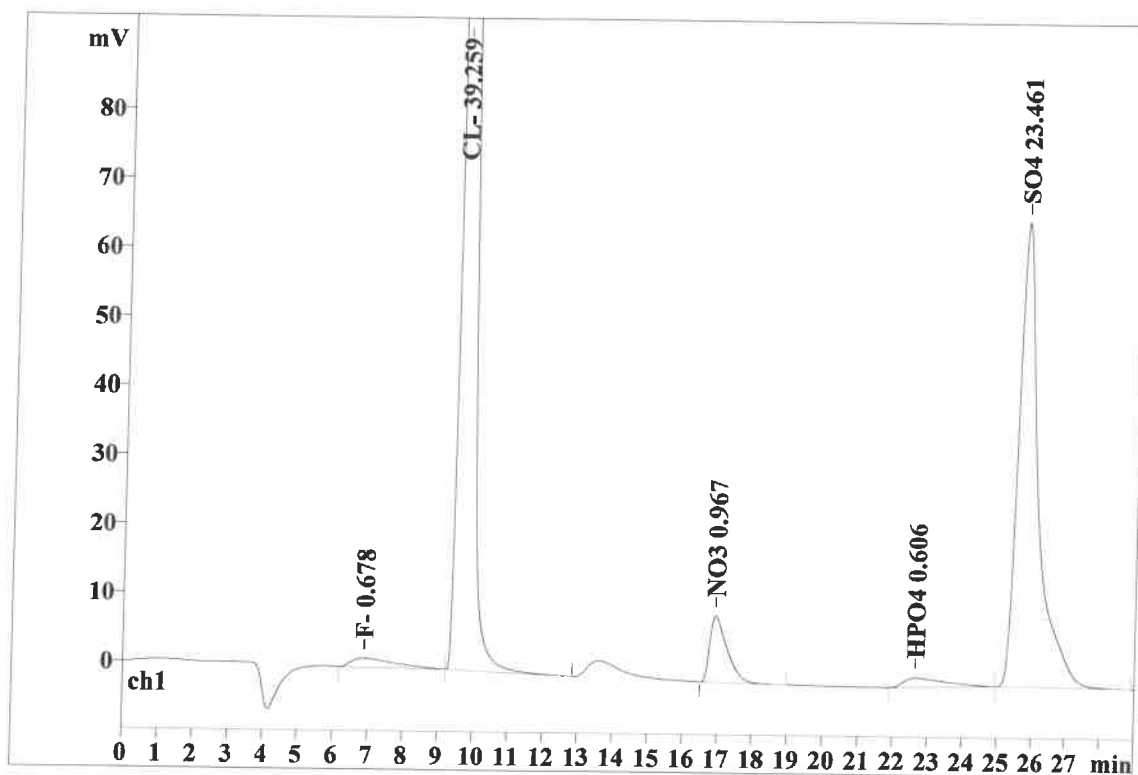

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.88	1.326	1.32	0.33	111.953	1.19
2	9.59	0.275	317.11	79.96	6085.284	64.56
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.92	0.525	9.60	2.42	333.571	3.54
6	22.64	1.312	1.35	0.34	111.889	1.19
7	25.69	0.553	67.17	16.94	2783.631	29.53
7	29.00	0.570	396.54	100.00	9426.328	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:29 PM
Printed by: wet


Ident: CCV
Analysis from: 10/6/2023 8:53:17 AM
File: _2023-10-06_

Last save: 10/6/2023 9:56:31 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35909

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

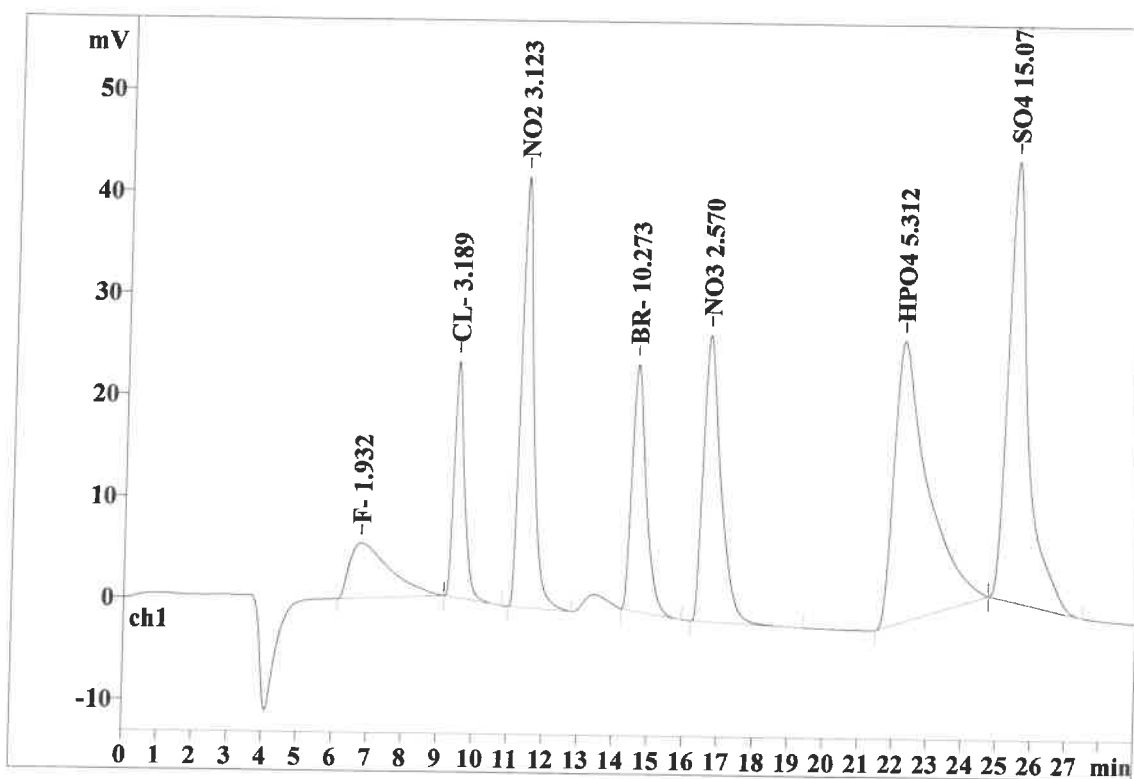

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.75	1.220	5.43	2.80	431.400	5.98
2	9.46	0.299	23.22	11.95	469.545	6.50
3	11.33	0.365	42.33	21.79	1049.028	14.53
4	14.57	0.421	24.28	12.49	679.801	9.42
5	16.60	0.524	28.13	14.47	979.815	13.57
6	22.17	0.930	27.70	14.25	1860.368	25.77
7	25.35	0.547	43.22	22.24	1749.208	24.23
7	29.00	0.615	194.31	99.99	7219.167	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:39 PM
Printed by: wet


Ident: CCB
Analysis from: 10/6/2023 9:24:57 AM
File: _2023-10-06_

Last save: 10/6/2023 9:53:57 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35910

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

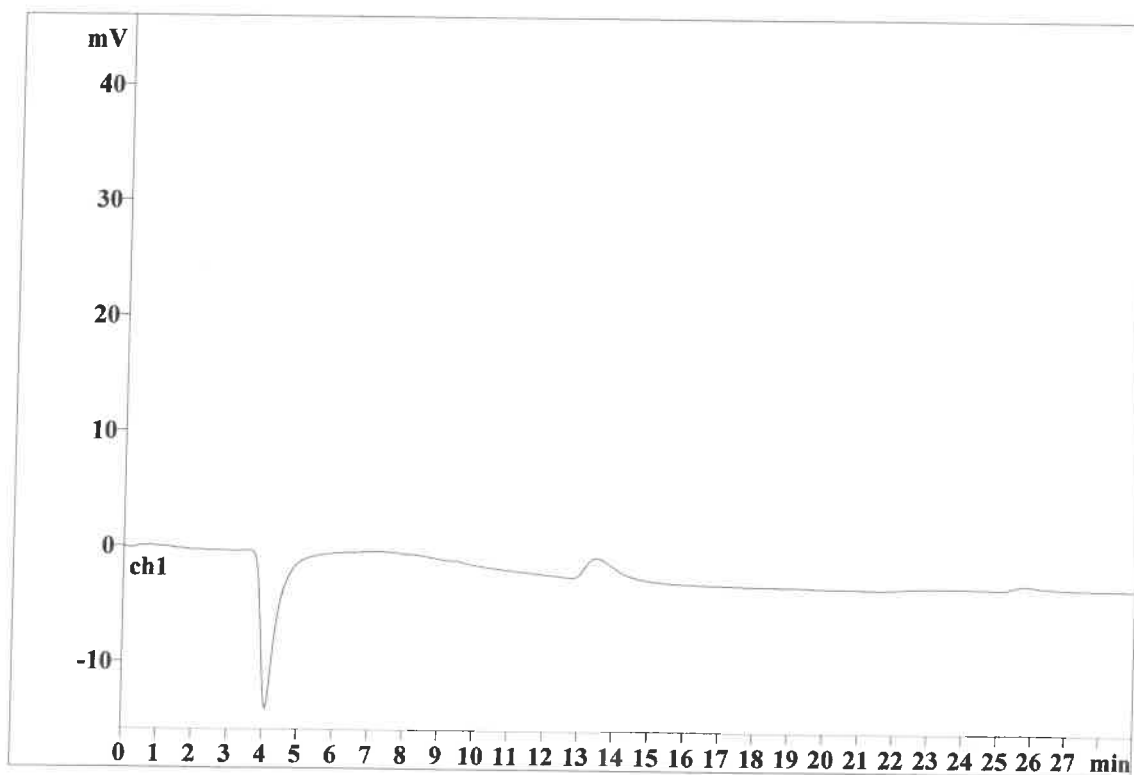

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:49 PM
Printed by: wet


Ident: LB127682BLW2
Analysis from: 10/6/2023 9:56:36 AM
File: _2023-10-06_

Last save: 10/10/2023 3:07:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35911

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

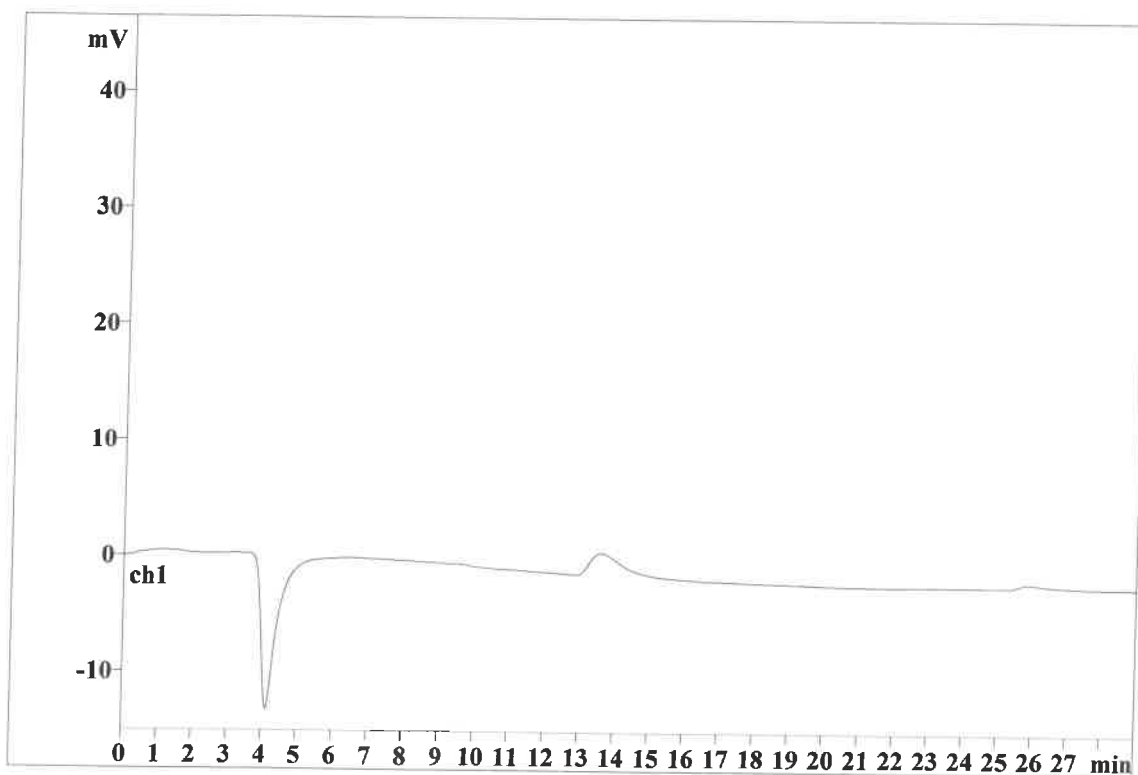

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:56:55 PM
Printed by: wet


Ident: LB127682BSW2
Analysis from: 10/6/2023 10:28:15 AM
File: _2023-10-06_

Last save: 10/10/2023 3:07:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35912

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

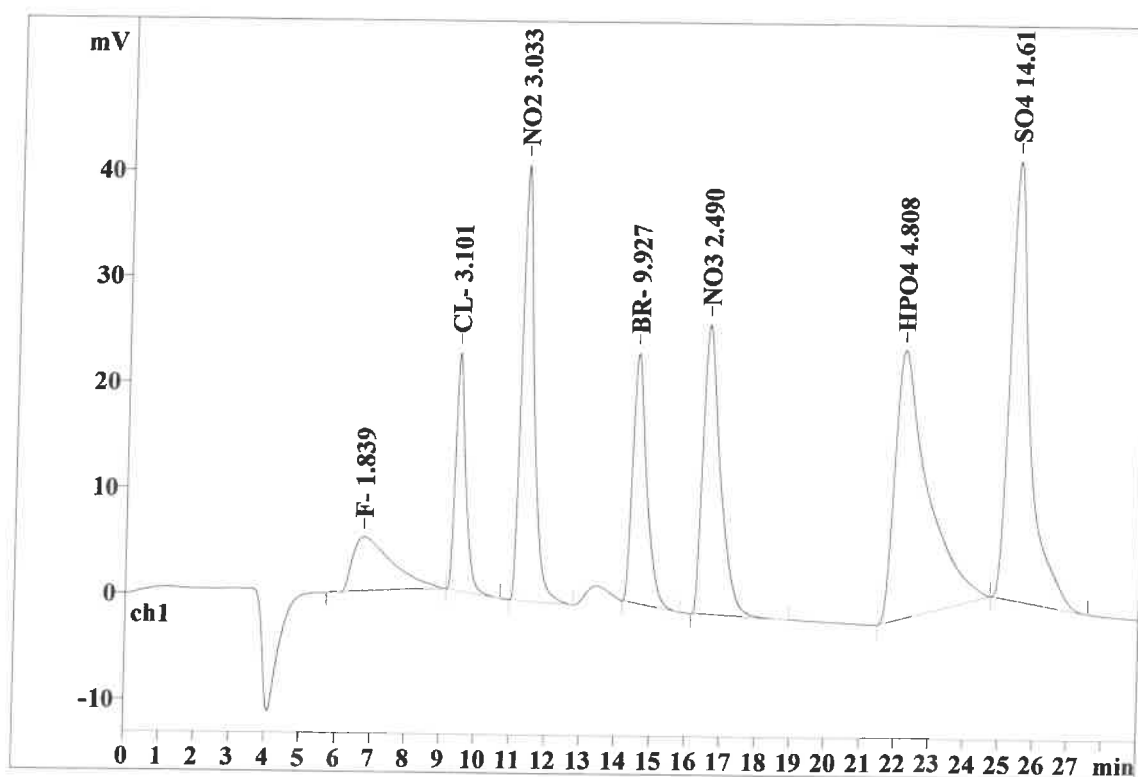

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.74	1.211	5.16	2.77	407.659	5.95
2	9.43	0.298	22.48	12.05	455.738	6.65
3	11.29	0.362	41.13	22.04	1017.261	14.85
4	14.52	0.416	23.60	12.64	655.469	9.57
5	16.53	0.517	27.39	14.67	947.471	13.83
6	22.15	0.899	25.40	13.61	1673.117	24.43
7	25.36	0.549	41.49	22.23	1692.390	24.71
7	29.00	0.607	186.65	100.00	6849.105	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:58:47 PM
Printed by: wet


Ident: LB127682BSW2
Analysis from: 10/6/2023 10:28:15 AM
File: _2023-10-06_

Last save: 10/10/2023 3:07:18 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35912

Last save: 10/3/2023 9:33:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

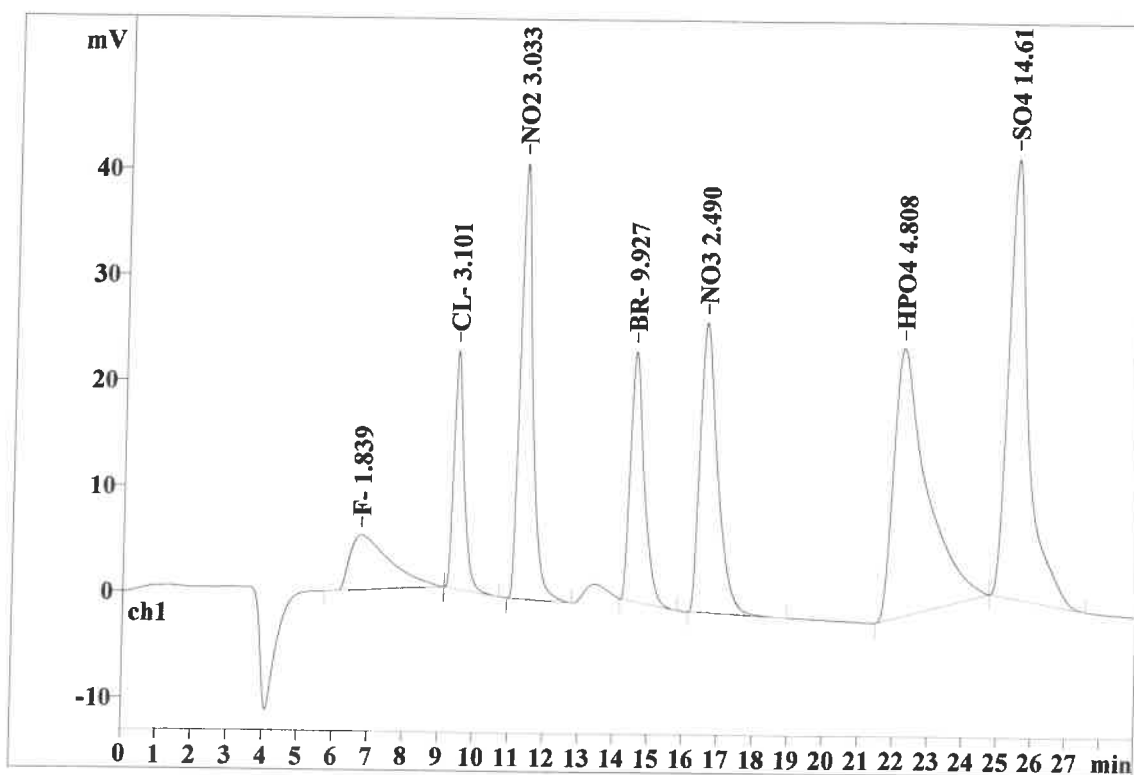

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.74	1.211	5.16	2.77	407.659	5.95
2	9.43	0.298	22.48	12.05	455.738	6.65
3	11.29	0.362	41.13	22.04	1017.261	14.85
4	14.52	0.416	23.60	12.64	655.469	9.57
5	16.53	0.517	27.39	14.67	947.471	13.83
6	22.15	0.899	25.40	13.61	1673.117	24.43
7	25.36	0.549	41.49	22.23	1692.390	24.71
7	29.00	0.607	186.65	100.00	6849.105	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:58:58 PM
Printed by: wet


Ident: 04723-01DLX2
Analysis from: 10/6/2023 11:00:01 AM
File: _2023-10-06_

Last save: 10/6/2023 11:29:01 AM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35913

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 38
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

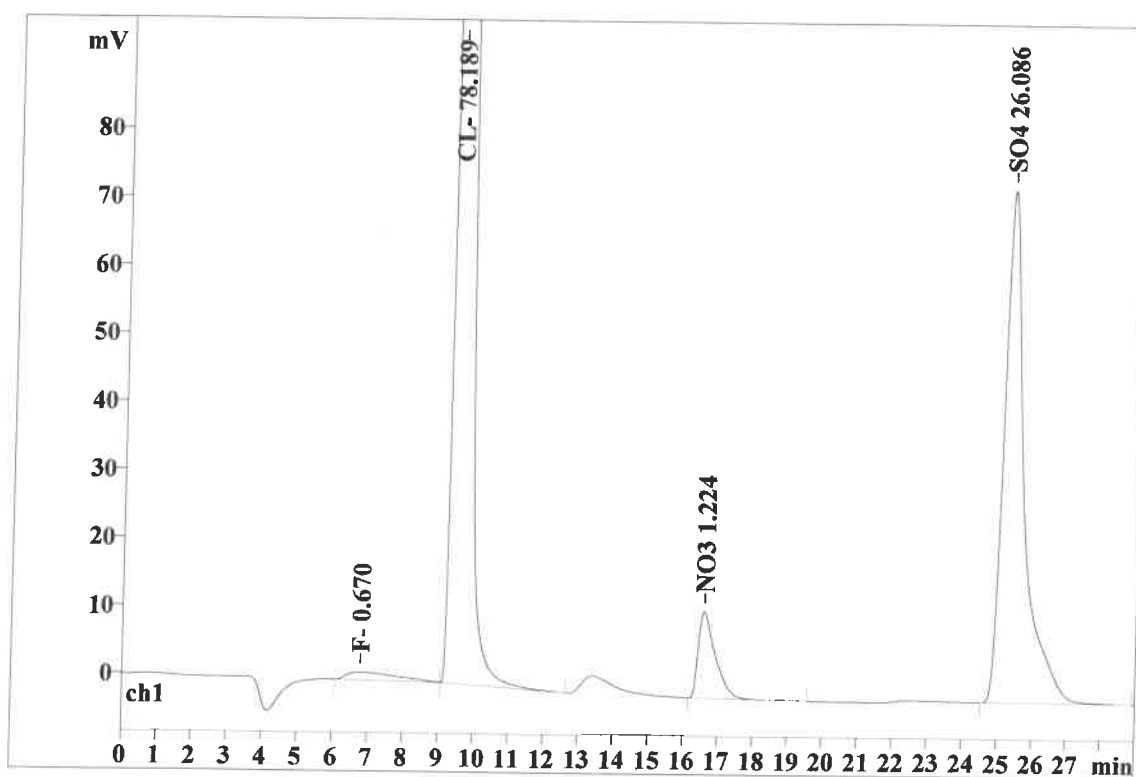

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.80	1.604	1.12	0.15	109.875	0.70
2	9.45	0.266	650.39	87.97	12146.319	76.87
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.58	0.513	12.68	1.72	436.987	2.77
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.26	0.548	75.09	10.16	3107.350	19.67
7	29.00	0.419	739.28	99.99	15800.532	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:59:06 PM
Printed by: wet


Ident: 04723-02DLX2
Analysis from: 10/6/2023 11:31:39 AM
File: _2023-10-06_

Last save: 10/6/2023 12:00:39 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35914

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 39
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

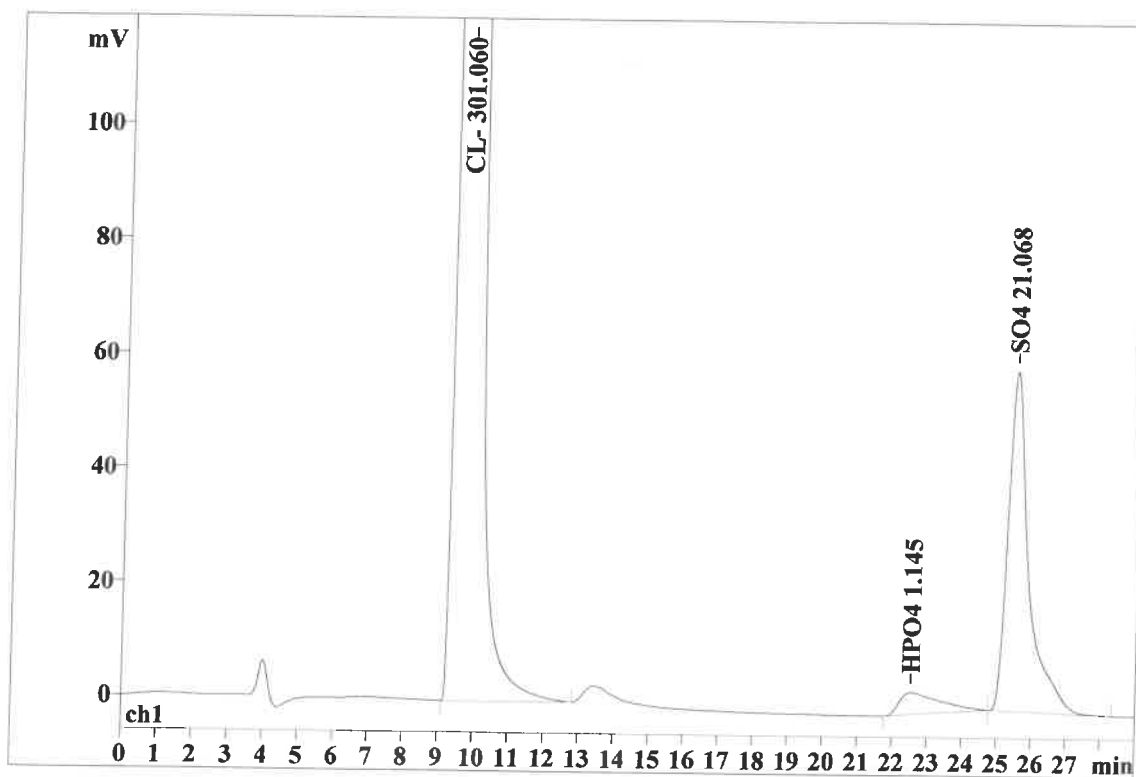

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.72	0.485	1536.38	96.05	46845.226	94.36
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	22.53	1.302	3.82	0.24	312.106	0.63
7	25.44	0.558	59.31	3.71	2488.618	5.01
7	29.00	0.335	1599.50	100.00	49645.950	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:59:14 PM
Printed by: wet


Ident: O4723-03DLX2
Analysis from: 10/6/2023 12:03:17 PM
File: _2023-10-06_

Last save: 10/6/2023 12:32:17 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35915

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 40
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

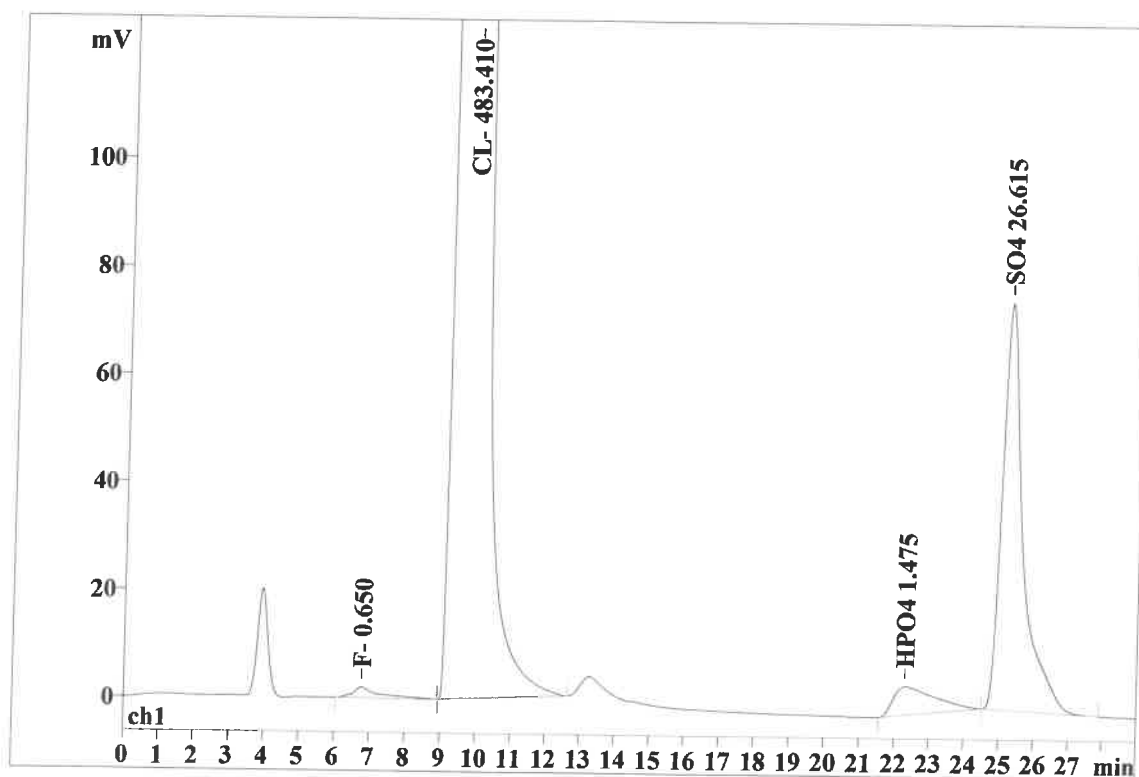

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.77	0.515	2.02	0.12	104.933	0.13
2	9.81	0.771	1630.58	95.17	75235.373	95.30
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	22.30	1.321	5.29	0.31	434.786	0.55
7	25.18	0.560	75.45	4.40	3172.482	4.02
7	29.00	0.452	1713.34	100.00	78947.574	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:59:21 PM
Printed by: wet


Ident: O4724-02DLX20
Analysis from: 10/6/2023 12:34:55 PM
File: _2023-10-06_

Last save: 10/6/2023 1:03:55 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35916

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 41
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

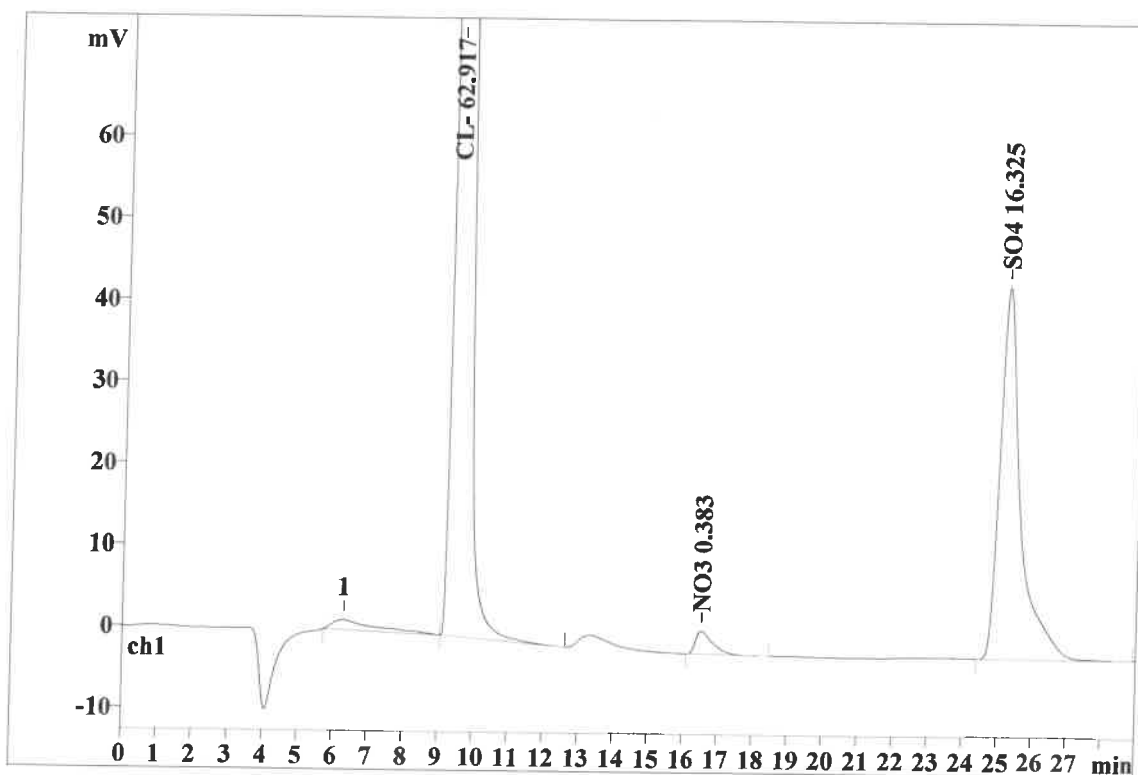

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.42	0.256	536.88	91.55	9768.492	82.25
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.52	0.513	2.84	0.48	97.954	0.82
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.17	0.552	45.45	7.75	1903.716	16.03
7	29.00	0.189	585.17	99.78	11770.162	99.10

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 3:59:40 PM
 Printed by: wet


Ident: O4724-03DLX2
 Analysis from: 10/6/2023 1:06:33 PM
 File: _2023-10-06_

Last save: 10/10/2023 3:59:38 PM

Method: AnionsIC2-091323.mtw
 Run operator: wet
 Analysis number: 35917

Last save: 10/6/2023 9:56:

SAMPLE:
 : IZ/MA
 Vial number: 42
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

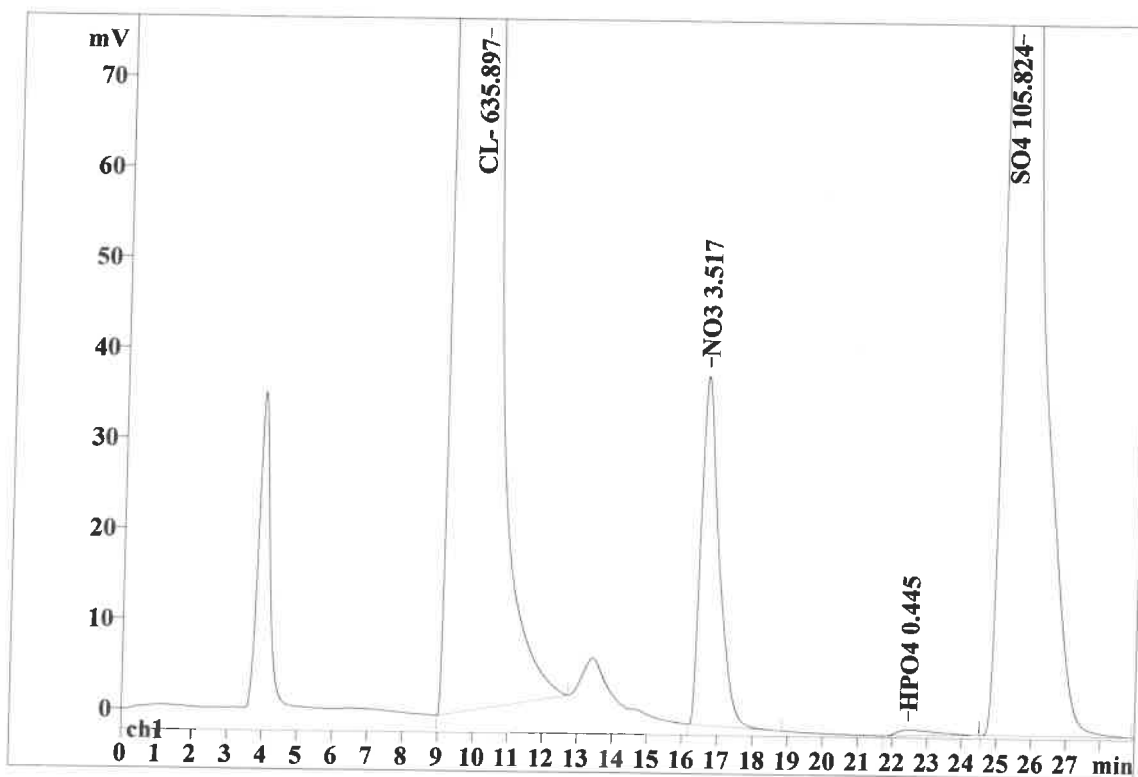

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	10.04	1.006	1662.85	82.97	98976.139	87.34
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.58	0.530	38.61	1.93	1361.945	1.20
6	22.45	1.286	0.65	0.03	51.991	0.05
7	25.31	0.571	302.03	15.07	12939.061	11.42
7	29.00	0.485	2004.16	100.00	113329.137	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 10/10/2023 4:00:25 PM
Printed by: wet


Ident: O4724-03DL2X10
Analysis from: 10/6/2023 1:38:11 PM
File: _2023-10-06_

Last save: 10/10/2023 4:00:22 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35918

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 43
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

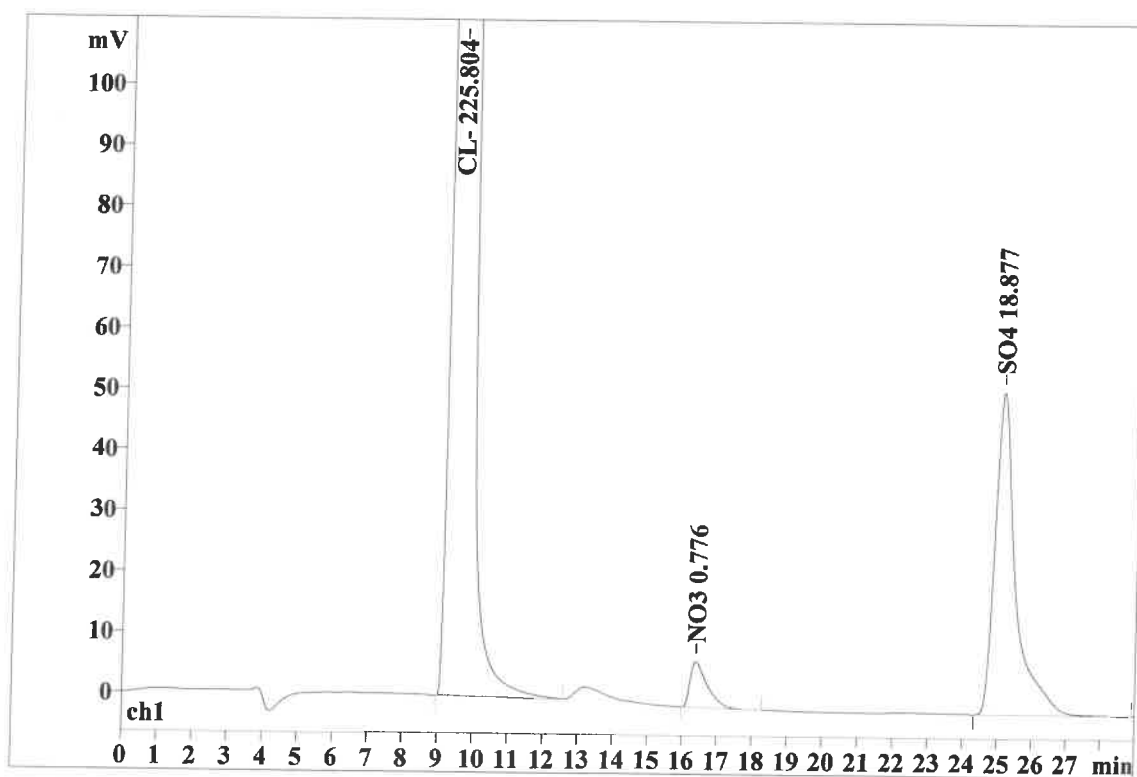

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.49	0.368	1444.78	95.98	35128.553	93.42
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.38	0.505	7.52	0.50	256.498	0.68
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.06	0.550	52.96	3.52	2218.399	5.90
7	29.00	0.203	1505.27	100.00	37603.450	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 4:00:33 PM
Printed by: wet


Ident: CCV
Analysis from: 10/6/2023 2:09:56 PM
File: _2023-10-06_

Last save: 10/6/2023 2:54:41 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35919

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

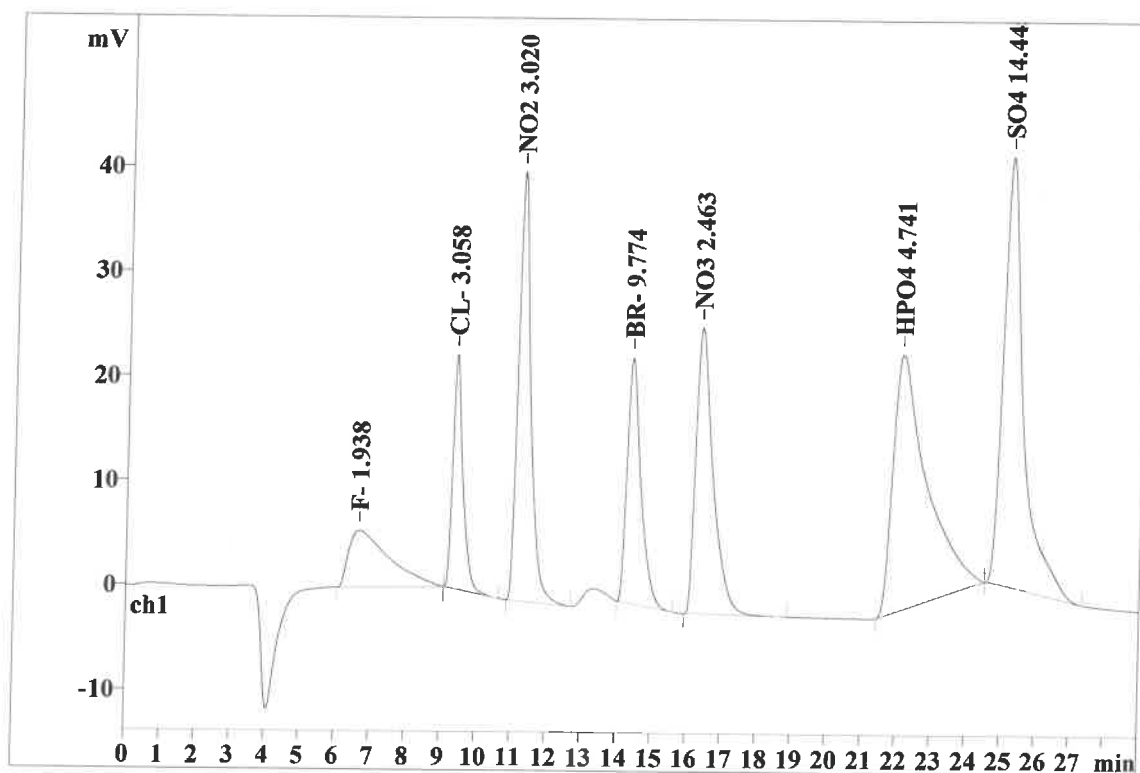

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.66	1.221	5.44	2.94	433.038	6.37
2	9.37	0.291	22.40	12.10	449.058	6.61
3	11.20	0.358	40.98	22.13	1012.757	14.90
4	14.37	0.408	23.44	12.66	644.707	9.49
5	16.34	0.504	27.34	14.77	936.878	13.78
6	22.09	0.933	24.48	13.22	1648.221	24.25
7	25.15	0.547	41.09	22.19	1671.904	24.60
7	29.00	0.609	185.16	100.00	6796.564	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/10/2023 4:00:40 PM
Printed by: wet


Ident: CCB
Analysis from: 10/6/2023 2:41:33 PM
File: _2023-10-06_

Last save: 10/6/2023 3:10:33 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 35920

Last save: 10/6/2023 9:56:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

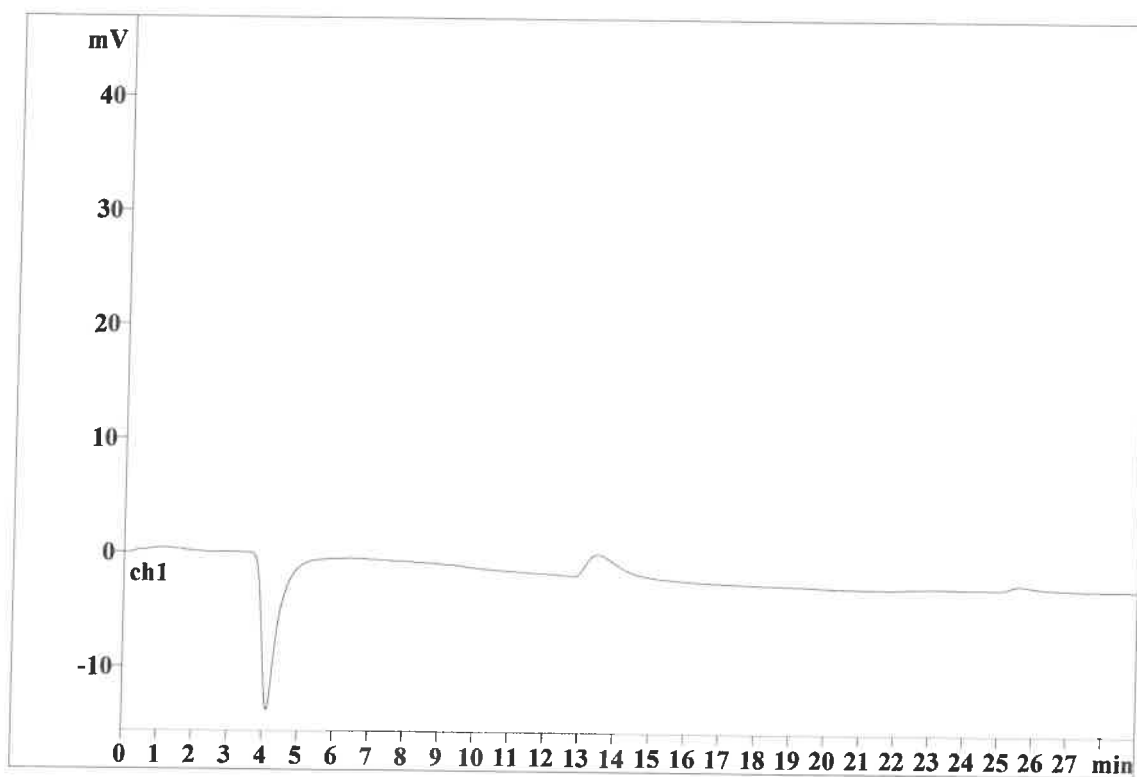

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD