


LB127694

SFAM01.1

INSTRUMENT-15: CV1

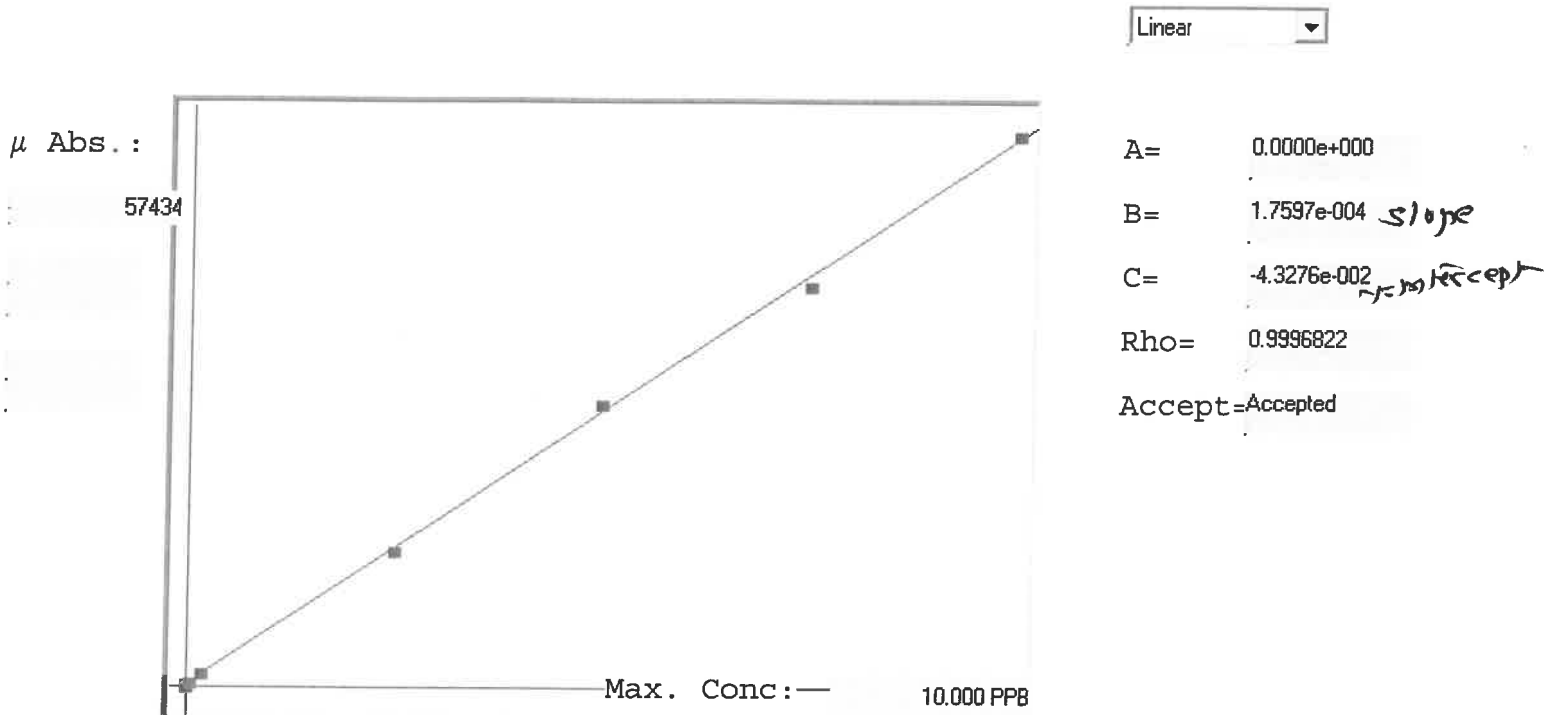

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.023	-0.023	113	0.000	113					18
0.05	0.050	0.059	0.009	581	0.0 %	581	0				7
0.20	0.200	0.214	0.014	1463	0.0 %	1463					1
2.50	2.500	2.471	-0.029	14286	0.0 %	14286					3
5.00	5.000	5.149	0.149	29505	0.0 %	29505					2
7.50	7.500	7.317	-0.183	41827	0.0 %	41827					1
10.0	10.000	10.064	0.064	57434	0.0 %	57434					

LB127694

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	113	-		0 SFAM01.1	PPB	10/9/2023 17:02	Std
	0.05 S01	581	-		0.05 SFAM01.1	PPB	10/9/2023 17:04	Std
	0.2 S02	1463	-		0.2 SFAM01.1	PPB	10/9/2023 17:07	Std
	2.5 S03	14286	-		2.5 SFAM01.1	PPB	10/9/2023 17:09	Std
	5 S04	29505	-		5 SFAM01.1	PPB	10/9/2023 17:11	Std
	7.5 S05	41827	-		7.5 SFAM01.1	PPB	10/9/2023 17:14	Std
	10 S06	57434	-		10 SFAM01.1	PPB	10/9/2023 17:30	Std
ICV005	ICV005	22972	3.9992 -		SFAM01.1	PPB	10/9/2023 17:33	SMPL
ICB005	ICB005	91	-0.0273 -		SFAM01.1	PPB	10/9/2023 17:35	SMPL
CCV053	CCV053	27964	4.8776 -		SFAM01.1	PPB	10/9/2023 17:37	SMPL
CCB053	CCB053	68	-0.0313 -		SFAM01.1	PPB	10/9/2023 17:40	SMPL
PB156251BL	PBW251	93	-0.0269 -		SFAM01.1	PPB	10/9/2023 17:42	SMPL
O4776-01	EXEQ4	242	-0.0007 -		SFAM01.1	PPB	10/9/2023 17:44	SMPL
O4776-02	EXEQ5	74	-0.0303 -		SFAM01.1	PPB	10/9/2023 17:46	SMPL
O4776-03	EXEQ7	82	-0.0288 -		SFAM01.1	PPB	10/9/2023 17:49	SMPL
O4776-04	EXEQ7D	111	-0.0237 -		SFAM01.1	PPB	10/9/2023 17:51	SMPL
O4776-05	EXEQ7S	6144	1.0379 -		SFAM01.1	PPB	10/9/2023 17:53	SMPL
CCV054	CCV054	28476	4.9677 -		SFAM01.1	PPB	10/9/2023 17:55	SMPL
CCB054	CCB054	50	-0.0345 -		SFAM01.1	PPB	10/9/2023 17:58	SMPL