

Clear table

Instrument ID: IC-2											Analyst :	IZ	Method:	300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 11:34		IZ/MA				
STD2	0.4370	0.6640	0.6720	2.2480	0.5650	0.9910	3.5010	2023-09-13_	9/13/23 12:04		IZ/MA				
STD3	0.8560	1.1860	1.1800	3.9540	0.9900	1.9910	5.9710	2023-09-13_	9/13/23 12:35		IZ/MA				
STD4	0.9990	1.5150	1.5110	5.0350	1.2610	2.6440	7.5340	2023-09-13_	9/13/23 13:17		IZ/MA				
STD5	1.8950	2.9390	2.9450	9.7600	2.4350	4.8490	14.4550	2023-09-13_	9/13/23 13:48		IZ/MA				
STD6	3.9370	5.9070	5.8970	19.6950	4.9130	9.9780	29.4710	2023-09-13_	9/13/23 14:19		IZ/MA				
STD7	5.0750	7.5900	7.5960	25.3080	6.3360	12.5480	38.0680	2023-09-13_	9/13/23 14:49		IZ/MA				
ICV	1.9120	2.8680	2.8940	9.5640	2.4030	5.0020	14.1400	2023-09-13_	9/13/23 15:20		IZ/MA				
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-09-13_	9/13/23 15:52		IZ/MA				
CCV	1.8040	3.0690	3.0070	9.8910	2.4450	4.7940	14.4990	2023-10-10_	10/10/23 13:08		IZ/MA				
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-10_	10/10/23 13:39		IZ/MA				
LB127741BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-10_	10/10/23 14:11		IZ/MA				
LB127741BSW	1.9960	3.2510	3.0900	10.2700	2.5960	5.0490	15.2750	2023-10-10_	10/10/23 14:43		IZ/MA				
O4821-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-10_	10/10/23 15:52		IZ/MA				
O4822-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-10_	10/10/23 16:24		IZ/MA				
O4822-02	0.0000	0.0000	0.0000	0.0000	0.2160	0.0000	0.0000	2023-10-10_	10/10/23 16:56		IZ/MA				
O4822-02MS	1.6350	2.8420	2.8050	8.9680	2.3510	3.7220	13.2720	2023-10-10_	10/10/23 17:27		IZ/MA				
O4822-02MSD	1.2460	2.2280	2.1910	6.9350	1.8580	2.7650	10.3310	2023-10-10_	10/10/23 17:59		IZ/MA				
CCV	1.9860	3.2510	3.2320	10.3580	2.6340	4.5180	15.2950	2023-10-10_	10/10/23 18:31		IZ/MA				
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-10_	10/10/23 19:34		IZ/MA				

Report date: 10/11/2023 2:43:34 PM
Printed by: wet


Ident: CCV
Analysis from: 10/10/2023 1:08:11 PM
File: _2023-10-10_

Last save: 10/11/2023 2:43:32 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36013

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

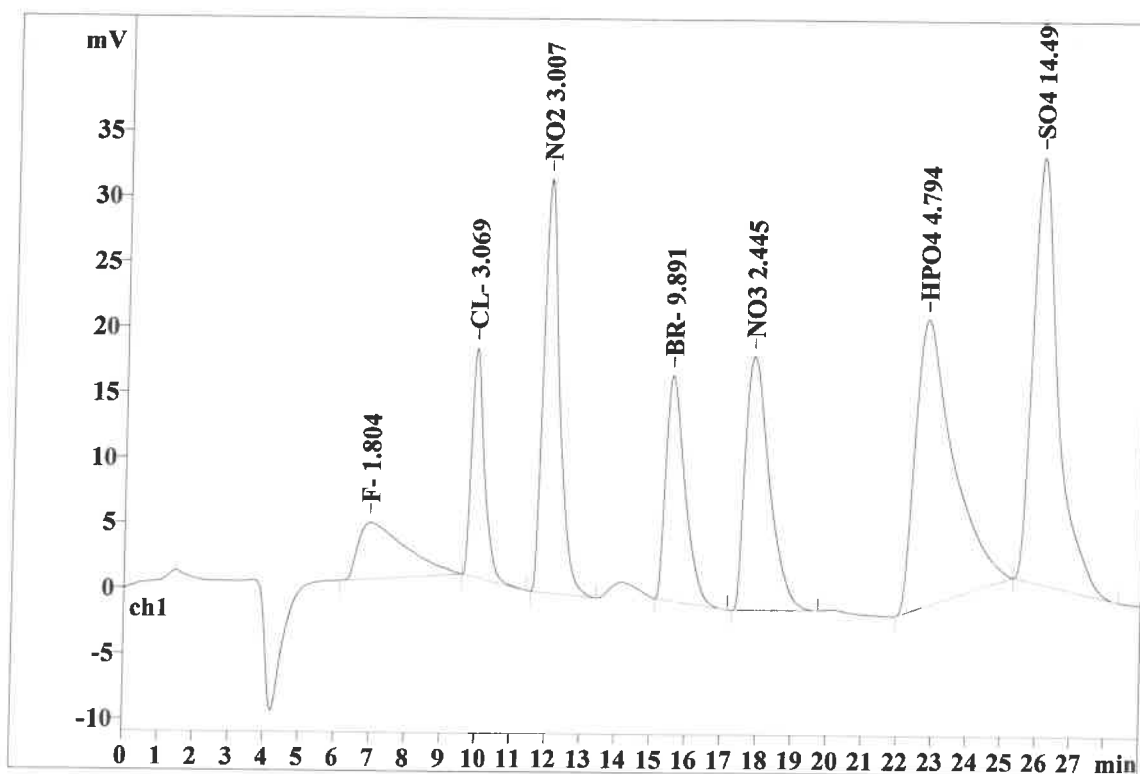

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.95	1.467	4.32	2.99	398.935	5.88
2	9.91	0.383	17.50	12.10	450.848	6.64
3	11.96	0.477	31.59	21.84	1007.948	14.85
4	15.52	0.581	17.24	11.92	652.901	9.62
5	17.82	0.737	19.42	13.42	929.533	13.70
6	22.74	1.110	21.98	15.20	1667.880	24.58
7	26.02	0.725	32.59	22.53	1678.547	24.73
7	29.00	0.783	144.63	100.00	6786.592	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:43:45 PM
Printed by: wet


Ident: CCB
Analysis from: 10/10/2023 1:39:52 PM
File: _2023-10-10_

Last save: 10/10/2023 2:08:52 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36014

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

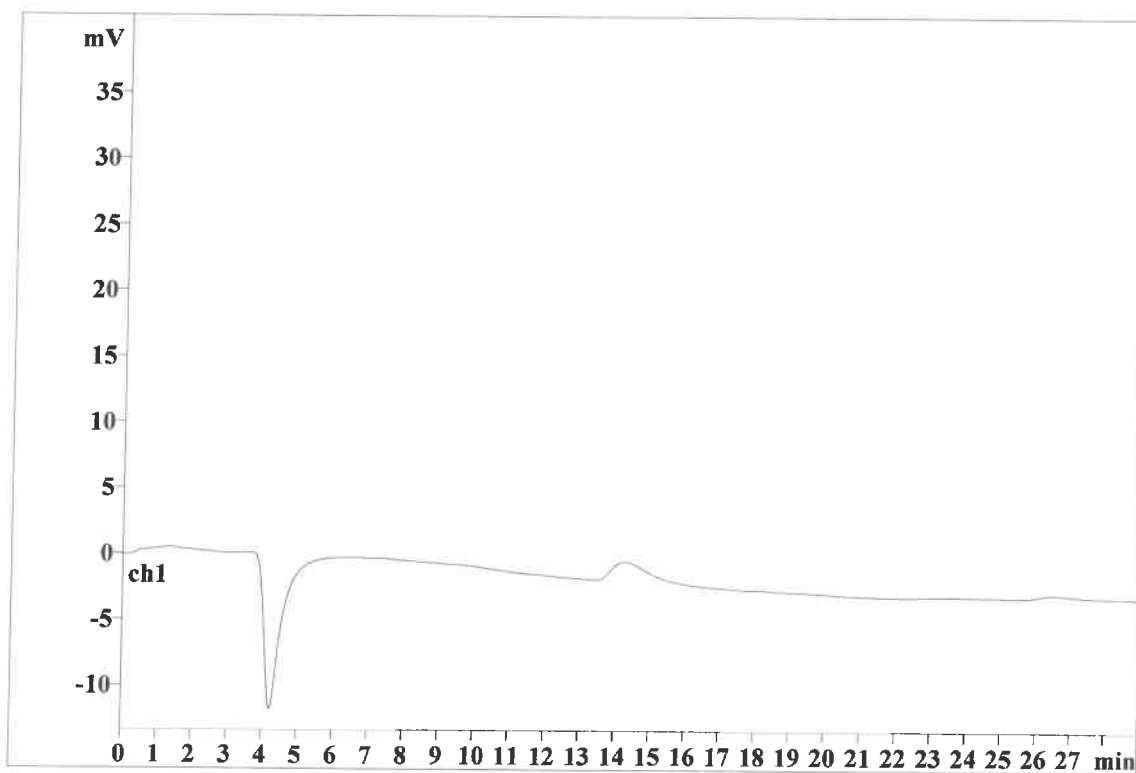

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:43:53 PM
Printed by: wet


Ident: LB127741BLW
Analysis from: 10/10/2023 2:11:30 PM
File: _2023-10-10_

Last save: 10/11/2023 2:43:13 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36015

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

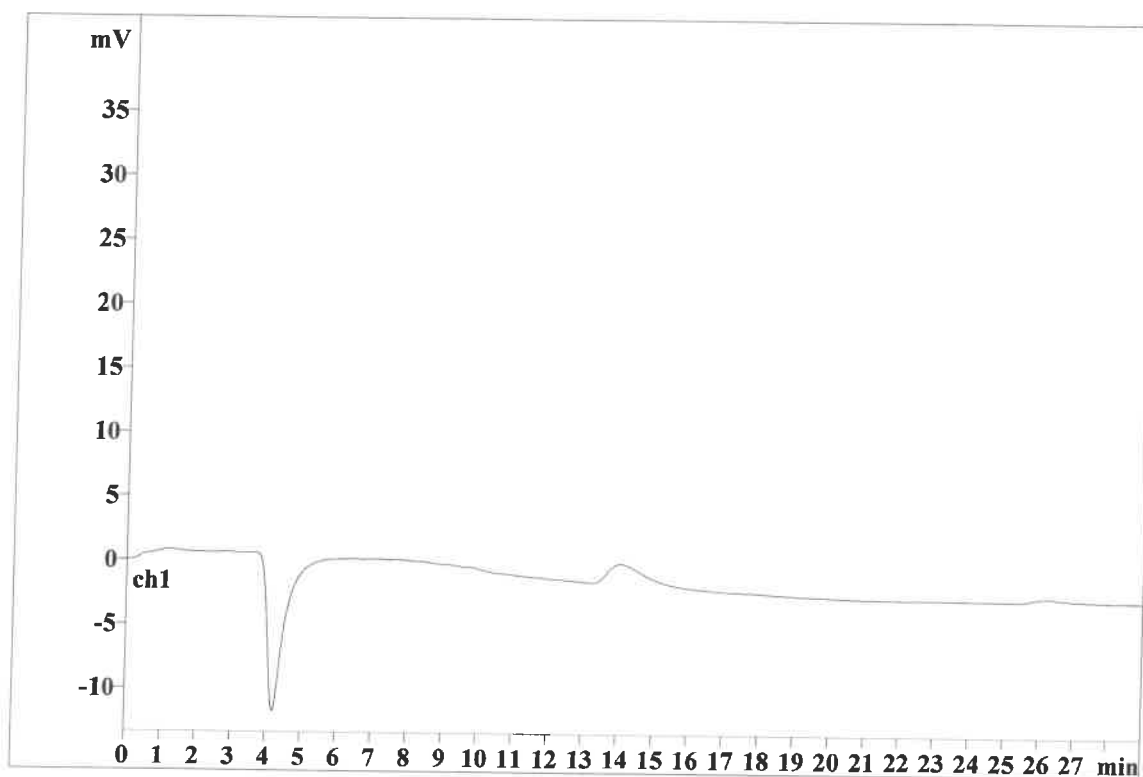

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:43:59 PM
Printed by: wet


Ident: LB127741BSW
Analysis from: 10/10/2023 2:43:17 PM
File: _2023-10-10_

Last save: 10/11/2023 2:43:13 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36016

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

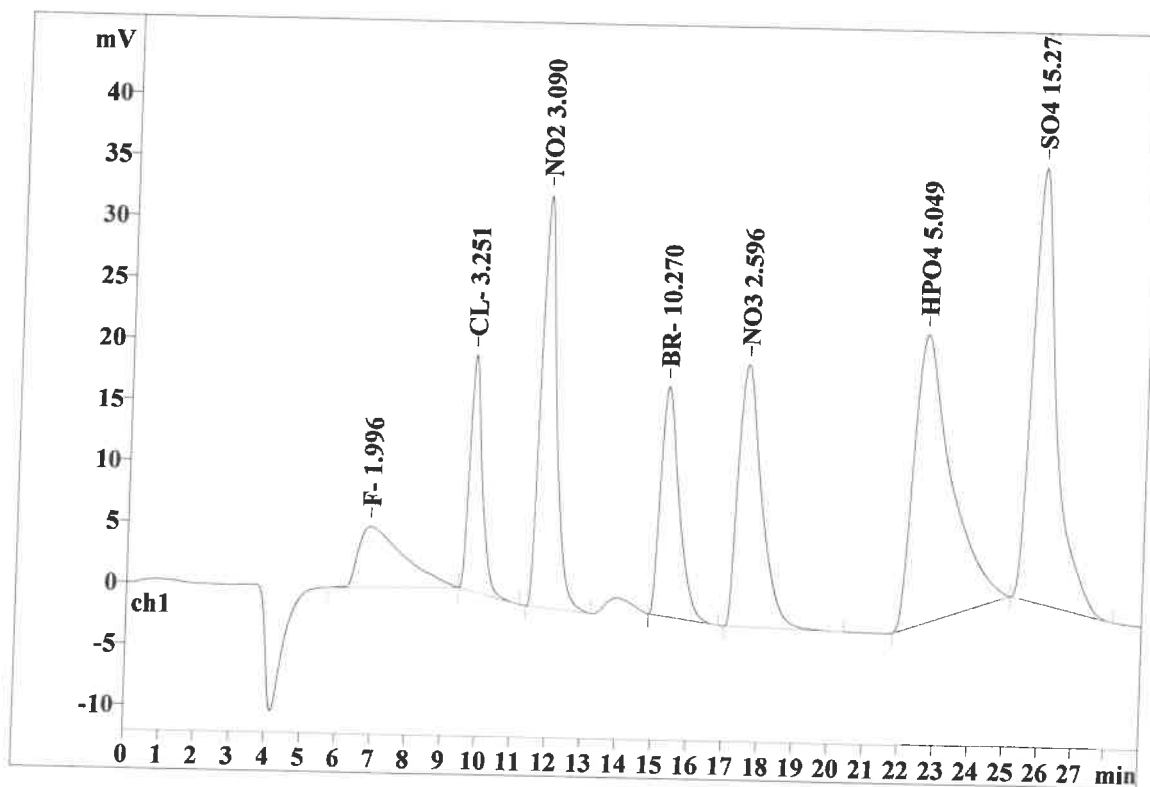

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.87	1.389	5.00	3.18	447.802	6.24
2	9.78	0.369	19.28	12.26	479.080	6.68
3	11.78	0.460	33.63	21.39	1037.337	14.47
4	15.26	0.554	18.74	11.92	679.595	9.48
5	17.50	0.704	21.40	13.61	990.341	13.81
6	22.58	1.073	23.69	15.06	1762.461	24.58
7	25.85	0.700	35.49	22.57	1774.298	24.74
7	29.00	0.750	157.22	99.99	7170.914	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:44:07 PM
Printed by: wet


Ident: 04821-01
Analysis from: 10/10/2023 3:52:53 PM
File: _2023-10-10_

Last save: 10/10/2023 4:21:53 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36017

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 24
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

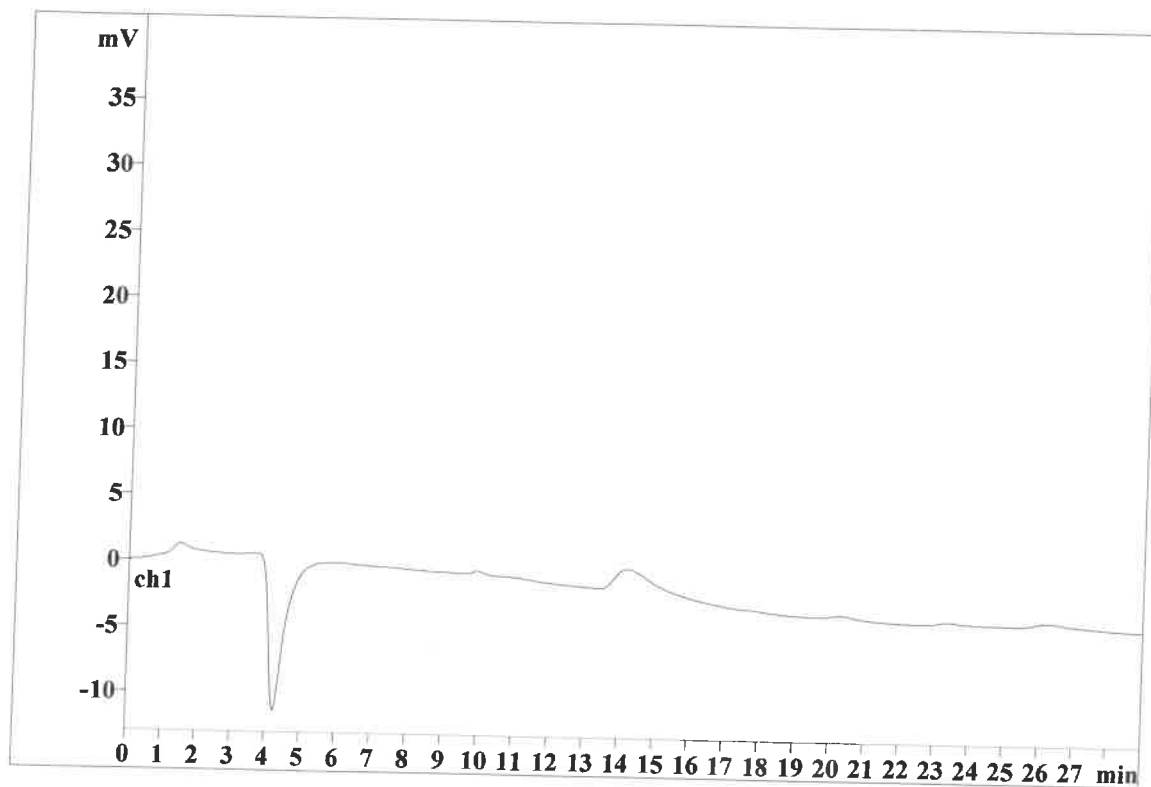

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:44:15 PM
Printed by: wet


Ident: 04822-01
Analysis from: 10/10/2023 4:24:31 PM
File: _2023-10-10_

Last save: 10/10/2023 4:53:31 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36018

Last save: 10/10/2023 9:25

SAMPLE:
:
Vial number: 25
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

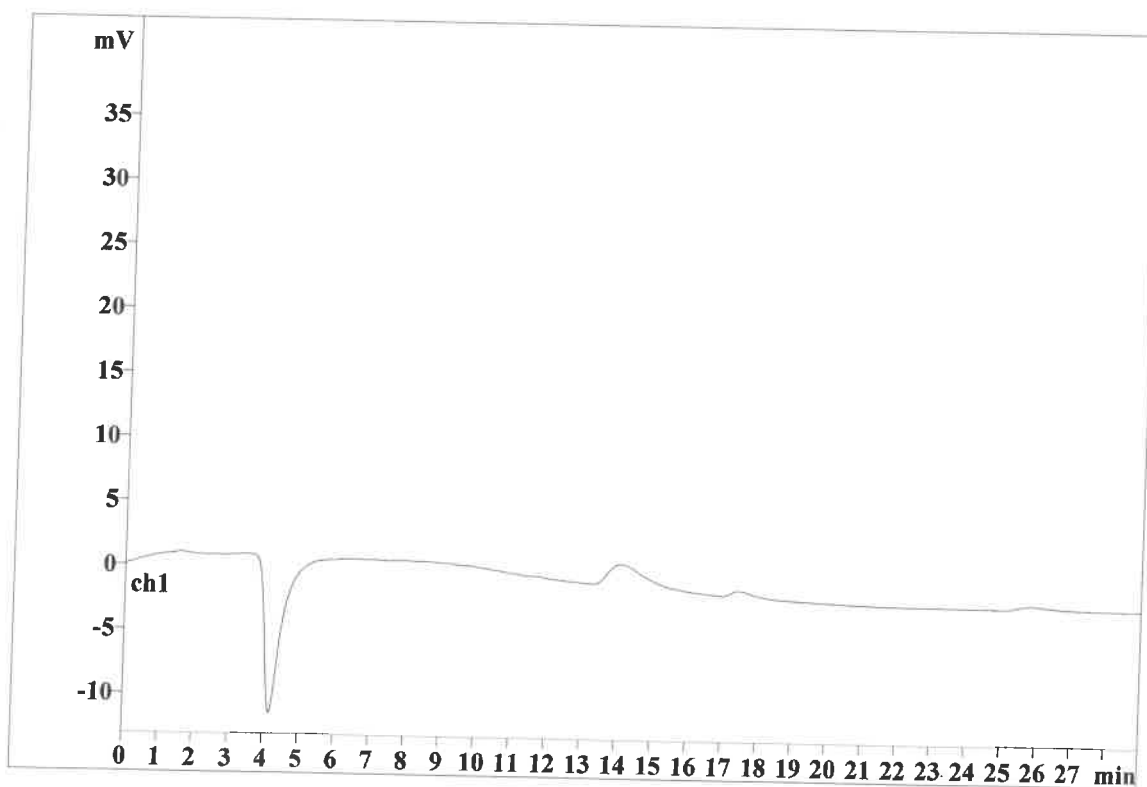

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:44:47 PM
Printed by: wet


Ident: 04822-02
Analysis from: 10/10/2023 4:56:09 PM
File: _2023-10-10_

Last save: 10/11/2023 2:44:42 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36019

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

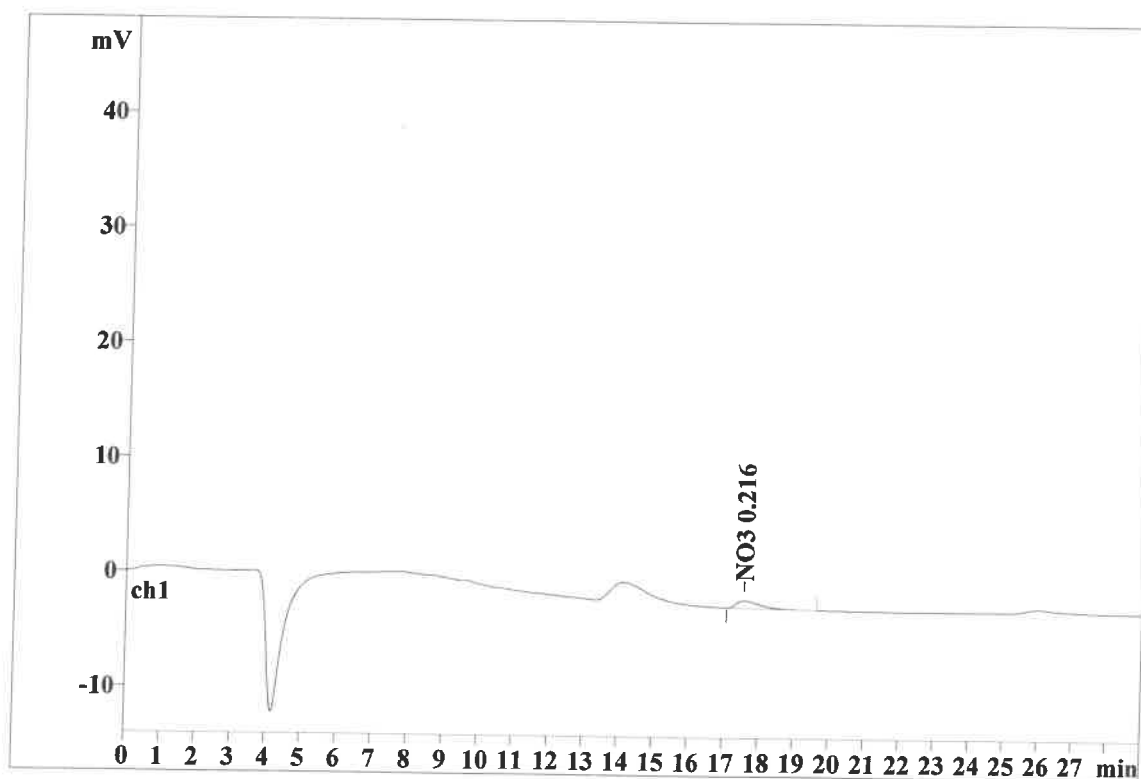

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.58	0.687	0.67	99.59	30.619	100.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	29.00	0.098	0.67	99.59	30.619	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:45:41 PM
Printed by: wet


Ident: O4822-02MS
Analysis from: 10/10/2023 5:27:47 PM
File: _2023-10-10_

Last save: 10/11/2023 2:45:40 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36020

Last save: 10/10/2023 9:25

SAMPLE:
:
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

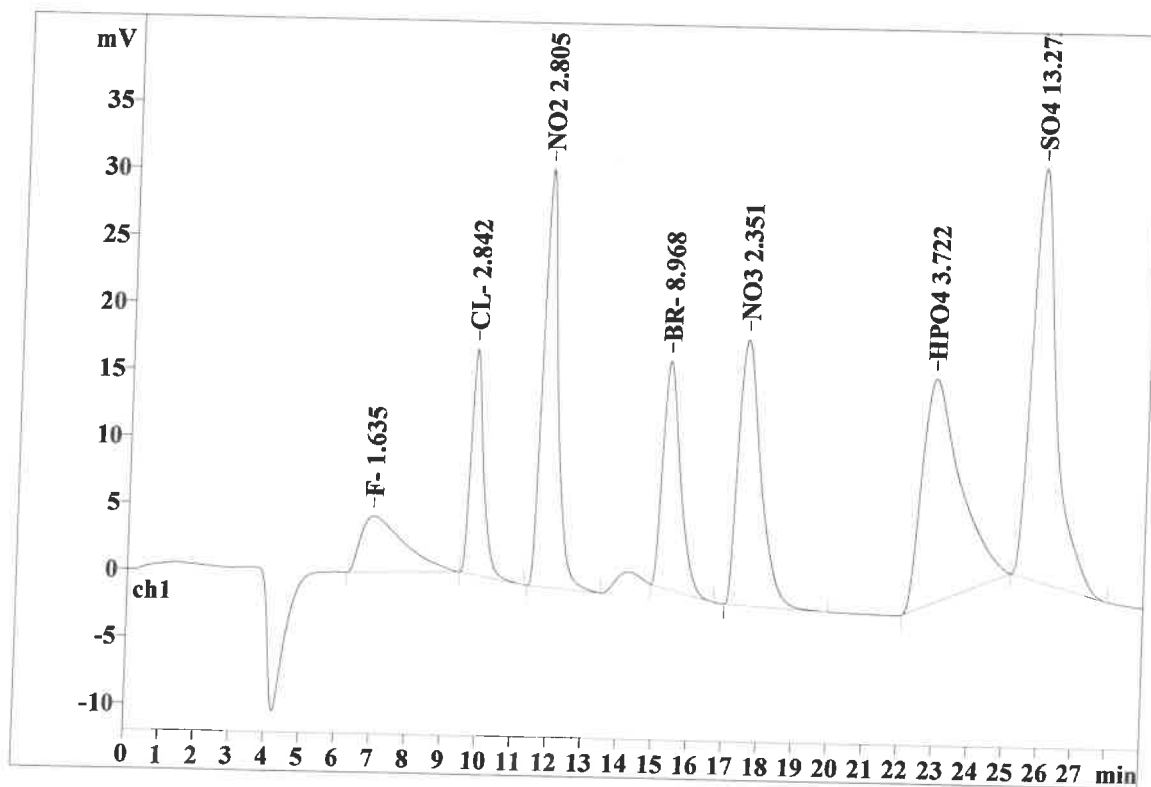

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.97	1.317	4.18	3.06	355.770	5.95
2	9.80	0.364	16.81	12.31	415.406	6.94
3	11.79	0.443	31.18	22.83	936.314	15.65
4	15.28	0.532	16.96	12.42	587.978	9.83
5	17.48	0.686	19.83	14.52	891.595	14.90
6	22.86	1.132	16.82	12.32	1269.667	21.22
7	25.84	0.704	30.79	22.54	1527.323	25.52
7	29.00	0.740	136.57	99.99	5984.053	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:45:57 PM
Printed by: wet


Ident: 04822-02MSD
Analysis from: 10/10/2023 5:59:24 PM
File: _2023-10-10_

Last save: 10/11/2023 2:45:55 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36021

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

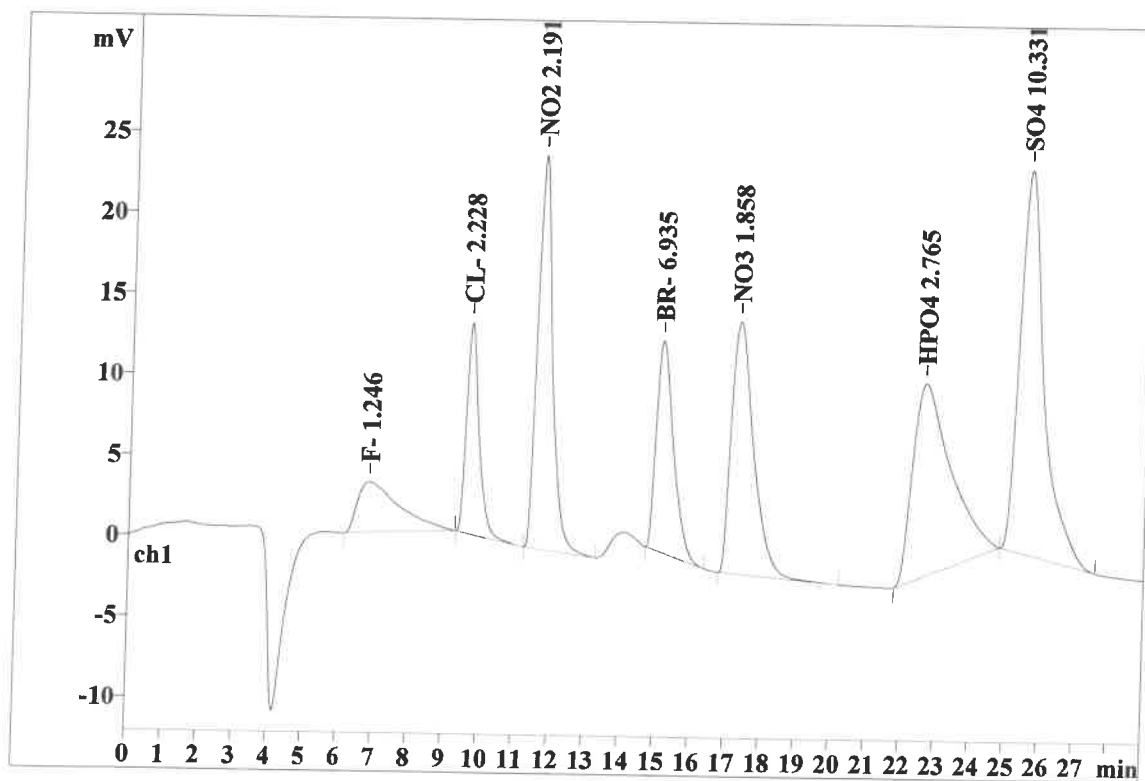

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.83	1.240	3.12	2.97	256.758	5.69
2	9.67	0.361	13.05	12.43	319.941	7.09
3	11.64	0.437	24.34	23.20	717.960	15.91
4	15.09	0.523	13.08	12.47	444.967	9.86
5	17.27	0.676	15.60	14.87	692.960	15.36
6	22.59	1.159	11.98	11.42	914.035	20.26
7	25.53	0.696	23.75	22.63	1164.736	25.82
7	29.00	0.727	104.91	99.98	4511.357	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:46:13 PM
Printed by: wet


Ident: CCV
Analysis from: 10/10/2023 6:31:09 PM
File: _2023-10-10_

Last save: 10/11/2023 2:46:12 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36022

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

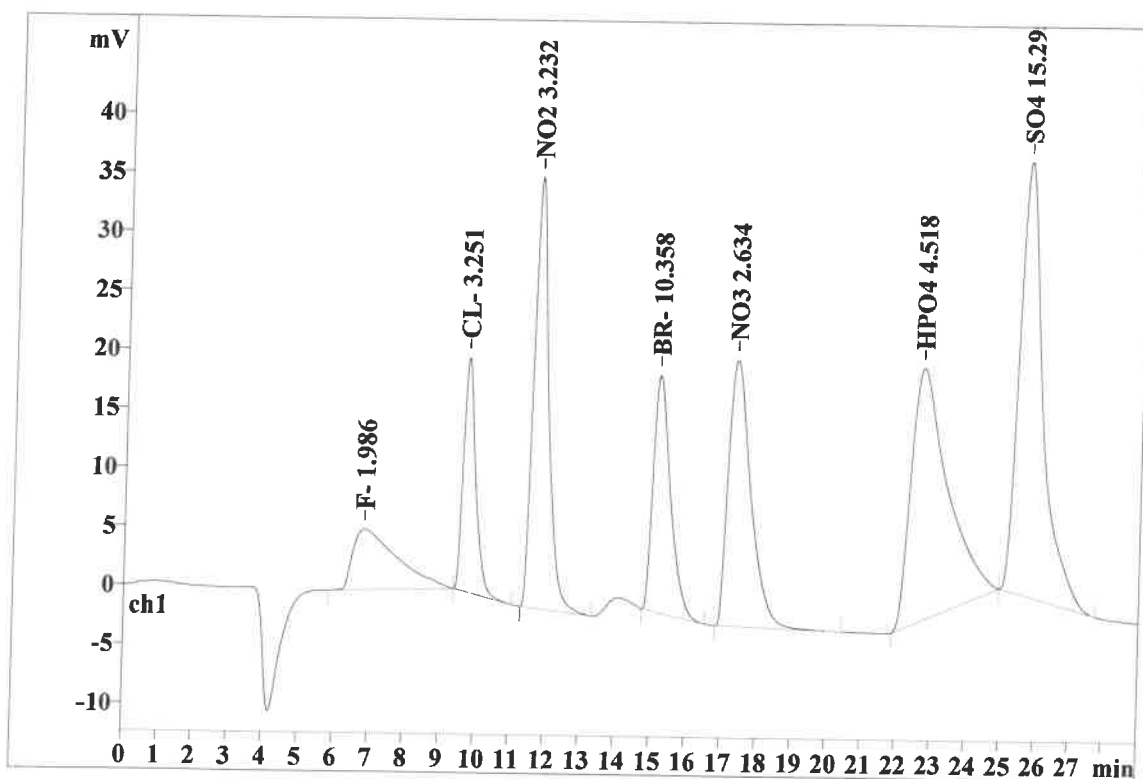

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.82	1.355	5.13	3.16	445.288	6.32
2	9.71	0.357	19.87	12.23	479.107	6.80
3	11.69	0.442	36.53	22.49	1087.745	15.44
4	15.15	0.523	20.08	12.36	685.780	9.73
5	17.33	0.677	22.56	13.89	1005.742	14.27
6	22.66	1.080	21.45	13.21	1565.415	22.22
7	25.64	0.684	36.74	22.63	1776.737	25.22
7	29.00	0.731	162.35	99.98	7045.814	100.00

This report has been created by IC Net
METROHM LTD

Report date: 10/11/2023 2:46:23 PM
Printed by: wet


Ident: CCB
Analysis from: 10/10/2023 7:34:31 PM
File: _2023-10-10_

Last save: 10/10/2023 8:03:31 PM

Method: AnionsIC2-091323.mtw
Run operator: wet
Analysis number: 36024

Last save: 10/10/2023 9:25

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

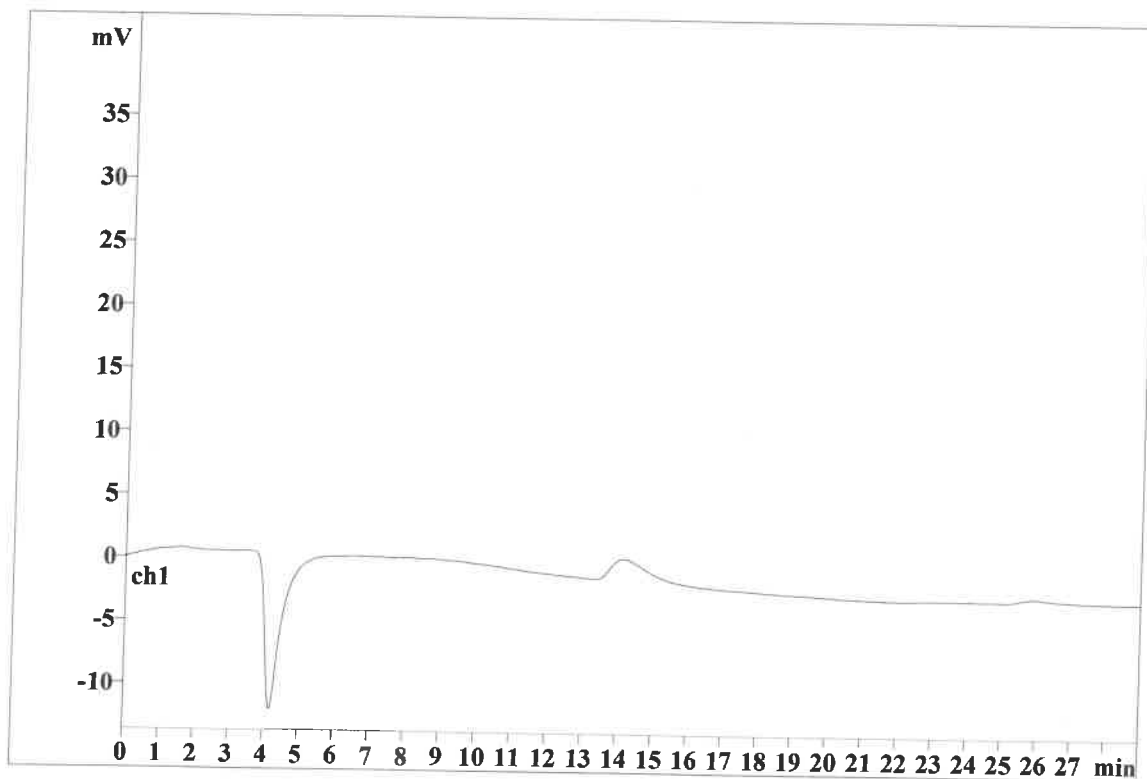

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD