

LB127824


7470A

INSTRUMENT ID: CYZ

Linear

μ Abs.:

43421

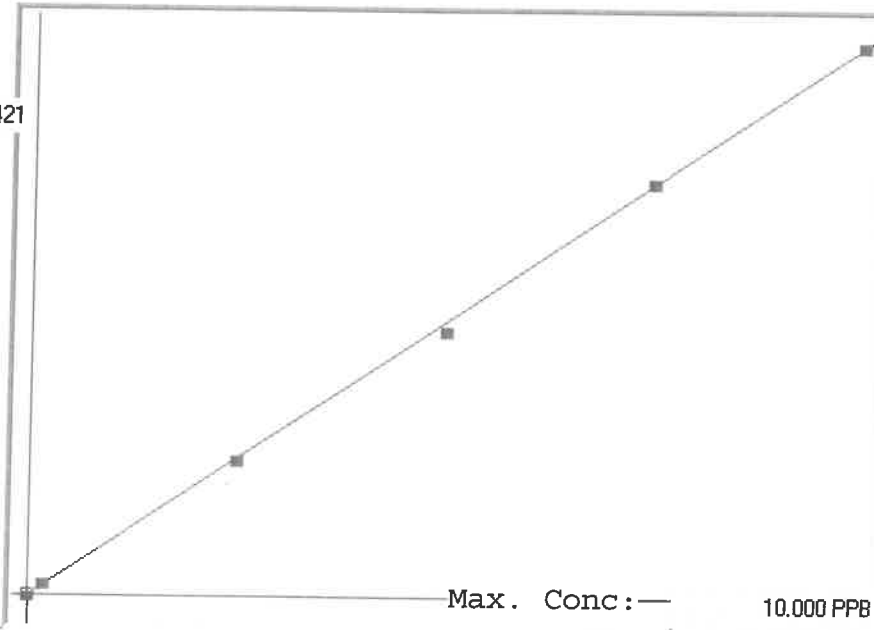

A= 0.0000e+000

B= 2.3069e-004

C= 1.3671e-002

Rho= 0.9998099

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/pd)
0.0	0.000	0.026	0.026	55	0.000	55	0				18
0.2	0.200	0.236	0.036	962	0.0 %	962					0
2.5	2.500	2.509	0.009	10816	0.0 %	10816					3
5.0	5.000	4.842	-0.158	20931	0.0 %	20931					1
7.5	7.500	7.557	0.057	32697	0.0 %	32697					0
10.0	10.000	10.030	0.030	43421	0.0 %	43421					

LB127824 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 17 Oct 2023 10:10:24

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	55	-	0.000	7470A	PPB	17 Oct 2023 10:18:49	S	Std
0.2 - 1	50.2	962	-	0.200	7470A	PPB	17 Oct 2023 10:21:06	S	Std
2.5 - 1	52.5	10816	-	2.500	7470A	PPB	17 Oct 2023 10:23:23	S	Std
5.0 - 1	55	20931	-	5.000	7470A	PPB	17 Oct 2023 10:25:36	S	Std
7.5 - 1	57.5	32697	-	7.500	7470A	PPB	17 Oct 2023 10:27:56	S	Std
10.0 - 1	511	43421	-	10.000	7470A	PPB	17 Oct 2023 10:35:34	S	Std
ICV21 - 1	ICV21	17467	4.0431	-	7470A	PPB	17 Oct 2023 10:38:17	U	SMPL
ICB21 - 1	ICB21	-207	-0.0341	-	7470A	PPB	17 Oct 2023 10:43:22	U	SMPL
CCV12 - 1	CCV12	21309	4.9294	-	7470A	PPB	17 Oct 2023 10:45:37	U	SMPL
CCB12 - 1	CCB12	-433	-0.0862	-	7470A	PPB	17 Oct 2023 10:47:54	U	SMPL
CRA - 1	CRA	737	0.1837	-	7470A	PPB	17 Oct 2023 10:50:10	U	SMPL
HighStd - 1	HighStd	42891	9.9082	-	7470A	PPB	17 Oct 2023 10:52:25	U	SMPL
ChkStd - 1	ChkStd	31212	7.2140	-	7470A	PPB	17 Oct 2023 10:54:41	U	SMPL
PB156408BL - 1	PBW	-188	-0.0297	-	7470A	PPB	17 Oct 2023 11:00:29	U	SMPL
PB156408BS - 1	LCSW	18860	4.3645	-	7470A	PPB	17 Oct 2023 11:02:44	U	SMPL
O4876-01 - 1	30103	-108	-0.0112	-	7470A	PPB	17 Oct 2023 11:05:01	U	SMPL
O4876-01DUP - 1	30103DUP	155	0.0494	-	7470A	PPB	17 Oct 2023 11:10:05	U	SMPL
O4876-01MS - 1	30103MS	19696	4.5578	-	7470A	PPB	17 Oct 2023 11:12:21	U	SMPL
O4876-01MSD - 1	30103MSD	18774	4.3446	-	7470A	PPB	17 Oct 2023 11:14:38	U	SMPL
O4876-02 - 1	30104	-286	-0.0523	-	7470A	PPB	17 Oct 2023 11:16:56	U	SMPL
CCV13 - 1	CCV13	21744	5.0298	-	7470A	PPB	17 Oct 2023 11:19:14	U	SMPL
CCB13 - 1	CCB13	-255	-0.0452	-	7470A	PPB	17 Oct 2023 11:21:29	U	SMPL
O4887-02 - 1	SU-622-VOC-04	-97	-0.0087	-	7470A	PPB	17 Oct 2023 11:23:45	U	SMPL
O4888-02 - 1	TR-304-VOC-01	-65	-0.0013	-	7470A	PPB	17 Oct 2023 11:26:01	U	SMPL
O4893-01 - 1	ROOSEVELT-BRIDGE-SANDBLAST-EAST	7	0.0153	-	7470A	PPB	17 Oct 2023 11:28:16	U	SMPL
PB156387TB - 1	PB156387TB	-68	-0.0020	-	7470A	PPB	17 Oct 2023 11:30:31	U	SMPL
O4876-01LX5 - 1		-2	0.0132	-	7470A	PPB	17 Oct 2023 11:32:47	U	SMPL
O4876-01A - 1		19376	4.4835	-	7470A	PPB	17 Oct 2023 11:35:03	U	SMPL
CCV14 - 1	CCV14	22222	5.1401	-	7470A	PPB	17 Oct 2023 11:37:19	U	SMPL
CCB14 - 1	CCB14	-245	-0.0428	-	7470A	PPB	17 Oct 2023 11:39:39	U	SMPL