


LB127987

7470A

INSTRUMENT ID: CV1

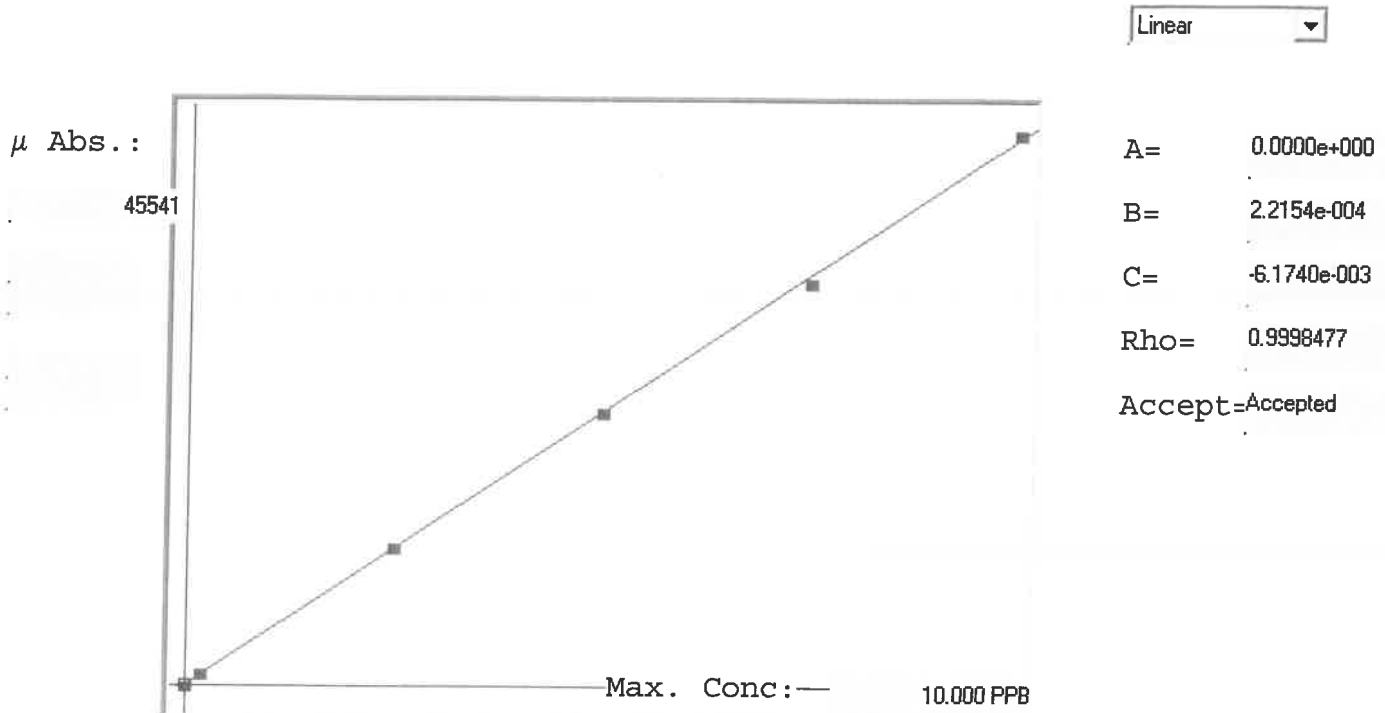

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Q(%)
0.0	0.000	-0.005	-0.005	4	0.000	4	0				1
0.2	0.200	0.222	0.022	1028	0.0 %	1028					1
2.5	2.500	2.514	0.014	11378	0.0 %	11378					1
5.0	5.000	5.017	0.017	22673	0.0 %	22673					1
7.5	7.500	7.370	-0.130	33293	0.0 %	33293					2
10.0	10.000	10.083	0.083	45541	0.0 %	45541					1

LB127987 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 Oct 2023 09:11:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	4	-	0.0000	7470A	PPB	26 Oct 2023 09:46:50	S	Std
0.2 - 1	50.2	1028	-	0.2000	7470A	PPB	26 Oct 2023 09:49:07	S	Std
2.5 - 1	52.5	11378	-	2.5000	7470A	PPB	26 Oct 2023 09:51:25	S	Std
5.0 - 1	55	22673	-	5.0000	7470A	PPB	26 Oct 2023 09:53:41	S	Std
7.5 - 1	57.5	33293	-	7.5000	7470A	PPB	26 Oct 2023 09:58:31	S	Std
10.0 - 1	516	45541	-	10.0000	7470A	PPB	26 Oct 2023 10:00:46	S	Std
ICV36 - 1	ICV36	16467	3.6419	-	7470A	PPB	26 Oct 2023 10:03:35	U	SMPL
ICB36 - 1	ICB36	-199	-0.0503	-	7470A	PPB	26 Oct 2023 10:08:44	U	SMPL
CCV81 - 1	CCV81	22403	4.9570	-	7470A	PPB	26 Oct 2023 10:10:59	U	SMPL
CCB81 - 1	CCB81	-27	-0.0122	-	7470A	PPB	26 Oct 2023 10:15:45	U	SMPL
CRA - 1	CRA	911	0.1956	-	7470A	PPB	26 Oct 2023 10:18:00	U	SMPL
HighStd - 1	HighStd	45454	10.0637	-	7470A	PPB	26 Oct 2023 10:20:15	U	SMPL
ChkStd - 1	ChkStd	31474	6.9665	-	7470A	PPB	26 Oct 2023 10:22:30	U	SMPL
PB156623BL - 1	PBW	-80	-0.0239	-	7470A	PPB	26 Oct 2023 10:27:23	U	SMPL
PB156623BS - 1	LCSW	16190	3.5805	-	7470A	PPB	26 Oct 2023 10:29:38	U	SMPL
O5010-02 - 1	343	-451	-0.1061	-	7470A	PPB	26 Oct 2023 10:31:55	U	SMPL
O5010-04 - 1	72-11985	-180	-0.0461	-	7470A	PPB	26 Oct 2023 10:34:12	U	SMPL
O5010-04DUP - 1	72-11985DUP	-89	-0.0259	-	7470A	PPB	26 Oct 2023 10:36:29	U	SMPL
O5010-04MS - 1	72-11985MS	16494	3.6479	-	7470A	PPB	26 Oct 2023 10:38:47	U	SMPL
O5010-04MSD - 1	72-11985MSD	18960	4.1942	-	7470A	PPB	26 Oct 2023 10:41:02	U	SMPL
CCV82 - 1	CCV82	23713	5.2472	-	7470A	PPB	26 Oct 2023 10:43:18	U	SMPL
CCB82 - 1	CCB82	-43	-0.0157	-	7470A	PPB	26 Oct 2023 10:48:07	U	SMPL
PB156597TB - 1	PB156597TB	-146	-0.0385	-	7470A	PPB	26 Oct 2023 10:50:22	U	SMPL
O5010-04LX5 - 1		69	0.0091	-	7470A	PPB	26 Oct 2023 10:52:37	U	SMPL
O5010-04A - 1		17815	3.9405	-	7470A	PPB	26 Oct 2023 10:54:52	U	SMPL
CCV83 - 1	CCV83	22031	4.8745	-	7470A	PPB	26 Oct 2023 10:59:44	U	SMPL
CCB83 - 1	CCB83	-358	-0.0855	-	7470A	PPB	26 Oct 2023 11:02:00	U	SMPL