


LB128008

SFAM01.1

INSTRUMENT ID: CV2

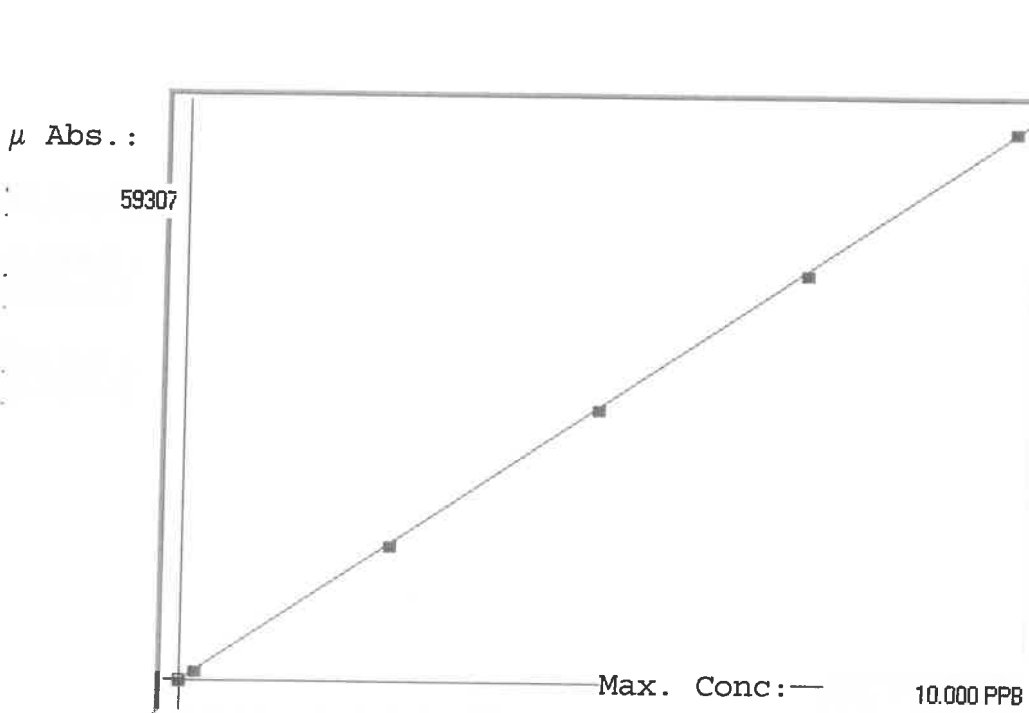

Linear

A= 0.0000e+000

B= 1.6925e-004 slope

C= 4.3167e-003 intercept

Rho= 0.9999708

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.013	0.013	53	0.000	53					
0.05	0.050					419					
0.20	0.200	0.201	0.001	1164	0.0 %	1164	0				
2.50	2.500	2.504	0.004	14767	0.0 %	14767					
5.00	5.000	4.993	-0.007	29475	0.0 %	29475					
7.50	7.500	7.447	-0.053	43977	0.0 %	43977					
10.0	10.000	10.042	0.042	59307	0.0 %	59307					

0.00-11

LB128008

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type
	0 S0	53	-		0 SFAM01.1	PPB	10/27/2023 13:39	Std
	0.2 S01	1164	-		0.2 SFAM01.1	PPB	10/27/2023 13:41	Std
	2.5 S02	14767	-		2.5 SFAM01.1	PPB	10/27/2023 13:44	Std
	5 S03	29475	-		5 SFAM01.1	PPB	10/27/2023 13:46	Std
	7.5 S04	43977	-		7.5 SFAM01.1	PPB	10/27/2023 13:48	Std
	10 S05	59307	-		10 SFAM01.1	PPB	10/27/2023 13:58	Std
ICV040	ICV040	23140	3.9207 -		SFAM01.1	PPB	10/27/2023 14:01	SMPL
ICB040	ICB040	-279	-0.0429 -		SFAM01.1	PPB	10/27/2023 14:03	SMPL
CCV095	CCV095	29318	4.9663 -		SFAM01.1	PPB	10/27/2023 14:05	SMPL
CCB095	CCB095	-267	-0.0409 -		SFAM01.1	PPB	10/27/2023 14:08	SMPL
O4877-02DLX5	MEZZ80	18921	3.2066 -		SFAM01.1	PPB	10/27/2023 14:10	SMPL
O4877-03DLX5	MEZZ81	19505	3.3055 -		SFAM01.1	PPB	10/27/2023 14:12	SMPL
O4877-15DLX5	MEZZ80	16003	2.7128 -		SFAM01.1	PPB	10/27/2023 14:14	SMPL
O4877-16DLX5	MEZZ31	18546	3.1431 -		SFAM01.1	PPB	10/27/2023 14:17	SMPL
O4921-02DLX2	MEZZ85	35349	5.987 -		SFAM01.1	PPB	10/27/2023 14:19	SMPL
CCV096	CCV096	29390	4.9784 -		SFAM01.1	PPB	10/27/2023 14:21	SMPL
CCB096	CCB096	-141	-0.0195 -		SFAM01.1	PPB	10/27/2023 14:23	SMPL