


LB128019

7470A

INSTRUMENT ID: CV1

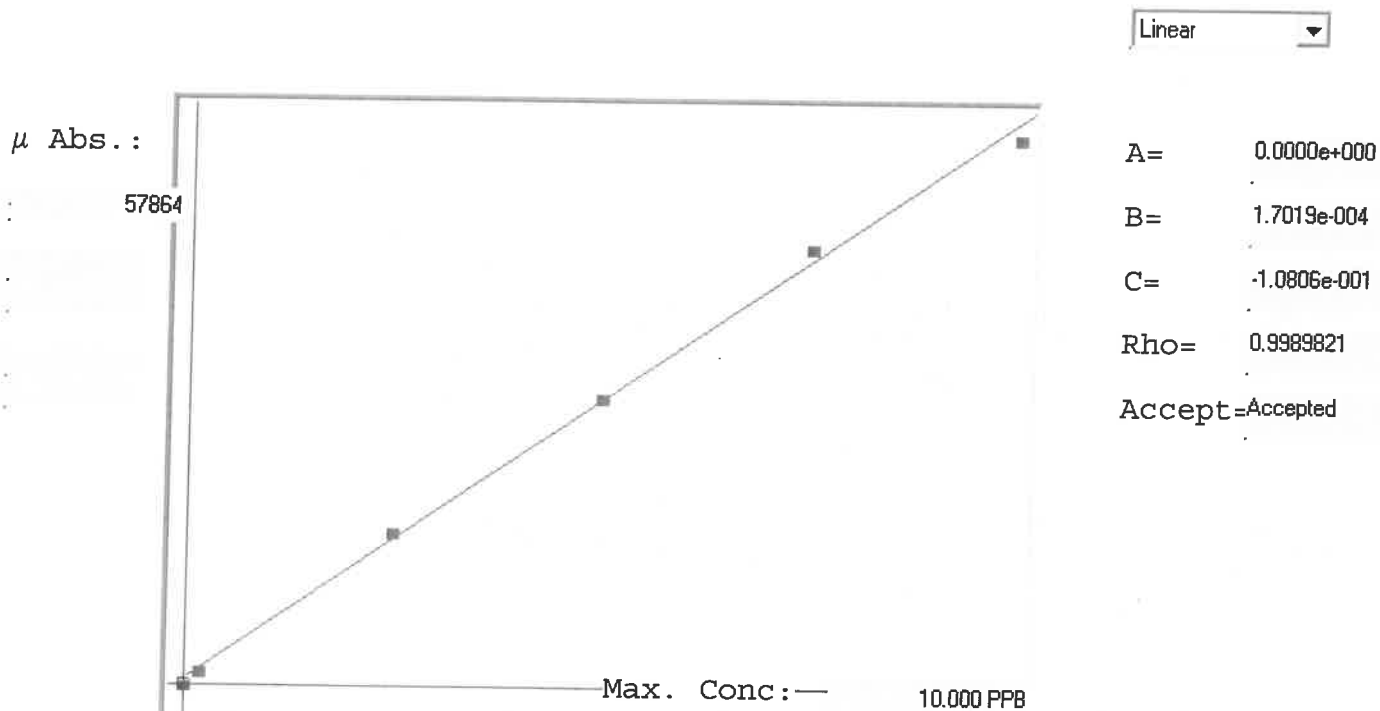

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0
0.0	0.000	-0.110	-0.110	-14	0.000	-14	0				
0.2	0.200	0.141	-0.059	1463	0.0 %	1463					
2.5	2.500	2.632	0.132	16098	0.0 %	16098					
5.0	5.000	5.047	0.047	30289	0.0 %	30289					
7.5	7.500	7.752	0.252	46182	0.0 %	46182					
10.0	10.000	9.740	-0.260	57864	0.0 %	57864					

LB128019 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Oct 2023 18:34:32

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-14	-	0.0000	7470A	PPB	27 Oct 2023 18:35:33	S	Std
0.2 - 1	50.2	1463	-	0.2000	7470A	PPB	27 Oct 2023 18:37:49	S	Std
2.5 - 1	52.5	16098	-	2.5000	7470A	PPB	27 Oct 2023 18:40:06	S	Std
5.0 - 1	55	30289	-	5.0000	7470A	PPB	27 Oct 2023 18:42:23	S	Std
7.5 - 1	57.5	46182	-	7.5000	7470A	PPB	27 Oct 2023 18:44:42	S	Std
10.0 - 1	50	57864	-	10.0000	7470A	PPB	27 Oct 2023 18:59:36	S	Std
ICV41 - 1	ICV41	23389	3.8724	-	7470A	PPB	27 Oct 2023 19:05:02	U	SMPL
ICB41 - 1	ICB41	362	-0.0465	-	7470A	PPB	27 Oct 2023 19:12:04	U	SMPL
CCV02 - 1	CCV02	28808	4.7947	-	7470A	PPB	27 Oct 2023 19:14:18	U	SMPL
CCB02 - 1	CCB02	102	-0.0907	-	7470A	PPB	27 Oct 2023 19:16:33	U	SMPL
CRA - 1	CRA	2009	0.2338	-	7470A	PPB	27 Oct 2023 19:18:50	U	SMPL
HighStd - 1	HighStd	58122	9.7836	-	7470A	PPB	27 Oct 2023 19:21:04	U	SMPL
ChkStd - 1	ChkStd	40130	6.7215	-	7470A	PPB	27 Oct 2023 19:23:19	U	SMPL
PB156725BL - 1	PBW	1008	0.0635	-	7470A	PPB	27 Oct 2023 19:28:19	U	SMPL
PB156725BS - 1	LCSW	23633	3.9140	-	7470A	PPB	27 Oct 2023 19:30:35	U	SMPL
O5036-01 - 1	BUR-1277	-119	-0.1283	-	7470A	PPB	27 Oct 2023 19:32:52	U	SMPL
O5036-01DUP - 1	BUR-1277DUP	58	-0.0982	-	7470A	PPB	27 Oct 2023 19:35:08	U	SMPL
O5036-01MS - 1	BUR-1277MS	23842	3.9495	-	7470A	PPB	27 Oct 2023 19:37:25	U	SMPL
O5036-01MSD - 1	BUR-1277MSD	23867	3.9538	-	7470A	PPB	27 Oct 2023 19:42:32	U	SMPL
CCV03 - 1	CCV03	28066	4.6684	-	7470A	PPB	27 Oct 2023 19:44:47	U	SMPL
CCB03 - 1	CCB03	523	-0.0191	-	7470A	PPB	27 Oct 2023 19:49:13	U	SMPL
O5036-01LX5 - 1		65	-0.0970	-	7470A	PPB	27 Oct 2023 19:51:27	U	SMPL
O5036-01A - 1		23571	3.9034	-	7470A	PPB	27 Oct 2023 19:53:43	U	SMPL
CCV04 - 1	CCV04	27687	4.6039	-	7470A	PPB	27 Oct 2023 19:55:58	U	SMPL
CCB04 - 1	CCB04	95	-0.0919	-	7470A	PPB	27 Oct 2023 19:58:14	U	SMPL