


LB1280T4

7471B

INSTRUMENT ID: CV1

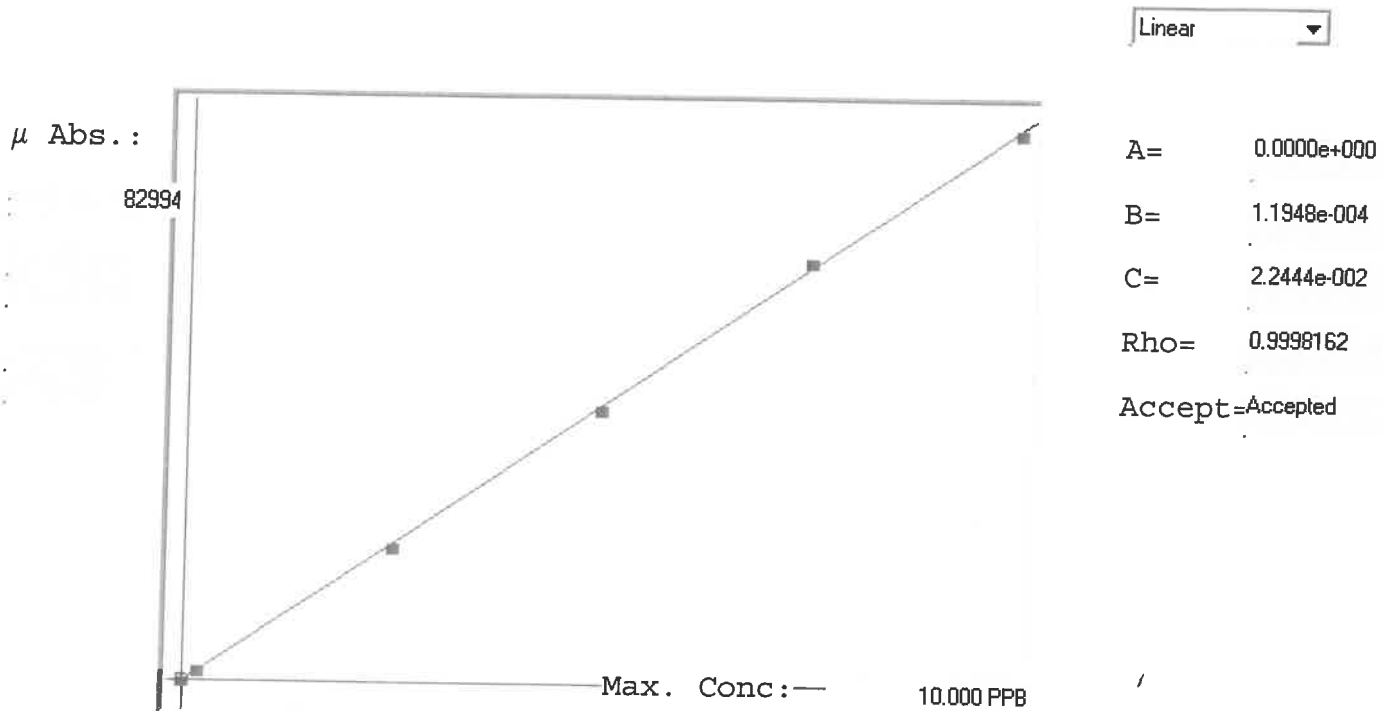

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%RSD
0.0	0.000	0.040	0.040	149	0.000	149					1
0.2	0.200	0.205	0.005	1529	0.0 %	1529					2
2.5	2.500	2.431	-0.069	20161	0.0 %	20161					-3
5.0	5.000	4.952	-0.048	41261	0.0 %	41261					-1
7.5	7.500	7.633	0.133	63695	0.0 %	63695					2
10.0	10.000	9.938	-0.062	82994	0.0 %	82994					-1

LB128054 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 30 Oct 2023 13:28:50

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	5.0	149	-	0.0000	7471B	PPB	30 Oct 2023 13:35:55	S	Std
0.2 - 1	5.0.2	1529	-	0.2000	7471B	PPB	30 Oct 2023 13:38:12	S	Std
2.5 - 1	5.2.5	20161	-	2.5000	7471B	PPB	30 Oct 2023 13:40:29	S	Std
5.0 - 1	5.5	41261	-	5.0000	7471B	PPB	30 Oct 2023 13:42:46	S	Std
7.5 - 1	5.7.5	63695	-	7.5000	7471B	PPB	30 Oct 2023 13:45:02	S	Std
10.0 - 1	5.10	82994	-	10.0000	7471B	PPB	30 Oct 2023 13:47:20	S	Std
ICV44 - 1	ICV44	32287	3.8801	-	7471B	PPB	30 Oct 2023 13:50:17	U	SMPL
ICB44 - 1	ICB44	-258	-0.0084	-	7471B	PPB	30 Oct 2023 13:52:32	U	SMPL
CCV10 - 1	CCV10	41073	4.9298	-	7471B	PPB	30 Oct 2023 13:54:49	U	SMPL
CCB10 - 1	CCB10	-275	-0.0104	-	7471B	PPB	30 Oct 2023 13:57:04	U	SMPL
CRA - 1	CRA	1381	0.1874	-	7471B	PPB	30 Oct 2023 13:59:21	U	SMPL
HighStd - 1	HighStd	81259	9.7312	-	7471B	PPB	30 Oct 2023 14:01:37	U	SMPL
ChkStd - 1	ChkStd	56673	6.7937	-	7471B	PPB	30 Oct 2023 14:03:52	U	SMPL
PB156779BL - 1	PBS	-498	-0.0371	-	7471B	PPB	30 Oct 2023 14:06:11	U	SMPL
O5092-01 - 1	CHRT-20058	1216	0.1677	-	7471B	PPB	30 Oct 2023 14:10:45	U	SMPL
O5092-01DUP - 1	CHRT-20058DUP	939	0.1346	-	7471B	PPB	30 Oct 2023 14:15:59	U	SMPL
O5092-01MS - 1	CHRT-20058MS	30274	3.6395	-	7471B	PPB	30 Oct 2023 14:18:16	U	SMPL
O5092-01MSD - 1	CHRT-20058MSD	30404	3.6551	-	7471B	PPB	30 Oct 2023 14:20:33	U	SMPL
O5092-03 - 1	CHRT-25651	-139	0.0058	-	7471B	PPB	30 Oct 2023 14:22:49	U	SMPL
CCV11 - 1	CCV11	38822	4.6608	-	7471B	PPB	30 Oct 2023 14:25:06	U	SMPL
CCB11 - 1	CCB11	-383	-0.0233	-	7471B	PPB	30 Oct 2023 14:27:21	U	SMPL
O5108-01 - 1	1023-A	13853	1.6776	-	7471B	PPB	30 Oct 2023 14:29:39	U	SMPL
O5108-02 - 1	1023-B	7111	0.8721	-	7471B	PPB	30 Oct 2023 14:31:55	U	SMPL
O5108-03 - 1	1023-C	31722	3.8126	-	7471B	PPB	30 Oct 2023 14:34:12	U	SMPL
O5135-02 - 1	CHRT-20413	197891	23.6662	-	7471B	PPB	30 Oct 2023 14:36:28	U	SMPL
O5137-01 - 1	FAIR-LAWN-CONC	482320	HIGH	-	7471B	PPB	30 Oct 2023 14:38:45	X	
O5138-01 - 1	348	7150	0.8767	-	7471B	PPB	30 Oct 2023 14:40:37	U	SMPL
O5142-01 - 1	PSC-124037	7077	0.8680	-	7471B	PPB	30 Oct 2023 14:42:57	U	SMPL
O5145-01 - 1	TR-06-10272023	908	0.1309	-	7471B	PPB	30 Oct 2023 14:45:14	U	SMPL
O5092-01LX5 - 1		111	0.0357	-	7471B	PPB	30 Oct 2023 14:47:32	U	SMPL
O5092-01A - 1		31708	3.8109	-	7471B	PPB	30 Oct 2023 14:49:48	U	SMPL
CCV12 - 1	CCV12	38316	4.6004	-	7471B	PPB	30 Oct 2023 14:52:03	U	SMPL
CCB12 - 1	CCB12	-146	0.0050	-	7471B	PPB	30 Oct 2023 14:54:19	U	SMPL
O5137-01DLX10 - 1		120893	14.4666	-	7471B	PPB	30 Oct 2023 14:56:35	U	SMPL
O5135-02DLX5 - 1		43838	5.2602	-	7471B	PPB	30 Oct 2023 14:58:50	U	SMPL
O5137-01DLX50 - 1		19964	2.4077	-	7471B	PPB	30 Oct 2023 15:01:08	U	SMPL
PB156779BS - 1	LCSS	30329	3.6461	-	7471B	PPB	30 Oct 2023 15:14:34	U	SMPL
CCV13 - 1	CCV13	37764	4.5344	-	7471B	PPB	30 Oct 2023 15:17:05	U	SMPL
CCB13 - 1	CCB13	-244	-0.0067	-	7471B	PPB	30 Oct 2023 15:19:21	U	SMPL