

Clear table

Instrument ID: IC-2										Analyst : IZ		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-13_	10/13/23 11:55		IZ/MA		
STD2	0.4760	0.6790	0.6900	2.2840	0.5760	1.1830	3.5590	2023-10-13_	10/13/23 12:26		IZ/MA		
STD3	0.8320	1.1990	1.1960	3.9990	1.0010	1.9570	6.0170	2023-10-13_	10/13/23 12:58		IZ/MA		
STD4	1.0190	1.5130	1.5130	5.0250	1.2570	2.5160	7.5280	2023-10-13_	10/13/23 13:29		IZ/MA		
STD5	1.8540	2.9090	2.9050	9.6870	2.4170	4.9030	14.3650	2023-10-13_	10/13/23 14:01		IZ/MA		
STD6	3.9210	5.8890	5.8710	19.6300	4.8970	9.6600	29.3630	2023-10-13_	10/13/23 14:33		IZ/MA		
STD7	5.0970	7.6110	7.6260	25.3750	6.3520	12.7810	38.1690	2023-10-13_	10/13/23 15:04		IZ/MA		
ICV	2.0270	2.9970	3.0100	9.9240	2.5070	5.2390	14.8000	2023-10-13_	10/13/23 16:39		IZ/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-10-13_	10/13/23 17:11		IZ/MA		
CCV	2.1140	3.0590	2.8200	10.2500	2.4660	6.5260	15.2860	2023-11-03_	11/3/23 17:58		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-03_	11/3/23 18:30		IZ/MA		
LB128206BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-03_	11/3/23 19:02		IZ/MA		
LB128206BSW	2.0310	3.0530	2.8260	10.2080	2.4770	5.7840	15.1740	2023-11-03_	11/3/23 19:33		IZ/MA		
O5241-04	0.4770	58.6300	0.0000	0.0000	0.5970	0.0000	16.6250	2023-11-03_	11/3/23 20:05		IZ/MA		
O5241-05	0.0000	53.5200	0.0000	0.0000	0.0000	0.0000	10.2320	2023-11-03_	11/3/23 20:37		IZ/MA		
O5241-08	0.0000	57.7810	0.0000	0.0000	0.0000	0.0000	12.8130	2023-11-03_	11/3/23 21:08		IZ/MA		
O5241-09	0.4930	41.2140	0.0000	0.0000	3.0710	0.0000	34.8540	2023-11-03_	11/3/23 21:40		IZ/MA		
O5241-13	0.0000	52.8240	0.0000	0.0000	0.0000	0.0000	22.2180	2023-11-03_	11/3/23 22:11		IZ/MA		
O5241-14	0.0000	42.2180	0.0000	0.0000	1.2120	0.0000	38.8260	2023-11-03_	11/3/23 22:43		IZ/MA		
O5241-15MS	3.4720	44.0950	1.3400	10.5940	3.7870	8.3760	55.6400	2023-11-03_	11/3/23 23:15		IZ/MA		
O5241-16MSD	3.5860	44.1740	1.4130	11.2930	4.0090	9.2650	57.2980	2023-11-03_	11/3/23 23:46		IZ/MA		
CCV	2.1990	3.1040	2.7320	10.3870	2.5470	7.1620	15.4720	2023-11-04_	11/4/23 0:18		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-04_	11/4/23 0:50		IZ/MA		
O5241-17	0.0000	41.7180	0.0000	0.0000	0.0000	0.0000	53.5430	2023-11-04_	11/4/23 1:21		IZ/MA		
O5241-18	0.0000	35.0510	0.0000	0.0000	0.0000	0.0000	10.2030	2023-11-04_	11/4/23 1:53		IZ/MA		
O5241-19	0.0000	41.6260	0.0000	0.0000	0.5310	0.0000	11.0490	2023-11-04_	11/4/23 2:25		IZ/MA		
O5241-20	0.0000	49.2160	0.0000	0.0000	0.0000	0.0000	12.4980	2023-11-04_	11/4/23 2:56		IZ/MA		
O5241-22	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-04_	11/4/23 3:28		IZ/MA		
O5241-23	0.0000	33.7740	0.0000	0.0000	0.0000	0.0000	9.9260	2023-11-04_	11/4/23 4:00		IZ/MA		
O5241-23MS	3.2410	35.6920	1.6460	10.5000	2.5440	7.9810	26.5070	2023-11-04_	11/4/23 4:31		IZ/MA		
O5241-23MSD	3.2640	35.7830	1.6520	10.6100	2.5880	8.5920	26.6770	2023-11-04_	11/4/23 5:03		IZ/MA		
CCV	2.1750	3.0640	2.6990	10.2230	2.4930	6.9240	15.1030	2023-11-04_	11/4/23 5:35		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-04_	11/4/23 6:06		IZ/MA		
CCV	2.0660	3.0950	2.8340	10.3760	2.5280	5.4830	15.1500	2023-11-06_	11/6/23 9:53		IZ/MA		

CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-06	11/6/23 10:27	IZ/MA
LB128206BLW2	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-06	11/6/23 10:59	IZ/MA
LB128206BSW2	1.8890	2.9570	2.7280	9.9170	2.4000	5.2250	14.5070	2.2060	1.7460	2023-11-06	11/6/23 11:31	IZ/MA
O5241-04DLX10	0.0000	4.5240	0.0000	0.0000	0.0000	0.0000	2.2060	2.2060	1.7460	2023-11-06	11/6/23 12:02	IZ/MA
O5241-05DLX10	0.0000	4.1970	0.0000	0.0000	0.0000	0.0000	1.7460	1.7460	2.0130	2023-11-06	11/6/23 12:34	IZ/MA
O5241-08DLX10	0.0000	4.6130	0.0000	0.0000	0.0000	0.0000	2.0130	2.0130	3.7910	2023-11-06	11/6/23 13:06	IZ/MA
O5241-09DLX10	0.0000	3.4340	0.0000	0.0000	0.3090	0.0000	3.7910	2.7200	2.7200	2023-11-06	11/6/23 13:37	IZ/MA
O5241-13DLX10	0.0000	4.1900	0.0000	0.0000	0.0000	0.0000	2.7200	18.8230	3.9820	2023-11-06	11/6/23 14:09	IZ/MA
O5241-14DLX2	0.0000	20.1400	0.0000	0.0000	0.6050	0.0000	18.8230	3.9820	9.9120	2023-11-06	11/6/23 15:12	IZ/MA
O5241-14DL2X10	0.0000	3.5660	0.0000	0.0000	0.1880	0.0000	3.9820	9.9120	14.7890	2023-11-06	11/6/23 15:44	IZ/MA
O5241-17DLX5	0.0000	7.1980	0.0000	0.0000	0.0000	0.0000	9.9120	14.7890	0.0000	2023-11-06	11/6/23 16:15	IZ/MA
CCV	2.0060	3.0190	2.6840	9.9740	2.3820	6.3660	14.7890	0.0000	0.0000	2023-11-06	11/6/23 16:47	IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	1.7910	2023-11-06	11/6/23 17:50	IZ/MA
O5241-18DLX10	0.0000	2.9730	0.0000	0.0000	0.0000	0.0000	1.7910	1.8690	2.0050	2023-11-06	11/6/23 18:22	IZ/MA
O5241-19DLX10	0.0000	3.4420	0.0000	0.0000	0.0000	0.0000	1.8690	2.0050	1.8280	2023-11-06	11/6/23 18:54	IZ/MA
O5241-20DLX10	0.0000	3.9290	0.0000	0.0000	0.0000	0.0000	2.0050	1.8280	14.9830	2023-11-06	11/6/23 19:25	IZ/MA
O5241-23DLX10	0.0000	2.8880	0.0000	0.0000	0.0000	0.0000	1.8280	14.9830	0.0000	2023-11-06	11/6/23 19:57	IZ/MA
CCV	2.1440	2.9800	2.7410	10.0140	2.4100	7.0350	14.9830	0.0000	0.0000	2023-11-06	11/6/23 20:29	IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-06		IZ/MA

Report date: 11/7/2023 9:27:45 AM
Printed by: wet


Ident: CCV
Analysis from: 11/3/2023 5:58:46 PM
File: _2023-11-03_

Last save: 11/3/2023 5:27:46 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36491

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

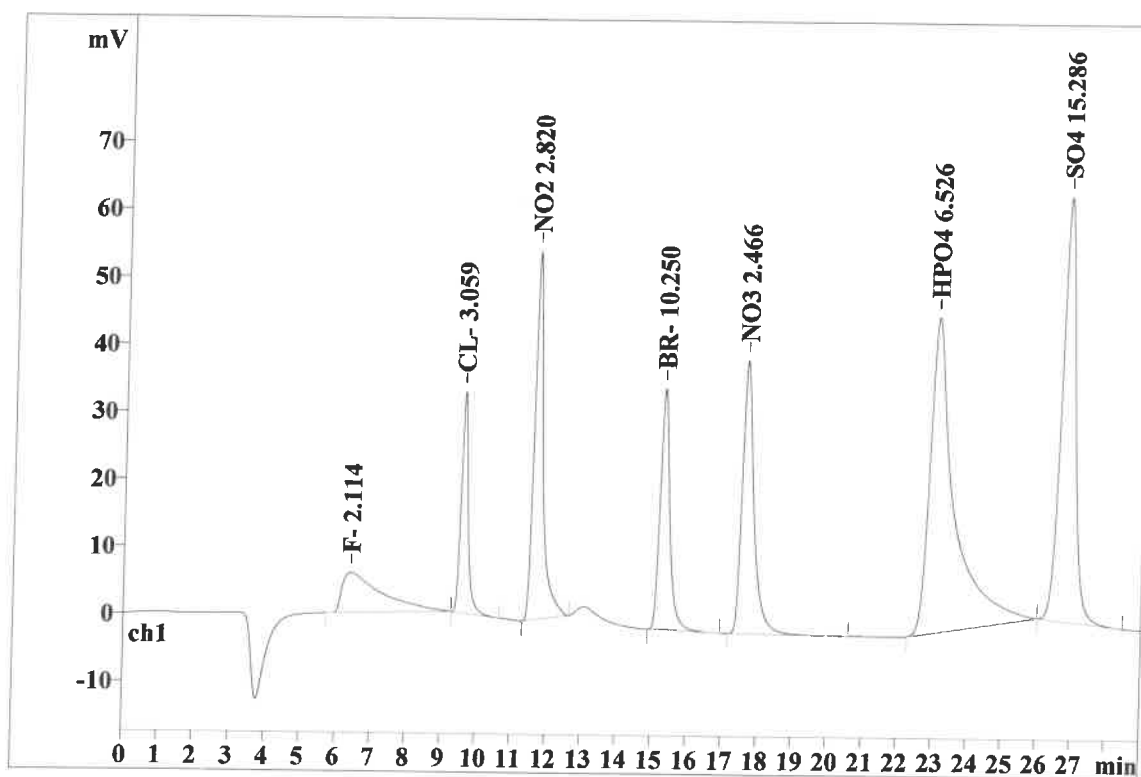

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.40	1.105	5.90	2.11	461.688	6.06
2	9.59	0.198	32.87	11.77	457.447	6.00
3	11.65	0.248	54.51	19.53	980.904	12.87
4	15.28	0.277	35.73	12.80	685.563	9.00
5	17.61	0.331	40.49	14.50	946.991	12.43
6	23.04	0.581	46.74	16.74	2297.137	30.15
7	26.80	0.425	62.91	22.54	1789.352	23.49
7	29.00	0.452	279.13	100.00	7619.082	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:27:52 AM
Printed by: wet


Ident: CCB
Analysis from: 11/3/2023 6:30:24 PM
File: _2023-11-03_

Last save: 11/3/2023 5:59:24 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36492

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

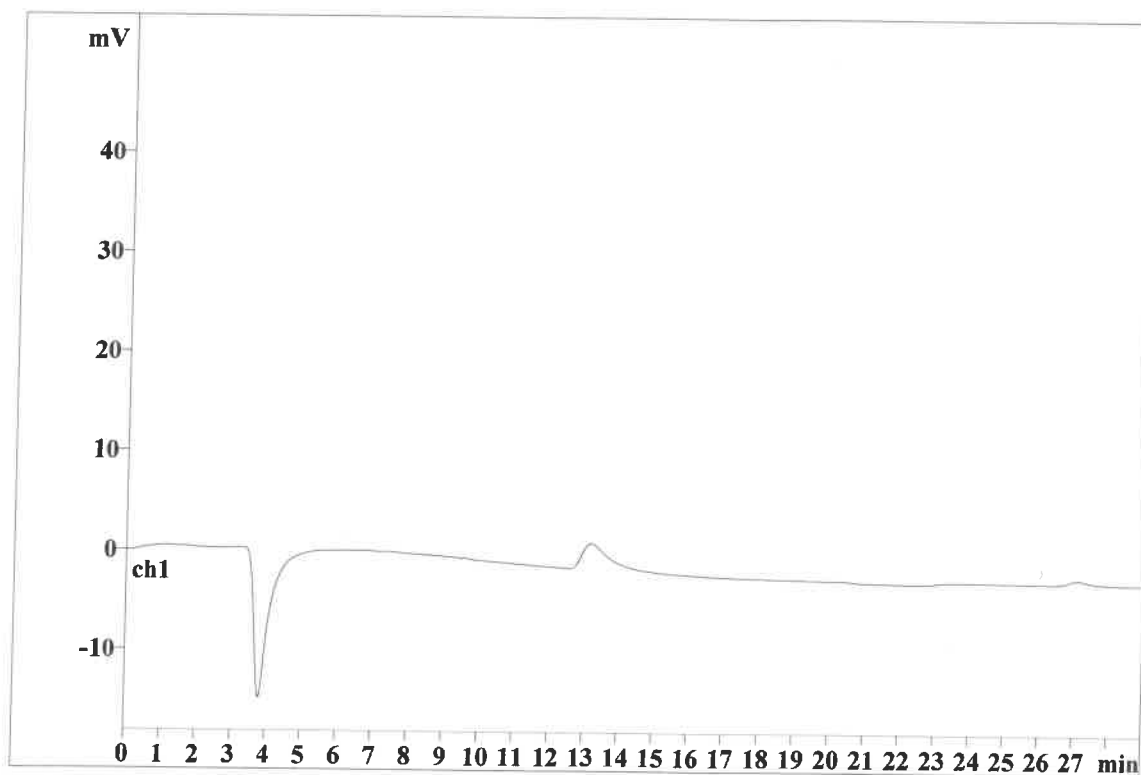

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:28:00 AM
Printed by: wet


Ident: LB128206BLW
Analysis from: 11/3/2023 7:02:02 PM
File: _2023-11-03_

Last save: 11/7/2023 9:25:53 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36493

Last save: 10/31/2023 10:3

SAMPLE:
:
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

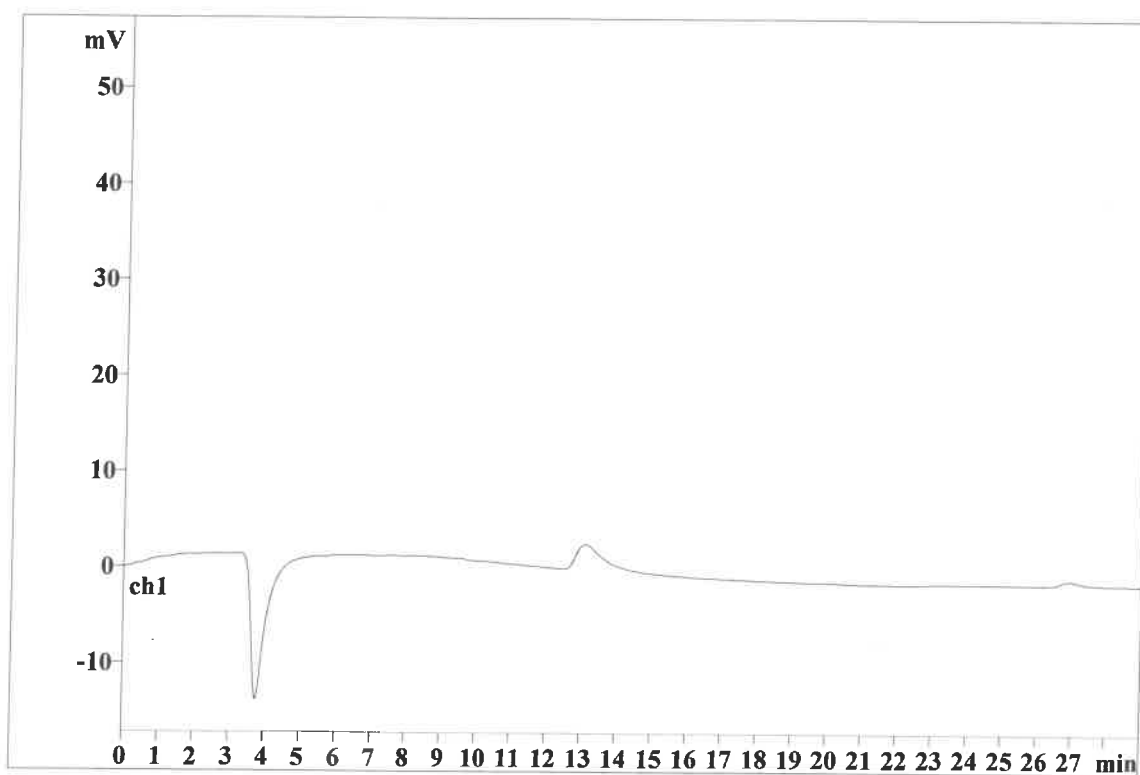

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:28:09 AM
Printed by: wet


Ident: LB128206BSW
Analysis from: 11/3/2023 7:33:40 PM
File: _2023-11-03_

Last save: 11/7/2023 9:25:53 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36494

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

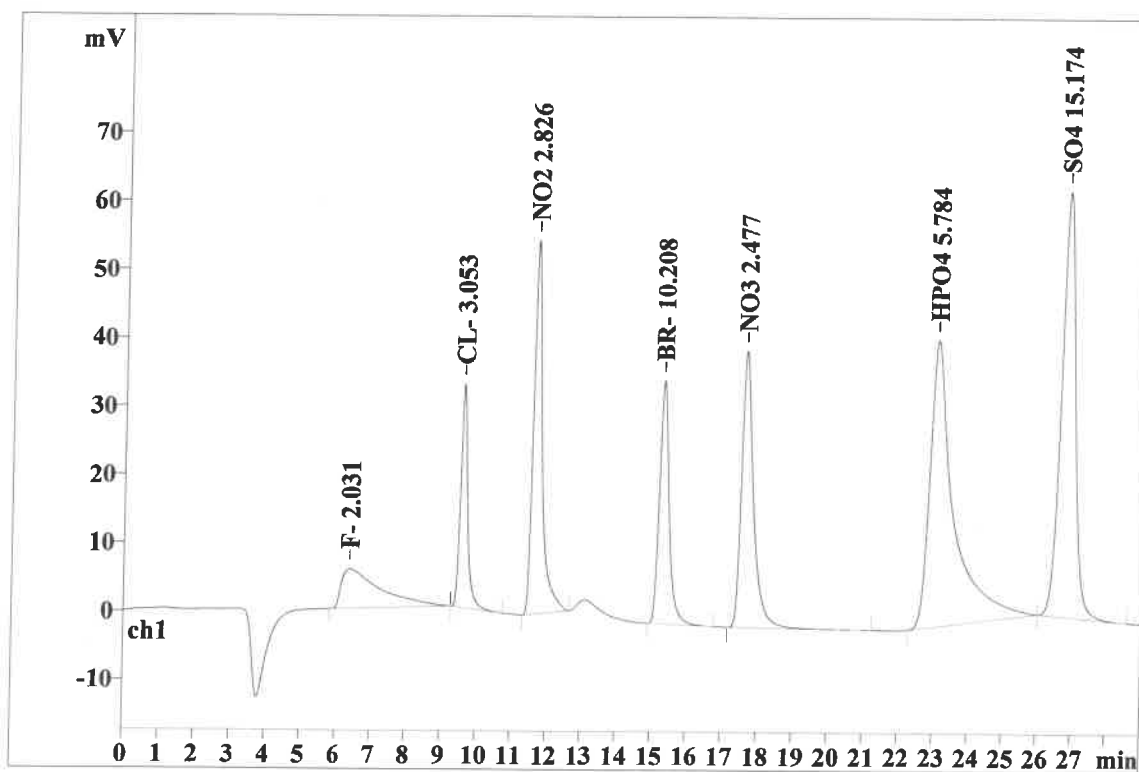

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.39	1.091	5.69	2.08	441.418	6.04
2	9.59	0.198	32.75	11.97	456.528	6.25
3	11.65	0.247	54.76	20.02	983.340	13.46
4	15.29	0.277	35.64	13.03	682.564	9.34
5	17.62	0.332	40.51	14.81	951.433	13.03
6	23.05	0.571	41.94	15.33	2013.321	27.56
7	26.81	0.426	62.25	22.76	1775.535	24.31
7	29.00	0.449	273.53	99.99	7304.139	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:28:21 AM
Printed by: wet


Ident: O5241-04
Analysis from: 11/3/2023 8:05:23 PM
File: _2023-11-03_

Last save: 11/3/2023 7:34:23 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36495

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

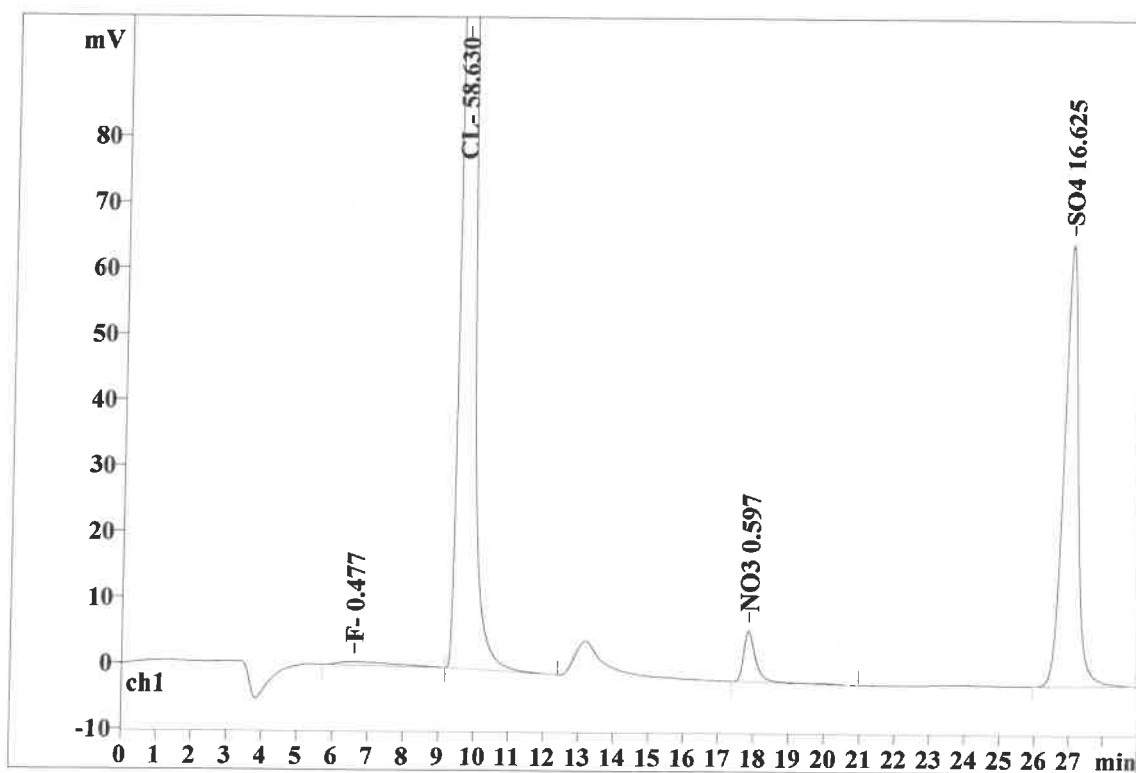

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.59	1.885	0.56	0.08	63.281	0.55
2	9.58	0.210	615.03	89.09	9260.779	80.79
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.84	0.330	7.69	1.11	184.095	1.61
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.93	0.427	67.09	9.72	1954.749	17.05
7	29.00	0.408	690.37	100.00	11462.904	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:28:29 AM
Printed by: wet


Ident: O5241-05
Analysis from: 11/3/2023 8:37:01 PM
File: _2023-11-03_

Last save: 11/3/2023 8:06:01 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36496

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

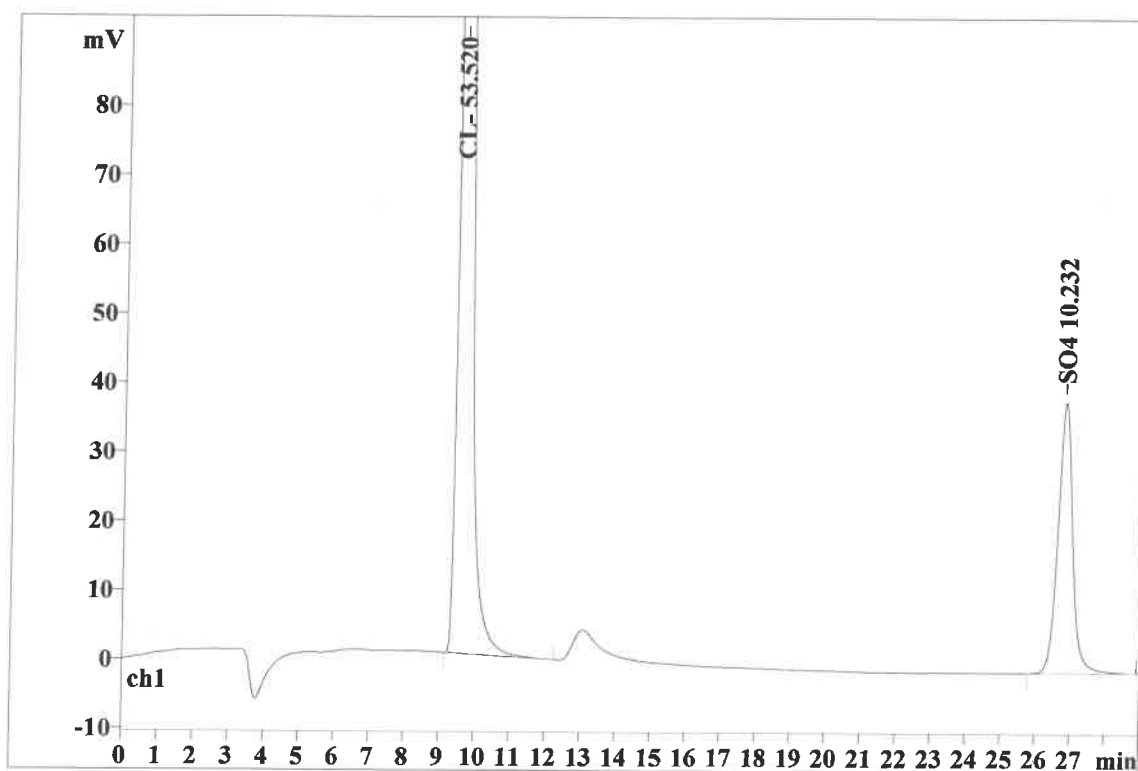

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.56	0.203	583.45	93.71	8451.327	87.89
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.80	0.435	39.18	6.29	1164.839	12.11
7	29.00	0.091	622.63	100.00	9616.166	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:28:37 AM
Printed by: wet


Ident: O5241-08
Analysis from: 11/3/2023 9:08:39 PM
File: _2023-11-03_

Last save: 11/3/2023 8:37:39 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36497

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 30
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

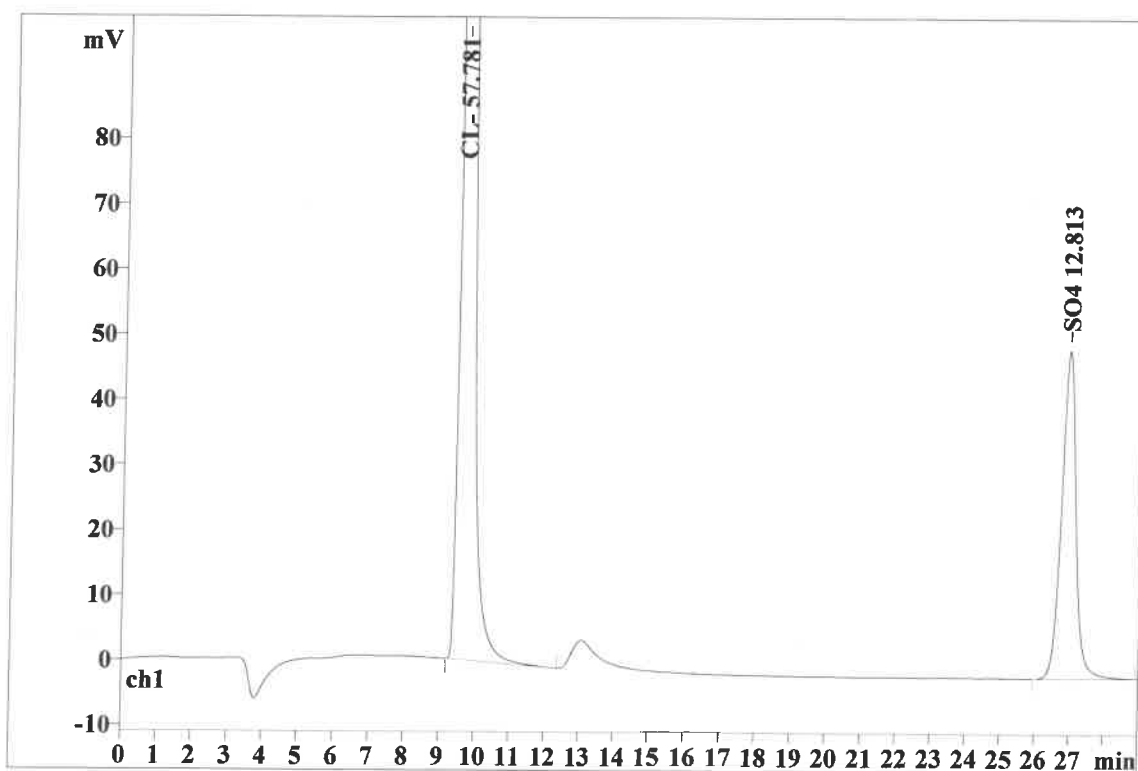

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.61	0.207	620.41	92.49	9126.252	86.02
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.92	0.432	50.40	7.51	1483.687	13.98
7	29.00	0.091	670.81	100.00	10609.938	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:40:46 AM
Printed by: wet


Ident: 05241-09
Analysis from: 11/3/2023 9:40:17 PM
File: _2023-11-03_

Last save: 11/3/2023 9:09:17 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36498

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 31
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

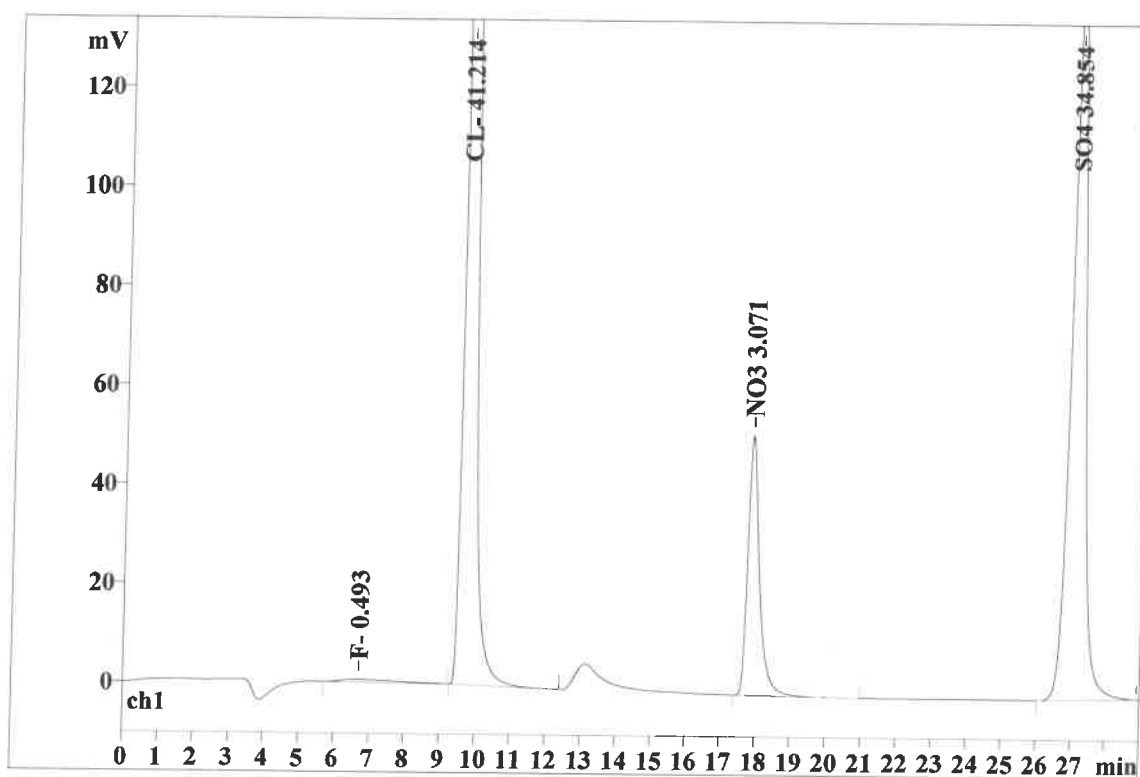

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.70	1.822	0.61	0.10	67.284	0.56
2	9.66	0.222	407.97	67.09	6501.800	54.32
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.85	0.322	52.40	8.62	1193.719	9.97
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.05	0.420	147.14	24.20	4207.351	35.15
7	29.00	0.398	608.13	100.00	11970.154	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:41:03 AM
Printed by: wet


Ident: 05241-13
Analysis from: 11/3/2023 10:11:55 PM
File: _2023-11-03_

Last save: 11/7/2023 9:40:59 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36499

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 32
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

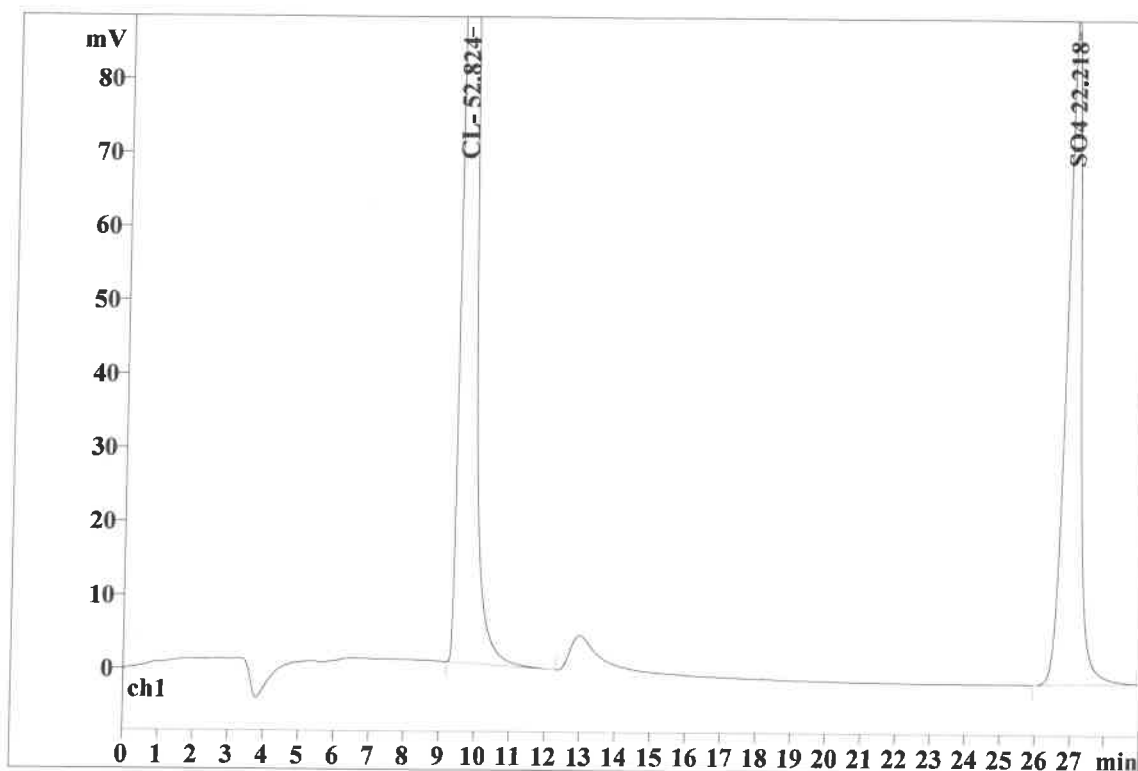

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.59	0.212	548.21	85.77	8340.999	75.92
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.93	0.426	90.91	14.22	2645.976	24.08
7	29.00	0.091	639.12	100.00	10986.975	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:41:24 AM
Printed by: wet


Ident: O5241-14
Analysis from: 11/3/2023 10:43:33 PM
File: _2023-11-03_

Last save: 11/7/2023 9:41:17 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36500

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 33
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

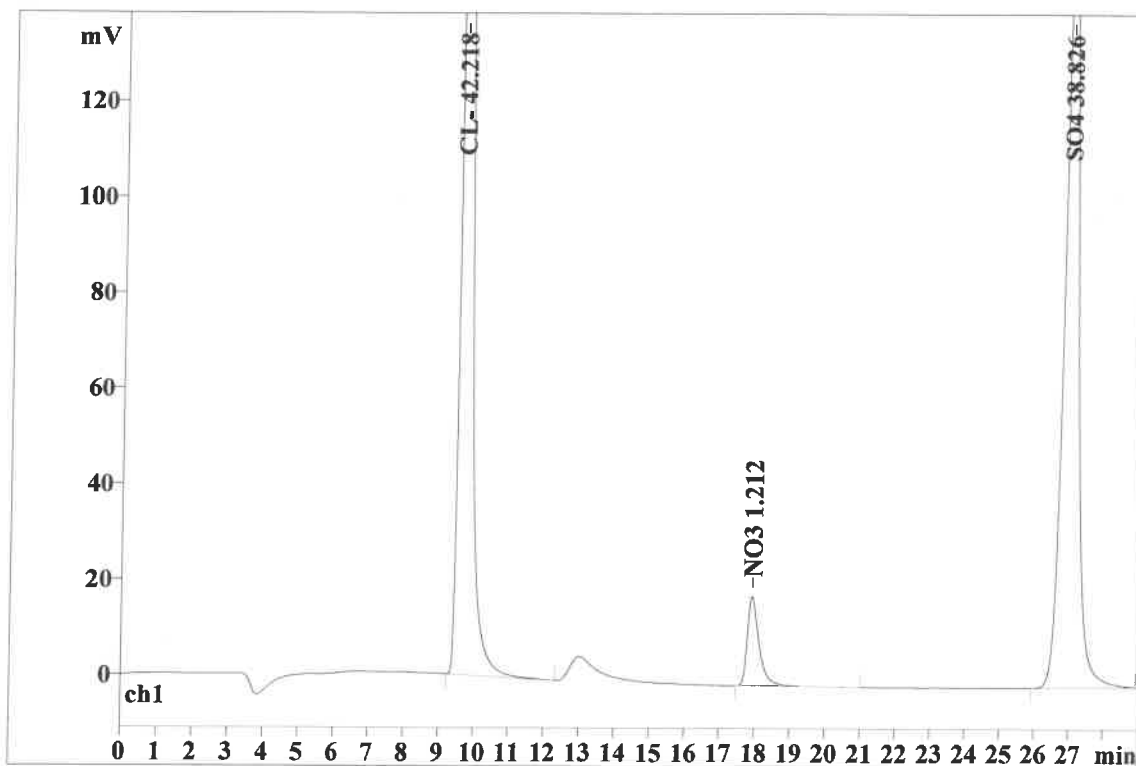

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.63	0.218	422.56	69.79	6660.923	56.47
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.91	0.331	18.71	3.09	435.320	3.69
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.93	0.419	164.17	27.12	4698.285	39.83
7	29.00	0.138	605.44	100.00	11794.528	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:41:57 AM
Printed by: wet


Ident: O5241-15MS
Analysis from: 11/3/2023 11:15:11 PM
File: _2023-11-03_

Last save: 11/7/2023 9:41:51 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36501

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 34
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

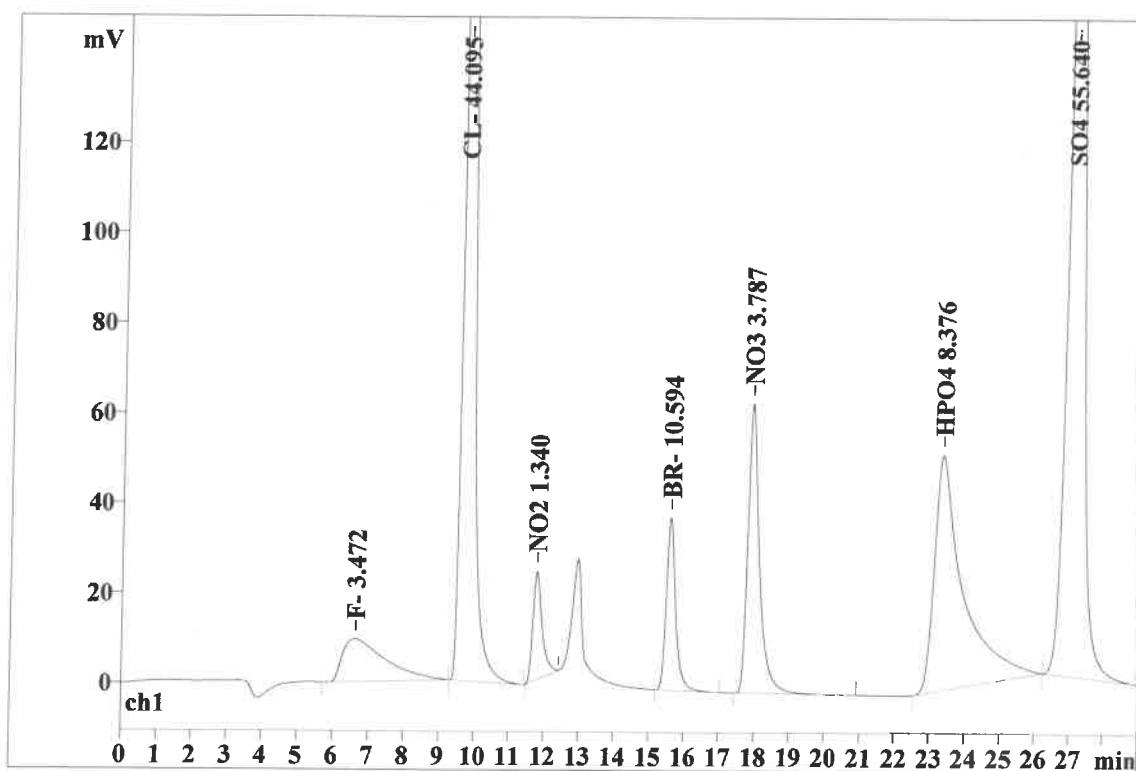

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.62	1.272	9.47	1.08	791.907	3.93
2	9.67	0.216	448.69	51.26	6958.314	34.52
3	11.78	0.260	24.02	2.74	432.013	2.14
4	15.58	0.267	38.33	4.38	710.048	3.52
5	17.88	0.325	64.21	7.34	1485.980	7.37
6	23.31	0.703	52.23	5.97	3004.412	14.90
7	27.04	0.419	238.40	27.23	6776.048	33.61
7	29.00	0.494	875.35	100.00	20158.724	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:42:22 AM
Printed by: wet


Ident: 05241-16MSD
Analysis from: 11/3/2023 11:46:48 PM
File: _2023-11-03_

Last save: 11/7/2023 9:42:18 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36502

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 35
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

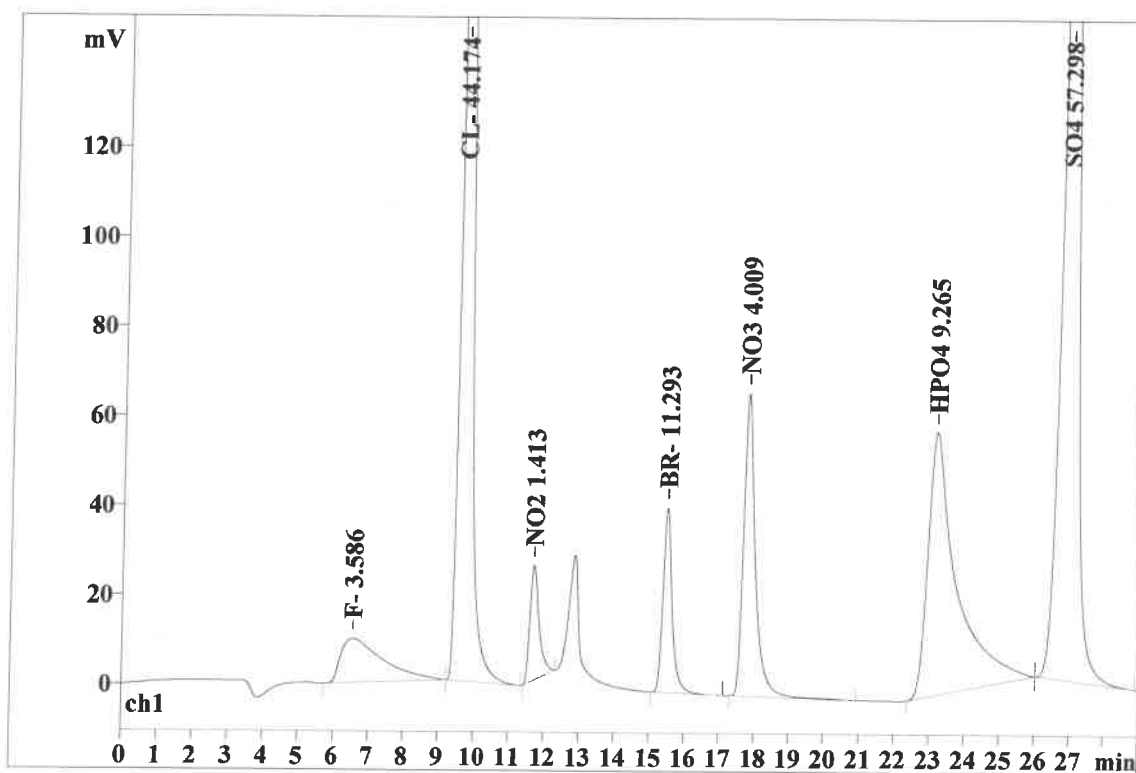

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.55	1.259	9.82	1.09	819.710	3.92
2	9.60	0.215	451.53	50.26	6970.782	33.34
3	11.68	0.257	25.81	2.87	459.031	2.20
4	15.46	0.265	41.26	4.59	759.827	3.63
5	17.75	0.324	67.62	7.53	1576.445	7.54
6	23.12	0.694	58.85	6.55	3344.425	15.99
7	26.83	0.422	243.56	27.11	6980.878	33.38
7	29.00	0.491	898.45	100.00	20911.100	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:42:31 AM
Printed by: wet


Ident: CCV
Analysis from: 11/4/2023 12:18:34 AM
File: _2023-11-04_

Last save: 11/3/2023 11:47:35 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36503

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

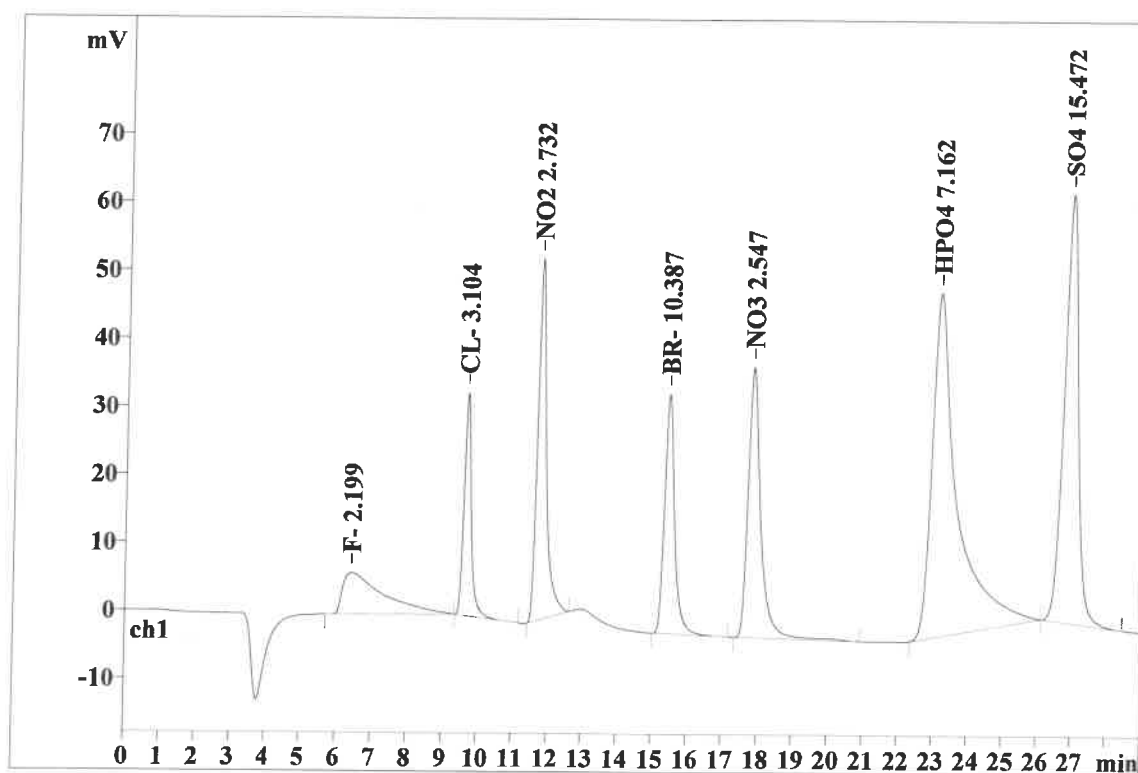

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.42	1.116	6.08	2.17	482.259	6.09
2	9.65	0.201	32.77	11.69	464.562	5.86
3	11.73	0.252	53.15	18.95	948.356	11.97
4	15.41	0.284	35.17	12.54	695.282	8.78
5	17.79	0.340	39.71	14.16	980.181	12.37
6	23.11	0.596	50.51	18.01	2540.280	32.06
7	26.88	0.429	63.00	22.47	1812.268	22.87
7	29.00	0.460	280.39	100.00	7923.188	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:42:39 AM
Printed by: wet


Ident: CCB
Analysis from: 11/4/2023 12:50:12 AM
File: _2023-11-04_

Last save: 11/4/2023 12:19:12 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36504

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

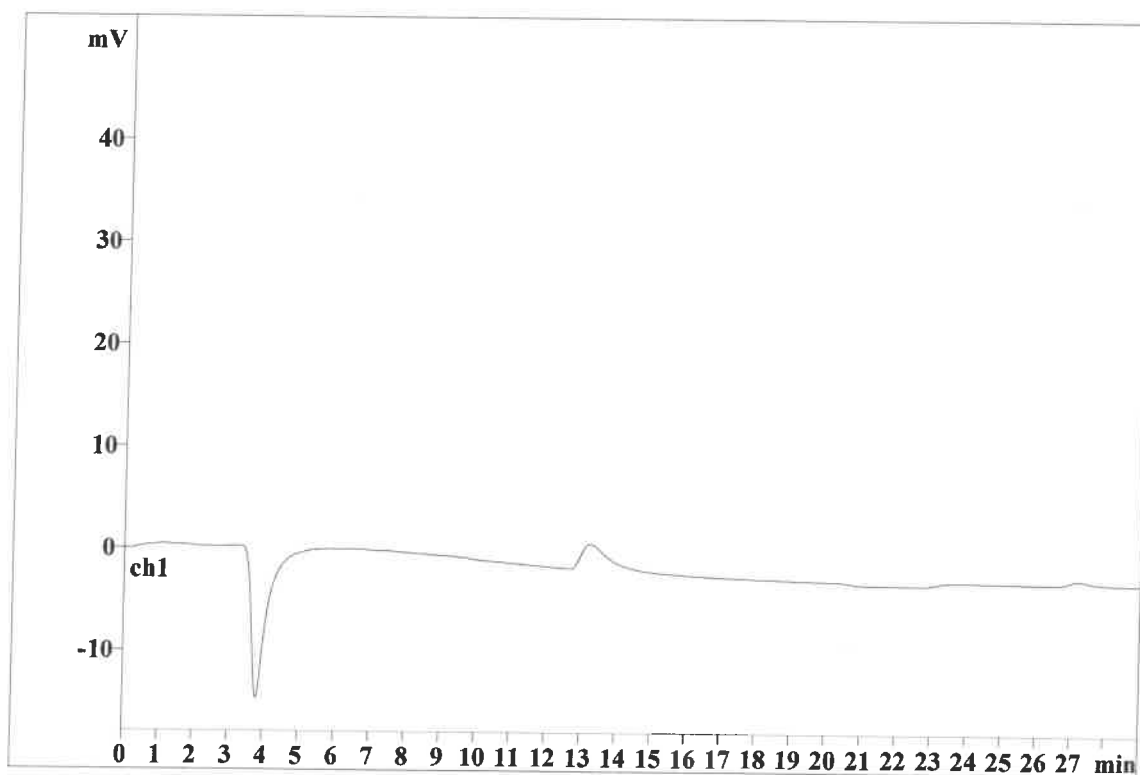

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:42:48 AM
Printed by: wet


Ident: O5241-17
Analysis from: 11/4/2023 1:21:58 AM
File: _2023-11-04_

Last save: 11/4/2023 12:50:58 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36505

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 36
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

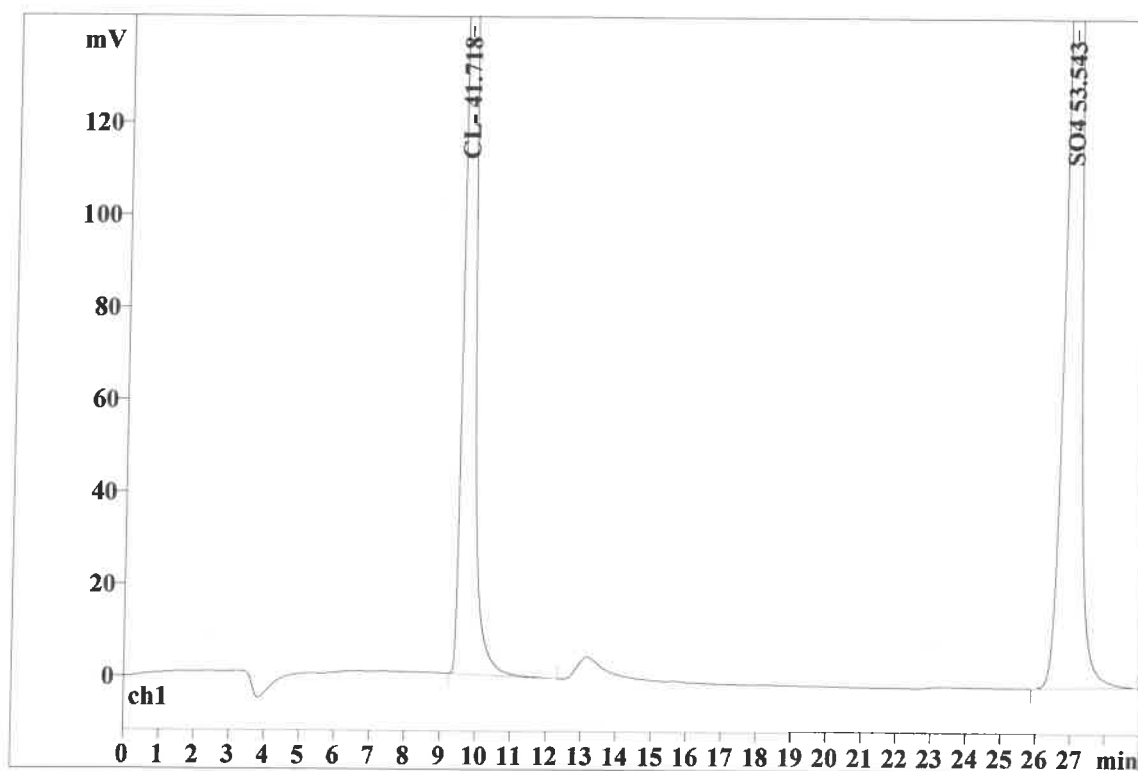

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.63	0.209	436.65	65.52	6581.656	50.25
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.89	0.417	229.80	34.48	6516.902	49.75
7	29.00	0.089	666.45	100.00	13098.558	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:42:58 AM
Printed by: wet


Ident: O5241-18
Analysis from: 11/4/2023 1:53:36 AM
File: _2023-11-04_

Last save: 11/4/2023 1:22:36 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36506

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 37
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

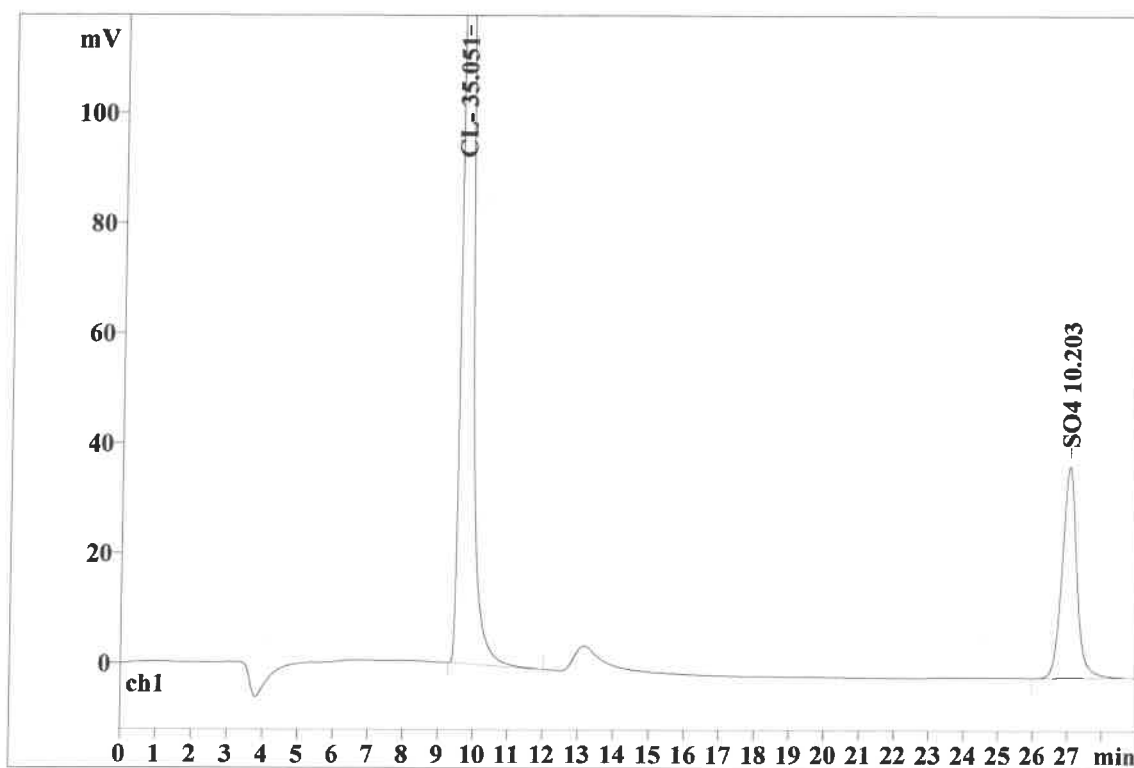

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.66	0.210	364.51	90.45	5525.467	82.63
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.01	0.441	38.46	9.54	1161.196	17.37
7	29.00	0.093	402.98	100.00	6686.663	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:43:06 AM
Printed by: wet


Ident: O5241-19
Analysis from: 11/4/2023 2:25:15 AM
File: _2023-11-04_

Last save: 11/4/2023 1:54:15 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36507

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 38
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

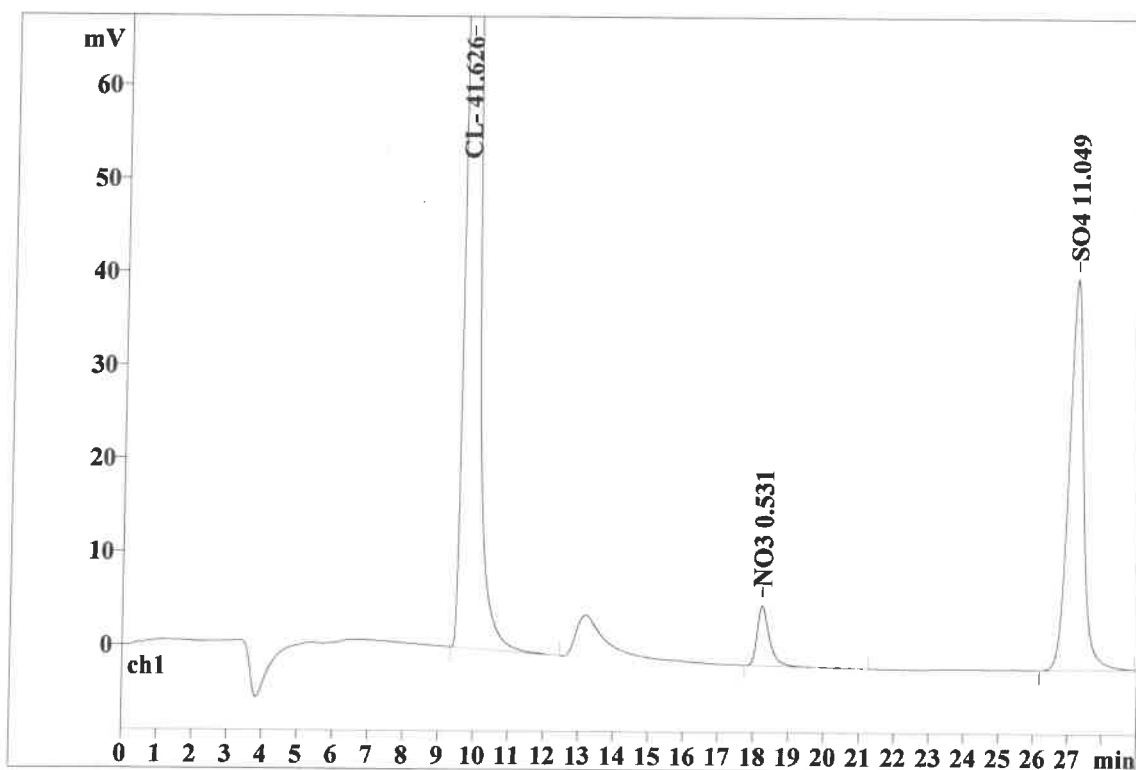

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.72	0.211	431.88	89.94	6567.069	82.19
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	18.22	0.346	6.44	1.34	157.126	1.97
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.14	0.442	41.88	8.72	1265.746	15.84
7	29.00	0.143	480.21	100.00	7989.941	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:43:13 AM
Printed by: wet


Ident: 05241-20
Analysis from: 11/4/2023 2:56:52 AM
File: _2023-11-04_

Last save: 11/4/2023 2:25:53 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36508

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 39
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

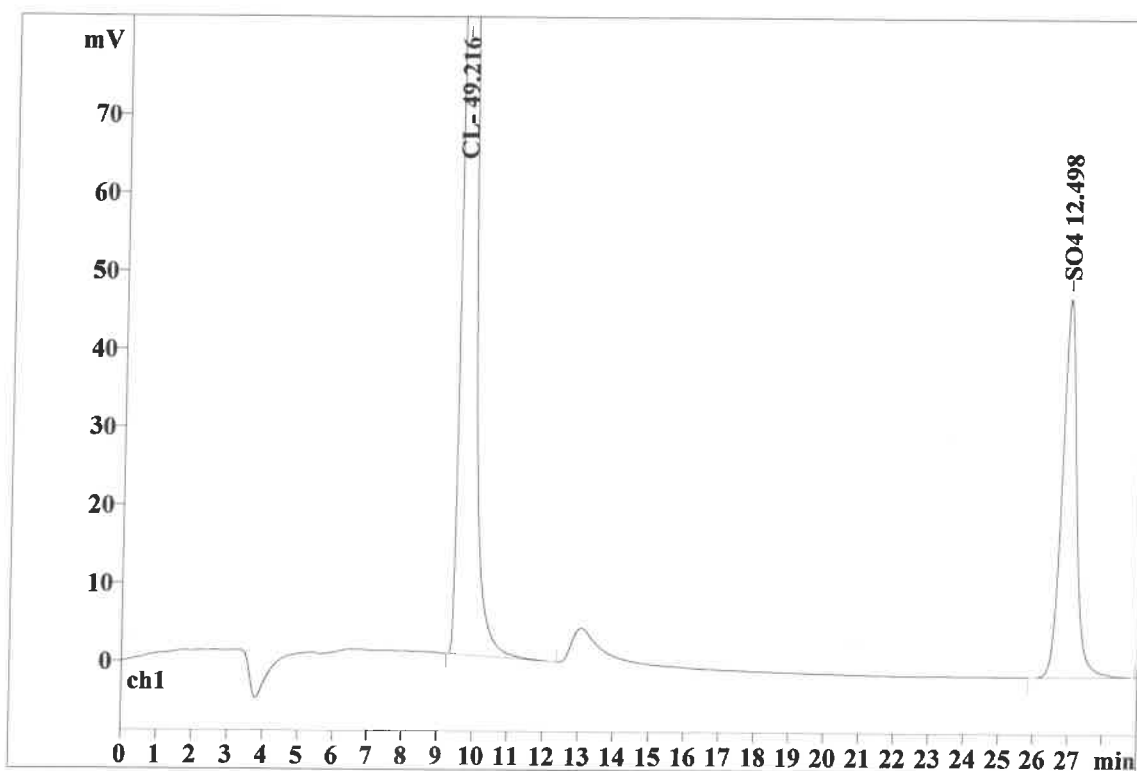

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.65	0.210	516.87	91.42	7769.560	84.32
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.94	0.437	48.48	8.58	1444.776	15.68
7	29.00	0.092	565.36	100.00	9214.336	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:43:20 AM
Printed by: wet


Ident: 05241-22
Analysis from: 11/4/2023 3:28:30 AM
File: _2023-11-04_

Last save: 11/4/2023 2:57:30 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36509

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 40
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

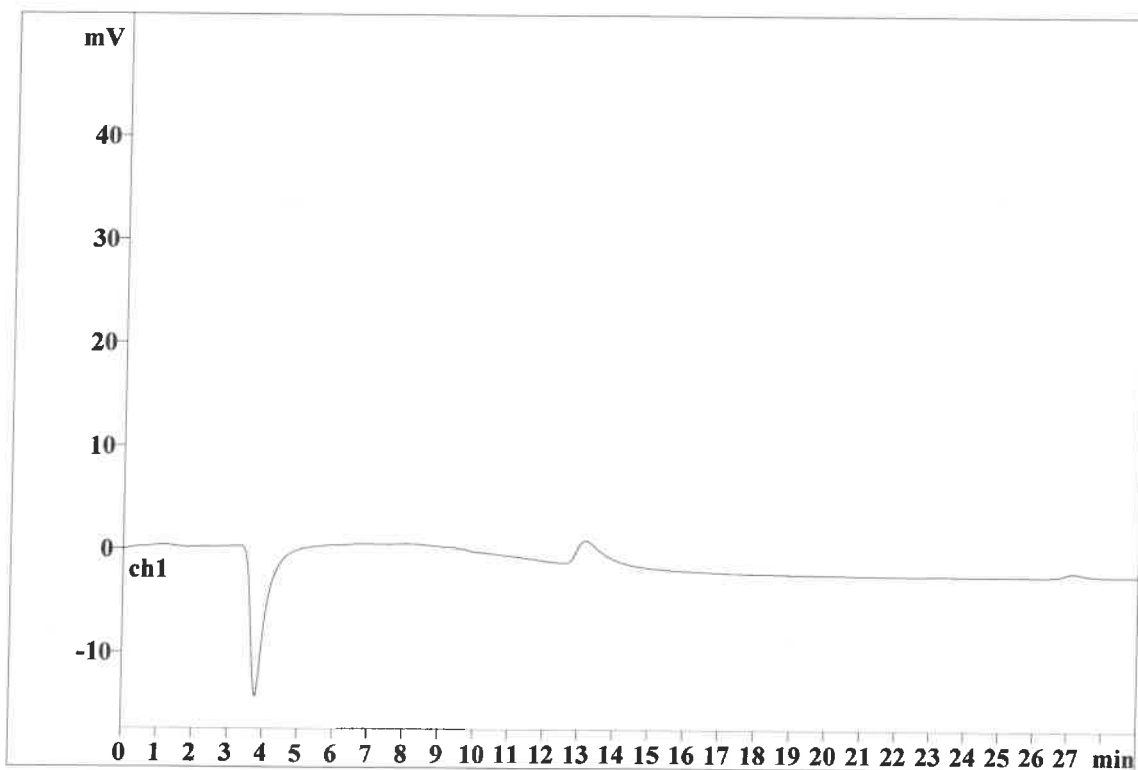

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:43:27 AM
Printed by: wet


Ident: 05241-23
Analysis from: 11/4/2023 4:00:08 AM
File: _2023-11-04_

Last save: 11/4/2023 3:29:09 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36510

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 41
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

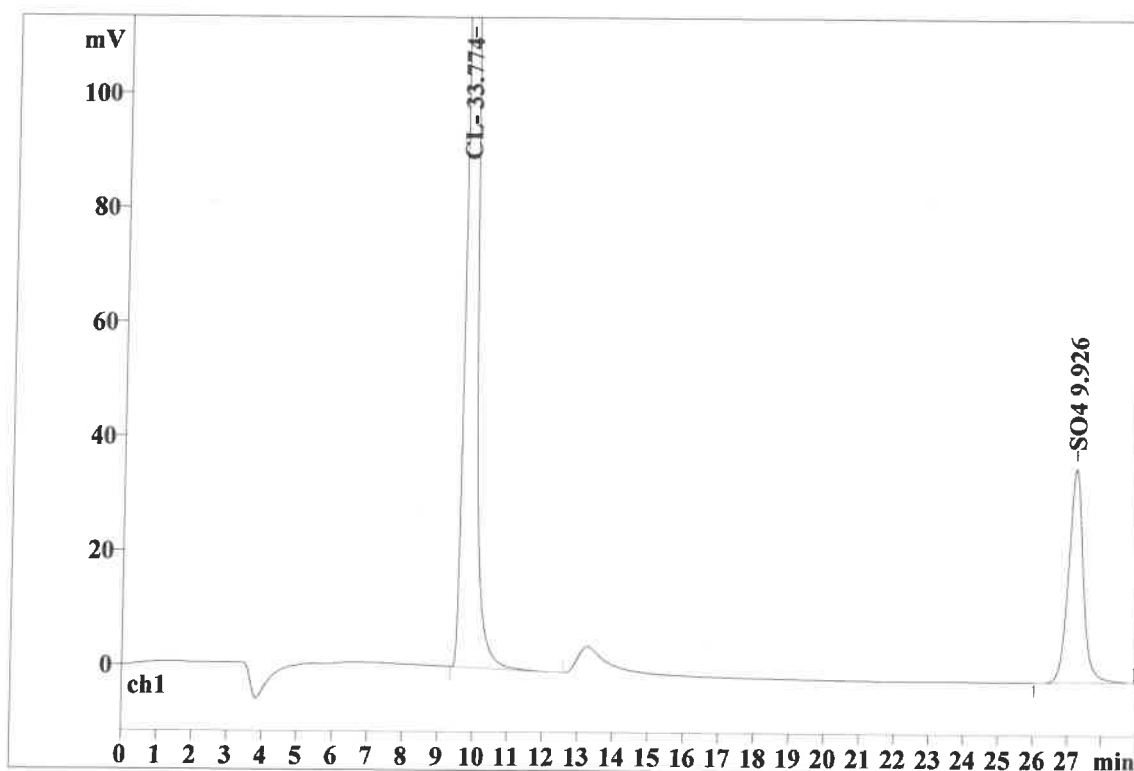

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.74	0.211	351.16	90.38	5323.229	82.53
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.18	0.443	37.36	9.62	1127.011	17.47
7	29.00	0.093	388.52	100.00	6450.240	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:43:49 AM
Printed by: wet


Ident: O5241-23MS
Analysis from: 11/4/2023 4:31:47 AM
File: _2023-11-04_

Last save: 11/7/2023 9:43:45 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36511

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 42
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

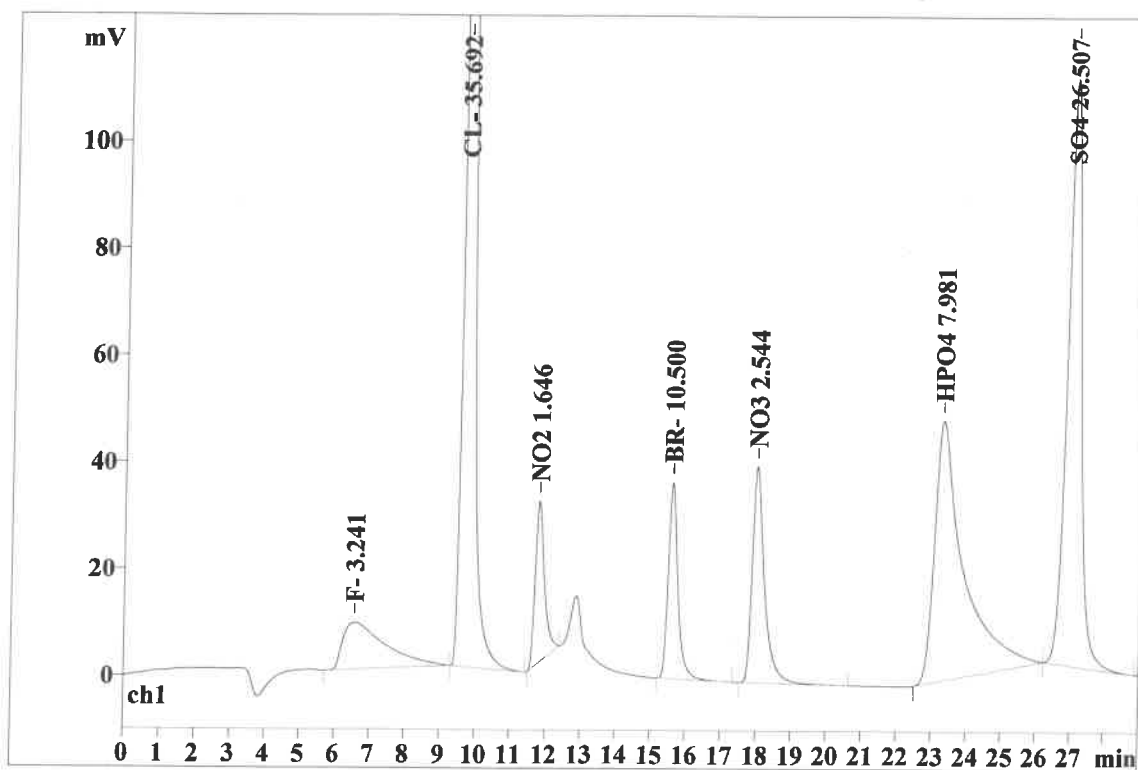

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.56	1.271	8.73	1.34	735.904	5.03
2	9.66	0.208	376.06	57.77	5627.056	38.49
3	11.78	0.263	30.38	4.67	545.523	3.73
4	15.59	0.275	36.73	5.64	703.339	4.81
5	17.98	0.340	40.51	6.22	978.657	6.69
6	23.27	0.717	48.78	7.49	2853.429	19.52
7	27.01	0.427	109.82	16.87	3175.883	21.72
7	29.00	0.500	651.01	100.00	14619.791	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:44:19 AM
Printed by: wet


Ident: O5241-23MSD
Analysis from: 11/4/2023 5:03:24 AM
File: _2023-11-04_

Last save: 11/7/2023 9:44:16 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36512

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 43
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

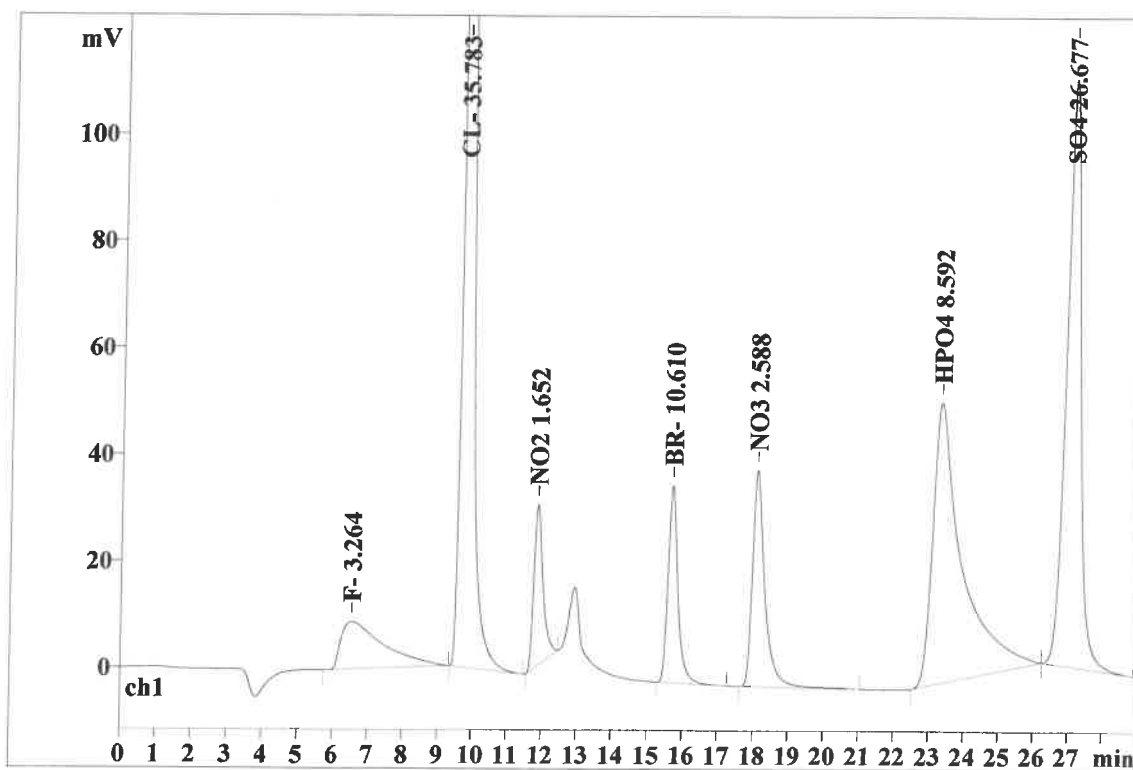

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.53	1.242	8.84	1.35	741.433	4.97
2	9.70	0.208	376.43	57.42	5641.542	37.80
3	11.84	0.266	30.30	4.62	548.025	3.67
4	15.66	0.276	36.97	5.64	711.164	4.77
5	18.06	0.340	40.57	6.19	996.764	6.68
6	23.29	0.719	52.61	8.02	3086.942	20.69
7	27.05	0.429	109.88	16.76	3197.003	21.42
7	29.00	0.497	655.60	100.00	14922.872	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:44:34 AM
Printed by: wet


Ident: CCV
Analysis from: 11/4/2023 5:35:10 AM
File: _2023-11-04_

Last save: 11/7/2023 9:44:31 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36513

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

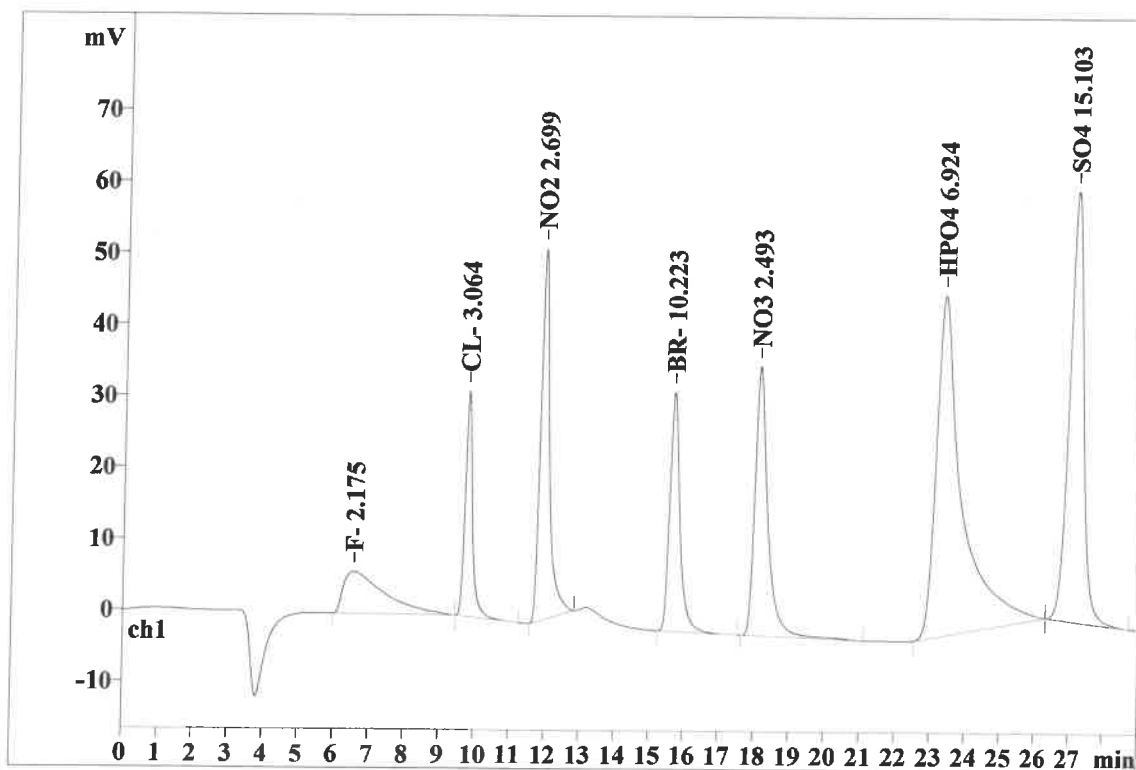

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.56	1.206	5.87	2.18	476.325	6.16
2	9.77	0.205	31.57	11.75	458.290	5.93
3	11.89	0.251	51.99	19.35	935.969	12.11
4	15.65	0.292	33.51	12.47	683.602	8.85
5	18.08	0.350	37.75	14.05	957.856	12.39
6	23.30	0.612	47.69	17.75	2449.190	31.69
7	27.11	0.437	60.27	22.43	1766.657	22.86
7	29.00	0.479	268.65	100.00	7727.890	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:44:43 AM
Printed by: wet


Ident: CCB
Analysis from: 11/4/2023 6:06:48 AM
File: _2023-11-04_

Last save: 11/4/2023 5:35:48 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36514

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

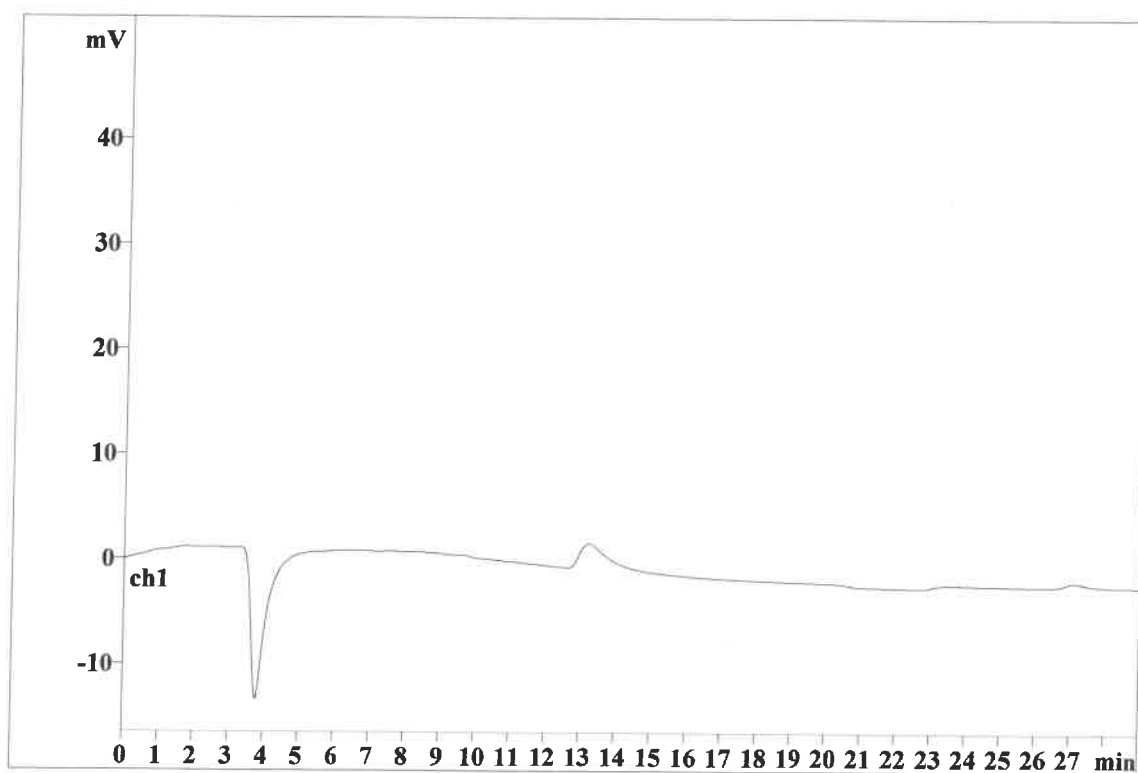

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:26:03 AM
Printed by: wet


Ident: CCV
Analysis from: 11/6/2023 9:53:38 AM
File: _2023-11-06_

Last save: 11/6/2023 10:25:01 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36518

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

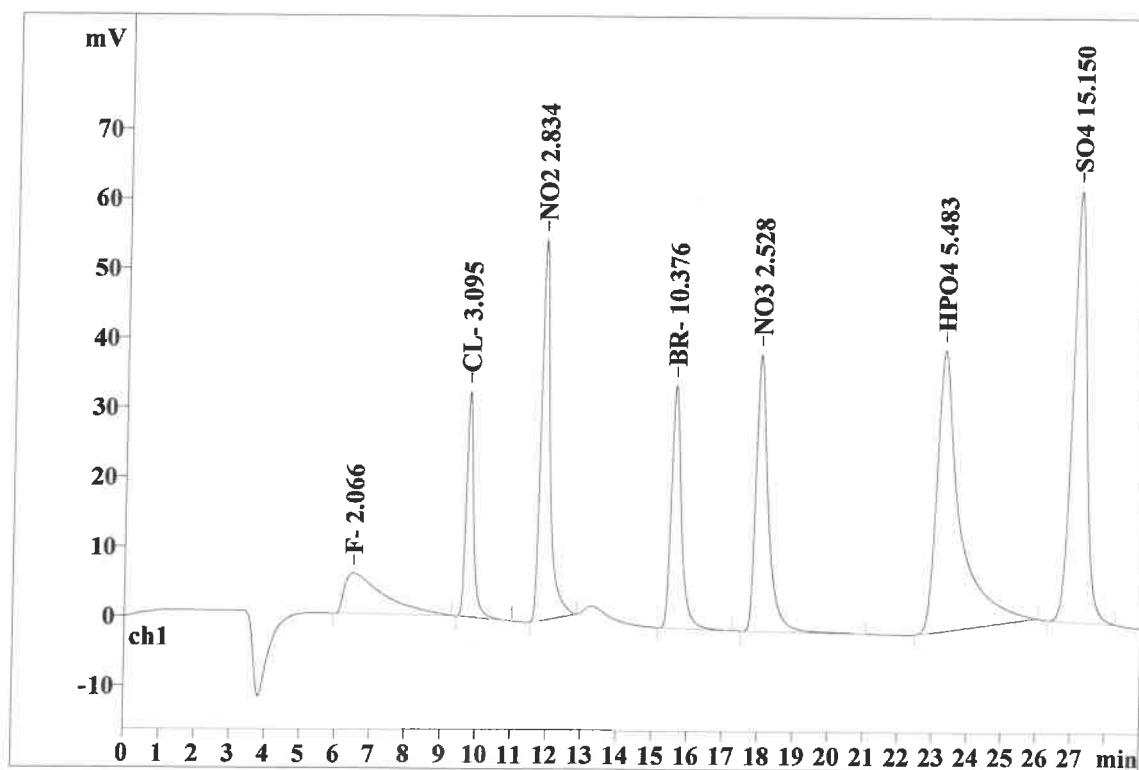

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.49	1.126	5.81	2.15	450.027	6.22
2	9.74	0.203	32.44	12.02	463.141	6.40
3	11.84	0.251	54.69	20.26	985.993	13.62
4	15.58	0.285	34.91	12.93	694.525	9.60
5	17.99	0.341	39.79	14.74	972.369	13.44
6	23.25	0.565	40.39	14.96	1898.331	26.23
7	27.14	0.429	61.93	22.94	1772.536	24.49
7	29.00	0.457	269.96	100.00	7236.922	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:26:10 AM
Printed by: wet


Ident: CCB
Analysis from: 11/6/2023 10:27:49 AM
File: _2023-11-06_

Last save: 11/6/2023 10:56:49 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36519

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

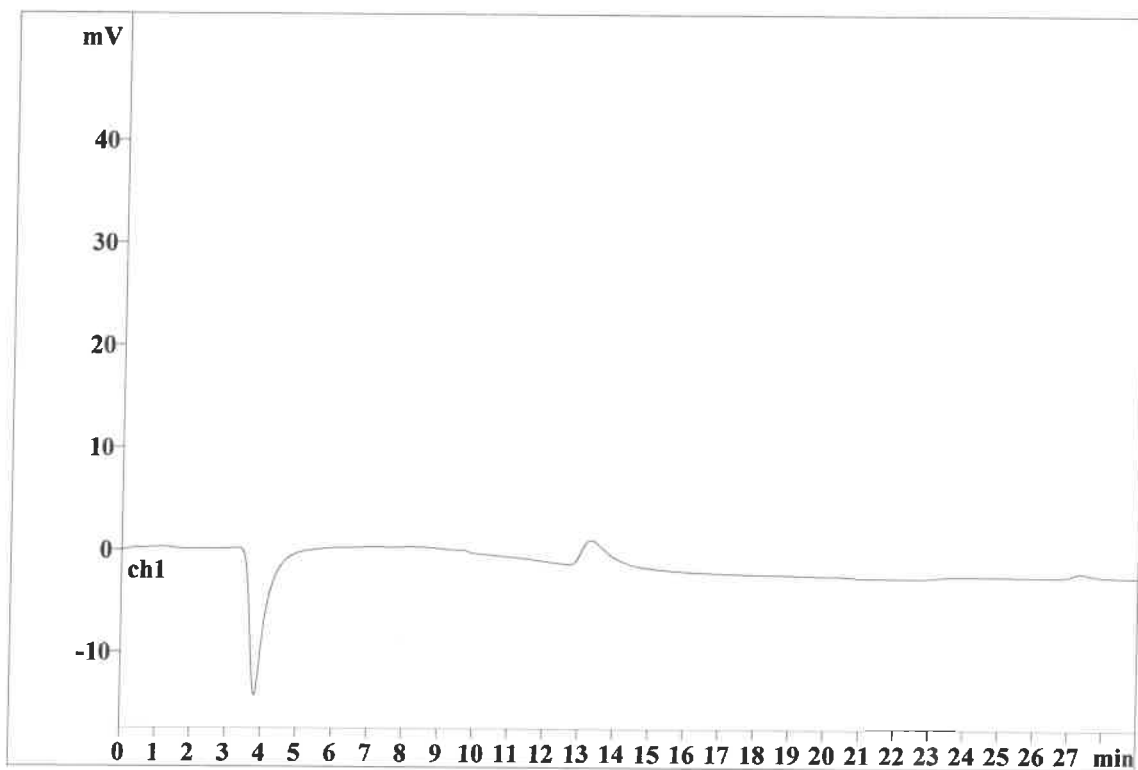

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:26:17 AM
Printed by: wet


Ident: LB128206BLW2
Analysis from: 11/6/2023 10:59:26 AM
File: _2023-11-06_

Last save: 11/7/2023 9:25:53 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36520

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

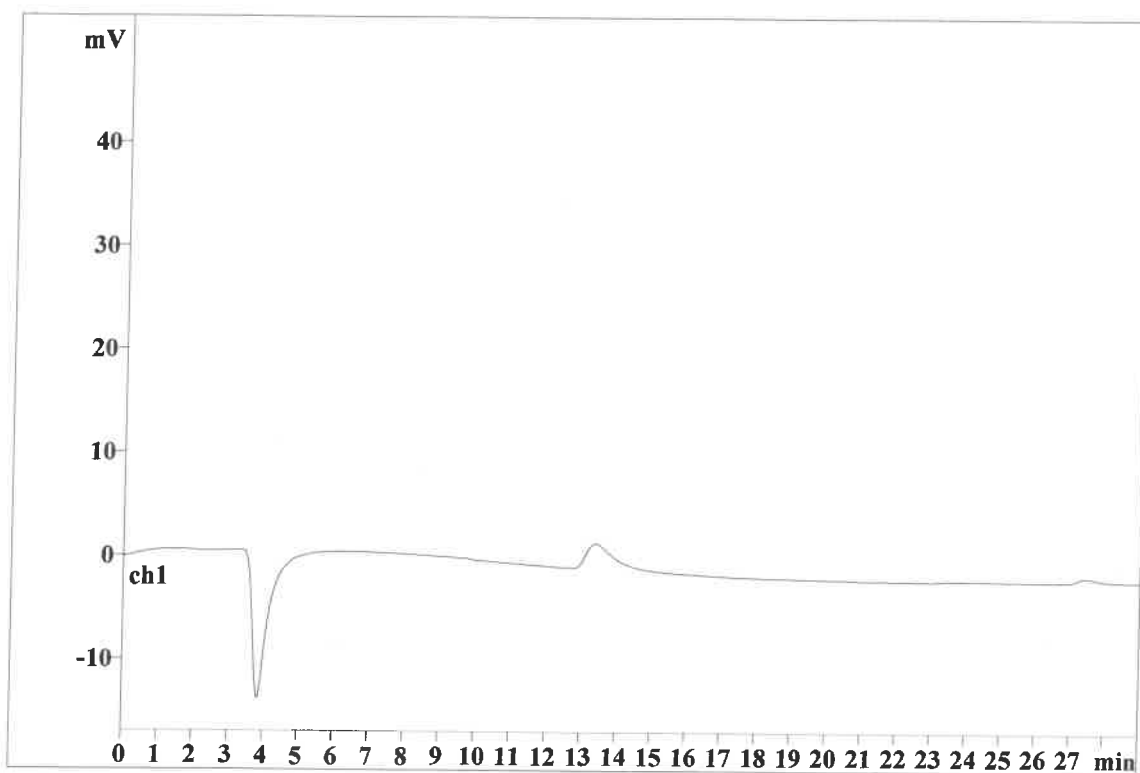

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:26:24 AM
Printed by: wet


Ident: LB128206BSW2
Analysis from: 11/6/2023 11:31:05 AM
File: _2023-11-06_

Last save: 11/7/2023 9:25:53 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36521

Last save: 10/31/2023 10:3

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

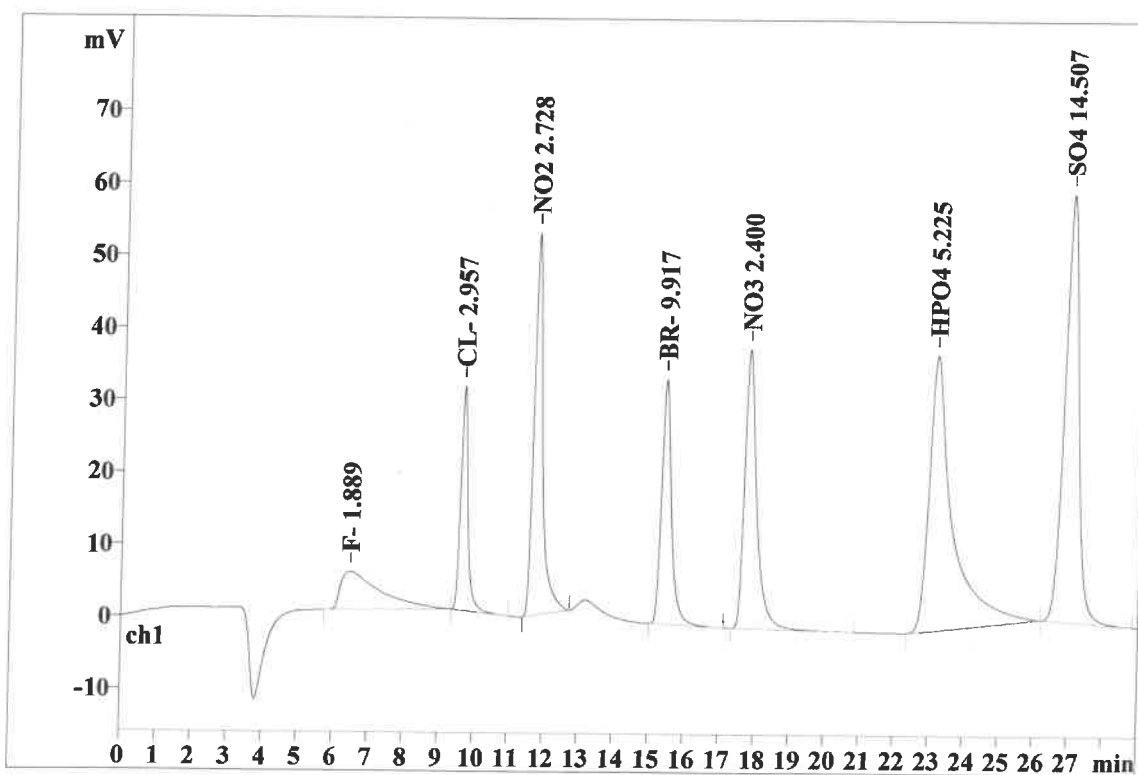

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.47	1.117	5.26	2.03	406.817	5.92
2	9.66	0.201	31.12	12.01	441.297	6.42
3	11.73	0.246	52.95	20.43	946.821	13.78
4	15.41	0.282	33.85	13.06	661.824	9.63
5	17.76	0.336	38.65	14.92	919.807	13.39
6	23.14	0.563	38.08	14.70	1799.416	26.20
7	26.99	0.427	59.20	22.85	1693.070	24.65
7	29.00	0.453	259.12	100.00	6869.052	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:45:11 AM
Printed by: wet


Ident: O5241-04DLX10
Analysis from: 11/6/2023 12:02:44 PM
File: _2023-11-06_

Last save: 11/7/2023 9:45:05 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36522

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

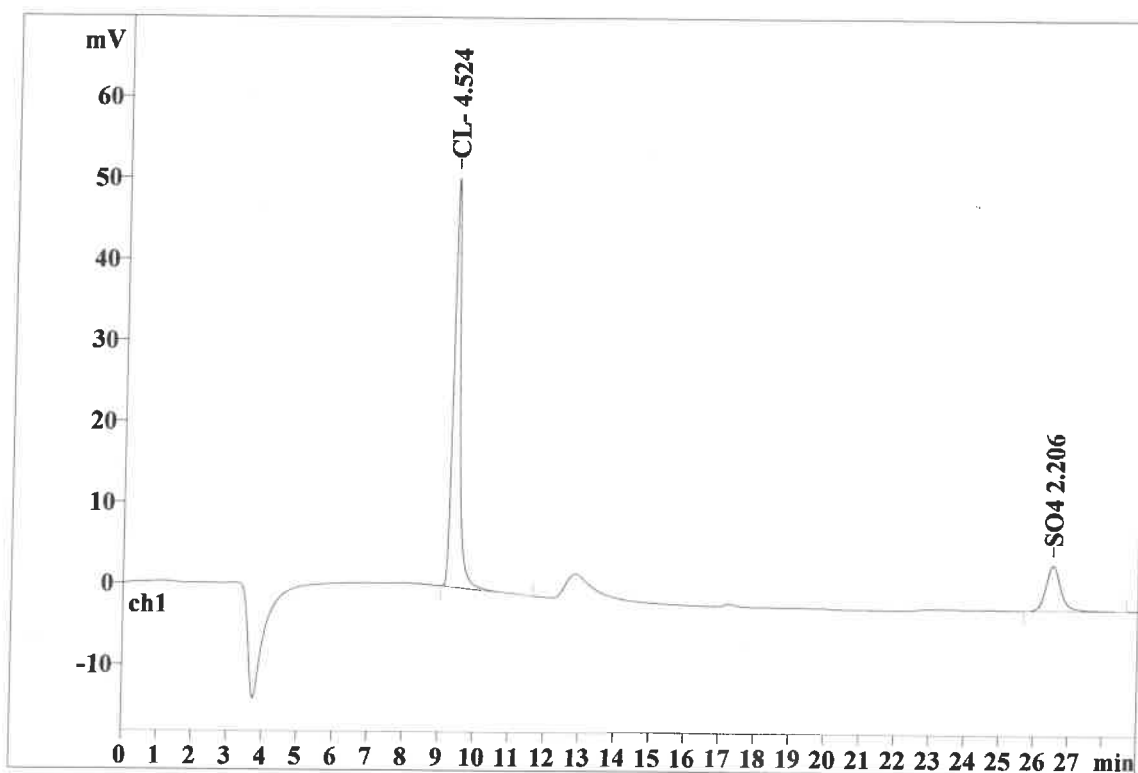

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.37	0.191	50.47	89.99	689.554	79.95
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.51	0.445	5.61	10.01	172.960	20.05
7	29.00	0.091	56.08	100.00	862.514	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:45:24 AM
Printed by: wet


Ident: 05241-05DLX10
Analysis from: 11/6/2023 12:34:22 PM
File: _2023-11-06_

Last save: 11/7/2023 9:45:23 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36523

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

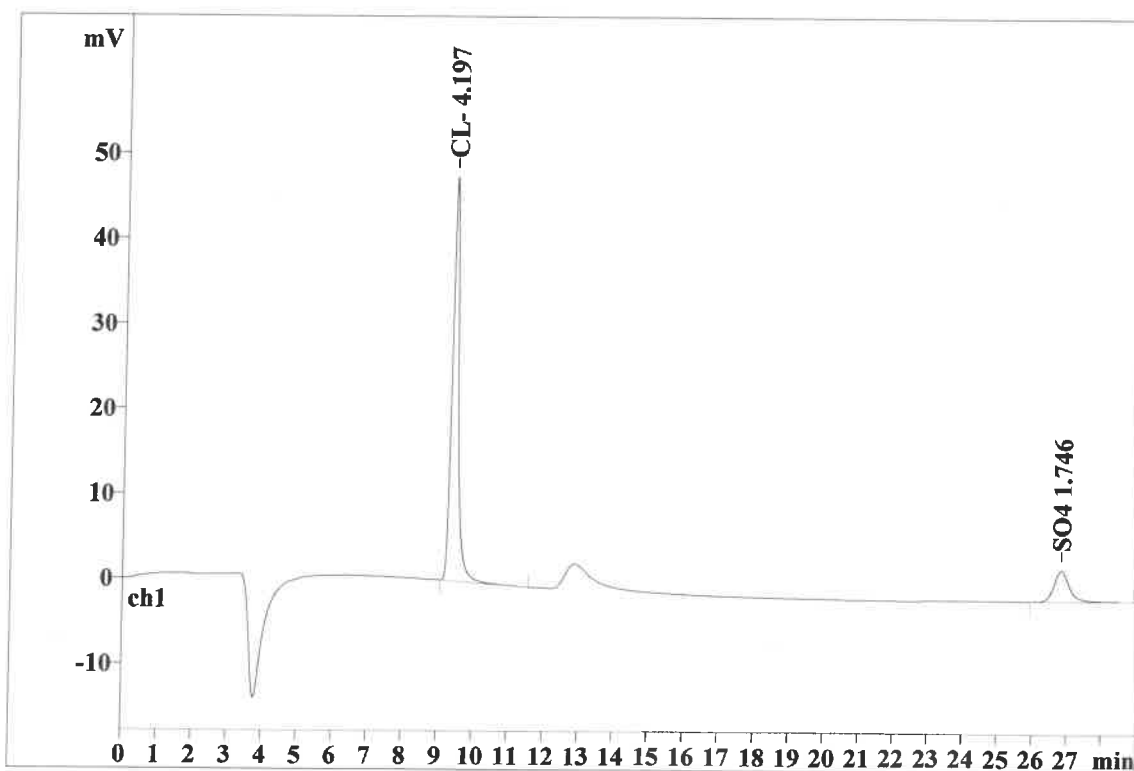

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.38	0.190	47.51	92.84	637.694	84.60
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.80	0.454	3.66	7.16	116.082	15.40
7	29.00	0.092	51.17	100.00	753.776	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:46:15 AM
Printed by: wet

Ident: O5241-08DLX10
Analysis from: 11/6/2023 1:06:00 PM
File: _2023-11-06_

Last save: 11/7/2023 9:46:13 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36524

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.24	0.186	53.14	91.74	703.682	82.51
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.68	0.452	4.78	8.26	149.167	17.49
7	29.00	0.091	57.93	100.00	852.849	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:46:36 AM
Printed by: wet


Ident: O5241-09DLX10
Analysis from: 11/6/2023 1:37:38 PM
File: _2023-11-06_

Last save: 11/7/2023 9:46:33 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36525

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

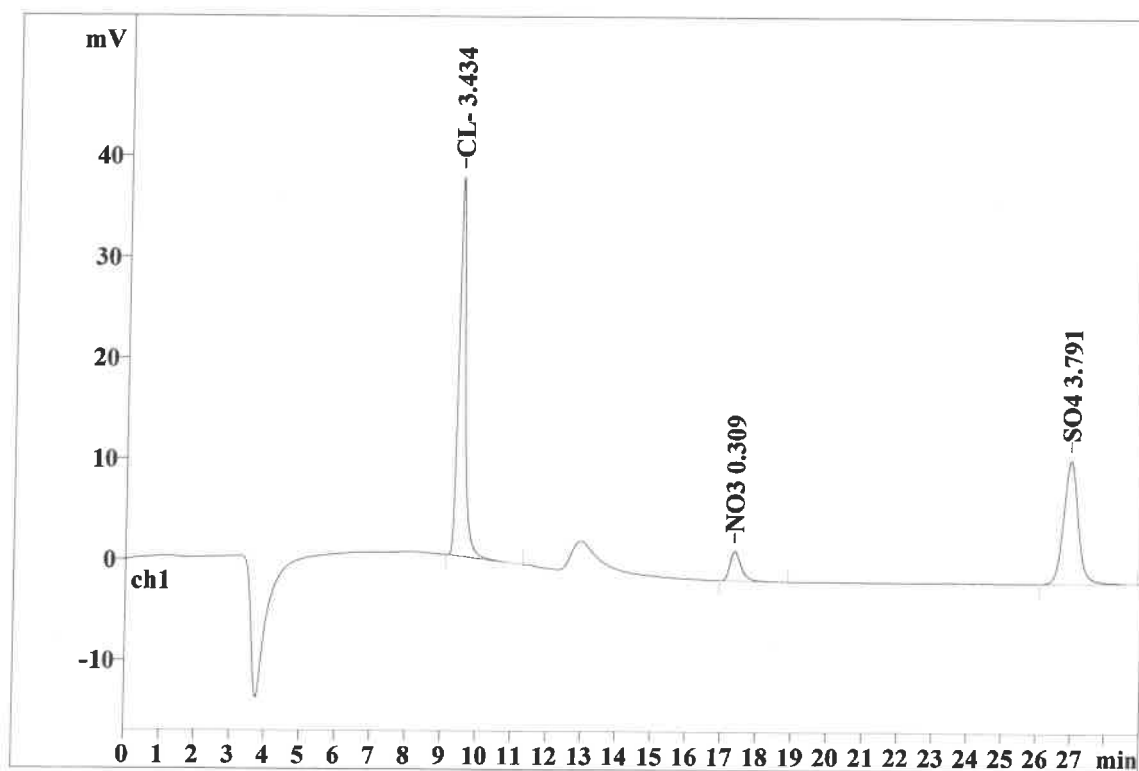

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.45	0.195	37.62	71.27	516.872	54.26
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.35	0.333	2.92	5.53	66.783	7.01
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.94	0.444	12.24	23.19	368.873	38.73
7	29.00	0.139	52.78	100.00	952.529	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:50:43 AM
Printed by: wet


Ident: O5241-14DLX2
Analysis from: 11/6/2023 2:40:54 PM
File: _2023-11-06_

Last save: 11/6/2023 3:09:54 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36527

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

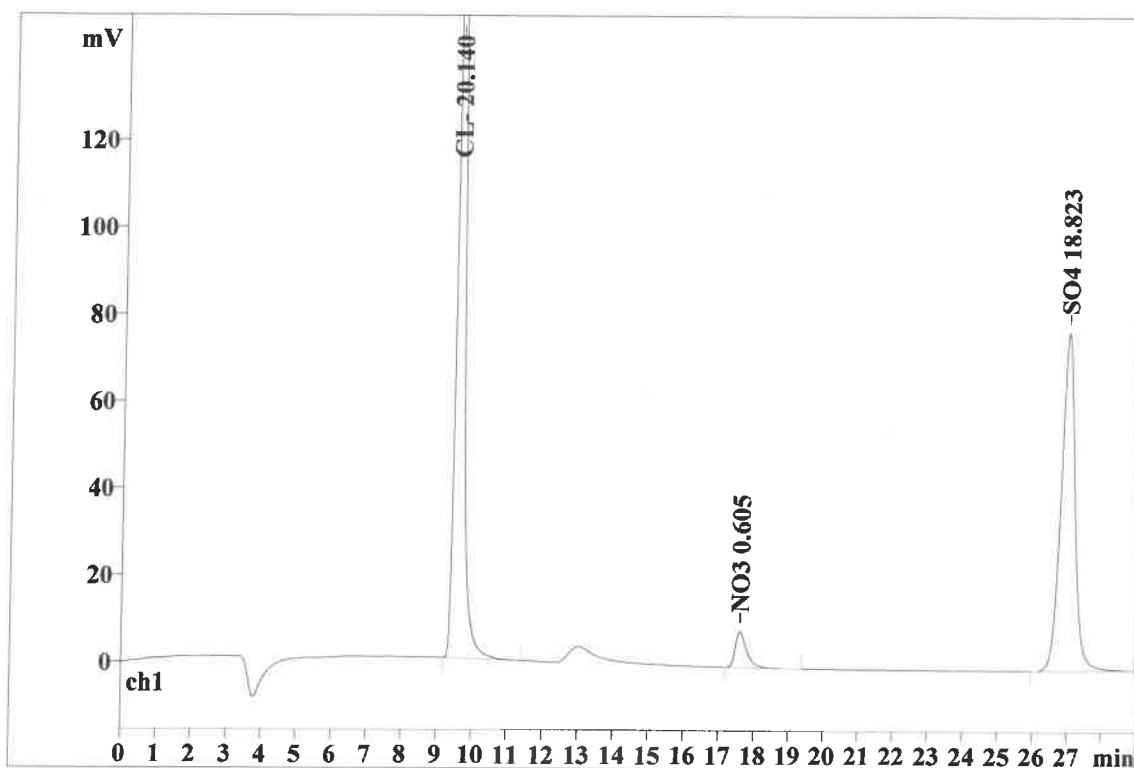

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.53	0.196	225.41	72.41	3163.339	56.72
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.60	0.329	8.23	2.64	187.316	3.36
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.94	0.424	77.64	24.94	2226.346	39.92
7	29.00	0.136	311.28	100.00	5577.002	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:55:35 AM
Printed by: wet


Ident: O5241-14DL2X10
Analysis from: 11/6/2023 3:12:32 PM
File: _2023-11-06_

Last save: 11/7/2023 9:55:34 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36528

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

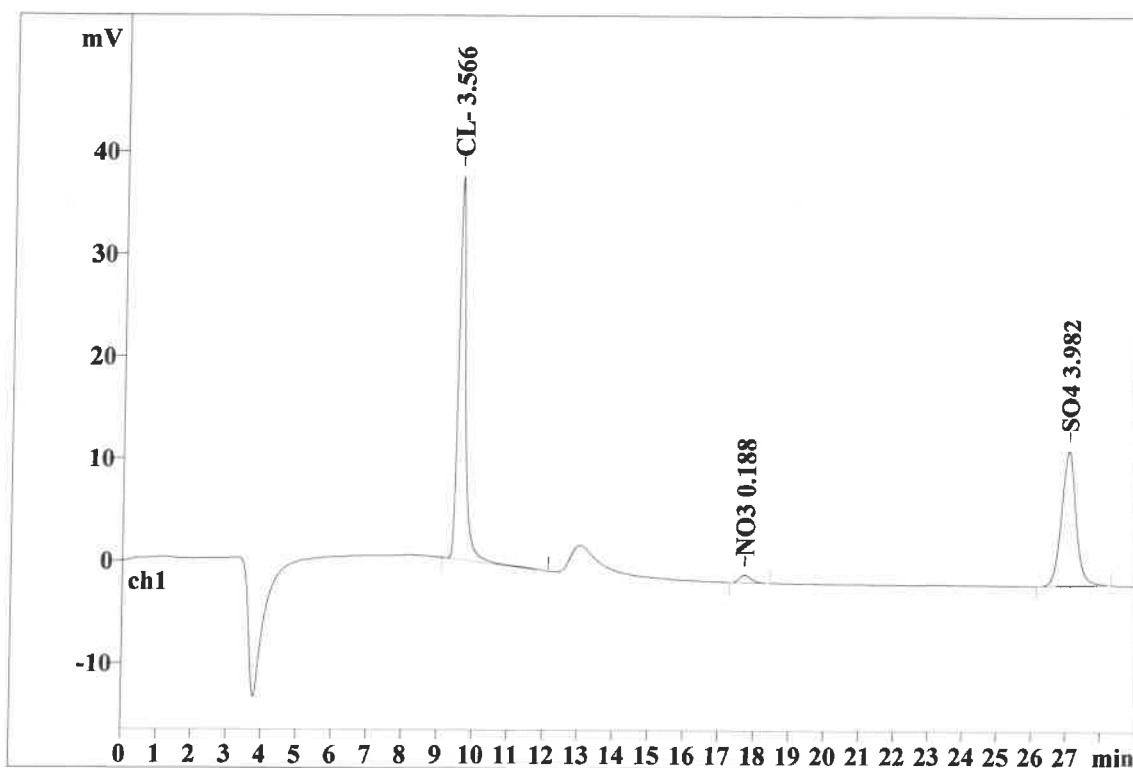

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.57	0.199	37.52	72.93	537.746	56.75
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.71	0.347	0.75	1.46	17.350	1.83
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.01	0.444	13.18	25.61	392.492	41.42
7	29.00	0.141	51.45	100.00	947.588	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:57:54 AM
Printed by: wet


Ident: O5241-17DLX5
Analysis from: 11/6/2023 3:44:10 PM
File: _2023-11-06_

Last save: 11/6/2023 4:13:09 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36529

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 24
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

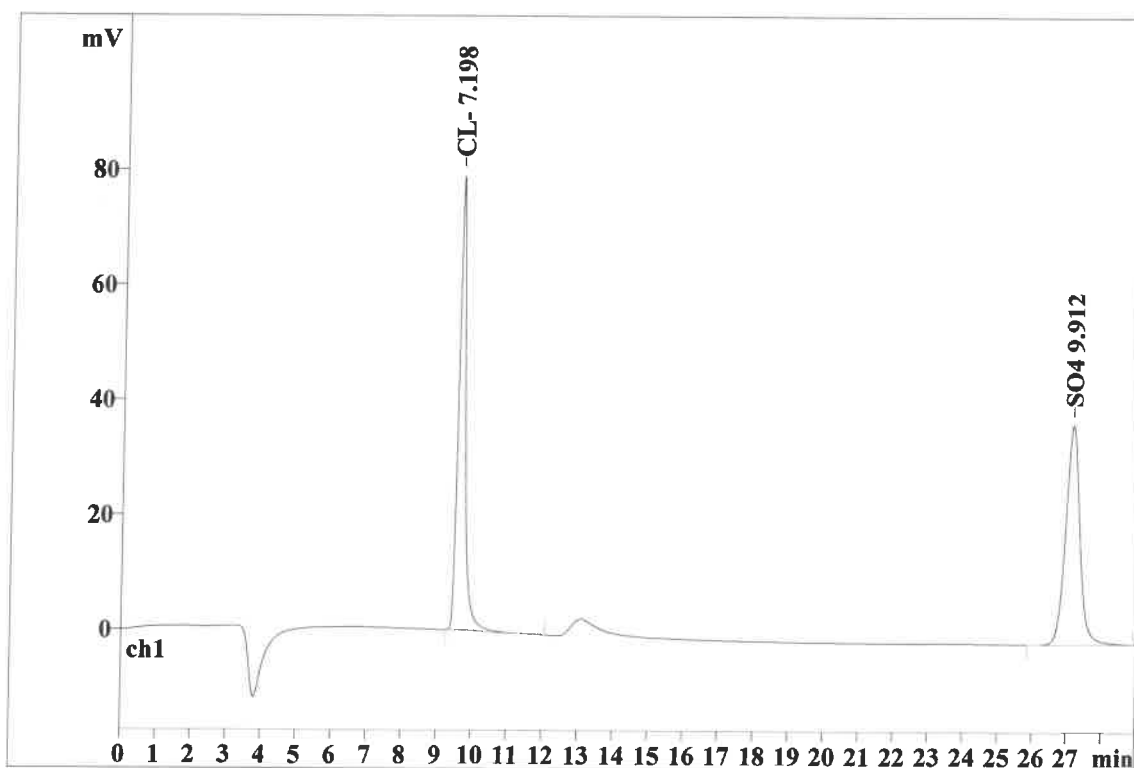

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.61	0.196	79.08	67.41	1113.193	49.73
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.12	0.436	38.22	32.58	1125.191	50.27
7	29.00	0.090	117.30	100.00	2238.384	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:58:09 AM
Printed by: wet


Ident: CCV
Analysis from: 11/6/2023 4:15:52 PM
File: _2023-11-06_

Last save: 11/7/2023 9:58:07 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36530

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

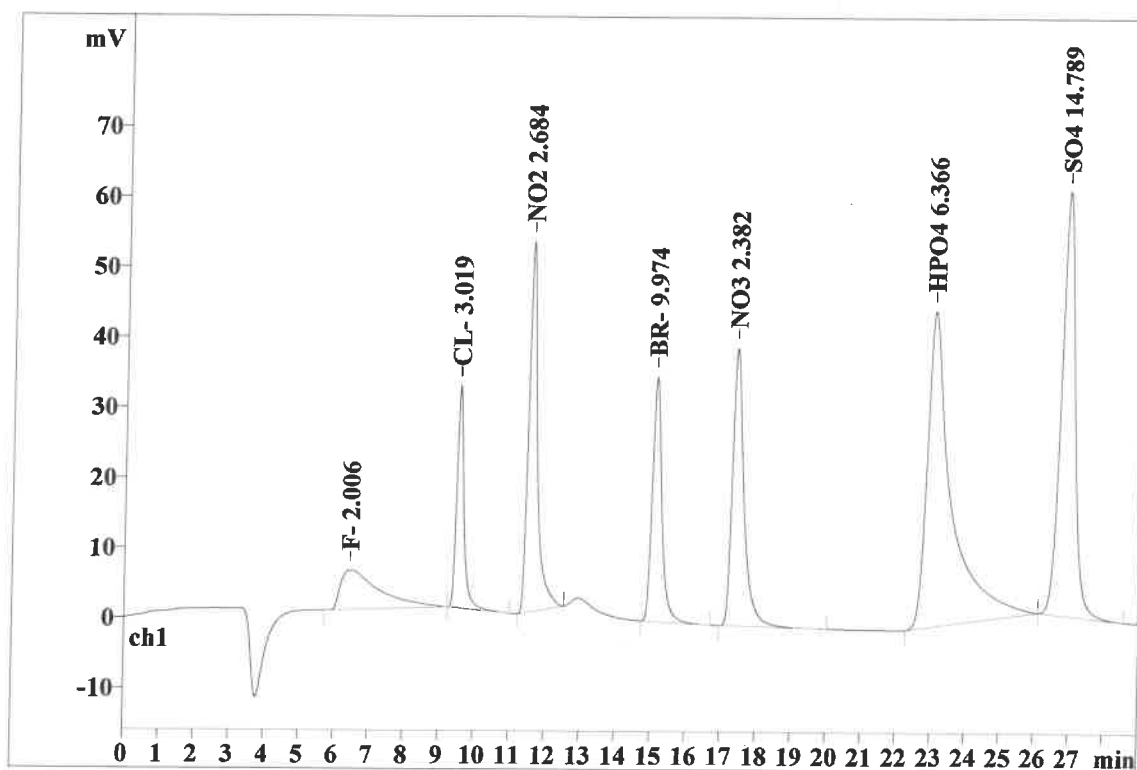

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.44	1.104	5.62	2.08	435.385	5.92
2	9.53	0.199	31.79	11.76	451.166	6.13
3	11.55	0.243	52.87	19.56	930.432	12.64
4	15.10	0.275	34.91	12.91	665.841	9.05
5	17.38	0.326	39.64	14.66	912.470	12.40
6	23.04	0.589	45.00	16.64	2235.894	30.38
7	26.88	0.426	60.52	22.39	1727.844	23.48
7	29.00	0.452	270.34	100.00	7359.032	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:50:20 AM
Printed by: wet


Ident: O5241-13DLX10
Analysis from: 11/6/2023 2:09:16 PM
File: _2023-11-06_

Last save: 11/6/2023 2:38:16 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36526

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

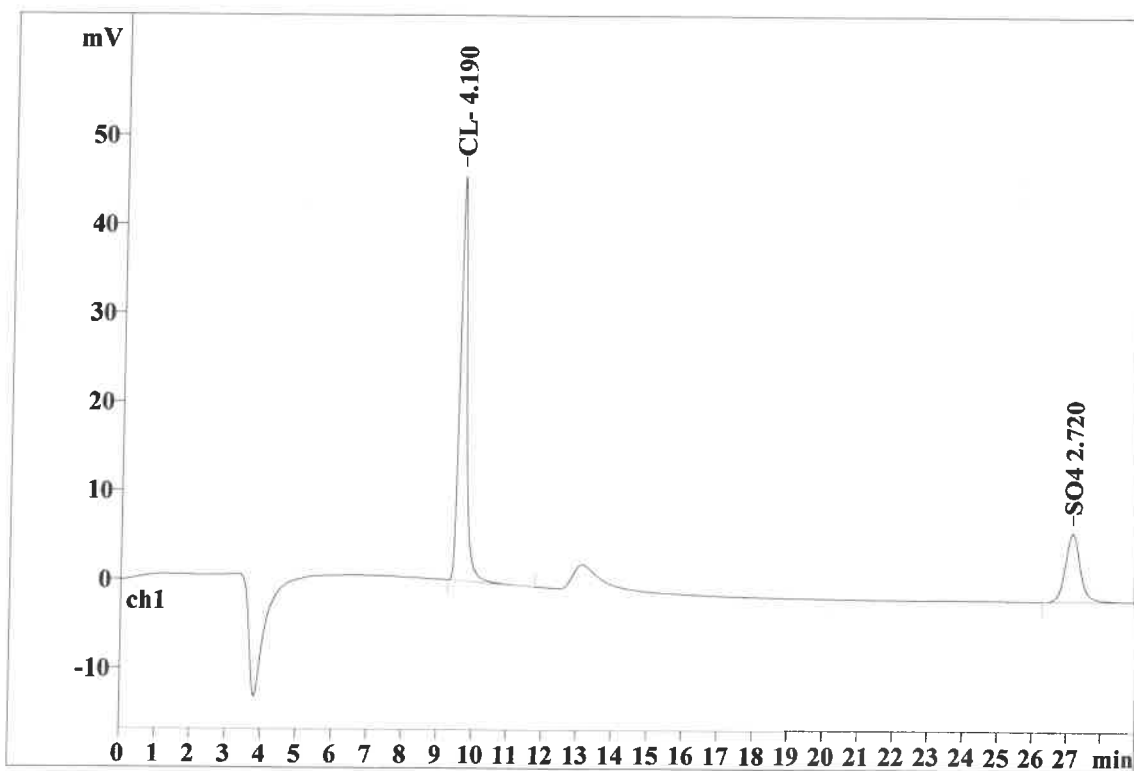

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.61	0.197	45.59	85.53	636.644	72.91
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	27.13	0.452	7.71	14.47	236.562	27.09
7	29.00	0.093	53.30	99.99	873.206	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:58:17 AM
Printed by: wet


Ident: CCB
Analysis from: 11/6/2023 4:47:30 PM
File: _2023-11-06_

Last save: 11/6/2023 5:16:30 PM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36531

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

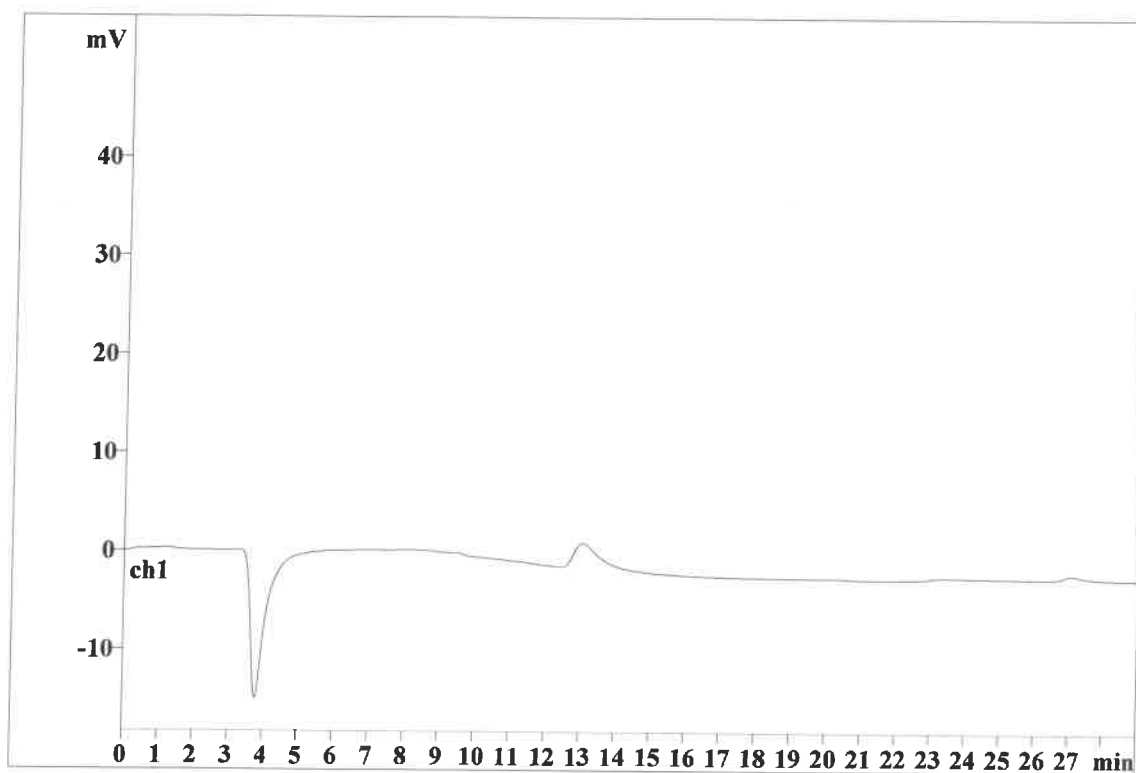

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:58:44 AM
Printed by: wet

Ident: O5241-18DLX10
Analysis from: 11/6/2023 5:50:50 PM
File: _2023-11-06_

Last save: 11/7/2023 9:58:39 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36533

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.19	0.187	32.96	89.43	443.921	78.48
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.54	0.449	3.89	10.56	121.709	21.52
7	29.00	0.091	36.86	99.99	565.630	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:59:02 AM
Printed by: wet


Ident: O5241-19DLX10
Analysis from: 11/6/2023 6:22:28 PM
File: _2023-11-06_

Last save: 11/7/2023 9:58:58 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36534

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

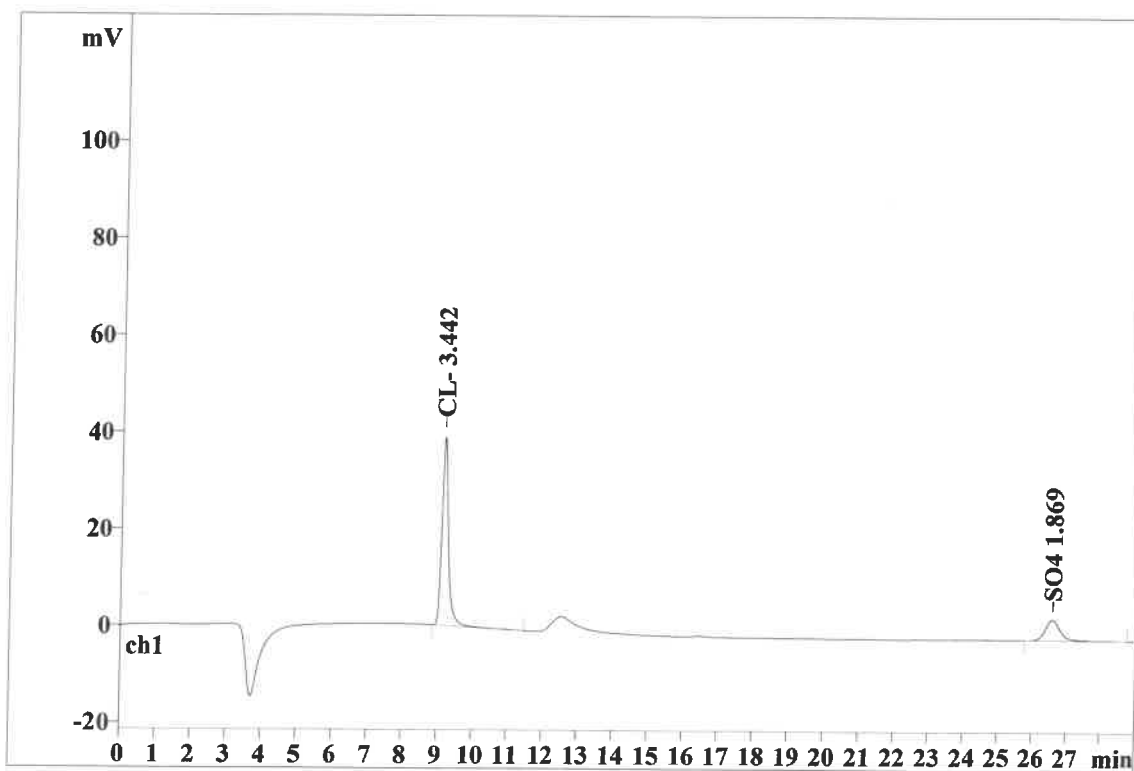

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.17	0.186	39.01	90.16	518.209	79.77
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.59	0.446	4.26	9.83	131.401	20.23
7	29.00	0.090	43.27	99.99	649.610	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:59:23 AM
Printed by: wet


Ident: O5241-20DLX10
Analysis from: 11/6/2023 6:54:06 PM
File: _2023-11-06_

Last save: 11/7/2023 9:59:21 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36535

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 28
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

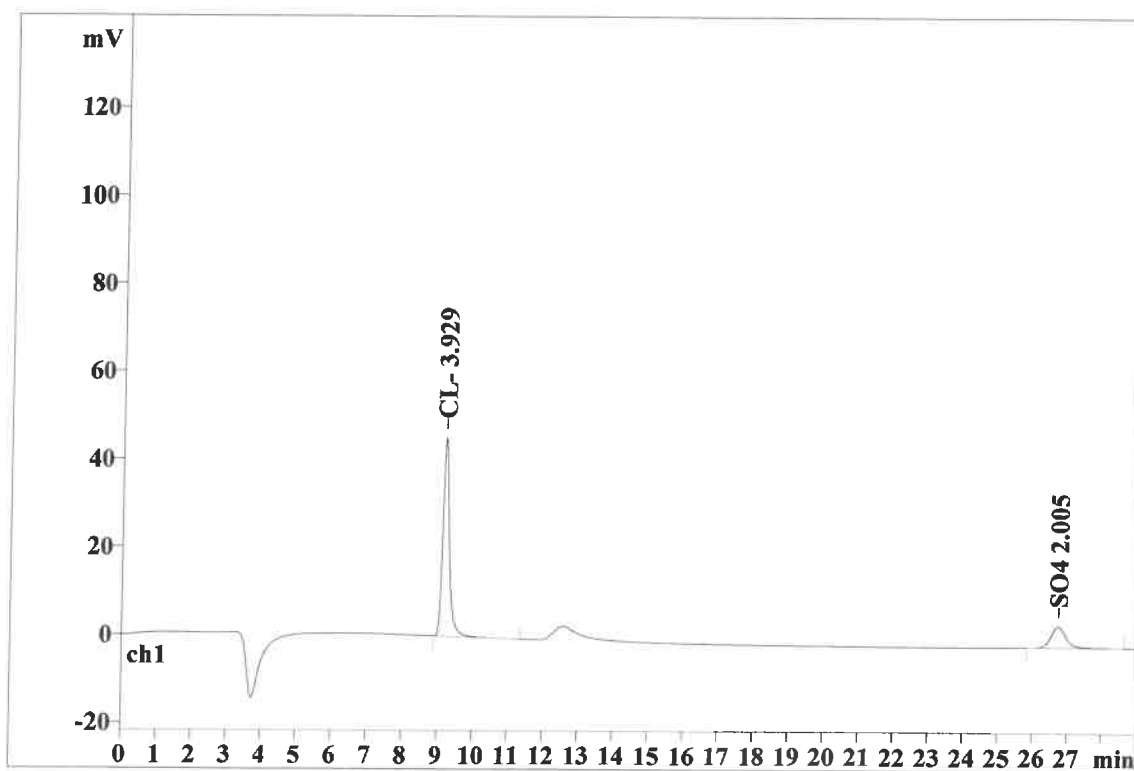

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.19	0.186	45.26	90.37	595.267	80.08
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.73	0.445	4.82	9.63	148.089	19.92
7	29.00	0.090	50.08	100.00	743.356	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 9:59:46 AM
Printed by: wet


Ident: O5241-23DLX10
Analysis from: 11/6/2023 7:25:45 PM
File: _2023-11-06_

Last save: 11/7/2023 9:59:43 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36536

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 29
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

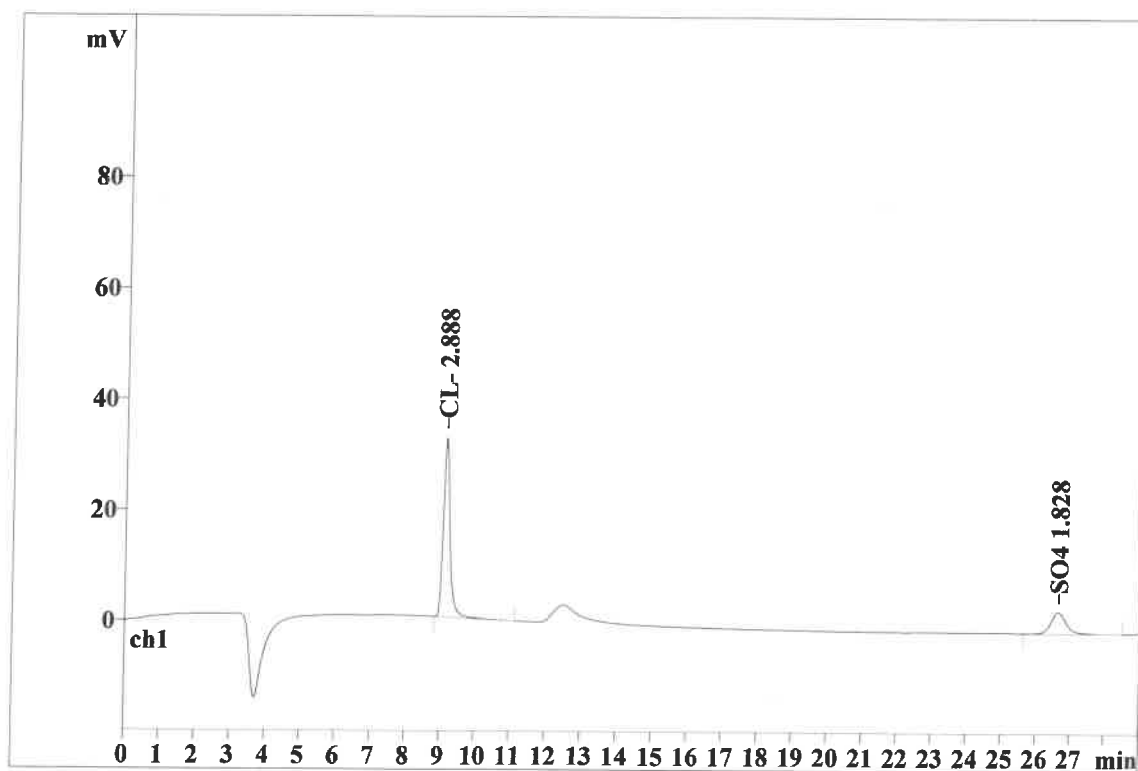

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.13	0.187	32.38	89.26	430.356	77.32
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.65	0.464	3.89	10.74	126.252	22.68
7	29.00	0.093	36.27	100.00	556.608	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 10:00:12 AM
Printed by: wet


Ident: CCV
Analysis from: 11/6/2023 7:57:29 PM
File: _2023-11-06_

Last save: 11/7/2023 10:00:09 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36537

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

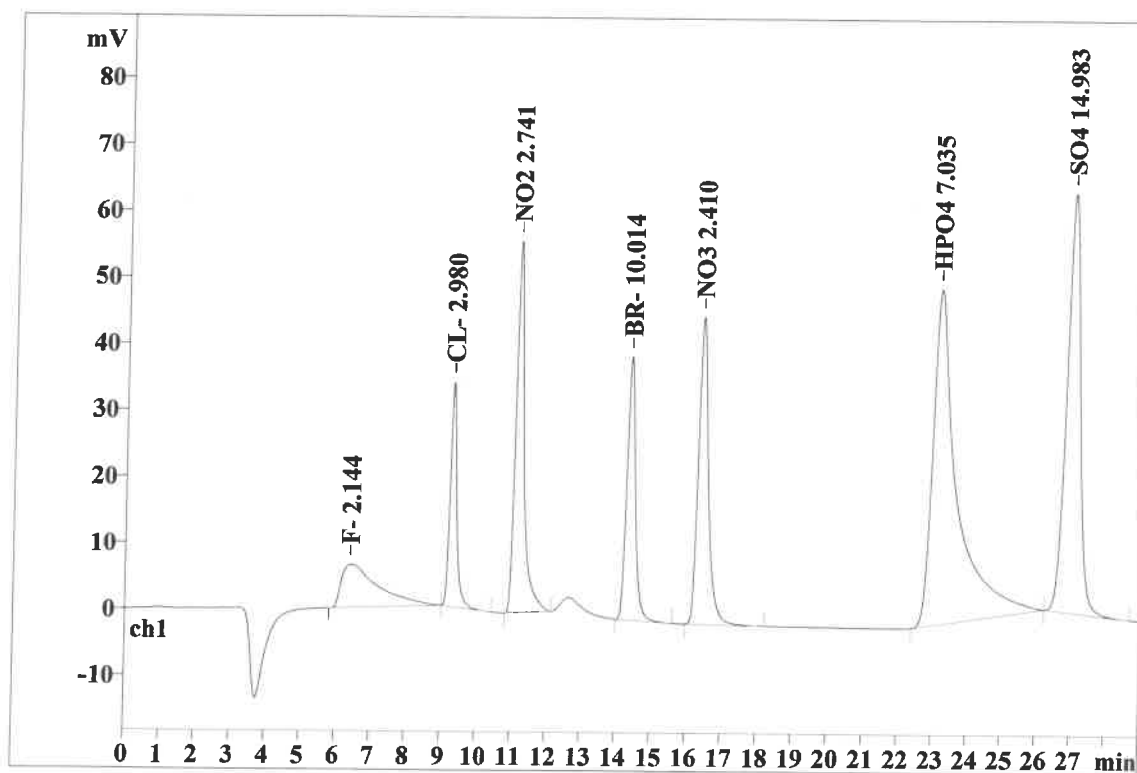

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.41	1.036	6.49	2.19	468.922	6.09
2	9.29	0.188	33.77	11.41	444.930	5.78
3	11.14	0.233	56.05	18.93	951.477	12.35
4	14.36	0.248	39.74	13.42	668.701	8.68
5	16.38	0.289	46.34	15.65	924.209	12.00
6	23.13	0.583	50.51	17.06	2491.710	32.35
7	26.97	0.417	63.14	21.33	1751.916	22.75
7	29.00	0.428	296.04	100.00	7701.865	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/7/2023 10:00:32 AM
Printed by: wet


Ident: CCB
Analysis from: 11/6/2023 8:29:07 PM
File: _2023-11-06_

Last save: 11/7/2023 10:00:31 AM

Method: AnionsIC2-101323.mtw
Run operator: wet
Analysis number: 36538

Last save: 10/31/2023 9:38

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

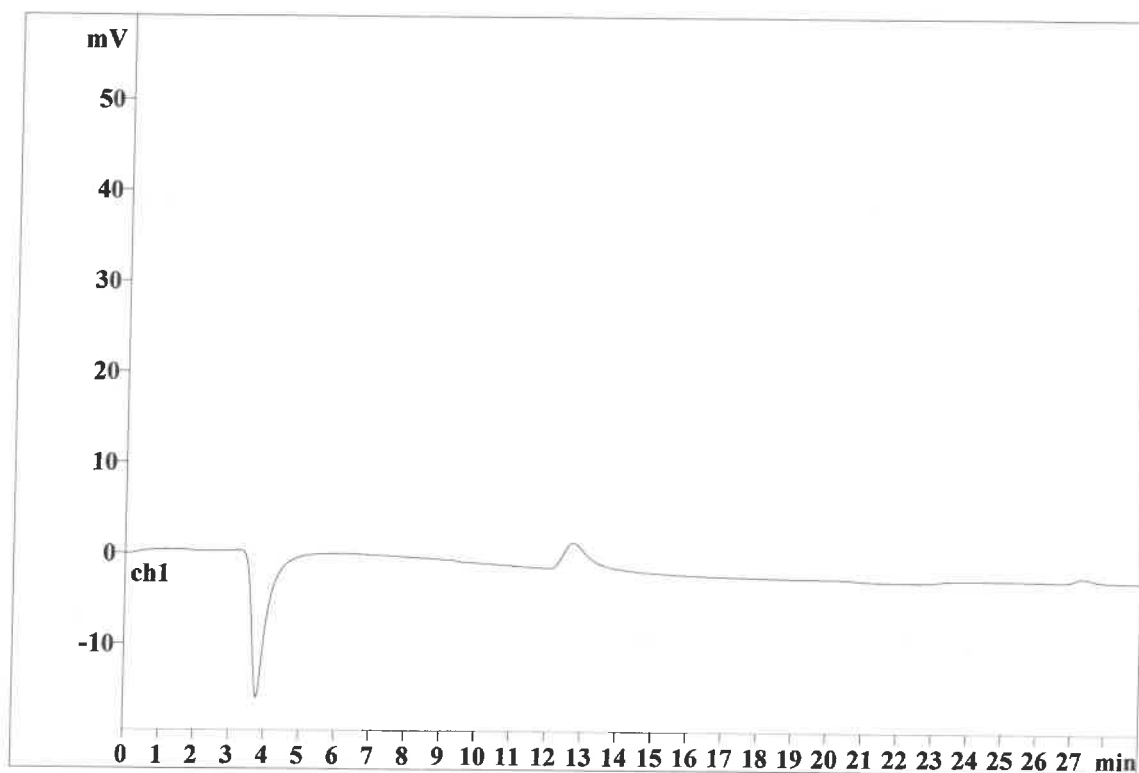

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

WORKLIST(Hardcopy Internal Chain)

LB122206

WorkList Name : Anions-110323-2 WorkList ID : 175271 Department : Wet-Chemistry Date : 11-03-2023 13:15:20

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
O5241-04	FSND-MW-33-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-05	FSND-MW-32-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-08	FSND-MW-31-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-09	FSND-MW-15-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-13	FSND-MW-24-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-14	FSND-EVAL-01S-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-22	FSND-RB-4-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-23	DUP-4-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-15	O5241-14MS	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-16	O5241-14MSD	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-17	FSND-MW-26-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-18	FSND-MW-34-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-19	FSND-MW-35-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A
O5241-20	FSND-EVAL-01D-20231102	Water	Anions Group1	Cool 4 deg C	EAEN05	I41	11/02/2023	9056A

Date/Time 11/03/23 16:10
 Raw Sample Received by: 12/20/ JAL
 Raw Sample Relinquished by: 12/20/ JAL