


LB128329

7471B

INSTRUMENT ID: CV1

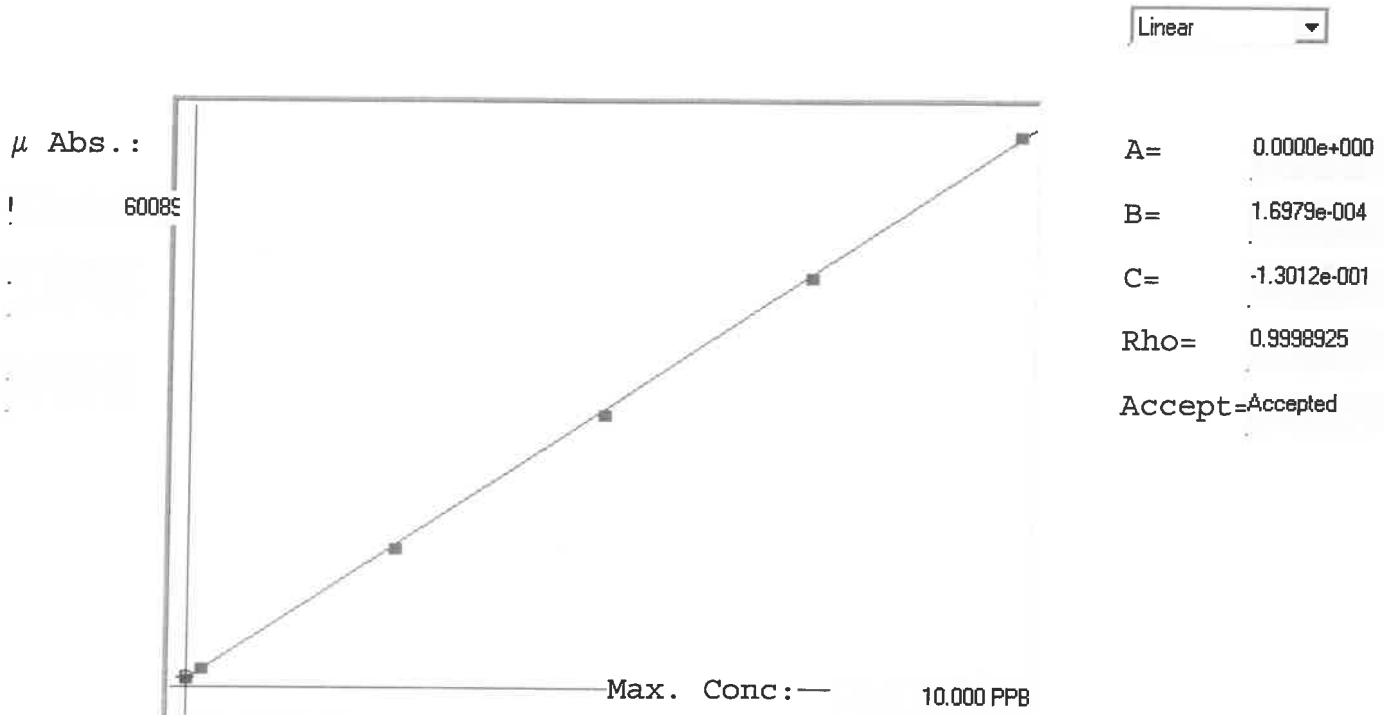

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/0
0.0	0.000	0.055	0.055	1091	0.000	1091					12
0.2	0.200	0.224	0.024	2086	0.0 %	2086					-2
2.5	2.500	2.460	-0.040	15255	0.0 %	15255					-2
5.0	5.000	4.924	-0.076	29765	0.0 %	29765					0
7.5	7.500	7.464	-0.036	44727	0.0 %	44727					1
10.0	10.000	10.073	0.073	60089	0.0 %	60089					

LB128323 INBSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 15 Nov 2023 10:38:24

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1091	-	0.0000	7471B	PPB	15 Nov 2023 10:41:47	S	Std
0.2 - 1	50.2	2086	-	0.2000	7471B	PPB	15 Nov 2023 10:44:04	S	Std
2.5 - 1	52.5	15255	-	2.5000	7471B	PPB	15 Nov 2023 10:46:21	S	Std
5.0 - 1	55	29765	-	5.0000	7471B	PPB	15 Nov 2023 10:48:39	S	Std
7.5 - 1	57.5	44727	-	7.5000	7471B	PPB	15 Nov 2023 10:50:56	S	Std
10.0 - 1	510	60089	-	10.0000	7471B	PPB	15 Nov 2023 10:53:14	S	Std
ICV73 - 1	ICV73	24639	4.0534	-	7471B	PPB	15 Nov 2023 10:56:27	U	SMPL
ICB73 - 1	ICB73	877	0.0188	-	7471B	PPB	15 Nov 2023 10:58:42	U	SMPL
CCV25 - 1	CCV25	30085	4.9781	-	7471B	PPB	15 Nov 2023 11:01:00	U	SMPL
CCB25 - 1	CCB25	864	0.0166	-	7471B	PPB	15 Nov 2023 11:03:15	U	SMPL
CRA - 1	CRA	1991	0.2079	-	7471B	PPB	15 Nov 2023 11:05:32	U	SMPL
HighStd - 1	HighStd	58913	9.8730	-	7471B	PPB	15 Nov 2023 11:07:47	U	SMPL
ChkStd - 1	ChkStd	42571	7.0982	-	7471B	PPB	15 Nov 2023 11:10:02	U	SMPL
PB157155BL - 1	PBS	754	-0.0021	-	7471B	PPB	15 Nov 2023 11:12:21	U	SMPL
PB157155BS - 1	LCSS	25035	4.1207	-	7471B	PPB	15 Nov 2023 11:14:40	U	SMPL
O5366-01 - 1	P-13(10-15)	10693	1.6855	-	7471B	PPB	15 Nov 2023 11:16:56	U	SMPL
O5366-02 - 1	P-14(10-15)	6476	0.9695	-	7471B	PPB	15 Nov 2023 11:19:14	U	SMPL
O5384-01 - 1	EO-01-11102023	8652	1.3389	-	7471B	PPB	15 Nov 2023 11:21:34	U	SMPL
O5384-03 - 1	EO-02-11102023	6071	0.9007	-	7471B	PPB	15 Nov 2023 11:23:53	U	SMPL
O5384-05 - 1	EO-03-11102023	2684	0.3256	-	7471B	PPB	15 Nov 2023 11:26:08	U	SMPL
CCV26 - 1	CCV26	29650	4.9043	-	7471B	PPB	15 Nov 2023 11:28:23	U	SMPL
CCB26 - 1	CCB26	1056	0.0492	-	7471B	PPB	15 Nov 2023 11:30:38	U	SMPL
O5385-01 - 1	HR-02-11102023	3726	0.5025	-	7471B	PPB	15 Nov 2023 11:32:55	U	SMPL
O5385-03 - 1	HR-03-11102023	5327	0.7744	-	7471B	PPB	15 Nov 2023 11:35:11	U	SMPL
O5388-01 - 1	TP-3	3262	0.4238	-	7471B	PPB	15 Nov 2023 11:37:27	U	SMPL
O5388-05 - 1	TP-4	3487	0.4620	-	7471B	PPB	15 Nov 2023 11:39:43	U	SMPL
O5401-01 - 1	ETGI-338	4482	0.6309	-	7471B	PPB	15 Nov 2023 11:41:59	U	SMPL
O5402-01 - 1	SOIL-DRUM-COMP	14178	2.2772	-	7471B	PPB	15 Nov 2023 11:44:16	U	SMPL
O5408-01 - 1	710-NEW-YORK-AVE	39861	6.6380	-	7471B	PPB	15 Nov 2023 11:46:32	U	SMPL
O5408-03 - 1	710-BROOKLYN-AVE	3018	0.3823	-	7471B	PPB	15 Nov 2023 11:48:50	U	SMPL
O5408-05 - 1	710-ELIZABETH-AVE	2370	0.2723	-	7471B	PPB	15 Nov 2023 11:51:09	U	SMPL
O5408-07 - 1	710-PLAINFIELD-AVE	4094	0.5650	-	7471B	PPB	15 Nov 2023 11:53:25	U	SMPL
CCV27 - 1	CCV27	29594	4.8948	-	7471B	PPB	15 Nov 2023 11:55:40	U	SMPL
CCB27 - 1	CCB27	1071	0.0517	-	7471B	PPB	15 Nov 2023 11:57:56	U	SMPL
O5408-09 - 1	710-RHINE-AVE	2149	0.2348	-	7471B	PPB	15 Nov 2023 12:00:12	U	SMPL
O5408-11 - 1	710-BOUND-BROOK-AVE	3490	0.4625	-	7471B	PPB	15 Nov 2023 12:02:28	U	SMPL
O5408-11DUP - 1	710-BOUND-BROOK-AVEDUP	3034	0.3850	-	7471B	PPB	15 Nov 2023 12:04:44	U	SMPL
O5408-11MS - 1	710-BOUND-BROOK-AVEMS	32285	5.3517	-	7471B	PPB	15 Nov 2023 12:07:00	U	SMPL
O5408-11MSD - 1	710-BOUND-BROOK-AVEMSD	30281	5.0114	-	7471B	PPB	15 Nov 2023 12:09:15	U	SMPL
O5412-01 - 1	MH-1	1558	0.1344	-	7471B	PPB	15 Nov 2023 12:11:33	U	SMPL
O5412-05 - 1	MH-2	1421	0.1112	-	7471B	PPB	15 Nov 2023 12:13:51	U	SMPL
O5408-11A - 1		28302	4.6754	-	7471B	PPB	15 Nov 2023 12:18:25	U	SMPL
O5408-11LX5 - 1		1550	0.1331	-	7471B	PPB	15 Nov 2023 12:29:03	U	SMPL
CCV28 - 1	CCV28	28340	4.6818	-	7471B	PPB	15 Nov 2023 12:34:16	U	SMPL
CCB28 - 1	CCB28	1017	0.0426	-	7471B	PPB	15 Nov 2023 12:36:31	U	SMPL