


LB 128341

7470A

INSTRUMENT ID: CV1

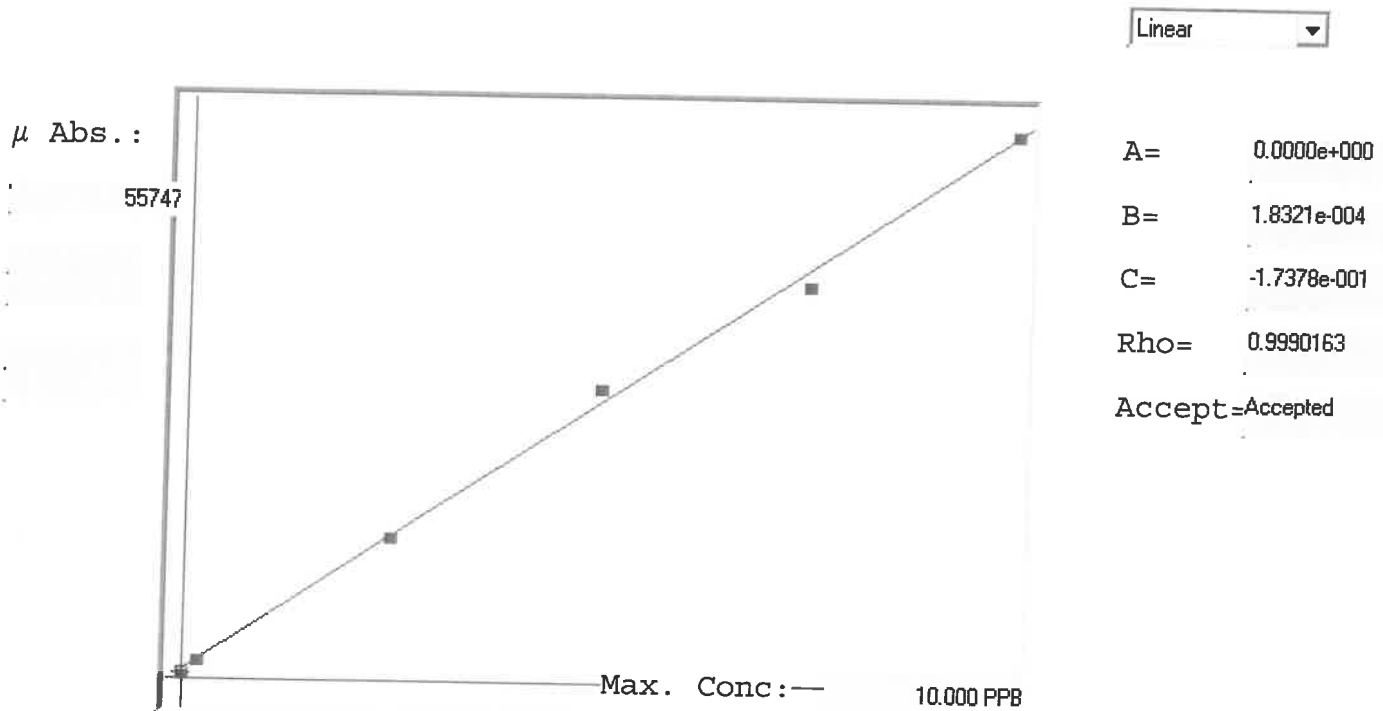

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.059	-0.059	627	0.000	627	0				4
0.2	0.200	0.208	0.008	2086	0.0 %	2086					4
2.5	2.500	2.481	-0.019	14493	0.0 %	14493					-1
5.0	5.000	5.293	0.293	29840	0.0 %	29840					6
7.5	7.500	7.237	-0.263	40449	0.0 %	40449					-4
10.0	10.000	10.039	0.039	55747	0.0 %	55747					0

LB128341 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Nov 2023 10:19:21

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	627	-	0.0000	7470A	PPB	16 Nov 2023 10:25:34	S	Std
0.2 - 1	50.2	2086	-	0.2000	7470A	PPB	16 Nov 2023 10:27:52	S	Std
2.5 - 1	52.5	14493	-	2.5000	7470A	PPB	16 Nov 2023 10:30:08	S	Std
5.0 - 1	55	29840	-	5.0000	7470A	PPB	16 Nov 2023 10:32:25	S	Std
7.5 - 1	57.5	40449	-	7.5000	7470A	PPB	16 Nov 2023 10:34:42	S	Std
10.0 - 1	510	55747	-	10.0000	7470A	PPB	16 Nov 2023 10:42:16	S	Std
ICV75 - 1	ICV75	24196	4.2591	-	7470A	PPB	16 Nov 2023 10:50:14	U	SMPL
ICB75 - 1	ICB75	441	-0.0930	-	7470A	PPB	16 Nov 2023 10:55:19	U	SMPL
CCV32 - 1	CCV32	28280	5.0073	-	7470A	PPB	16 Nov 2023 10:57:34	U	SMPL
CCB32 - 1	CCB32	629	-0.0585	-	7470A	PPB	16 Nov 2023 10:59:48	U	SMPL
CRA - 1	CRA	1939	0.1815	-	7470A	PPB	16 Nov 2023 11:02:05	U	SMPL
HighStd - 1	HighStd	55869	10.0617	-	7470A	PPB	16 Nov 2023 11:04:20	U	SMPL
ChkStd - 1	ChkStd	36568	6.5257	-	7470A	PPB	16 Nov 2023 11:06:36	U	SMPL
PB157156BL - 1	PBW	707	-0.0443	-	7470A	PPB	16 Nov 2023 11:11:29	U	SMPL
PB157156BS - 1	LCSW	20559	3.5927	-	7470A	PPB	16 Nov 2023 11:13:45	U	SMPL
O5137-07 - 1	FAIR-LAWN-CONC	-96	-0.1914	-	7470A	PPB	16 Nov 2023 11:16:01	U	SMPL
O5382-01 - 1	S-11	1203	0.0466	-	7470A	PPB	16 Nov 2023 11:18:18	U	SMPL
O5382-02 - 1	S-12	1274	0.0596	-	7470A	PPB	16 Nov 2023 11:20:35	U	SMPL
O5382-03 - 1	S-13	1533	0.1071	-	7470A	PPB	16 Nov 2023 11:22:55	U	SMPL
O5382-04 - 1	S-14	593	-0.0651	-	7470A	PPB	16 Nov 2023 11:25:12	U	SMPL
CCV33 - 1	CCV33	30553	5.4237	-	7470A	PPB	16 Nov 2023 11:27:29	U	SMPL
CCB33 - 1	CCB33	503	-0.0816	-	7470A	PPB	16 Nov 2023 11:29:44	U	SMPL
O5382-05 - 1	S-15	1450	0.0919	-	7470A	PPB	16 Nov 2023 11:32:01	U	SMPL
O5382-06 - 1	S-16	631	-0.0582	-	7470A	PPB	16 Nov 2023 11:34:17	U	SMPL
O5382-07 - 1	S-17	693	-0.0468	-	7470A	PPB	16 Nov 2023 11:36:34	U	SMPL
O5382-08 - 1	S-18	765	-0.0336	-	7470A	PPB	16 Nov 2023 11:38:49	U	SMPL
O5382-09 - 1	S-19	594	-0.0650	-	7470A	PPB	16 Nov 2023 11:41:05	U	SMPL
O5382-10 - 1	S-20	583	-0.0670	-	7470A	PPB	16 Nov 2023 11:43:21	U	SMPL
O5388-04 - 1	TP-3	274	-0.1236	-	7470A	PPB	16 Nov 2023 11:45:37	U	SMPL
O5388-08 - 1	TP-4	382	-0.1038	-	7470A	PPB	16 Nov 2023 11:47:54	U	SMPL
O5400-01 - 1	DRY-PAINT-CHIPS	408	-0.0990	-	7470A	PPB	16 Nov 2023 11:50:11	U	SMPL
O5402-02 - 1	SOIL-DRUM-COMP	336	-0.1122	-	7470A	PPB	16 Nov 2023 11:52:27	U	SMPL
CCV34 - 1	CCV34	29822	5.2898	-	7470A	PPB	16 Nov 2023 11:54:42	U	SMPL
CCB34 - 1	CCB34	588	-0.0661	-	7470A	PPB	16 Nov 2023 11:56:58	U	SMPL
O5402-02DUP - 1	SOIL-DRUM-COMPDUP	544	-0.0741	-	7470A	PPB	16 Nov 2023 11:59:13	U	SMPL
O5402-02MS - 1	SOIL-DRUM-COMPMS	19607	3.4183	-	7470A	PPB	16 Nov 2023 12:01:29	U	SMPL
O5402-02MSD - 1	SOIL-DRUM-COMPMSD	20826	3.6417	-	7470A	PPB	16 Nov 2023 12:06:27	U	SMPL
PB157127TB - 1	PB157127TB	653	-0.0542	-	7470A	PPB	16 Nov 2023 12:12:05	U	SMPL
O5402-02LX5 - 1		0	-0.1738	-	7470A	PPB	16 Nov 2023 12:14:21	U	SMPL
O5402-02LX5 - 1		161	-0.1443	-	7470A	PPB	16 Nov 2023 12:16:12	U	SMPL
O5402-02A - 1		24908	4.3895	-	7470A	PPB	16 Nov 2023 12:18:28	U	SMPL
CCV35 - 1	CCV35	28224	4.9970	-	7470A	PPB	16 Nov 2023 12:20:45	U	SMPL
CCB35 - 1	CCB35	753	-0.0358	-	7470A	PPB	16 Nov 2023 12:25:40	U	SMPL