

66128372

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/20/2023 15:02

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.012	0.0	0.102	
ICB1	0.003	0.0	0.032	
CCV1	1.016	0.0	0.102	
CCB1	0.002	0.0	0.032	
PB157258BL	0.005	0.0	0.033	
PB157258BS	1.006	0.0	0.102	
O5422-04	0.004	0.0	0.032	
O5422-06	0.001	0.0	0.032	
O5422-06DUP	-0.003	0.0	0.032	
O5422-06MS	0.996	0.0	0.101	
O5422-06MSD	0.990	0.0	0.101	
CCV2	0.992	0.0	0.101	
CCB2	0.001	0.0	0.032	

N	13
Mean	0.464
SD	0.5191
CV%	111.98

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 20 14:24:13 2023

Mon Nov 20 15:02:24 2023

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPM	A	Phenolics-	P	-0.0009	mg/l	11/20/2023 14:24:13	
0.1PPM	A	Phenolics-	P	0.05	mg/l	11/20/2023 14:24:14	
0.2PPM	A	Phenolics-	P	0.1008	mg/l	11/20/2023 14:24:15	
0.4PPM	A	Phenolics-	P	0.2549	mg/l	11/20/2023 14:24:16	
1.0PPM	A	Phenolics-	P	0.5114	mg/l	11/20/2023 14:24:17	
1.3PPM	A	Phenolics-	P	0.9748	mg/l	11/20/2023 14:24:18	
2.0PPM	A	Phenolics-	P	2.0091	mg/l	11/20/2023 14:24:19	
ICV1	S	Phenolics-	P	1.0123	mg/l	11/20/2023 14:48:24	
ICB1	S	Phenolics-	P	0.0032	mg/l	11/20/2023 14:48:25	
CCV1	S	Phenolics-	P	1.0164	mg/l	11/20/2023 14:48:28	
CCB1	S	Phenolics-	P	0.0022	mg/l	11/20/2023 14:48:29	
PB157258BL	S	Phenolics-	P	0.0052	mg/l	11/20/2023 14:48:32	
PB157258BS	S	Phenolics-	P	1.0065	mg/l	11/20/2023 14:48:34	
O5422-04	S	Phenolics-	P	0.0038	mg/l	11/20/2023 14:58:25	
O5422-06	S	Phenolics-	P	0.001	mg/l	11/20/2023 14:58:27	
O5422-06DUP	S	Phenolics-	P	-0.0031	mg/l	11/20/2023 14:58:30	
O5422-06MS	S	Phenolics-	P	0.9958	mg/l	11/20/2023 14:58:31	
O5422-06MSD	S	Phenolics-	P	0.9903	mg/l	11/20/2023 14:58:33	
CCV2	S	Phenolics-	P	0.9917	mg/l	11/20/2023 14:58:36	
CCB2	S	Phenolics-	P	0.0009	mg/l	11/20/2023 15:02:23	

06128372

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

11/20/2023 14:25

Reviewed by : RM

Instrument ID : Konelab


Test Phenolics-

Accepted 11/20/2023 14:25

Factor 14.46
Bias 0.032

Coeff. of det. 0.999724

Errors

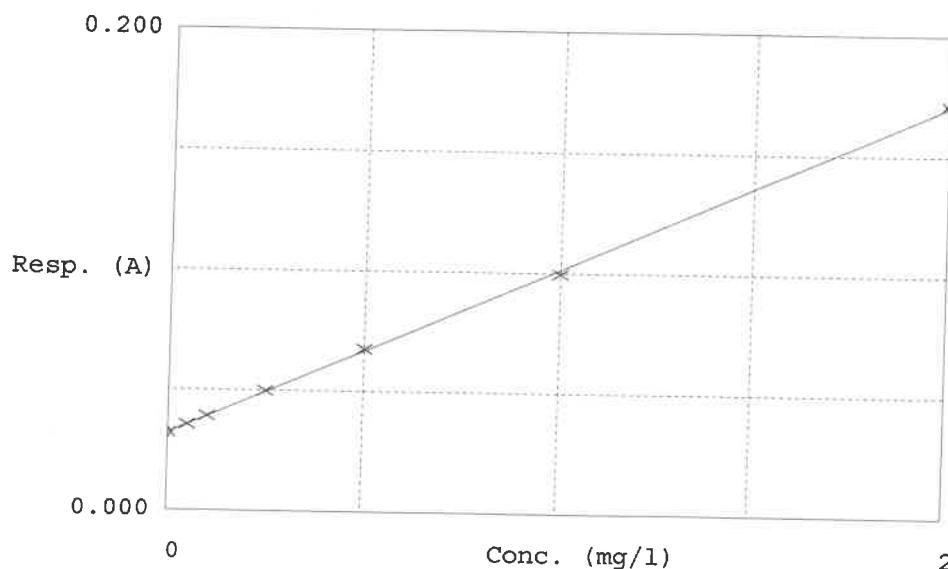

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.032	-0.0009	0.0000	-
2	Phenol-2	0.036	0.0500	0.0500	0.0
3	Phenol-2	0.039	0.1008	0.1000	0.8
4	Phenol-2	0.050	0.2549	0.2500	2.0
5	Phenol-2	0.068	0.5114	0.5000	2.3
6	Phenol-2	0.100	0.9748	1.0000	-2.5
7	Phenol-2	0.171	2.0091	2.0000	0.5

11/20/2023
RM