


LB128721

7471B

INSTRUMENT ID: CV1

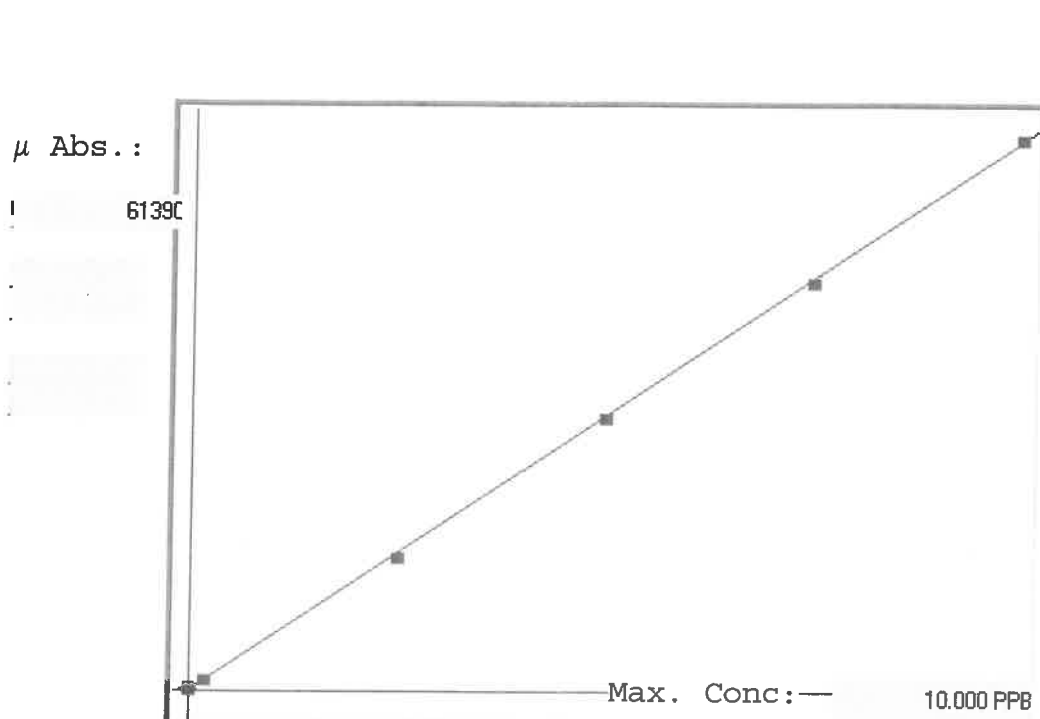

Linear

A= 0.0000e+000

B= 1.6380e-004

C= -8.4098e-003

Rho= 0.9999519

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	(%)
0.0	0.000	0.037	0.037	279	0.000	279					9
0.2	0.200	0.219	0.019	1386	0.0 %	1386					-2
2.5	2.500	2.453	-0.047	15026	0.0 %	15026					0
5.0	5.000	4.978	-0.022	30445	0.0 %	30445					0
7.5	7.500	7.465	-0.035	45628	0.0 %	45628					0
10.0	10.000	10.047	0.047	61390	0.0 %	61390					0

LB128721 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 13 Dec 2023 17:22:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50	279	-	0.0000	7471B	PPB	13 Dec 2023 17:30:54	S	Std
0.2 - 1	50.2	1386	-	0.2000	7471B	PPB	13 Dec 2023 17:33:11	S	Std
2.5 - 1	52.5	15026	-	2.5000	7471B	PPB	13 Dec 2023 17:35:28	S	Std
5.0 - 1	55	30445	-	5.0000	7471B	PPB	13 Dec 2023 17:37:45	S	Std
7.5 - 1	57.5	45628	-	7.5000	7471B	PPB	13 Dec 2023 17:40:04	S	Std
10.0 - 1	51.0	61390	-	10.0000	7471B	PPB	13 Dec 2023 17:42:29	S	Std
ICV23 - 1	ICV23	23745	3.8810	-	7471B	PPB	13 Dec 2023 17:45:30	U	SMPL
ICB23 - 1	ICB23	-299	-0.0574	-	7471B	PPB	13 Dec 2023 17:47:47	U	SMPL
CCV03 - 1	CCV03	31210	5.1038	-	7471B	PPB	13 Dec 2023 17:50:08	U	SMPL
CCB03 - 1	CCB03	-219	-0.0443	-	7471B	PPB	13 Dec 2023 17:52:23	U	SMPL
CRA - 1	CRA	1359	0.2142	-	7471B	PPB	13 Dec 2023 17:54:50	U	SMPL
HighStd - 1	HighStd	61680	10.0948	-	7471B	PPB	13 Dec 2023 17:57:06	U	SMPL
ChkStd - 1	ChkStd	43156	7.0606	-	7471B	PPB	13 Dec 2023 17:59:22	U	SMPL
PB157754BL - 1	PBS	-404	-0.0746	-	7471B	PPB	13 Dec 2023 18:01:54	U	SMPL
PB157754BS - 1	LCSS	23423	3.8283	-	7471B	PPB	13 Dec 2023 18:04:23	U	SMPL
O5758-01 - 1	SP-COMP-1	5004	0.8112	-	7471B	PPB	13 Dec 2023 18:06:39	U	SMPL
O5758-10 - 1	SP-COMP-2	1626	0.2579	-	7471B	PPB	13 Dec 2023 18:09:04	U	SMPL
O5758-19 - 1	SP-COMP-3	1989	0.3174	-	7471B	PPB	13 Dec 2023 18:11:24	U	SMPL
O5758-28 - 1	SP-COMP-4	1712	0.2720	-	7471B	PPB	13 Dec 2023 18:13:42	U	SMPL
O5758-37 - 1	SP-COMP-5	1731	0.2751	-	7471B	PPB	13 Dec 2023 18:15:58	U	SMPL
CCV04 - 1	CCV04	31861	5.2104	-	7471B	PPB	13 Dec 2023 18:18:13	U	SMPL
CCB04 - 1	CCB04	-243	-0.0482	-	7471B	PPB	13 Dec 2023 18:20:29	U	SMPL
O5760-01 - 1	CONCRETE-1	734	0.1118	-	7471B	PPB	13 Dec 2023 18:22:54	U	SMPL
O5760-03 - 1	CONCRETE-2	660	0.0997	-	7471B	PPB	13 Dec 2023 18:25:09	U	SMPL
O5760-05 - 1	SLAB	339	0.0471	-	7471B	PPB	13 Dec 2023 18:27:24	U	SMPL
O5765-01 - 1	RT-SB-01-10-11	15371	2.5094	-	7471B	PPB	13 Dec 2023 18:29:40	U	SMPL
O5765-02 - 1	RT-SB-02-10-11	14170	2.3126	-	7471B	PPB	13 Dec 2023 18:31:57	U	SMPL
O5765-03 - 1	RT-SB-03-9.5-10.5	3600	0.5813	-	7471B	PPB	13 Dec 2023 18:34:18	U	SMPL
O5767-01 - 1	SP-E1-COMP	12142	1.9805	-	7471B	PPB	13 Dec 2023 18:36:38	U	SMPL
O5767-04 - 1	SP-E2-COMP	9451	1.5397	-	7471B	PPB	13 Dec 2023 18:38:57	U	SMPL
O5767-07 - 1	SP-E3-COMP	12419	2.0258	-	7471B	PPB	13 Dec 2023 18:41:17	U	SMPL
O5769-01 - 1	WC-1	11982	1.9542	-	7471B	PPB	13 Dec 2023 18:43:35	U	SMPL
CCV05 - 1	CCV05	32391	5.2972	-	7471B	PPB	13 Dec 2023 18:45:54	U	SMPL
CCB05 - 1	CCB05	-155	-0.0338	-	7471B	PPB	13 Dec 2023 18:48:12	U	SMPL
O5789-01 - 1	E8965C-5-001	307106	50.2956	-	7471B	PPB	13 Dec 2023 18:50:37	U	SMPL
O5789-01DUP - 1	E8965C-5-001DUP	310939	HIGH	-	7471B	PPB	13 Dec 2023 18:52:53	X	
O5789-01MS - 1	E8965C-5-001MS	336026	HIGH	-	7471B	PPB	13 Dec 2023 18:59:40	X	
O5789-01MSD - 1	E8965C-5-001MSD	336426	HIGH	-	7471B	PPB	13 Dec 2023 19:01:29	X	
O5789-01LX5 - 1		70708	11.5736	-	7471B	PPB	13 Dec 2023 19:03:36	U	SMPL
O5789-01A - 1		342091	HIGH	-	7471B	PPB	13 Dec 2023 19:06:11	X	
CCV06 - 1	CCV06	32273	5.2779	-	7471B	PPB	13 Dec 2023 19:08:16	U	SMPL
CCB06 - 1	CCB06	-292	-0.0562	-	7471B	PPB	13 Dec 2023 19:10:48	U	SMPL
O5789-01DLX10 - 1		38086	6.2301	-	7471B	PPB	13 Dec 2023 19:13:14	U	SMPL
O5789-01DUPDLX10 - 1		35851	5.8640	-	7471B	PPB	13 Dec 2023 19:18:13	U	SMPL
O5789-01MSDLX10 - 1		46609	7.6262	-	7471B	PPB	13 Dec 2023 19:20:30	U	SMPL
O5789-01MSDDLX10 - 1		48671	7.9639	-	7471B	PPB	13 Dec 2023 19:22:57	U	SMPL
O5789-01LDLX50 - 1		6288	1.0216	-	7471B	PPB	13 Dec 2023 19:25:25	U	SMPL
O5789-01ADLX10 - 1		49280	8.0637	-	7471B	PPB	13 Dec 2023 19:27:52	U	SMPL
CCV07 - 1	CCV07	32004	5.2339	-	7471B	PPB	13 Dec 2023 19:30:10	U	SMPL
CCV07 - 1	CCV07	-105	-0.0256	-	7471B	PPB	13 Dec 2023 19:32:36	U	SMPL