

Clear table


Instrument ID: IC-2										Analyst : IZ		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-13_	11/13/23 11:15		IZ/MA		
STD2	0.4460	0.6910	0.6780	2.3880	0.5830	1.1770	3.6150	2023-11-13_	11/13/23 11:46		IZ/MA		
STD3	0.9080	1.2240	1.2230	4.0930	1.0240	2.0120	6.1460	2023-11-13_	11/13/23 12:18		IZ/MA		
STD4	1.0340	1.4550	1.4610	4.9090	1.2270	2.3440	7.2520	2023-11-13_	11/13/23 12:50		IZ/MA		
STD5	1.8310	2.9140	2.9130	9.6260	2.4080	4.9320	14.3270	2023-11-13_	11/13/23 13:21		IZ/MA		
STD6	3.8100	5.9380	5.9770	19.4790	4.9100	9.9890	29.7250	2023-11-13_	11/13/23 13:53		IZ/MA		
STD7	5.1700	7.5780	7.5490	25.5050	6.3470	12.5460	37.9350	2023-11-13_	11/13/23 14:25		IZ/MA		
ICV	1.8710	3.0150	3.0190	9.9380	2.5400	5.0020	14.8020	2023-11-13_	11/13/23 14:56		IZ/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-13_	11/13/23 15:28		IZ/MA		
CCV	1.9670	3.0730	2.9450	10.0020	2.5180	5.3520	14.4150	2023-12-13_	12/13/23 18:44		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-12-13_	12/13/23 19:48		IZ/MA		
LB128751BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-12-13_	12/13/23 20:19		IZ/MA		
LB128751BSW	2.0660	3.0200	2.9060	9.9840	2.5310	4.9270	14.3390	2023-12-13_	12/13/23 20:51		IZ/MA		
O5812-01	0.5470	20.1950	0.0000	0.0000	0.3210	0.7640	11.7500	2023-12-13_	12/13/23 21:23		IZ/MA		
O5812-01MS	2.8640	22.7230	2.7890	9.8090	2.6370	6.2400	25.0060	2023-12-13_	12/13/23 21:54		IZ/MA		
O5812-01MSD	2.9330	22.5800	2.7030	9.5930	2.6060	6.3930	24.6320	2023-12-13_	12/13/23 22:26		IZ/MA		
O5812-01DLX5	0.0000	3.6390	0.0000	0.0000	0.0000	0.0000	2.9490	2023-12-13_	12/13/23 22:58		IZ/MA		
CCV	2.0830	3.0630	2.8570	10.0840	2.5690	4.9230	14.3630	2023-12-14_	12/14/23 1:36		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-12-14_	12/14/23 2:39		IZ/MA		

Clear table

Instrument ID: IC-2											
Analyst : IZ				Method: 300.0 / 9056A							
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2023-11-13_	11/13/23 11:15		IZ/MA
STD2	0.4460	0.6910	0.6780	2.3880	0.5830	1.1770	3.6150	2023-11-13_	11/13/23 11:46		IZ/MA
STD3	0.8770	1.2240	1.2230	4.0930	1.0240	2.0120	6.1460	2023-11-13_	11/13/23 12:18		IZ/MA
STD4	1.0340	1.4550	1.4610	4.9090	1.2270	2.3440	7.2520	2023-11-13_	11/13/23 12:50		IZ/MA
STD5	1.8310	2.9140	2.9130	9.6260	2.4080	4.9320	14.3270	2023-11-13_	11/13/23 13:21		IZ/MA
STD6	3.8100	5.9380	5.9770	19.4790	4.9100	9.9890	29.7250	2023-11-13_	11/13/23 13:53		IZ/MA
STD7	5.1700	7.5780	7.5490	25.5050	6.3470	12.5460	37.9350	2023-11-13_	11/13/23 14:25		IZ/MA
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	11.5000	15.1667	13.0000	19.4000	16.6000	17.7000	20.5000				
STD3	9.6250	2.0000	1.9167	2.3250	2.4000	0.6000	2.4333				
STD4	3.4000	-3.0000	-2.6000	-1.8200	-1.8400	-6.2400	-3.3067				
STD5	-8.4500	-2.8667	-2.9000	-3.7400	-3.6800	-1.3600	-4.4867				
STD6	-4.7500	-1.0333	-0.3833	-2.6050	-1.8000	-0.1100	-0.9167				
STD7	3.4000	1.0400	0.6533	2.0200	1.5520	0.3680	2.5270				

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.0824636 \cdot A + 4.8961$
 RSD: 7.482 %
 Correlation coefficient: 0.996945

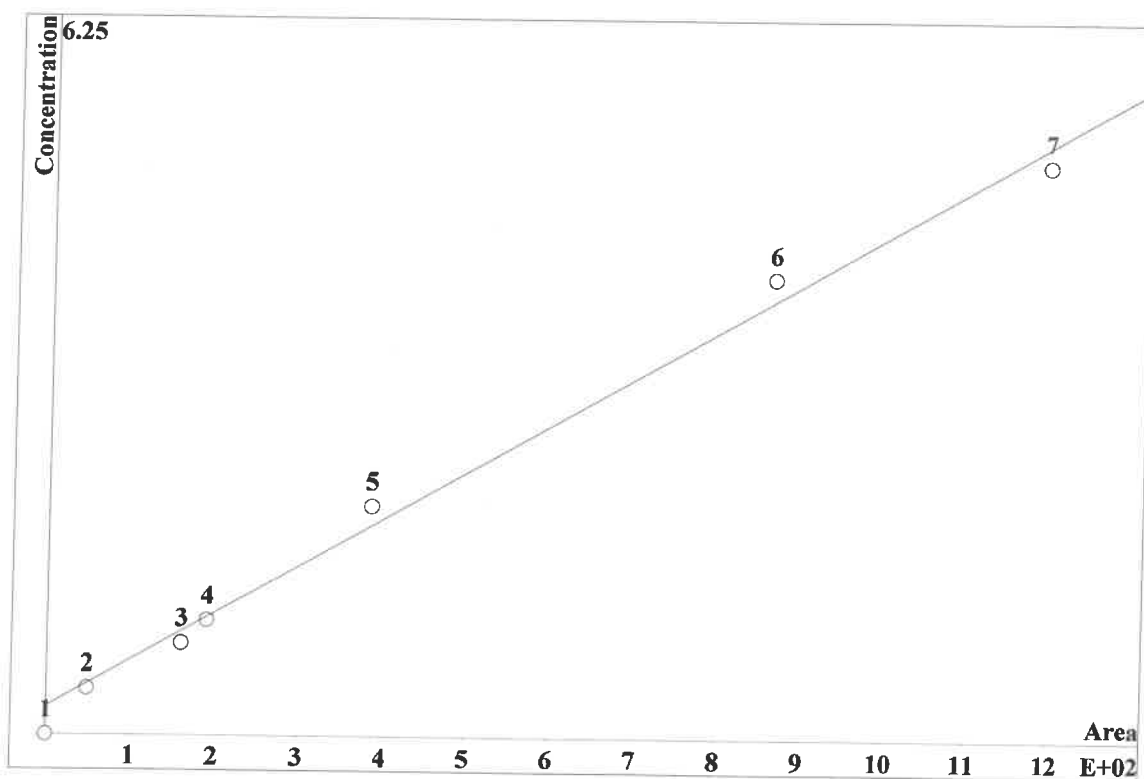


K3 = 0 K2 = 0 K1 = 0.0824636 K0 = 4.8961
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	0.7345	48.88	0.4	20	6.542		
3	1.859	161	0.8	20	6.542		
4	2.263	191.4	1	20	6.542		
5	4.934	384.8	2	20	6.542		
6	11.6	864.7	4	20	6.542		
7	15.42	1194	5	20	6.542		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.127309 \cdot A + 2.88862$
 RSD: 2.540 %
 Correlation coefficient: 0.999648

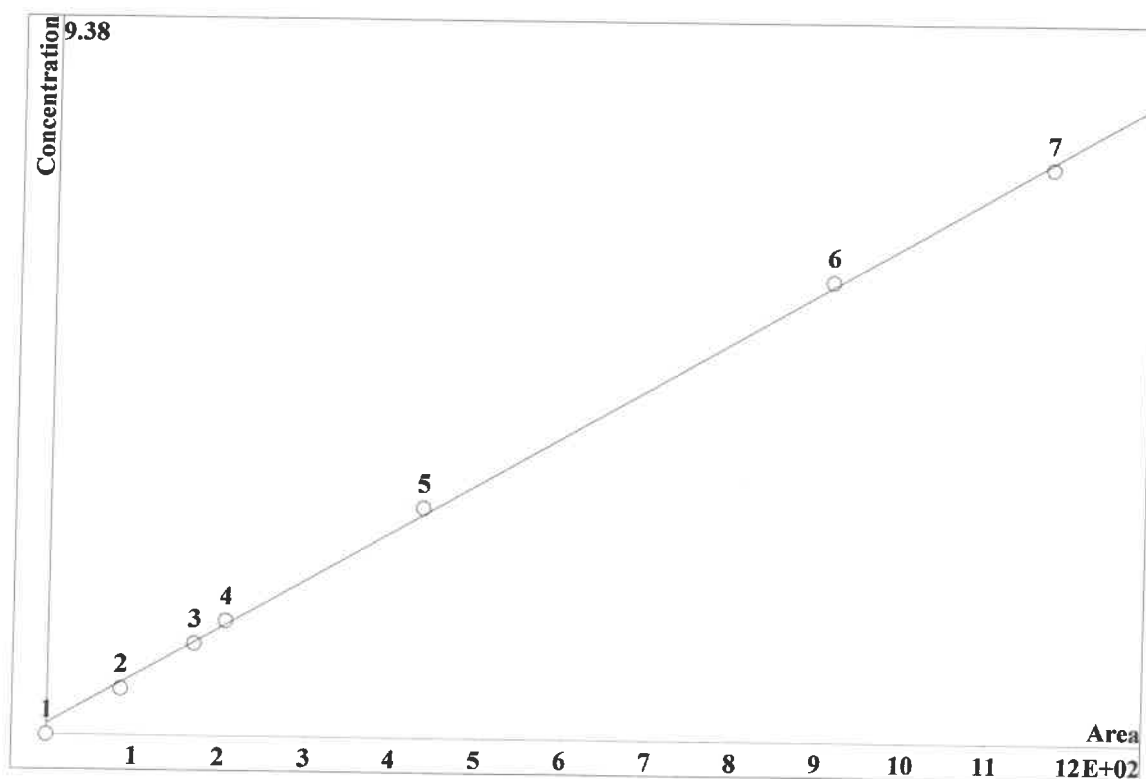


K3 = 0 K2 = 0 K1 = 0.127309 K0 = 2.88862
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.277	85.79	0.6	20	9.354		
3	12.48	169.6	1.2	20	9.354		
4	14.81	205.9	1.5	20	9.354		
5	32.17	435.1	3	20	9.354		
6	67.53	910.2	6	20	9.354		
7	87.51	1168	7.5	20	9.354		
1.□							

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.0571772 \cdot A + 3.49324$
 RSD: 2.070 %
 Correlation coefficient: 0.999766

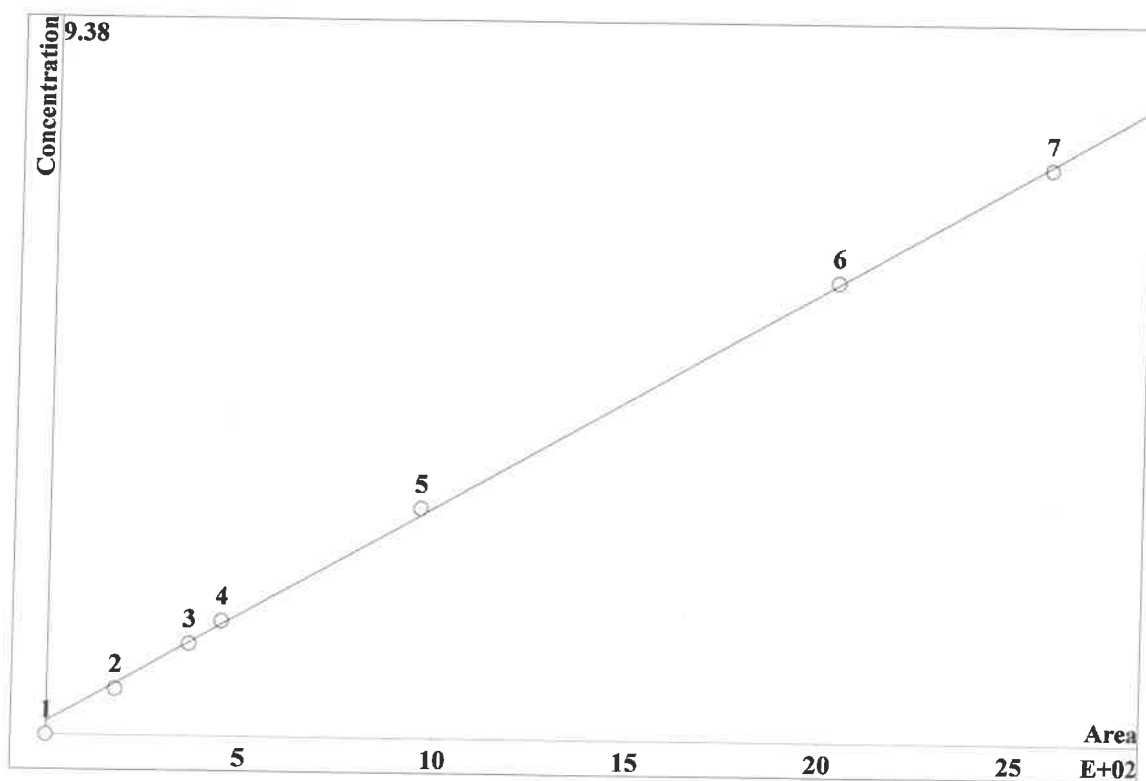


K3 = 0 K2 = 0 K1 = 0.0571772 K0 = 3.49324
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	10.93	176	0.6	20	11.31		
3	22.24	366.7	1.2	20	11.31		
4	26.54	449.8	1.5	20	11.31		
5	56.87	957.9	3	20	11.31		
6	112.8	2029	6	20	11.31		
7	144.1	2579	7.5	20	11.31		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.276865 \cdot A + 14.159$
 RSD: 4.150 %
 Correlation coefficient: 0.999061

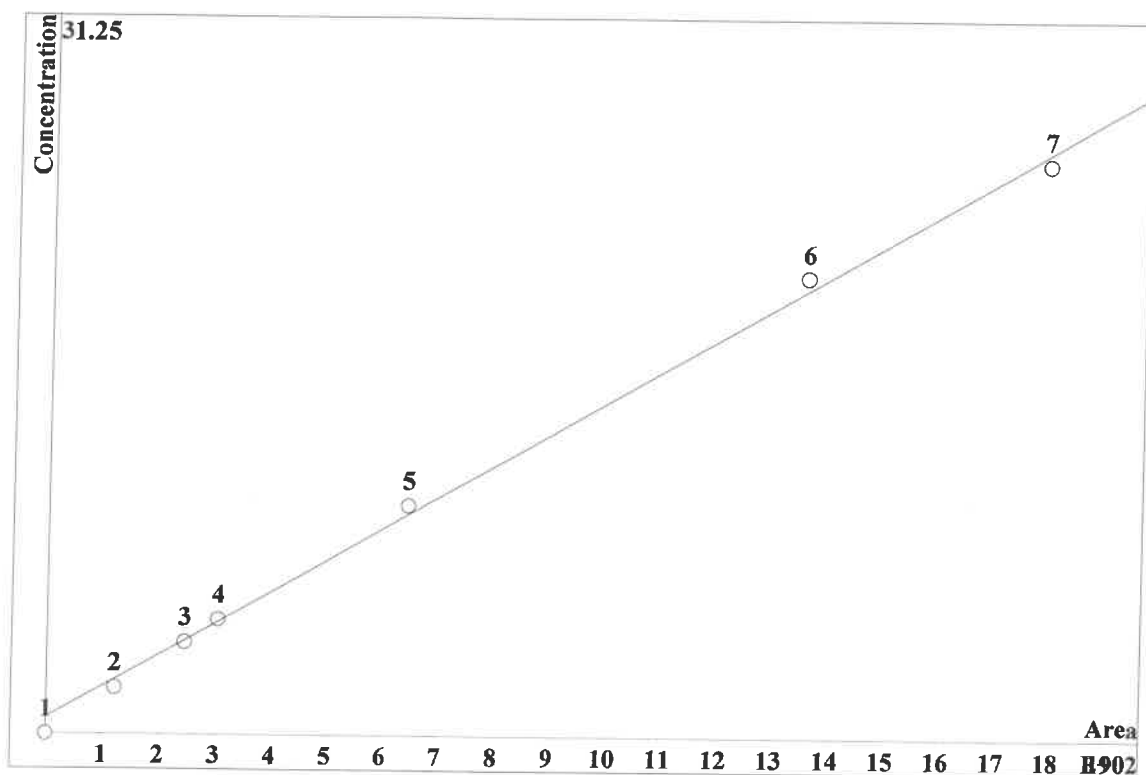


K3 = 0 K2 = 0 K1 = 0.276865 K0 = 14.159
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.545	121.4	2	20	14.7		
3	13.33	244.5	4	20	14.7		
4	15.68	303.5	5	20	14.7		
5	35.1	644.2	10	20	14.7		
6	73.84	1356	20	20	14.7		
7	97.91	1791	25	20	14.7		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.0494246 \cdot A + 3.88198$
 RSD: 3.349 %
 Correlation coefficient: 0.999389

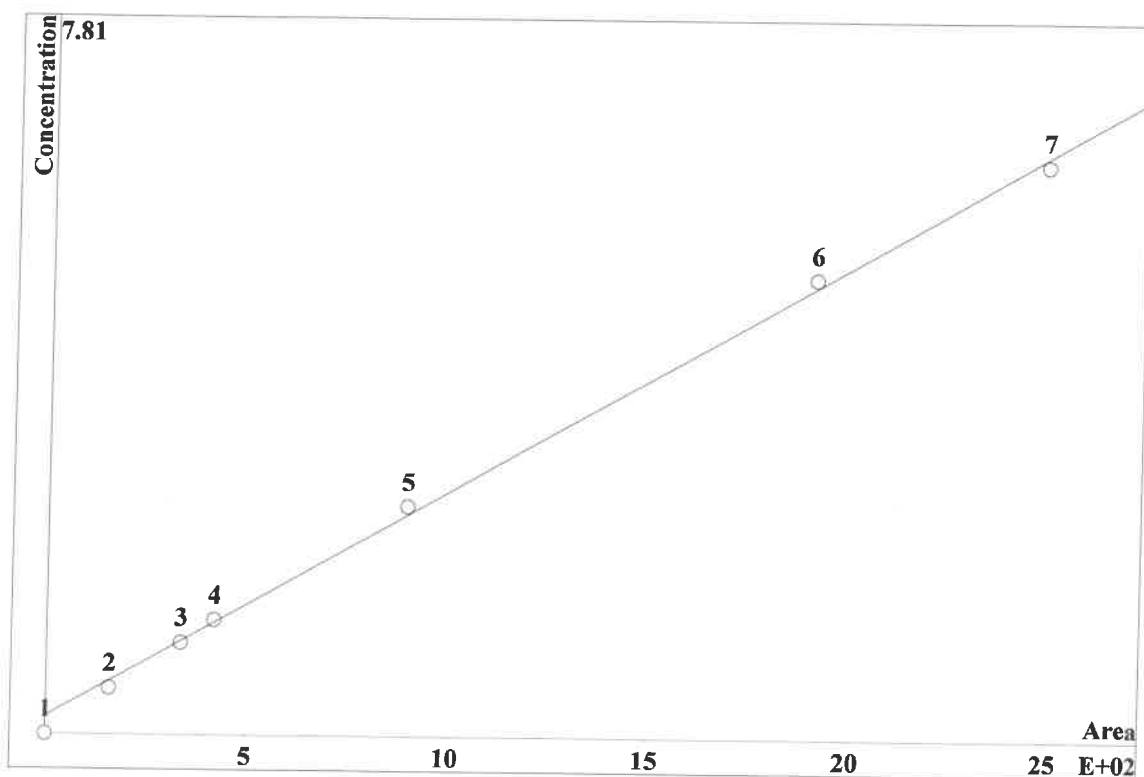


K3 = 0 K2 = 0 K1 = 0.0494246 K0 = 3.88198
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.109	157.4	0.5	20	16.9		
3	15.11	335.9	1	20	16.9		
4	17.74	417.9	1.25	20	16.9		
5	39.98	896	2.5	20	16.9		
6	83.87	1908	5	20	16.9		
7	111.9	2490	6.25	20	16.9		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.045178 \cdot A + 11.6897$
 RSD: 2.273 %
 Correlation coefficient: 0.999718

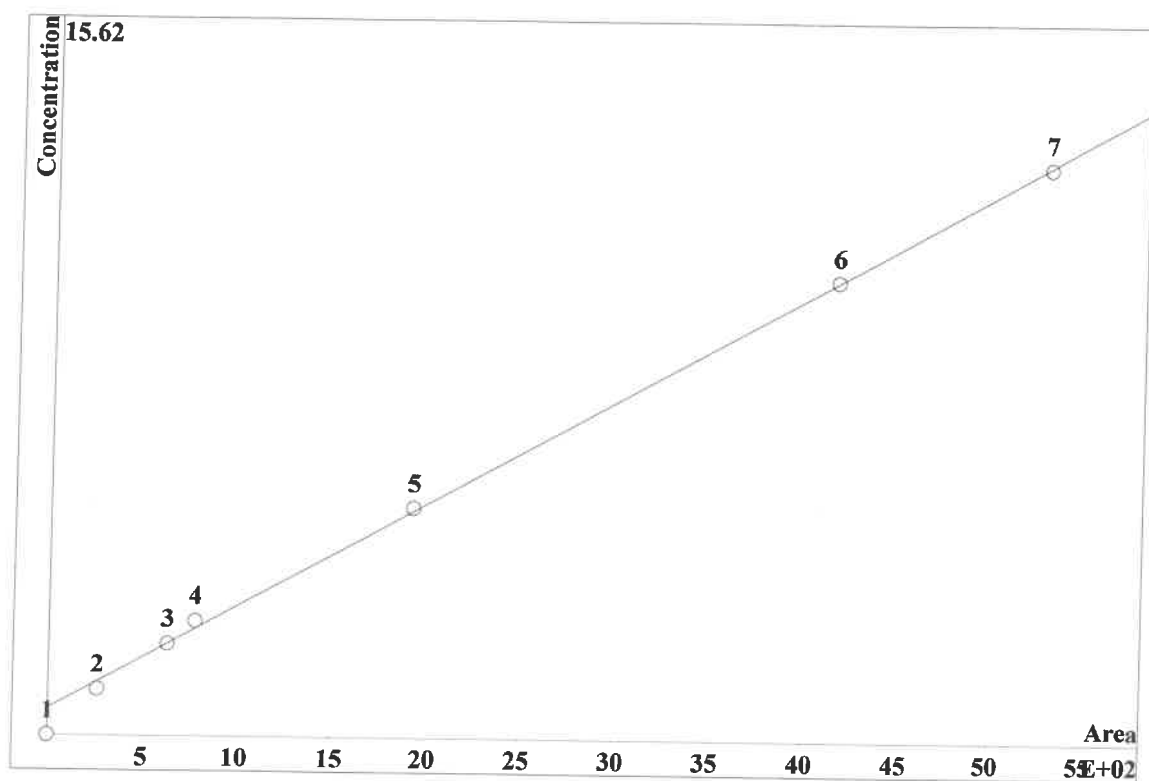


K3 = 0 K2 = 0 K1 = 0.045178 K0 = 11.6897
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.984	262.1	1	20	23.14		
3	12.35	632	2	20	23.14		
4	15.33	779	2.5	20	23.14		
5	41.06	1925	5	20	23.14		
6	97.96	4163	10	20	23.14		
7	129.7	5295	12.5	20	23.14		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-111323.mtw
 Equation: $Q = 0.160188 \cdot A + 18.8161$
 RSD: 3.290 %
 Correlation coefficient: 0.999410

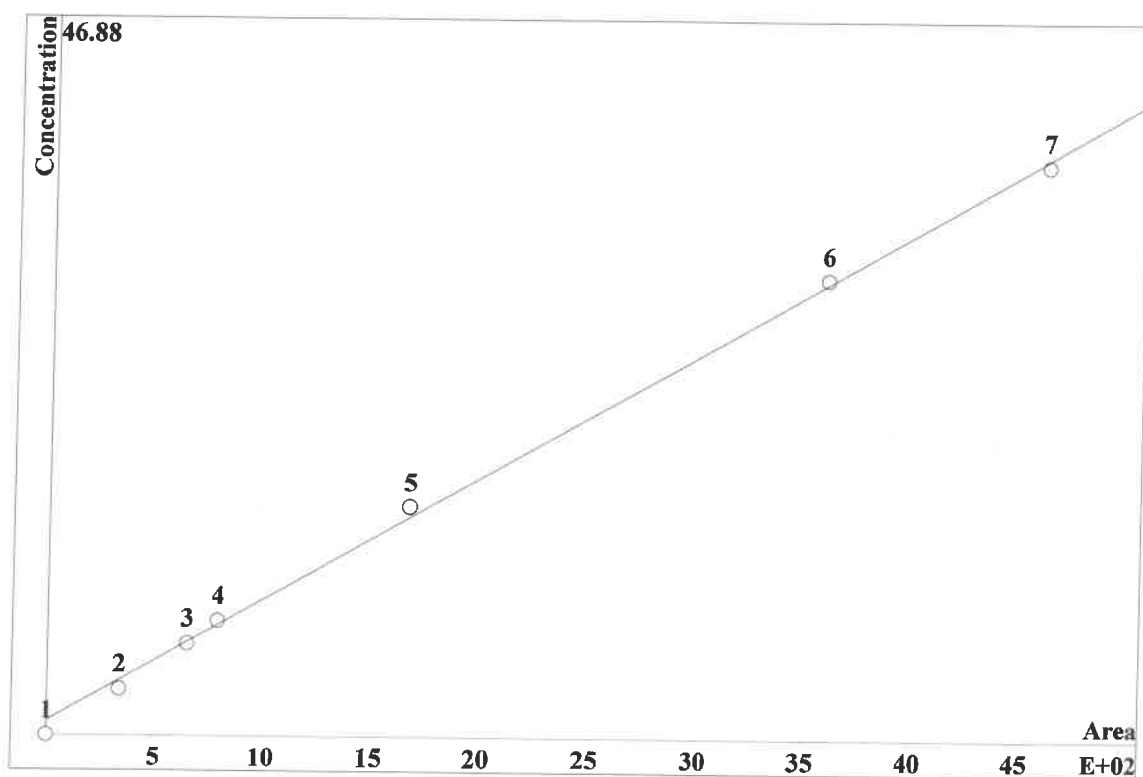

K3 = 0 K2 = 0 K1 = 0.160188 K0 = 18.8161
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	11.38	333.9	3	20	26.6		
3	22.51	649.8	6	20	26.6		
4	27.05	788	7.5	20	26.6		
5	59.42	1671	15	20	26.6		
6	128.5	3594	30	20	26.6		
7	168.8	4619	37.5	20	26.6		

Report date: 11/14/2023 9:58:57 AM
Printed by: wet


Ident: STD1
Analysis from: 11/13/2023 11:15:19 AM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36595

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

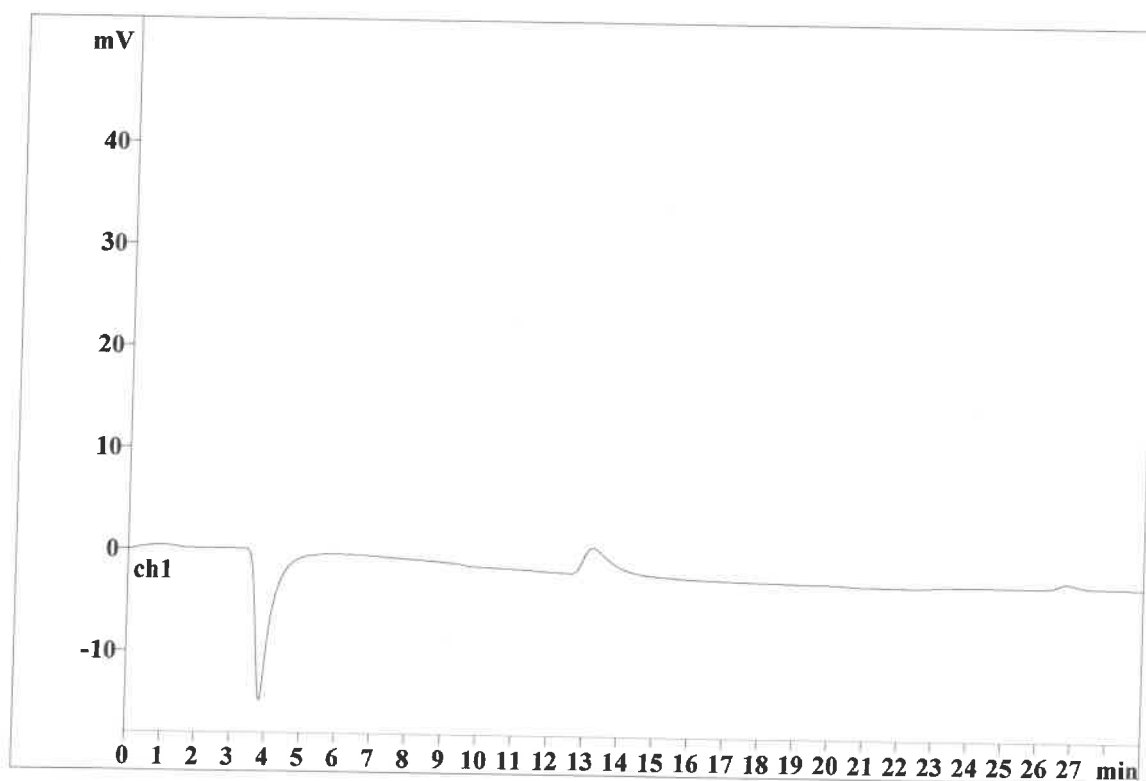

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:05 AM
Printed by: wet


Ident: STD2
Analysis from: 11/13/2023 11:46:57 AM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36596

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

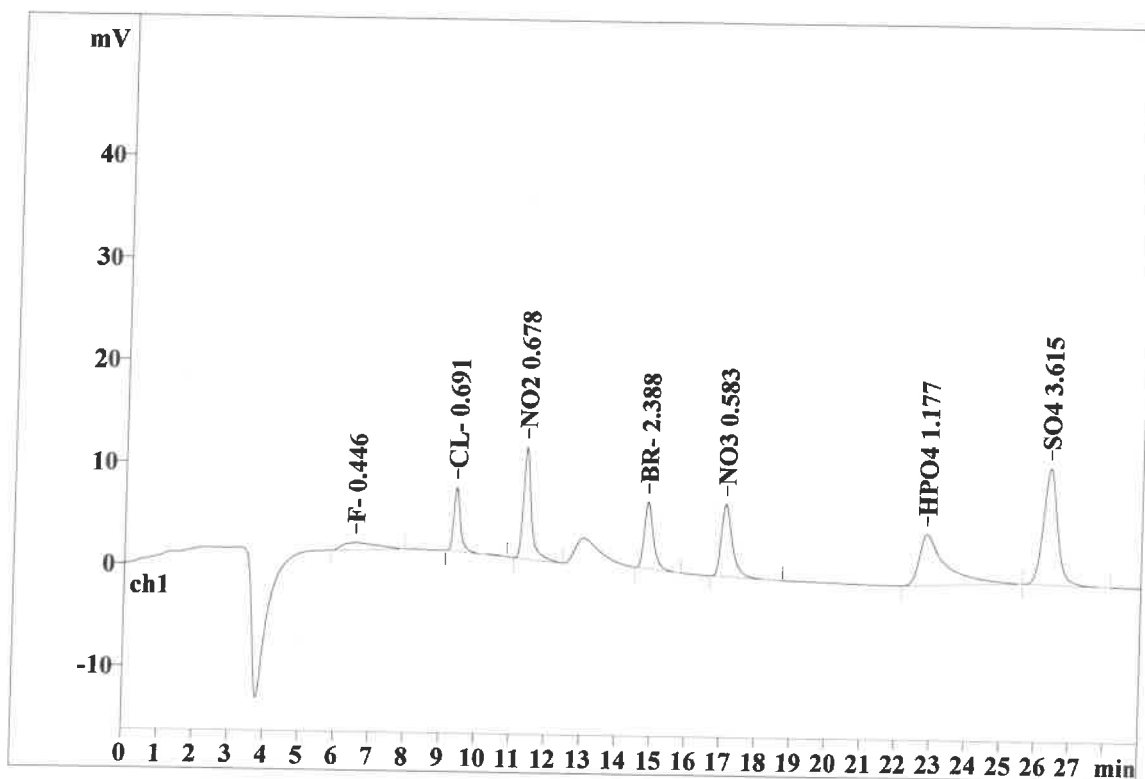

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.53	1.162	0.73	1.53	48.875	4.12
2	9.38	0.190	6.28	13.08	85.789	7.24
3	11.36	0.221	10.93	22.79	176.022	14.85
4	14.82	0.271	6.54	13.64	121.368	10.24
5	17.05	0.319	7.11	14.82	157.437	13.28
6	22.83	0.633	4.98	10.39	262.123	22.11
7	26.34	0.433	11.38	23.73	333.932	28.17
7	29.00	0.461	47.96	99.99	1185.547	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:16 AM
Printed by: wet


Ident: STD3
Analysis from: 11/13/2023 12:18:35 PM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36597

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

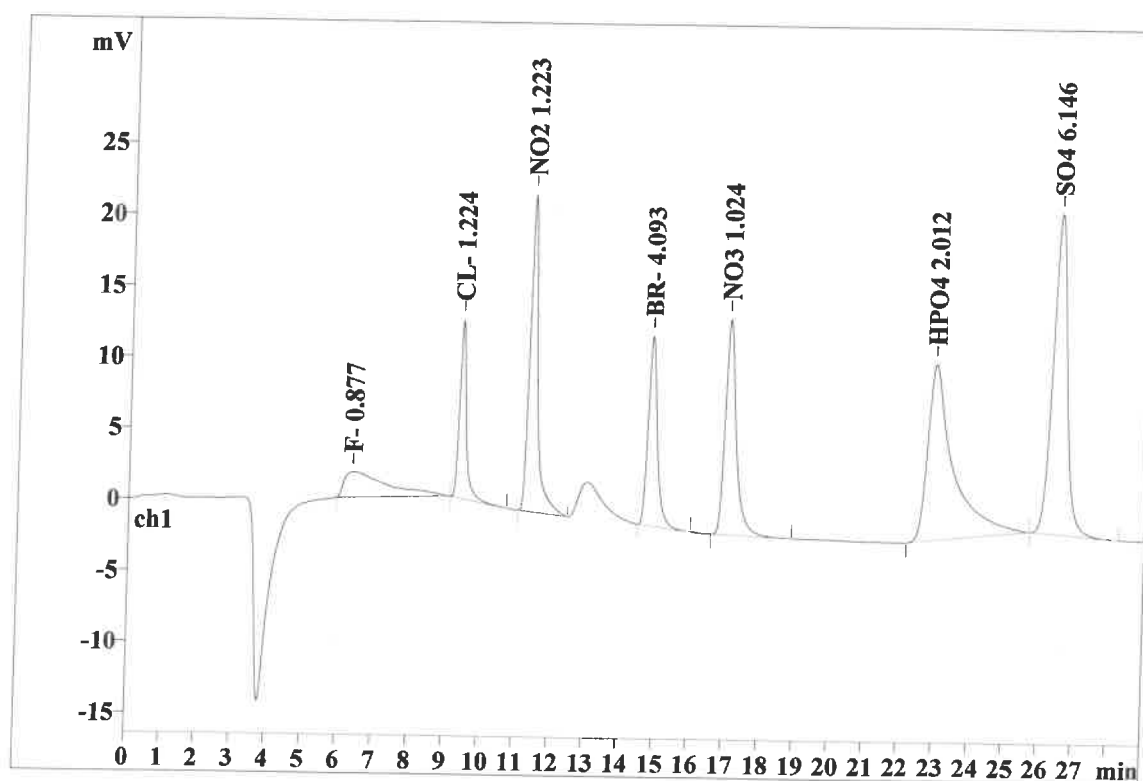

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.35	1.217	1.79	1.80	153.302	6.01
2	9.40	0.188	12.49	12.51	169.615	6.65
3	11.37	0.225	22.23	22.27	366.682	14.37
4	14.82	0.267	13.33	13.35	244.492	9.58
5	17.03	0.317	15.11	15.14	335.927	13.16
6	22.93	0.623	12.35	12.37	632.024	24.77
7	26.46	0.430	22.51	22.55	649.843	25.47
7	29.00	0.467	99.81	99.99	2551.886	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:22 AM
Printed by: wet


Ident: STD4
Analysis from: 11/13/2023 12:50:13 PM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36598

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

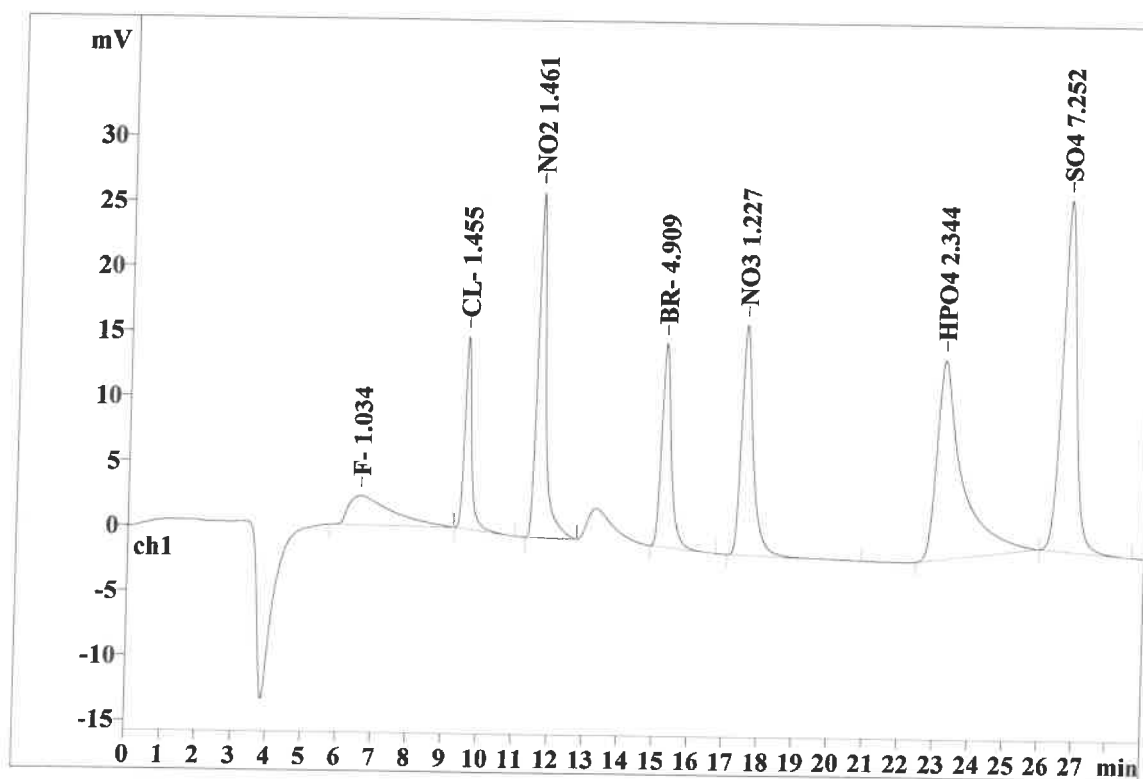

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.59	1.278	2.26	1.89	191.357	6.10
2	9.58	0.194	14.81	12.40	205.927	6.57
3	11.62	0.232	26.54	22.23	449.780	14.34
4	15.21	0.281	15.68	13.13	303.485	9.68
5	17.51	0.334	17.74	14.85	417.944	13.33
6	23.18	0.620	15.33	12.84	779.037	24.85
7	26.72	0.433	27.05	22.65	787.988	25.13
7	29.00	0.482	119.41	100.00	3135.519	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:28 AM
Printed by: wet


Ident: STD5
Analysis from: 11/13/2023 1:21:51 PM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36599

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

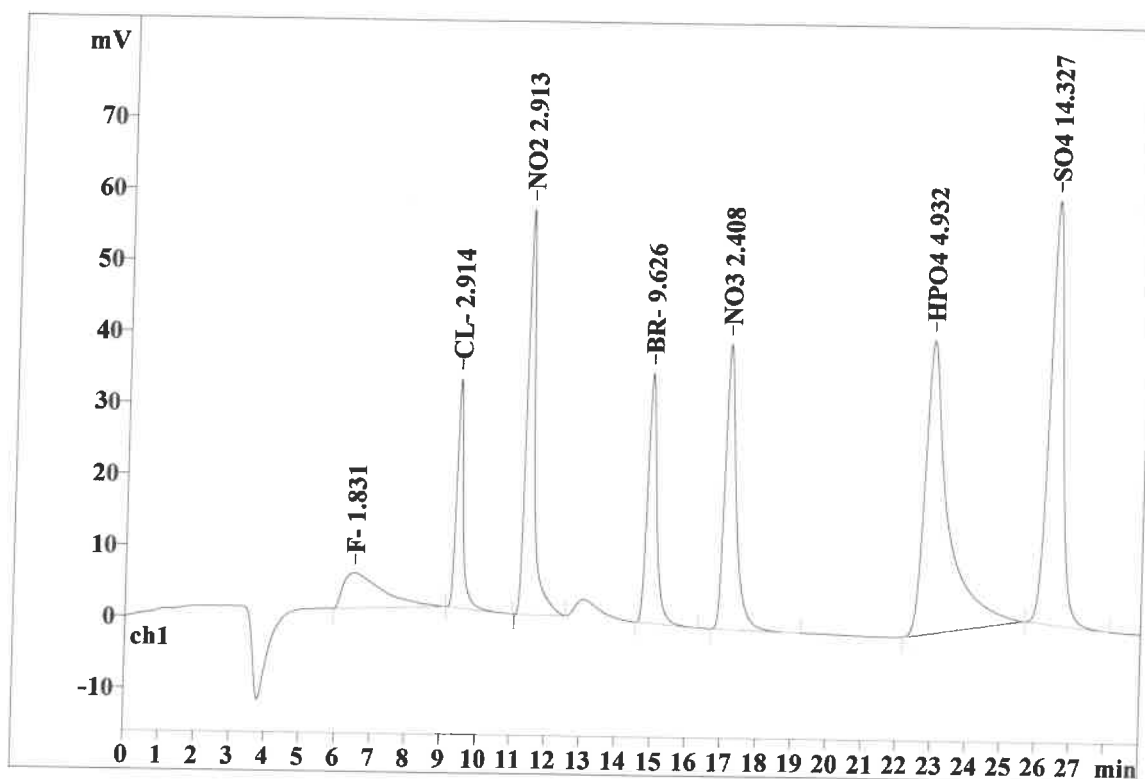

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.49	1.170	4.93	1.83	384.816	5.57
2	9.43	0.187	32.17	11.93	435.100	6.29
3	11.40	0.228	56.86	21.10	957.862	13.85
4	14.89	0.265	35.10	13.02	644.190	9.32
5	17.10	0.317	39.98	14.83	895.955	12.96
6	22.90	0.570	41.06	15.23	1924.579	27.84
7	26.44	0.419	59.42	22.05	1671.302	24.17
7	29.00	0.451	269.52	100.00	6913.805	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:35 AM
Printed by: wet


Ident: STD6
Analysis from: 11/13/2023 1:53:28 PM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36600

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

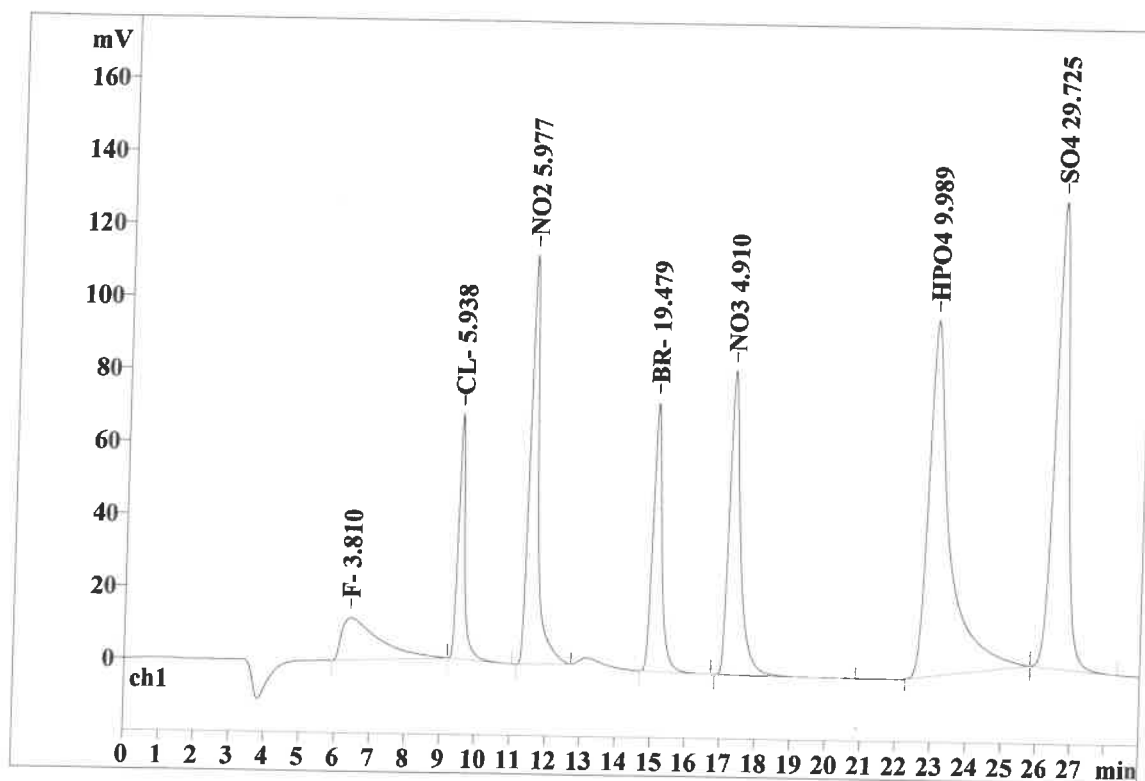

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.42	1.084	11.60	2.01	864.694	5.83
2	9.50	0.187	67.54	11.72	910.158	6.14
3	11.49	0.244	112.82	19.58	2029.438	13.69
4	15.06	0.264	73.84	12.82	1356.007	9.15
5	17.25	0.318	83.86	14.56	1908.470	12.87
6	22.98	0.517	97.96	17.00	4163.229	28.08
7	26.57	0.416	128.50	22.30	3593.795	24.24
7	29.00	0.433	576.10	100.00	14825.792	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:43 AM
Printed by: wet


Ident: STD7
Analysis from: 11/13/2023 2:25:07 PM
File: _2023-11-13_

Last save: 11/13/2023 3:01:30 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36601

Last save: 11/13/2023 2:22

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

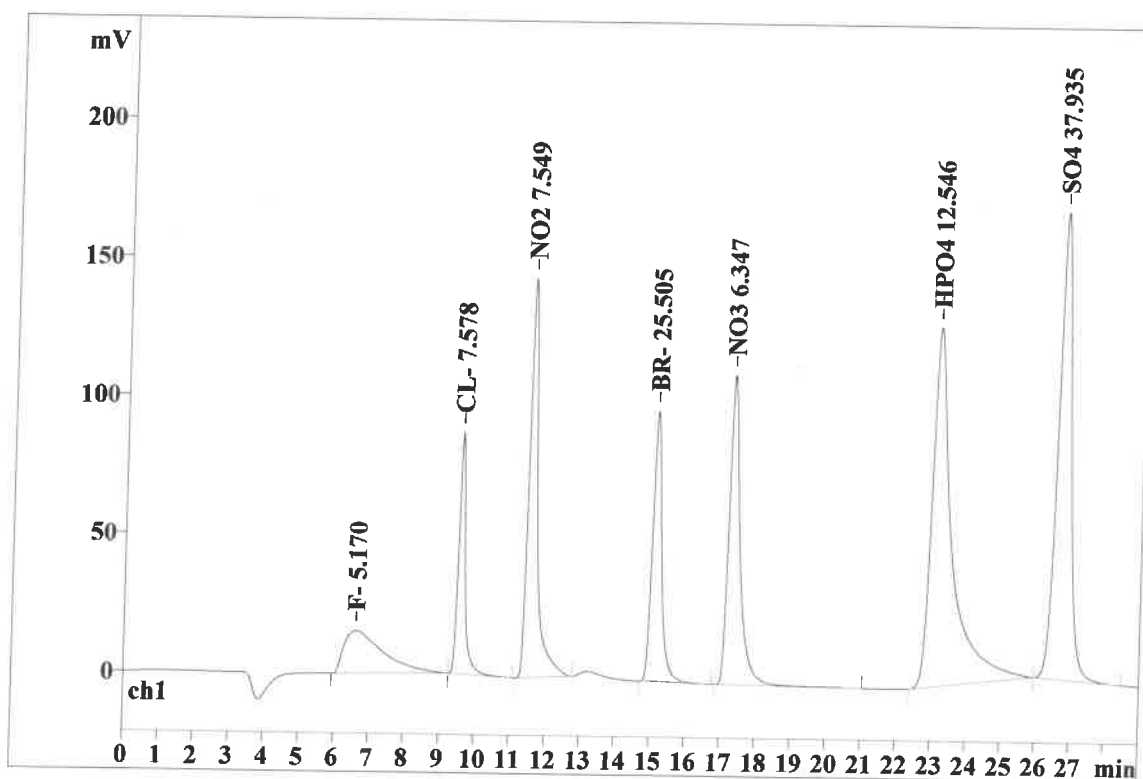

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.61	1.174	15.42	2.04	1194.475	6.24
2	9.56	0.184	87.51	11.59	1167.813	6.10
3	11.52	0.241	144.14	19.08	2579.488	13.48
4	15.10	0.263	97.91	12.96	1791.287	9.36
5	17.26	0.307	111.85	14.81	2489.846	13.01
6	23.10	0.499	129.68	17.17	5295.395	27.67
7	26.70	0.407	168.78	22.35	4618.805	24.14
7	29.00	0.439	755.28	100.00	19137.110	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:51 AM
Printed by: wet


Ident: ICV
Analysis from: 11/13/2023 2:56:45 PM
File: _2023-11-13_

Last save: 11/13/2023 3:25:45 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36602

Last save: 11/13/2023 2:54

SAMPLE:
: IZ/MA
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

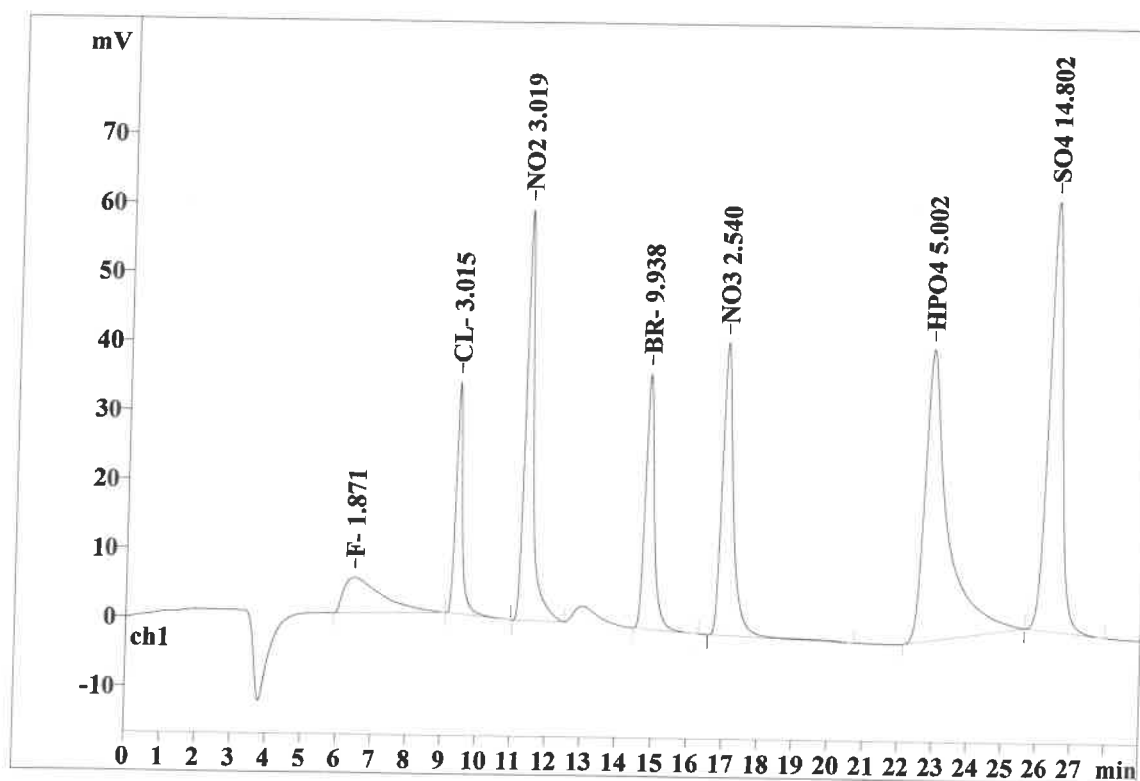

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.46	1.152	5.13	1.82	394.403	5.52
2	9.39	0.186	33.55	11.90	450.957	6.31
3	11.35	0.227	59.43	21.08	994.871	13.93
4	14.81	0.261	36.94	13.11	666.736	9.33
5	16.97	0.310	42.42	15.05	949.414	13.29
6	22.86	0.561	42.17	14.96	1955.766	27.38
7	26.39	0.415	62.23	22.08	1730.620	24.23
7	29.00	0.445	281.87	100.00	7142.766	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/14/2023 9:59:58 AM
Printed by: wet

Ident: ICB
Analysis from: 11/13/2023 3:28:23 PM
File: _2023-11-13_


Last save: 11/13/2023 3:57:23 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36603

Last save: 11/13/2023 2:54

SAMPLE:

: IZ/MA
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

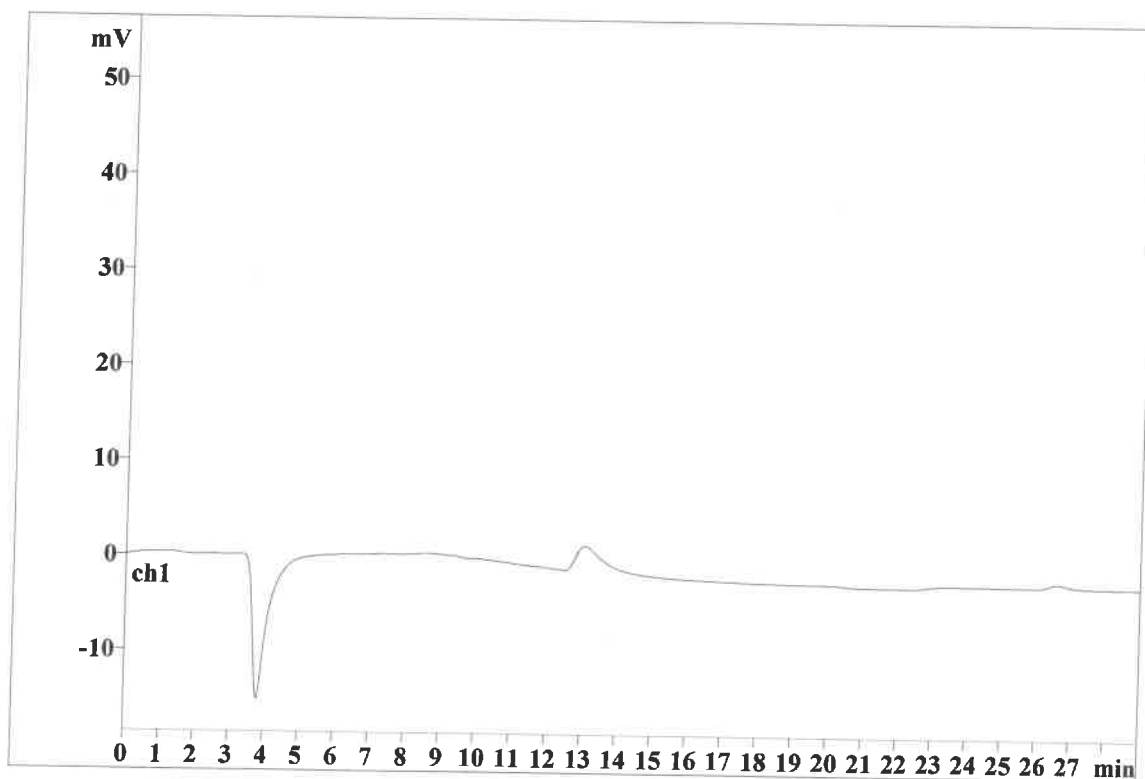

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:47:13 AM
Printed by: wet


Ident: CCV
Analysis from: 12/13/2023 6:44:49 PM
File: _2023-12-13_

Last save: 12/15/2023 9:47:14 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36928

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

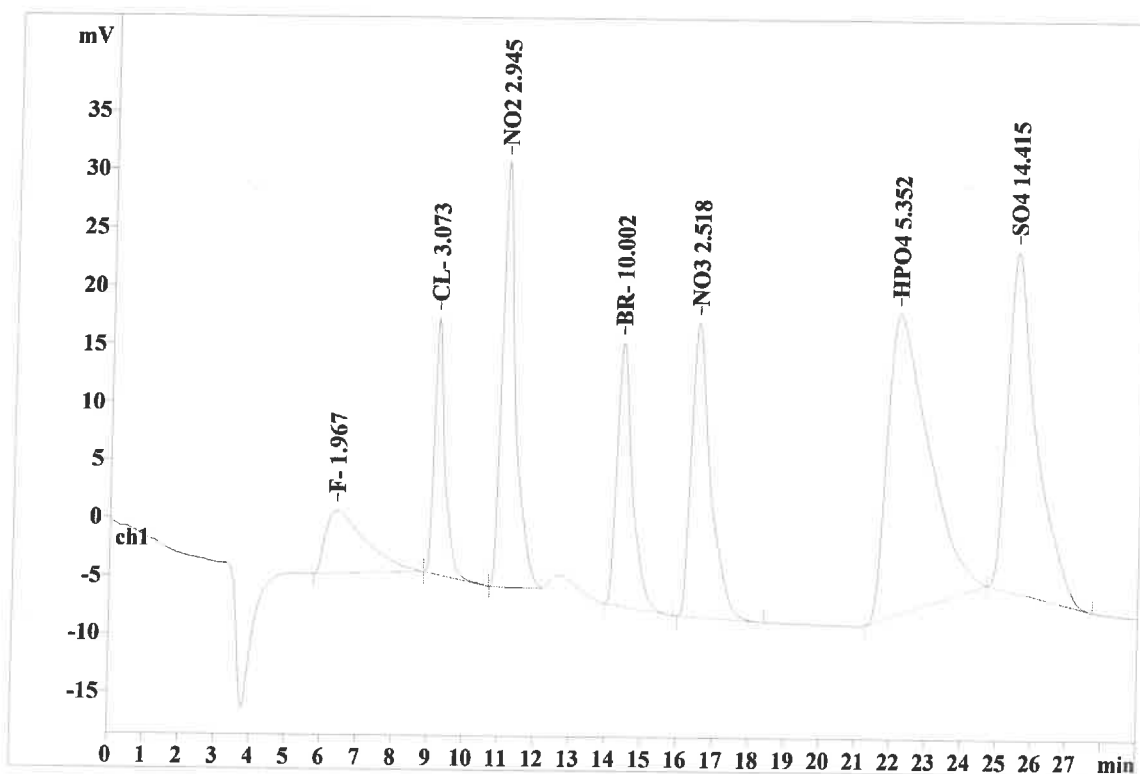

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.36	1.179	5.41	3.24	417.728	5.7
2	9.17	0.289	21.99	13.15	460.036	6.3
3	11.06	0.366	36.52	21.84	969.051	13.3
4	14.36	0.427	22.67	13.56	671.378	9.2
5	16.45	0.531	25.33	15.15	940.479	12.9
6	22.10	1.273	25.98	15.54	2110.390	29.1
7	25.43	0.810	29.26	17.51	1682.287	23.2
7	29.00	0.696	167.15	99.99	7251.349	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:47:00 AM
Printed by: wet


Ident: CCB
Analysis from: 12/13/2023 7:48:13 PM
File: _2023-12-13_

Last save: 12/15/2023 9:47:00 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36930

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

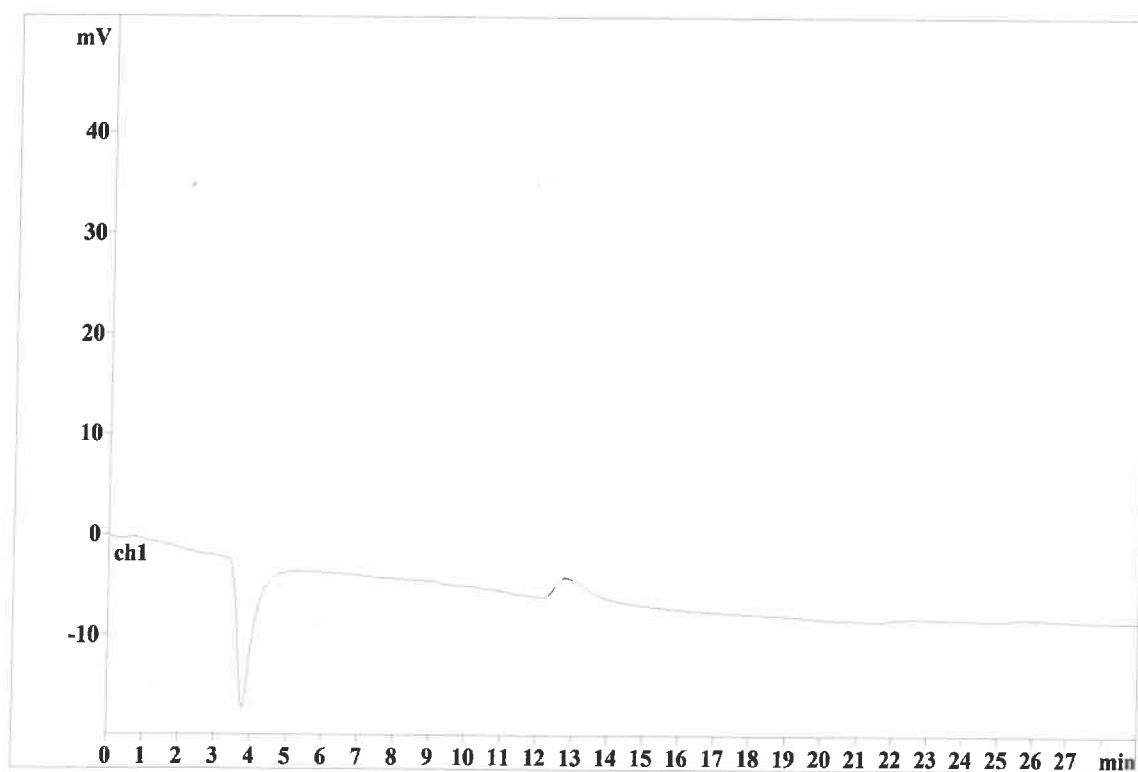

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:41:56 AM
Printed by: wet


Ident: LB128751BLW
Analysis from: 12/13/2023 8:19:50 PM
File: _2023-12-13_

Last save: 12/15/2023 9:41:08 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36931

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

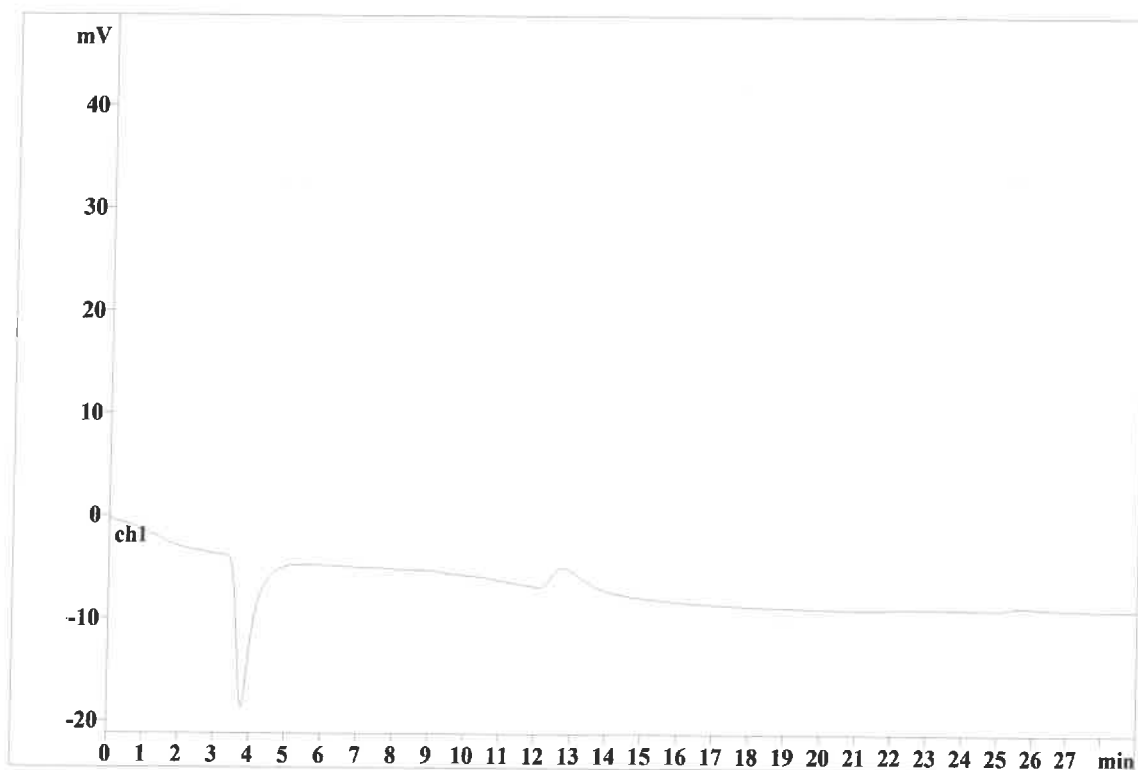

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:42:02 AM
Printed by: wet


Ident: LB128751BSW
Analysis from: 12/13/2023 8:51:28 PM
File: _2023-12-13_

Last save: 12/15/2023 9:41:08 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36932

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

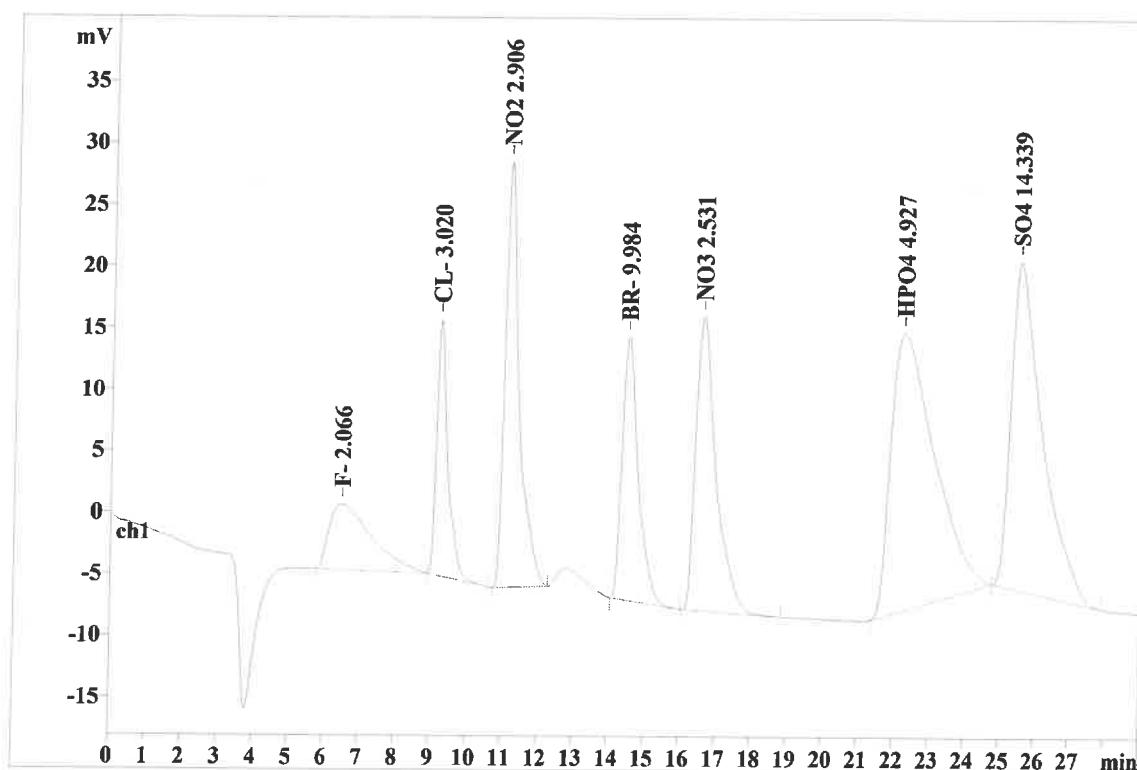

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.50	1.286	5.33	3.44	441.734	6.2
2	9.22	0.303	20.76	13.40	451.817	6.4
3	11.12	0.381	34.50	22.27	955.540	13.5
4	14.49	0.459	21.32	13.76	670.103	9.4
5	16.58	0.572	23.82	15.37	945.660	13.3
6	22.21	1.331	22.58	14.57	1922.393	27.2
7	25.49	0.920	26.64	17.19	1672.858	23.6
7	29.00	0.750	154.95	100.00	7060.104	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:42:17 AM
Printed by: wet


Ident: 05812-01
Analysis from: 12/13/2023 9:23:12 PM
File: _2023-12-13_

Last save: 12/13/2023 9:52:14 PM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36933

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 45
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

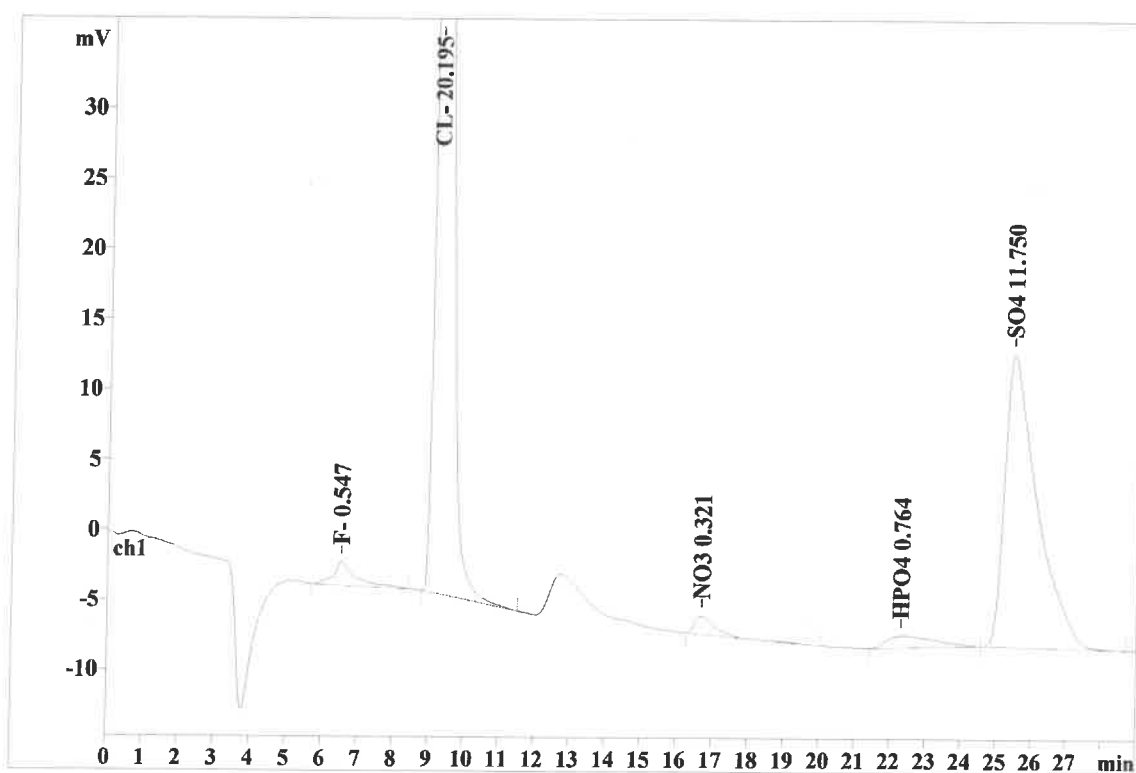

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.52	0.445	1.69	0.98	73.334	1.5
2	9.18	0.290	147.51	85.68	3149.864	66.9
3	0.00	0.000	0.00	0.00	0.000	0.0
4	0.00	0.000	0.00	0.00	0.000	0.0
5	16.70	0.558	1.28	0.74	51.225	1.0
6	22.32	1.570	0.84	0.49	79.309	1.6
7	25.42	0.947	20.84	12.11	1349.588	28.6
7	29.00	0.544	172.16	100.00	4703.321	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:42:33 AM
Printed by: wet


Ident: 05812-01MS
Analysis from: 12/13/2023 9:54:49 PM
File: _2023-12-13_

Last save: 12/13/2023 10:23:52 P

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36934

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 46
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

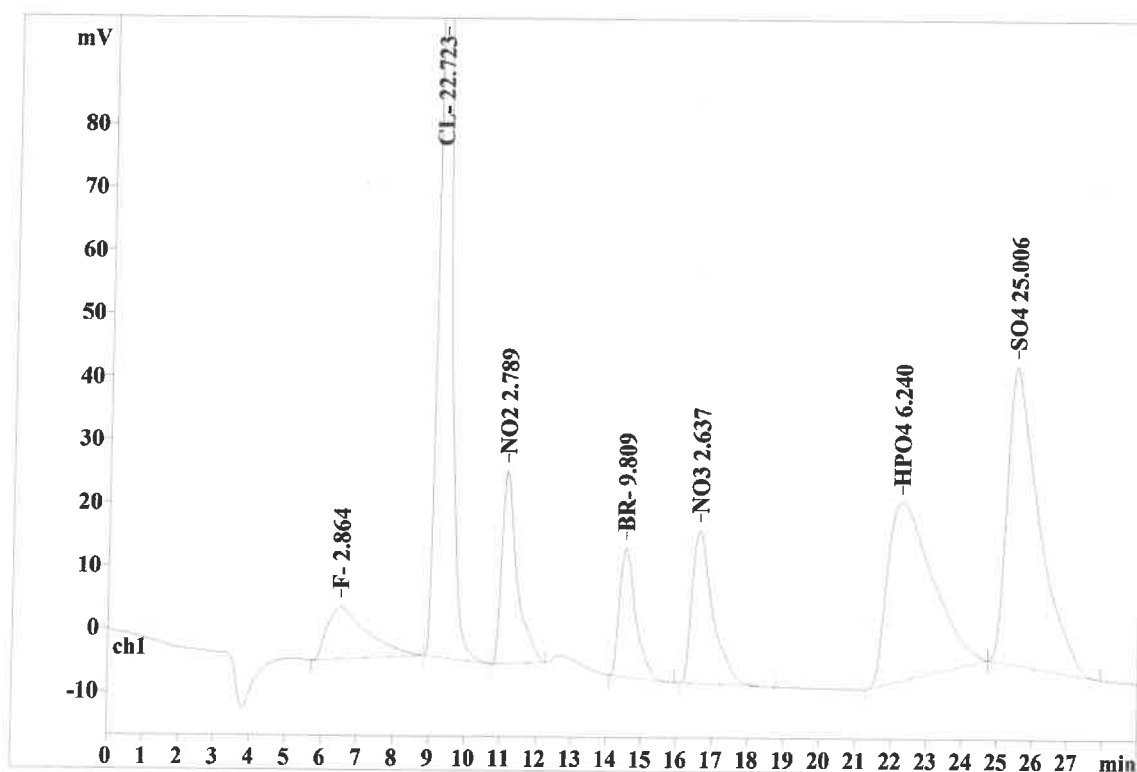

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.51	1.153	8.41	2.59	635.171	5.1
2	9.20	0.293	165.22	50.95	3547.007	28.9
3	11.12	0.414	30.60	9.44	914.603	7.4
4	14.51	0.475	20.31	6.26	657.405	5.3
5	16.59	0.588	24.28	7.49	988.464	8.0
6	22.22	1.401	28.29	8.72	2503.494	20.4
7	25.43	0.943	47.18	14.55	3004.624	24.5
7	29.00	0.753	324.30	100.00	12250.768	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:42:41 AM
Printed by: wet


Ident: O5812-01MSD
Analysis from: 12/13/2023 10:26:27 PM
File: _2023-12-13_

Last save: 12/13/2023 10:55:30 P

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36935

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 47
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

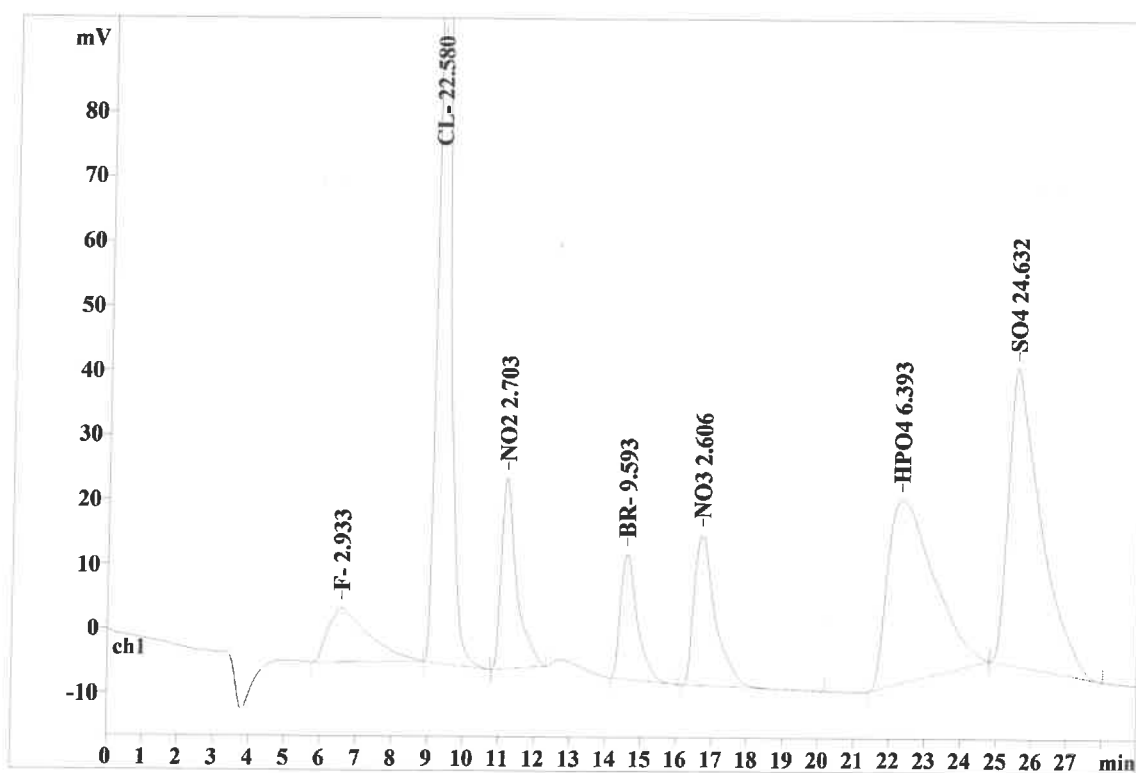

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.56	1.205	8.41	2.65	651.856	5.3
2	9.23	0.298	162.21	51.14	3524.540	28.8
3	11.16	0.416	29.49	9.30	884.435	7.2
4	14.57	0.489	19.32	6.09	641.840	5.2
5	16.67	0.605	23.23	7.32	975.954	7.9
6	22.28	1.435	28.43	8.96	2571.368	21.0
7	25.49	0.957	46.09	14.53	2957.967	24.2
7	29.00	0.772	317.18	100.00	12207.960	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:43:06 AM
Printed by: wet


Ident: 05812-01DLX5
Analysis from: 12/13/2023 10:58:06 PM
File: _2023-12-13_

Last save: 12/15/2023 9:43:02 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36936

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 48
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

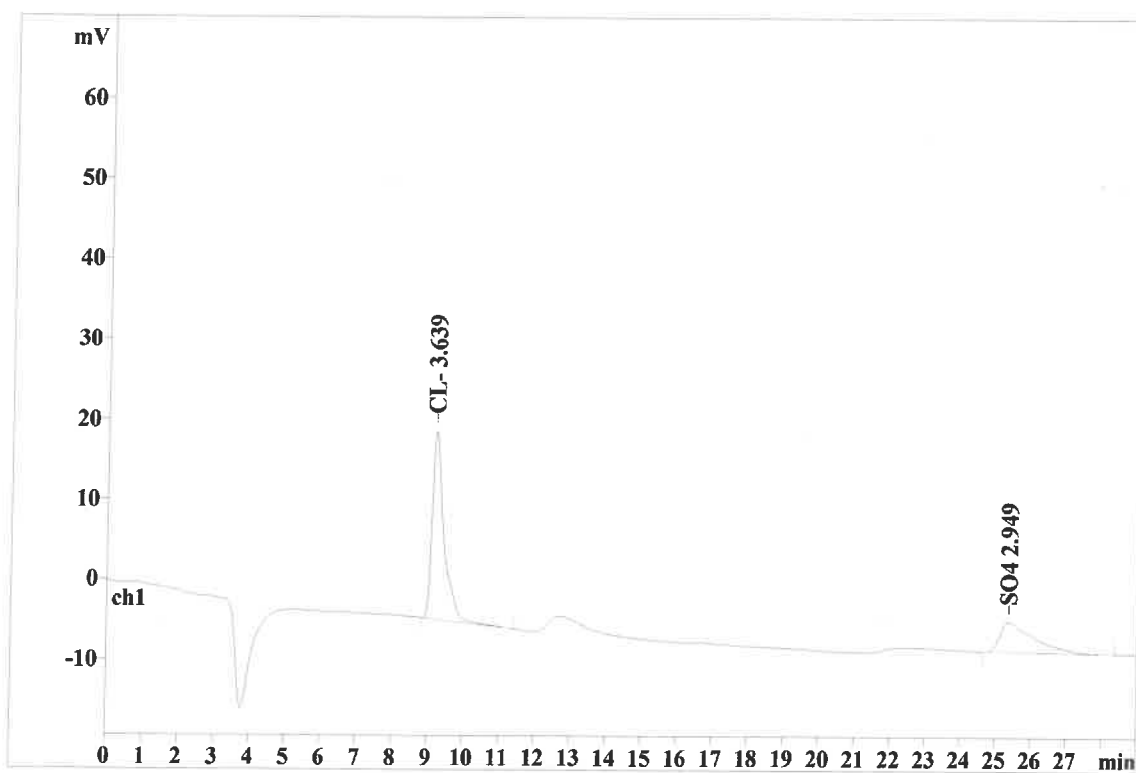

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	0.00	0.000	0.00	0.00	0.000	0.0
2	9.19	0.321	23.46	86.21	549.043	68.6
3	0.00	0.000	0.00	0.00	0.000	0.0
4	0.00	0.000	0.00	0.00	0.000	0.0
5	0.00	0.000	0.00	0.00	0.000	0.0
6	0.00	0.000	0.00	0.00	0.000	0.0
7	25.36	1.000	3.75	13.78	250.757	31.3
7	29.00	0.189	27.21	99.99	799.800	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:44:15 AM
Printed by: wet


Ident: CCV
Analysis from: 12/14/2023 1:36:20 AM
File: _2023-12-14_

Last save: 12/14/2023 2:05:22 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36941

Last save: 12/8/2023 12:

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

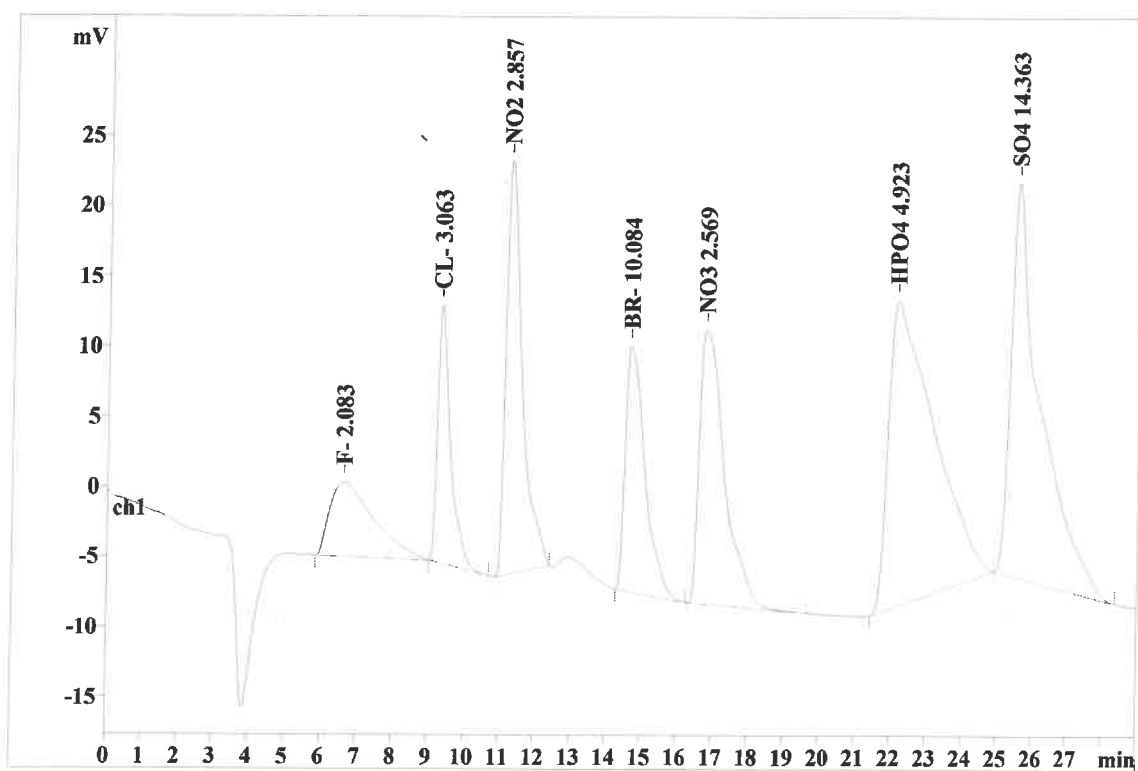

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Are
1	6.60	1.326	5.26	3.76	445.910	6.3
2	9.30	0.355	18.33	13.09	458.571	6.4
3	11.23	0.458	29.41	21.00	938.150	13.2
4	14.64	0.575	17.55	12.53	677.323	9.5
5	16.74	0.718	19.55	13.96	961.121	13.5
6	22.12	1.393	21.82	15.58	1920.541	27.1
7	25.51	0.711	28.13	20.08	1675.809	23.6
7	29.00	0.791	140.05	99.99	7077.425	100.0

This report has been created by IC Net
METROHM LTD

Report date: 12/15/2023 9:44:22 AM
Printed by: wet


Ident: CCB
Analysis from: 12/14/2023 2:39:51 AM
File: _2023-12-14_

Last save: 12/14/2023 3:08:54 AM

Method: AnionsIC2-111323.mtw
Run operator: wet
Analysis number: 36943

Last save: 12/8/2023 12:

SAMPLE:
:
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

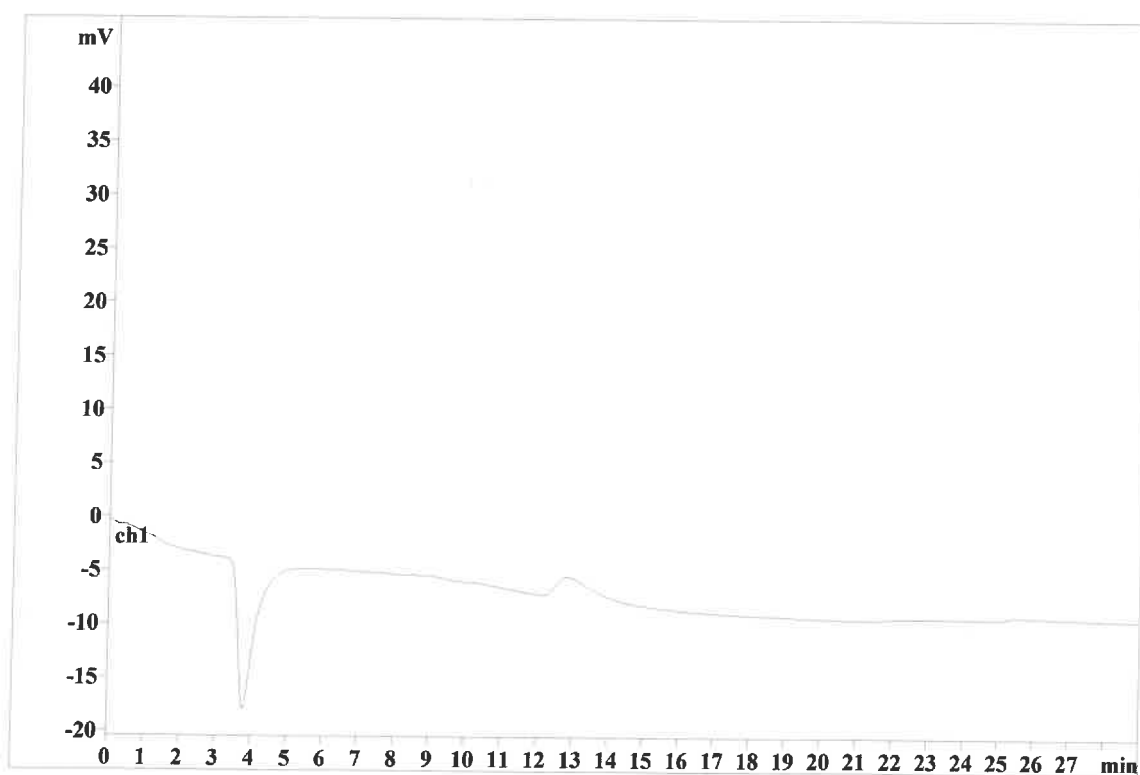

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD