


LB128757

7470A

INSTRUMENT ID: CV2

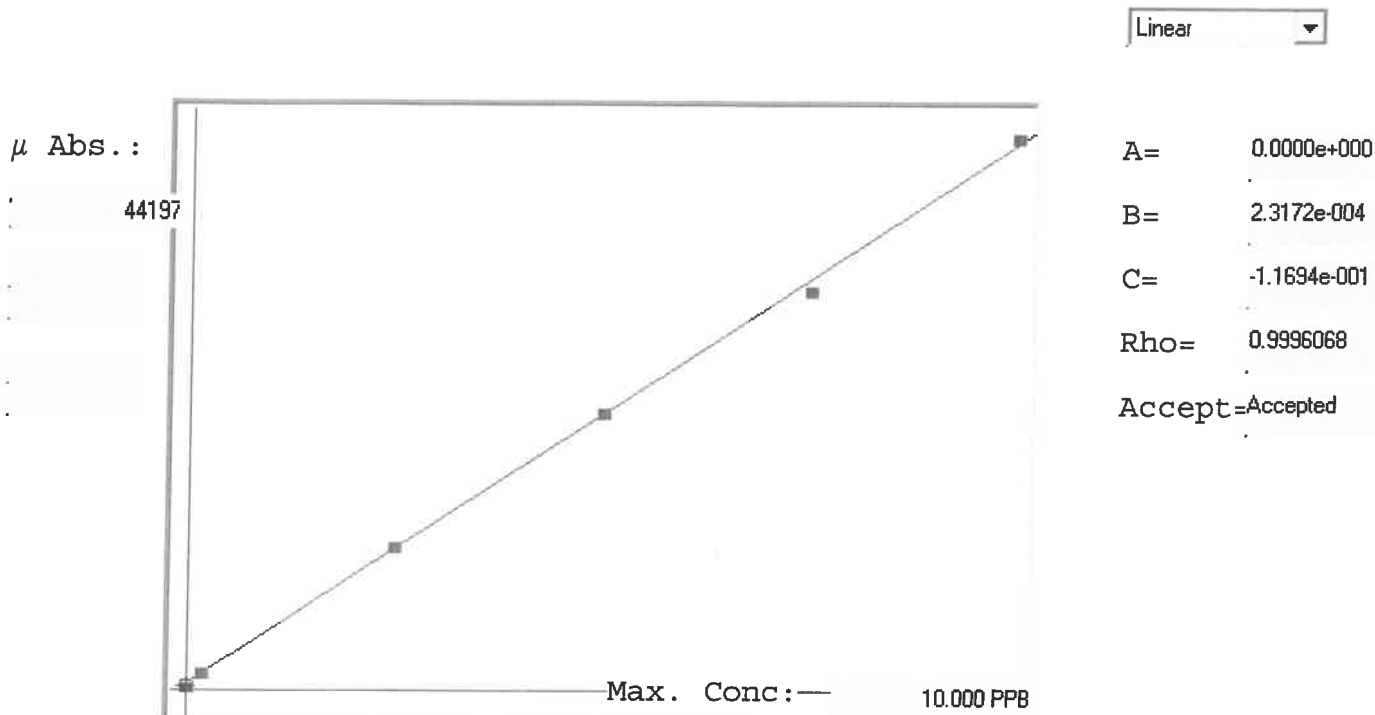

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	✓/VD
0.0	0.000	-0.021	-0.021	416	0.000	416	0				14
0.2	0.200	0.227	0.027	1485	0.0 %	1485					2
2.5	2.500	2.553	0.053	11523	0.0 %	11523					1
5.0	5.000	5.026	0.026	22195	0.0 %	22195					3
7.5	7.500	7.290	-0.210	31965	0.0 %	31965					1
10.0	10.000	10.124	0.124	44197	0.0 %	44197					

LB128757 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Dec 2023 14:07:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	56	416	-	0.000	7470A	PPB	15 Dec 2023 14:19:30	S	Std
0.2 - 1	50.2	1485	-	0.200	7470A	PPB	15 Dec 2023 14:21:47	S	Std
2.5 - 1	52.5	11523	-	2.500	7470A	PPB	15 Dec 2023 14:24:05	S	Std
5.0 - 1	55	22195	-	5.000	7470A	PPB	15 Dec 2023 14:26:22	S	Std
7.5 - 1	57.5	31965	-	7.500	7470A	PPB	15 Dec 2023 14:28:40	S	Std
10.0 - 1	510	44197	-	10.000	7470A	PPB	15 Dec 2023 14:36:15	S	Std
ICV27 - 1	ICV27	16072	3.6072	-	7470A	PPB	15 Dec 2023 14:39:05	U	SMPL
ICB27 - 1	ICB27	322	-0.0423	-	7470A	PPB	15 Dec 2023 14:43:59	U	SMPL
CCV21 - 1	CCV21	22127	5.0103	-	7470A	PPB	15 Dec 2023 14:46:14	U	SMPL
CCB21 - 1	CCB21	369	-0.0314	-	7470A	PPB	15 Dec 2023 14:51:08	U	SMPL
CRA - 1	CRA	1442	0.2172	-	7470A	PPB	15 Dec 2023 14:57:00	U	SMPL
HighStd - 1	HighStd	44030	10.0856	-	7470A	PPB	15 Dec 2023 14:59:15	U	SMPL
ChkStd - 1	ChkStd	28991	6.6008	-	7470A	PPB	15 Dec 2023 15:01:30	U	SMPL
PB157842BL - 1	PBW	-25	-0.1227	-	7470A	PPB	15 Dec 2023 15:06:35	U	SMPL
PB157842BS - 1	LCSW	16783	3.7720	-	7470A	PPB	15 Dec 2023 15:08:51	U	SMPL
O5803-03 - 1	600572408-	-277	-0.1811	-	7470A	PPB	15 Dec 2023 15:11:08	U	SMPL
O5803-03DUP - 1	600572408-DUP	-41	-0.1264	-	7470A	PPB	15 Dec 2023 15:13:27	U	SMPL
O5803-03MS - 1	600572408-MS	16818	3.7801	-	7470A	PPB	15 Dec 2023 15:15:44	U	SMPL
O5803-03MSD - 1	600572408-MSD	16539	3.7154	-	7470A	PPB	15 Dec 2023 15:18:01	U	SMPL
CCV22 - 1	CCV22	22359	5.0640	-	7470A	PPB	15 Dec 2023 15:20:19	U	SMPL
CCB22 - 1	CCB22	291	-0.0495	-	7470A	PPB	15 Dec 2023 15:28:56	U	SMPL
P[B157761TB - 1	P[B157761TB	347	-0.0365	-	7470A	PPB	15 Dec 2023 15:33:41	U	SMPL
O5803-03LX5 - 1		-26	-0.1230	-	7470A	PPB	15 Dec 2023 15:35:56	U	SMPL
O5803-03A - 1		16206	3.6383	-	7470A	PPB	15 Dec 2023 15:38:11	U	SMPL
CCV23 - 1	CCV23	21624	4.8937	-	7470A	PPB	15 Dec 2023 15:42:12	U	SMPL
CCB23 - 1	CCB23	243	-0.0606	-	7470A	PPB	15 Dec 2023 15:44:27	U	SMPL