


LB128907

7470A

INSTRUMENT ID: CV1

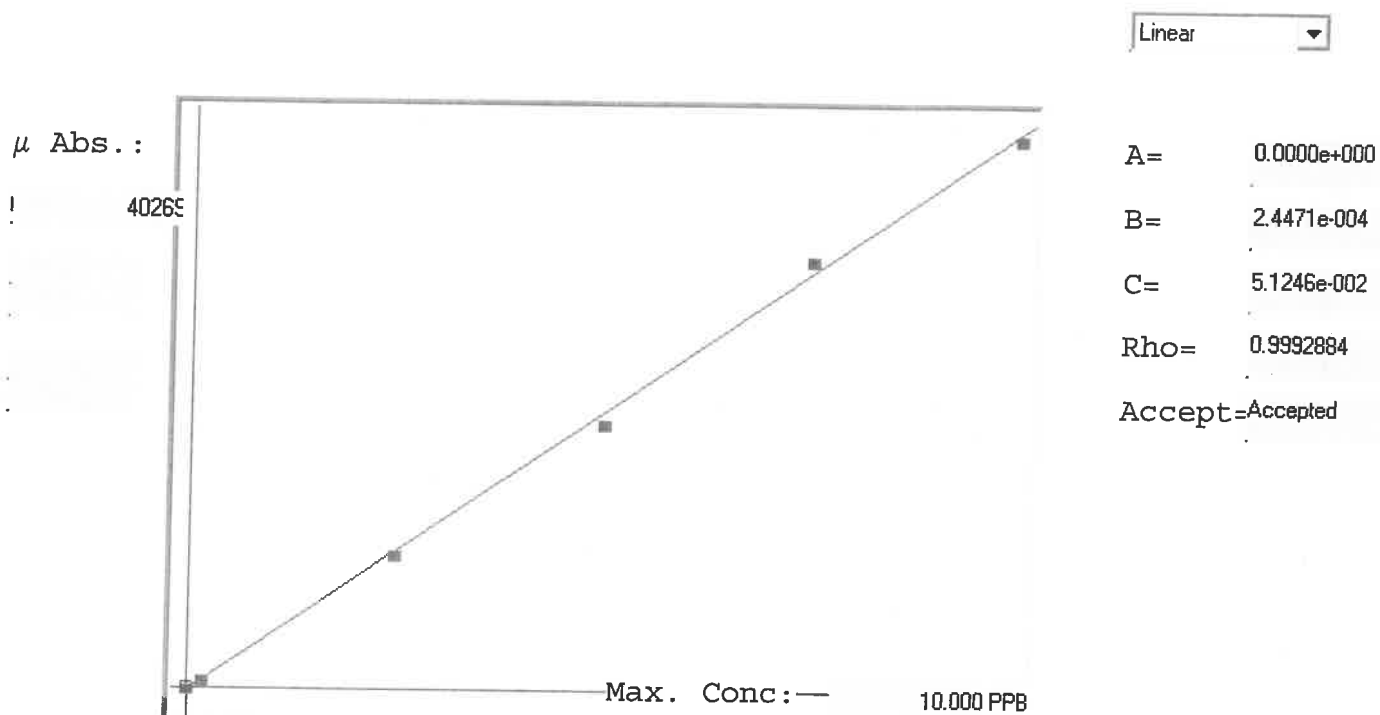

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/vl
0.0	0.000	0.069	0.069	74	0.000	74	0				1
0.2	0.200	0.217	0.017	676	0.0 %	676					8
2.5	2.500	2.440	-0.060	9763	0.0 %	9763					-2
5.0	5.000	4.815	-0.185	19465	0.0 %	19465					-4
7.5	7.500	7.754	0.254	31475	0.0 %	31475					3
10.0	10.000	9.906	-0.094	40269	0.0 %	40269					-1

LB128907 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Dec 2023 18:21:27

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	74	-	0.0000	7470A	PPB	22 Dec 2023 18:23:16	S	Std
0.2 - 1	502	676	-	0.2000	7470A	PPB	22 Dec 2023 18:25:34	S	Std
2.5 - 1	52.5	9763	-	2.5000	7470A	PPB	22 Dec 2023 18:27:51	S	Std
5.0 - 1	55	19465	-	5.0000	7470A	PPB	22 Dec 2023 18:30:08	S	Std
7.5 - 1	59.5	31475	-	7.5000	7470A	PPB	22 Dec 2023 18:32:27	S	Std
10.0 - 1	510	40269	-	10.0000	7470A	PPB	22 Dec 2023 18:40:34	S	Std
ICV39 - 1	ICV39	14730	3.6558	-	7470A	PPB	22 Dec 2023 18:43:22	U	SMPL
ICB39 - 1	ICB39	-264	-0.0134	-	7470A	PPB	22 Dec 2023 18:45:37	U	SMPL
CCV60 - 1	CCV60	19499	4.8229	-	7470A	PPB	22 Dec 2023 18:47:55	U	SMPL
CCB60 - 1	CCB60	-263	-0.0131	-	7470A	PPB	22 Dec 2023 18:50:10	U	SMPL
CRA - 1	CRA	565	0.1895	-	7470A	PPB	22 Dec 2023 18:52:28	U	SMPL
HighStd - 1	HighStd	39532	9.7252	-	7470A	PPB	22 Dec 2023 18:54:43	U	SMPL
ChkStd - 1	ChkStd	28795	7.0977	-	7470A	PPB	22 Dec 2023 18:56:59	U	SMPL
PB158013BL - 1	PBW	-520	-0.0760	-	7470A	PPB	22 Dec 2023 18:59:17	U	SMPL
PB158013BS - 1	LCSW	14581	3.6194	-	7470A	PPB	22 Dec 2023 19:03:52	U	SMPL
O5926-02 - 1	MR-319-0-2	-320	-0.0271	-	7470A	PPB	22 Dec 2023 19:06:11	U	SMPL
O5926-04 - 1	MR-320-0-2	-130	0.0194	-	7470A	PPB	22 Dec 2023 19:08:29	U	SMPL
O5926-06 - 1	MR-319-3.7-4.7	-63	0.0358	-	7470A	PPB	22 Dec 2023 19:10:46	U	SMPL
O5978-03 - 1	N41547	-42	0.0410	-	7470A	PPB	22 Dec 2023 19:13:03	U	SMPL
O5980-02 - 1	MR-315-0-2	-7	0.0495	-	7470A	PPB	22 Dec 2023 19:15:18	U	SMPL
CCV61 - 1	CCV61	18933	4.6844	-	7470A	PPB	22 Dec 2023 19:17:34	U	SMPL
CCB61 - 1	CCB61	-255	-0.0112	-	7470A	PPB	22 Dec 2023 19:19:49	U	SMPL
O5990-02 - 1	ETGI-281	-53	0.0383	-	7470A	PPB	22 Dec 2023 19:22:07	U	SMPL
O5993-01 - 1	E8965C-S-002	48	0.0630	-	7470A	PPB	22 Dec 2023 19:24:22	U	SMPL
O5993-01DUP - 1	E8965C-S-002DUP	84	0.0718	-	7470A	PPB	22 Dec 2023 19:26:39	U	SMPL
O5993-01MS - 1	E8965C-S-002MS	18063	4.4715	-	7470A	PPB	22 Dec 2023 19:28:54	U	SMPL
O5993-01MSD - 1	E8965C-S-002MSD	16816	4.1663	-	7470A	PPB	22 Dec 2023 19:31:10	U	SMPL
PB158023BL - 1	PBW	-296	-0.0212	-	7470A	PPB	22 Dec 2023 19:33:29	U	SMPL
PB158023BS - 1	LCSW	17767	4.3990	-	7470A	PPB	22 Dec 2023 19:35:47	U	SMPL
O5917-01 - 1	GM38-AOP-SLEEVE-SCRAPING	323	0.1303	-	7470A	PPB	22 Dec 2023 19:38:04	U	SMPL
O5917-01DUP - 1	GM38-AOP-SLEEVE-SCRAPINGDUP	476	0.1677	-	7470A	PPB	22 Dec 2023 19:43:10	U	SMPL
O5917-01MS - 1	GM38-AOP-SLEEVE-SCRAPINGMS	13647	3.3908	-	7470A	PPB	22 Dec 2023 19:45:25	U	SMPL
CCV62 - 1	CCV62	19102	4.7257	-	7470A	PPB	22 Dec 2023 19:50:27	U	SMPL
CCB62 - 1	CCB62	-300	-0.0222	-	7470A	PPB	22 Dec 2023 19:52:42	U	SMPL
O5917-01MSD - 1	GM38-AOP-SLEEVE-SCRAPINGMSD	12920	3.2129	-	7470A	PPB	22 Dec 2023 19:55:01	U	SMPL
O5917-02 - 1	GM38-AOP-EFFLUENT	144	0.0865	-	7470A	PPB	22 Dec 2023 19:57:18	U	SMPL
PB157982TB - 1	PB157982TB	-70	0.0341	-	7470A	PPB	22 Dec 2023 19:59:36	U	SMPL
O5993-01LX5 - 1		-87	0.0300	-	7470A	PPB	22 Dec 2023 20:01:52	U	SMPL
O5993-01A - 1		13273	3.2993	-	7470A	PPB	22 Dec 2023 20:04:07	U	SMPL
O5917-01LX5 - 1		-145	0.0158	-	7470A	PPB	22 Dec 2023 20:06:24	U	SMPL
O5917-01A - 1		11786	2.9354	-	7470A	PPB	22 Dec 2023 20:08:42	U	SMPL
CCV63 - 1	CCV63	19006	4.7022	-	7470A	PPB	22 Dec 2023 20:10:59	U	SMPL
CCB63 - 1	CCB63	-304	-0.0231	-	7470A	PPB	22 Dec 2023 20:13:18	U	SMPL