


LB128946

7470A

INSTRUMENT ID: CV1

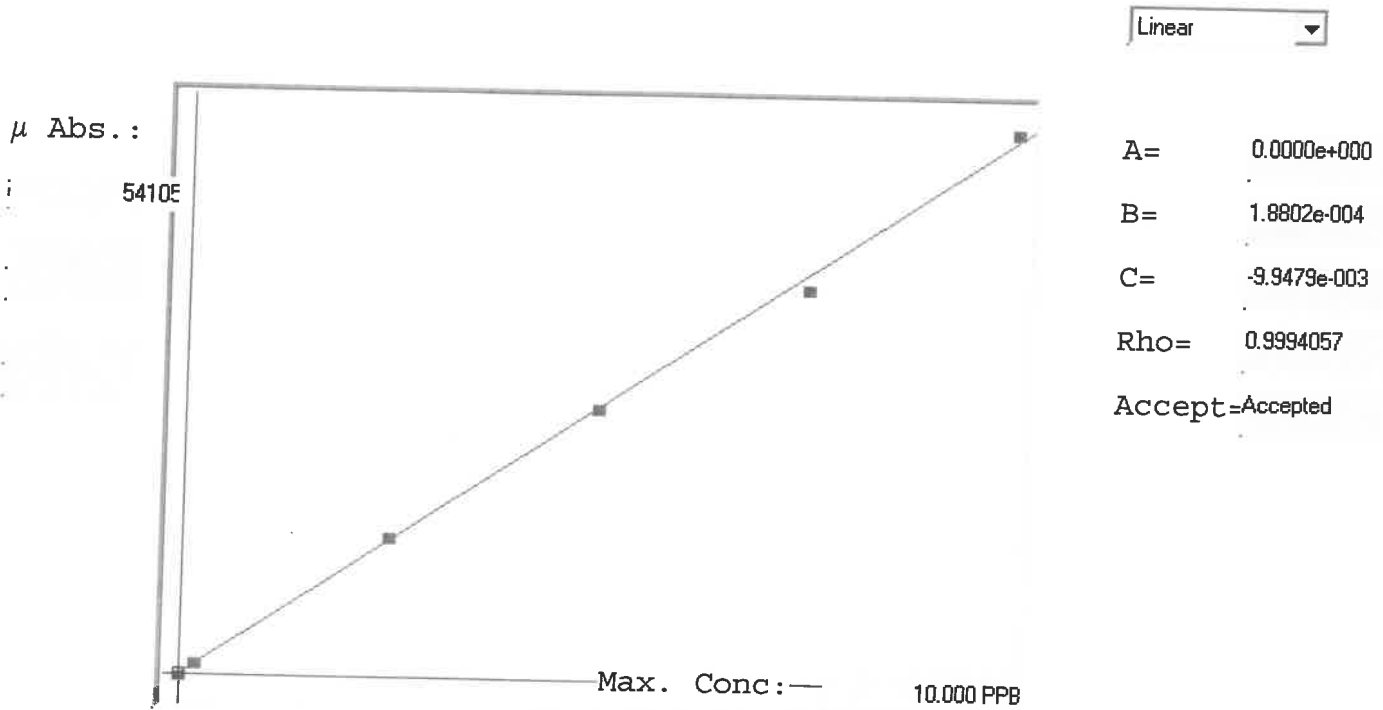

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.011	0.011	112	0.000	112	0				
0.2	0.200	0.210	0.010	1168	0.0 %	1168					
2.5	2.500	2.568	0.068	13711	0.0 %	13711					
5.0	5.000	5.004	0.004	26668	0.0 %	26668					
7.5	7.500	7.244	-0.256	38579	0.0 %	38579					
10.0	10.000	10.163	0.163	54105	0.0 %	54105					

15032

LB128946 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Dec 2023 12:14:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD	112	-	0.0000	7470A	PPB	27 Dec 2023 13:05:52	S	Std
0.2 - 1	SD	1168	-	0.2000	7470A	PPB	27 Dec 2023 13:08:13	S	Std
2.5 - 1	SD	13711	-	2.5000	7470A	PPB	27 Dec 2023 13:10:31	S	Std
5.0 - 1	SD	26668	-	5.0000	7470A	PPB	27 Dec 2023 13:12:48	S	Std
7.5 - 1	SD	38579	-	7.5000	7470A	PPB	27 Dec 2023 13:15:06	S	Std
10.0 - 1	SD	54105	-	10.0000	7470A	PPB	27 Dec 2023 13:22:45	S	Std
ICV41 - 1	ICV41	20363	3.8188	-	7470A	PPB	27 Dec 2023 13:28:08	U	SMPL
ICB41 - 1	ICB41	-243	-0.0556	-	7470A	PPB	27 Dec 2023 13:30:23	U	SMPL
CCV70 - 1	CCV70	24715	4.6371	-	7470A	PPB	27 Dec 2023 13:32:40	U	SMPL
CCB70 - 1	CCB70	-245	-0.0560	-	7470A	PPB	27 Dec 2023 13:34:57	U	SMPL
CRA - 1	CRA	1012	0.1803	-	7470A	PPB	27 Dec 2023 13:37:15	U	SMPL
HighStd - 1	HighStd	54104	10.1629	-	7470A	PPB	27 Dec 2023 13:39:33	U	SMPL
ChkStd - 1	ChkStd	33695	6.3255	-	7470A	PPB	27 Dec 2023 13:41:49	U	SMPL
PB158085BL - 1	PBW	-12	-0.0122	-	7470A	PPB	27 Dec 2023 13:47:02	U	SMPL
PB158085BS - 1	LCSW	18709	3.5078	-	7470A	PPB	27 Dec 2023 13:51:59	U	SMPL
O6014-04 - 1	AUD-1306	-297	-0.0658	-	7470A	PPB	27 Dec 2023 13:54:15	U	SMPL
O6014-04DUP - 1	AUD-1306DUP	-54	-0.0201	-	7470A	PPB	27 Dec 2023 13:56:33	U	SMPL
O6014-04MS - 1	AUD-1306MS	18722	3.5102	-	7470A	PPB	27 Dec 2023 13:58:50	U	SMPL
O6014-04MSD - 1	AUD-1306MSD	17833	3.3431	-	7470A	PPB	27 Dec 2023 14:01:07	U	SMPL
O6014-06 - 1	AUD-1307	-277	-0.0620	-	7470A	PPB	27 Dec 2023 14:03:25	U	SMPL
CCV71 - 1	CCV71	24468	4.5906	-	7470A	PPB	27 Dec 2023 14:05:48	U	SMPL
CCB71 - 1	CCB71	-242	-0.0554	-	7470A	PPB	27 Dec 2023 14:08:04	U	SMPL
PB158086BL - 1	PBW	145	0.0173	-	7470A	PPB	27 Dec 2023 14:10:21	U	SMPL
O5994-02 - 1	WC-A-COMP	-234	-0.0539	-	7470A	PPB	27 Dec 2023 14:14:53	U	SMPL
O5994-05 - 1	WC-B-COMP	-148	-0.0378	-	7470A	PPB	27 Dec 2023 14:17:11	U	SMPL
O5994-08 - 1	WC-C-COMP	847	0.1493	-	7470A	PPB	27 Dec 2023 14:19:27	U	SMPL
O5994-11 - 1	WC-D-COMP	-122	-0.0329	-	7470A	PPB	27 Dec 2023 14:21:44	U	SMPL
O6012-02 - 1	ASH-SAMPLE	-28	-0.0152	-	7470A	PPB	27 Dec 2023 14:24:00	U	SMPL
O6015-02 - 1	MR-317-0-2	42	-0.0021	-	7470A	PPB	27 Dec 2023 14:26:17	U	SMPL
O6015-04 - 1	MR-317-0-2D	26	-0.0051	-	7470A	PPB	27 Dec 2023 14:28:35	U	SMPL
O6015-06 - 1	MR-323-0-2	32	-0.0039	-	7470A	PPB	27 Dec 2023 14:30:50	U	SMPL
CCV72 - 1	CCV72	25038	4.6978	-	7470A	PPB	27 Dec 2023 14:33:06	U	SMPL
CCB72 - 1	CCB72	-224	-0.0521	-	7470A	PPB	27 Dec 2023 14:35:22	U	SMPL
O6015-08 - 1	MR-323-6-8	-23	-0.0143	-	7470A	PPB	27 Dec 2023 14:37:40	U	SMPL
O6016-02 - 1	MR-322-0-2	-9	-0.0116	-	7470A	PPB	27 Dec 2023 14:39:55	U	SMPL
O6016-04 - 1	MR-322-4-6	56	0.0006	-	7470A	PPB	27 Dec 2023 14:42:11	U	SMPL
O6016-04DUP - 1	MR-322-4-6DUP	9	-0.0083	-	7470A	PPB	27 Dec 2023 14:44:27	U	SMPL
O6016-04MS - 1	MR-322-4-6MS	18831	3.5307	-	7470A	PPB	27 Dec 2023 14:46:43	U	SMPL
O6016-04MSD - 1	MR-322-4-6MSD	17470	3.2748	-	7470A	PPB	27 Dec 2023 14:48:59	U	SMPL
PB158046TB - 1		-294	-0.0652	-	7470A	PPB	27 Dec 2023 14:51:18	U	SMPL
PB158048TB - 1		-15	-0.0128	-	7470A	PPB	27 Dec 2023 14:53:37	U	SMPL
PB158086BS - 1	LCSW	19975	3.7458	-	7470A	PPB	27 Dec 2023 14:55:54	U	SMPL
CCV73 - 1	CCV73	25748	4.8313	-	7470A	PPB	27 Dec 2023 14:58:10	U	SMPL
CCB73 - 1	CCB73	-289	-0.0643	-	7470A	PPB	27 Dec 2023 15:00:27	U	SMPL
O6014-04LX5 - 1		54	0.0002	-	7470A	PPB	27 Dec 2023 15:02:46	U	SMPL
O6014-04A - 1		20944	3.9280	-	7470A	PPB	27 Dec 2023 15:05:01	U	SMPL
O6016-04LX5 - 1		-257	-0.0583	-	7470A	PPB	27 Dec 2023 15:07:17	U	SMPL
O6016-04A - 1		20690	3.8803	-	7470A	PPB	27 Dec 2023 15:09:35	U	SMPL
CCV74 - 1	CCV74	24879	4.6679	-	7470A	PPB	27 Dec 2023 15:11:50	U	SMPL
CCB74 - 1	CCB74	-296	-0.0656	-	7470A	PPB	27 Dec 2023 15:14:09	U	SMPL