


L3128957

7471B

INSTRUMENT ID: CV1

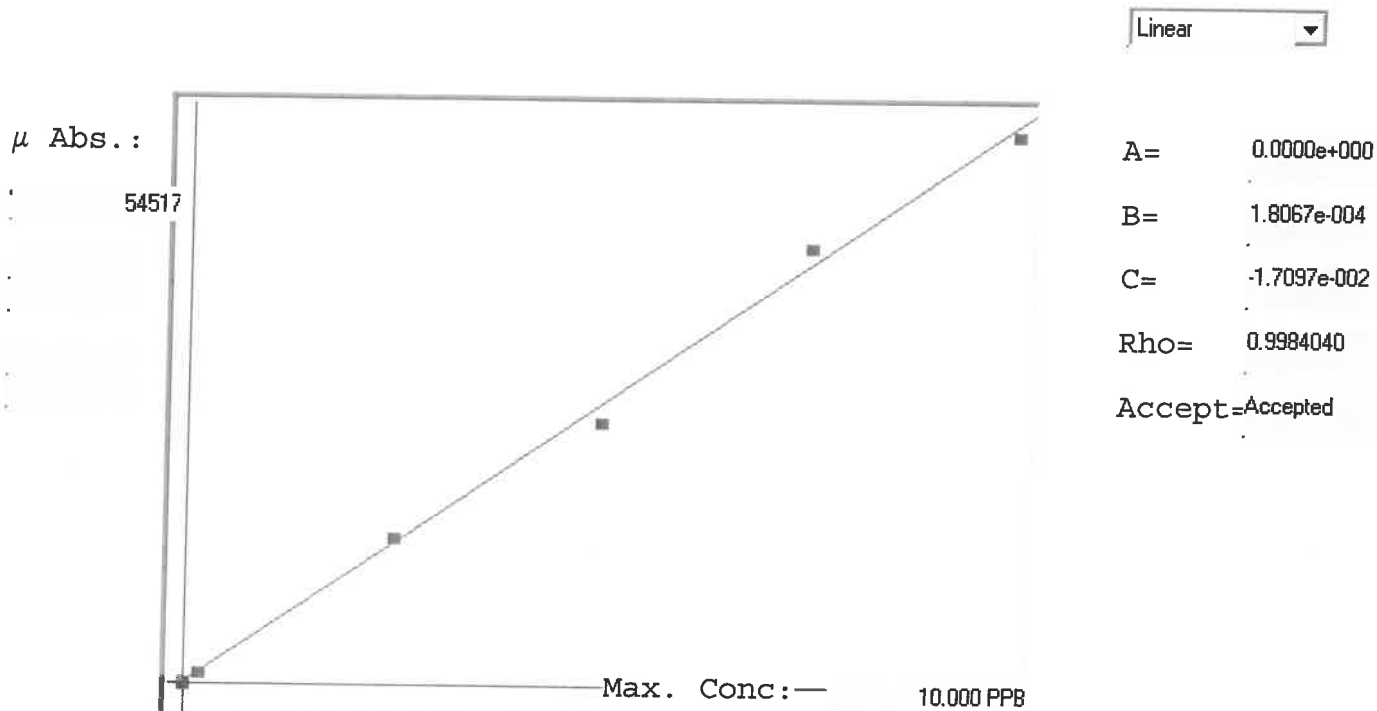

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	D/O
0.0	0.000	-0.004	-0.004	71	0.000	71					1
0.2	0.200	0.203	0.003	1216	0.0 %	1216					2
2.5	2.500	2.624	0.124	14619	0.0 %	14619					5
5.0	5.000	4.694	-0.306	26074	0.0 %	26074					6
7.5	7.500	7.851	0.351	43550	0.0 %	43550					5
10.0	10.000	9.833	-0.167	54517	0.0 %	54517					2

LB128957 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 27 Dec 2023 17:50:15

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S6	71	-	0.0000	7471B	PPB	27 Dec 2023 17:53:14	S	Std
0.2 - 1	S1.2	1216	-	0.2000	7471B	PPB	27 Dec 2023 17:55:31	S	Std
2.5 - 1	S2.5	14619	-	2.5000	7471B	PPB	27 Dec 2023 17:57:48	S	Std
5.0 - 1	S5	26074	-	5.0000	7471B	PPB	27 Dec 2023 18:00:06	S	Std
7.5 - 1	S7.5	43550	-	7.5000	7471B	PPB	27 Dec 2023 18:05:31	S	Std
10.0 - 1	S10	54517	-	10.0000	7471B	PPB	27 Dec 2023 18:10:37	S	Std
ICV42 - 1	ICV42	20026	3.6010	-	7471B	PPB	27 Dec 2023 18:13:31	U	SMPL
ICB42 - 1	ICB42	-333	-0.0773	-	7471B	PPB	27 Dec 2023 18:15:48	U	SMPL
CCV75 - 1	CCV75	27369	4.9277	-	7471B	PPB	27 Dec 2023 18:18:13	U	SMPL
CCB75 - 1	CCB75	-305	-0.0722	-	7471B	PPB	27 Dec 2023 18:20:27	U	SMPL
CRA - 1	CRA	1190	0.1979	-	7471B	PPB	27 Dec 2023 18:22:56	U	SMPL
HighStd - 1	HighStd	55568	10.0225	-	7471B	PPB	27 Dec 2023 18:25:11	U	SMPL
ChkStd - 1	ChkStd	38641	6.9643	-	7471B	PPB	27 Dec 2023 18:27:27	U	SMPL
PB158120BL - 1	PBS	-348	-0.0800	-	7471B	PPB	27 Dec 2023 18:30:01	U	SMPL
PB158120BS - 1	LCSS	25292	4.5525	-	7471B	PPB	27 Dec 2023 18:32:28	U	SMPL
O5977-07 - 1	34725	3410	0.5990	-	7471B	PPB	27 Dec 2023 18:34:44	U	SMPL
O5990-01 - 1	ETGI-281	143	0.0087	-	7471B	PPB	27 Dec 2023 18:37:08	U	SMPL
O6018-01 - 1	COMP-1	3171	0.5558	-	7471B	PPB	27 Dec 2023 18:39:27	U	SMPL
O6018-01DUP - 1	COMP-1DUP	2756	0.4808	-	7471B	PPB	27 Dec 2023 18:41:45	U	SMPL
O6018-01MS - 1	COMP-1MS	25029	4.5049	-	7471B	PPB	27 Dec 2023 18:44:02	U	SMPL
CCV76 - 1	CCV76	25200	4.5358	-	7471B	PPB	27 Dec 2023 18:46:18	U	SMPL
CCB76 - 1	CCB76	-182	-0.0500	-	7471B	PPB	27 Dec 2023 18:48:43	U	SMPL
O6018-01MSD - 1	COMP-1MSD	25413	4.5743	-	7471B	PPB	27 Dec 2023 18:51:09	U	SMPL
O6018-02 - 1	COMP-2	2617	0.4557	-	7471B	PPB	27 Dec 2023 18:53:24	U	SMPL
O6018-03 - 1	COMP-3	2120	0.3659	-	7471B	PPB	27 Dec 2023 18:55:49	U	SMPL
O6018-01LX5 - 1		541	0.0806	-	7471B	PPB	27 Dec 2023 18:58:06	U	SMPL
O6018-01A - 1		21100	3.7951	-	7471B	PPB	27 Dec 2023 19:00:23	U	SMPL
CCV77 - 1	CCV77	25946	4.6706	-	7471B	PPB	27 Dec 2023 19:02:40	U	SMPL
CCB77 - 1	CCB77	-233	-0.0592	-	7471B	PPB	27 Dec 2023 19:05:06	U	SMPL