


LB128975

7471B

INSTRUMENT ID: CV2

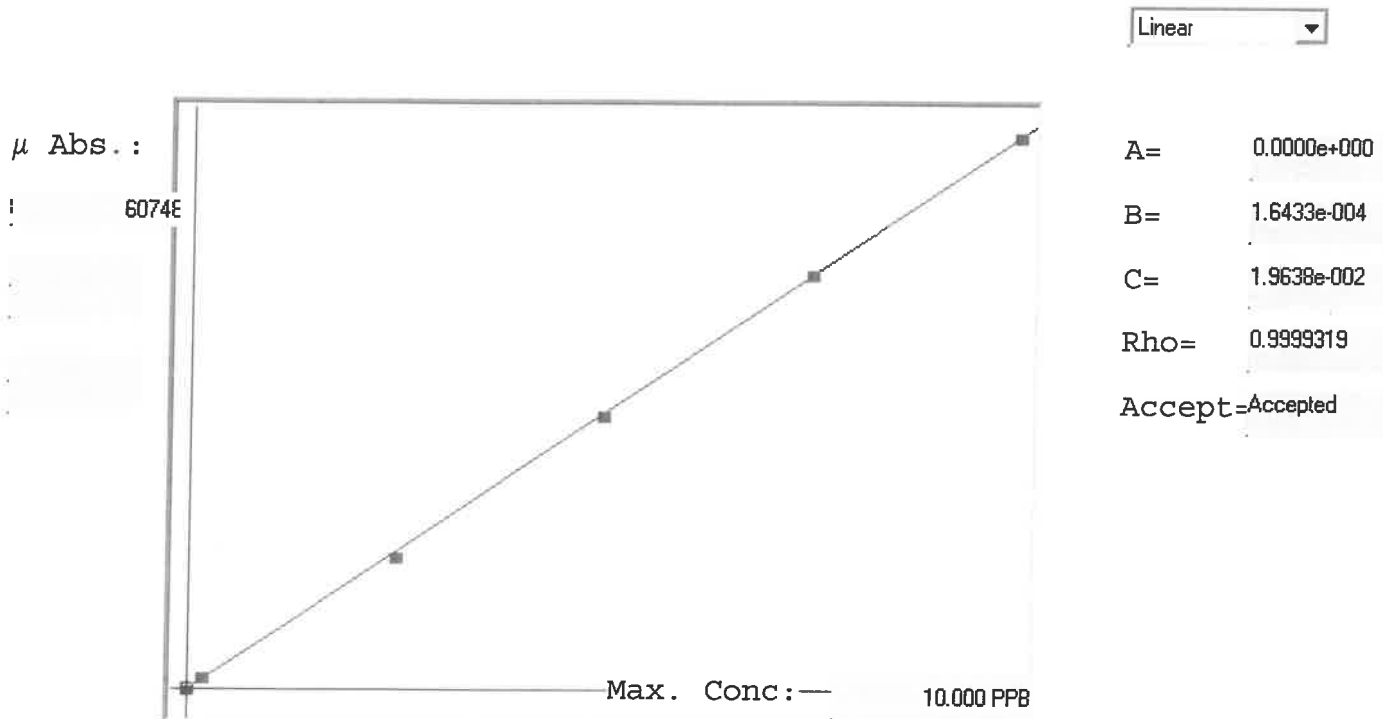

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.030	0.030	62	0.000	62					
0.2	0.200	0.237	0.037	1320	0.0 %	1320					
2.5	2.500	2.414	-0.086	14569	0.0 %	14569					
5.0	5.000	4.983	-0.017	30204	0.0 %	30204					
7.5	7.500	7.534	0.034	45728	0.0 %	45728					
10.0	10.000	10.002	0.002	60748	0.0 %	60748					

0/611
19
3
000
0

LB128975 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 29 Dec 2023 09:51:22

Sample ID	Extended ID	µ Abs	Conc.	Std Conc Method	Units	Date	Type	Type
0.0 - 1	50	62	-	0.00007471B	PPB	29 Dec 2023 10:24:09	S	Std
0.2 - 1	50.2	1320	-	0.20007471B	PPB	29 Dec 2023 10:26:28	S	Std
2.5 - 1	52.5	14569	-	2.50007471B	PPB	29 Dec 2023 10:28:47	S	Std
5.0 - 1	55	30204	-	5.00007471B	PPB	29 Dec 2023 10:31:04	S	Std
7.5 - 1	57.5	45728	-	7.50007471B	PPB	29 Dec 2023 10:33:25	S	Std
10.0 - 1	510	60748	-	10.00007471B	PPB	29 Dec 2023 10:35:50	S	Std
ICV45 - 1	ICV45	24040	3.9702	-7471B	PPB	29 Dec 2023 10:40:25	U	SMPL
ICB45 - 1	ICB45	-319	-0.0328	-7471B	PPB	29 Dec 2023 10:42:40	U	SMPL
CCV87 - 1	CCV87	30074	4.9618	-7471B	PPB	29 Dec 2023 10:45:02	U	SMPL
CCB87 - 1	CCB87	-309	-0.0311	-7471B	PPB	29 Dec 2023 10:47:17	U	SMPL
CRA - 1	CRA	1177	0.2131	-7471B	PPB	29 Dec 2023 10:49:44	U	SMPL
HighStd - 1	HighStd	61039	10.0503	-7471B	PPB	29 Dec 2023 10:52:00	U	SMPL
ChkStd - 1	ChkStd	43107	7.1035	-7471B	PPB	29 Dec 2023 10:57:47	U	SMPL
PB158158BL - 1	PB158158BL	-412	-0.0481	-7471B	PPB	29 Dec 2023 11:00:03	U	SMPL
PB158158BS - 1	PB158158BS	24036	3.9695	-7471B	PPB	29 Dec 2023 11:02:30	U	SMPL
O4699-01 - 1	LOD-MDL-SOIL-01-QT4-2023	204	0.0532	-7471B	PPB	29 Dec 2023 11:04:47	U	SMPL
O4699-03 - 1	MDL-SOIL-03-QT4-2023	247	0.0602	-7471B	PPB	29 Dec 2023 11:11:47	U	SMPL
O5994-01 - 1	WC-A-COMP	4162	0.7036	-7471B	PPB	29 Dec 2023 11:14:04	U	SMPL
O5994-04 - 1	WC-B-COMP	6967	1.1645	-7471B	PPB	29 Dec 2023 11:16:21	U	SMPL
O5994-07 - 1	WC-C-COMP	132645	21.8175	-7471B	PPB	29 Dec 2023 11:18:39	U	SMPL
CCV88 - 1	CCV88	29520	4.8707	-7471B	PPB	29 Dec 2023 11:20:57	U	SMPL
CCB88 - 1	CCB88	-236	-0.0191	-7471B	PPB	29 Dec 2023 11:23:34	U	SMPL
O5994-10 - 1	WC-D-COMP	2963	0.5066	-7471B	PPB	29 Dec 2023 11:26:01	U	SMPL
O6011-01 - 1	SU-03-122223	6377	1.0676	-7471B	PPB	29 Dec 2023 11:28:16	U	SMPL
O6016-01 - 1	MR-322-0-2	546	0.1094	-7471B	PPB	29 Dec 2023 11:30:33	U	SMPL
O6016-03 - 1	MR-322-4-6	399	0.0852	-7471B	PPB	29 Dec 2023 11:32:51	U	SMPL
O6027-01 - 1	CONTAINMENT	229	0.0573	-7471B	PPB	29 Dec 2023 11:35:08	U	SMPL
O6027-03 - 1	PIERS	160	0.0458	-7471B	PPB	29 Dec 2023 11:37:24	U	SMPL
O6027-05 - 1	CURB	251	0.0608	-7471B	PPB	29 Dec 2023 11:39:41	U	SMPL
O6027-07 - 1	STONES	692	0.1334	-7471B	PPB	29 Dec 2023 11:41:59	U	SMPL
O6031-01 - 1	MR-321-0-2	13295	2.2044	-7471B	PPB	29 Dec 2023 11:44:15	U	SMPL
O6031-03 - 1	MR-321-10-12	2653	0.4556	-7471B	PPB	29 Dec 2023 11:46:31	U	SMPL
CCV89 - 1	CCV89	30611	5.0500	-7471B	PPB	29 Dec 2023 11:48:49	U	SMPL
CCB89 - 1	CCB89	-157	-0.0062	-7471B	PPB	29 Dec 2023 11:51:06	U	SMPL
O6033-01 - 1	OR-05-122723	2583	0.4441	-7471B	PPB	29 Dec 2023 11:53:31	U	SMPL
O6034-01 - 1	EO-03-122723	1639	0.2890	-7471B	PPB	29 Dec 2023 11:55:47	U	SMPL
O6035-01 - 1	TR-5-122723	3907	0.6617	-7471B	PPB	29 Dec 2023 12:03:19	U	SMPL
O6035-01DUP - 1	TR-5-122723DUP	3706	0.6287	-7471B	PPB	29 Dec 2023 12:07:56	U	SMPL
O6035-01MS - 1	TR-5-122723MS	28133	4.6428	-7471B	PPB	29 Dec 2023 12:13:16	U	SMPL
O6035-01MSD - 1	TR-5-122723MSD	25712	4.2449	-7471B	PPB	29 Dec 2023 12:15:33	U	SMPL
O4699-01RE - 1	LOD-MDL-SOIL-01-QT4-2023RE	967	0.1785	-7471B	PPB	29 Dec 2023 12:17:58	U	SMPL
O6035-01LX5 - 1		857	0.1605	-7471B	PPB	29 Dec 2023 12:20:18	U	SMPL
O6035-01A - 1		28905	4.7697	-7471B	PPB	29 Dec 2023 12:22:35	U	SMPL
O5994-07DLX5 - 1		29755	4.9093	-7471B	PPB	29 Dec 2023 12:24:51	U	SMPL
CCV90 - 1	CCV90	30627	5.0526	-7471B	PPB	29 Dec 2023 12:27:15	U	SMPL
CCB90 - 1	CCB90	-124	-0.0007	-7471B	PPB	29 Dec 2023 12:29:38	U	SMPL