

LB129113


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

47925

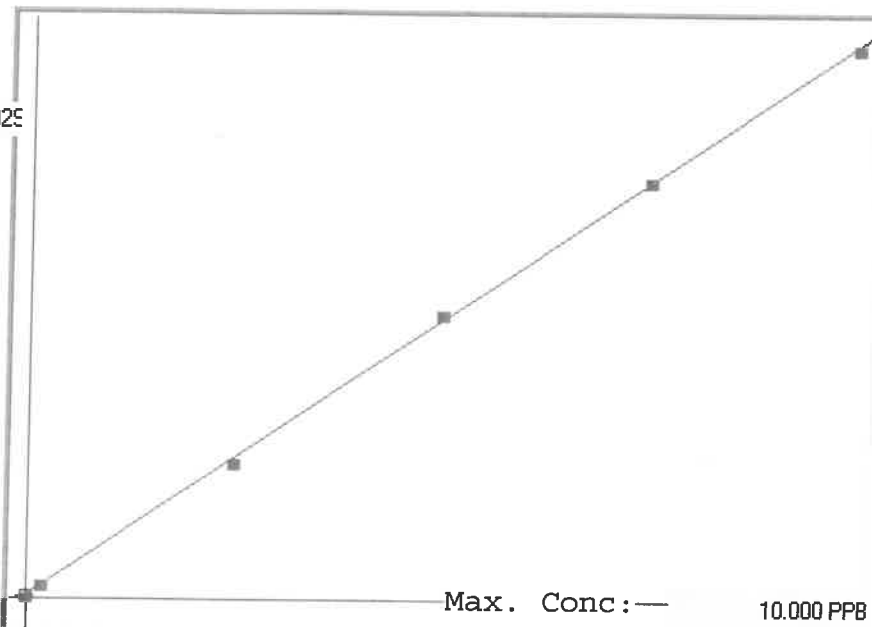

A= 0.0000e+000

B= 2.0839e-004

C= -5.1936e-002

Rho= 0.9998359

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%RSD
0.0	0.000	-0.005	-0.005	223	0.000	223	0				
0.2	0.200	0.206	0.006	1240	0.0 %	1240					
2.5	2.500	2.413	-0.087	11828	0.0 %	11828					
5.0	5.000	5.118	0.118	24811	0.0 %	24811					
7.5	7.500	7.532	0.032	36393	0.0 %	36393					
10.0	10.000	9.936	-0.064	47929	0.0 %	47929					

102621

LB129113 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Jan 2024 10:43:47

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	223	-	0.0000	7470A	PPB	11 Jan 2024 11:00:24	S	Std
0.2 - 1	50.2	1240	-	0.2000	7470A	PPB	11 Jan 2024 11:02:41	S	Std
2.5 - 1	52.5	11828	-	2.5000	7470A	PPB	11 Jan 2024 11:04:59	S	Std
5.0 - 1	55	24811	-	5.0000	7470A	PPB	11 Jan 2024 11:07:16	S	Std
7.5 - 1	57.5	36393	-	7.5000	7470A	PPB	11 Jan 2024 11:09:34	S	Std
10.0 - 1	510	47929	-	10.0000	7470A	PPB	11 Jan 2024 11:11:52	S	Std
ICV62 - 1	ICV62	18210	3.7428	-	7470A	PPB	11 Jan 2024 11:21:51	U	SMPL
ICB62 - 1	ICB62	494	0.0510	-	7470A	PPB	11 Jan 2024 11:24:06	U	SMPL
CCV57 - 1	CCV57	24852	5.1269	-	7470A	PPB	11 Jan 2024 11:26:23	U	SMPL
CCB57 - 1	CCB57	422	0.0360	-	7470A	PPB	11 Jan 2024 11:28:38	U	SMPL
CRA - 1	CRA	1206	0.1994	-	7470A	PPB	11 Jan 2024 11:30:56	U	SMPL
HighStd - 1	HighStd	48366	10.0269	-	7470A	PPB	11 Jan 2024 11:33:11	U	SMPL
ChkStd - 1	ChkStd	34224	7.0799	-	7470A	PPB	11 Jan 2024 11:35:26	U	SMPL
PB158350BS - 1	LCSW	20095	4.1356	-	7470A	PPB	11 Jan 2024 11:40:05	U	SMPL
P1056-02 - 1	MR-311P-0-2	-111	-0.0751	-	7470A	PPB	11 Jan 2024 11:42:21	U	SMPL
P1056-04 - 1	MR-311P-30-32	77	-0.0359	-	7470A	PPB	11 Jan 2024 11:44:40	U	SMPL
P1067-02 - 1	SP-A-COMP(0-8)	92	-0.0328	-	7470A	PPB	11 Jan 2024 11:46:57	U	SMPL
P1067-05 - 1	SP-B-COMP(0-8)	152	-0.0203	-	7470A	PPB	11 Jan 2024 11:49:14	U	SMPL
P1067-08 - 1	SP-C-COMP(0-8)	180	-0.0144	-	7470A	PPB	11 Jan 2024 11:51:30	U	SMPL
PB158350BL - 1	PBW	570	0.0668	-	7470A	PPB	11 Jan 2024 11:54:01	U	SMPL
CCV58 - 1	CCV58	24782	5.1123	-	7470A	PPB	11 Jan 2024 11:56:35	U	SMPL
CCB58 - 1	CCB58	414	0.0343	-	7470A	PPB	11 Jan 2024 11:58:49	U	SMPL
P1087-01 - 1	COMP-1	112	-0.0286	-	7470A	PPB	11 Jan 2024 12:01:07	U	SMPL
P1087-02 - 1	COMP-2	163	-0.0180	-	7470A	PPB	11 Jan 2024 12:03:22	U	SMPL
P1087-03 - 1	COMP-3	199	-0.0105	-	7470A	PPB	11 Jan 2024 12:05:38	U	SMPL
P1087-03DUP - 1	COMP-3DUP	184	-0.0136	-	7470A	PPB	11 Jan 2024 12:07:54	U	SMPL
P1087-03MS - 1	COMP-3MS	20219	4.1614	-	7470A	PPB	11 Jan 2024 12:10:11	U	SMPL
P1087-03MSD - 1	COMP-3MSD	19480	4.0075	-	7470A	PPB	11 Jan 2024 12:12:28	U	SMPL
PB158376BL - 1	PBW	-61	-0.0646	-	7470A	PPB	11 Jan 2024 12:14:47	U	SMPL
PB158376BS - 1	LCSW	17147	3.5213	-	7470A	PPB	11 Jan 2024 12:17:07	U	SMPL
P1083-01 - 1	GROUND-WATER-TOTE	30	-0.0457	-	7470A	PPB	11 Jan 2024 12:19:24	U	SMPL
P1083-03 - 1	OILY-WATER-TOTE	2557	0.4809	-	7470A	PPB	11 Jan 2024 12:21:42	U	SMPL
CCV59 - 1	CCV59	23578	4.8614	-	7470A	PPB	11 Jan 2024 12:23:58	U	SMPL
CCB59 - 1	CCB59	396	0.0306	-	7470A	PPB	11 Jan 2024 12:26:15	U	SMPL
P1084-01 - 1	OWS-PROJECT-COMP	4889	0.9669	-	7470A	PPB	11 Jan 2024 12:28:34	U	SMPL
P1084-01DUP - 1	OWS-PROJECT-COMPDUP	5315	1.0556	-	7470A	PPB	11 Jan 2024 12:30:49	U	SMPL
P1084-01MS - 1	OWS-PROJECT-COMPMS	19742	4.0620	-	7470A	PPB	11 Jan 2024 12:33:06	U	SMPL
P1084-01MSD - 1	OWS-PROJECT-COMPMSD	18060	3.7115	-	7470A	PPB	11 Jan 2024 12:35:24	U	SMPL
P1098-01 - 1	AUD-1310	-43	-0.0609	-	7470A	PPB	11 Jan 2024 12:37:43	U	SMPL
PB158317TB - 1		184	-0.0136	-	7470A	PPB	11 Jan 2024 12:40:02	U	SMPL
P1087-03LX5 - 1		94	-0.0323	-	7470A	PPB	11 Jan 2024 12:42:19	U	SMPL
P1087-03A - 1		19111	3.9306	-	7470A	PPB	11 Jan 2024 12:44:36	U	SMPL
P1084-01LX5 - 1		1072	0.1715	-	7470A	PPB	11 Jan 2024 12:50:39	U	SMPL
P1084-01A - 1		24312	5.0144	-	7470A	PPB	11 Jan 2024 12:52:54	U	SMPL
CCV60 - 1	CCV60	24035	4.9567	-	7470A	PPB	11 Jan 2024 12:55:10	U	SMPL
CCB60 - 1	CCB60	433	0.0383	-	7470A	PPB	11 Jan 2024 12:57:29	U	SMPL