


LB129158

7471B

INSTRUMENT ID: CV1

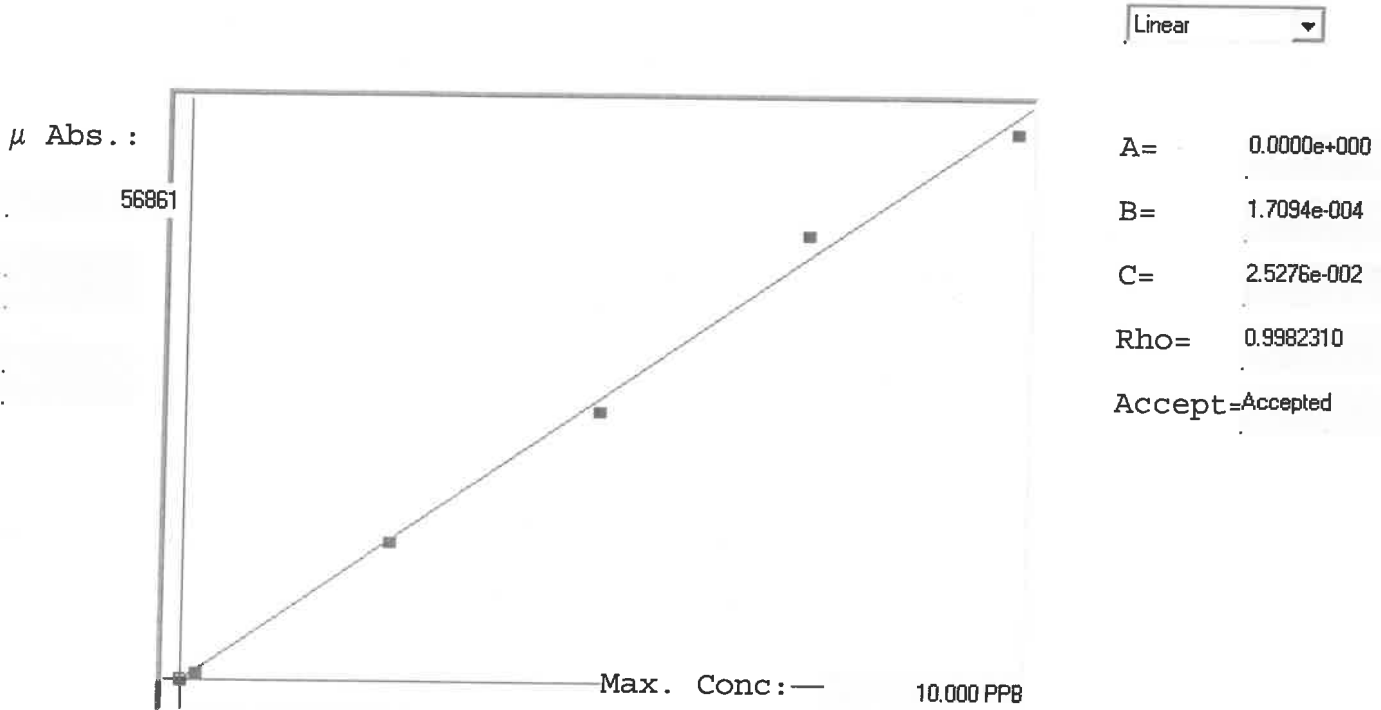

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/6/11
0.0	0.000	0.034	0.034	50	0.000	50					1
0.2	0.200	0.192	-0.008	973	0.0 %	973					-4
2.5	2.500	2.486	-0.014	14396	0.0 %	14396					-1
5.0	5.000	4.811	-0.189	27999	0.0 %	27999					-4
7.5	7.500	7.932	0.432	46256	0.0 %	46256					-6
10.0	10.000	9.745	-0.255	56861	0.0 %	56861					-3

LB129158 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Jan 2024 11:47:58

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	50	-	0.0000	7471B	PPB	16 Jan 2024 12:16:54	S	Std
0.2 - 1	50.2	973	-	0.2000	7471B	PPB	16 Jan 2024 12:19:12	S	Std
2.5 - 1	52.5	14396	-	2.5000	7471B	PPB	16 Jan 2024 12:24:04	S	Std
5.0 - 1	55.0	27999	-	5.0000	7471B	PPB	16 Jan 2024 12:26:23	S	Std
7.5 - 1	57.5	46256	-	7.5000	7471B	PPB	16 Jan 2024 12:28:44	S	Std
10.0 - 1	510	56861	-	10.0000	7471B	PPB	16 Jan 2024 12:37:20	S	Std
ICV67 - 1	ICV67	22262	3.8307	-	7471B	PPB	16 Jan 2024 12:42:50	U	SMPL
ICB67 - 1	ICB67	-247	-0.0169	-	7471B	PPB	16 Jan 2024 12:45:07	U	SMPL
CCV75 - 1	CCV75	31212	5.3606	-	7471B	PPB	16 Jan 2024 13:04:52	U	SMPL
CCB75 - 1	CCB75	-251	-0.0176	-	7471B	PPB	16 Jan 2024 13:07:10	U	SMPL
CRA - 1	CRA	965	0.1902	-	7471B	PPB	16 Jan 2024 13:09:37	U	SMPL
HighStd - 1	HighStd	57208	9.8043	-	7471B	PPB	16 Jan 2024 13:14:28	U	SMPL
ChkStd - 1	ChkStd	39728	6.8163	-	7471B	PPB	16 Jan 2024 13:16:47	U	SMPL
PB158461BL - 1	PBS	-327	-0.0306	-	7471B	PPB	16 Jan 2024 13:19:18	U	SMPL
PB158461BS - 1	LCSS	22461	3.8647	-	7471B	PPB	16 Jan 2024 13:24:19	U	SMPL
P1132-01 - 1	RBR200010	3028	0.5429	-	7471B	PPB	16 Jan 2024 13:31:24	U	SMPL
P1132-01DUP - 1	RBR200010DUP	2784	0.5012	-	7471B	PPB	16 Jan 2024 13:33:42	U	SMPL
P1132-01MS - 1	RBR200010MS	27497	4.7255	-	7471B	PPB	16 Jan 2024 13:38:44	U	SMPL
P1132-01MSD - 1	RBR200010MSD	26048	4.4779	-	7471B	PPB	16 Jan 2024 13:41:02	U	SMPL
P1132-03 - 1	RBR200027	4187	0.7410	-	7471B	PPB	16 Jan 2024 13:43:26	U	SMPL
CCV76 - 1	CCV76	29139	5.0062	-	7471B	PPB	16 Jan 2024 13:48:01	U	SMPL
CCB76 - 1	CCB76	-365	-0.0371	-	7471B	PPB	16 Jan 2024 13:50:22	U	SMPL
P1134-01 - 1	NWB-1137-1138-1139	3117	0.5581	-	7471B	PPB	16 Jan 2024 13:52:48	U	SMPL
P1135-01 - 1	360	2599	0.4695	-	7471B	PPB	16 Jan 2024 13:55:04	U	SMPL
P1136-01 - 1	MH-F	1337	0.2538	-	7471B	PPB	16 Jan 2024 13:57:22	U	SMPL
P1136-03 - 1	MH-C	2637	0.4760	-	7471B	PPB	16 Jan 2024 13:59:39	U	SMPL
P1139-01 - 1	MR-314-0-2	16254	2.8037	-	7471B	PPB	16 Jan 2024 14:01:54	U	SMPL
P1139-03 - 1	MR-314-16-18	5979	1.0473	-	7471B	PPB	16 Jan 2024 14:04:12	U	SMPL
P1140-01 - 1	MR-309-0-2	13431	2.3211	-	7471B	PPB	16 Jan 2024 14:06:31	U	SMPL
P1140-03 - 1	MR-309-37-39	5033	0.8856	-	7471B	PPB	16 Jan 2024 14:08:52	U	SMPL
P1147-01 - 1	MH-E	329	0.0815	-	7471B	PPB	16 Jan 2024 14:11:12	U	SMPL
P1147-03 - 1	MH-D	1343	0.2548	-	7471B	PPB	16 Jan 2024 14:13:29	U	SMPL
CCV77 - 1	CCV77	27973	4.8069	-	7471B	PPB	16 Jan 2024 14:18:23	U	SMPL
CCB77 - 1	CCB77	-229	-0.0139	-	7471B	PPB	16 Jan 2024 14:20:41	U	SMPL
P1132-01LX5 - 1		506	0.1118	-	7471B	PPB	16 Jan 2024 14:23:08	U	SMPL
P1132-01A - 1		27873	4.7898	-	7471B	PPB	16 Jan 2024 14:27:27	U	SMPL
CCV78 - 1	CCV78	27683	4.7573	-	7471B	PPB	16 Jan 2024 14:29:42	U	SMPL
CCB78 - 1	CCB78	-270	-0.0209	-	7471B	PPB	16 Jan 2024 14:32:07	U	SMPL