


LA129180

7470A

INSTRUMENT ID: CV1

Linear

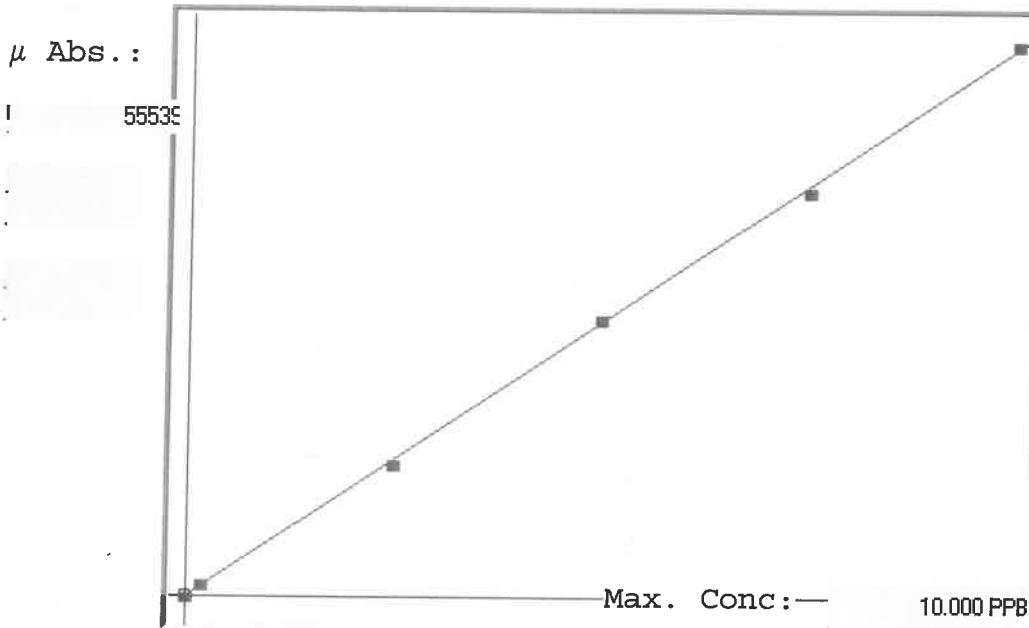

A= 0.0000e+000

B= 1.8107e-004

C= 8.7551e-003

Rho= 0.9998224

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	9/1/1
0.0	0.000	0.021	0.021	67	0.000	67	0				
0.2	0.200	0.239	0.039	1269	0.0 %	1269					20
2.5	2.500	2.418	-0.082	13304	0.0 %	13304					-3
5.0	5.000	5.066	0.066	27931	0.0 %	27931					1
7.5	7.500	7.392	-0.108	40775	0.0 %	40775					1
10.0	10.000	10.065	0.065	55539	0.0 %	55539					1

LB129180 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 19 Jan 2024 09:58:54

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	67	-	0.0000	7470A	PPB	19 Jan 2024 10:17:18	S	Std
0.2 - 1	50-2	1269	-	0.2000	7470A	PPB	19 Jan 2024 10:19:38	S	Std
2.5 - 1	52-5	13304	-	2.5000	7470A	PPB	19 Jan 2024 10:21:55	S	Std
5.0 - 1	55	27931	-	5.0000	7470A	PPB	19 Jan 2024 10:24:12	S	Std
7.5 - 1	57-7	40775	-	7.5000	7470A	PPB	19 Jan 2024 10:26:29	S	Std
10.0 - 1	510	55539	-	10.0000	7470A	PPB	19 Jan 2024 10:31:32	S	Std
ICV72 - 1	ICV72	20840	3.7822	-	7470A	PPB	19 Jan 2024 10:34:44	U	SMPL
ICB72 - 1	ICB72	55	0.0187	-	7470A	PPB	19 Jan 2024 10:36:58	U	SMPL
CCV90 - 1	CCV90	27070	4.9102	-	7470A	PPB	19 Jan 2024 10:39:16	U	SMPL
CCB90 - 1	CCB90	92	0.0254	-	7470A	PPB	19 Jan 2024 10:41:32	U	SMPL
CRA - 1	CRA	1159	0.2186	-	7470A	PPB	19 Jan 2024 10:43:51	U	SMPL
HighStd - 1	HighStd	55160	9.9964	-	7470A	PPB	19 Jan 2024 10:46:07	U	SMPL
ChkStd - 1	ChkStd	37892	6.8697	-	7470A	PPB	19 Jan 2024 10:48:22	U	SMPL
PB158525BL - 1	PBW	54	0.0185	-	7470A	PPB	19 Jan 2024 10:50:41	U	SMPL
PB158525BS - 1	LCSW	24619	4.4664	-	7470A	PPB	19 Jan 2024 10:53:00	U	SMPL
P1152-01 - 1	A2421	19	0.0122	-	7470A	PPB	19 Jan 2024 10:55:17	U	SMPL
P1152-01DUP - 1	A2421DUP	183	0.0419	-	7470A	PPB	19 Jan 2024 10:57:37	U	SMPL
P1152-01MS - 1	A2421MS	18692	3.3933	-	7470A	PPB	19 Jan 2024 10:59:54	U	SMPL
P1152-01MSD - 1	A2421MSD	18749	3.4036	-	7470A	PPB	19 Jan 2024 11:02:14	U	SMPL
CCV91 - 1	CCV91	28280	5.1293	-	7470A	PPB	19 Jan 2024 11:04:32	U	SMPL
CCB91 - 1	CCB91	-4	0.0080	-	7470A	PPB	19 Jan 2024 11:06:54	U	SMPL
P1152-01LX5 - 1		-17	0.0057	-	7470A	PPB	19 Jan 2024 11:09:12	U	SMPL
P1152-01A - 1		21271	3.8602	-	7470A	PPB	19 Jan 2024 11:11:27	U	SMPL
CCV92 - 1	CCV92	28750	5.2144	-	7470A	PPB	19 Jan 2024 11:13:42	U	SMPL
CCB92 - 1	CCB92	88	0.0247	-	7470A	PPB	19 Jan 2024 11:16:00	U	SMPL