


LB129207

7471B

INSTRUMENT ID: CV1

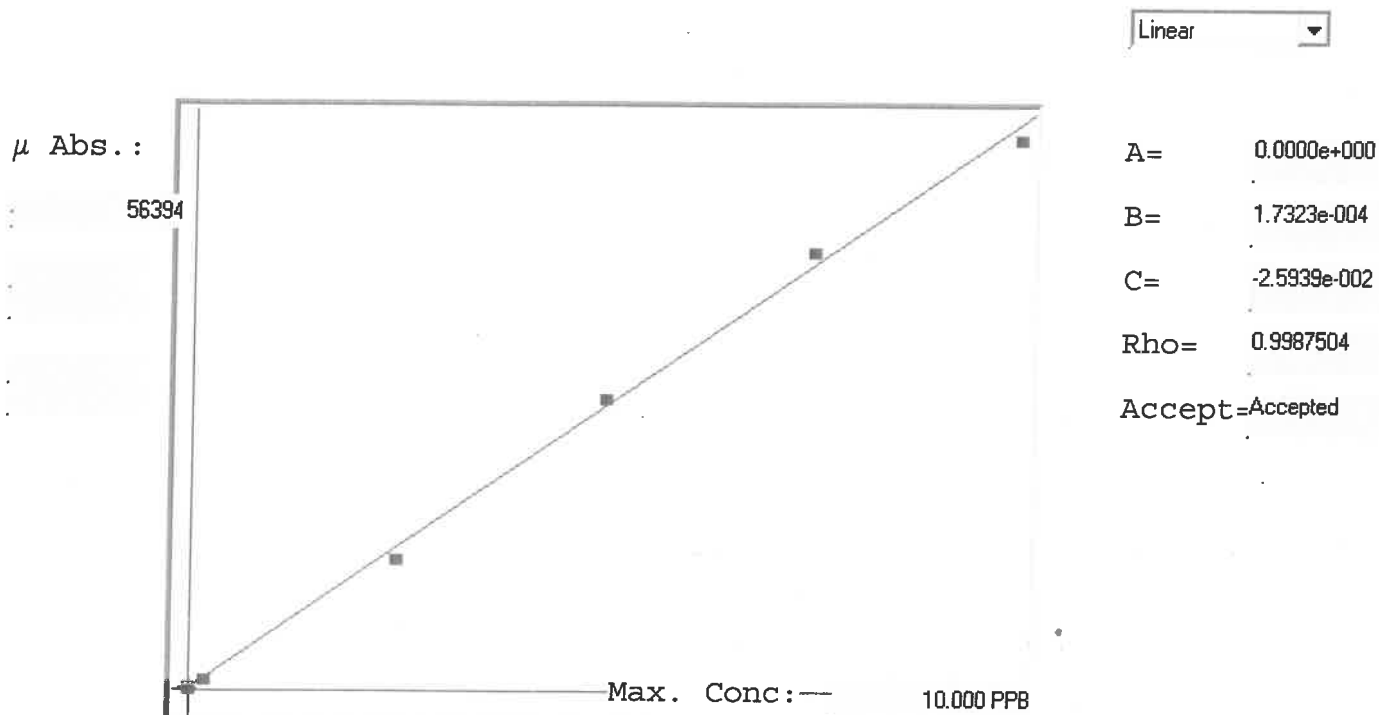

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0 D
0.0	0.000	0.038	0.038	369	0.000	369					
0.2	0.200	0.179	-0.021	1182	0.0 %	1182					-11
2.5	2.500	2.311	-0.189	13490	0.0 %	13490					-8
5.0	5.000	5.151	0.151	29884	0.0 %	29884					3
7.5	7.500	7.779	0.279	45054	0.0 %	45054					4
10.0	10.000	9.743	-0.257	56394	0.0 %	56394					-3

LB129207 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Jan 2024 13:33:26

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	369	-	0.0000	7471B	PPB	22 Jan 2024 13:37:46	S	Std
0.2 - 1	51.2	1182	-	0.2000	7471B	PPB	22 Jan 2024 13:40:03	S	Std
2.5 - 1	52.5	13490	-	2.5000	7471B	PPB	22 Jan 2024 13:42:20	S	Std
5.0 - 1	55	29884	-	5.0000	7471B	PPB	22 Jan 2024 13:44:37	S	Std
7.5 - 1	57.5	45054	-	7.5000	7471B	PPB	22 Jan 2024 13:46:56	S	Std
10.0 - 1	510	56394	-	10.0000	7471B	PPB	22 Jan 2024 13:49:21	S	Std
ICV76 - 1	ICV76	21367	3.6754	-	7471B	PPB	22 Jan 2024 13:52:34	U	SMPL
ICB76 - 1	ICB76	-58	-0.0360	-	7471B	PPB	22 Jan 2024 13:54:50	U	SMPL
CCV09 - 1	CCV09	30432	5.2457	-	7471B	PPB	22 Jan 2024 13:57:15	U	SMPL
CCB09 - 1	CCB09	-98	-0.0429	-	7471B	PPB	22 Jan 2024 13:59:30	U	SMPL
CRA - 1	CRA	1234	0.1878	-	7471B	PPB	22 Jan 2024 14:09:30	U	SMPL
HighStd - 1	HighStd	54867	9.4785	-	7471B	PPB	22 Jan 2024 14:11:44	U	SMPL
ChkStd - 1	ChkStd	41946	7.2402	-	7471B	PPB	22 Jan 2024 14:13:59	U	SMPL
PB158556BL - 1	PBS	-366	-0.0893	-	7471B	PPB	22 Jan 2024 14:16:20	U	SMPL
PB158556BS - 1	LCSS	22766	3.9177	-	7471B	PPB	22 Jan 2024 14:18:49	U	SMPL
P1180-01 - 1	EO-01-011824	4723	0.7922	-	7471B	PPB	22 Jan 2024 14:21:05	U	SMPL
P1182-01 - 1	OR-03-011824	1696	0.2679	-	7471B	PPB	22 Jan 2024 14:23:30	U	SMPL
P1183-01 - 1	MR-305-0-2	15421	2.6454	-	7471B	PPB	22 Jan 2024 14:25:49	U	SMPL
P1183-01DUP - 1	MR-305-0-2DUP	15329	2.6294	-	7471B	PPB	22 Jan 2024 14:28:07	U	SMPL
P1183-01MS - 1	MR-305-0-2MS	39349	6.7903	-	7471B	PPB	22 Jan 2024 14:30:26	U	SMPL
CCV10 - 1	CCV10	30427	5.2448	-	7471B	PPB	22 Jan 2024 14:32:46	U	SMPL
CCB10 - 1	CCB10	-18	-0.0291	-	7471B	PPB	22 Jan 2024 14:35:12	U	SMPL
P1183-01MSD - 1	MR-305-0-2MSD	35411	6.1082	-	7471B	PPB	22 Jan 2024 14:40:16	U	SMPL
P1183-03 - 1	MR-305-25-27	6047	1.0216	-	7471B	PPB	22 Jan 2024 14:42:33	U	SMPL
P1200-01 - 1	CHRT-24376	565	0.0719	-	7471B	PPB	22 Jan 2024 14:45:00	U	SMPL
P1203-01 - 1	72-11977	3714	0.6174	-	7471B	PPB	22 Jan 2024 14:47:18	U	SMPL
P1183-01LX5 - 1		3179	0.5247	-	7471B	PPB	22 Jan 2024 14:49:34	U	SMPL
P1183-01A - 1		39495	6.8156	-	7471B	PPB	22 Jan 2024 14:51:53	U	SMPL
CCV11 - 1	CCV11	30693	5.2909	-	7471B	PPB	22 Jan 2024 14:54:11	U	SMPL
CCB11 - 1	CCB11	-58	-0.0360	-	7471B	PPB	22 Jan 2024 14:56:39	U	SMPL