

16129462

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

2/8/2024 15:15

Reviewed by : RM Instrument ID : Konelab

Test: Phenolics-

Sample Id	<i>Null</i> Result	Dil. 1 +	Response	Errors
ICV1	0.996	0.0	0.106	
ICB1	0.019	0.0	0.008	
CCV1	0.995	0.0	0.106	
CCB1	0.017	0.0	0.008	
PB158891BL	0.015	0.0	0.007	
PB158891BS	0.975	0.0	0.104	
P1187-11	0.048	0.0	0.011	
P1327-01	0.045	0.0	0.010	
P1327-01DUP	0.044	0.0	0.010	
P1327-01MS	1.061	0.0	0.113	
P1327-01MSD	1.064	0.0	0.113	
P1410-04	0.045	0.0	0.010	
P1410-06	0.042	0.0	0.010	
P1187-10	0.034	0.0	0.009	
CCV2	1.006	0.0	0.107	
CCB2	0.017	0.0	0.008	
N	16			
Mean	0.401			
SD	0.4923			
CV%	122.63			

Aquakem v. 7.2AQ1

Results from time period:

Thu Feb 08 13:48:57 2024

Thu Feb 08 15:06:36 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0018	mg/l	2/8/2024 13:48:57	
0.05PPM	A	Phenolics-	P	0.049	mg/l	2/8/2024 13:48:58	
0.1PPM	A	Phenolics-	P	0.1037	mg/l	2/8/2024 13:48:59	
0.25PPM	A	Phenolics-	P	0.2562	mg/l	2/8/2024 13:49:00	
0.50PPM	A	Phenolics-	P	0.5043	mg/l	2/8/2024 13:49:01	
1.0PPM	A	Phenolics-	P	0.974	mg/l	2/8/2024 13:49:02	
2.0PPM	A	Phenolics-	P	2.011	mg/l	2/8/2024 13:49:03	
ICV1	S	Phenolics-	P	0.9958	mg/l	2/8/2024 14:39:30	
ICB1	S	Phenolics-	P	0.019	mg/l	2/8/2024 14:39:31	
CCV1	S	Phenolics-	P	0.9946	mg/l	2/8/2024 14:39:33	
CCB1	S	Phenolics-	P	0.0171	mg/l	2/8/2024 14:39:35	
PB158891BL	S	Phenolics-	P	0.0146	mg/l	2/8/2024 14:39:37	
PB158891BS	S	Phenolics-	P	0.9754	mg/l	2/8/2024 14:39:40	
P1187-11	S	Phenolics-	P	0.0483	mg/l	2/8/2024 14:49:31	
P1327-01	S	Phenolics-	P	0.0452	mg/l	2/8/2024 14:49:35	
P1327-01DUP	S	Phenolics-	P	0.0439	mg/l	2/8/2024 14:49:36	
P1327-01MS	S	Phenolics-	P	1.0606	mg/l	2/8/2024 14:49:37	
P1327-01MSD	S	Phenolics-	P	1.0644	mg/l	2/8/2024 14:49:38	
P1410-04	S	Phenolics-	P	0.0454	mg/l	2/8/2024 14:49:39	
P1410-06	S	Phenolics-	P	0.0419	mg/l	2/8/2024 14:49:40	
P1187-10	S	Phenolics-	P	0.0343	mg/l	2/8/2024 15:06:34	
CCV2	S	Phenolics-	P	1.0055	mg/l	2/8/2024 15:06:35	
CCB2	S	Phenolics-	P	0.0171	mg/l	2/8/2024 15:06:36	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

2/9/2024 9:35


Test Phenolics-

Accepted 2/8/2024 13:59

Factor 9.909
Bias 0.006

Coeff. of det. 0.999724

Errors

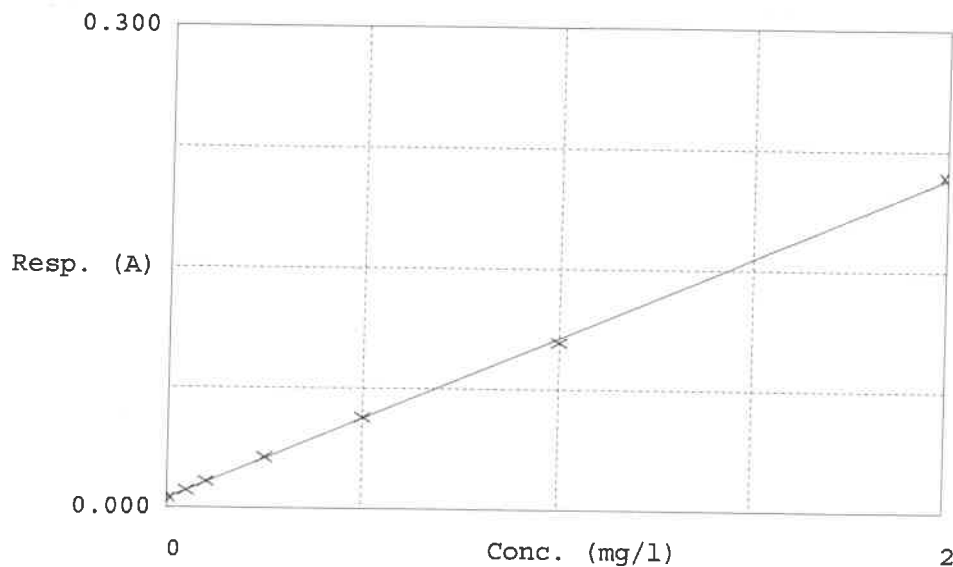

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	0.0018	0.0000	-
2	Phenol-2	0.011	0.0490	0.0500	-2.0
3	Phenol-2	0.016	0.1037	0.1000	3.7
4	Phenol-2	0.032	0.2562	0.2500	2.5
5	Phenol-2	0.057	0.5043	0.5000	0.9
6	Phenol-2	0.104	0.9740	1.0000	-2.6
7	Phenol-2	0.209	2.0110	2.0000	0.6

02/08/2024
RM