

UB129552


SFAM01.1

INSTRUMENT ID: CV1

Linear

μ Abs.:

49413

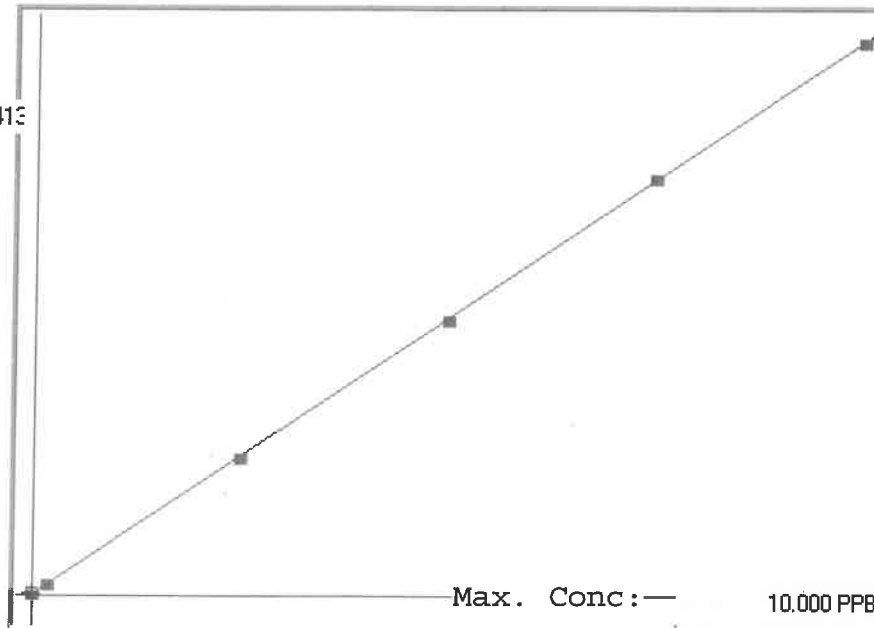

A= 0.0000e+000

B= 2.0248e-004 slope

C= -2.0170e-002 $\approx$ intercept

Rho= 0.9999862

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Std ID
0.00	0.000	0.020	0.020	198	0.000	198					0.00
0.05	0.050					442	0				0.05
0.20	0.200	0.193	-0.007	1055	0.0 %	1055					0.20
2.50	2.500	2.473	-0.027	12315	0.0 %	12315					2.50
5.00	5.000	4.999	-0.001	24786	0.0 %	24786					5.00
7.50	7.500	7.530	0.030	37286	0.0 %	37286					7.50
10.0	10.000	9.985	-0.015	49413	0.0 %	49413					10.0

LB129552

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Stnd Conc	Method	Units	Date	Type
	0 S0	198	-		0 SFAM01.1	PPB	2/15/2024 16:00	Std
	0.2 S01	1055	-		0.2 SFAM01.1	PPB	2/15/2024 16:02	Std
	2.5 S02	12315	-		2.5 SFAM01.1	PPB	2/15/2024 16:04	Std
	5 S03	24786	-		5 SFAM01.1	PPB	2/15/2024 16:07	Std
	7.5 S04	37286	-		7.5 SFAM01.1	PPB	2/15/2024 16:09	Std
	10 S05	49413	-		10 SFAM01.1	PPB	2/15/2024 16:11	Std
ICV12	ICV12	20341	4.0985 -		SFAM01.1	PPB	2/15/2024 16:14	SMPL
ICB12	ICB12	116	0.0033 -		SFAM01.1	PPB	2/15/2024 16:19	SMPL
CCV038	CCV038	25289	5.1004 -		SFAM01.1	PPB	2/15/2024 16:21	SMPL
CCB038	CCB038	92	-0.0015 -		SFAM01.1	PPB	2/15/2024 16:26	SMPL
PBW04	PBW04	145	0.0092 -		SFAM01.1	PPB	2/15/2024 16:28	SMPL
PBW05	PBW05	181	0.0165 -		SFAM01.1	PPB	2/15/2024 16:31	SMPL
MDL04	MDL04	375	0.0558 -		SFAM01.1	PPB	2/15/2024 16:33	SMPL
MDL05	MDL05	342	0.0491 -		SFAM01.1	PPB	2/15/2024 16:35	SMPL
CCV039	CCV039	25331	5.1089 -		SFAM01.1	PPB	2/15/2024 16:37	SMPL
CCB039	CCB039	115	0.0031 -		SFAM01.1	PPB	2/15/2024 16:42	SMPL