


LB129590

7470A

INSTRUMENT ID: CV1

Linear

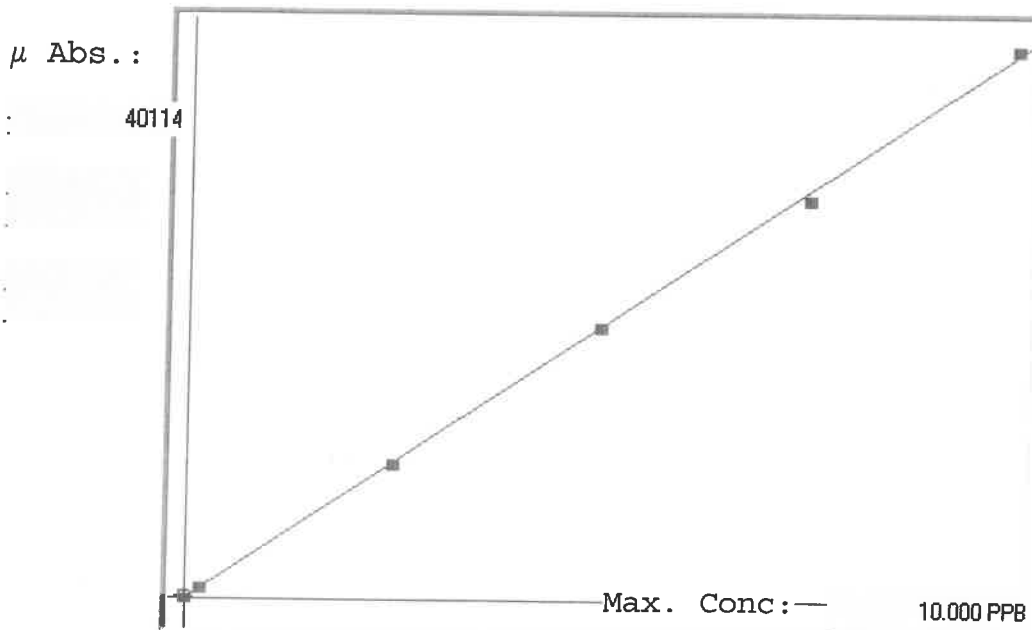

A= 0.0000e+000

B= 2.5213e-004

C= -2.6867e-003

Rho= 0.9997710

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.040	0.040	170	0.000	170	0				6
0.2	0.200	0.212	0.012	850	0.0 %	850					-1
2.5	2.500	2.483	-0.017	9860	0.0 %	9860					0
5.0	5.000	5.005	0.005	19862	0.0 %	19862					-2
7.5	7.500	7.348	-0.152	29156	0.0 %	29156					1
10.0	10.000	10.111	0.111	40114	0.0 %	40114					

LB129590 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Feb 2024 09:42:26

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	170	-	0.0000	7470A	PPB	20 Feb 2024 09:57:27	S	Std
0.2 - 1	50.2	850	-	0.2000	7470A	PPB	20 Feb 2024 09:59:44	S	Std
2.5 - 1	52.5	9880	-	2.5000	7470A	PPB	20 Feb 2024 10:02:01	S	Std
5.0 - 1	55	19862	-	5.0000	7470A	PPB	20 Feb 2024 10:04:18	S	Std
7.5 - 1	57.5	29156	-	7.5000	7470A	PPB	20 Feb 2024 10:06:36	S	Std
10.0 - 1	510	40114	-	10.0000	7470A	PPB	20 Feb 2024 10:11:33	S	Std
ICV16 - 1	ICV16	14575	3.6721	-	7470A	PPB	20 Feb 2024 10:14:26	U	SMPL
ICB16 - 1	ICB16	264	0.0638	-	7470A	PPB	20 Feb 2024 10:16:40	U	SMPL
CCV50 - 1	CCV50	19832	4.9976	-	7470A	PPB	20 Feb 2024 10:18:58	U	SMPL
CCB50 - 1	CCB50	240	0.0578	-	7470A	PPB	20 Feb 2024 10:21:13	U	SMPL
CRA - 1	CRA	766	0.1904	-	7470A	PPB	20 Feb 2024 10:23:31	U	SMPL
HighStd - 1	HighStd	40538	10.2182	-	7470A	PPB	20 Feb 2024 10:25:46	U	SMPL
ChkStd - 1	ChkStd	26404	6.6546	-	7470A	PPB	20 Feb 2024 10:28:01	U	SMPL
PB159122BL - 1	PBW	-308	-0.0798	-	7470A	PPB	20 Feb 2024 10:30:19	U	SMPL
PB159122BS - 1	LCSW	16053	4.0448	-	7470A	PPB	20 Feb 2024 10:35:14	U	SMPL
P1514-02 - 1	ETGI-343	-151	-0.0408	-	7470A	PPB	20 Feb 2024 10:37:30	U	SMPL
P1514-02DUP - 1	ETGI-343DUP	1	-0.0024	-	7470A	PPB	20 Feb 2024 10:39:49	U	SMPL
P1514-02MS - 1	ETGI-343MS	14433	3.6363	-	7470A	PPB	20 Feb 2024 10:44:37	U	SMPL
P1514-02MSD - 1	ETGI-343MSD	14742	3.7142	-	7470A	PPB	20 Feb 2024 10:46:54	U	SMPL
P1516-01 - 1	COMP-1	-146	-0.0395	-	7470A	PPB	20 Feb 2024 10:49:11	U	SMPL
CCV51 - 1	CCV51	19780	4.9845	-	7470A	PPB	20 Feb 2024 10:51:28	U	SMPL
CCB51 - 1	CCB51	225	0.0540	-	7470A	PPB	20 Feb 2024 10:53:44	U	SMPL
P1516-03 - 1	00043	-10	-0.0052	-	7470A	PPB	20 Feb 2024 10:56:02	U	SMPL
PB159123BL - 1	PBW	-1	-0.0029	-	7470A	PPB	20 Feb 2024 10:58:17	U	SMPL
PB159123BS - 1	LCSW	14711	3.7064	-	7470A	PPB	20 Feb 2024 11:00:34	U	SMPL
P1516-02 - 1	00042	-168	-0.0450	-	7470A	PPB	20 Feb 2024 11:02:49	U	SMPL
P1516-02DUP - 1	00042DUP	-9	-0.0050	-	7470A	PPB	20 Feb 2024 11:05:08	U	SMPL
P1516-02MS - 1	00042MS	14636	3.6875	-	7470A	PPB	20 Feb 2024 11:07:24	U	SMPL
P1516-02MSD - 1	00042MSD	14164	3.5685	-	7470A	PPB	20 Feb 2024 11:09:41	U	SMPL
P1528-01 - 1	IDW-20240215	-44	-0.0138	-	7470A	PPB	20 Feb 2024 11:12:00	U	SMPL
PB159142BL - 1	PBW	47	0.0092	-	7470A	PPB	20 Feb 2024 11:14:19	U	SMPL
PB159142BS - 1	LCSW	16421	4.1376	-	7470A	PPB	20 Feb 2024 11:16:34	U	SMPL
CCV52 - 1	CCV52	20102	5.0656	-	7470A	PPB	20 Feb 2024 11:18:50	U	SMPL
CCB52 - 1	CCB52	155	0.0364	-	7470A	PPB	20 Feb 2024 11:21:14	U	SMPL
P1462-01 - 1	20240762-39N-N-FIELD-BLANK-1	312	0.0760	-	7470A	PPB	20 Feb 2024 11:31:06	U	SMPL
P1491-01 - 1	20240762-39N-N-FIELD-BLANK-1	273	0.0661	-	7470A	PPB	20 Feb 2024 11:33:21	U	SMPL
P1521-01 - 1	CG-MW-23	2075	5.0205	-	7470A	PPB	20 Feb 2024 11:35:37	U	SMPL
P1521-01DUP - 1	CG-MW-23DUP	1899	0.4761	-	7470A	PPB	20 Feb 2024 11:37:52	U	SMPL
P1521-01MS - 1	CG-MW-23MS	19136	4.8221	-	7470A	PPB	20 Feb 2024 11:40:08	U	SMPL
P1521-01MSD - 1	CG-MW-23MSD	18561	4.6771	-	7470A	PPB	20 Feb 2024 11:42:25	U	SMPL
PB159106TB - 1	PB159106TB	-141	-0.0382	-	7470A	PPB	20 Feb 2024 11:44:44	U	SMPL
PB159106TB - 1	PB159106TB	32	0.0054	-	7470A	PPB	20 Feb 2024 11:47:02	U	SMPL
CCV53 - 1	CCV53	20007	5.0417	-	7470A	PPB	20 Feb 2024 11:49:19	U	SMPL
CCB53 - 1	CCB53	119	0.0273	-	7470A	PPB	20 Feb 2024 11:51:35	U	SMPL
P1514-02LX5 - 1		-4	-0.0037	-	7470A	PPB	20 Feb 2024 11:53:53	U	SMPL
P1514-02A - 1		16895	4.2571	-	7470A	PPB	20 Feb 2024 11:56:08	U	SMPL
P1516-02LX5 - 1		-216	-0.0571	-	7470A	PPB	20 Feb 2024 11:58:24	U	SMPL
P1516-02A - 1		17129	4.3161	-	7470A	PPB	20 Feb 2024 12:00:42	U	SMPL
P1521-01LX5 - 1		314	0.0765	-	7470A	PPB	20 Feb 2024 12:02:57	U	SMPL
P1521-01A - 1		18571	4.6796	-	7470A	PPB	20 Feb 2024 12:05:16	U	SMPL
CCV54 - 1	CCV54	20425	5.1471	-	7470A	PPB	20 Feb 2024 12:07:32	U	SMPL
CCB54 - 1	CCB54	-21	-0.0080	-	7470A	PPB	20 Feb 2024 12:09:54	U	SMPL