

16129601

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Pat

Instrument ID : Konelab

2/20/2024 15:34

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.934	0.0	0.104	
ICB1	0.004	0.0	0.010	
CCV1	0.933	0.0	0.104	
CCB1	0.002	0.0	0.010	
PB159083BL	0.003	0.0	0.010	
PB159083BS	0.929	0.0	0.103	
P1187-03	0.021	0.0	0.012	
PB159085BL	0.005	0.0	0.010	
PB159085BS	0.934	0.0	0.104	
P1187-09	0.021	0.0	0.012	
CCV2	0.935	0.0	0.104	
CCB2	0.002	0.0	0.010	

N	12
Mean	0.394
SD	0.4763
CV%	121.02

Aquakem v. 7.2AQ1

Results from time period:

Tue Feb 20 13:40:51 2024

Tue Feb 20 15:27:34 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0013	mg/l	2/20/2024 13:40:51	
0.05PPM	A	Phenolics-	P	0.0568	mg/l	2/20/2024 13:40:52	
0.1PPM	A	Phenolics-	P	0.1026	mg/l	2/20/2024 13:40:53	
0.25PPM	A	Phenolics-	P	0.2527	mg/l	2/20/2024 13:40:54	
0.50PPM	A	Phenolics-	P	0.4987	mg/l	2/20/2024 13:40:55	
1.0PPM	A	Phenolics-	P	0.9764	mg/l	2/20/2024 13:40:56	
2.0PPM	A	Phenolics-	P	2.0115	mg/l	2/20/2024 13:40:57	
ICV1	S	Phenolics-	P	0.9341	mg/l	2/20/2024 15:17:21	
ICB1	S	Phenolics-	P	0.0042	mg/l	2/20/2024 15:17:23	
CCV1	S	Phenolics-	P	0.9331	mg/l	2/20/2024 15:17:25	
CCB1	S	Phenolics-	P	0.0019	mg/l	2/20/2024 15:17:27	
PB159083BL	S	Phenolics-	P	0.0034	mg/l	2/20/2024 15:17:29	
PB159083BS	S	Phenolics-	P	0.929	mg/l	2/20/2024 15:17:32	
P1187-03	S	Phenolics-	P	0.0206	mg/l	2/20/2024 15:27:24	
PB159085BL	S	Phenolics-	P	0.0049	mg/l	2/20/2024 15:27:25	
PB159085BS	S	Phenolics-	P	0.9343	mg/l	2/20/2024 15:27:27	
P1187-09	S	Phenolics-	P	0.0205	mg/l	2/20/2024 15:27:29	
CCV2	S	Phenolics-	P	0.9353	mg/l	2/20/2024 15:27:32	
CCB2	S	Phenolics-	P	0.0018	mg/l	2/20/2024 15:27:33	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

2/20/2024 13:49


Test Phenolics-

Accepted 2/20/2024 13:49

Factor 9.94
Bias 0.010

Coeff. of det. 0.999761

Errors

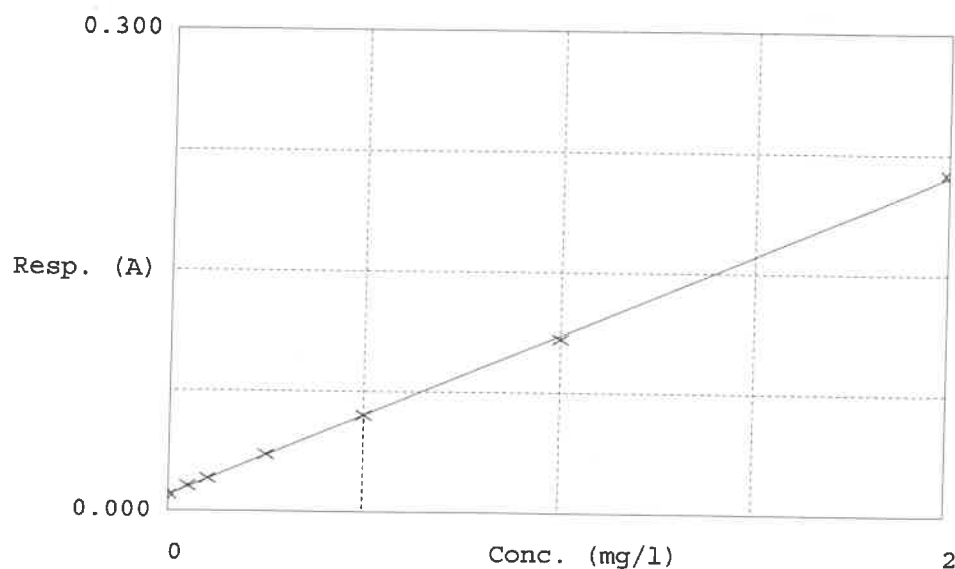

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.010	0.0013	0.0000	
2	Phenol-2	0.016	0.0568	0.0500	13.6
3	Phenol-2	0.020	0.1026	0.1000	2.6
4	Phenol-2	0.035	0.2527	0.2500	1.1
5	Phenol-2	0.060	0.4987	0.5000	-0.3
6	Phenol-2	0.108	0.9764	1.0000	-2.4
7	Phenol-2	0.212	2.0115	2.0000	0.6

02/20/2024
RM