


LB129758

7470A

INSTRUMENT ID: CV1

Linear

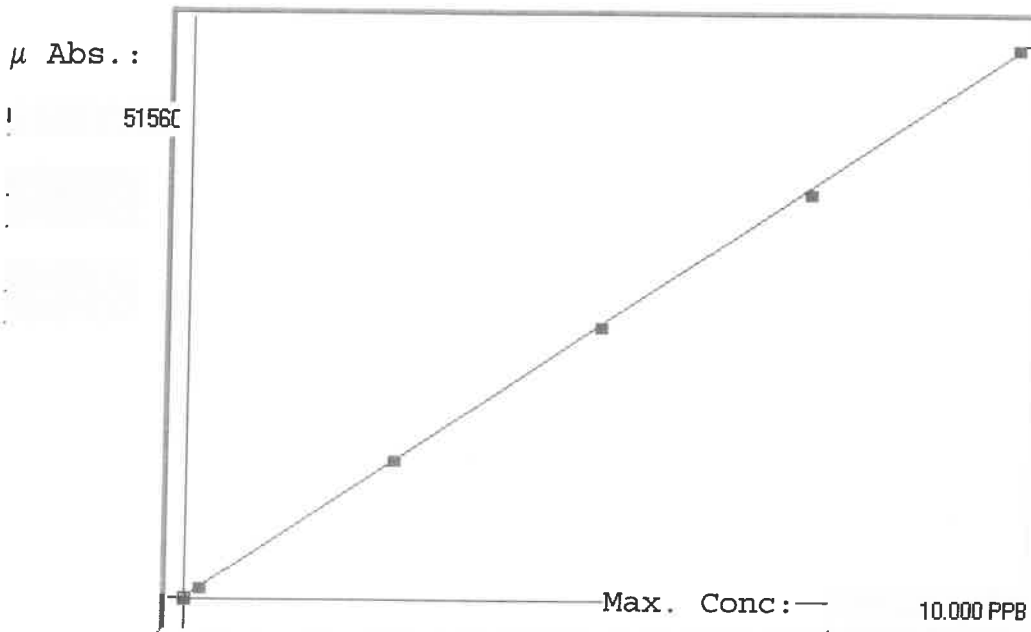

A= 0.0000e+000

B= 1.9540e-004

C= -2.5241e-002

Rho= 0.9999491

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%SD
0.0	0.000	0.000	0.000	131	0.000	131	0				1
0.2	0.200	0.202	0.002	1165	0.0 %	1165					1
2.5	2.500	2.526	0.026	13055	0.0 %	13055					1
5.0	5.000	4.993	-0.007	25684	0.0 %	25684					0
7.5	7.500	7.428	-0.072	38145	0.0 %	38145					1
10.0	10.000	10.050	0.050	51560	0.0 %	51560					1

LB129758 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Mar 2024 11:22:22

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	131	-	0.0000	7470A	PPB	04 Mar 2024 11:34:47	S	Std
0.2 - 1	51.2	1165	-	0.2000	7470A	PPB	04 Mar 2024 11:37:04	S	Std
2.5 - 1	52.5	13055	-	2.5000	7470A	PPB	04 Mar 2024 11:39:21	S	Std
5.0 - 1	55	25684	-	5.0000	7470A	PPB	04 Mar 2024 11:41:38	S	Std
7.5 - 1	57.5	38145	-	7.5000	7470A	PPB	04 Mar 2024 11:43:55	S	Std
10.0 - 1	51V	51560	-	10.0000	7470A	PPB	04 Mar 2024 11:46:13	S	Std
ICV31 - 1	ICV31	18857	3.6595	-	7470A	PPB	04 Mar 2024 11:49:03	U	SMPL
ICB31 - 1	ICB31	426	0.0580	-	7470A	PPB	04 Mar 2024 11:52:20	U	SMPL
CCV17 - 1	CCV17	25029	4.8655	-	7470A	PPB	04 Mar 2024 11:58:40	U	SMPL
CCB17 - 1	CCB17	358	0.0447	-	7470A	PPB	04 Mar 2024 12:01:29	U	SMPL
CRA - 1	CRA	1086	0.1870	-	7470A	PPB	04 Mar 2024 12:03:44	U	SMPL
HighStd - 1	HighStd	49146	9.5780	-	7470A	PPB	04 Mar 2024 12:05:59	U	SMPL
ChkStd - 1	ChkStd	34303	6.6776	-	7470A	PPB	04 Mar 2024 12:08:14	U	SMPL
PB159407BL - 1	PBW	-266	-0.0772	-	7470A	PPB	04 Mar 2024 12:10:33	U	SMPL
PB159407BS - 1	LCSW	19439	3.7732	-	7470A	PPB	04 Mar 2024 12:15:25	U	SMPL
P1602-03 - 1	WC-1	-57	-0.0364	-	7470A	PPB	04 Mar 2024 12:17:41	U	SMPL
P1602-06 - 1	WC-2	29	-0.0196	-	7470A	PPB	04 Mar 2024 12:20:00	U	SMPL
P1602-09 - 1	WC-3	48	-0.0159	-	7470A	PPB	04 Mar 2024 12:22:17	U	SMPL
P1602-12 - 1	WC-4	89	-0.0079	-	7470A	PPB	04 Mar 2024 12:24:34	U	SMPL
P1639-10 - 1	SP-5	84	-0.0088	-	7470A	PPB	04 Mar 2024 12:26:49	U	SMPL
CCV18 - 1	CCV18	25031	4.8659	-	7470A	PPB	04 Mar 2024 12:29:04	U	SMPL
CCB18 - 1	CCB18	240	0.0217	-	7470A	PPB	04 Mar 2024 12:31:20	U	SMPL
P1639-20 - 1	SP-6	0	-0.0252	-	7470A	PPB	04 Mar 2024 12:33:39	U	SMPL
P1639-30 - 1	SP-7	53	-0.0149	-	7470A	PPB	04 Mar 2024 12:35:54	U	SMPL
P1639-40 - 1	SP-8	35	-0.0184	-	7470A	PPB	04 Mar 2024 12:38:10	U	SMPL
P1659-04 - 1	TP-16	-5	-0.0262	-	7470A	PPB	04 Mar 2024 12:40:26	U	SMPL
P1659-08 - 1	TP-7	43	-0.0168	-	7470A	PPB	04 Mar 2024 12:42:41	U	SMPL
P1659-08DUP - 1	TP-7DUP	0	-0.0252	-	7470A	PPB	04 Mar 2024 12:44:57	U	SMPL
P1659-08MS - 1	TP-7MS	15099	2.9251	-	7470A	PPB	04 Mar 2024 12:47:14	U	SMPL
P1659-08MSD - 1	TP-7MSD	14889	2.8841	-	7470A	PPB	04 Mar 2024 12:49:30	U	SMPL
PB159408BL - 1	PBW	85	-0.0086	-	7470A	PPB	04 Mar 2024 12:51:50	U	SMPL
PB159408BS - 1	LCSW	18961	3.6798	-	7470A	PPB	04 Mar 2024 12:54:08	U	SMPL
CCV19 - 1	CCV19	24014	4.6671	-	7470A	PPB	04 Mar 2024 12:56:23	U	SMPL
CCB19 - 1	CCB19	349	0.0430	-	7470A	PPB	04 Mar 2024 12:59:28	U	SMPL
P1613-04 - 1	1850	310	0.0353	-	7470A	PPB	04 Mar 2024 13:01:43	U	SMPL
P1613-04DUP - 1	1850DUP	452	0.0631	-	7470A	PPB	04 Mar 2024 13:03:59	U	SMPL
P1613-04MS - 1	1850MS	3787	0.7147	-	7470A	PPB	04 Mar 2024 13:06:14	U	SMPL
P1613-04MSD - 1	1850MSD	2921	0.5455	-	7470A	PPB	04 Mar 2024 13:09:20	U	SMPL
PB159348TB - 1	PB159348TB	55	-0.0145	-	7470A	PPB	04 Mar 2024 13:12:14	U	SMPL
P1659-08LX5 - 1		42	-0.0170	-	7470A	PPB	04 Mar 2024 13:14:30	U	SMPL
P1659-08A - 1		21558	4.1872	-	7470A	PPB	04 Mar 2024 13:16:46	U	SMPL
P1613-04LX5 - 1		-96	-0.0440	-	7470A	PPB	04 Mar 2024 13:19:03	U	SMPL
P1613-04A - 1		14030	2.7162	-	7470A	PPB	04 Mar 2024 13:21:22	U	SMPL
CCV20 - 1	CCV20	26279	5.1097	-	7470A	PPB	04 Mar 2024 13:26:54	U	SMPL
CCB20 - 1	CCB20	-213	-0.0669	-	7470A	PPB	04 Mar 2024 13:29:09	U	SMPL
P1620-10 - 1	SP-1	72	-0.0112	-	7470A	PPB	04 Mar 2024 13:31:28	U	SMPL
P1620-20 - 1	SP-2	96	-0.0065	-	7470A	PPB	04 Mar 2024 13:33:43	U	SMPL
P1620-30 - 1	SP-3	100	-0.0057	-	7470A	PPB	04 Mar 2024 13:35:59	U	SMPL
P1620-40 - 1	SP-4	85	-0.0086	-	7470A	PPB	04 Mar 2024 13:38:14	U	SMPL
CCV21 - 1	CCV21	24016	4.6675	-	7470A	PPB	04 Mar 2024 13:40:30	U	SMPL
CCB21 - 1	CCB21	-123	-0.0493	-	7470A	PPB	04 Mar 2024 13:42:46	U	SMPL